

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111224\
 Data File : PS028405.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2024 18:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 23:57:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 08 17:46:43 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	7.746	1372.7E6	707.3E6	497.222	443.894
Target Compounds							
2) T	3,5-DICHL...	6.402	0.000	520009	0	<MDL	N.D. #
3) T	4-Nitroph...	7.033	0.000	7259609	0	3.915	N.D. #
6) T	MCP	7.669f	0.000	22250311	0	2.721	N.D. #
8) T	DICHLORPROP	8.102f	8.715f	1203393	9647150	<MDL	5.416 #
10) T	Pentachlo...	8.725f	0.000	558719	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.310f	9.957f	5769404	2234921	<MDL	<MDL #
12) T	2,4,5-T	9.555	10.322	1838323	2849416	<MDL	<MDL #
15) T	Picloram	11.142	12.369	11651327	6837191	<MDL	<MDL #
16) T	DCPA	0.000	12.369f	0	6837191	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111224\
Data File : PS028405.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2024 18:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 23:57:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110924.M
Quant Title : 8080.M
QLast Update : Fri Nov 08 17:46:43 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

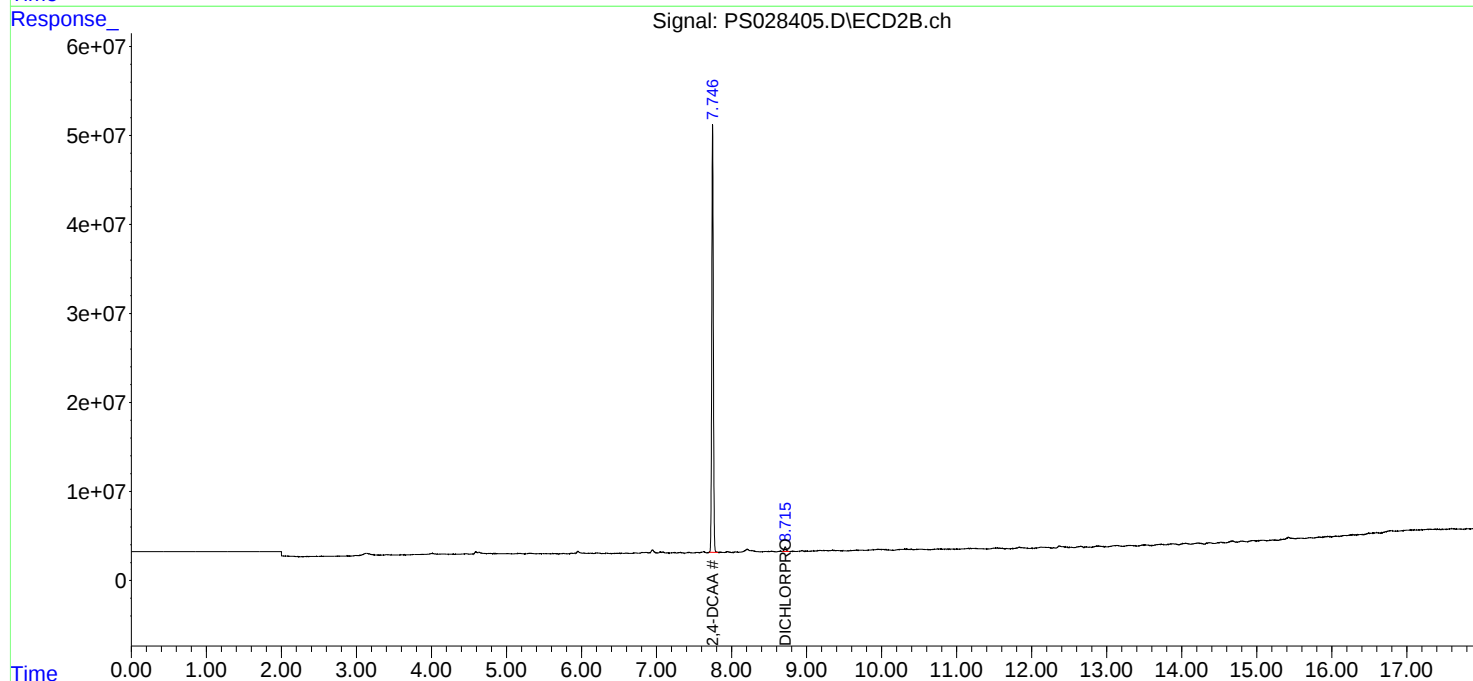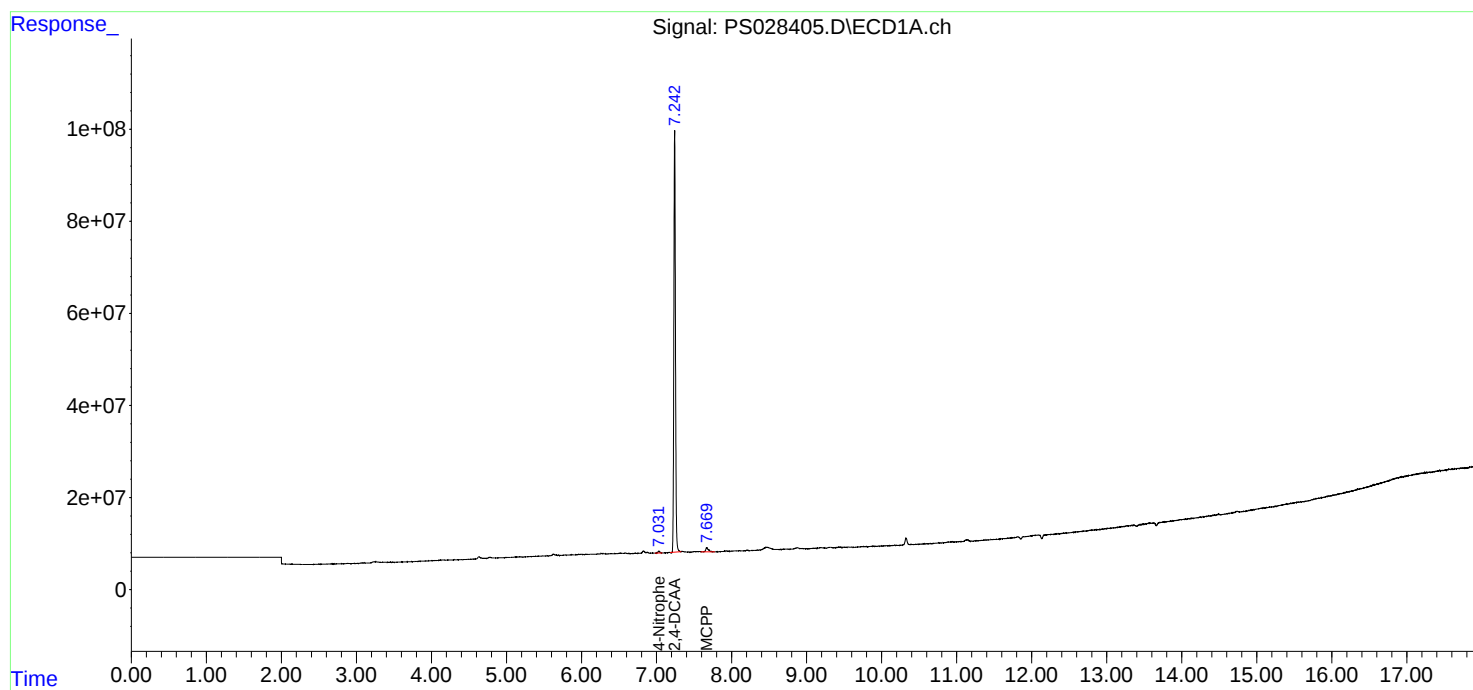


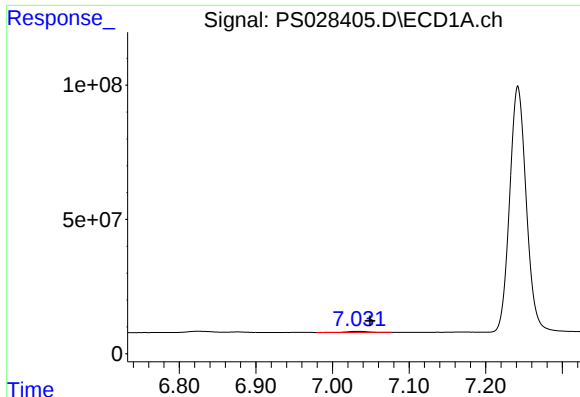

#3 4-Nitrophenol


R.T.: 7.033 min
Delta R.T.: -0.016 min
Response: 7259609
Conc: 3.92 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

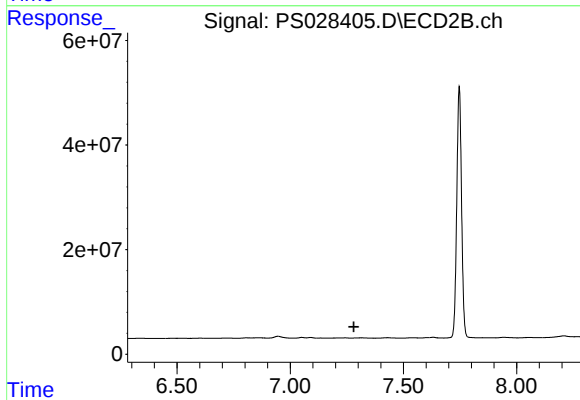


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 7.281 min
Response: 0
Conc: N.D.

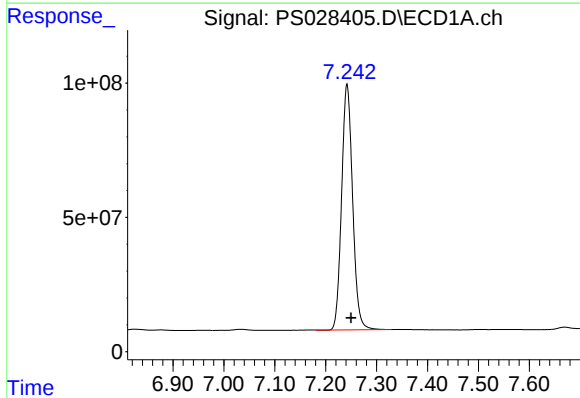


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: -0.008 min
Response: 1372708223
Conc: 497.22 ng/ml

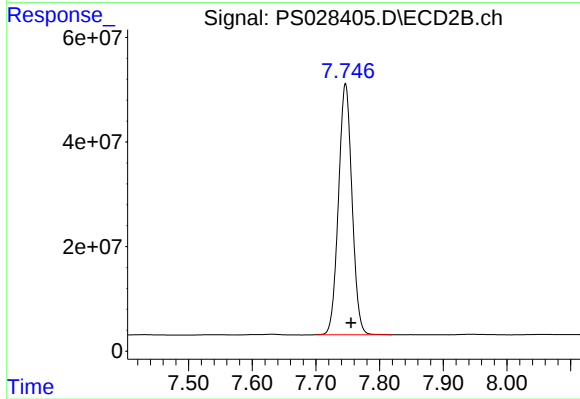

#4 2,4-DCAA


R.T.: 7.746 min
Delta R.T.: -0.009 min
Response: 707309965
Conc: 443.89 ng/ml

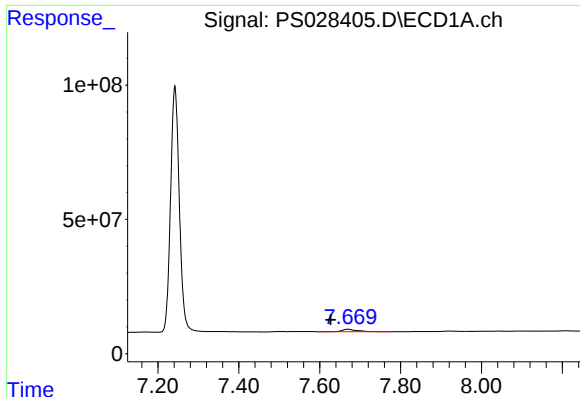

#6 MCP


R.T.: 7.669 min
Delta R.T.: 0.042 min
Response: 22250311
Conc: 2.72 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

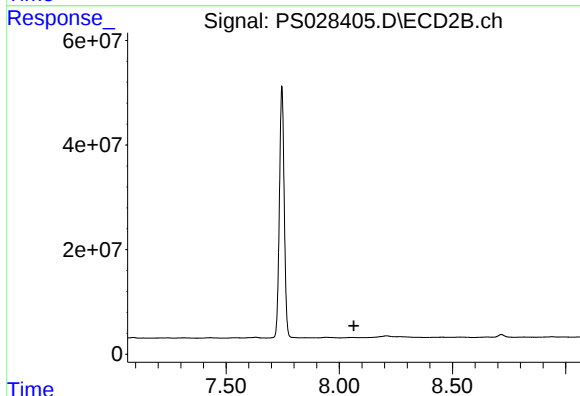


#6 MCP

R.T.: 0.000 min
Exp R.T. : 8.064 min
Response: 0
Conc: N.D.

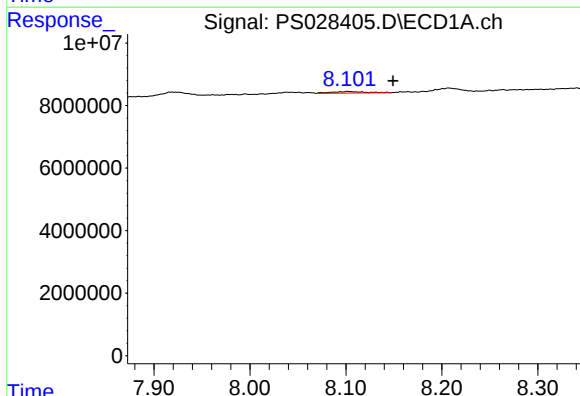

#8 DICHLORPROP

R.T.: 8.102 min
Delta R.T.: -0.047 min
Response: 1203393
Conc: N.D.

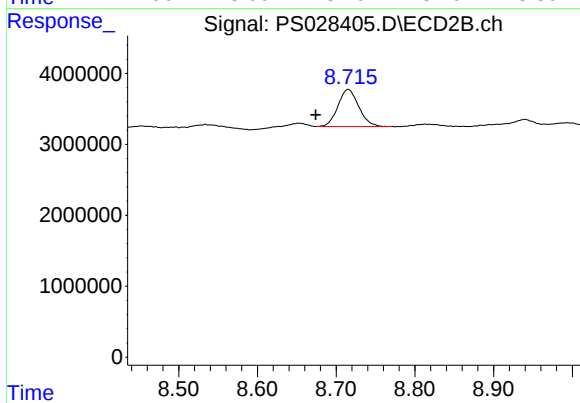

#8 DICHLORPROP

R.T.: 8.715 min
Delta R.T.: 0.041 min
Response: 9647150
Conc: 5.42 ng/ml