

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111225\
 Data File : PS032369.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2025 09:52
 Operator : AR\AJ
 Sample : Q3598-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 EO-CONCRETE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 21:07:18 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.283	7.617	1088.5E6	1208.5E6	240.225	331.506 #
Target Compounds							
1) T	Dalapon	2.635	2.611	2488.5E6	3927.8E6	346.651	564.830 #
2) T	3,5-DICHL...	6.436	6.585	1041393	4359541	<MDL	<MDL #
5) T	DICAMBA	7.479	0.000	42753565	0	2.266	N.D. #
6) T	MCP	7.670f	7.866f	10831515	25768215	<MDL	1.937 #
7) T	MCPA	7.795	8.192f	159.7E6	-6884639	11.898	N.D. #
8) T	DICHLORPROP	8.190	8.486f	11400581	19150695	2.563	4.016 #
9) T	2,4-D	8.398	8.892f	28243474	9965477	6.260	1.900 #
10) T	Pentachlo...	8.696	9.361	12006082	35806508	<MDL	<MDL #
11) T	2,4,5-TP ...	9.330f	9.739	56171779	129.8E6	2.159	4.832 #
12) T	2,4,5-T	9.606f	10.182	50785440	297.6E6	2.130	12.549 #
13) T	2,4-DB	10.181f	0.000	668.4E6	0	253.649	N.D. #
14) T	DINOSEB	11.338	11.129	154.4E6	93351579	7.420	5.278 #
15) T	Picloram	11.156f	12.249f	6014260	1232.0E6	<MDL	33.134 #
16) T	DCPA	11.611f	12.137	93016562	13276428	2.772	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111225\
Data File : PS032369.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2025 09:52
Operator : AR\AJ
Sample : Q3598-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
EO-CONCRETE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 21:07:18 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

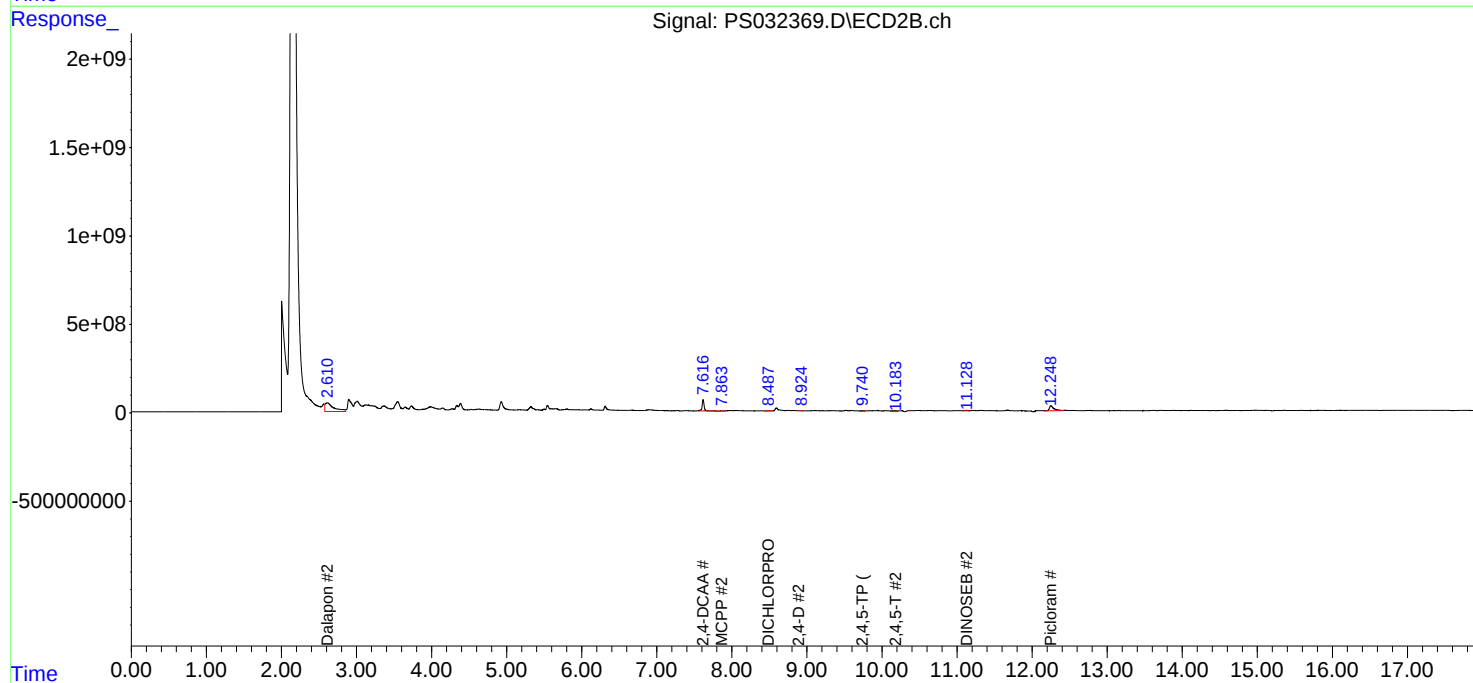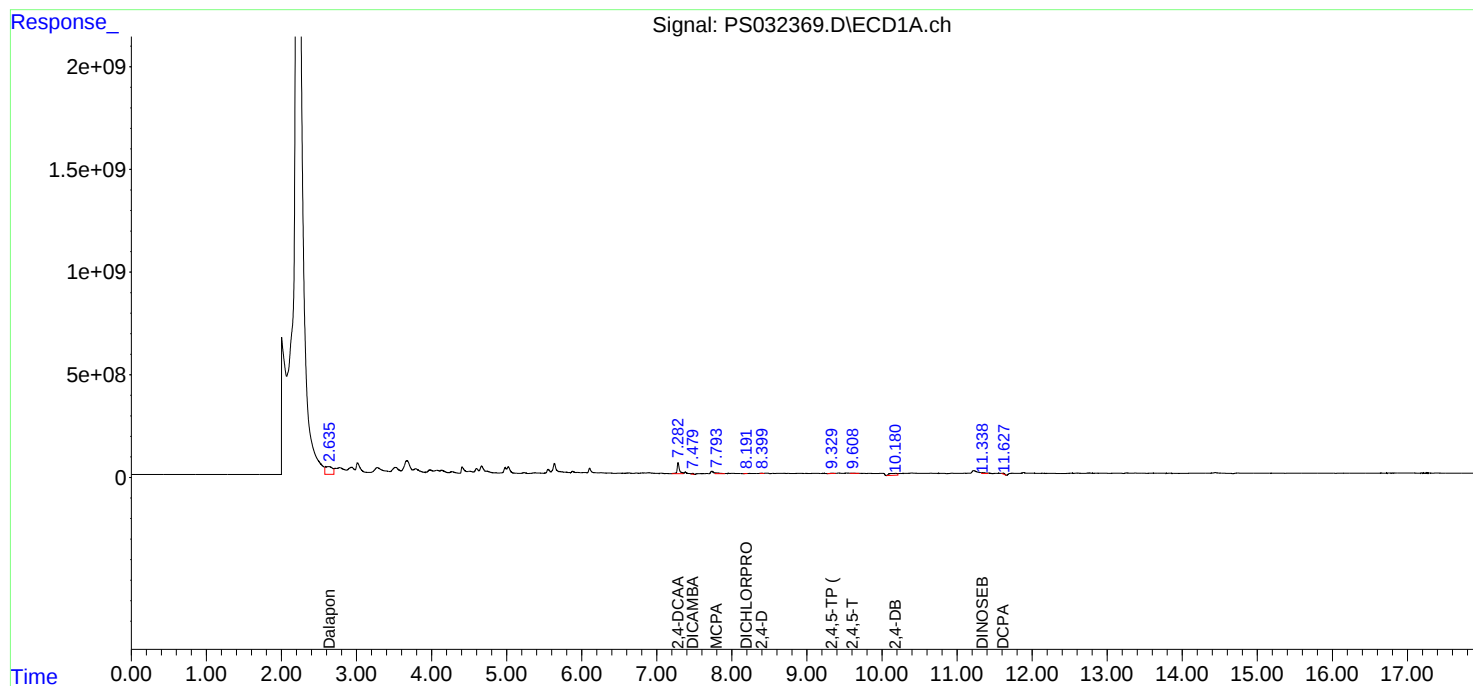


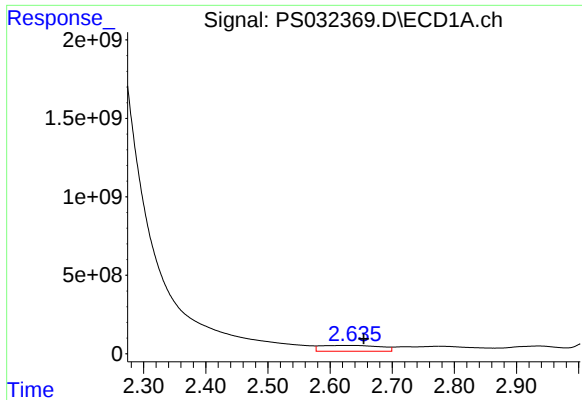

#1 Dalapon


R.T.: 2.635 min
Delta R.T.: -0.019 min
Response: 2488527341
Conc: 346.65 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-CONCRETE

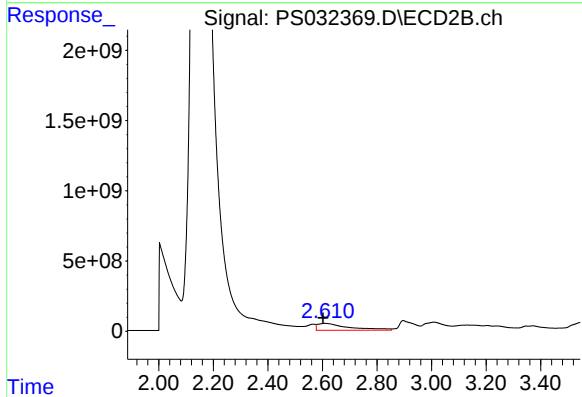


#1 Dalapon

R.T.: 2.611 min
Delta R.T.: 0.008 min
Response: 3927827162
Conc: 564.83 ng/ml

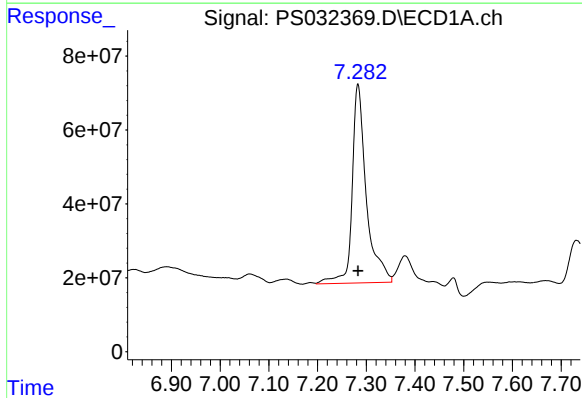


#4 2,4-DCAA

R.T.: 7.283 min
Delta R.T.: 0.000 min
Response: 1088526031
Conc: 240.23 ng/ml

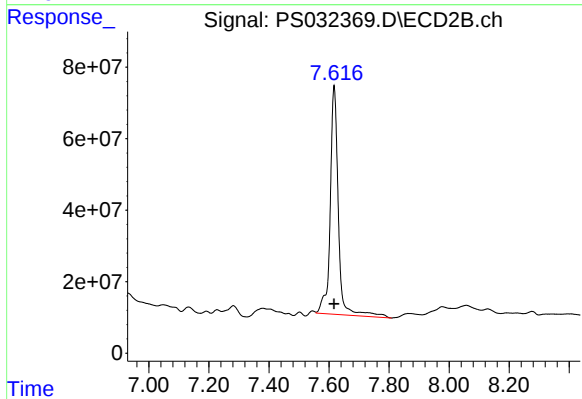

#4 2,4-DCAA


R.T.: 7.617 min
Delta R.T.: 0.000 min
Response: 1208503378
Conc: 331.51 ng/ml

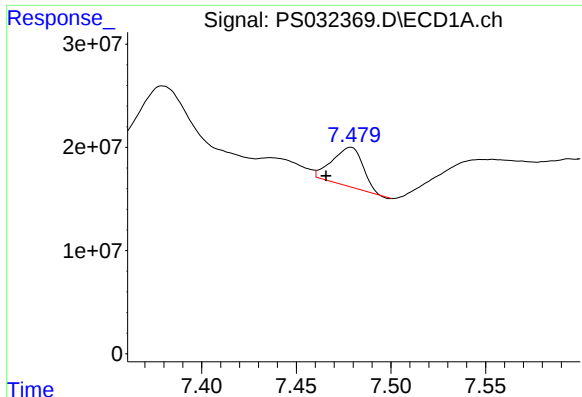

#5 DICAMBA


R.T.: 7.479 min
Delta R.T.: 0.013 min
Response: 42753565
Conc: 2.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-CONCRETE

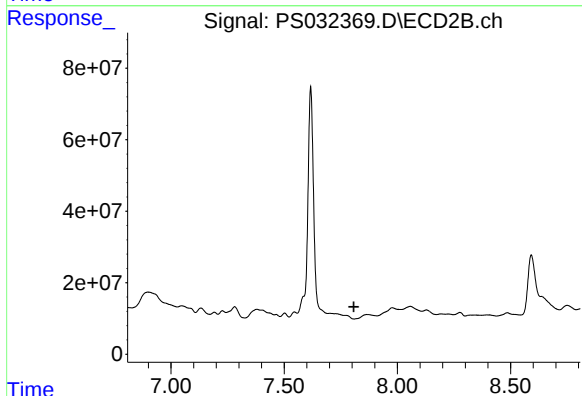


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.808 min
Response: 0
Conc: N.D.

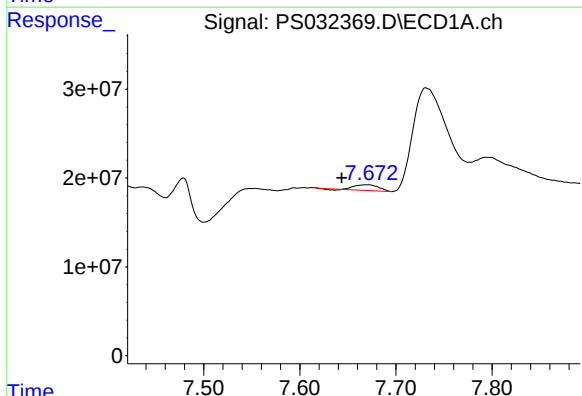


#6 MCP

R.T.: 7.670 min
Delta R.T.: 0.026 min
Response: 10831515
Conc: N.D.

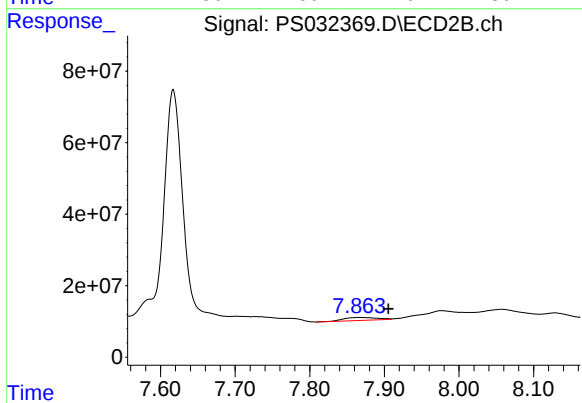

#6 MCP


R.T.: 7.866 min
Delta R.T.: -0.040 min
Response: 25768215
Conc: 1.94 ug/ml

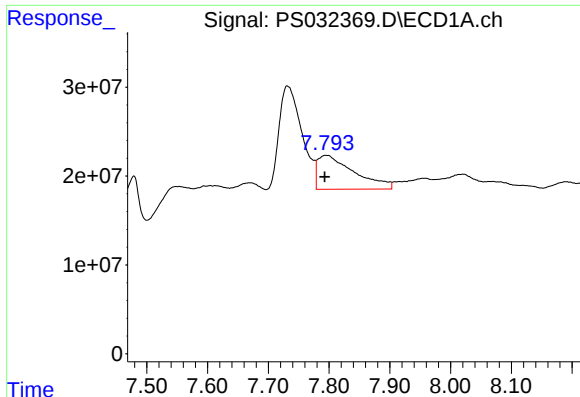

#7 MCPA


R.T.: 7.795 min
Delta R.T.: 0.003 min
Response: 159736089
Conc: 11.90 ug/ml

Instrument :
ECD_S
ClientSampleId :
EO-CONCRETE

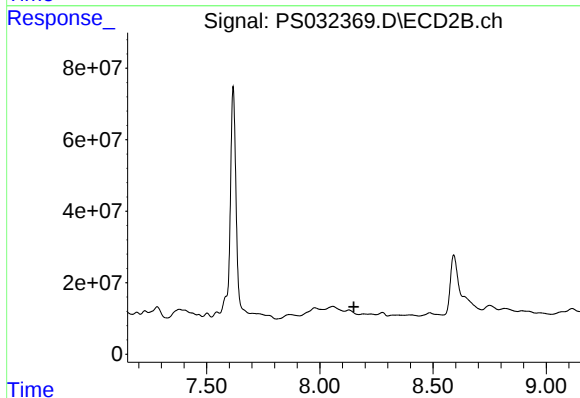


#7 MCPA

R.T.: 8.192 min
Delta R.T.: 0.042 min
Response: -6884639
Conc: N.D.

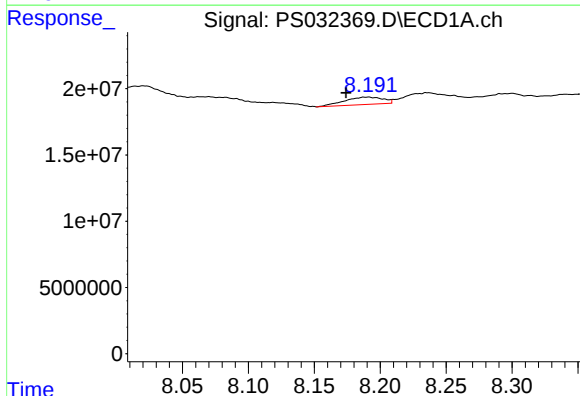


#8 DICHLORPROP

R.T.: 8.190 min
Delta R.T.: 0.016 min
Response: 11400581
Conc: 2.56 ng/ml

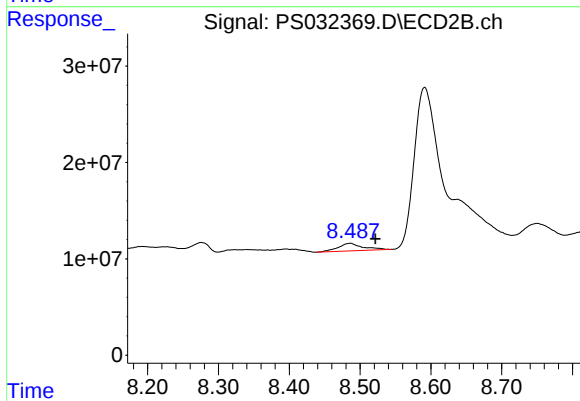

#8 DICHLORPROP


R.T.: 8.486 min
Delta R.T.: -0.036 min
Response: 19150695
Conc: 4.02 ng/ml

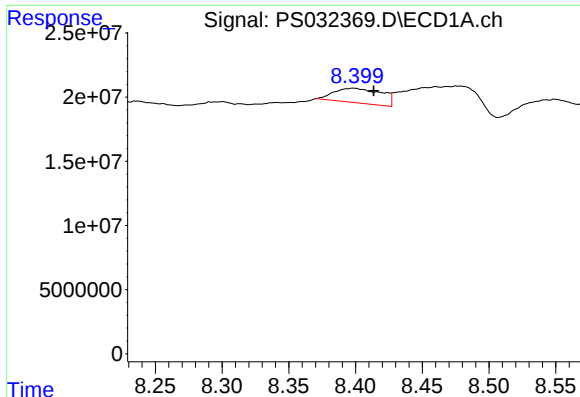

#9 2,4-D


R.T.: 8.398 min
Delta R.T.: -0.016 min
Response: 28243474
Conc: 6.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-CONCRETE

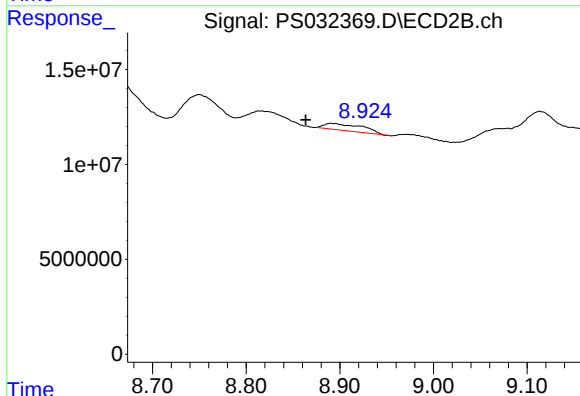


#9 2,4-D

R.T.: 8.892 min
Delta R.T.: 0.028 min
Response: 9965477
Conc: 1.90 ng/ml

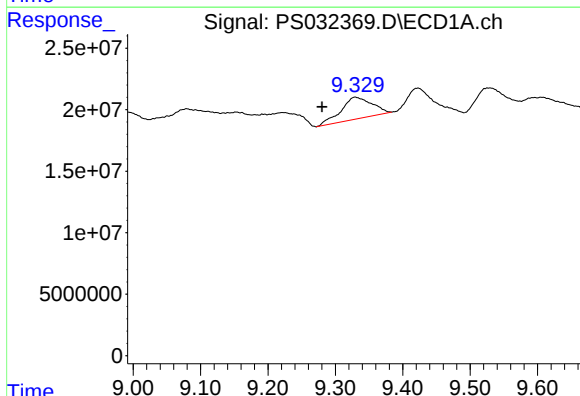


#11 2,4,5-TP (SILVEX)

R.T.: 9.330 min
Delta R.T.: 0.049 min
Response: 56171779
Conc: 2.16 ng/ml

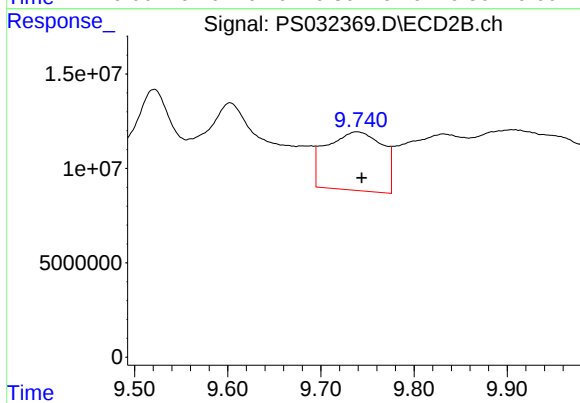

#11 2,4,5-TP (SILVEX)


R.T.: 9.739 min
Delta R.T.: -0.005 min
Response: 129756903
Conc: 4.83 ng/ml

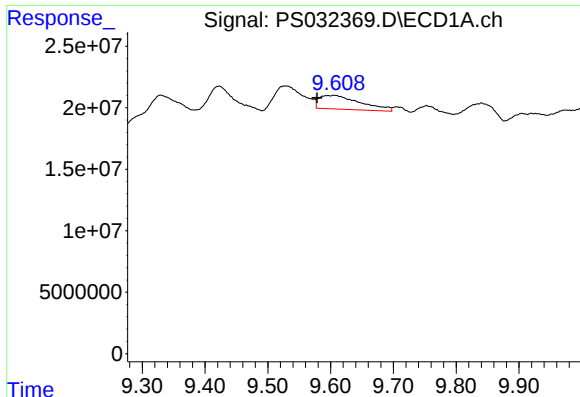

#12 2,4,5-T


R.T.: 9.606 min
Delta R.T.: 0.028 min
Response: 50785440
Conc: 2.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-CONCRETE

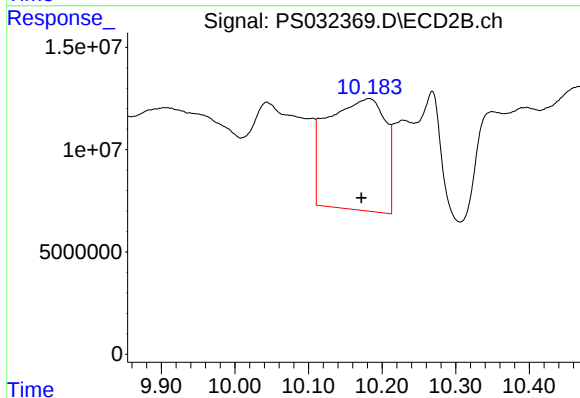


#12 2,4,5-T

R.T.: 10.182 min
Delta R.T.: 0.010 min
Response: 297639237
Conc: 12.55 ng/ml

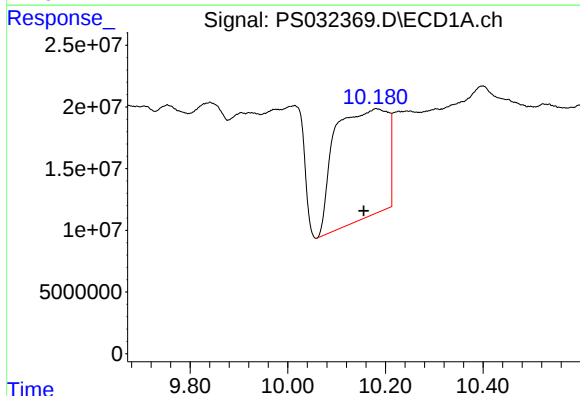


#13 2,4-DB

R.T.: 10.181 min
Delta R.T.: 0.026 min
Response: 668393808
Conc: 253.65 ng/ml

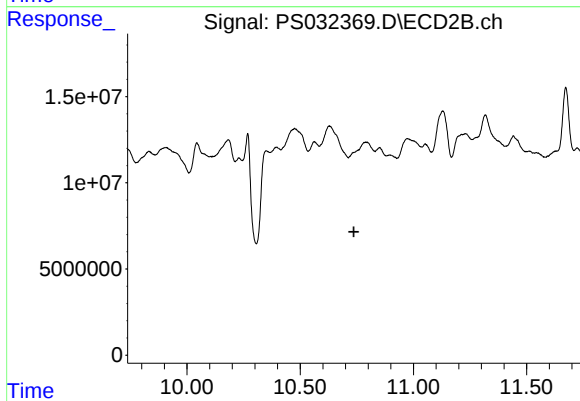

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.737 min
Response: 0
Conc: N.D.

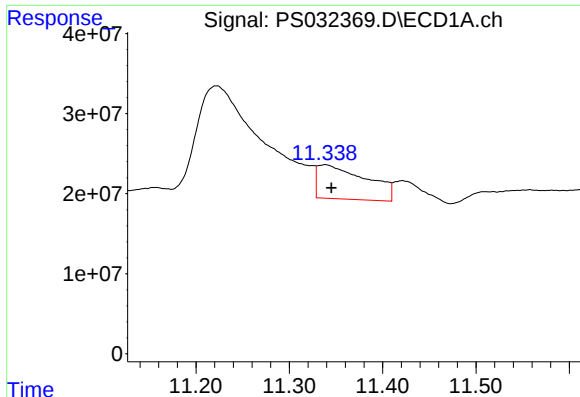

#14 DINOSEB


R.T.: 11.338 min
Delta R.T.: -0.007 min
Response: 154393778
Conc: 7.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-CONCRETE

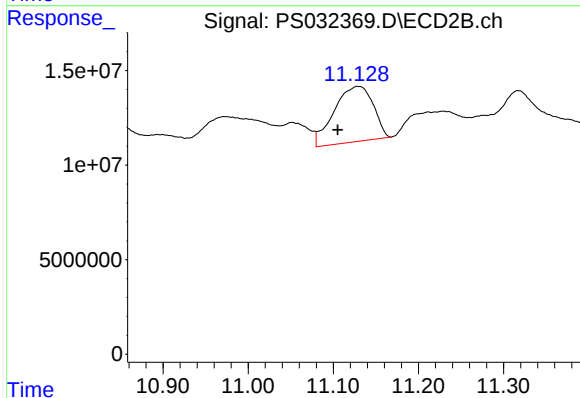


#14 DINOSEB

R.T.: 11.129 min
Delta R.T.: 0.024 min
Response: 93351579
Conc: 5.28 ng/ml

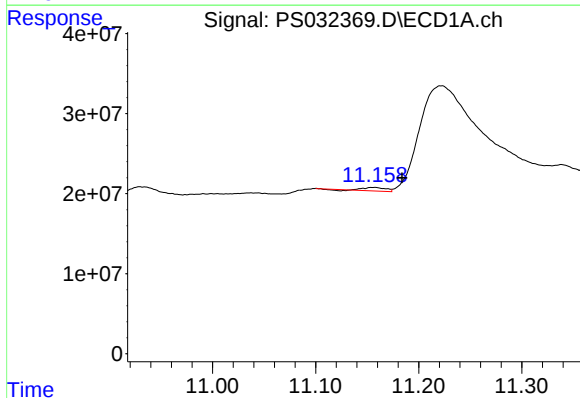


#15 Picloram

R.T.: 11.156 min
Delta R.T.: -0.028 min
Response: 6014260
Conc: N.D.

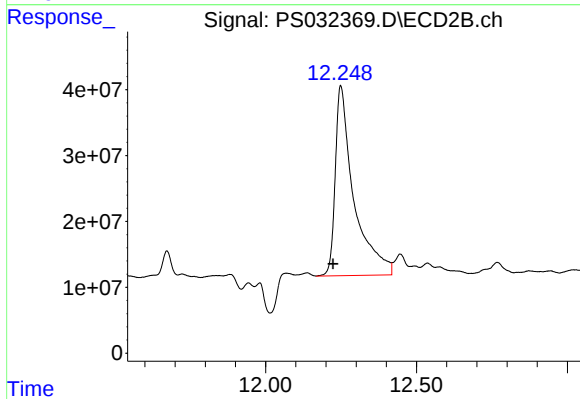

#15 Picloram


R.T.: 12.249 min
Delta R.T.: 0.026 min
Response: 1231988623
Conc: 33.13 ng/ml

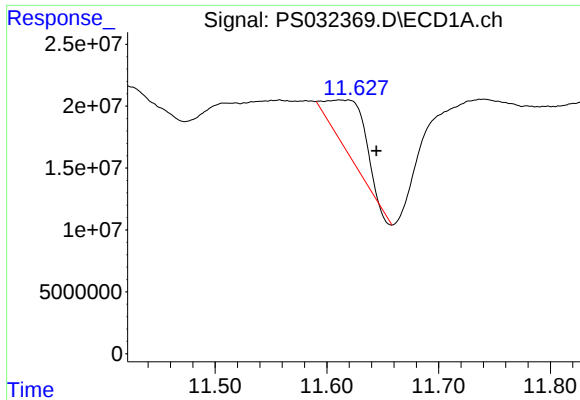

#16 DCPA

R.T.: 11.611 min
Delta R.T.: -0.033 min
Response: 93016562
Conc: 2.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-CONCRETE

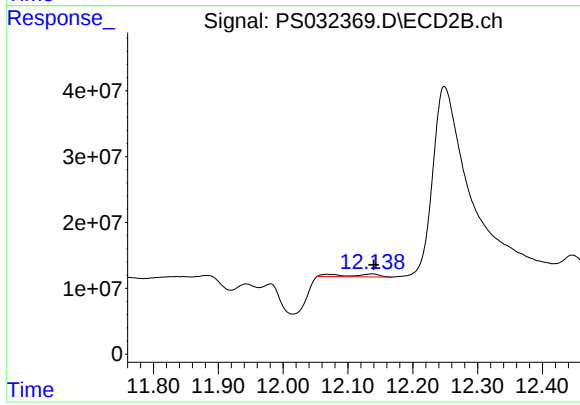

#16 DCPA

R.T.: 12.137 min
Delta R.T.: -0.002 min
Response: 13276428
Conc: N.D.