

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111225\
 Data File : PS032373.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2025 14:20
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 21:09:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.285	7.616	1848.9E6	1992.0E6	408.029	546.440 #
Target Compounds							
2) T	3,5-DICHL...	6.442	6.604	20378594	5124572	3.152	<MDL #
3) T	4-Nitroph...	7.135f	0.000	433543	0	<MDL	N.D. #
6) T	MCP	7.660	7.902	-129535	43511165	N.D.	3.271
7) T	MCPA	7.791	0.000	1737840	0	<MDL	N.D. #
8) T	DICHLORPROP	8.193	0.000	2558522	0	<MDL	N.D. #
9) T	2,4-D	8.446f	0.000	57885811	0	12.830	N.D. #
10) T	Pentachlo...	8.708	9.358	7606592	3910459	<MDL	<MDL #
11) T	2,4,5-TP ...	9.281	9.774f	2492281	2071004	<MDL	<MDL #
12) T	2,4,5-T	9.574	10.141f	924768	9409902	<MDL	<MDL #
13) T	2,4-DB	10.153	0.000	556440	0	<MDL	N.D. #
14) T	DINOSEB	11.349	11.113	8756554	2352083	<MDL	<MDL #
15) T	Picloram	11.197	0.000	17608233	0	<MDL	N.D. #
16) T	DCPA	11.648	12.171f	4578685	50798322	<MDL	1.594 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111225\
Data File : PS032373.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2025 14:20
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 21:09:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

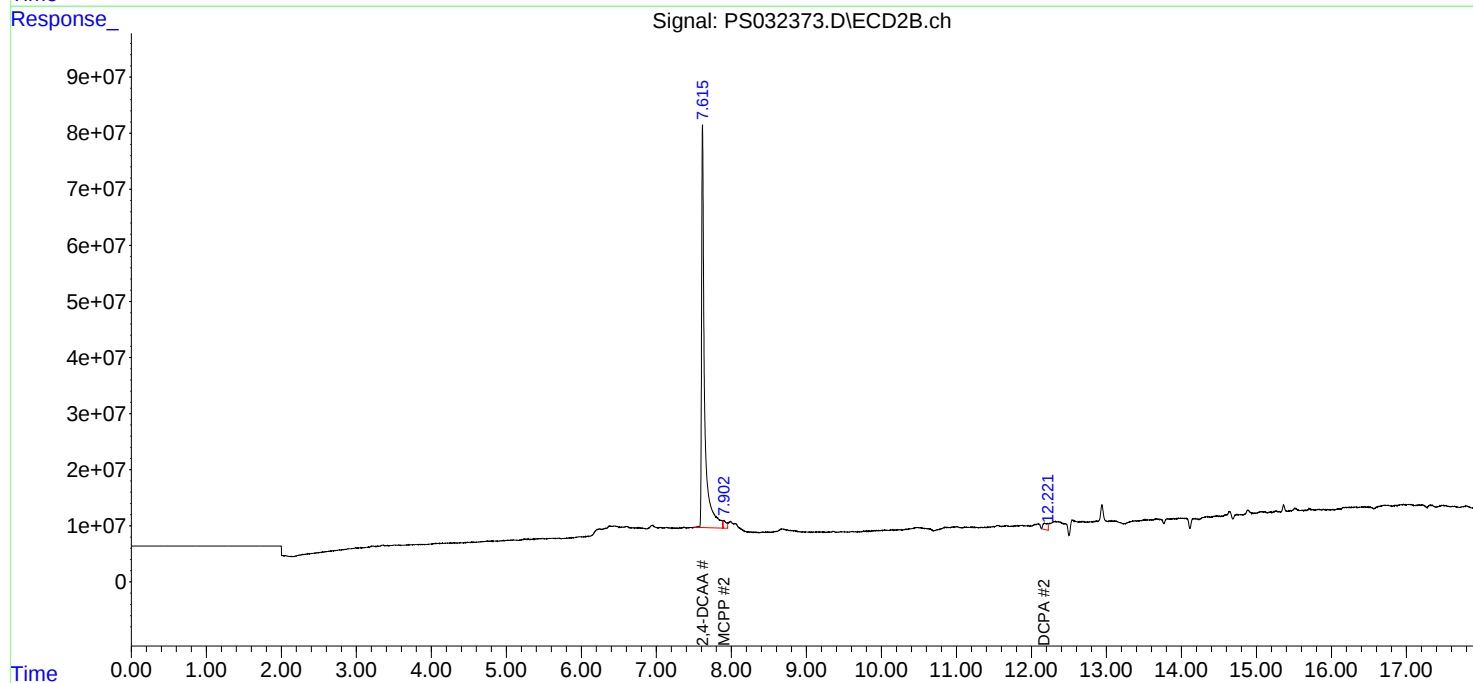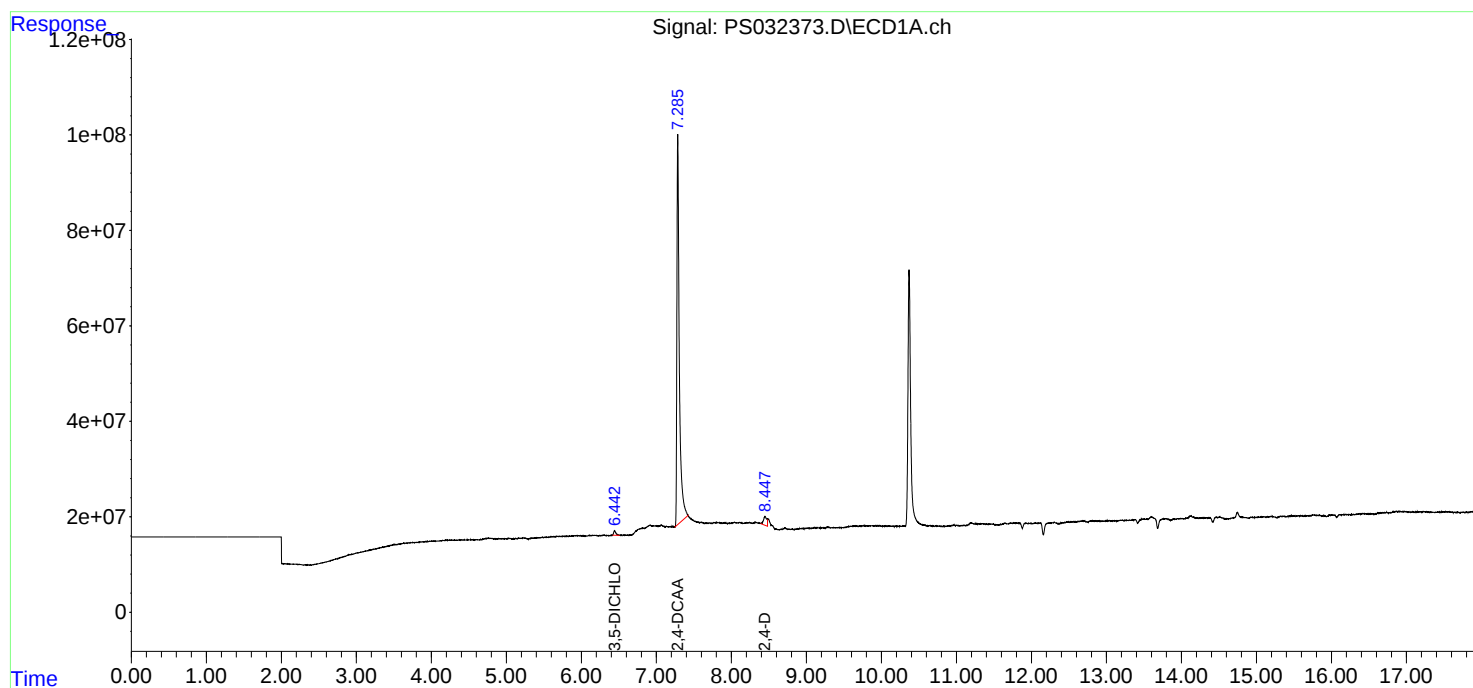


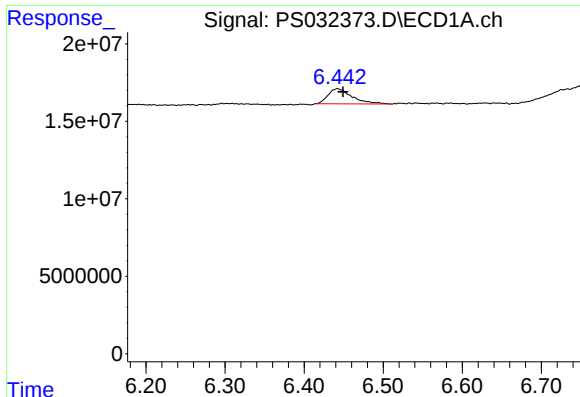

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.442 min
Delta R.T.: -0.007 min
Response: 20378594
Conc: 3.15 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

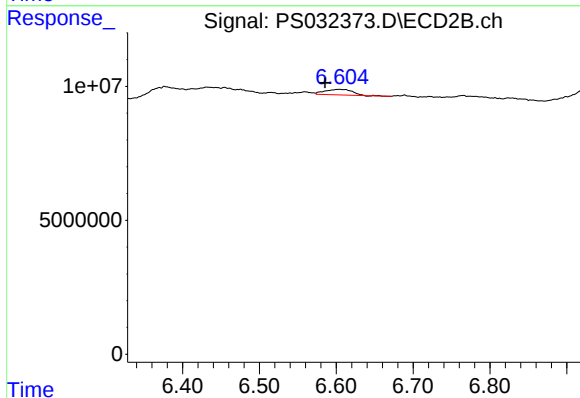


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.604 min
Delta R.T.: 0.019 min
Response: 5124572
Conc: N.D.

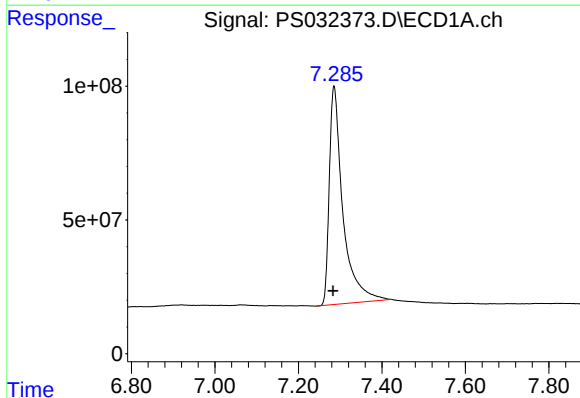


#4 2,4-DCAA

R.T.: 7.285 min
Delta R.T.: 0.002 min
Response: 1848890454
Conc: 408.03 ng/ml

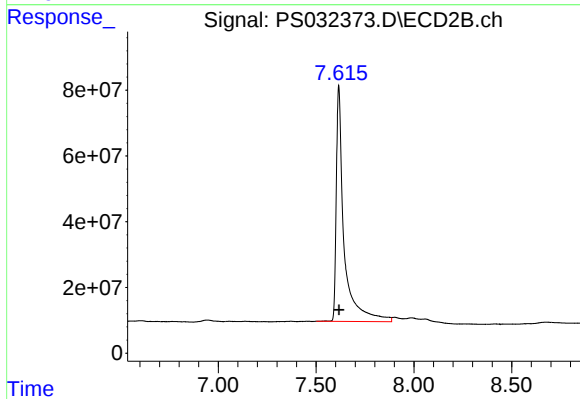

#4 2,4-DCAA


R.T.: 7.616 min
Delta R.T.: -0.002 min
Response: 1992045976
Conc: 546.44 ng/ml

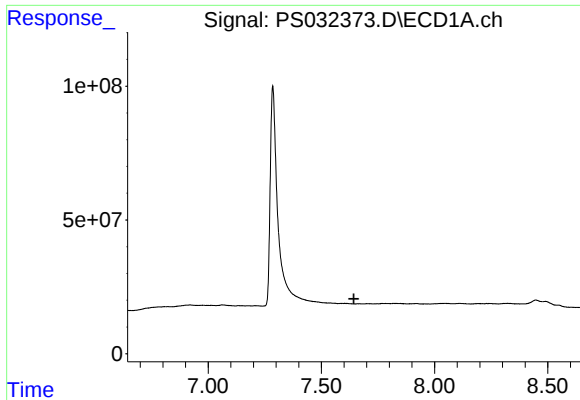

#6 MCPP


R.T.: 7.660 min
Delta R.T.: 0.017 min
Response: -129535
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

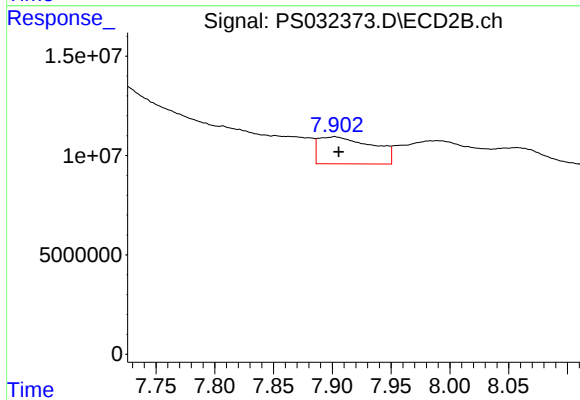


#6 MCPP

R.T.: 7.902 min
Delta R.T.: -0.004 min
Response: 43511165
Conc: 3.27 ug/ml

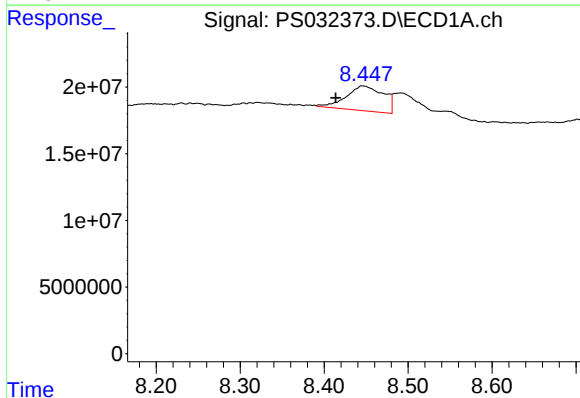


#9 2,4-D

R.T.: 8.446 min
Delta R.T.: 0.032 min
Response: 57885811
Conc: 12.83 ng/ml

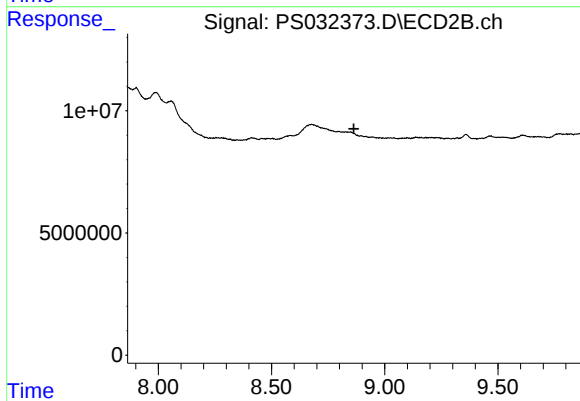

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.864 min
Response: 0
Conc: N.D.

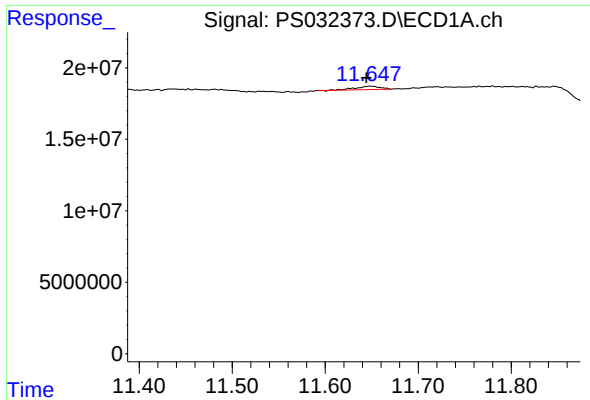

#16 DCPA

R.T.: 11.648 min
Delta R.T.: 0.004 min
Response: 4578685
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

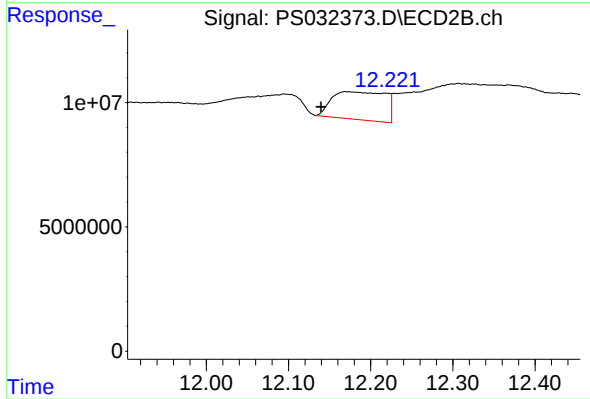

#16 DCPA

R.T.: 12.171 min
Delta R.T.: 0.031 min
Response: 50798322
Conc: 1.59 ng/ml