

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111225\
 Data File : PS032381.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2025 19:40
 Operator : AR\AJ
 Sample : Q3601-13RX
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 21:15:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.266	7.635	7217945	46650381	1.593	12.797 #
Target Compounds							
1) T	Dalapon	2.627f	2.609	2372.5E6	2910.5E6	330.494	418.536 #
2) T	3,5-DICHL...	6.499f	6.554f	4945584	3010644	<MDL	<MDL #
3) T	4-Nitroph...	7.136f	7.191	6462467	-1051886	4.814	N.D. #
5) T	DICAMBA	7.490	0.000	15444496	0	<MDL	N.D. #
6) T	MCPD	7.663	7.888	6093946	19844840	<MDL	1.492 #
7) T	MCPA	7.753f	0.000	253.4E6	0	18.878	N.D. #
8) T	DICHLORPROP	8.157	0.000	266545	0	<MDL	N.D. #
9) T	2,4-D	8.399	8.841	53147224	-28623019	11.780	N.D. #
10) T	Pentachlo...	8.703	9.362	11079776	26392975	<MDL	<MDL #
11) T	2,4,5-TP ...	9.268	9.740	643616	52936993	<MDL	1.971 #
12) T	2,4,5-T	9.541f	10.189	-13377847	41738696	N.D.	1.760
13) T	2,4-DB	10.188f	10.743	58630744	44833582	22.250	11.888 #
14) T	DINOSEB	11.384f	11.137f	1431246	10363919	<MDL	<MDL #
15) T	Picloram	11.167	12.246	9381671	10585282	<MDL	<MDL #
16) T	DCPA	11.631	0.000	12794076	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111225\
Data File : PS032381.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2025 19:40
Operator : AR\AJ
Sample : Q3601-13RX
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 21:15:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

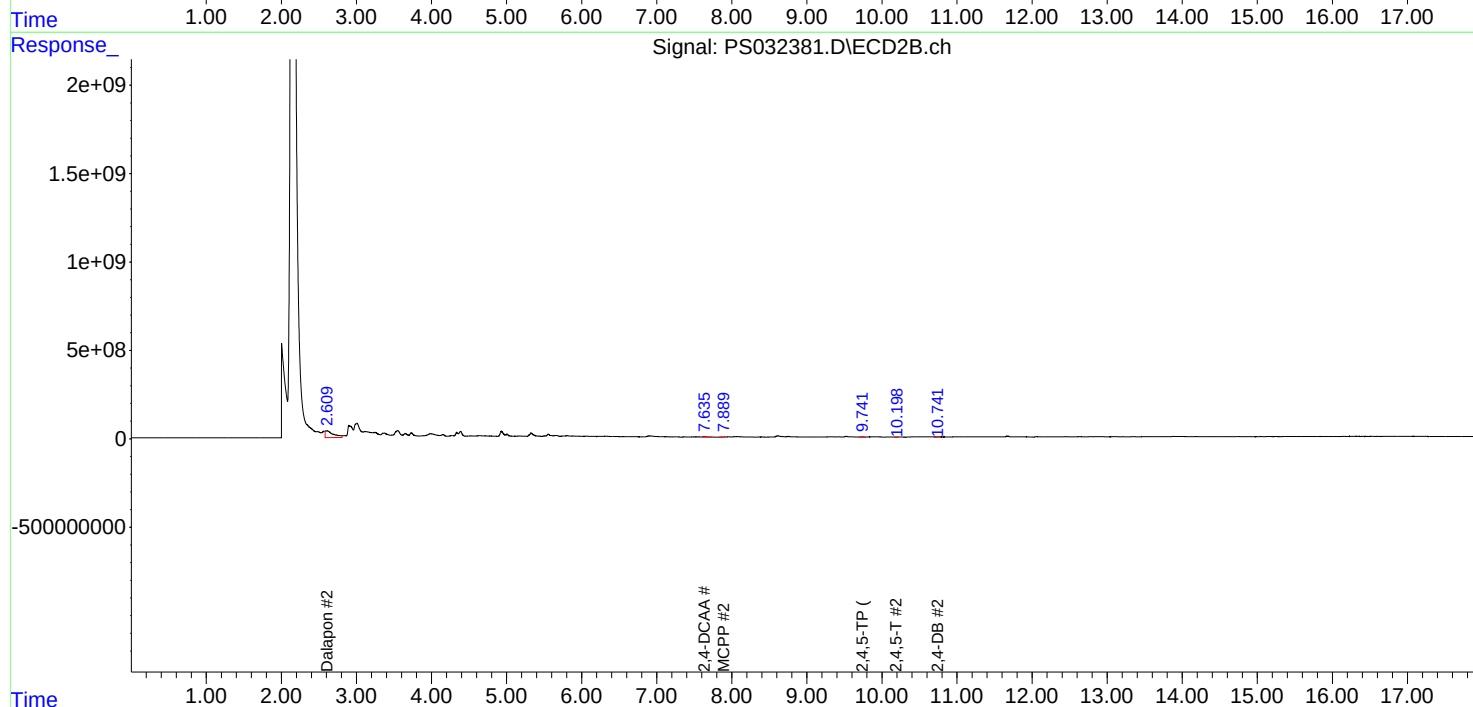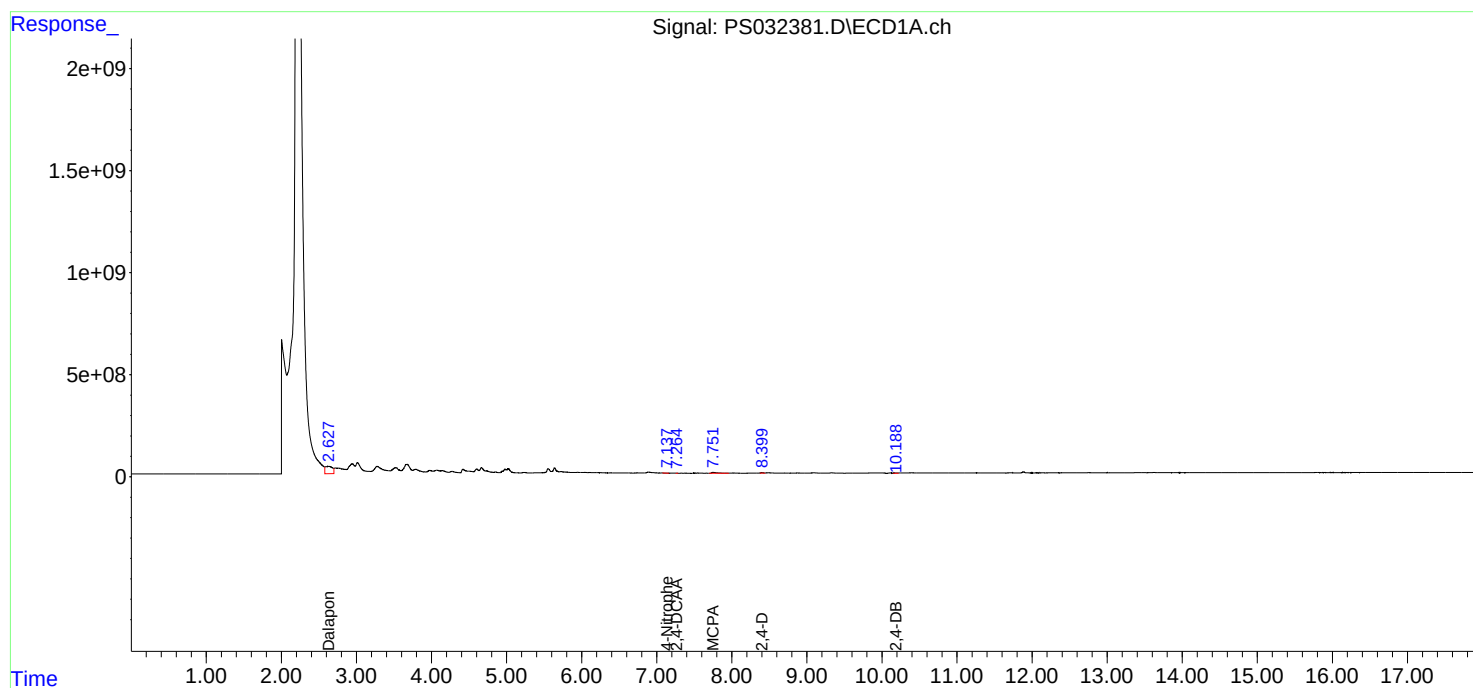


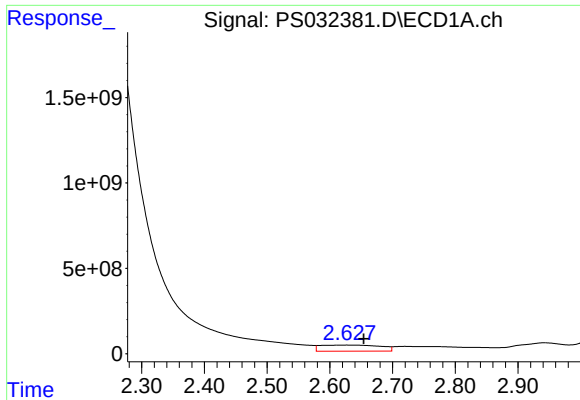

#1 Dalapon


R.T.: 2.627 min
Delta R.T.: -0.027 min
Response: 2372545252
Conc: 330.49 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-4

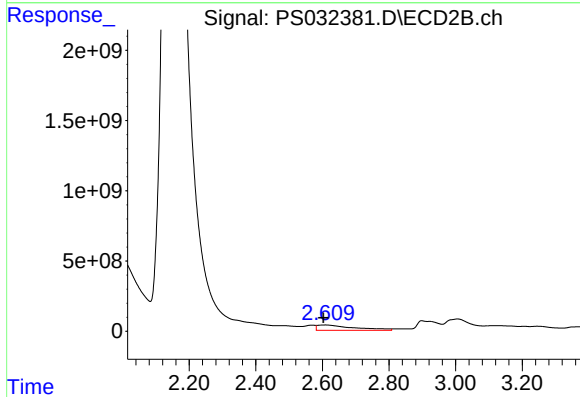


#1 Dalapon

R.T.: 2.609 min
Delta R.T.: 0.006 min
Response: 2910496371
Conc: 418.54 ng/ml

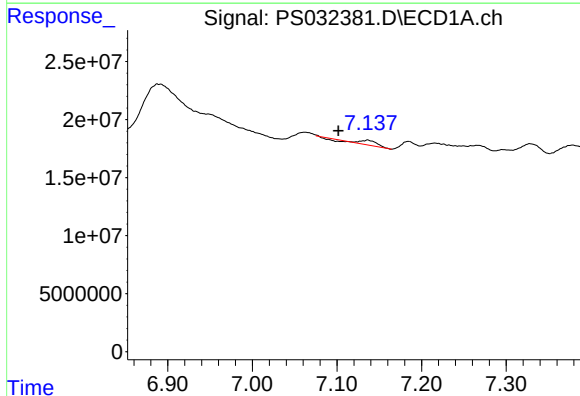


#3 4-Nitrophenol

R.T.: 7.136 min
Delta R.T.: 0.034 min
Response: 6462467
Conc: 4.81 ng/ml

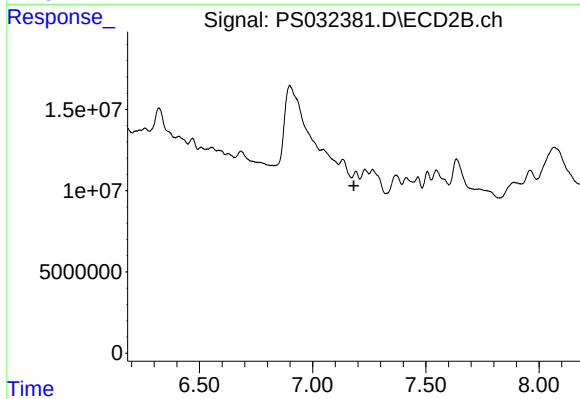

#3 4-Nitrophenol


R.T.: 7.191 min
Delta R.T.: 0.009 min
Response: -1051886
Conc: N.D.

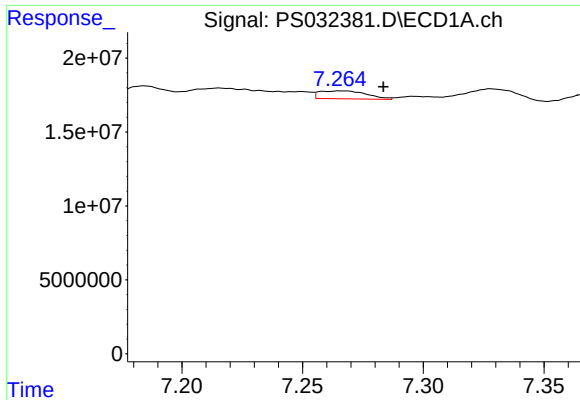

#4 2,4-DCAA


R.T.: 7.266 min
Delta R.T.: -0.018 min
Response: 7217945
Conc: 1.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-4

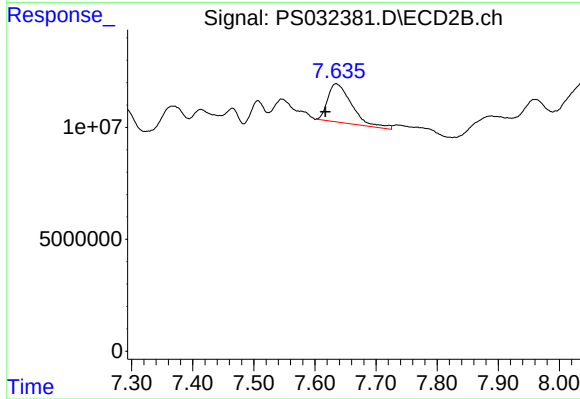


#4 2,4-DCAA

R.T.: 7.635 min
Delta R.T.: 0.018 min
Response: 46650381
Conc: 12.80 ng/ml

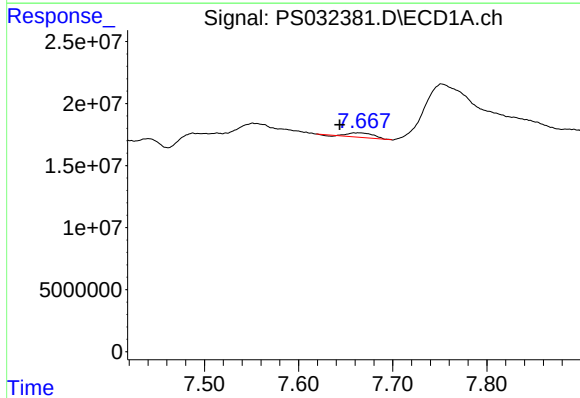


#6 MCP

R.T.: 7.663 min
Delta R.T.: 0.019 min
Response: 6093946
Conc: N.D.

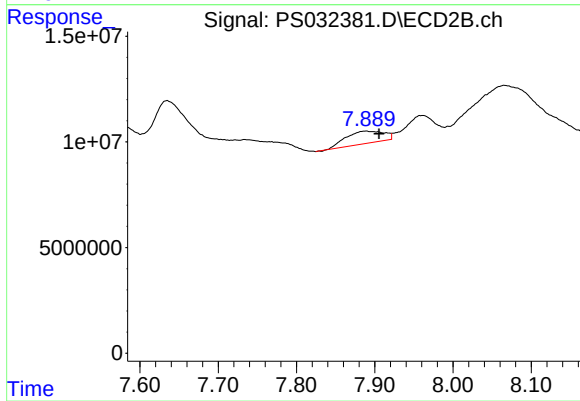

#6 MCP


R.T.: 7.888 min
Delta R.T.: -0.017 min
Response: 19844840
Conc: 1.49 ug/ml

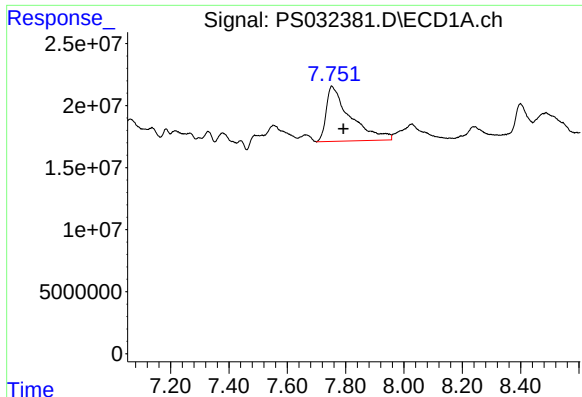

#7 MCPA


R.T.: 7.753 min
Delta R.T.: -0.040 min
Response: 253449482
Conc: 18.88 ug/ml

Instrument :
ECD_S
ClientSampleId :
TP-4

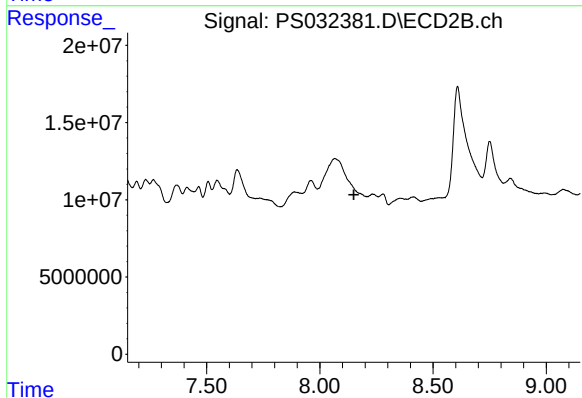


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

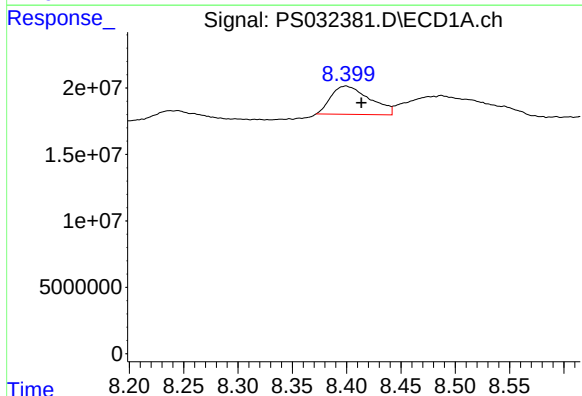


#9 2,4-D

R.T.: 8.399 min
Delta R.T.: -0.014 min
Response: 53147224
Conc: 11.78 ng/ml

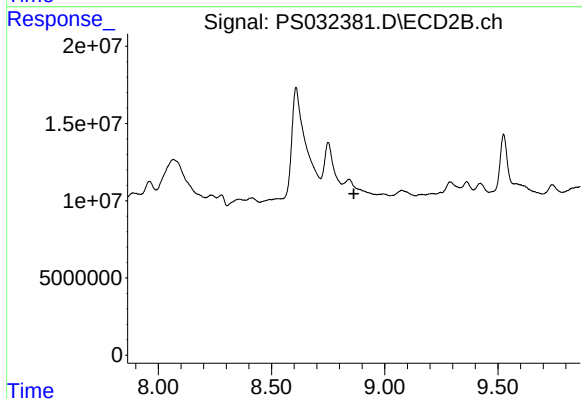

#9 2,4-D


R.T.: 8.841 min
Delta R.T.: -0.022 min
Response: -28623019
Conc: N.D.

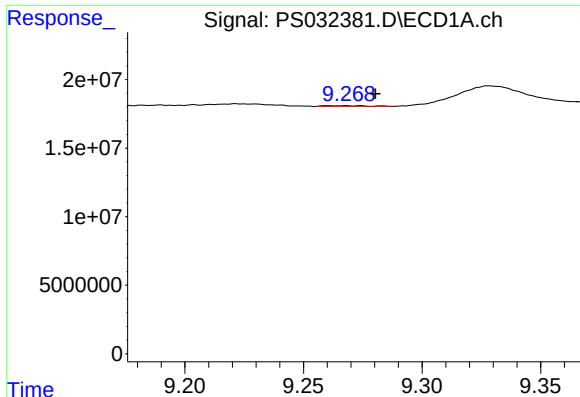

#11 2,4,5-TP (SILVEX)


R.T.: 9.268 min
Delta R.T.: -0.013 min
Response: 643616
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-4

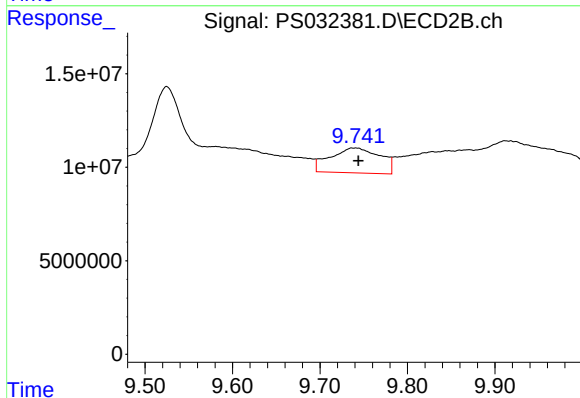


#11 2,4,5-TP (SILVEX)

R.T.: 9.740 min
Delta R.T.: -0.004 min
Response: 52936993
Conc: 1.97 ng/ml

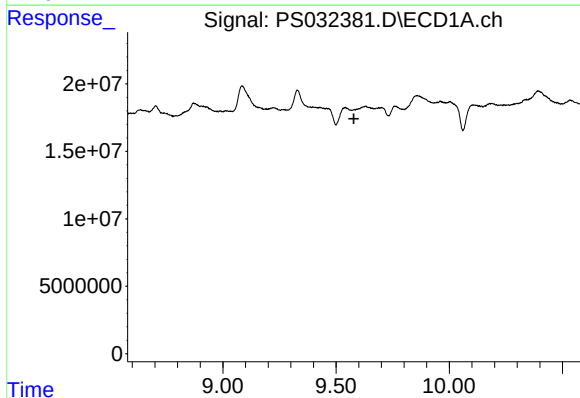


#12 2,4,5-T

R.T.: 9.541 min
Delta R.T.: -0.038 min
Response: -13377847
Conc: N.D.

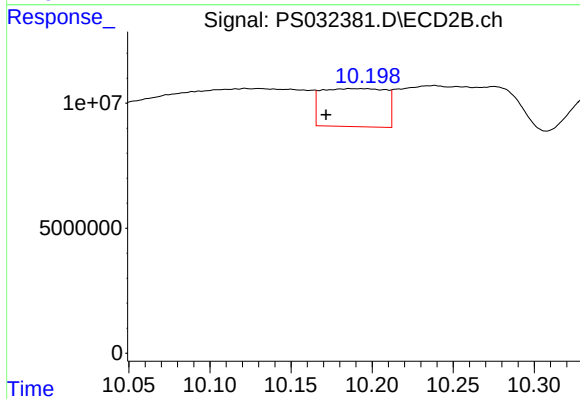

#12 2,4,5-T


R.T.: 10.189 min
Delta R.T.: 0.017 min
Response: 41738696
Conc: 1.76 ng/ml

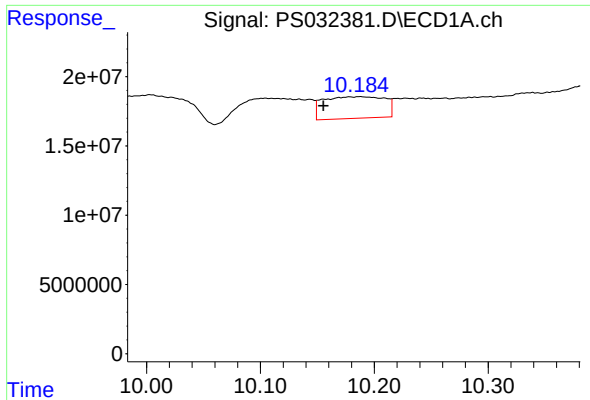

#13 2,4-DB

R.T.: 10.188 min
Delta R.T.: 0.033 min
Response: 58630744
Conc: 22.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-4

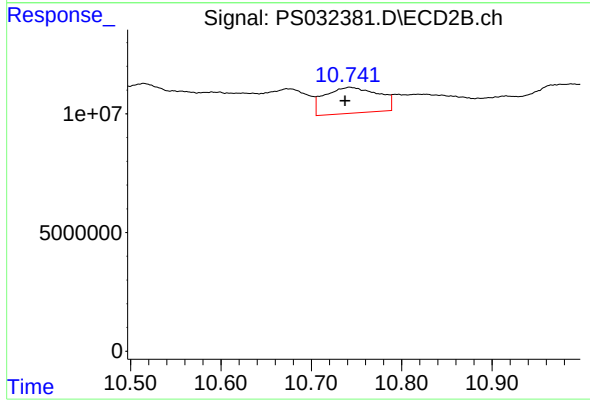

#13 2,4-DB

R.T.: 10.743 min
Delta R.T.: 0.006 min
Response: 44833582
Conc: 11.89 ng/ml