

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS111319\  
 Data File : PS007683.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 13 Nov 2019 08:49  
 Operator : SM\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 13 11:08:52 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS110619.M  
 Quant Title : 8080.M  
 QLast Update : Wed Nov 06 02:45:11 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound | RT#1  | RT#2  | Resp#1  | Resp#2   | ng/ml   | ng/ml    |
|-----------------------------|----------|-------|-------|---------|----------|---------|----------|
| -----                       |          |       |       |         |          |         |          |
| System Monitoring Compounds |          |       |       |         |          |         |          |
| 4) S                        | 2,4-DCAA | 5.410 | 0.000 | 588.7E6 | 0        | 427.433 | N.D. #   |
| Target Compounds            |          |       |       |         |          |         |          |
| 12) T                       | 2,4,5-T  | 0.000 | 7.215 | 0       | 23406501 | N.D.    | 6.338    |
| 15) T                       | Picloram | 8.967 | 8.891 | 101.1E6 | 85784941 | 9.102   | 14.642 # |
| 16) T                       | DCPA     | 0.000 | 8.891 | 0       | 85784941 | N.D.    | 16.417   |
| -----                       |          |       |       |         |          |         |          |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS111319\  
Data File : PS007683.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 13 Nov 2019 08:49  
Operator : SM\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampled :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 13 11:08:52 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS110619.M  
Quant Title : 8080.M  
QLast Update : Wed Nov 06 02:45:11 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

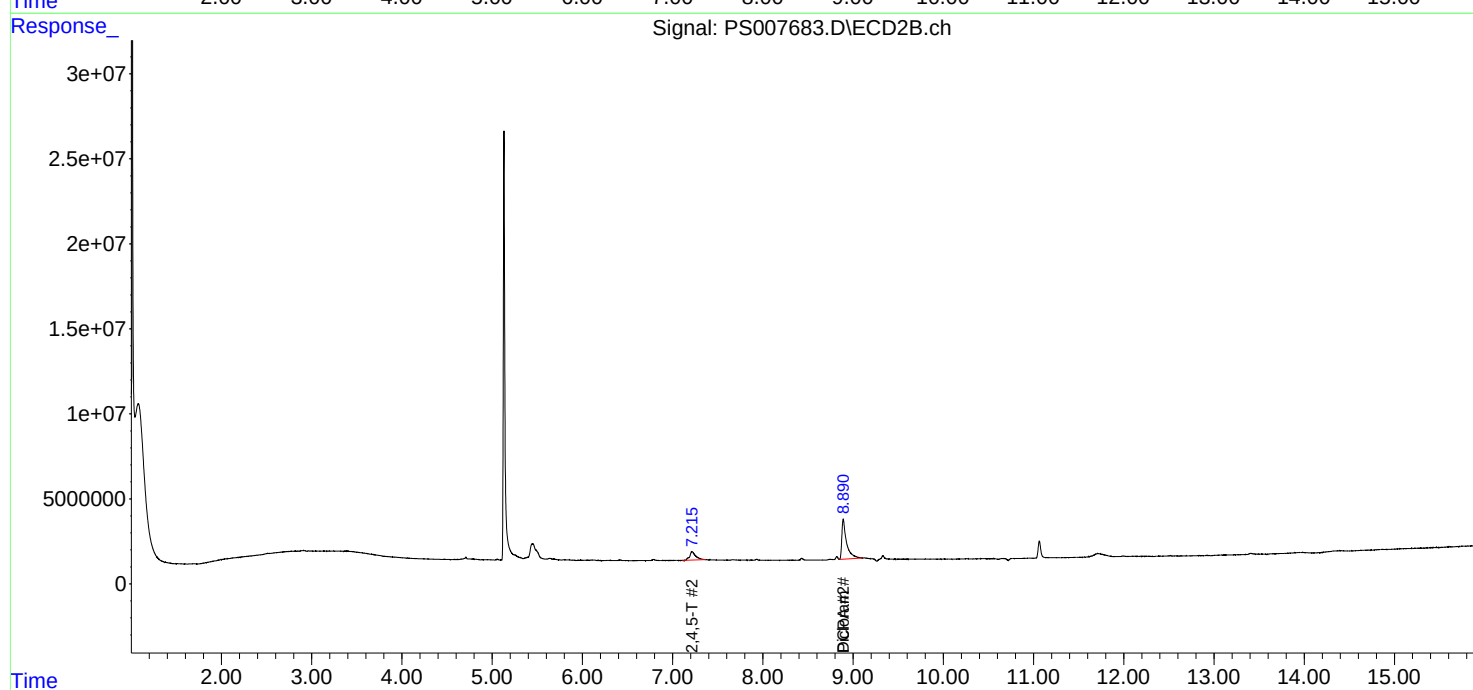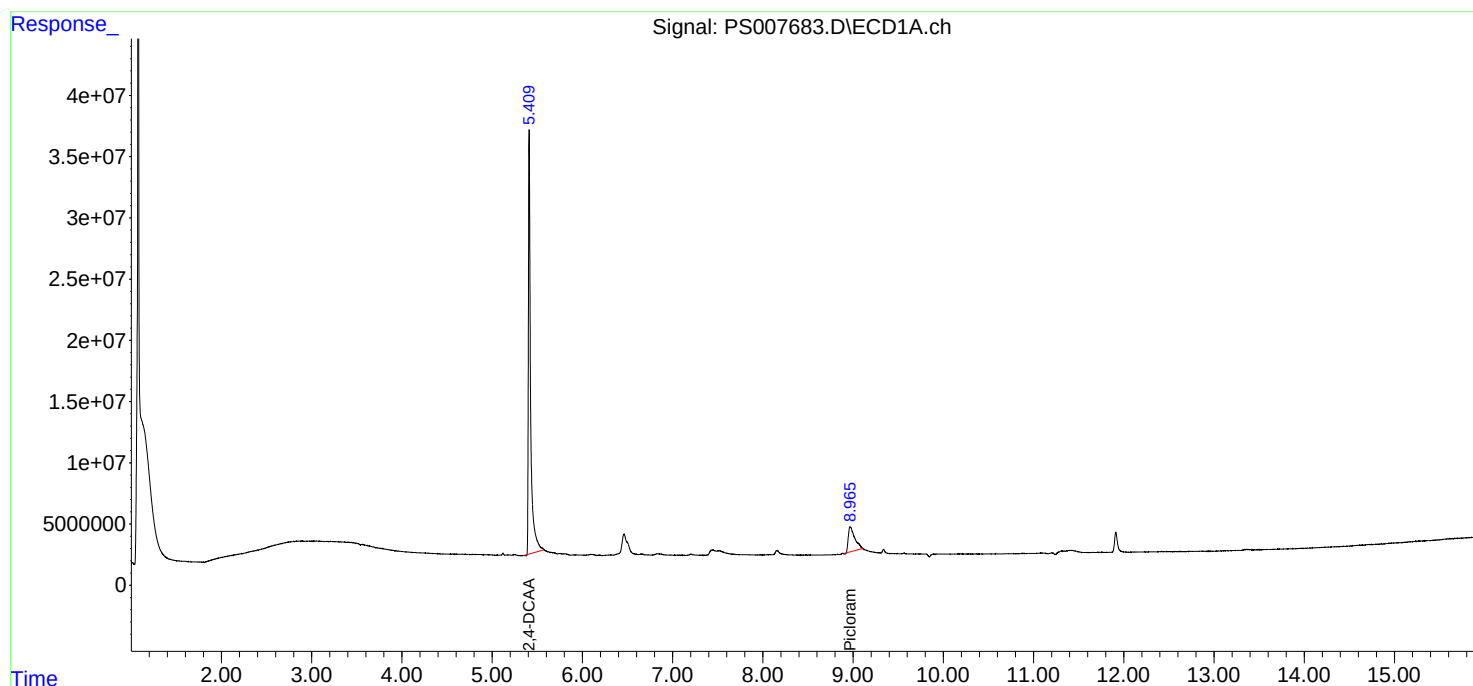


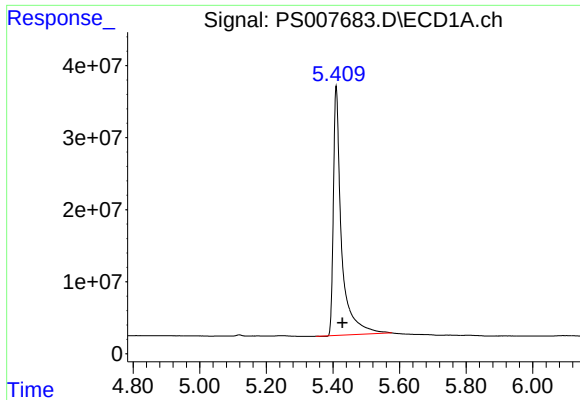

#4 2,4-DCAA


R.T.: 5.410 min  
Delta R.T.: -0.018 min  
Response: 588654354  
Conc: 427.43 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

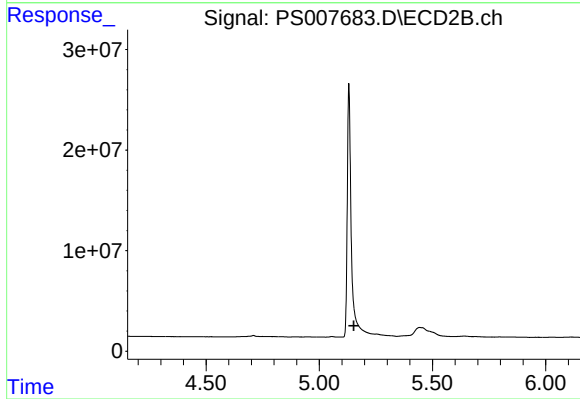


#4 2,4-DCAA

R.T.: 0.000 min  
Exp R.T. : 5.153 min  
Response: 0  
Conc: N.D.

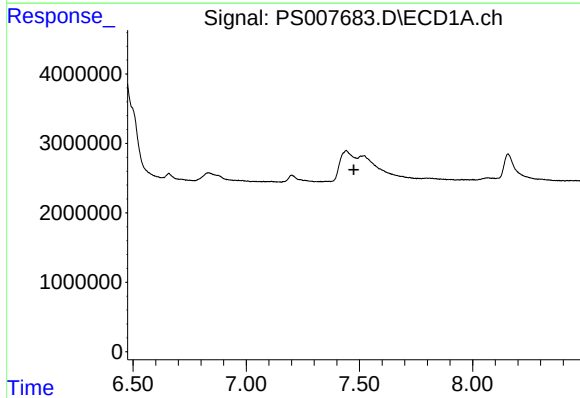


#12 2,4,5-T

R.T.: 0.000 min  
Exp R.T. : 7.475 min  
Response: 0  
Conc: N.D.

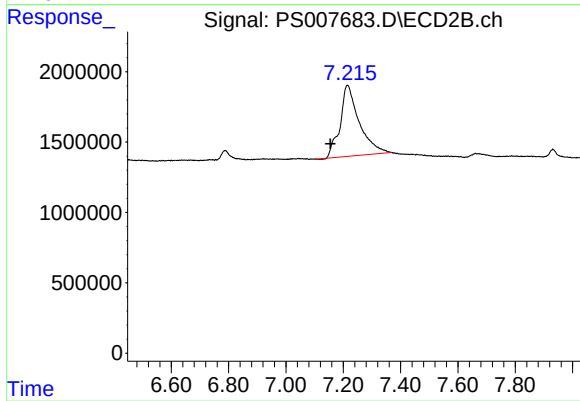

#12 2,4,5-T


R.T.: 7.215 min  
Delta R.T.: 0.059 min  
Response: 23406501  
Conc: 6.34 ng/ml

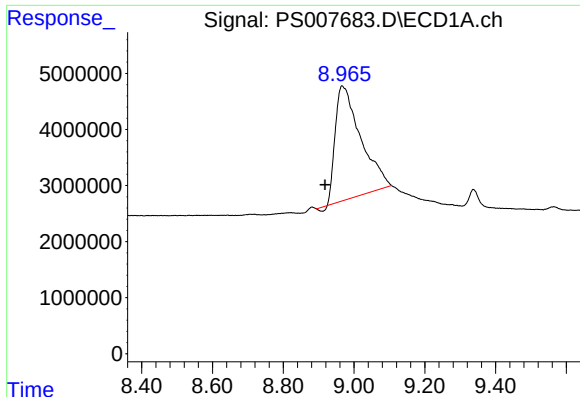

#15 Picloram


R.T.: 8.967 min  
Delta R.T.: 0.049 min  
Response: 101064366  
Conc: 9.10 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

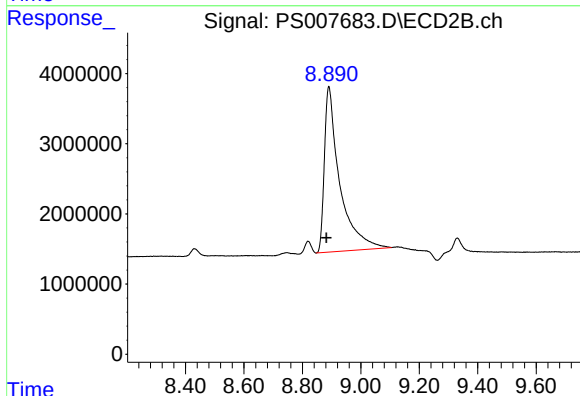


#15 Picloram

R.T.: 8.891 min  
Delta R.T.: 0.009 min  
Response: 85784941  
Conc: 14.64 ng/ml

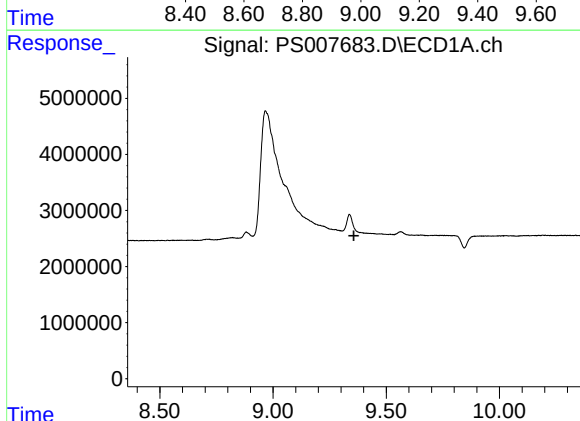

#16 DCPA

R.T.: 0.000 min  
Exp R.T. : 9.357 min  
Response: 0  
Conc: N.D.

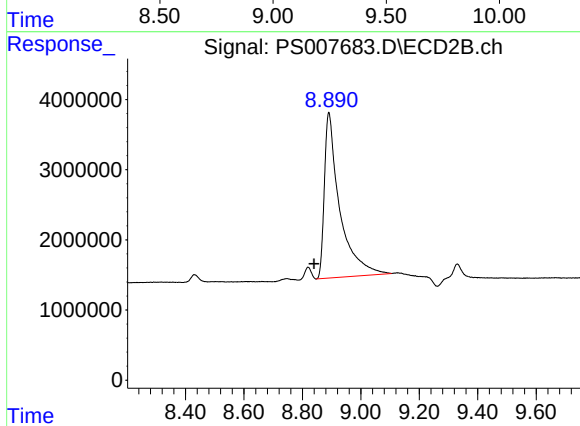

#16 DCPA

R.T.: 8.891 min  
Delta R.T.: 0.051 min  
Response: 85784941  
Conc: 16.42 ng/ml