

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111324\
 Data File : PS028487.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2024 11:20
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 13:42:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.240	7.741	1400.5E6	706.9E6	547.971	546.997
Target Compounds							
2) T	3,5-DICHL...	6.405	0.000	1061686	0	<MDL	N.D. #
3) T	4-Nitroph...	7.028	0.000	8598070	0	5.062	N.D. #
6) T	MCP	7.665f	0.000	15725017	0	2.235	N.D. #
7) T	MCPA	7.798f	8.258f	1341765	5564450	<MDL	<MDL #
8) T	DICHLORPROP	8.141	8.709f	215375	6169104	<MDL	4.224 #
12) T	2,4,5-T	9.502f	10.316	7513514	7905240	<MDL	<MDL #
13) T	2,4-DB	10.097	0.000	2151575	0	<MDL	N.D. #
14) T	DINOSEB	11.320	0.000	6184539	0	<MDL	N.D. #
15) T	Picloram	11.138	12.360	134.3E6	31055468	4.768	2.744 #
16) T	DCPA	11.615	12.360f	10754339	31055468	<MDL	3.202 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111324\
Data File : PS028487.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2024 11:20
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 13:42:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

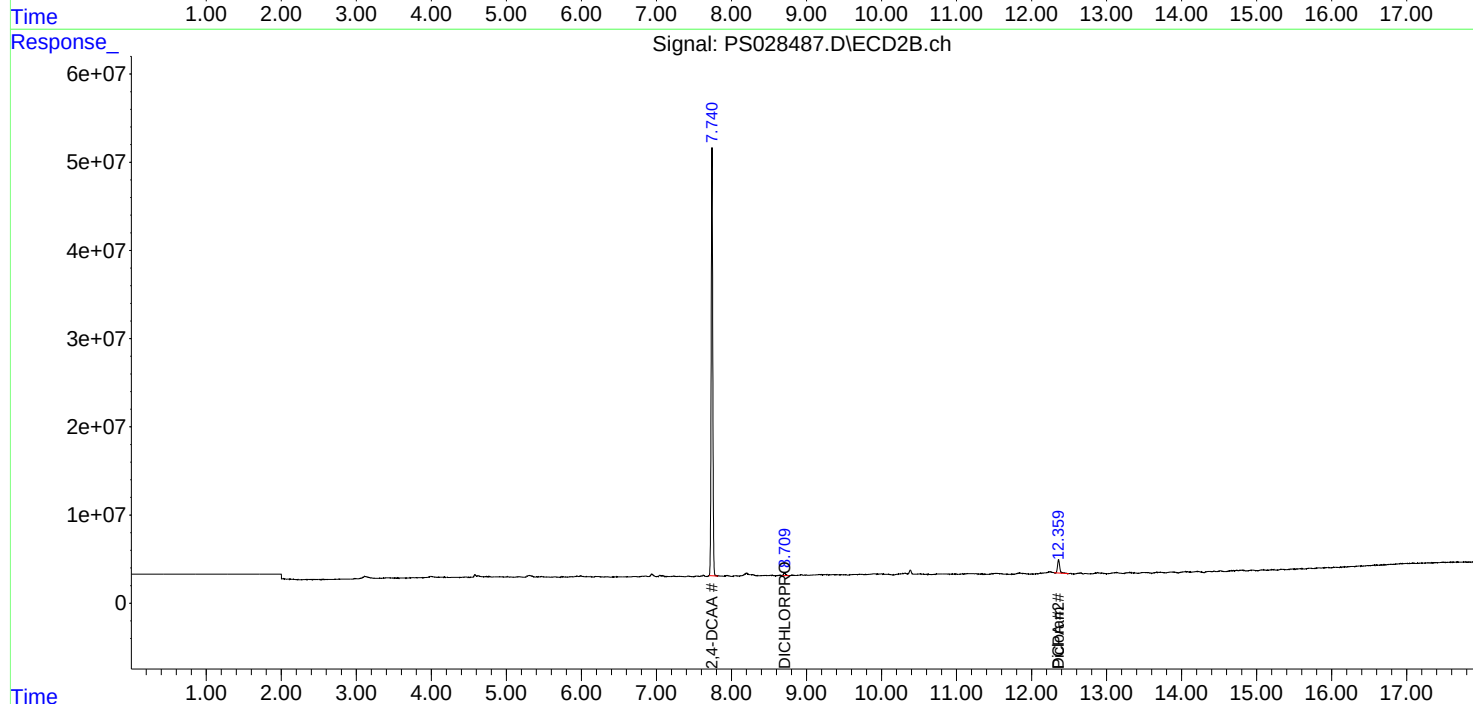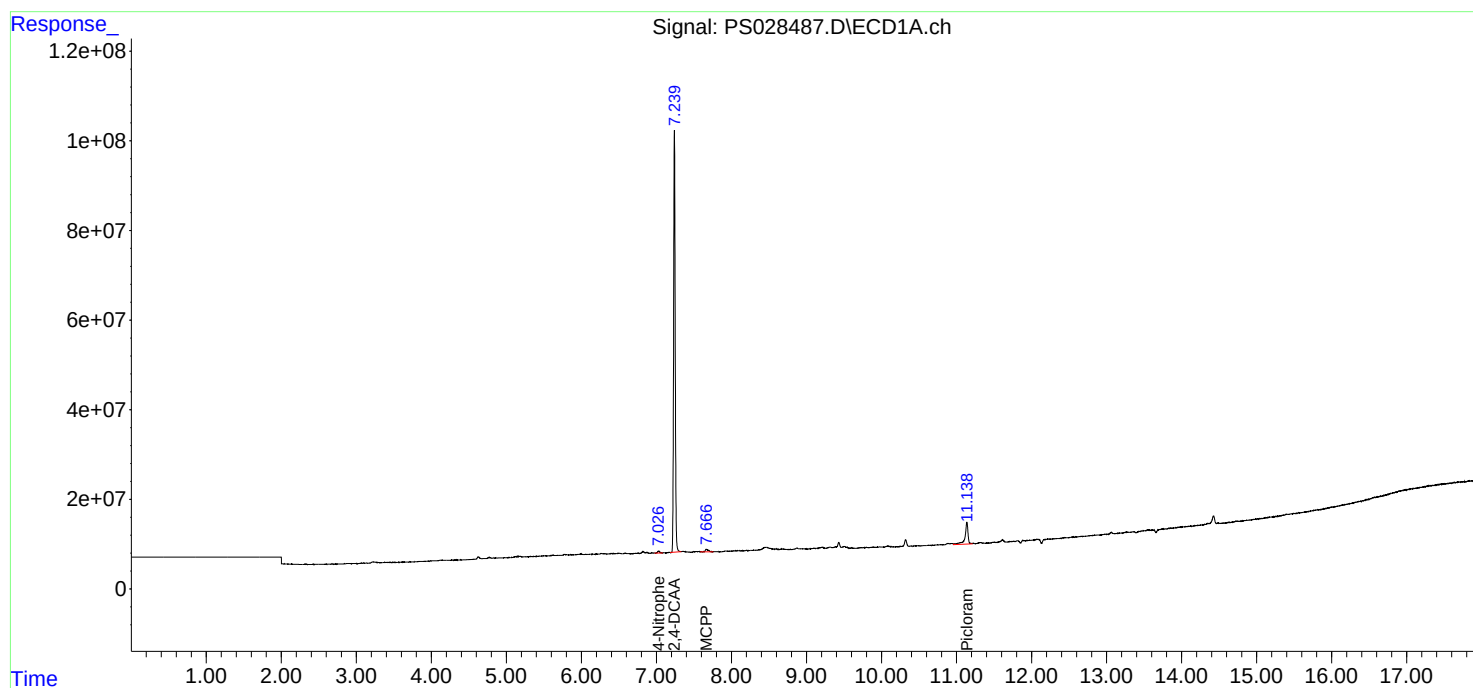


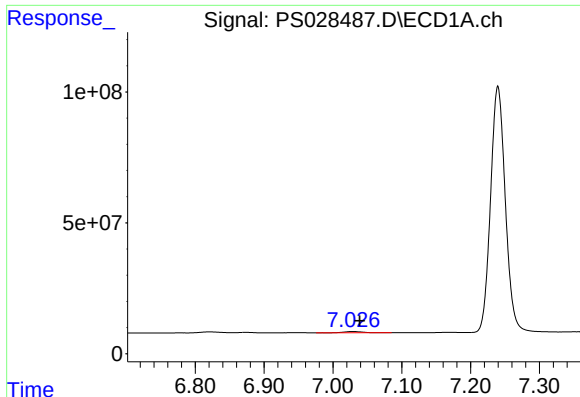

#3 4-Nitrophenol


R.T.: 7.028 min
Delta R.T.: -0.010 min
Response: 8598070
Conc: 5.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

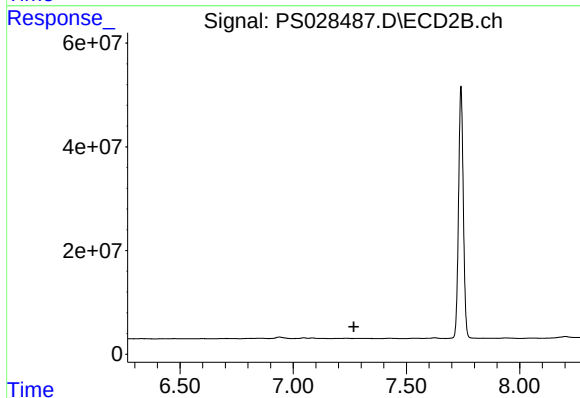


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.268 min
Response: 0
Conc: N.D.

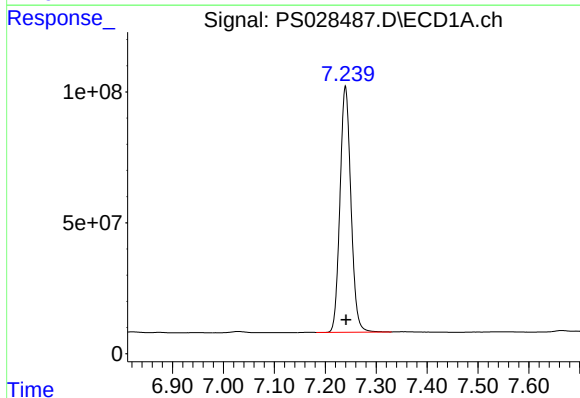


#4 2,4-DCAA

R.T.: 7.240 min
Delta R.T.: -0.001 min
Response: 1400548590
Conc: 547.97 ng/ml

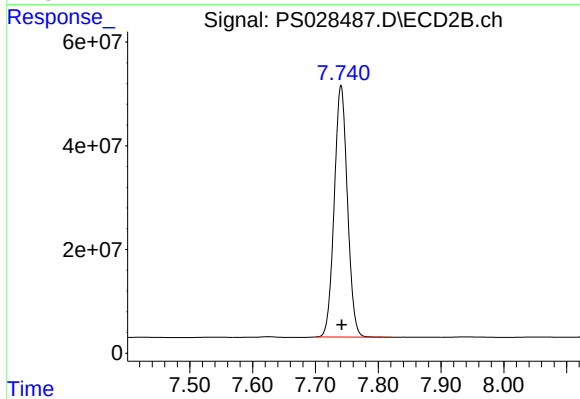

#4 2,4-DCAA


R.T.: 7.741 min
Delta R.T.: -0.001 min
Response: 706886411
Conc: 547.00 ng/ml

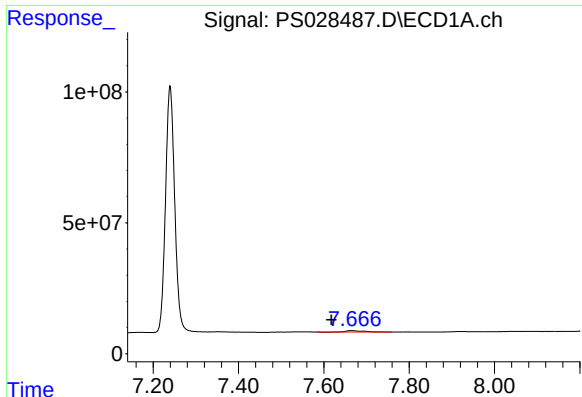

#6 MCP


R.T.: 7.665 min
Delta R.T.: 0.047 min
Response: 15725017
Conc: 2.24 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

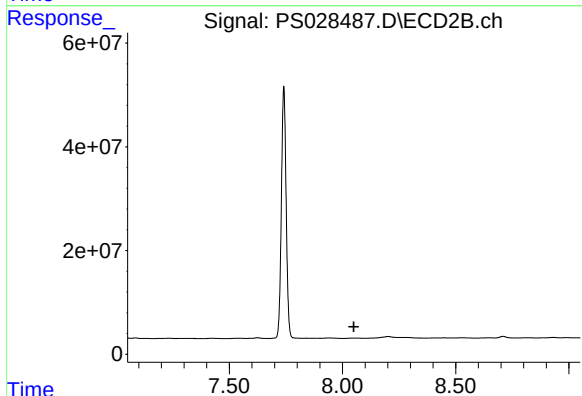


#6 MCP

R.T.: 0.000 min
Exp R.T. : 8.051 min
Response: 0
Conc: N.D.

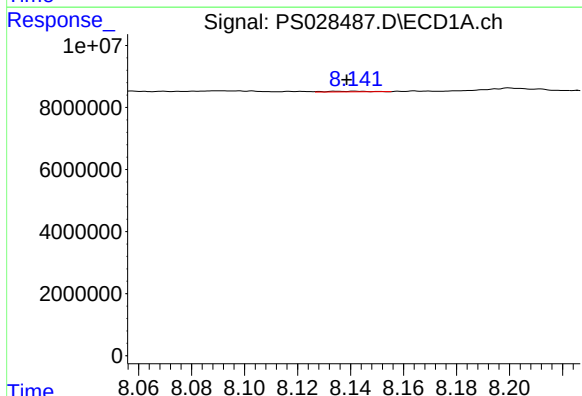


#8 DICHLORPROP

R.T.: 8.141 min
Delta R.T.: 0.003 min
Response: 215375
Conc: N.D.

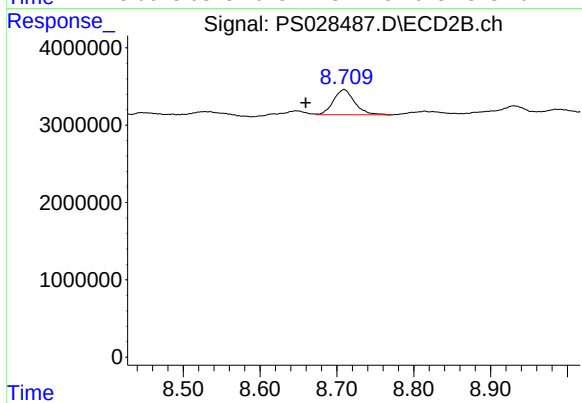

#8 DICHLORPROP


R.T.: 8.709 min
Delta R.T.: 0.050 min
Response: 6169104
Conc: 4.22 ng/ml

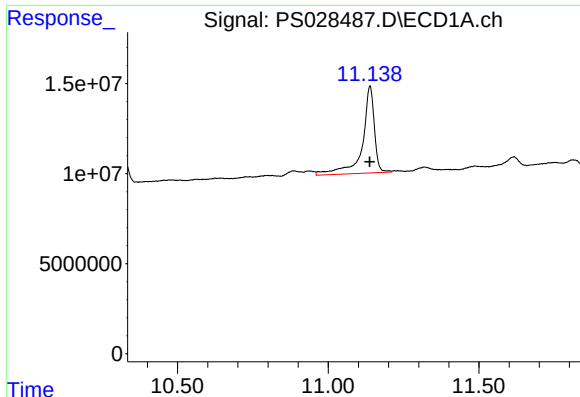

#15 Picloram


R.T.: 11.138 min
Delta R.T.: 0.000 min
Response: 134260660
Conc: 4.77 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

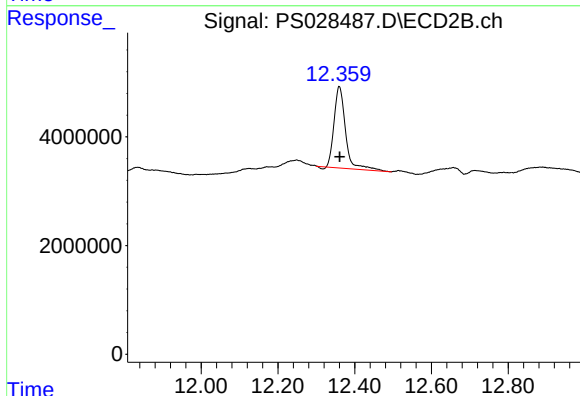


#15 Picloram

R.T.: 12.360 min
Delta R.T.: -0.001 min
Response: 31055468
Conc: 2.74 ng/ml

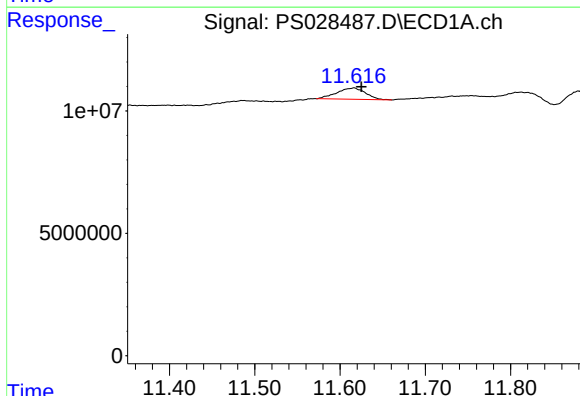

#16 DCPA

R.T.: 11.615 min
Delta R.T.: -0.010 min
Response: 10754339
Conc: N.D.

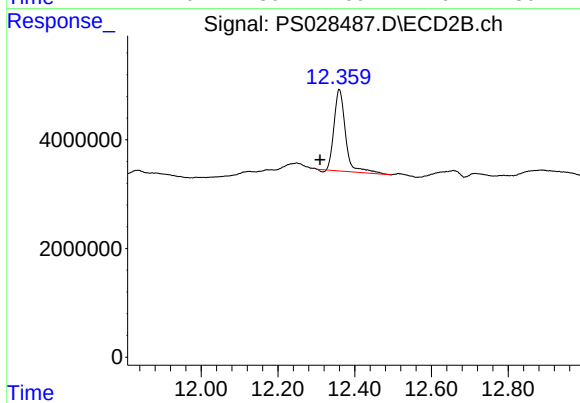

#16 DCPA

R.T.: 12.360 min
Delta R.T.: 0.050 min
Response: 31055468
Conc: 3.20 ng/ml