

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111324\
 Data File : PS028494.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2024 14:12
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 14:53:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.240	7.741	1406.7E6	707.5E6	550.375	547.457
Target Compounds							
1) T	Dalapon	2.648	0.000	726851	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.398	0.000	1402466	0	<MDL	N.D. #
3) T	4-Nitroph...	7.030	0.000	8256822	0	4.861	N.D. #
6) T	MCPD	7.666f	0.000	12763681	0	1.814	N.D. #
7) T	MCPA	7.798f	0.000	909858	0	<MDL	N.D. #
8) T	DICHLORPROP	8.139	8.709f	201185	5261113	<MDL	3.602 #
10) T	Pentachlo...	8.672	0.000	2879610	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	9.892	0	2143530	N.D.	<MDL
12) T	2,4,5-T	9.500f	10.313	7309162	8597057	<MDL	1.026 #
13) T	2,4-DB	10.096	0.000	3154790	0	1.157	N.D. #
14) T	DINOSEB	11.316	0.000	7499754	0	<MDL	N.D. #
15) T	Picloram	11.138	12.360	154.8E6	35771839	5.497	3.160 #
16) T	DCPA	11.612	0.000	12880922	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111324\
Data File : PS028494.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2024 14:12
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 14:53:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

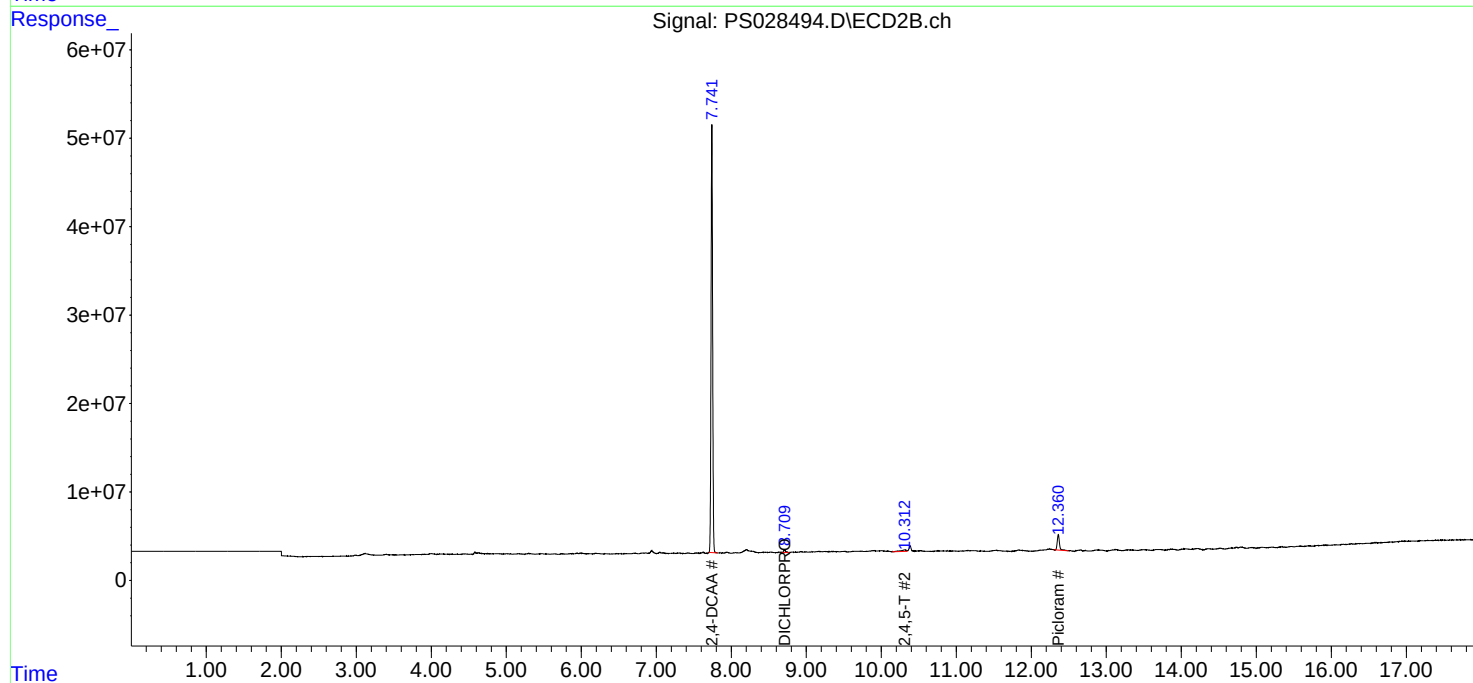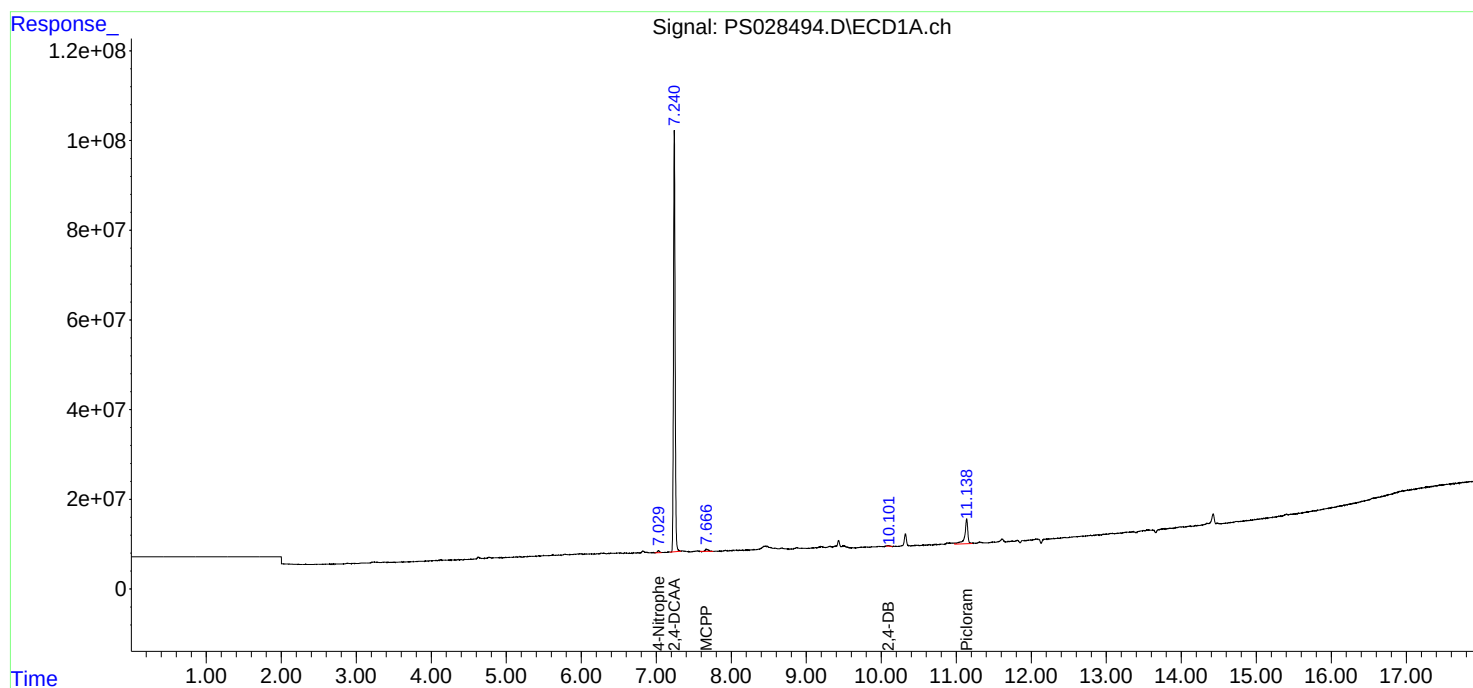


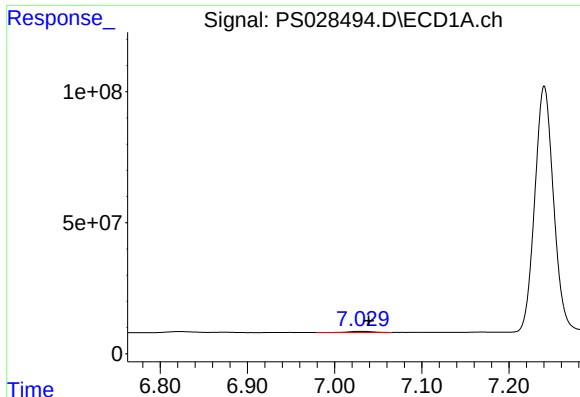

#3 4-Nitrophenol


R.T.: 7.030 min
Delta R.T.: -0.009 min
Response: 8256822
Conc: 4.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

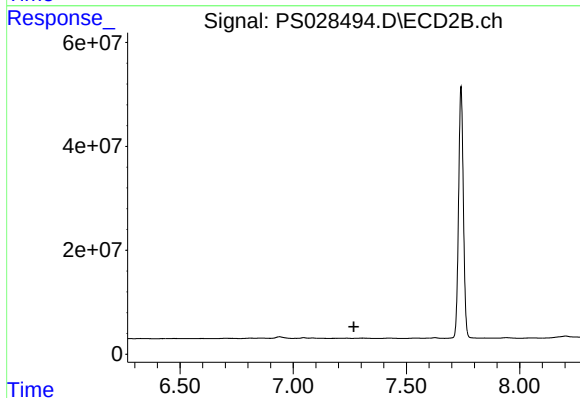


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.268 min
Response: 0
Conc: N.D.

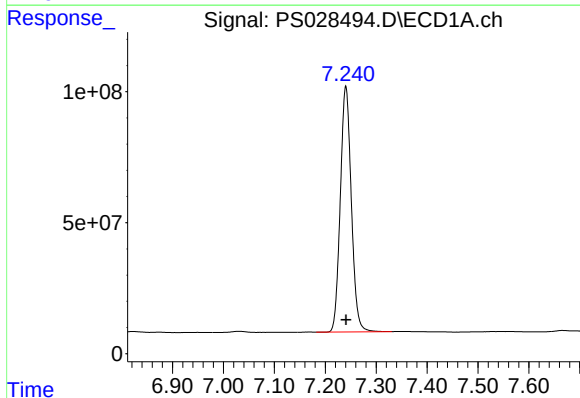


#4 2,4-DCAA

R.T.: 7.240 min
Delta R.T.: 0.000 min
Response: 1406694163
Conc: 550.38 ng/ml

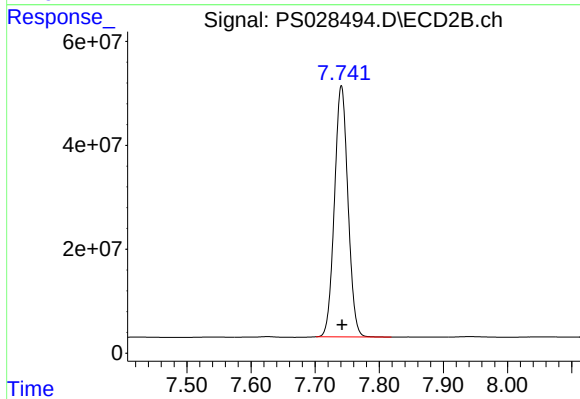

#4 2,4-DCAA


R.T.: 7.741 min
Delta R.T.: -0.001 min
Response: 707481808
Conc: 547.46 ng/ml

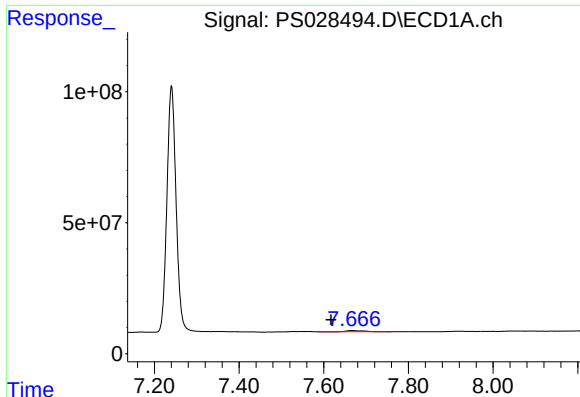

#6 MCP


R.T.: 7.666 min
Delta R.T.: 0.049 min
Response: 12763681
Conc: 1.81 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

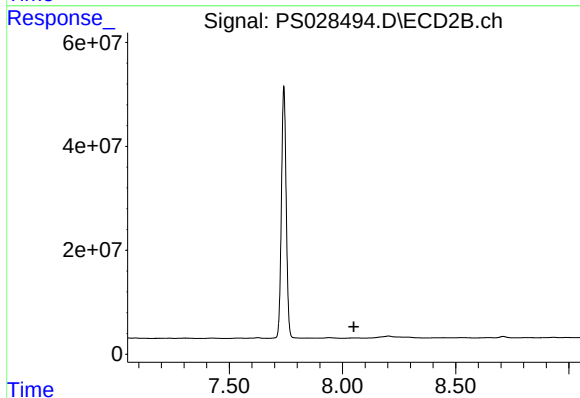


#6 MCP

R.T.: 0.000 min
Exp R.T.: 8.051 min
Response: 0
Conc: N.D.

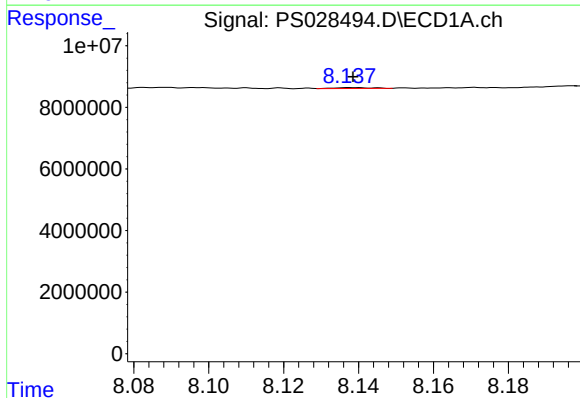


#8 DICHLORPROP

R.T.: 8.139 min
Delta R.T.: 0.000 min
Response: 201185
Conc: N.D.

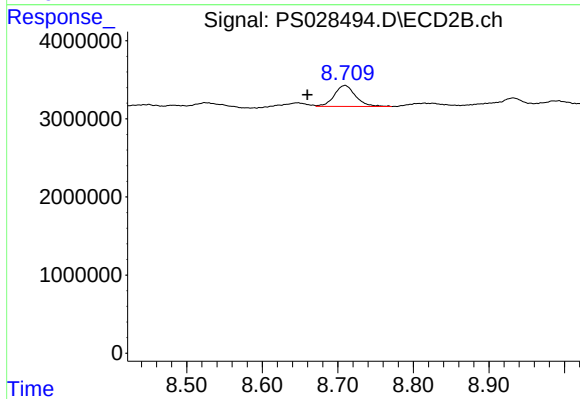

#8 DICHLORPROP


R.T.: 8.709 min
Delta R.T.: 0.050 min
Response: 5261113
Conc: 3.60 ng/ml

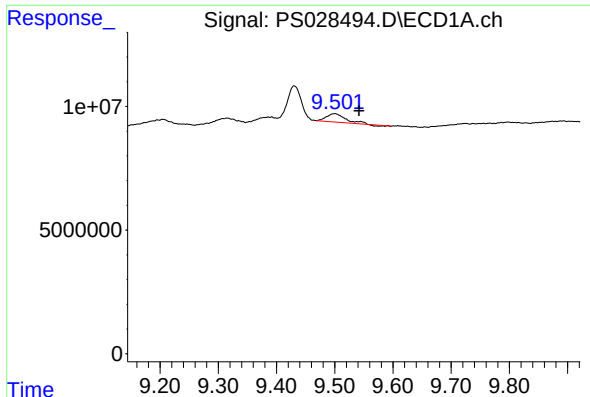

#12 2,4,5-T


R.T.: 9.500 min
Delta R.T.: -0.042 min
Response: 7309162
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

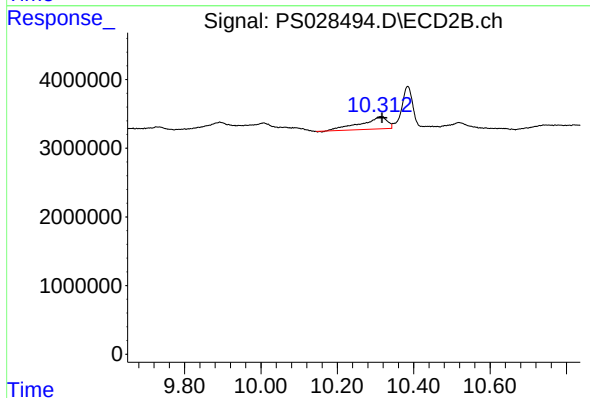


#12 2,4,5-T

R.T.: 10.313 min
Delta R.T.: -0.004 min
Response: 8597057
Conc: 1.03 ng/ml

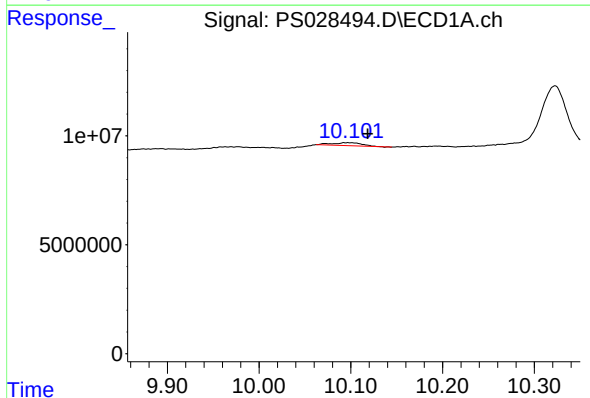


#13 2,4-DB

R.T.: 10.096 min
Delta R.T.: -0.022 min
Response: 3154790
Conc: 1.16 ng/ml

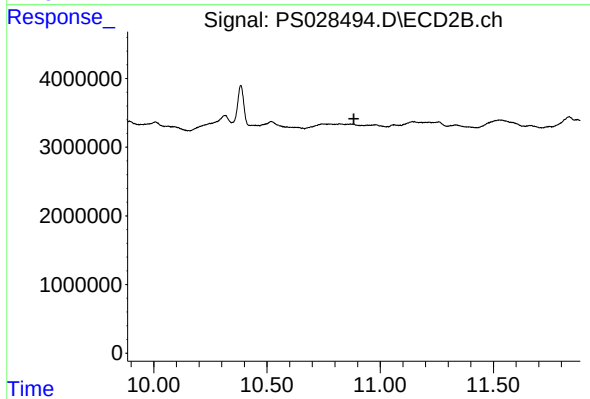

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 10.884 min
Response: 0
Conc: N.D.

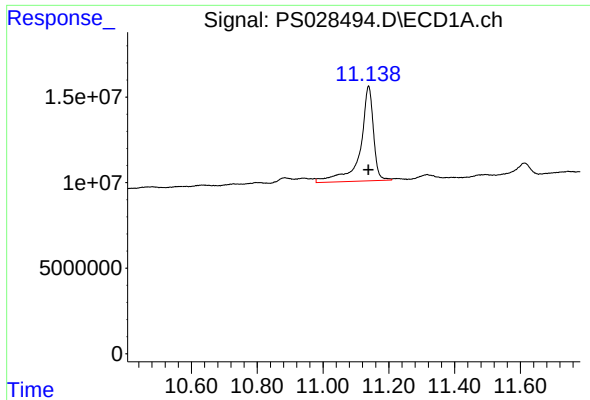

#15 Picloram

R.T.: 11.138 min
Delta R.T.: 0.000 min
Response: 154800371
Conc: 5.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

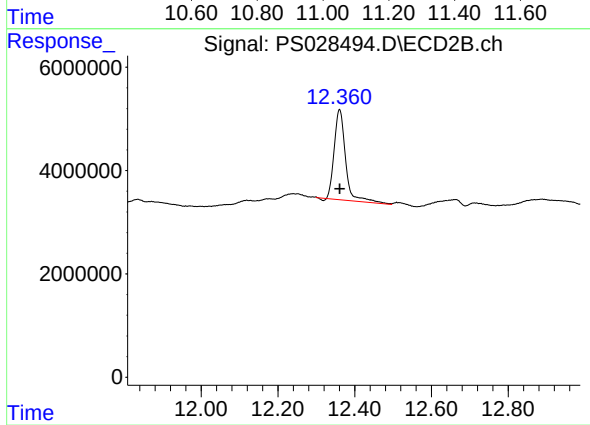

#15 Picloram

R.T.: 12.360 min
Delta R.T.: 0.000 min
Response: 35771839
Conc: 3.16 ng/ml