

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111324\
 Data File : PS028506.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2024 19:07
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 23:40:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.240	7.740	1433.8E6	733.3E6	560.991	567.426
Target Compounds							
1) T	Dalapon	2.631	0.000	299319	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.395	0.000	637028	0	<MDL	N.D. #
3) T	4-Nitroph...	7.028	0.000	10088083	0	5.940	N.D. #
6) T	MCP	7.666f	0.000	25281946	0	3.594	N.D. #
7) T	MCPA	7.805f	0.000	254658	0	<MDL	N.D. #
8) T	DICHLORPROP	8.098f	8.708f	1198762	10234373	<MDL	7.007 #
10) T	Pentachlo...	8.702f	0.000	3099160	0	<MDL	N.D. #
12) T	2,4,5-T	9.544	10.312	2196333	7910554	<MDL	<MDL #
15) T	Picloram	11.137	12.360	21571996	7527038	<MDL	<MDL #
16) T	DCPA	11.624	0.000	2419108	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111324\
Data File : PS028506.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2024 19:07
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 23:40:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

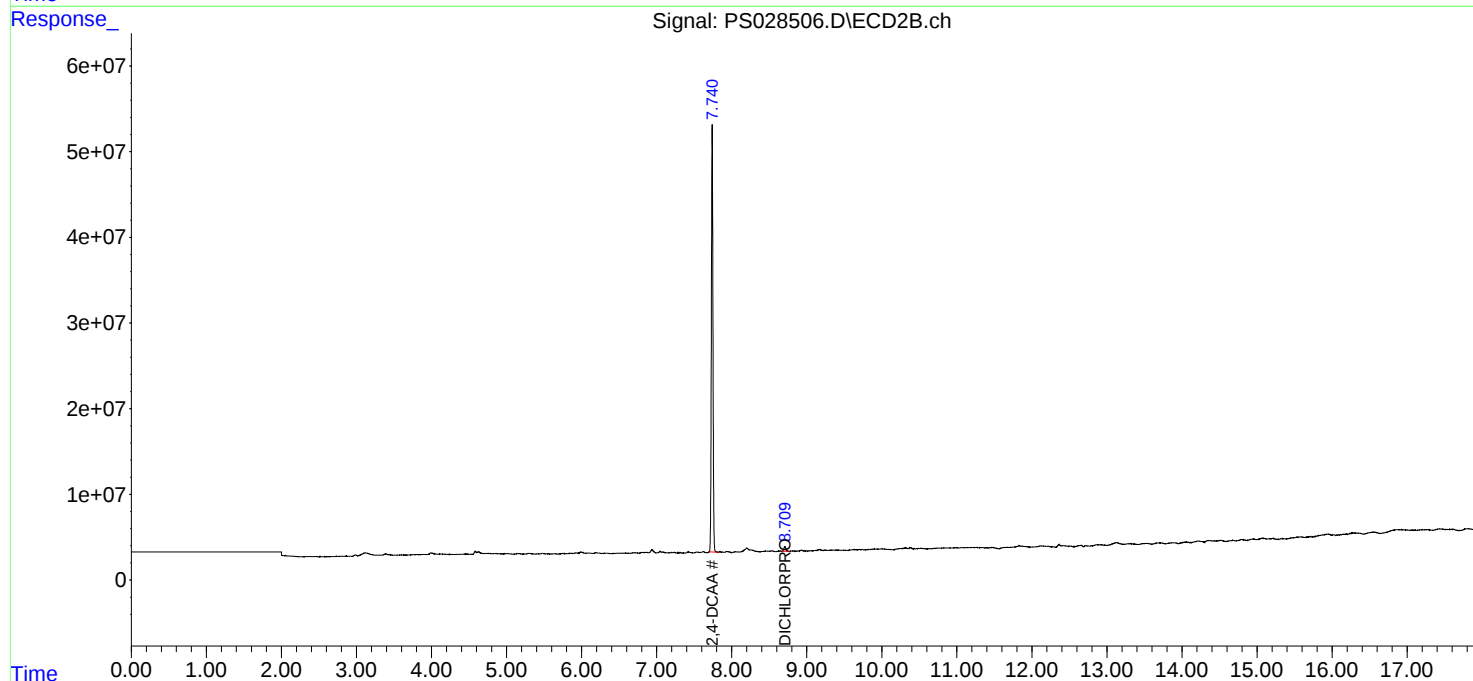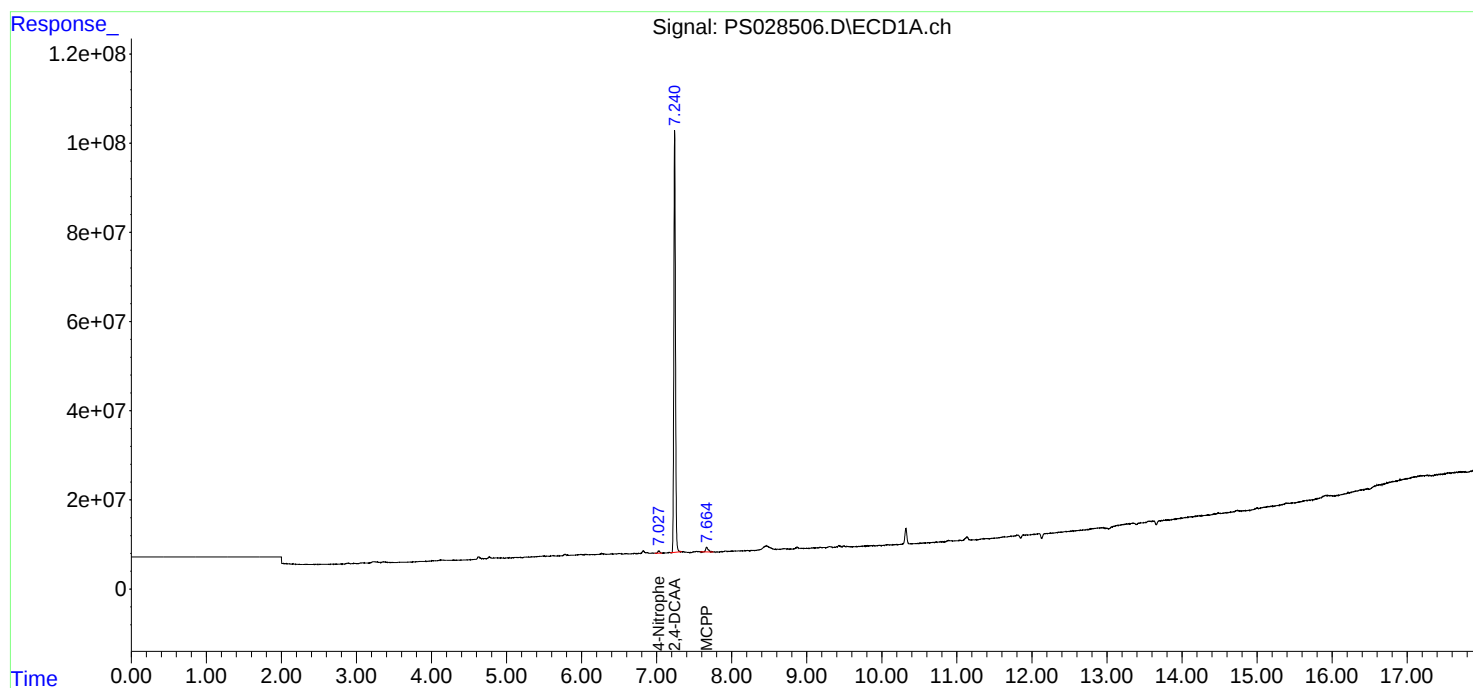


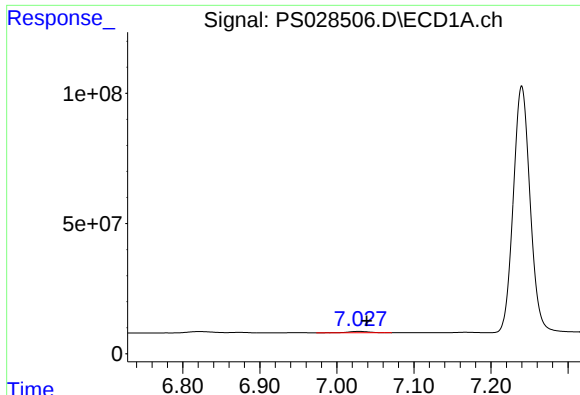

#3 4-Nitrophenol


R.T.: 7.028 min
Delta R.T.: -0.011 min
Response: 10088083
Conc: 5.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

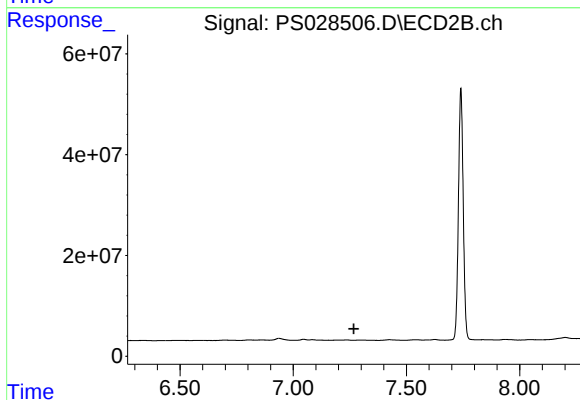


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

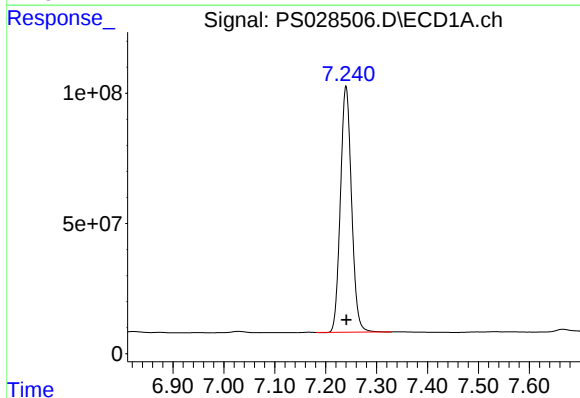


#4 2,4-DCAA

R.T.: 7.240 min
Delta R.T.: 0.000 min
Response: 1433825479
Conc: 560.99 ng/ml

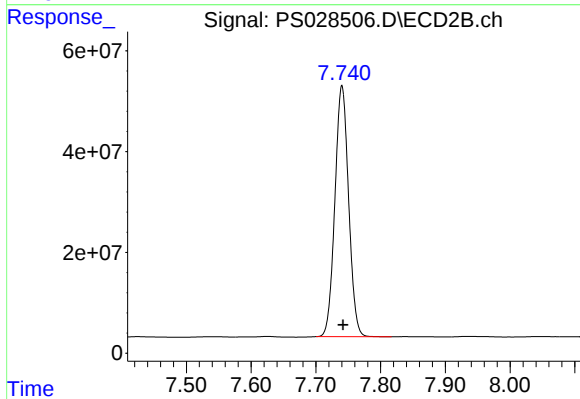

#4 2,4-DCAA


R.T.: 7.740 min
Delta R.T.: -0.002 min
Response: 733287226
Conc: 567.43 ng/ml

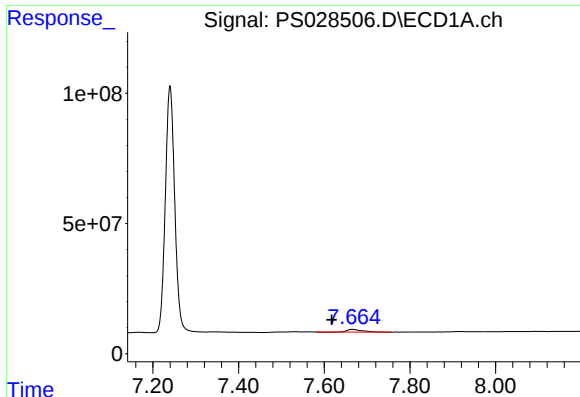

#6 MCP


R.T.: 7.666 min
Delta R.T.: 0.049 min
Response: 25281946
Conc: 3.59 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

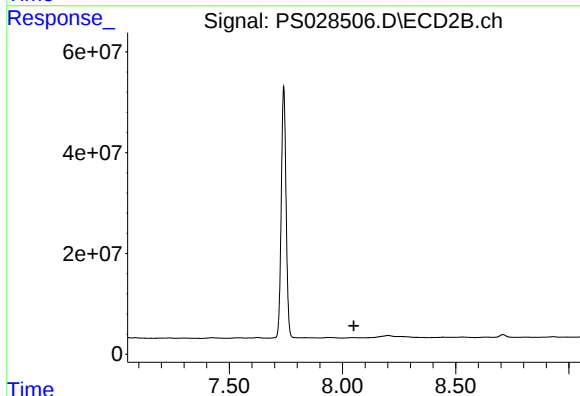


#6 MCP

R.T.: 0.000 min
Exp R.T.: 8.051 min
Response: 0
Conc: N.D.

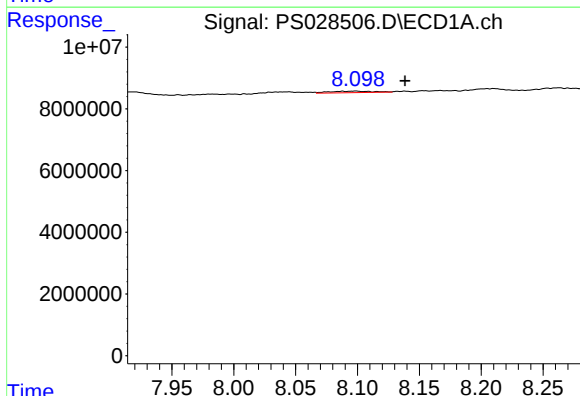

#8 DICHLORPROP

R.T.: 8.098 min
Delta R.T.: -0.041 min
Response: 1198762
Conc: N.D.

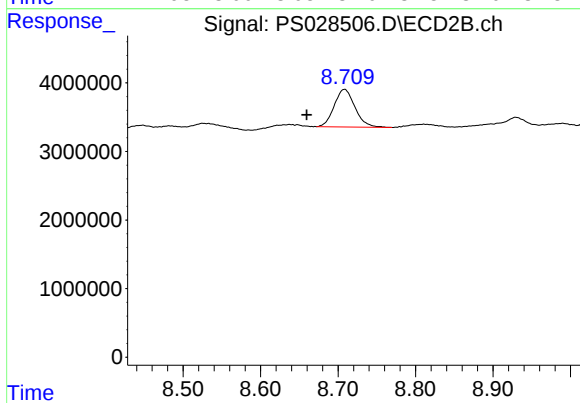

#8 DICHLORPROP

R.T.: 8.708 min
Delta R.T.: 0.049 min
Response: 10234373
Conc: 7.01 ng/ml