

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111324\
 Data File : PS028515.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2024 22:48
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 23:47:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.239	7.740	1444.0E6	734.1E6	564.973	568.026
Target Compounds							
1) T	Dalapon	2.649	0.000	1245530	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.398	0.000	1340244	0	<MDL	N.D. #
3) T	4-Nitroph...	7.027	0.000	9827803	0	5.786	N.D. #
5) T	DICAMBA	0.000	7.936	0	3014685	N.D.	<MDL
6) T	MCPD	7.665f	0.000	30845728	0	4.385	N.D. #
7) T	MCPA	0.000	8.267f	0	6153031	N.D.	<MDL
8) T	DICHLORPROP	8.145	8.708f	570947	13723061	<MDL	9.396 #
10) T	Pentachlo...	8.704f	0.000	3392234	0	<MDL	N.D. #
12) T	2,4,5-T	9.541	10.315	2918058	5592637	<MDL	<MDL #
13) T	2,4-DB	10.103	0.000	858531	0	<MDL	N.D. #
15) T	Picloram	11.137	12.358	47760789	15406587	1.696	1.361
16) T	DCPA	11.617	12.358f	5718884	15406587	<MDL	1.589 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111324\
Data File : PS028515.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2024 22:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 23:47:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

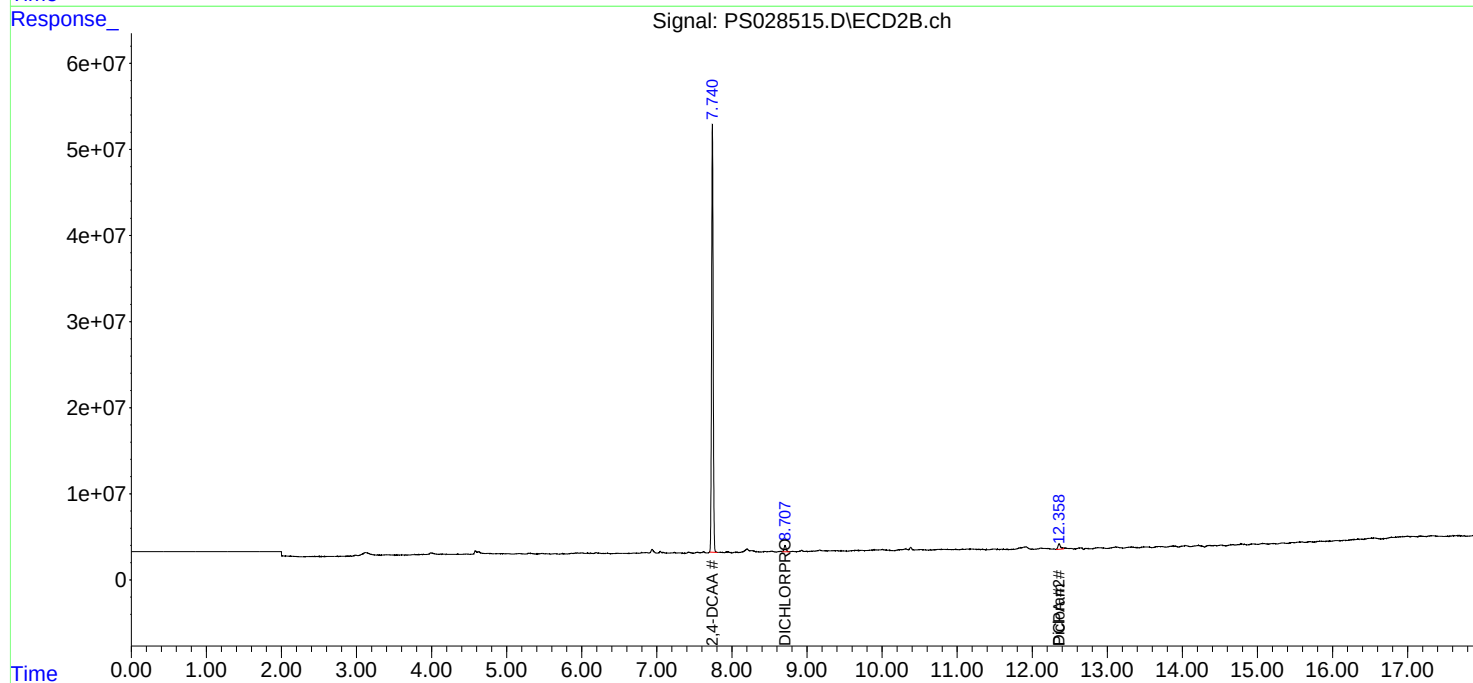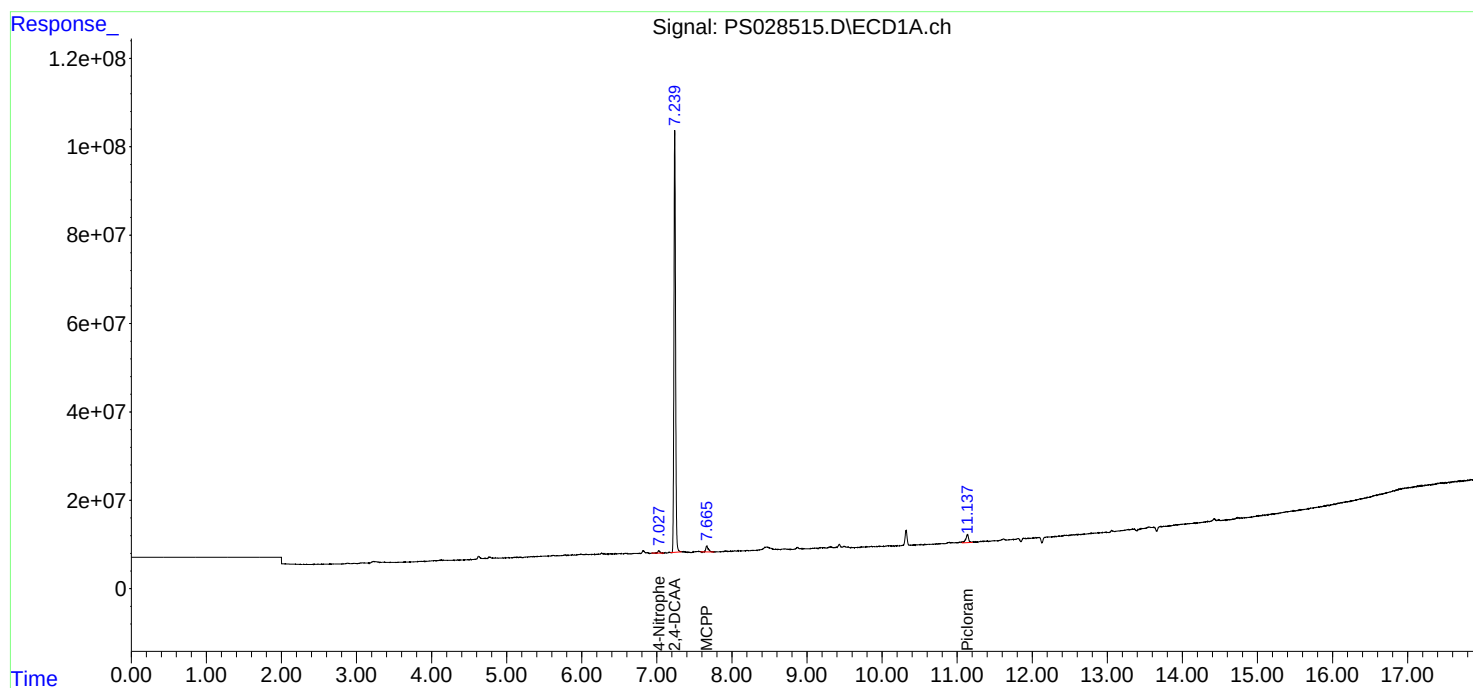


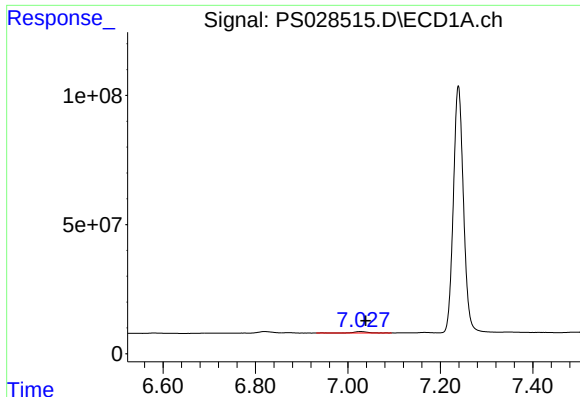

#3 4-Nitrophenol


R.T.: 7.027 min
Delta R.T.: -0.012 min
Response: 9827803
Conc: 5.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

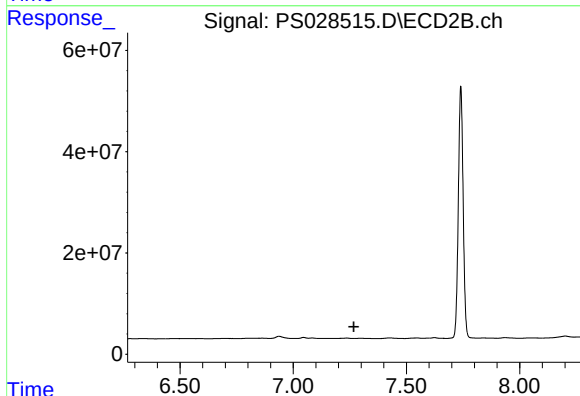


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

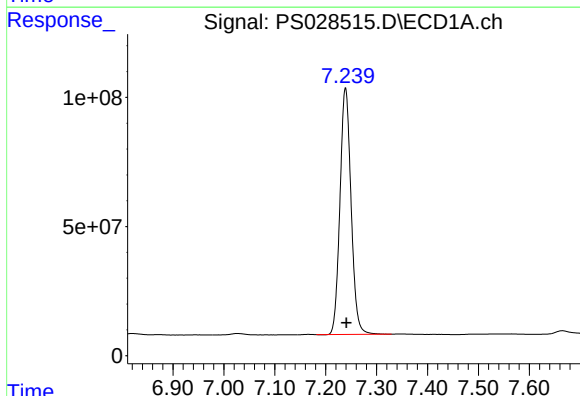


#4 2,4-DCAA

R.T.: 7.239 min
Delta R.T.: -0.002 min
Response: 1444003495
Conc: 564.97 ng/ml

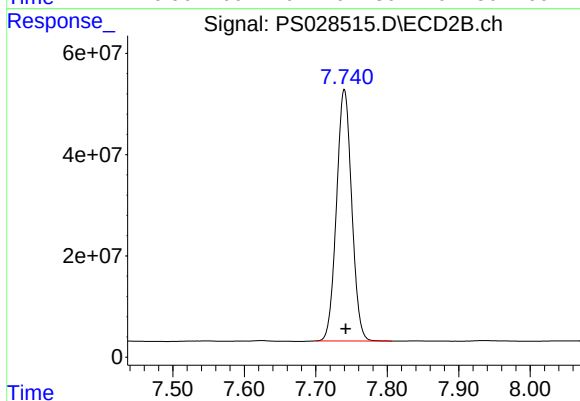

#4 2,4-DCAA


R.T.: 7.740 min
Delta R.T.: -0.002 min
Response: 734062603
Conc: 568.03 ng/ml

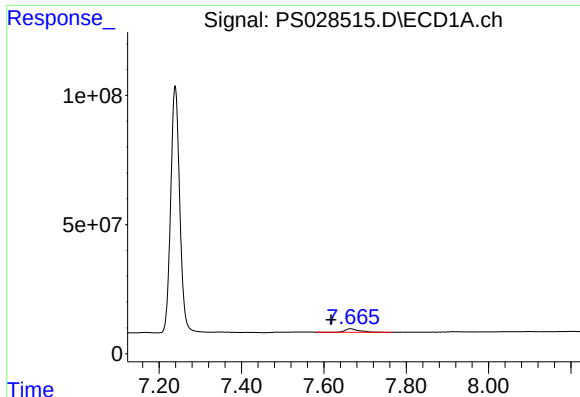

#6 MCP


R.T.: 7.665 min
Delta R.T.: 0.047 min
Response: 30845728
Conc: 4.38 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

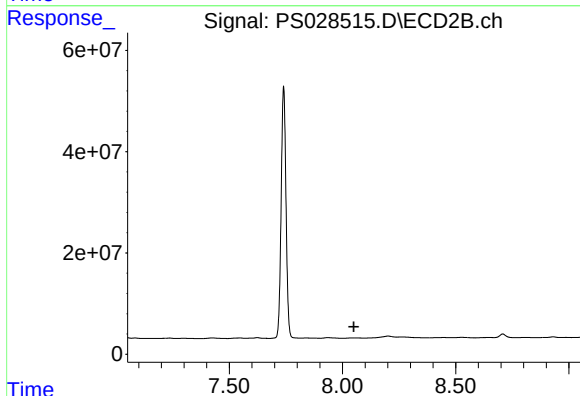


#6 MCP

R.T.: 0.000 min
Exp R.T. : 8.051 min
Response: 0
Conc: N.D.

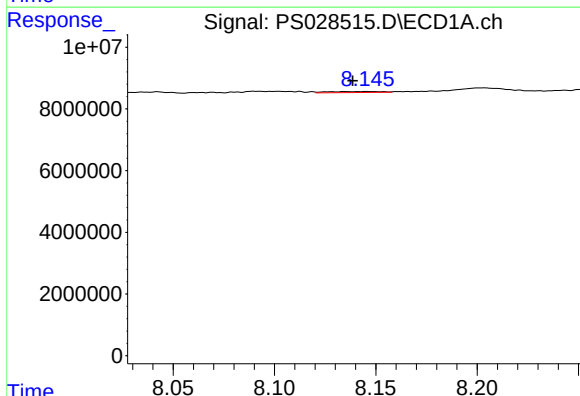


#8 DICHLORPROP

R.T.: 8.145 min
Delta R.T.: 0.006 min
Response: 570947
Conc: N.D.

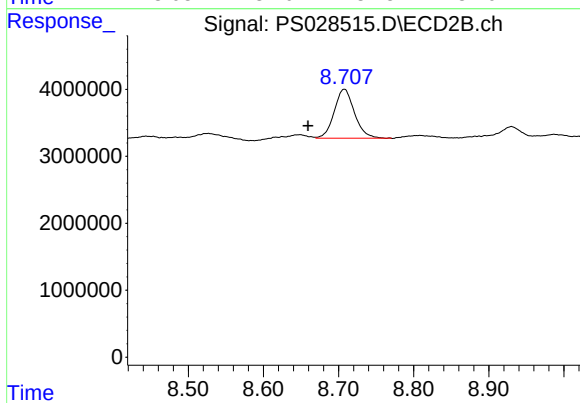

#8 DICHLORPROP


R.T.: 8.708 min
Delta R.T.: 0.048 min
Response: 13723061
Conc: 9.40 ng/ml

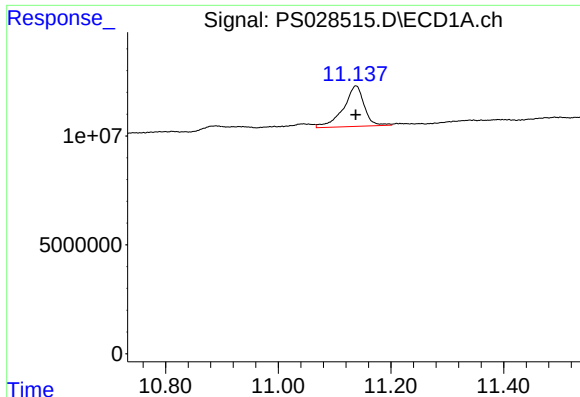

#15 Picloram


R.T.: 11.137 min
Delta R.T.: 0.000 min
Response: 47760789
Conc: 1.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

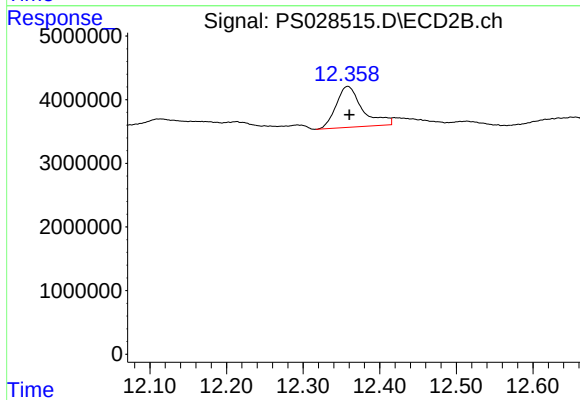


#15 Picloram

R.T.: 12.358 min
Delta R.T.: -0.003 min
Response: 15406587
Conc: 1.36 ng/ml

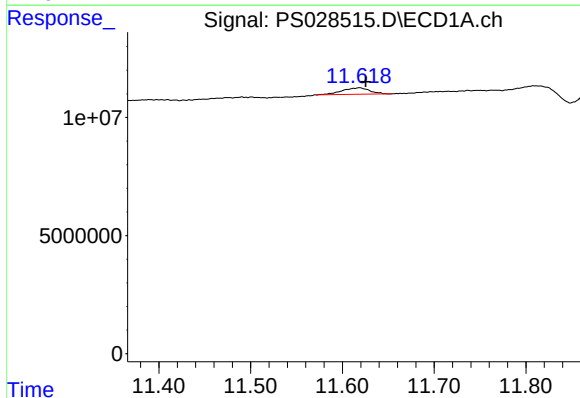

#16 DCPA

R.T.: 11.617 min
Delta R.T.: -0.008 min
Response: 5718884
Conc: N.D.

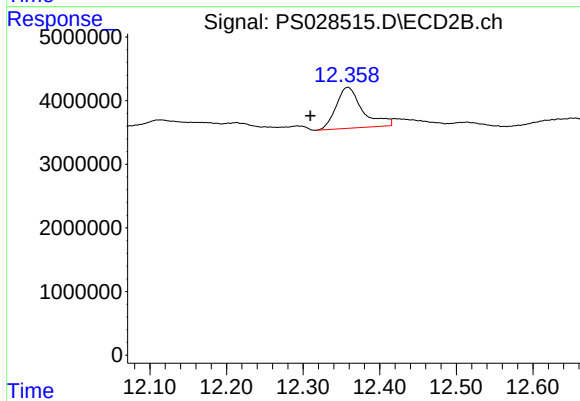

#16 DCPA

R.T.: 12.358 min
Delta R.T.: 0.049 min
Response: 15406587
Conc: 1.59 ng/ml