

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111324\
 Data File : PS028527.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2024 03:43
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 03:55:30 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.240	7.740	1459.9E6	745.2E6	571.201	576.670
Target Compounds							
1) T	Dalapon	2.664f	0.000	1424920	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.396	0.000	240619	0	<MDL	N.D. #
3) T	4-Nitroph...	7.028	0.000	10286363	0	6.056	N.D. #
5) T	DICAMBA	0.000	7.934	0	3468583	N.D.	<MDL
6) T	MCPD	7.666f	0.000	27246092	0	3.873	N.D. #
7) T	MCPA	0.000	8.263f	0	4845462	N.D.	<MDL
8) T	DICHLORPROP	8.165f	8.707f	789625	12638681	<MDL	8.653 #
12) T	2,4,5-T	9.546	10.312	1937667	3521652	<MDL	<MDL #
15) T	Picloram	11.139	12.360	17165333	5372468	<MDL	<MDL #
16) T	DCPA	11.618	0.000	2319982	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111324\
Data File : PS028527.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2024 03:43
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 03:55:30 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

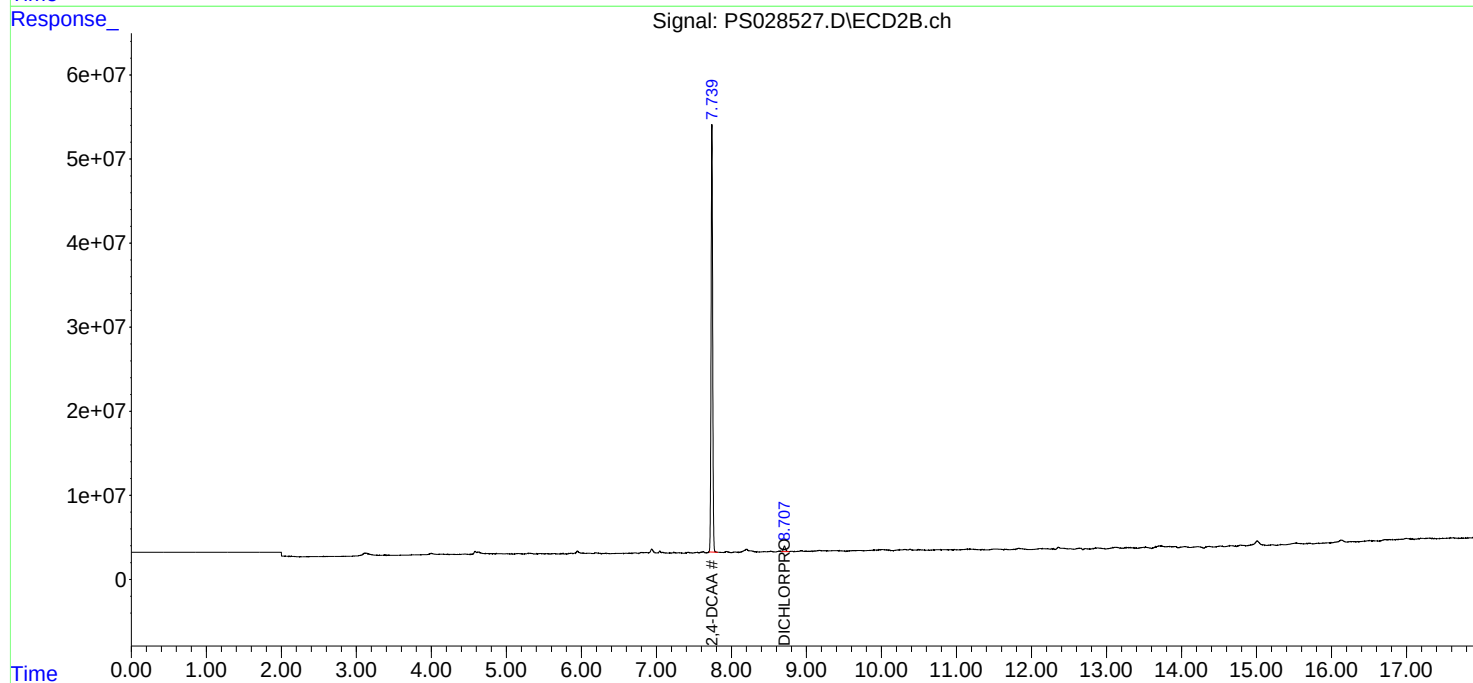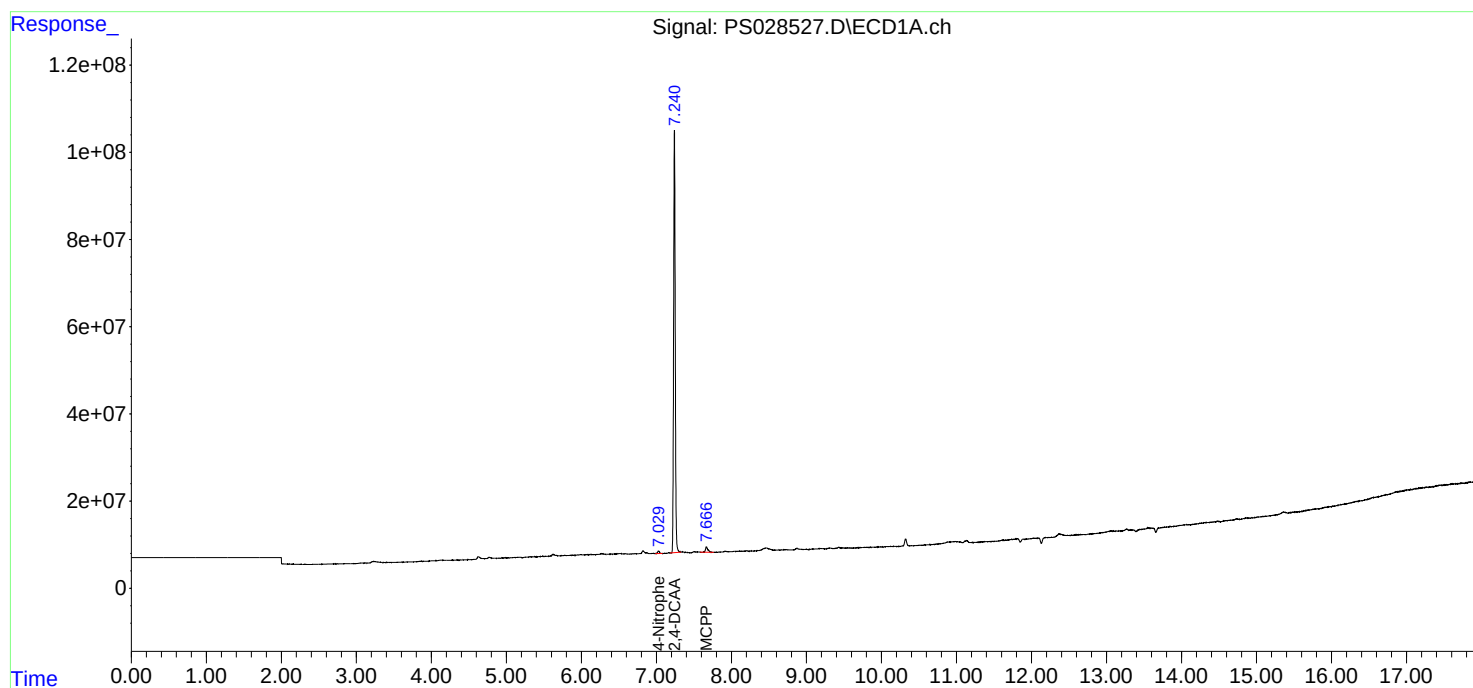


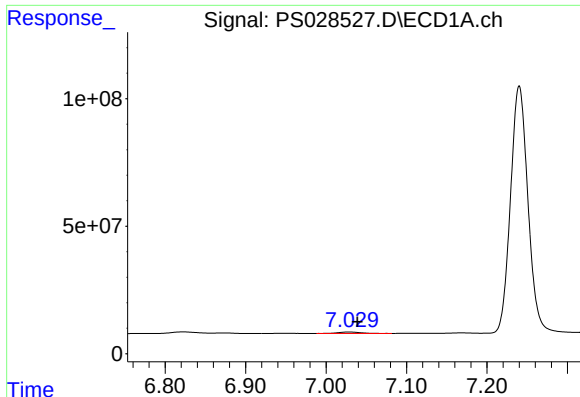

#3 4-Nitrophenol


R.T.: 7.028 min
Delta R.T.: -0.011 min
Response: 10286363
Conc: 6.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

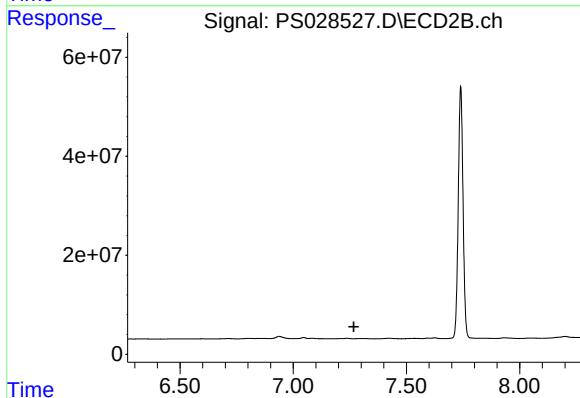


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

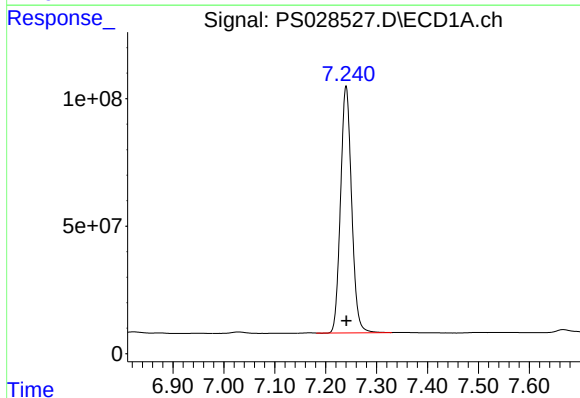


#4 2,4-DCAA

R.T.: 7.240 min
Delta R.T.: 0.000 min
Response: 1459921788
Conc: 571.20 ng/ml

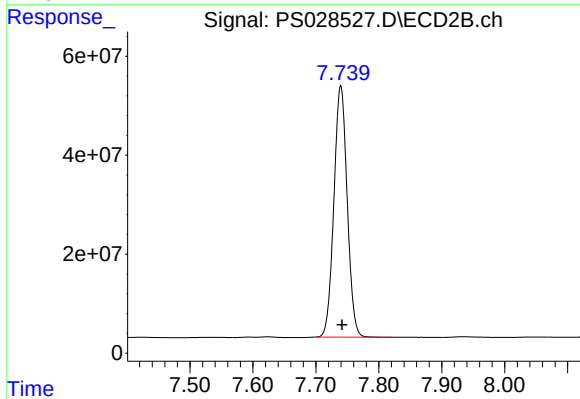

#4 2,4-DCAA


R.T.: 7.740 min
Delta R.T.: -0.002 min
Response: 745233525
Conc: 576.67 ng/ml

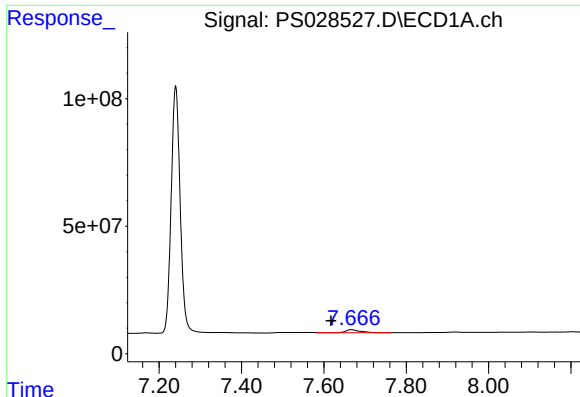

#6 MCP


R.T.: 7.666 min
Delta R.T.: 0.049 min
Response: 27246092
Conc: 3.87 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

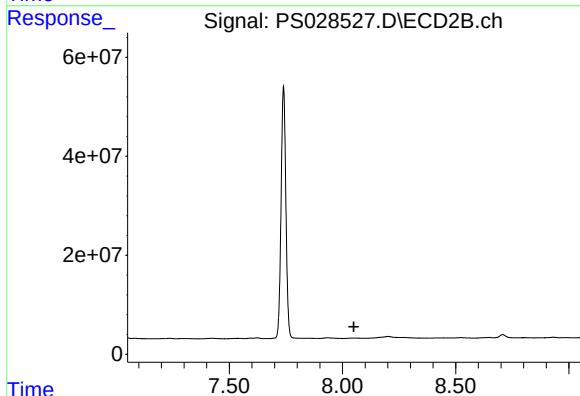


#6 MCP

R.T.: 0.000 min
Exp R.T.: 8.051 min
Response: 0
Conc: N.D.

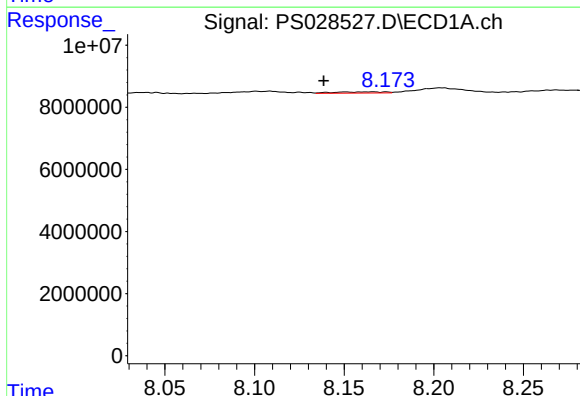

#8 DICHLORPROP

R.T.: 8.165 min
Delta R.T.: 0.026 min
Response: 789625
Conc: N.D.

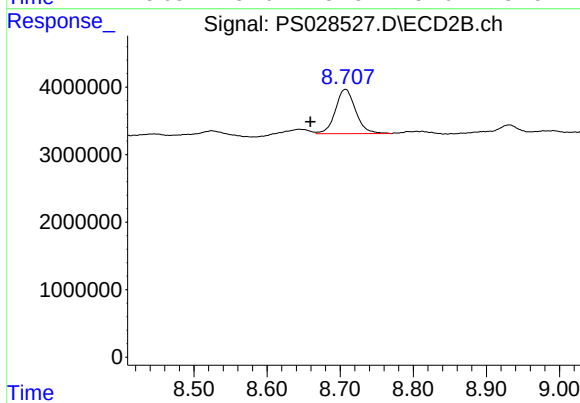

#8 DICHLORPROP

R.T.: 8.707 min
Delta R.T.: 0.048 min
Response: 12638681
Conc: 8.65 ng/ml