

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111418\
 Data File : PS002422.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2018 16:35
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 02:36:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.405	10.965	127.3E6	786417	417.905	2.149 #
Target Compounds							
1) T	Dalapon	2.931	2.368	288.3E6	268.7E6	653.900	624.344
3) T	4-Nitroph...	10.998	10.129	111.0E6	2157184	683.809	12.312 #
5) T	DICAMBA	11.714	11.175	977.4E6	-945303877	705.422	N.D. #
6) T	MCP	0.000	11.468	0	4723901	N.D.	5.208 #
7) T	MCPA	0.000	11.782	0	94336161	N.D.	67.037 #
8) T	DICHLORPROP	12.901	0.000	243.0E6	0	701.952	N.D. #
10) T	Pentachlo...	13.638	13.316	3492.4E6	-699397132	721.998	N.D. #
11) T	2,4,5-TP ...	14.506	13.936	1348.2E6	1443.3E6	717.470	715.515
12) T	2,4,5-T	14.904	14.500	1088.8E6	1097.8E6	645.913	702.250
14) T	DINOSEB	17.127	15.578	1005.7E6	1051.1E6	704.206	702.313
15) T	Picloram	16.896	16.810	1471.0E6	547.9E6	692.644	205.948 #
16) T	DCPA	0.000	16.810	0	547.9E6	N.D.	228.452 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111418\
Data File : PS002422.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2018 16:35
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 02:36:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

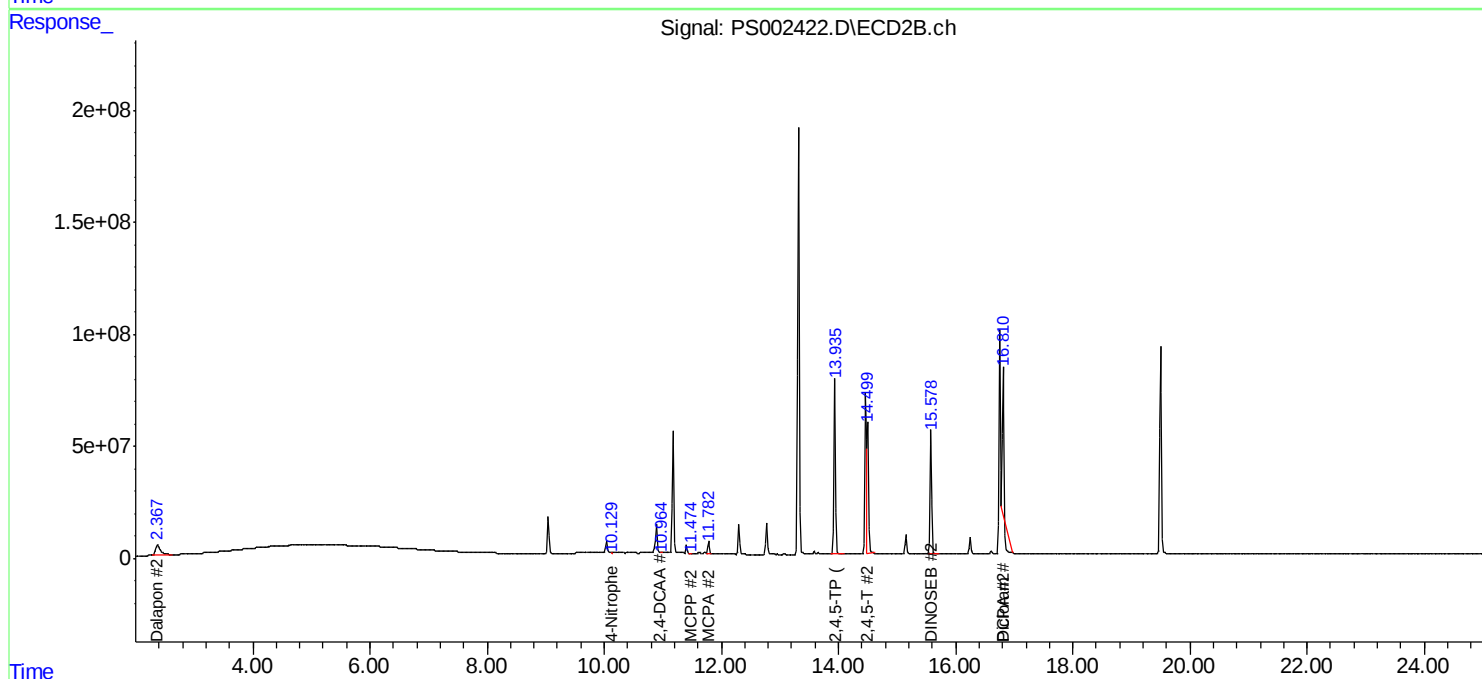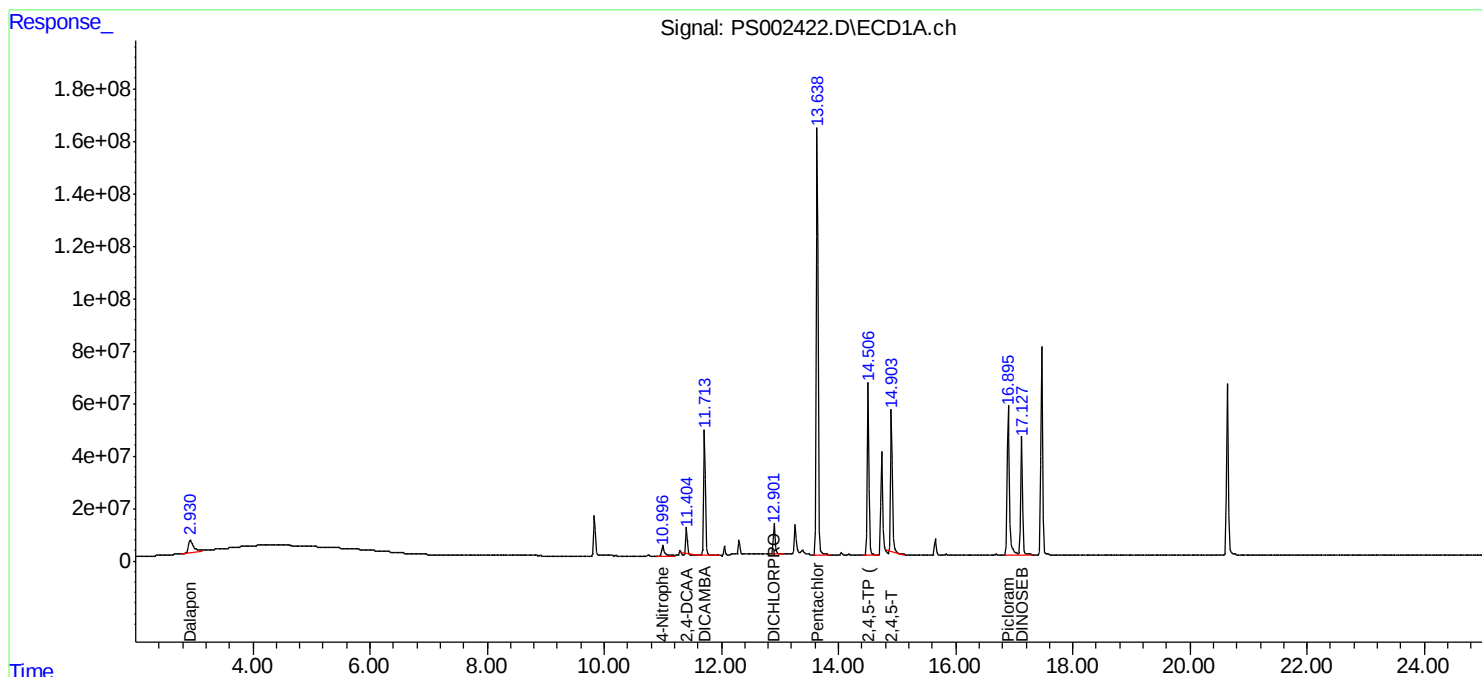


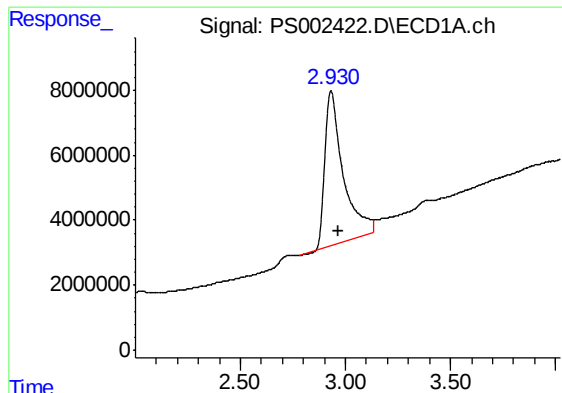

#1 Dalapon


R.T.: 2.931 min
Delta R.T.: -0.038 min
Response: 288337304
Conc: 653.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

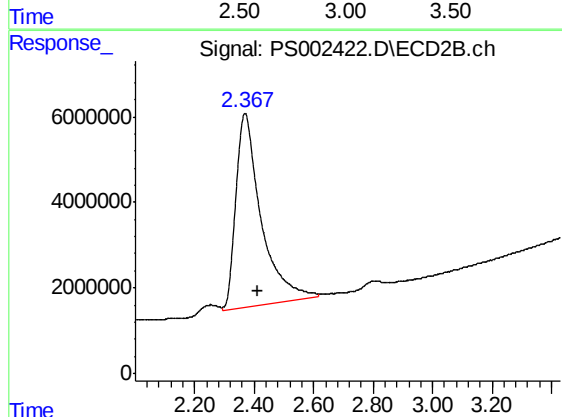


#1 Dalapon

R.T.: 2.368 min
Delta R.T.: -0.044 min
Response: 268713664
Conc: 624.34 ng/ml

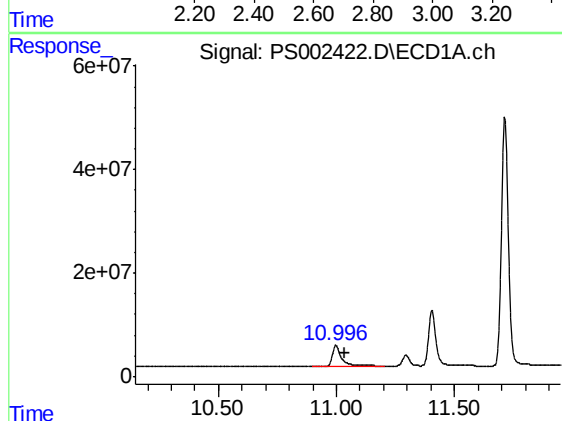


#3 4-Nitrophenol

R.T.: 10.998 min
Delta R.T.: -0.040 min
Response: 110950365
Conc: 683.81 ng/ml

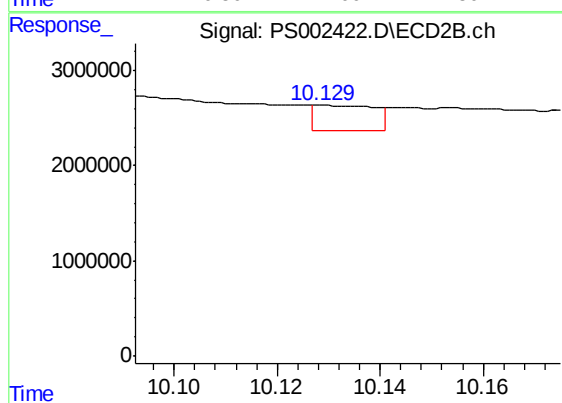

#3 4-Nitrophenol


R.T.: 10.129 min
Delta R.T.: 0.046 min
Response: 2157184
Conc: 12.31 ng/ml

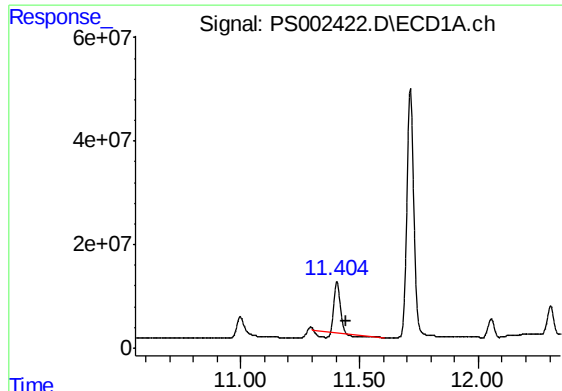

#4 2,4-DCAA


R.T.: 11.405 min
Delta R.T.: -0.039 min
Response: 127293849
Conc: 417.91 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

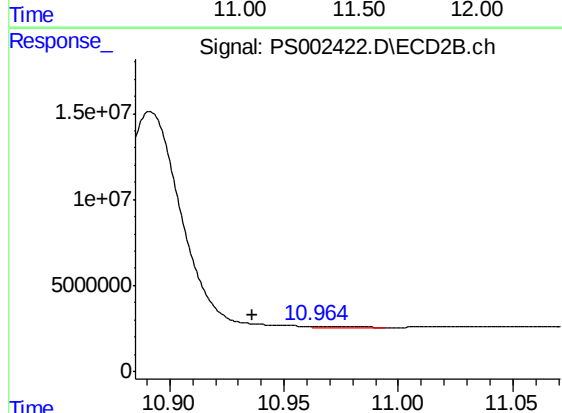


#4 2,4-DCAA

R.T.: 10.965 min
Delta R.T.: 0.029 min
Response: 786417
Conc: 2.15 ng/ml

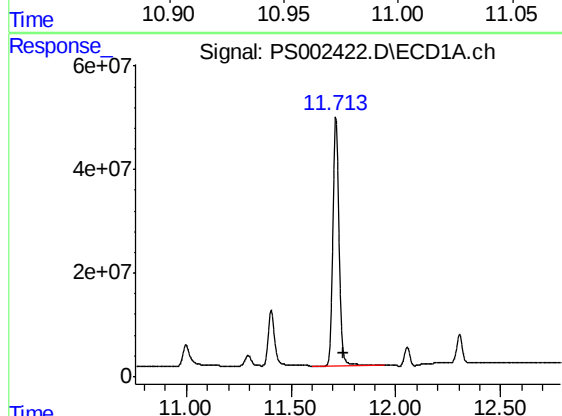


#5 DICAMBA

R.T.: 11.714 min
Delta R.T.: -0.038 min
Response: 977444927
Conc: 705.42 ng/ml

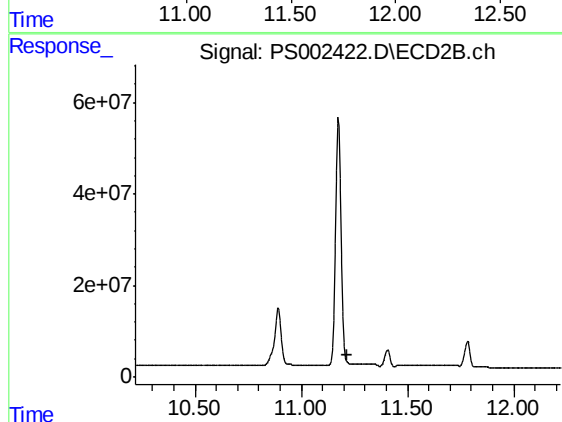

#5 DICAMBA


R.T.: 11.175 min
Delta R.T.: -0.045 min
Response: -945303877
Conc: N.D.

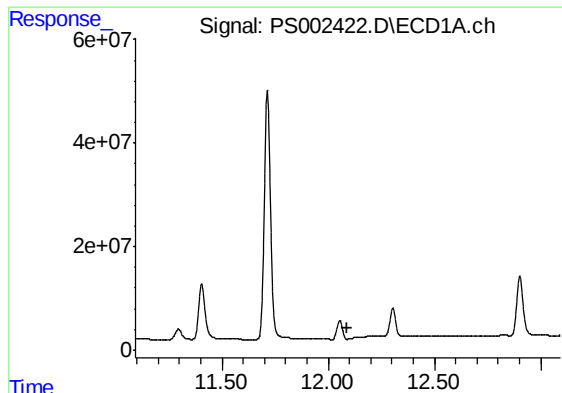

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 12.093 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

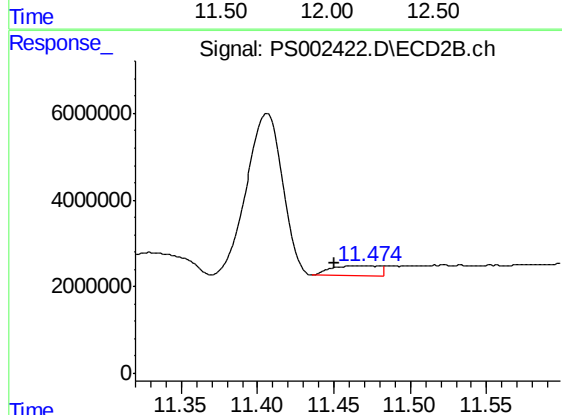


#6 MCPP

R.T.: 11.468 min
Delta R.T.: 0.017 min
Response: 4723901
Conc: 5.21 ug/ml

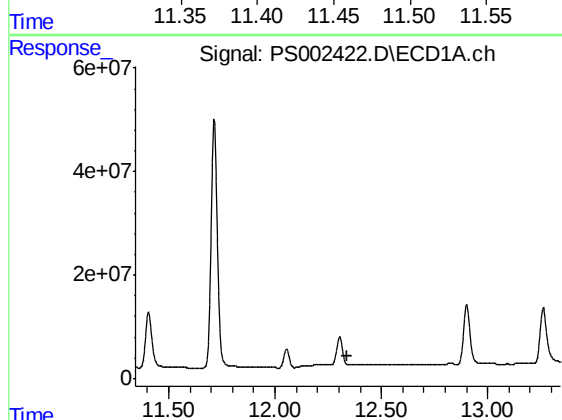


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 12.343 min
Response: 0
Conc: N.D.

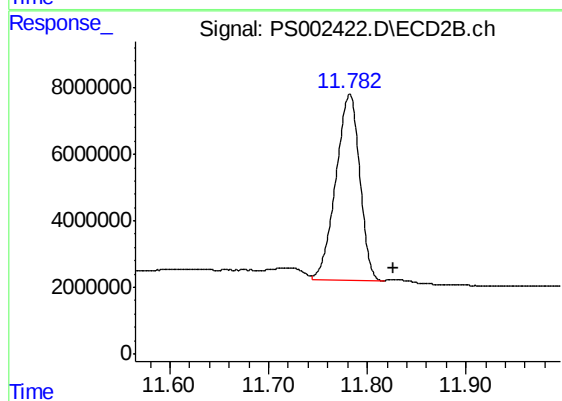

#7 MCPA


R.T.: 11.782 min
Delta R.T.: -0.044 min
Response: 94336161
Conc: 67.04 ug/ml

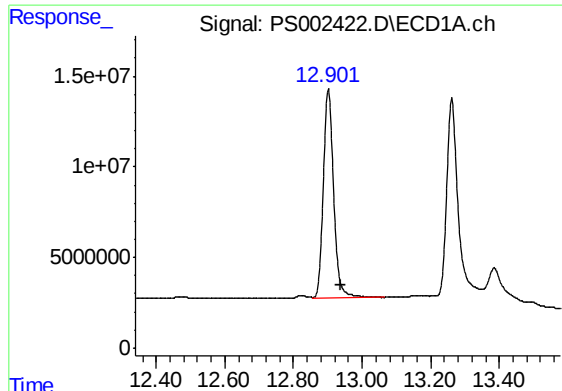

#8 DICHLORPROP


R.T.: 12.901 min
Delta R.T.: -0.038 min
Response: 243024642
Conc: 701.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

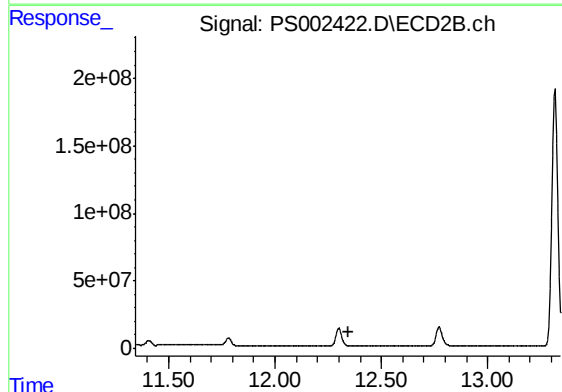


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.343 min
Response: 0
Conc: N.D.

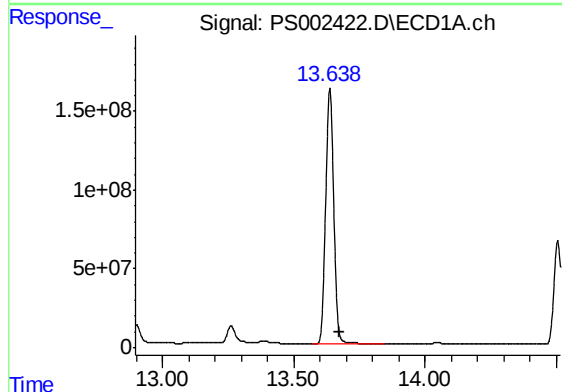


#10 Pentachlorophenol

R.T.: 13.638 min
Delta R.T.: -0.037 min
Response: 3492417431
Conc: 722.00 ng/ml

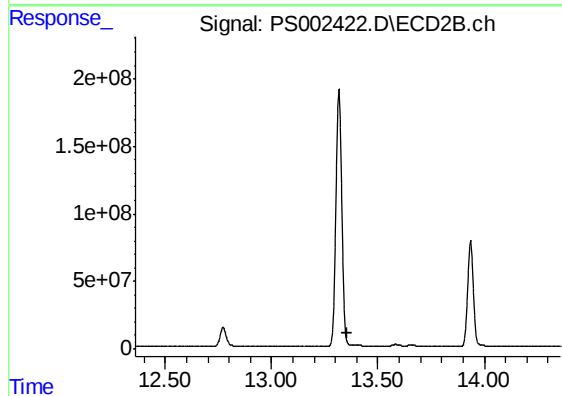

#10 Pentachlorophenol


R.T.: 13.316 min
Delta R.T.: -0.043 min
Response: -699397132
Conc: N.D.

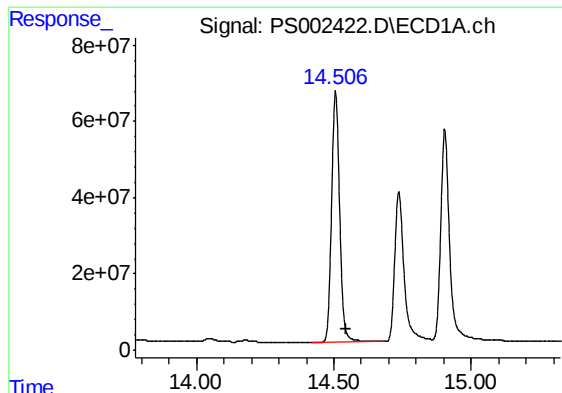

#11 2,4,5-TP (SILVEX)


R.T.: 14.506 min
Delta R.T.: -0.037 min
Response: 1348230900
Conc: 717.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

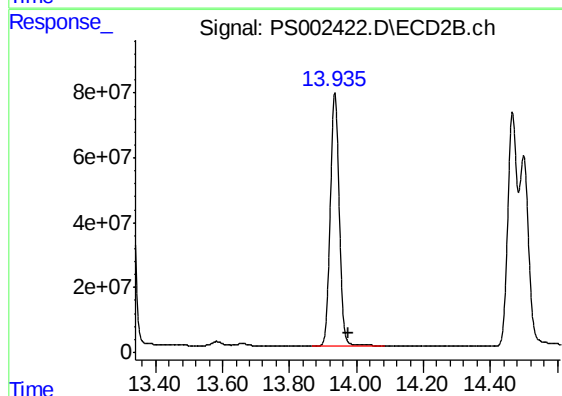


#11 2,4,5-TP (SILVEX)

R.T.: 13.936 min
Delta R.T.: -0.041 min
Response: 1443339321
Conc: 715.51 ng/ml

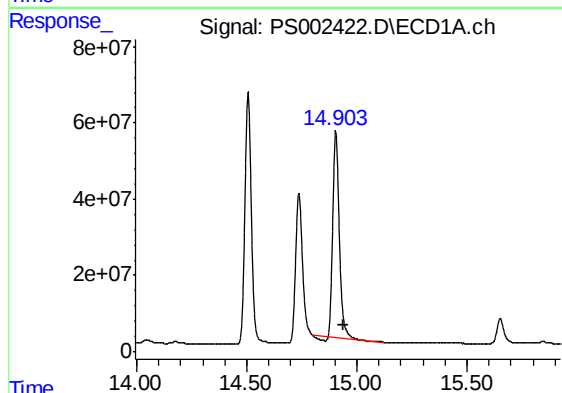


#12 2,4,5-T

R.T.: 14.904 min
Delta R.T.: -0.035 min
Response: 1088761068
Conc: 645.91 ng/ml

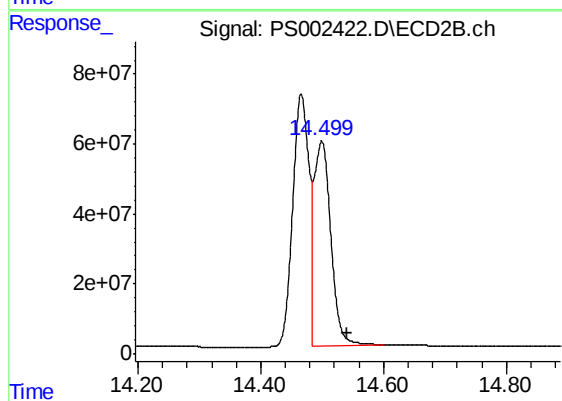

#12 2,4,5-T


R.T.: 14.500 min
Delta R.T.: -0.041 min
Response: 1097774244
Conc: 702.25 ng/ml

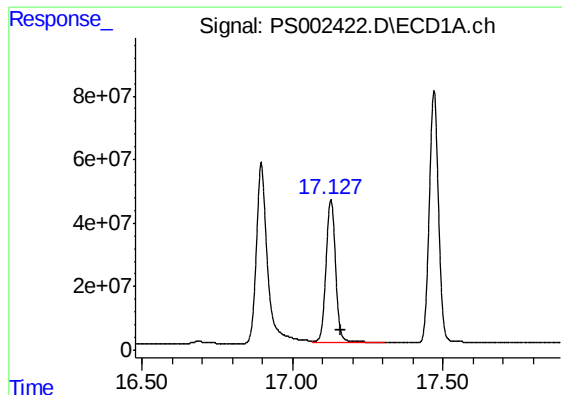

#14 DINOSEB


R.T.: 17.127 min
Delta R.T.: -0.035 min
Response: 1005682773
Conc: 704.21 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

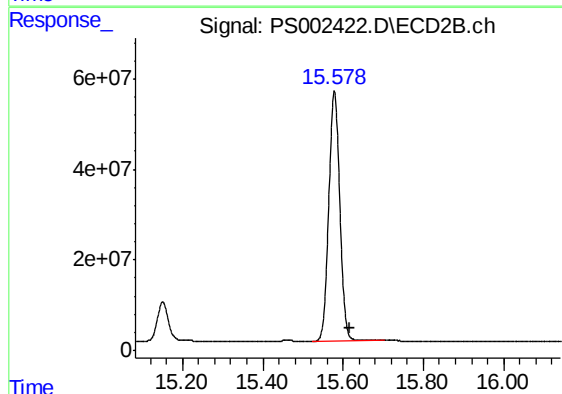


#14 DINOSEB

R.T.: 15.578 min
Delta R.T.: -0.040 min
Response: 1051144854
Conc: 702.31 ng/ml

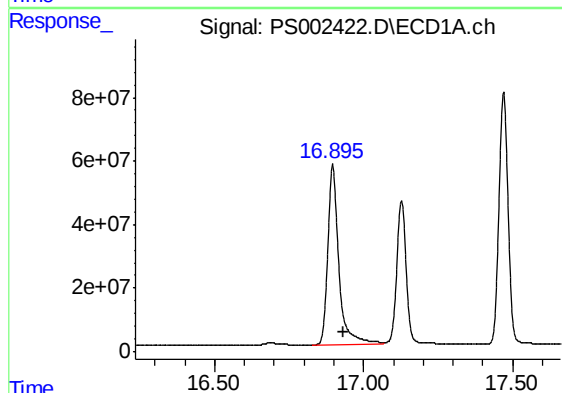


#15 Picloram

R.T.: 16.896 min
Delta R.T.: -0.035 min
Response: 1470989300
Conc: 692.64 ng/ml

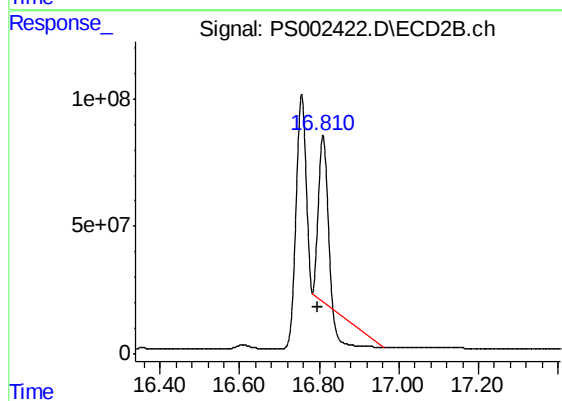

#15 Picloram


R.T.: 16.810 min
Delta R.T.: 0.015 min
Response: 547883309
Conc: 205.95 ng/ml

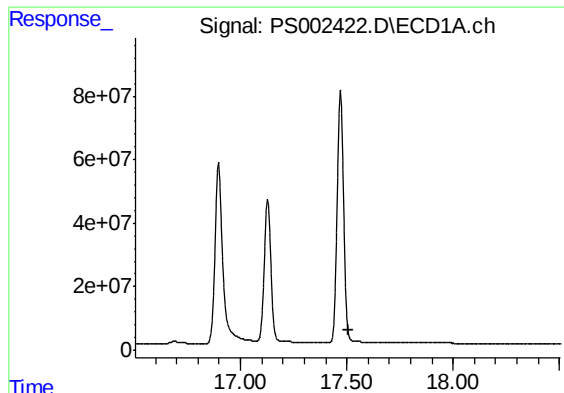

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.506 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

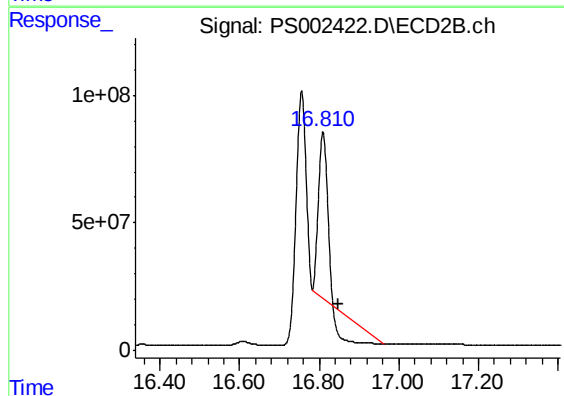

#16 DCPA

R.T.: 16.810 min
Delta R.T.: -0.038 min
Response: 547883309
Conc: 228.45 ng/ml