

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111418\
 Data File : PS002430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2018 21:16
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 02:38:55 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.403	10.895	184.7E6	271.0E6	606.457	740.495
Target Compounds							
1) T	Dalapon	2.929	2.372	294.5E6	288.3E6	667.942	669.898
2) T	3,5-DICHL...	0.000	9.051	0	166.1E6	N.D.	366.308 #
3) T	4-Nitroph...	10.997	10.042	116.2E6	118.8E6	715.969	678.270
5) T	DICAMBA	11.711	11.178	986.8E6	-955983436	712.174	N.D. #
6) T	MCPD	0.000	11.456	0	440098	N.D.	0.485 #
7) T	MCPA	0.000	11.784	0	110.5E6	N.D.	78.532 #
8) T	DICHLORPROP	12.898	0.000	246.0E6	0	710.675	N.D. #
10) T	Pentachlo...	13.633	13.317	3503.1E6	-499062418	724.199	N.D. #
11) T	2,4,5-TP ...	14.501	13.936	1355.1E6	1444.6E6	721.132	716.154
12) T	2,4,5-T	14.899	14.500	1153.9E6	1107.9E6	684.531	708.751
14) T	DINOSEB	17.121	15.577	1007.2E6	1049.7E6	705.250	701.371
15) T	Picloram	16.891	16.807	1454.9E6	585.2E6	685.075	219.978 #
16) T	DCPA	0.000	16.807	0	585.2E6	N.D.	244.015 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111418\
Data File : PS002430.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2018 21:16
Operator : EI\SJ
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 02:38:55 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

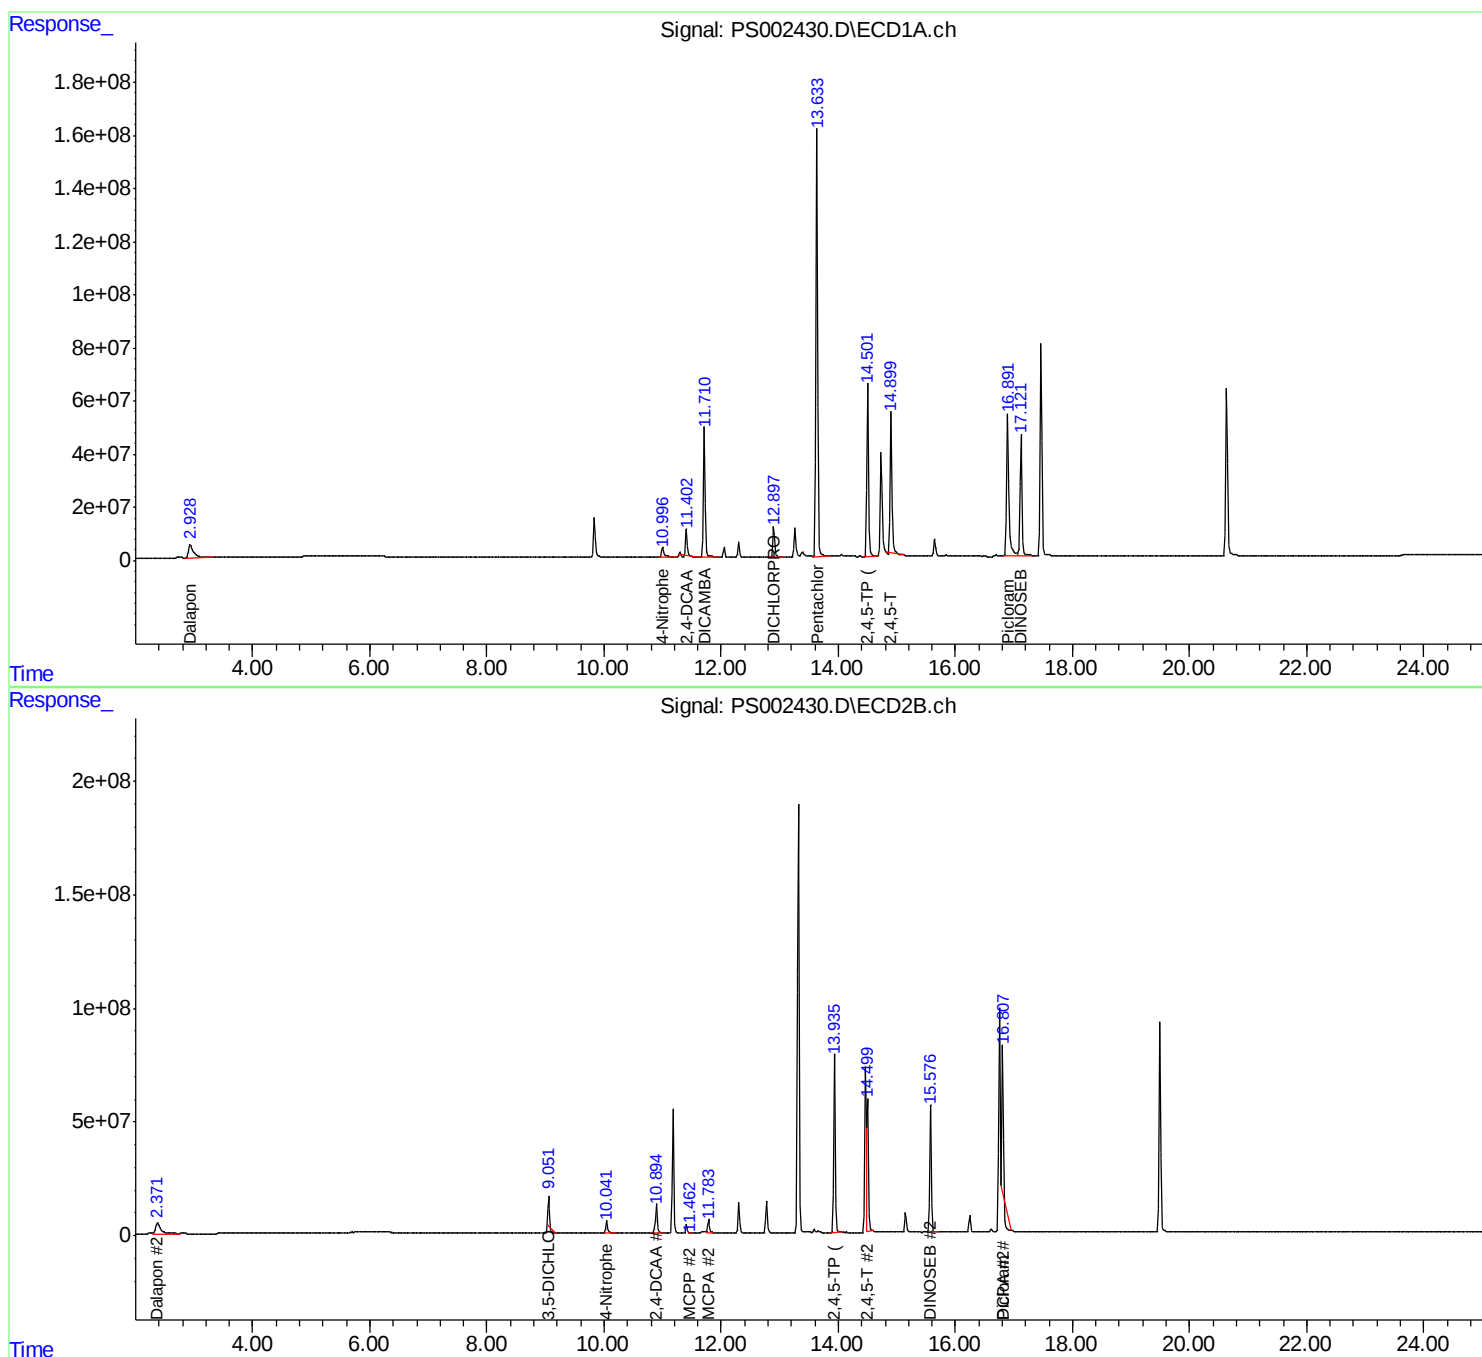


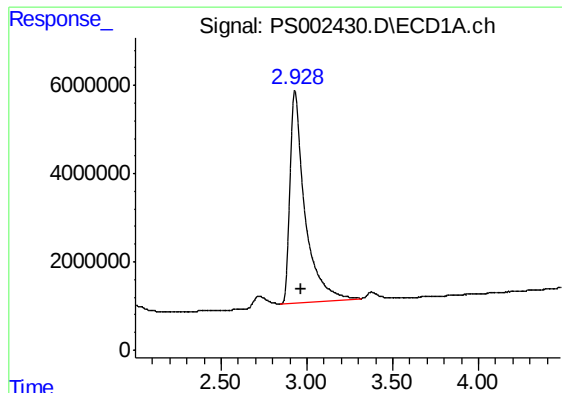

#1 Dalapon


R.T.: 2.929 min
Delta R.T.: -0.040 min
Response: 294528840
Conc: 667.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

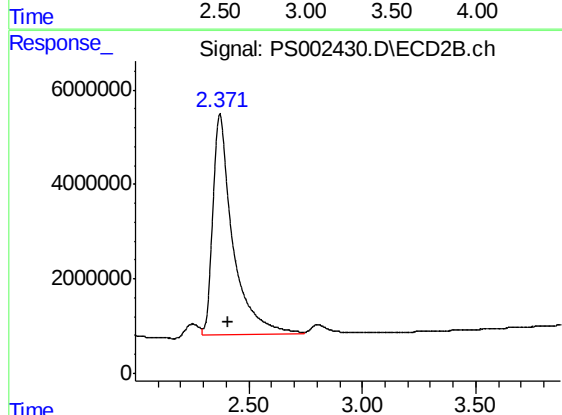


#1 Dalapon

R.T.: 2.372 min
Delta R.T.: -0.040 min
Response: 288319728
Conc: 669.90 ng/ml

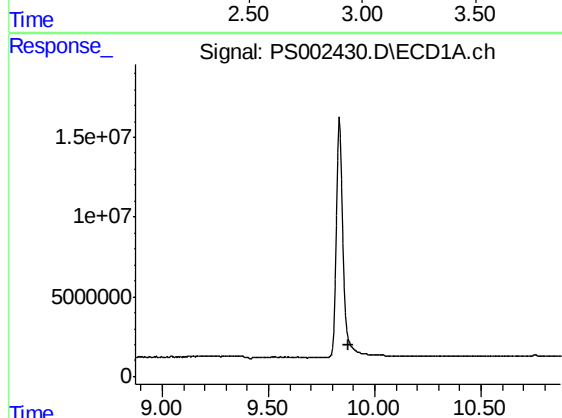


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.874 min
Response: 0
Conc: N.D.

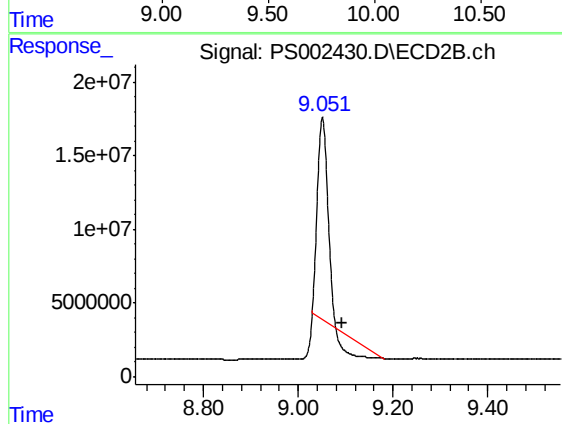

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.051 min
Delta R.T.: -0.041 min
Response: 166064620
Conc: 366.31 ng/ml

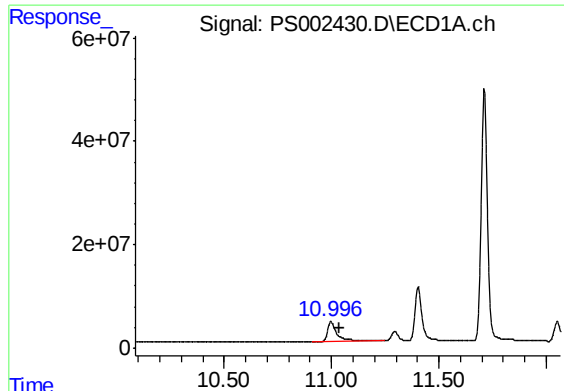

#3 4-Nitrophenol


R.T.: 10.997 min
Delta R.T.: -0.041 min
Response: 116168371
Conc: 715.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

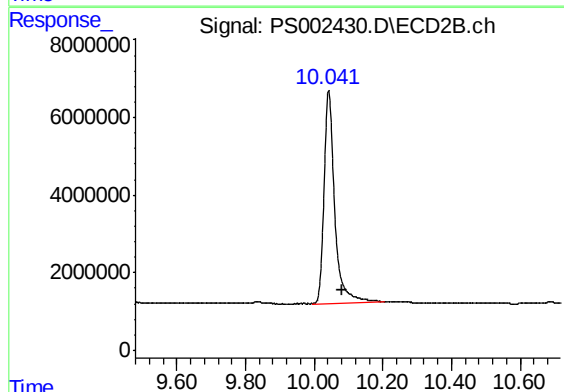


#3 4-Nitrophenol

R.T.: 10.042 min
Delta R.T.: -0.041 min
Response: 118841262
Conc: 678.27 ng/ml

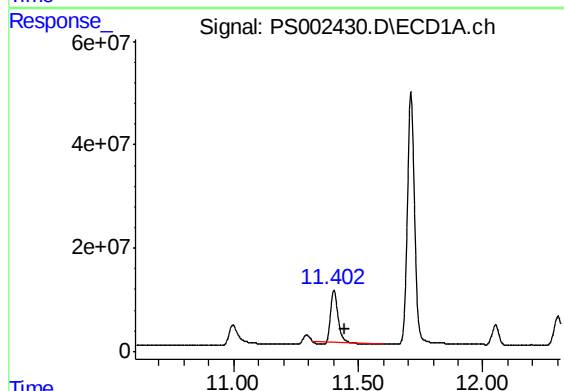


#4 2,4-DCAA

R.T.: 11.403 min
Delta R.T.: -0.041 min
Response: 184726452
Conc: 606.46 ng/ml

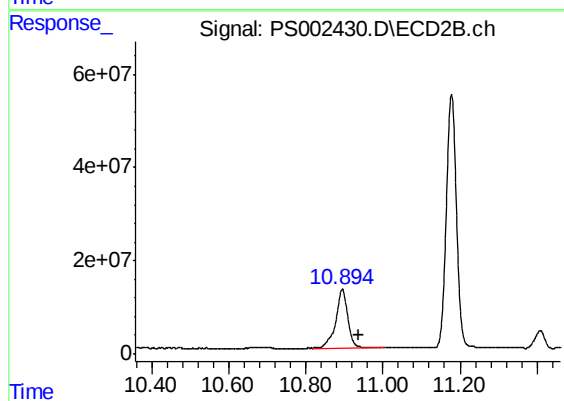

#4 2,4-DCAA


R.T.: 10.895 min
Delta R.T.: -0.041 min
Response: 270956046
Conc: 740.49 ng/ml

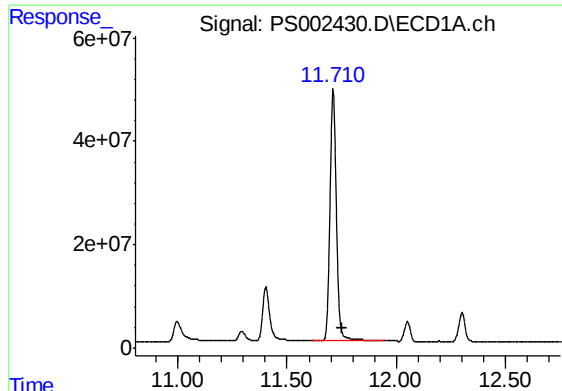

#5 DICAMBA


R.T.: 11.711 min
Delta R.T.: -0.041 min
Response: 986801228
Conc: 712.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

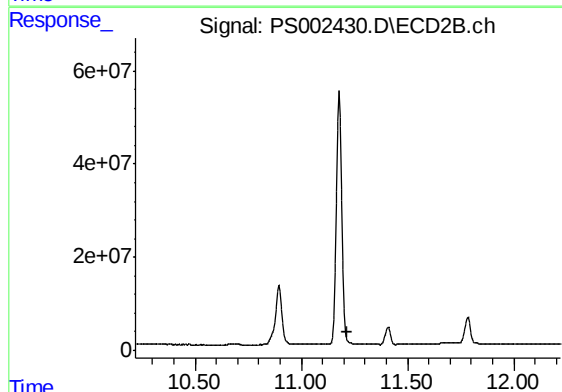


#5 DICAMBA

R.T.: 11.178 min
Delta R.T.: -0.041 min
Response: -955983436
Conc: N.D.

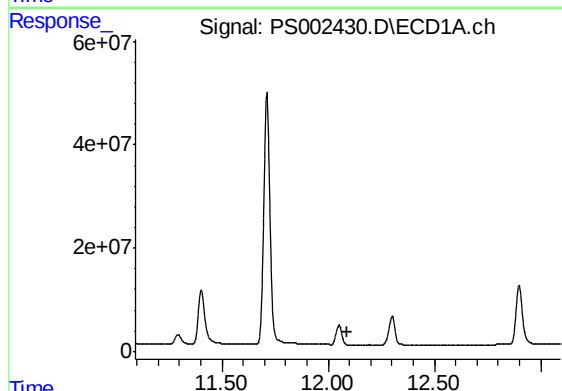


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 12.093 min
Response: 0
Conc: N.D.

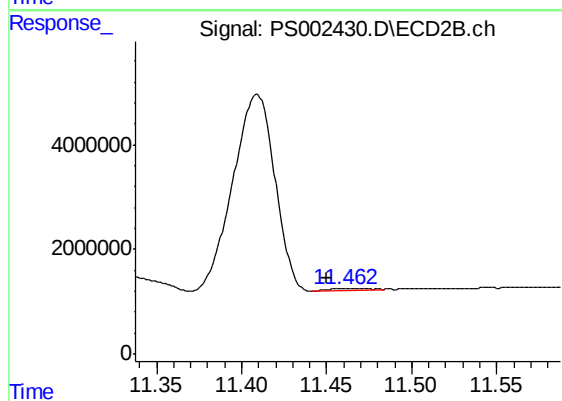

#6 MCPP


R.T.: 11.456 min
Delta R.T.: 0.006 min
Response: 440098
Conc: 0.49 ug/ml

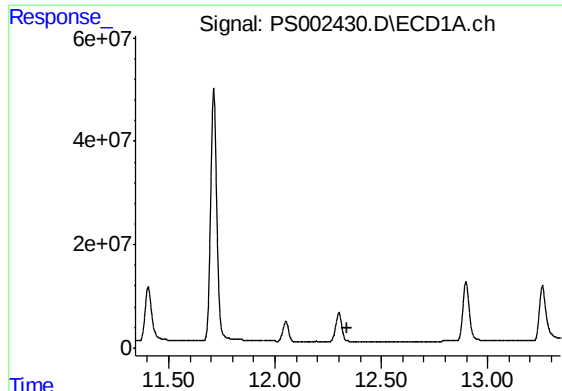

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

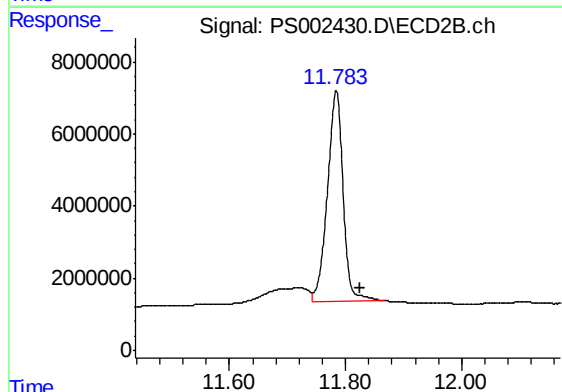


#7 MCPA

R.T.: 11.784 min
Delta R.T.: -0.042 min
Response: 110511319
Conc: 78.53 ug/ml

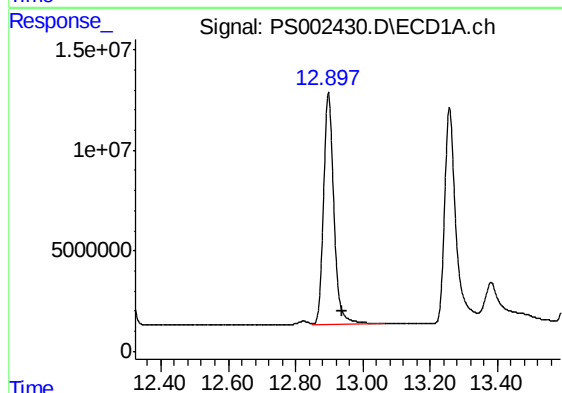


#8 DICHLORPROP

R.T.: 12.898 min
Delta R.T.: -0.041 min
Response: 246044404
Conc: 710.67 ng/ml

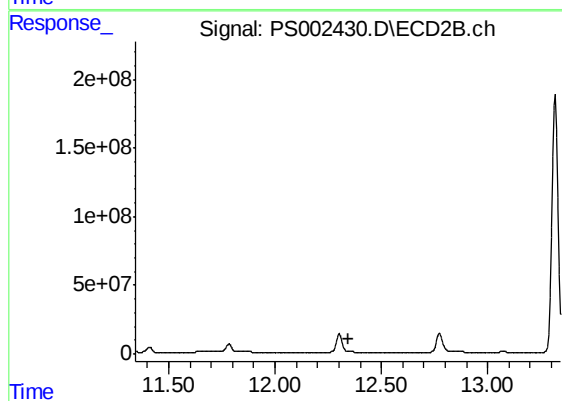

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.343 min
Response: 0
Conc: N.D.

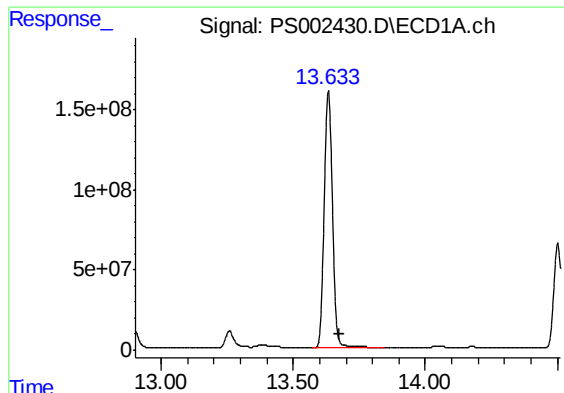

#10 Pentachlorophenol


R.T.: 13.633 min
Delta R.T.: -0.042 min
Response: 3503063154
Conc: 724.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

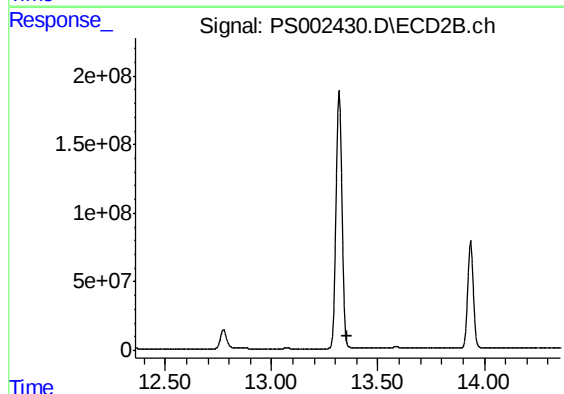


#10 Pentachlorophenol

R.T.: 13.317 min
Delta R.T.: -0.041 min
Response: -499062418
Conc: N.D.

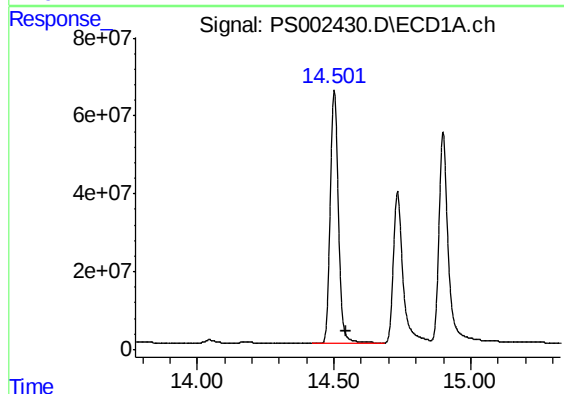


#11 2,4,5-TP (SILVEX)

R.T.: 14.501 min
Delta R.T.: -0.042 min
Response: 1355111047
Conc: 721.13 ng/ml

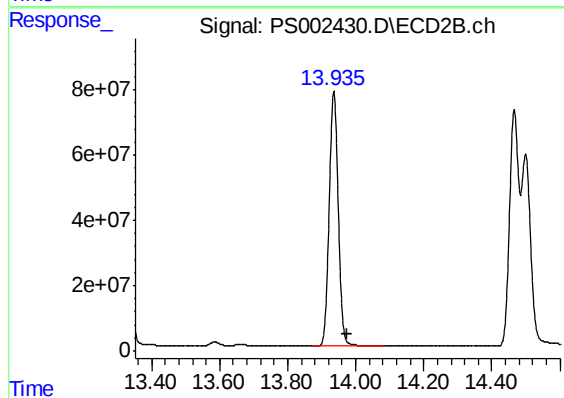

#11 2,4,5-TP (SILVEX)


R.T.: 13.936 min
Delta R.T.: -0.041 min
Response: 1444628668
Conc: 716.15 ng/ml

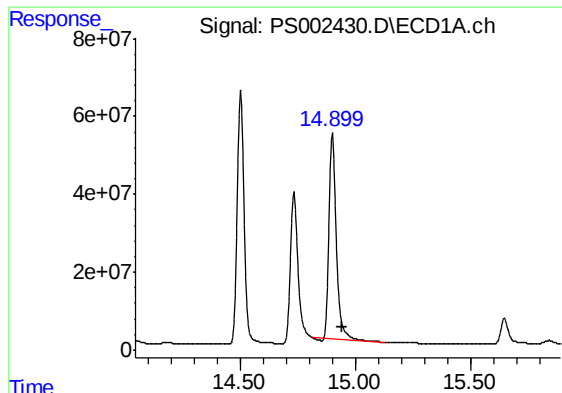

#12 2,4,5-T


R.T.: 14.899 min
Delta R.T.: -0.040 min
Response: 1153856695
Conc: 684.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

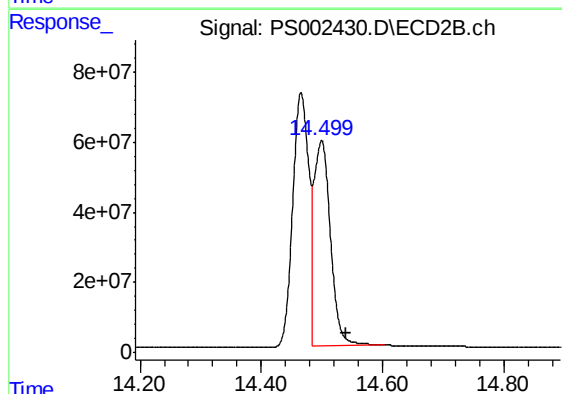


#12 2,4,5-T

R.T.: 14.500 min
Delta R.T.: -0.041 min
Response: 1107935635
Conc: 708.75 ng/ml

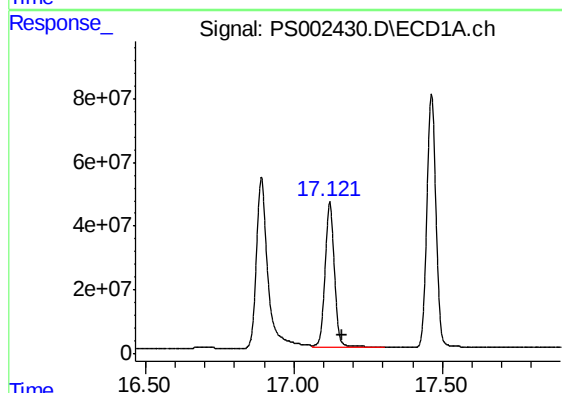


#14 DINOSEB

R.T.: 17.121 min
Delta R.T.: -0.042 min
Response: 1007174369
Conc: 705.25 ng/ml

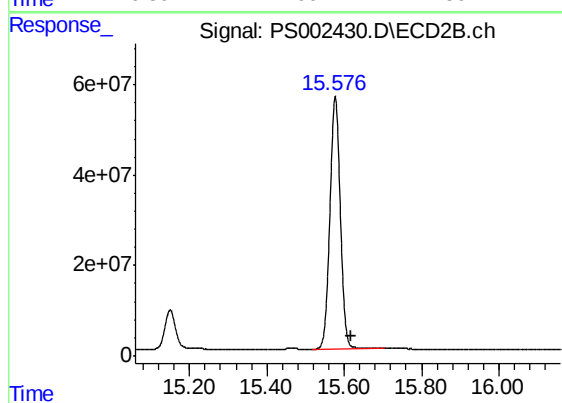

#14 DINOSEB


R.T.: 15.577 min
Delta R.T.: -0.042 min
Response: 1049733667
Conc: 701.37 ng/ml

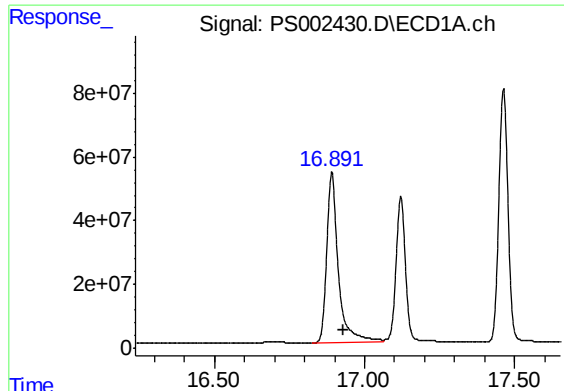

#15 Picloram


R.T.: 16.891 min
Delta R.T.: -0.040 min
Response: 1454913634
Conc: 685.07 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDCCC750

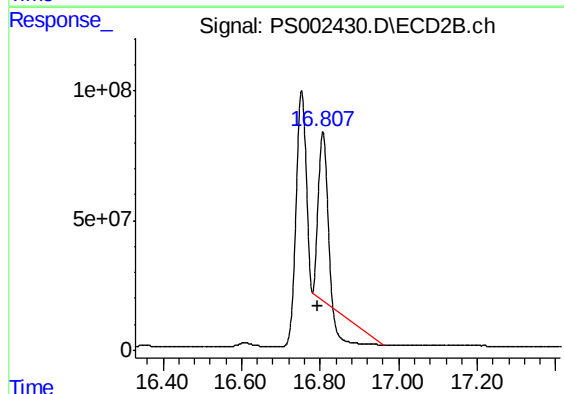


#15 Picloram

R.T.: 16.807 min
Delta R.T.: 0.012 min
Response: 585207423
Conc: 219.98 ng/ml

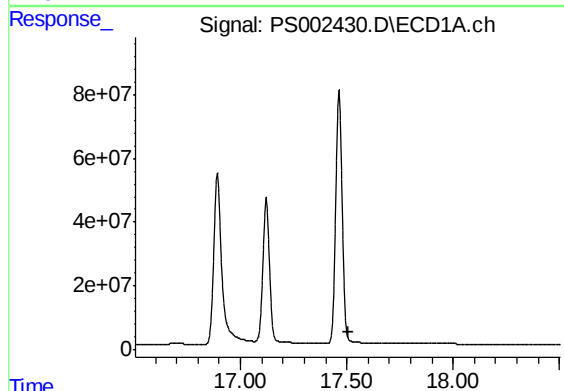

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.506 min
Response: 0
Conc: N.D.

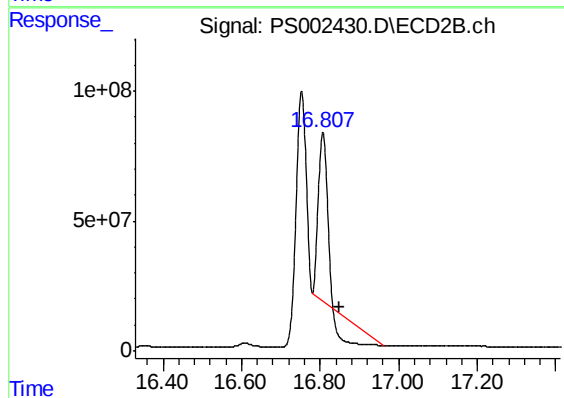

#16 DCPA

R.T.: 16.807 min
Delta R.T.: -0.041 min
Response: 585207423
Conc: 244.02 ng/ml