

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111418\
 Data File : PS002432.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2018 22:18
 Operator : EI\SJ
 Sample : J5925-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-5S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 02:39:22 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.444	10.937	138.1E6	137.1E6	453.408	374.806
Target Compounds							
1) T	Dalapon	0.000	2.375	0	2568324	N.D.	5.967 #
3) T	4-Nitroph...	11.091	10.095	2257247	4222505	13.912	24.099 #
6) T	MCP	12.124	0.000	13049540	0	13.904	N.D. #
7) T	MCPA	0.000	11.837	0	1719304	N.D.	1.222 #
8) T	DICHLORPROP	0.000	12.290	0	421251	N.D.	1.271 #
10) T	Pentachlo...	0.000	13.354	0	446035	N.D.	0.088 #
11) T	2,4,5-TP ...	0.000	13.969	0	203031	N.D.	0.101 #
12) T	2,4,5-T	0.000	14.550	0	223082	N.D.	0.143 #
13) T	2,4-DB	15.634	0.000	3547551	0	18.312	N.D. #
14) T	DINOSEB	0.000	15.668	0	817383	N.D.	0.546 #
15) T	Picloram	0.000	16.860	0	7481362	N.D.	2.812 #
16) T	DCPA	0.000	16.860	0	7481362	N.D.	3.120 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111418\
Data File : PS002432.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2018 22:18
Operator : EI\SJ
Sample : J5925-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-5S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 02:39:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

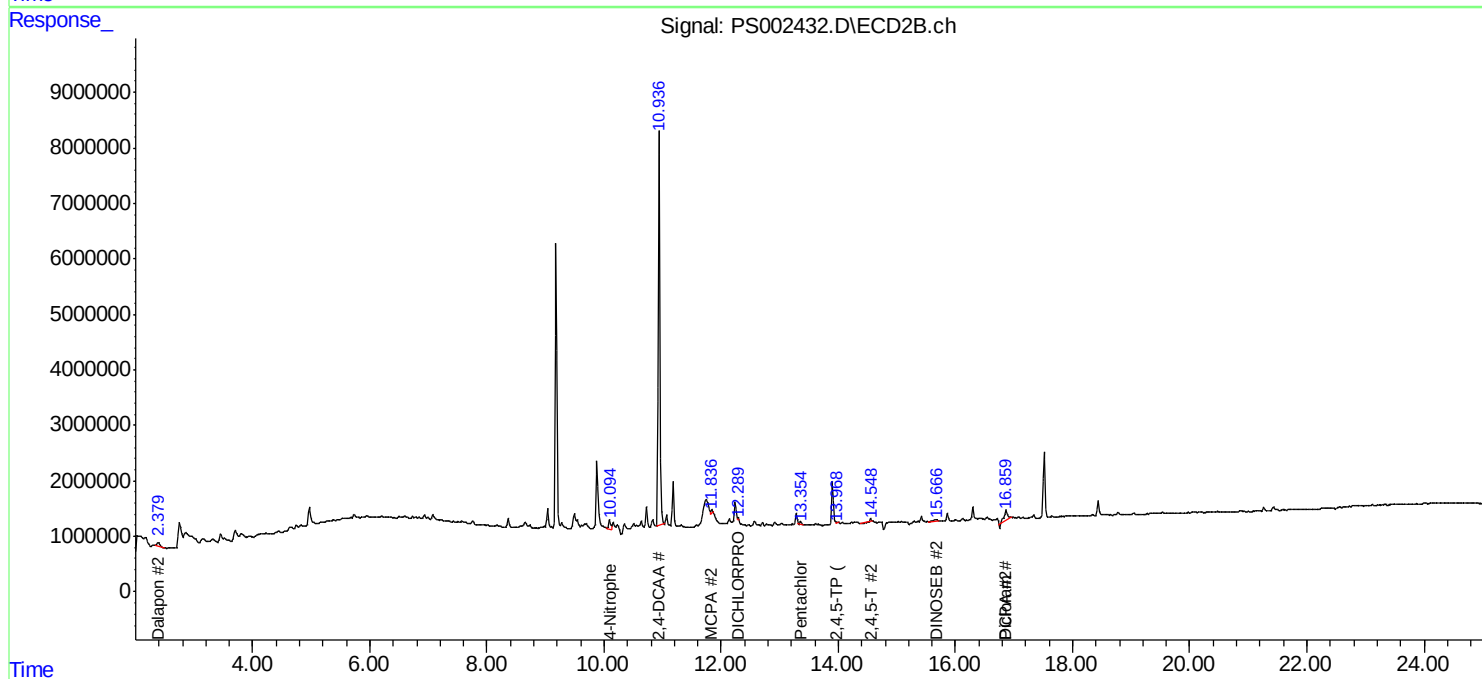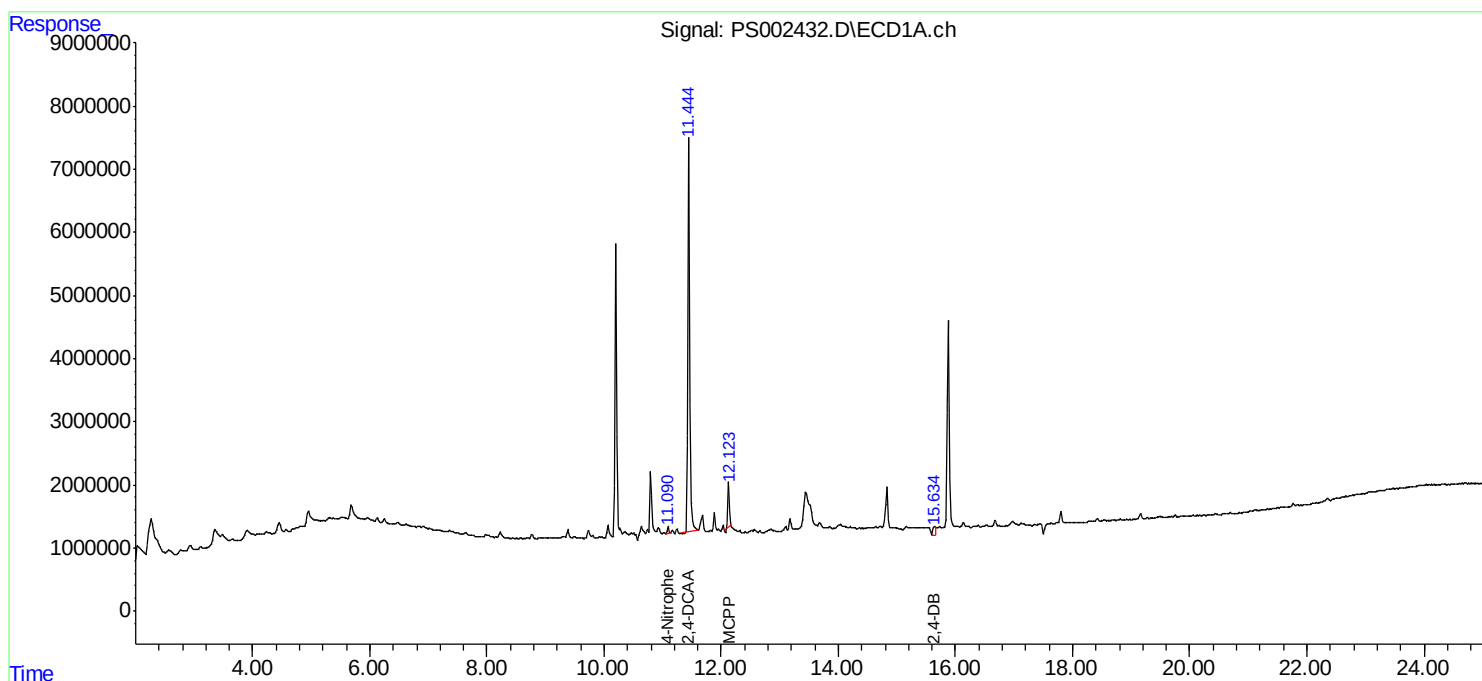


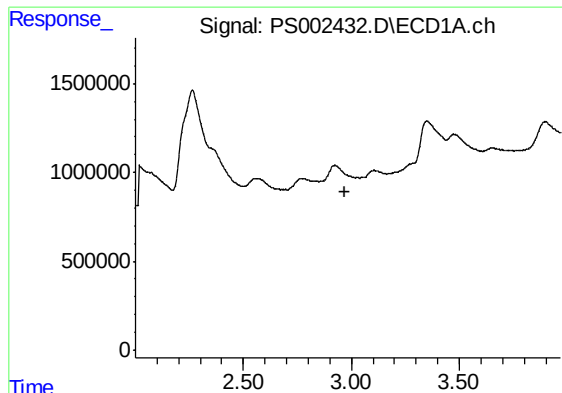

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.969 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-5S

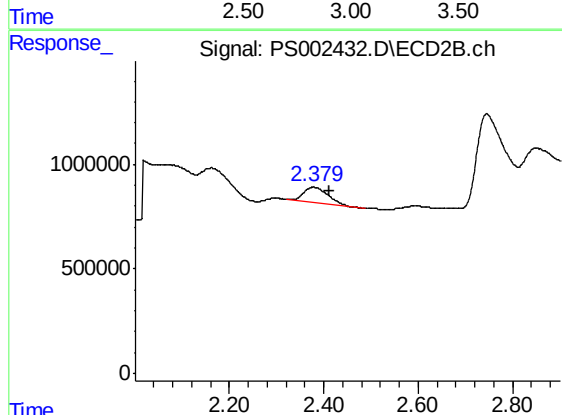


#1 Dalapon

R.T.: 2.375 min
Delta R.T.: -0.037 min
Response: 2568324
Conc: 5.97 ng/ml

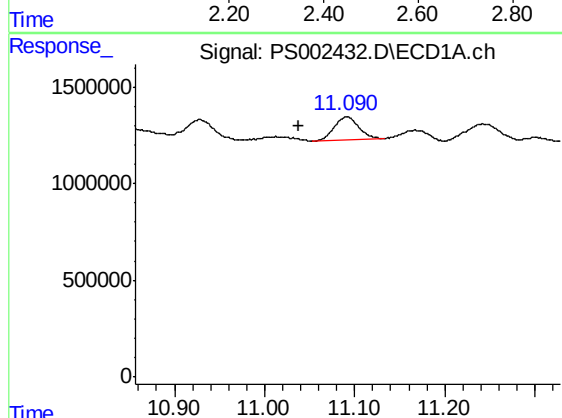


#3 4-Nitrophenol

R.T.: 11.091 min
Delta R.T.: 0.054 min
Response: 2257247
Conc: 13.91 ng/ml

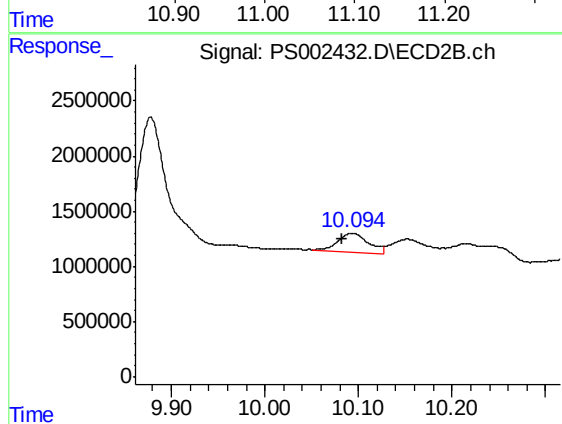

#3 4-Nitrophenol


R.T.: 10.095 min
Delta R.T.: 0.011 min
Response: 4222505
Conc: 24.10 ng/ml

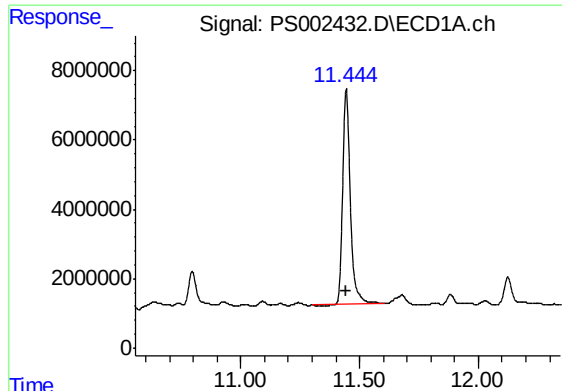

#4 2,4-DCAA


R.T.: 11.444 min
Delta R.T.: 0.000 min
Response: 138107770
Conc: 453.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-5S

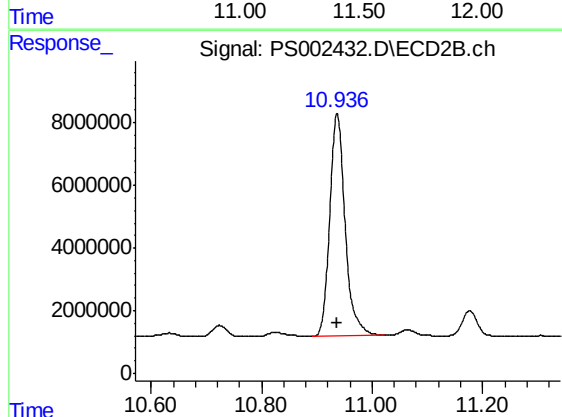


#4 2,4-DCAA

R.T.: 10.937 min
Delta R.T.: 0.000 min
Response: 137146050
Conc: 374.81 ng/ml

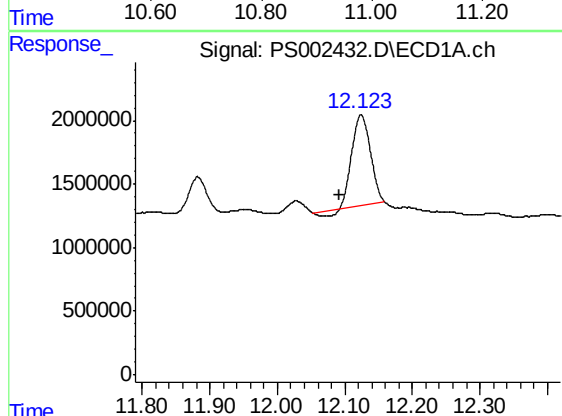


#6 MCPP

R.T.: 12.124 min
Delta R.T.: 0.031 min
Response: 13049540
Conc: 13.90 ug/ml

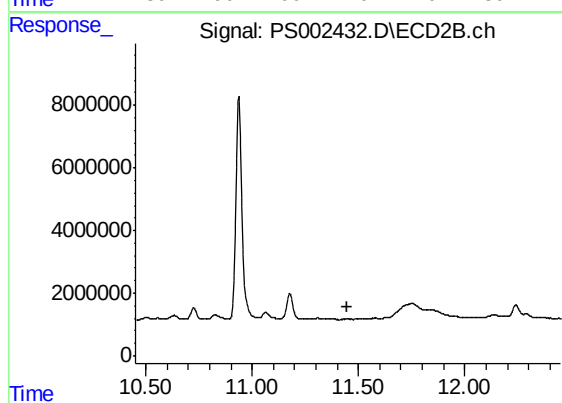

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 11.450 min
Response: 0
Conc: N.D.

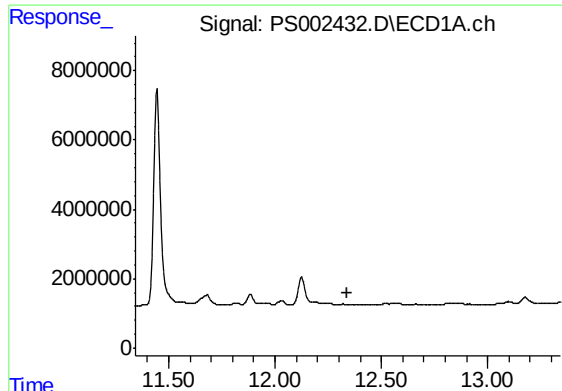

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-5S

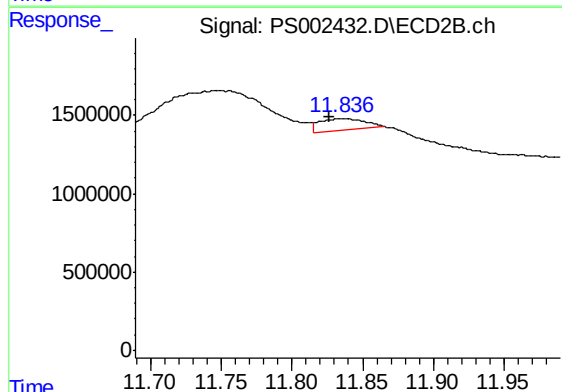


#7 MCPA

R.T.: 11.837 min
Delta R.T.: 0.010 min
Response: 1719304
Conc: 1.22 ug/ml

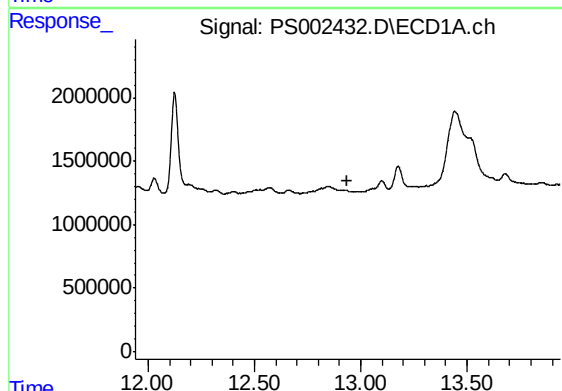


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.939 min
Response: 0
Conc: N.D.

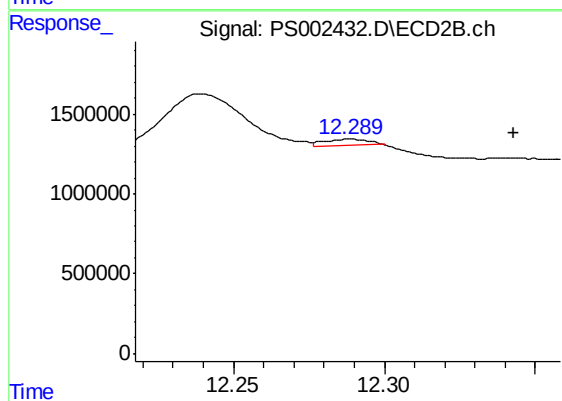

#8 DICHLORPROP


R.T.: 12.290 min
Delta R.T.: -0.053 min
Response: 421251
Conc: 1.27 ng/ml

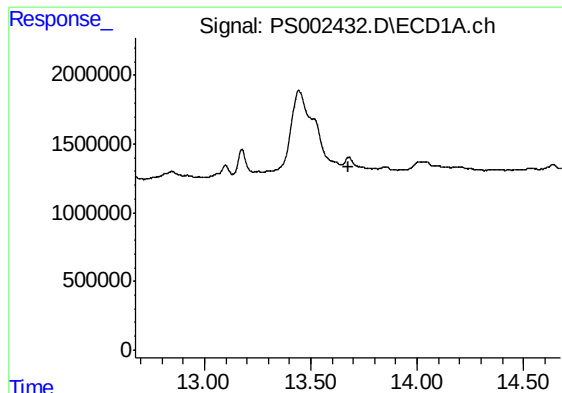

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.675 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-5S

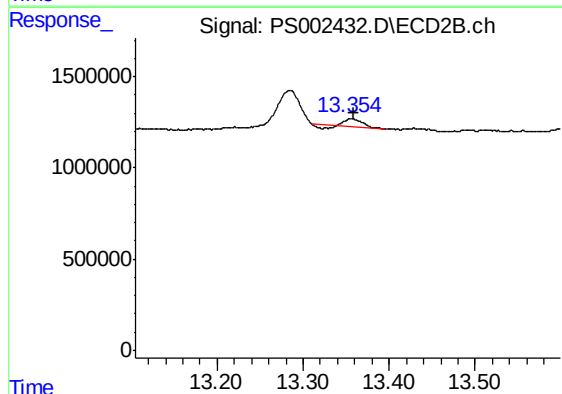


#10 Pentachlorophenol

R.T.: 13.354 min
Delta R.T.: -0.004 min
Response: 446035
Conc: 0.09 ng/ml

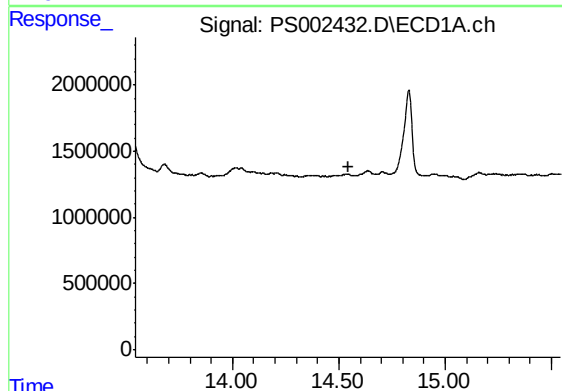


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.543 min
Response: 0
Conc: N.D.

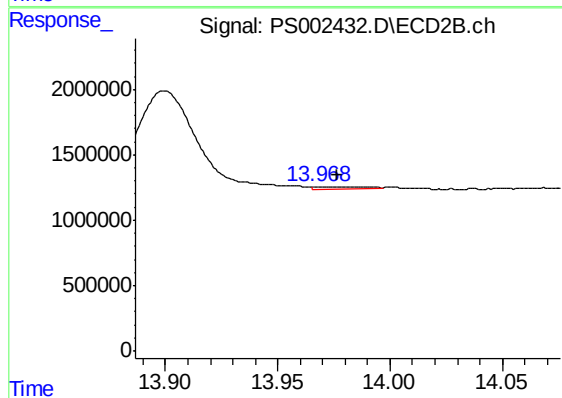

#11 2,4,5-TP (SILVEX)


R.T.: 13.969 min
Delta R.T.: -0.008 min
Response: 203031
Conc: 0.10 ng/ml

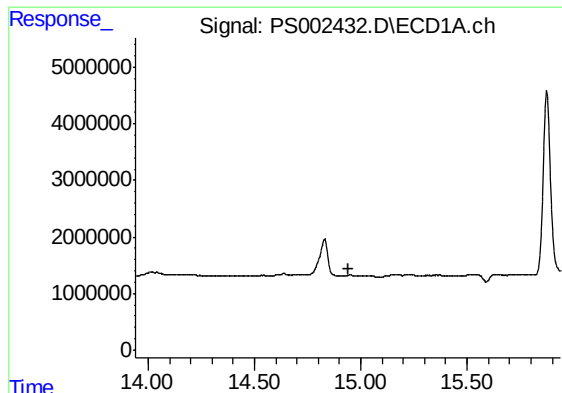

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 14.940 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-5S

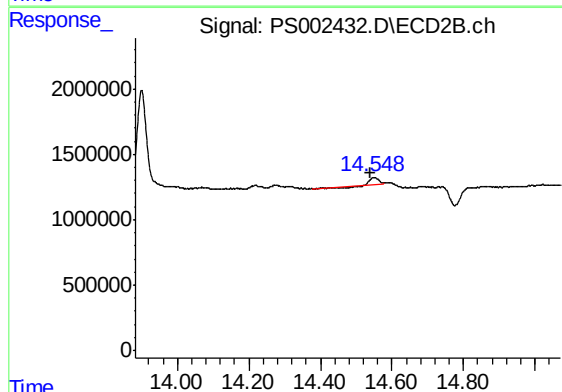


#12 2,4,5-T

R.T.: 14.550 min
Delta R.T.: 0.009 min
Response: 223082
Conc: 0.14 ng/ml

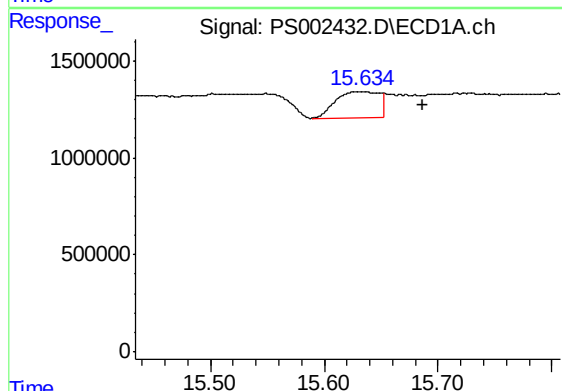


#13 2,4-DB

R.T.: 15.634 min
Delta R.T.: -0.052 min
Response: 3547551
Conc: 18.31 ng/ml

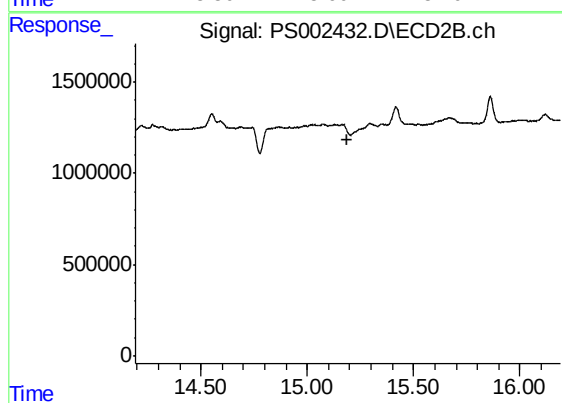

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 15.191 min
Response: 0
Conc: N.D.

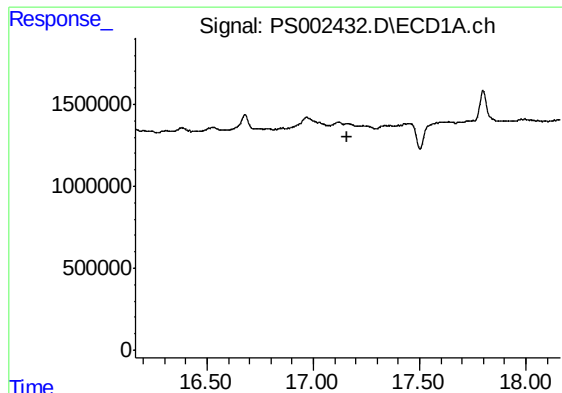

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.163 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-5S

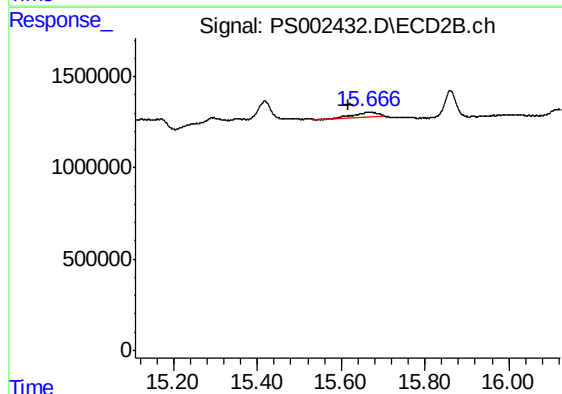


#14 DINOSEB

R.T.: 15.668 min
Delta R.T.: 0.049 min
Response: 817383
Conc: 0.55 ng/ml

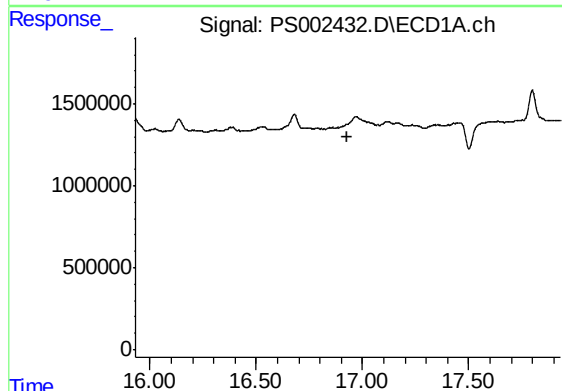


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.931 min
Response: 0
Conc: N.D.

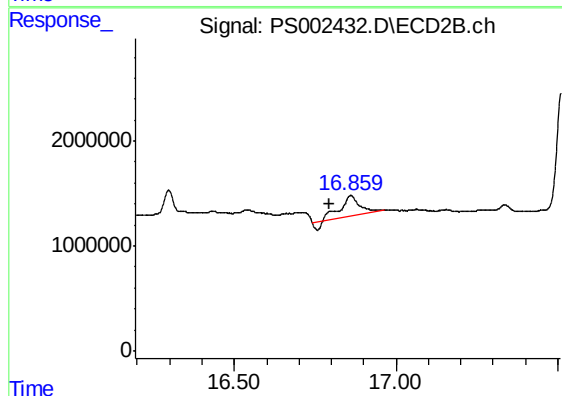

#15 Picloram


R.T.: 16.860 min
Delta R.T.: 0.065 min
Response: 7481362
Conc: 2.81 ng/ml

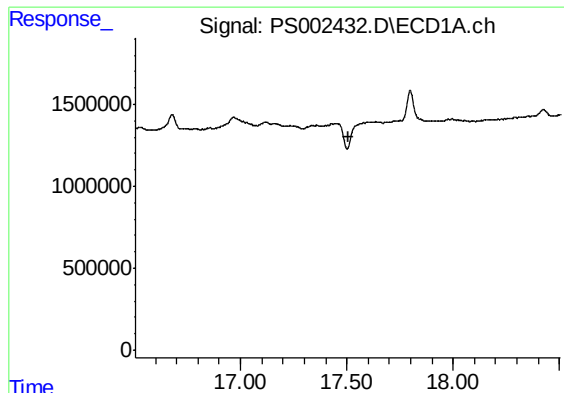

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.506 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-5S

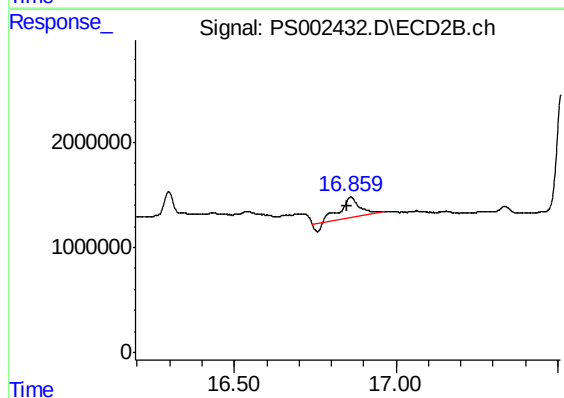

#16 DCPA

R.T.: 16.860 min
Delta R.T.: 0.012 min
Response: 7481362
Conc: 3.12 ng/ml