

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111418\
 Data File : PS002433.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2018 22:49
 Operator : EI\SJ
 Sample : J5925-16
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-6S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 02:39:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.423	10.915	121.5E6	119.6E6	398.897	326.772
Target Compounds							
1) T	Dalapon	2.904	2.351	3948427	1557614	8.954	3.619 #
2) T	3,5-DICHL...	0.000	9.159	0	61670620	N.D.	136.034 #
3) T	4-Nitroph...	11.070	10.070	1879016	3435801	11.581	19.609 #
5) T	DICAMBA	0.000	11.156	0	5642889	N.D.	4.171 #
6) T	MCPD	12.103	0.000	13522921	0	14.409	N.D. #
7) T	MCPA	0.000	11.813	0	4826482	N.D.	3.430 #
10) T	Pentachlo...	13.658	13.338	3637092	1354220	0.752	0.266 #
11) T	2,4,5-TP ...	0.000	13.950	0	363763	N.D.	0.180 #
12) T	2,4,5-T	0.000	14.526	0	656589	N.D.	0.420 #
14) T	DINOSEB	0.000	15.643	0	1633048	N.D.	1.091 #
15) T	Picloram	0.000	16.839	0	9531193	N.D.	3.583 #
16) T	DCPA	0.000	16.839	0	9531193	N.D.	3.974 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111418\
Data File : PS002433.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2018 22:49
Operator : EI\SJ
Sample : J5925-16
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-6S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 02:39:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

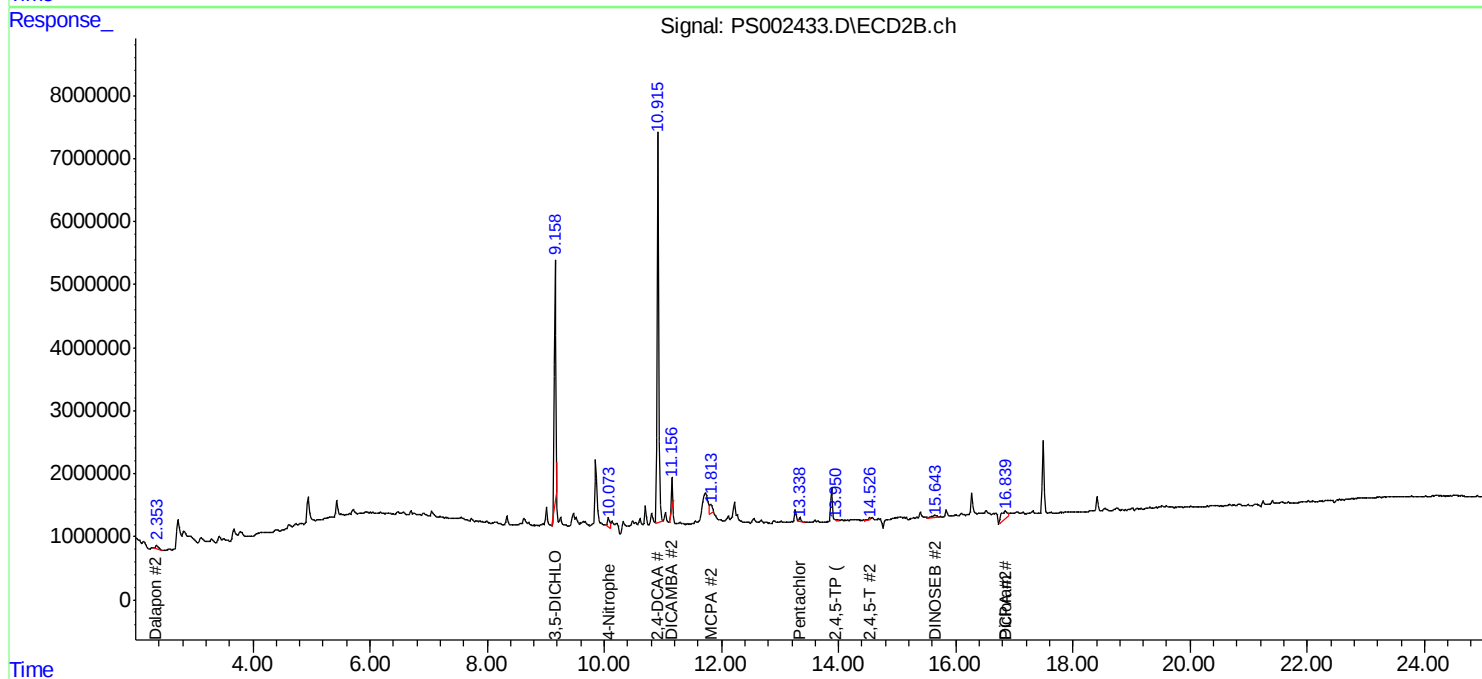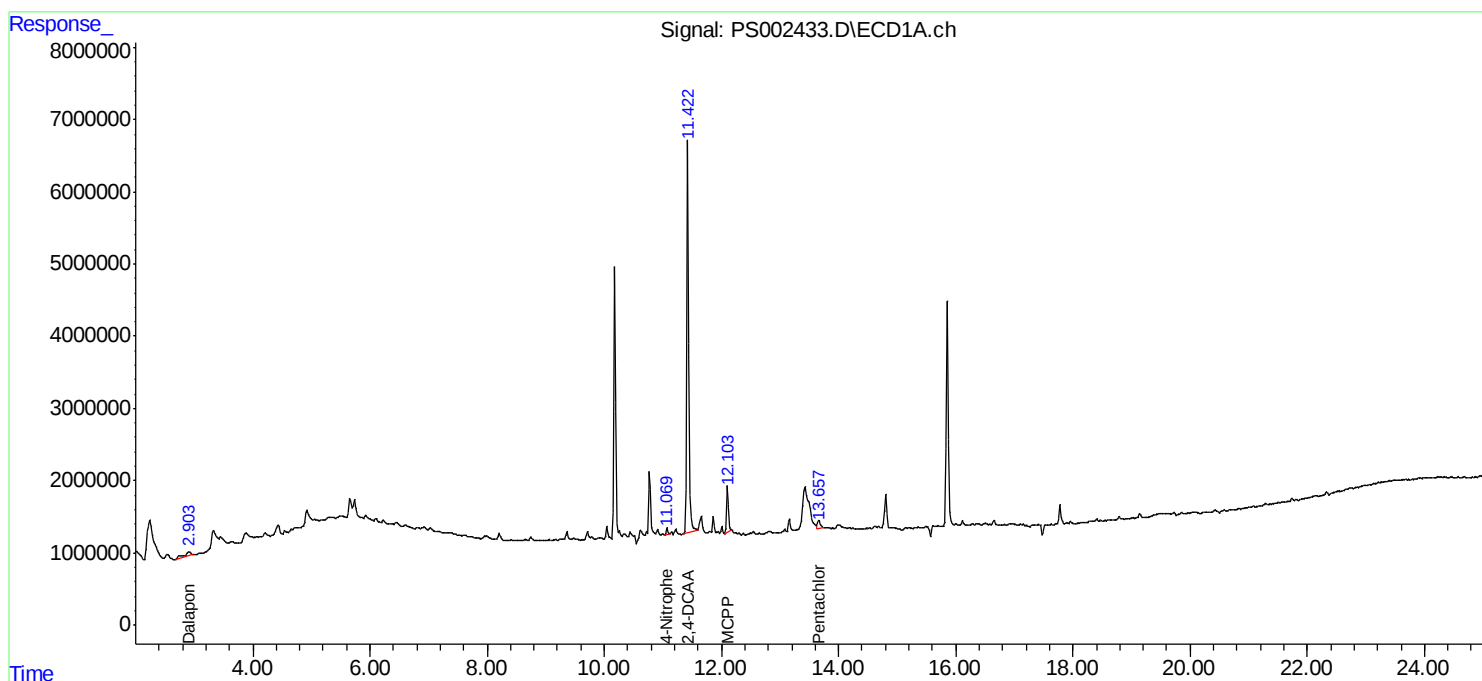


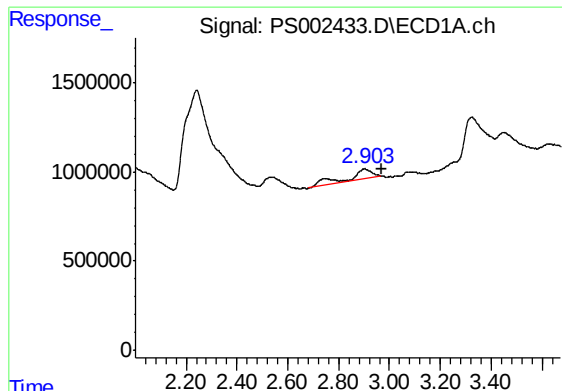

#1 Dalapon


R.T.: 2.904 min
Delta R.T.: -0.065 min
Response: 3948427
Conc: 8.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6S

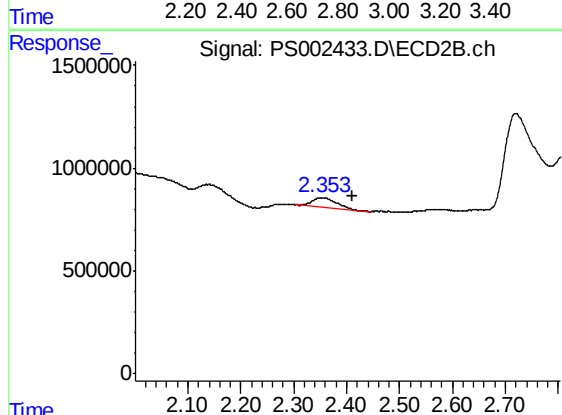


#1 Dalapon

R.T.: 2.351 min
Delta R.T.: -0.061 min
Response: 1557614
Conc: 3.62 ng/ml

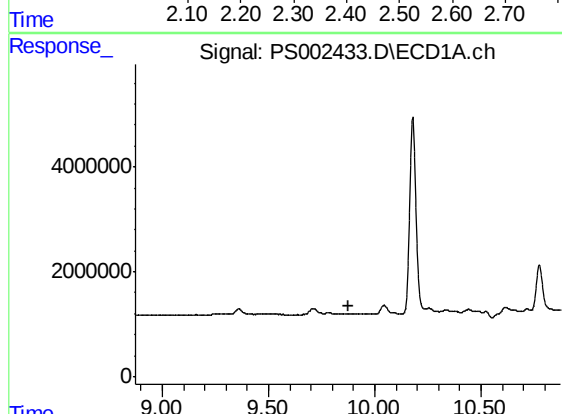


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.874 min
Response: 0
Conc: N.D.

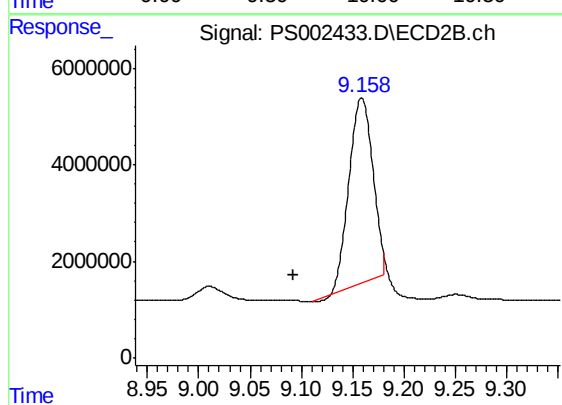

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.159 min
Delta R.T.: 0.067 min
Response: 61670620
Conc: 136.03 ng/ml

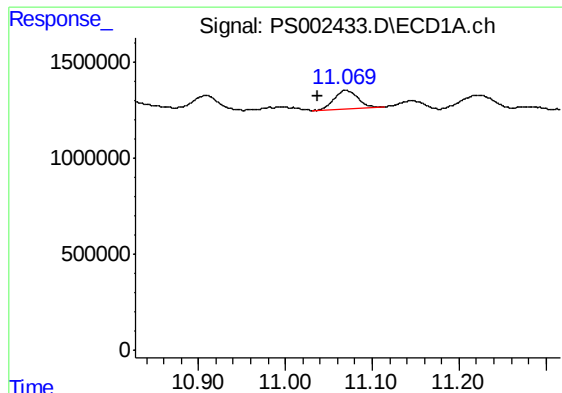

#3 4-Nitrophenol


R.T.: 11.070 min
Delta R.T.: 0.032 min
Response: 1879016
Conc: 11.58 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-6S

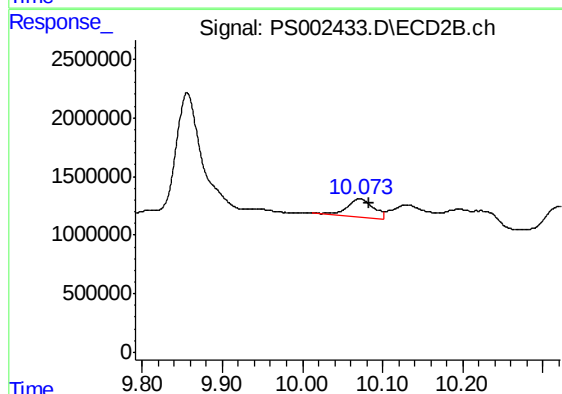


#3 4-Nitrophenol

R.T.: 10.070 min
Delta R.T.: -0.013 min
Response: 3435801
Conc: 19.61 ng/ml

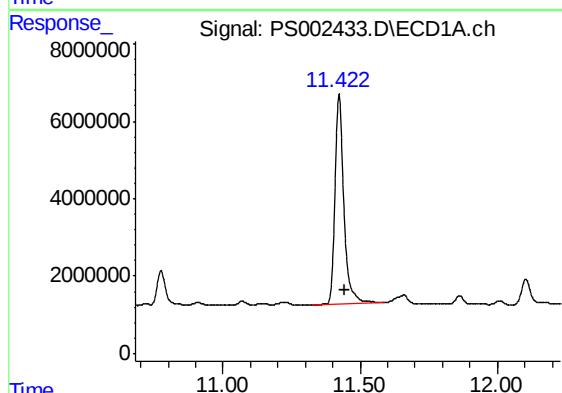


#4 2,4-DCAA

R.T.: 11.423 min
Delta R.T.: -0.021 min
Response: 121503730
Conc: 398.90 ng/ml

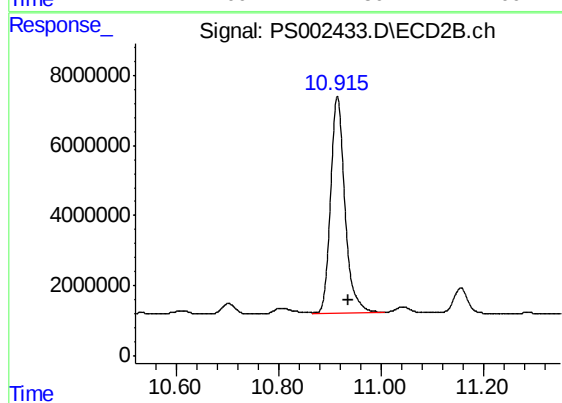

#4 2,4-DCAA


R.T.: 10.915 min
Delta R.T.: -0.021 min
Response: 119569839
Conc: 326.77 ng/ml

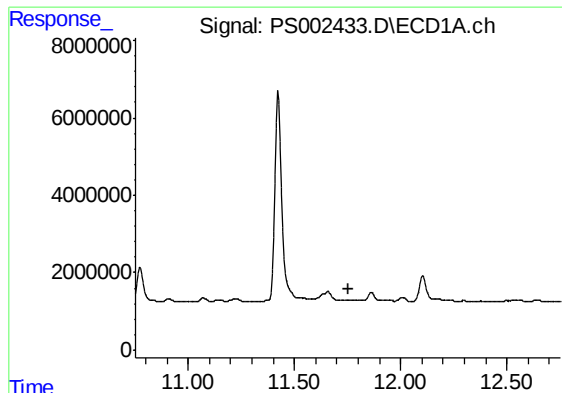

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6S

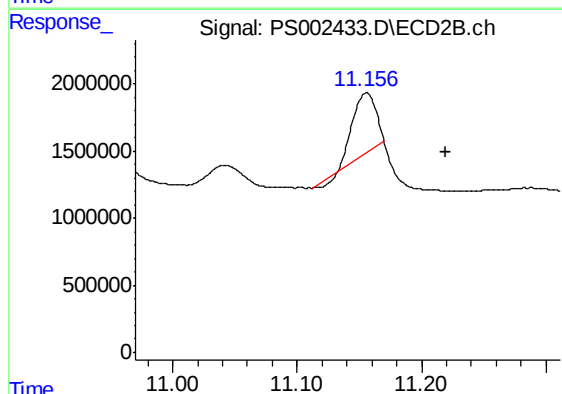


#5 DICAMBA

R.T.: 11.156 min
Delta R.T.: -0.063 min
Response: 5642889
Conc: 4.17 ng/ml

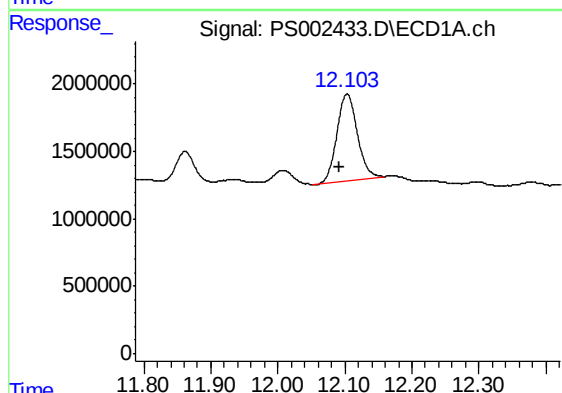


#6 MCPP

R.T.: 12.103 min
Delta R.T.: 0.011 min
Response: 13522921
Conc: 14.41 ug/ml

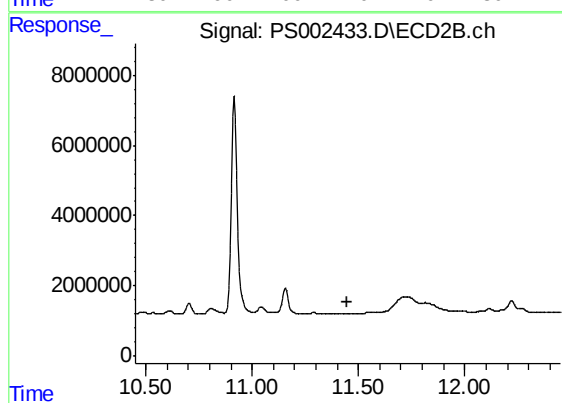

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.450 min
Response: 0
Conc: N.D.

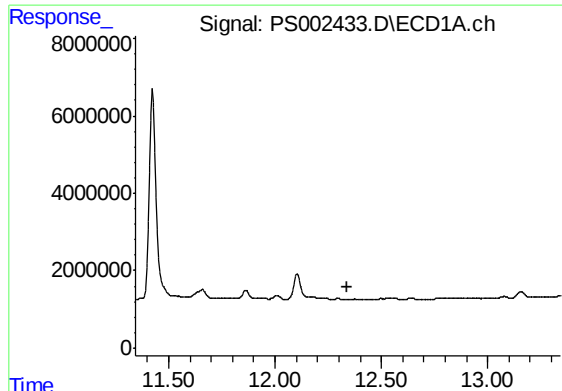

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6S

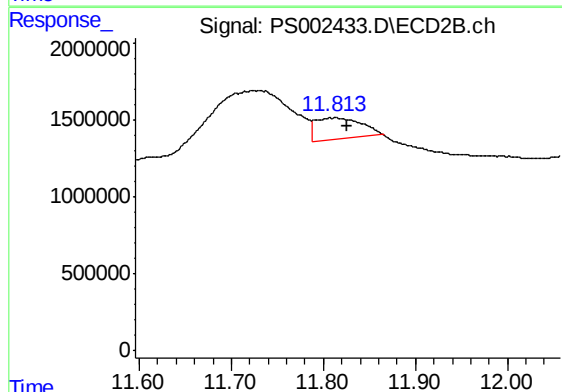


#7 MCPA

R.T.: 11.813 min
Delta R.T.: -0.013 min
Response: 4826482
Conc: 3.43 ug/ml

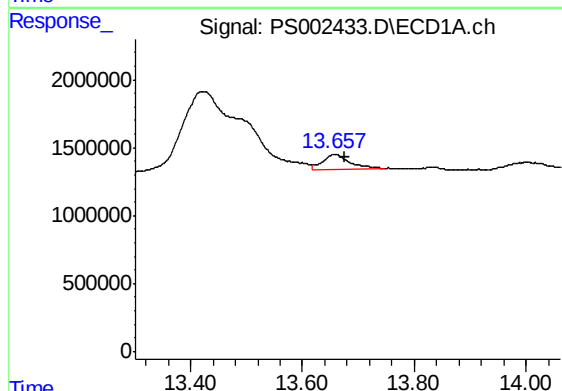


#10 Pentachlorophenol

R.T.: 13.658 min
Delta R.T.: -0.017 min
Response: 3637092
Conc: 0.75 ng/ml

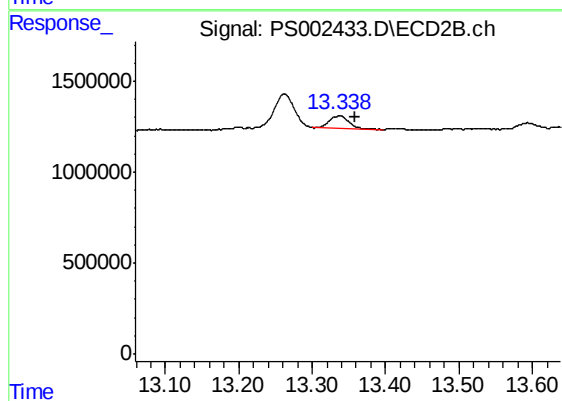

#10 Pentachlorophenol


R.T.: 13.338 min
Delta R.T.: -0.021 min
Response: 1354220
Conc: 0.27 ng/ml

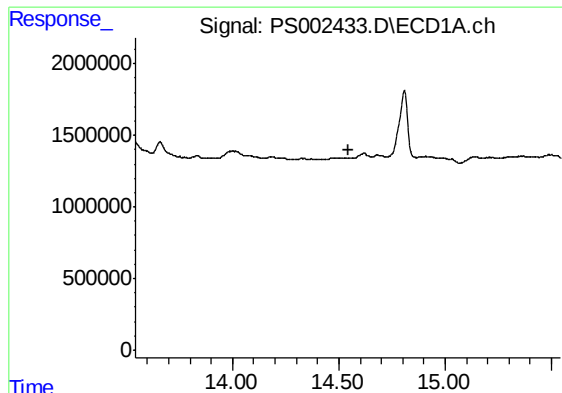

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.543 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6S

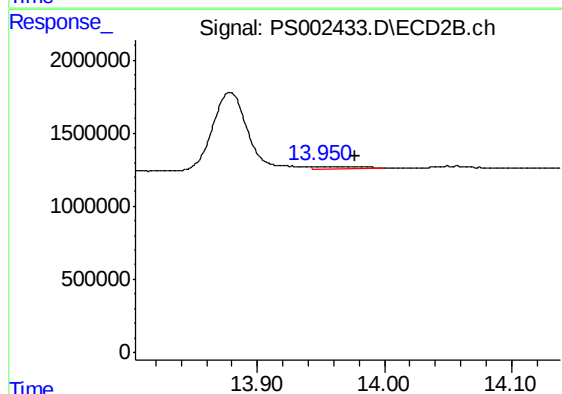


#11 2,4,5-TP (SILVEX)

R.T.: 13.950 min
Delta R.T.: -0.027 min
Response: 363763
Conc: 0.18 ng/ml

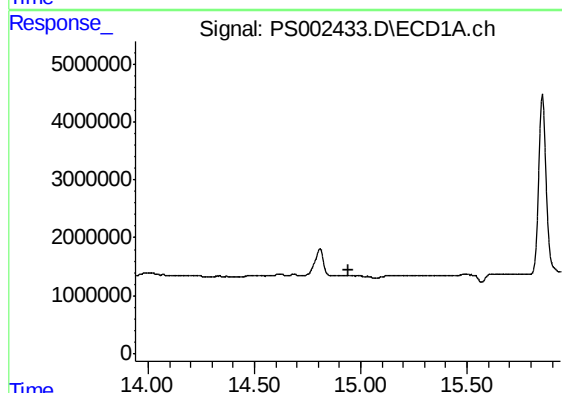


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.940 min
Response: 0
Conc: N.D.

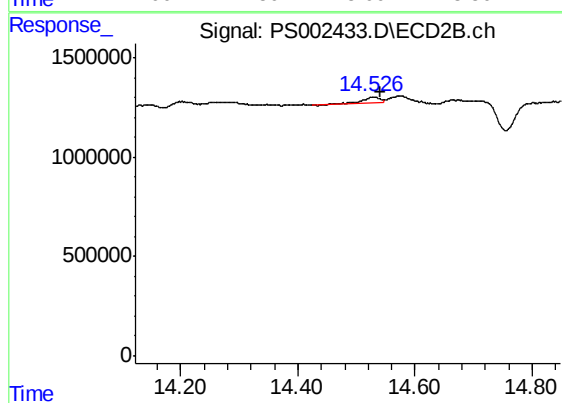

#12 2,4,5-T


R.T.: 14.526 min
Delta R.T.: -0.014 min
Response: 656589
Conc: 0.42 ng/ml

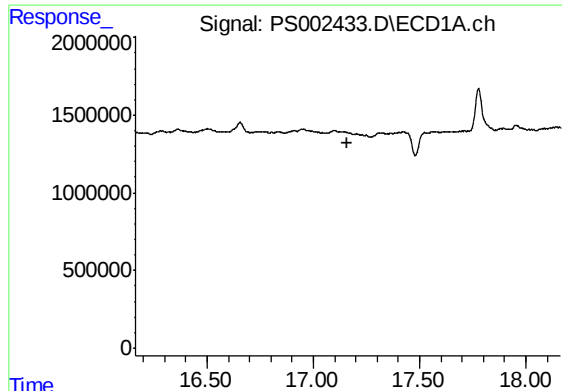

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.163 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6S

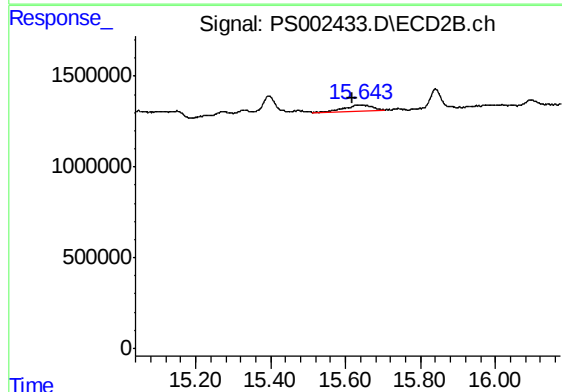


#14 DINOSEB

R.T.: 15.643 min
Delta R.T.: 0.025 min
Response: 1633048
Conc: 1.09 ng/ml

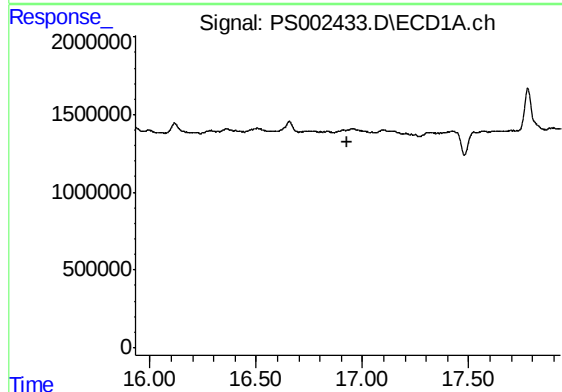


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.931 min
Response: 0
Conc: N.D.

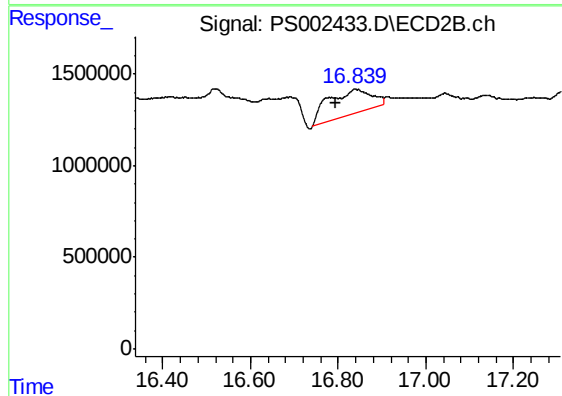

#15 Picloram


R.T.: 16.839 min
Delta R.T.: 0.044 min
Response: 9531193
Conc: 3.58 ng/ml

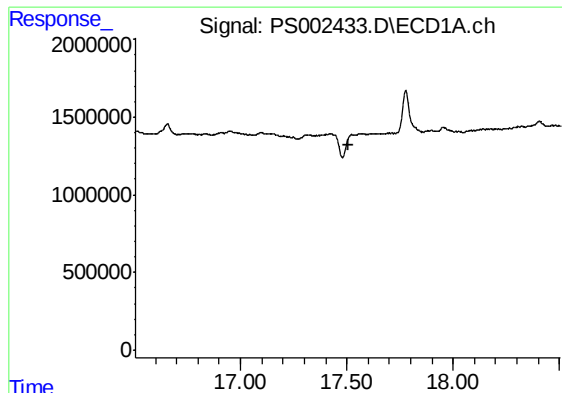

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.506 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-6S

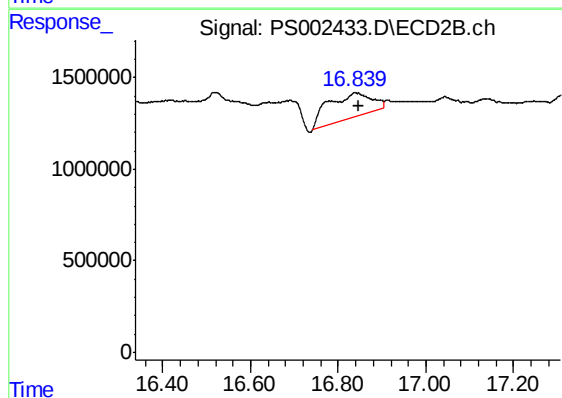

#16 DCPA

R.T.: 16.839 min
Delta R.T.: -0.009 min
Response: 9531193
Conc: 3.97 ng/ml