

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111420\
 Data File : PS013215.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2020 08:27
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 12:57:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 03 03:59:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.471f	0.000	182.7E6	0	148.361	N.D. #
12) T	2,4,5-T	9.426f	0.000	8668810	0	1.638	N.D. #
15) T	Picloram	10.979	11.042f	37016435	58456397	5.629	16.195 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111420\
Data File : PS013215.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2020 08:27
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 12:57:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110220.M
Quant Title : 8080.M
QLast Update : Tue Nov 03 03:59:48 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

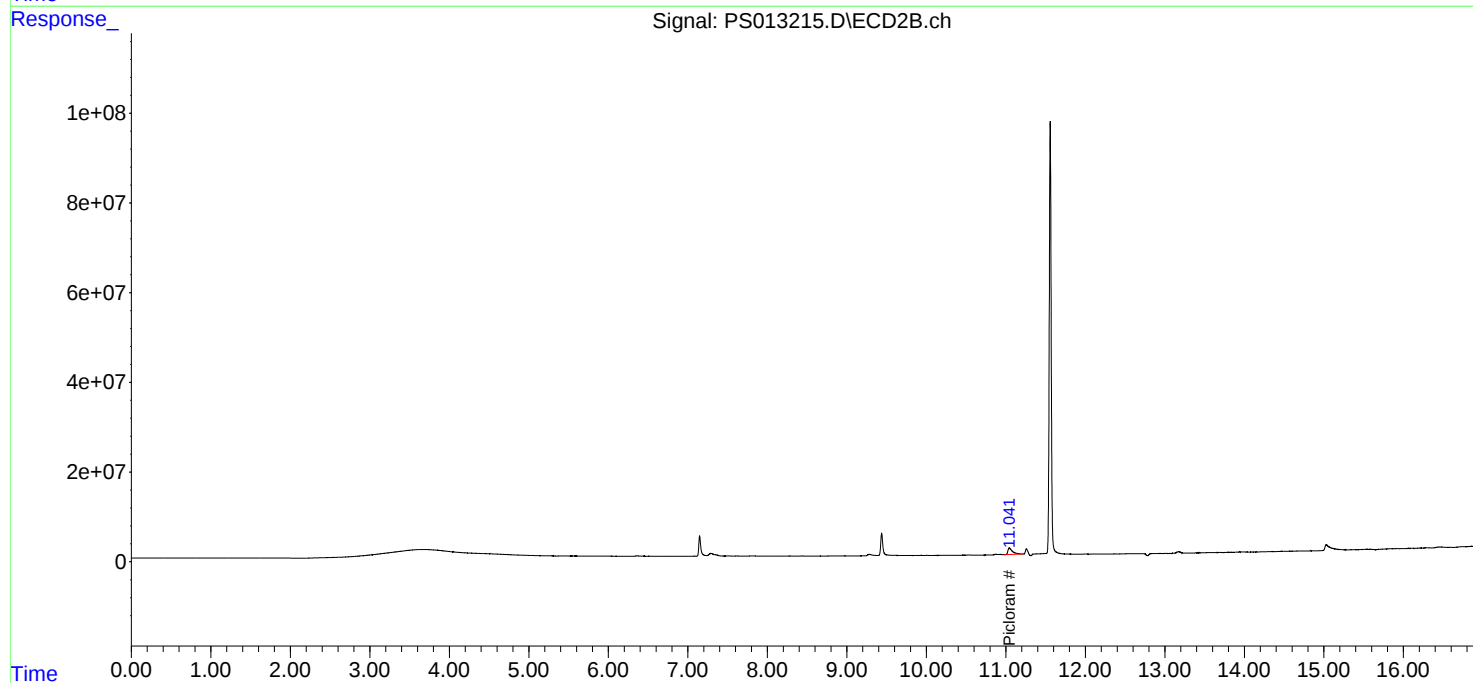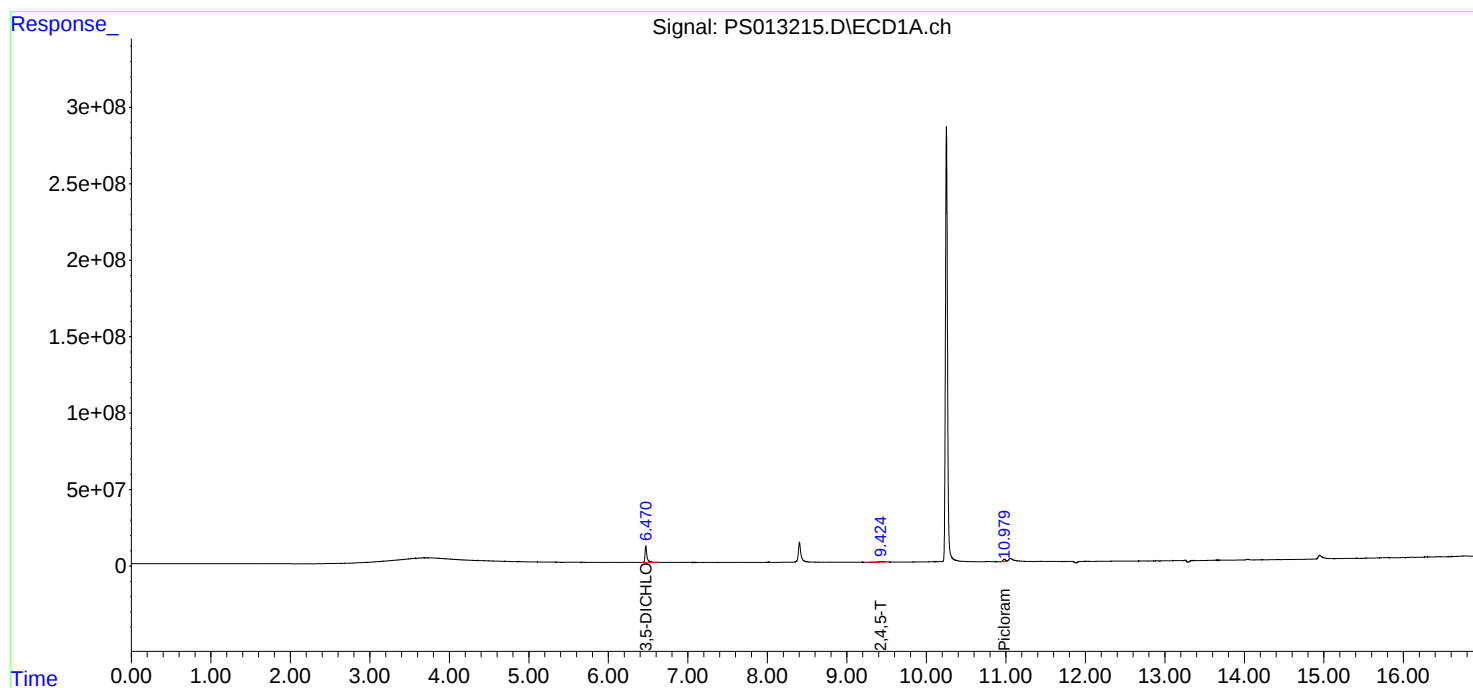


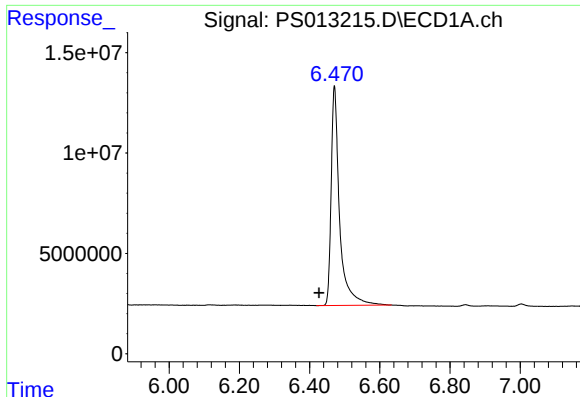

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.471 min
Delta R.T.: 0.044 min
Response: 182717643
Conc: 148.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

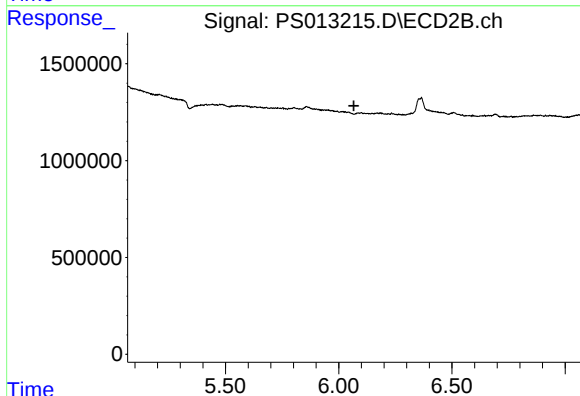


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.067 min
Response: 0
Conc: N.D.

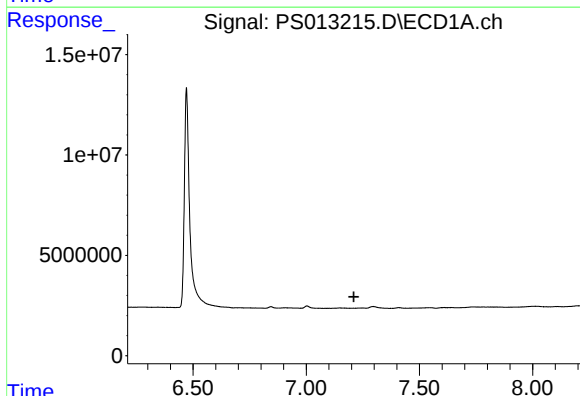


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.211 min
Response: 0
Conc: N.D.

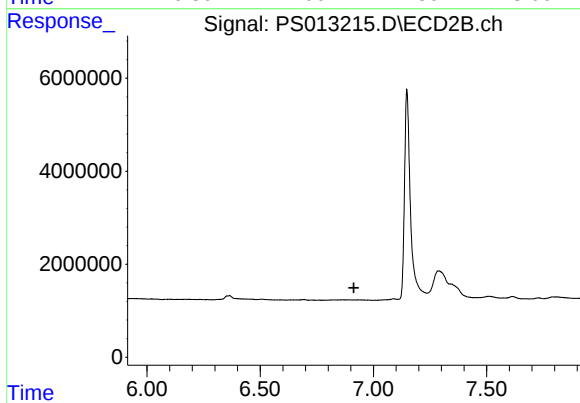

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.914 min
Response: 0
Conc: N.D.

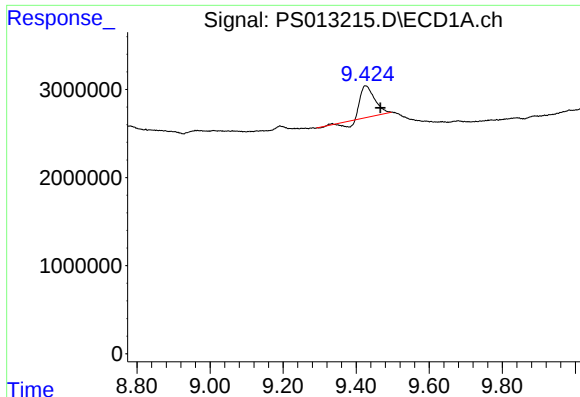

#12 2,4,5-T


R.T.: 9.426 min
Delta R.T.: -0.041 min
Response: 8668810
Conc: 1.64 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

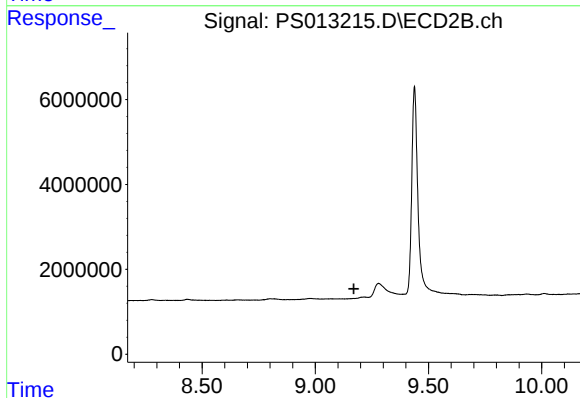


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.170 min
Response: 0
Conc: N.D.

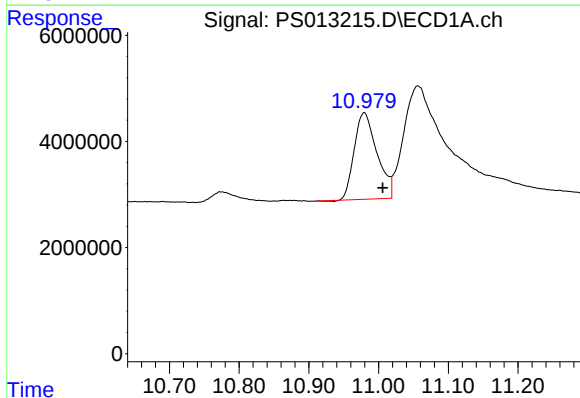

#15 Picloram

R.T.: 10.979 min
Delta R.T.: -0.027 min
Response: 37016435
Conc: 5.63 ng/ml

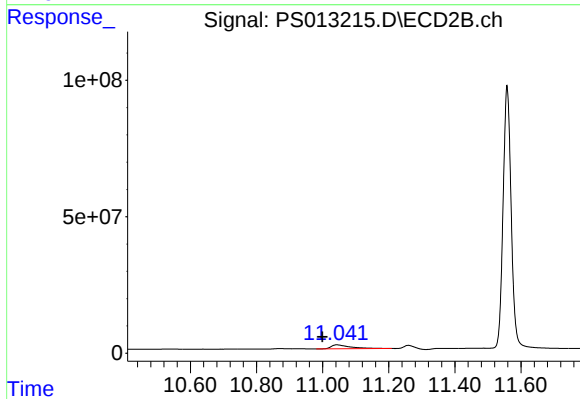

#15 Picloram

R.T.: 11.042 min
Delta R.T.: 0.043 min
Response: 58456397
Conc: 16.20 ng/ml