

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111422\
 Data File : PS021150.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2022 09:41
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 13:43:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
 Quant Title : 8080.M
 QLast Update : Mon Oct 31 10:07:57 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	6.353f	0.000	756579	0	<MDL	N.D.	#
Target Compounds								
1) T	Dalapon	2.497	0.000	600230	0	<MDL	N.D.	#
3) T	4-Nitroph...	6.241	0.000	2149282	0	1.429	N.D.	#
6) T	MCP	6.682	0.000	1497070	0	<MDL	N.D.	#
7) T	MCPA	6.776f	0.000	2207903	0	<MDL	N.D.	#
8) T	DICHLORPROP	7.107f	0.000	680090	0	<MDL	N.D.	#
10) T	Pentachlo...	7.574	0.000	693221	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	8.124	0.000	1418237	0	<MDL	N.D.	#
12) T	2,4,5-T	8.387	9.168f	831011	1244127	<MDL	<MDL	#
13) T	2,4-DB	8.865	0.000	452696	0	<MDL	N.D.	#
15) T	Picloram	9.813f	10.934	14753266	5674774	<MDL	<MDL	#
16) T	DCPA	10.207	10.863	256199	1562338	<MDL	<MDL	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111422\
Data File : PS021150.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2022 09:41
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 13:43:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS102822.M
Quant Title : 8080.M
QLast Update : Mon Oct 31 10:07:57 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

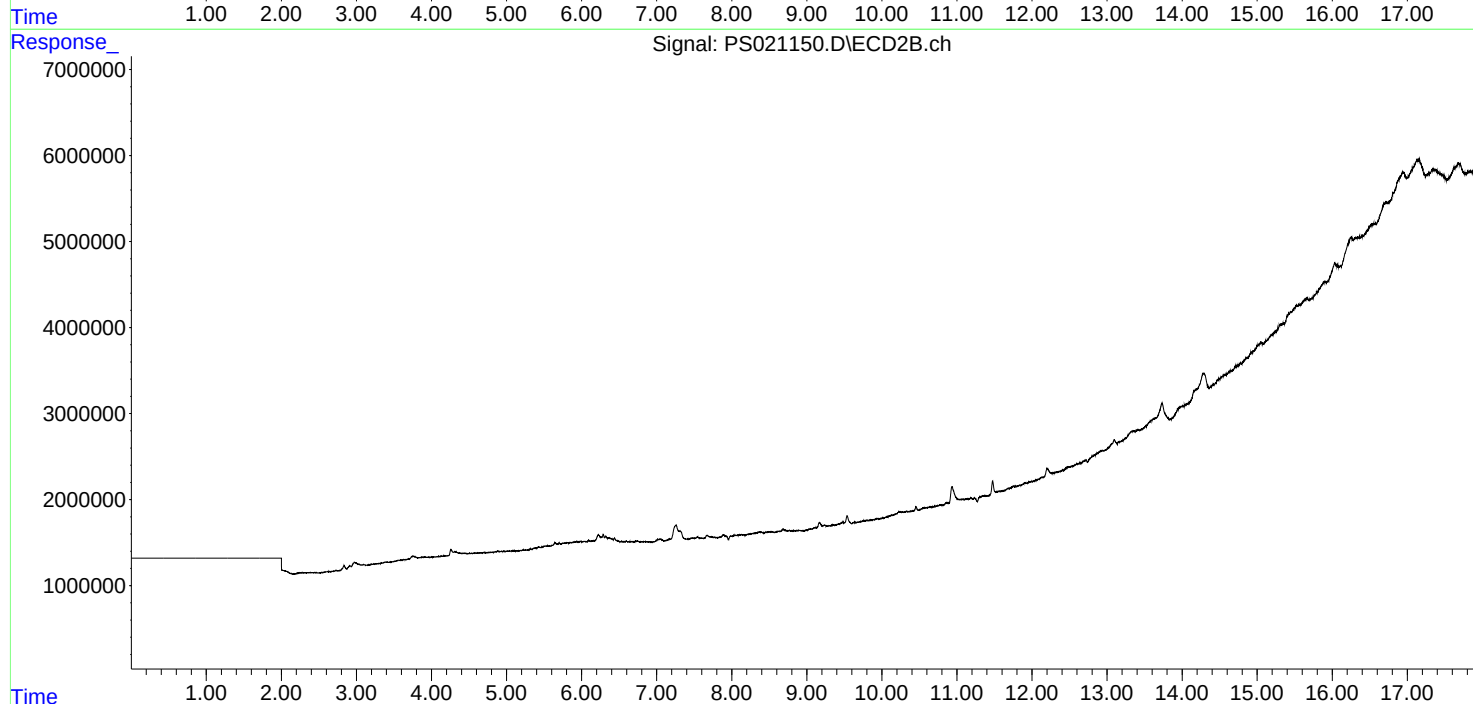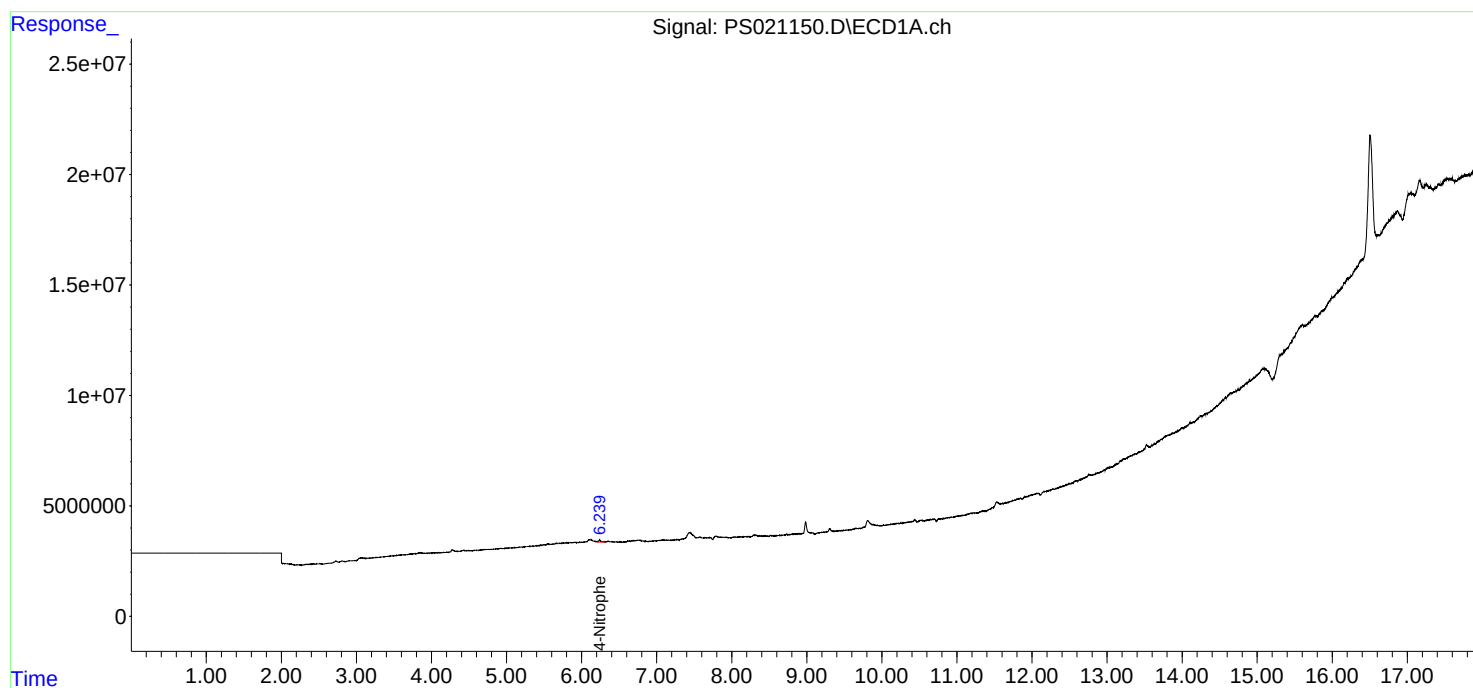


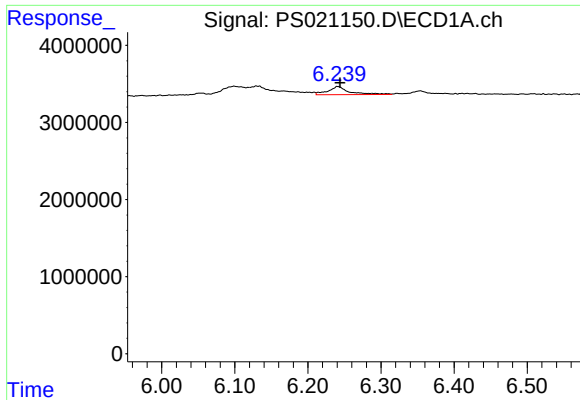

#3 4-Nitrophenol


R.T.: 6.241 min
Delta R.T.: -0.003 min
Response: 2149282
Conc: 1.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

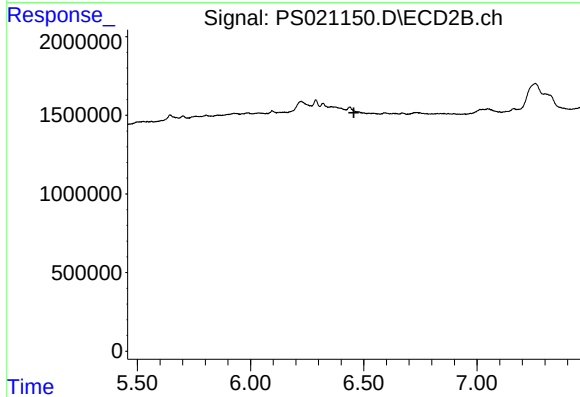


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

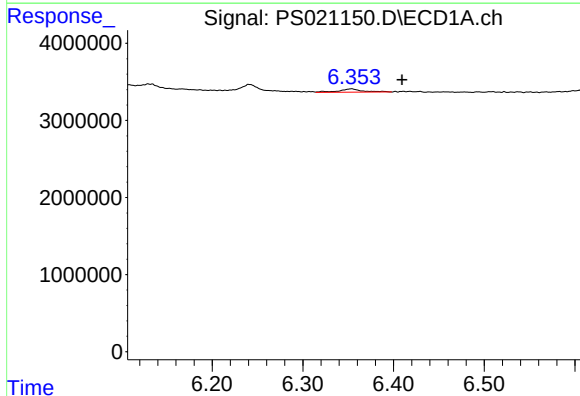

#4 2,4-DCAA

R.T.: 6.353 min
Delta R.T.: -0.056 min
Response: 756579
Conc: N.D.

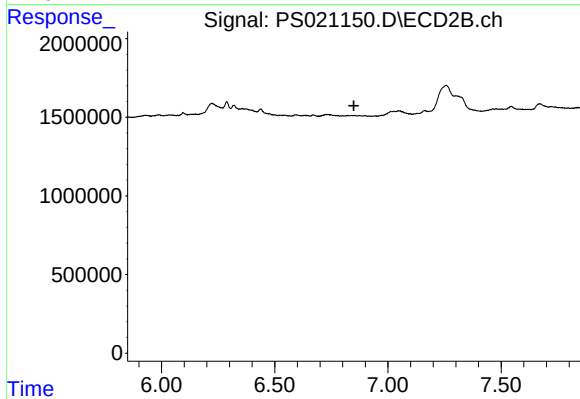

#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.850 min
Response: 0
Conc: N.D.