

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111423\
 Data File : PS024830.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2023 19:13
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 20:54:49 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 03 15:07:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.356	6.775	1030.0E6	339.2E6	504.542	502.757
Target Compounds							
1) T	Dalapon	2.513	2.572	7021866	3561213	2.915	3.380
3) T	4-Nitroph...	0.000	6.372	0	789674	N.D.	1.798
7) T	MCPA	0.000	7.235	0	8070180	N.D.	2.618
8) T	DICHLORPROP	0.000	7.564	0	2824468	N.D.	3.866
9) T	2,4-D	0.000	7.780 ^f	0	818198	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.613	0	449357	N.D.	<MDL
12) T	2,4,5-T	0.000	8.987	0	548653	N.D.	<MDL
15) T	Picloram	9.684	10.770	44080568	12558945	2.478	2.067
16) T	DCPA	0.000	10.770	0	12558945	N.D.	2.499



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111423\
Data File : PS024830.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2023 19:13
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 20:54:49 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
Quant Title : 8080.M
QLast Update : Fri Nov 03 15:07:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

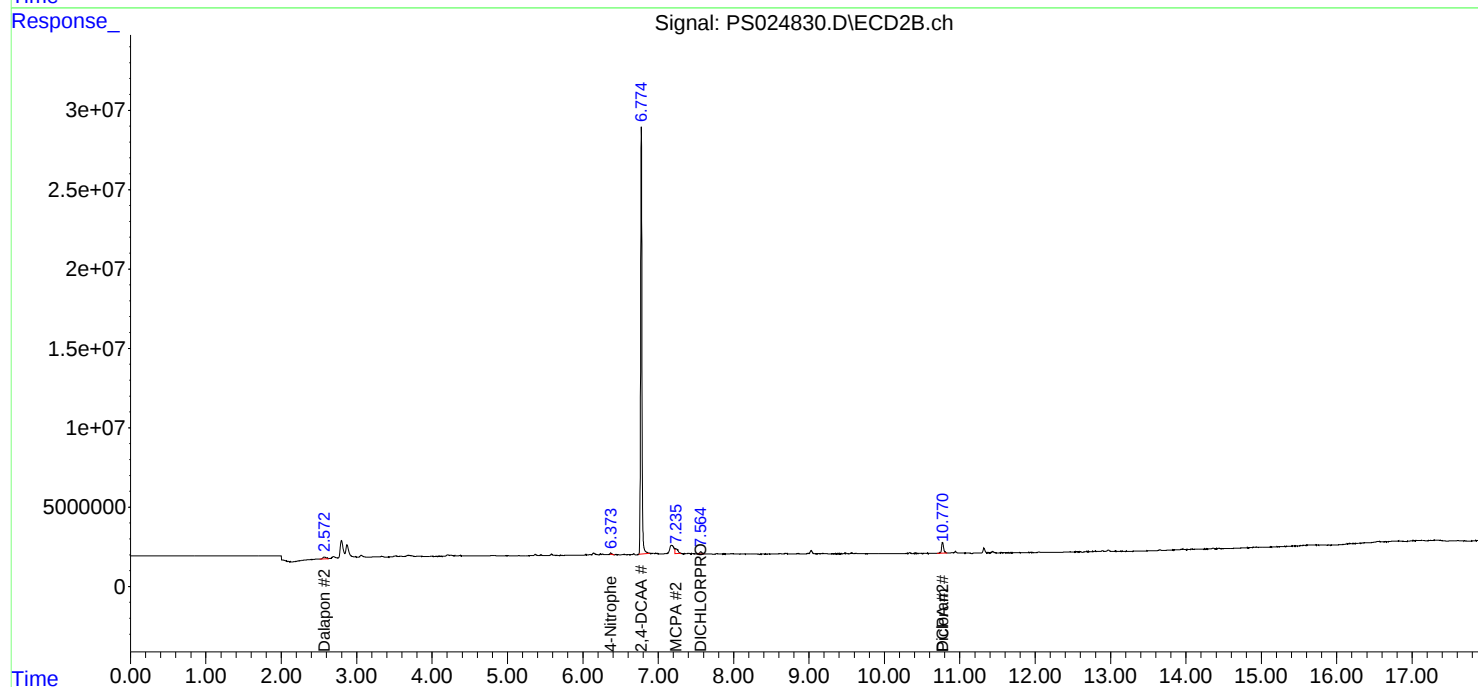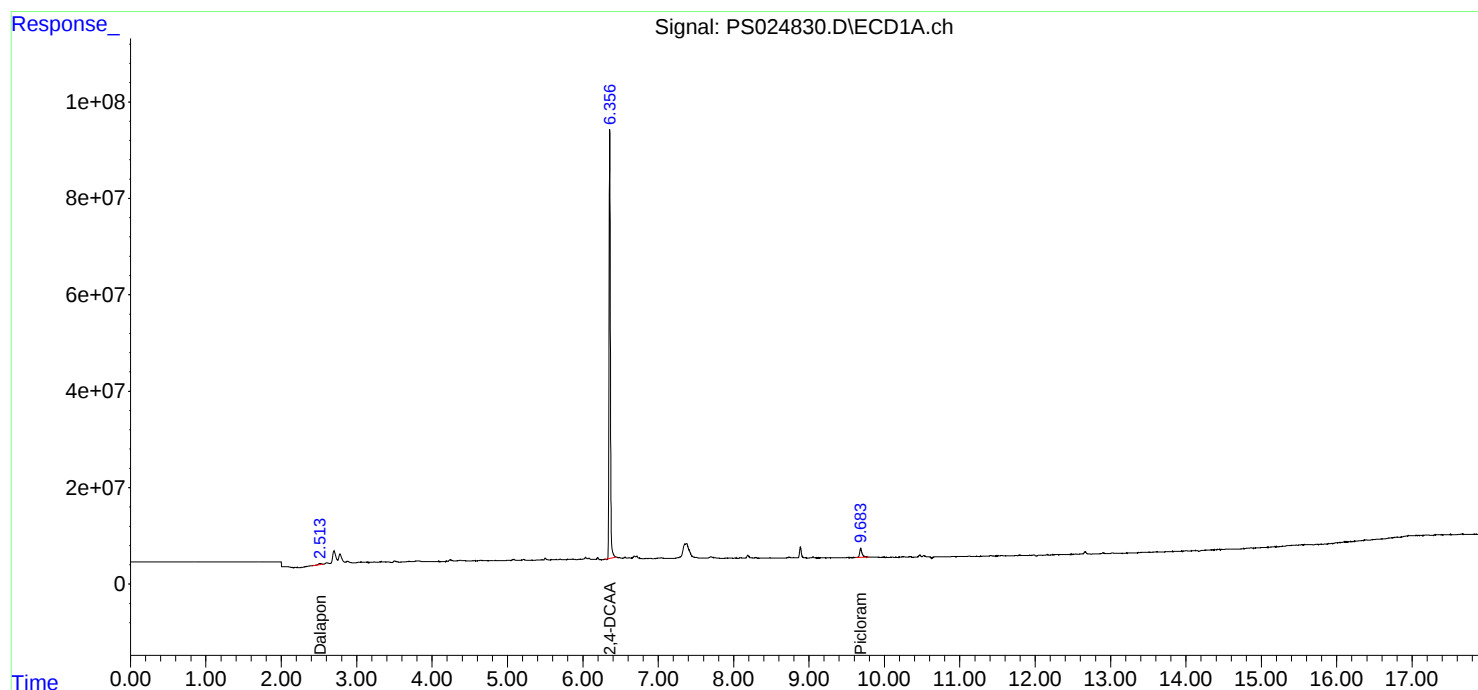


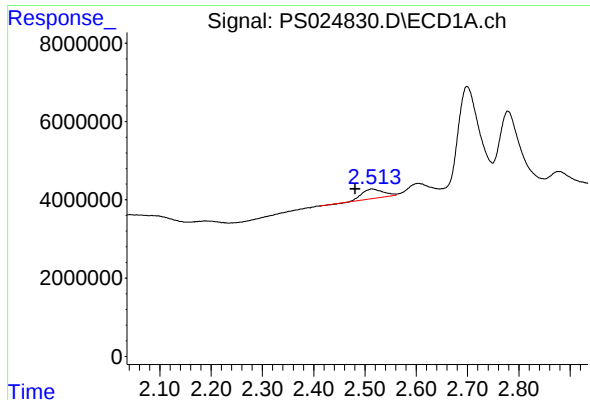

#1 Dalapon


R.T.: 2.513 min
Delta R.T.: 0.032 min
Response: 7021866
Conc: 2.91 ng/ml

Instrument :
ECD_S
ClientSampleId :

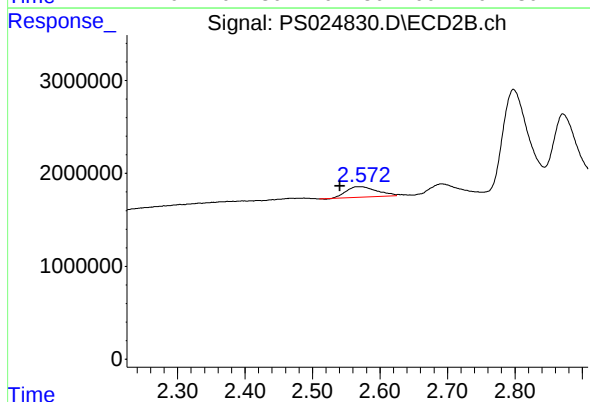


#1 Dalapon

R.T.: 2.572 min
Delta R.T.: 0.032 min
Response: 3561213
Conc: 3.38 ng/ml

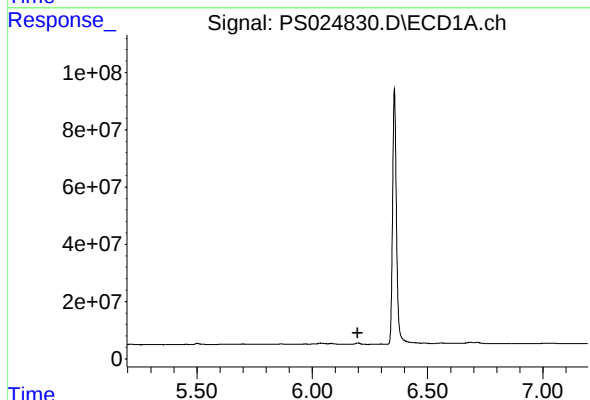


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.196 min
Response: 0
Conc: N.D.

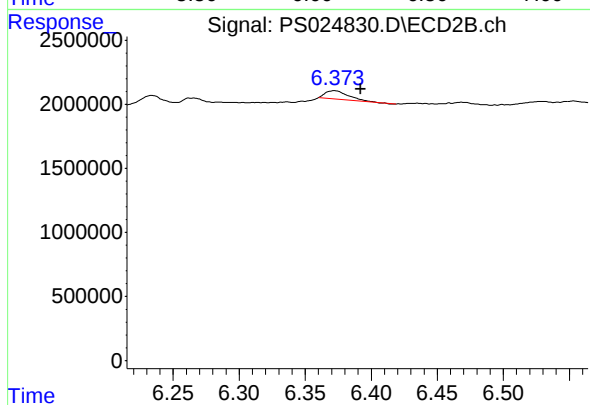

#3 4-Nitrophenol


R.T.: 6.372 min
Delta R.T.: -0.020 min
Response: 789674
Conc: 1.80 ng/ml

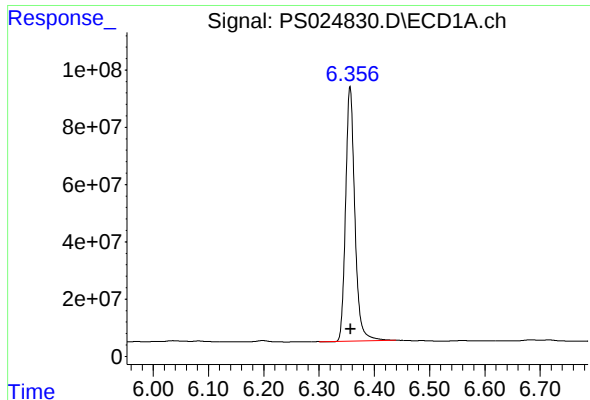

#4 2,4-DCAA


R.T.: 6.356 min
Delta R.T.: -0.001 min
Response: 1030023147
Conc: 504.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

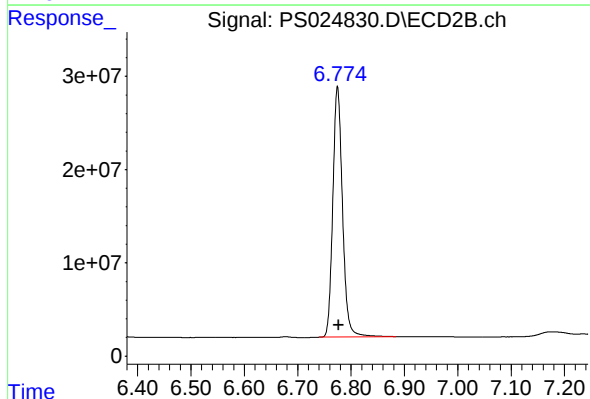


#4 2,4-DCAA

R.T.: 6.775 min
Delta R.T.: -0.002 min
Response: 339159332
Conc: 502.76 ng/ml

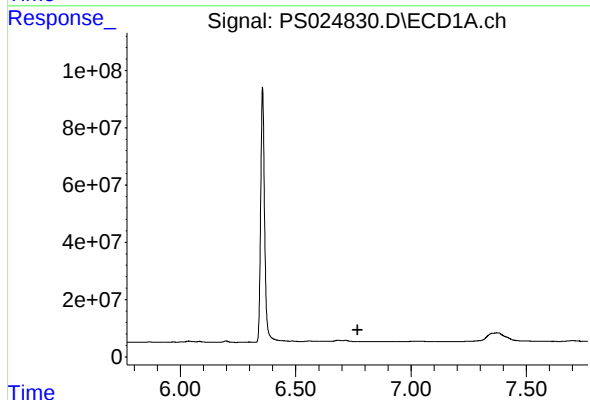


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.768 min
Response: 0
Conc: N.D.

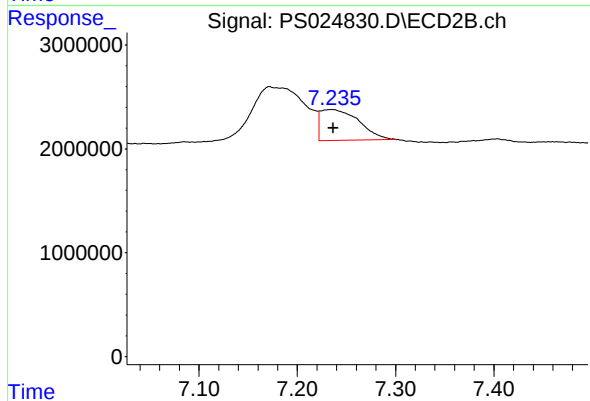

#7 MCPA


R.T.: 7.235 min
Delta R.T.: -0.001 min
Response: 8070180
Conc: 2.62 ug/ml

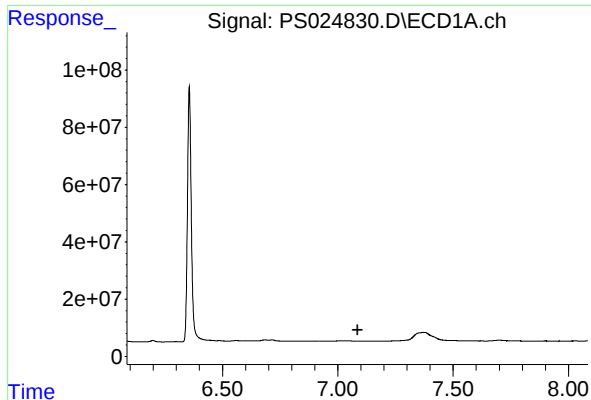

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.085 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

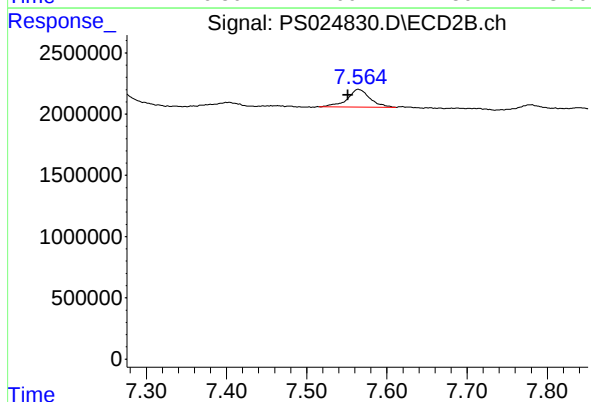


#8 DICHLORPROP

R.T.: 7.564 min
Delta R.T.: 0.013 min
Response: 2824468
Conc: 3.87 ng/ml

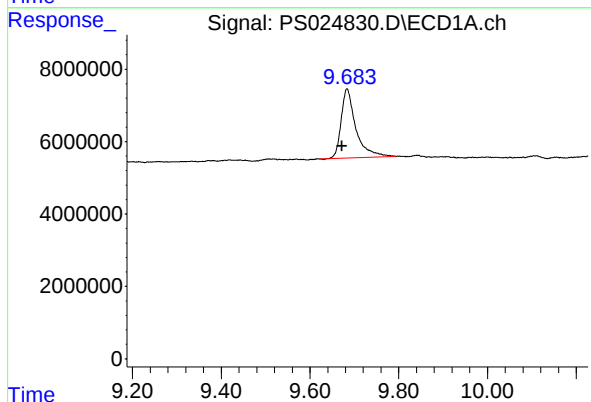


#15 Picloram

R.T.: 9.684 min
Delta R.T.: 0.011 min
Response: 44080568
Conc: 2.48 ng/ml

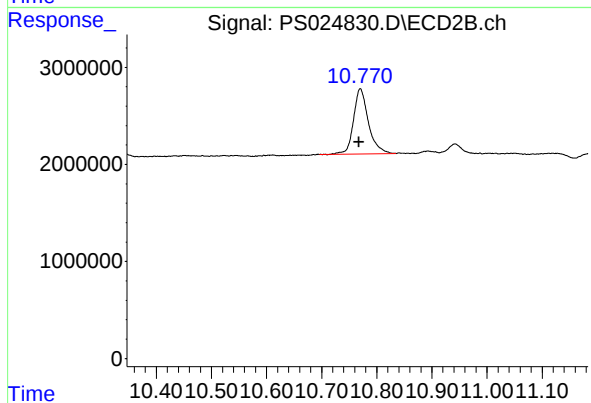

#15 Picloram


R.T.: 10.770 min
Delta R.T.: 0.002 min
Response: 12558945
Conc: 2.07 ng/ml

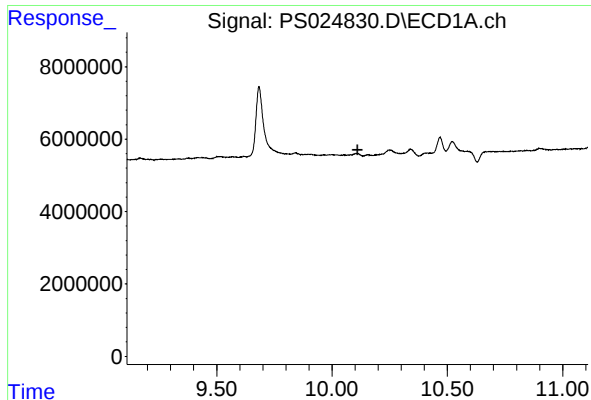

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.111 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

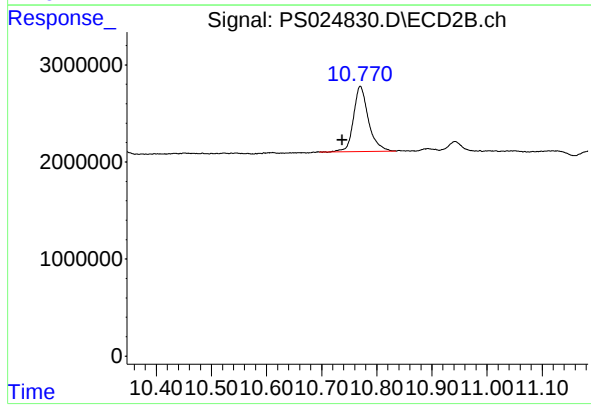

#16 DCPA

R.T.: 10.770 min
Delta R.T.: 0.032 min
Response: 12558945
Conc: 2.50 ng/ml