

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111424\
 Data File : PS028530.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2024 09:21
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 00:15:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.239	7.738	1491.5E6	752.1E6	583.545	582.019
Target Compounds							
3) T	4-Nitroph...	7.029	0.000	10322797	0	6.078	N.D. #
5) T	DICAMBA	0.000	7.934	0	3123783	N.D.	<MDL
6) T	MCPD	7.569f	0.000	442204	0	<MDL	N.D. #
7) T	MCPA	7.799f	8.262f	453552	4501231	<MDL	<MDL #
8) T	DICHLORPROP	8.162	8.706f	1190542	8867135	<MDL	6.071 #
9) T	2,4-D	8.372	0.000	1703782	0	<MDL	N.D. #
10) T	Pentachlo...	8.707f	0.000	3613490	0	<MDL	N.D. #
12) T	2,4,5-T	9.543	10.312	5354028	4552600	<MDL	<MDL #
13) T	2,4-DB	10.105	0.000	1501342	0	<MDL	N.D. #
14) T	DINOSEB	11.332	0.000	1415604	0	<MDL	N.D. #
15) T	Picloram	11.140	12.358	96395755	39444347	3.423	3.485
16) T	DCPA	11.621	12.358f	5062732	39444347	<MDL	4.067 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111424\
Data File : PS028530.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2024 09:21
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 00:15:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

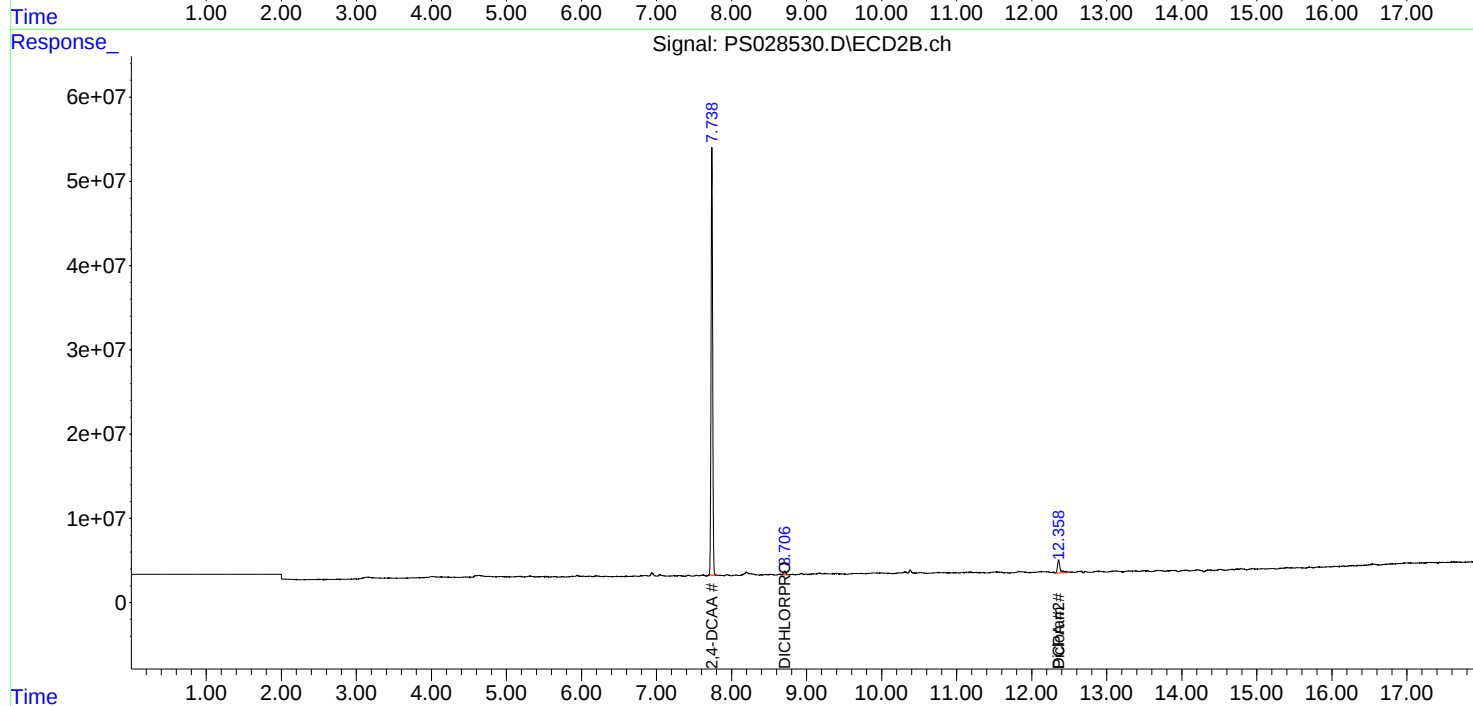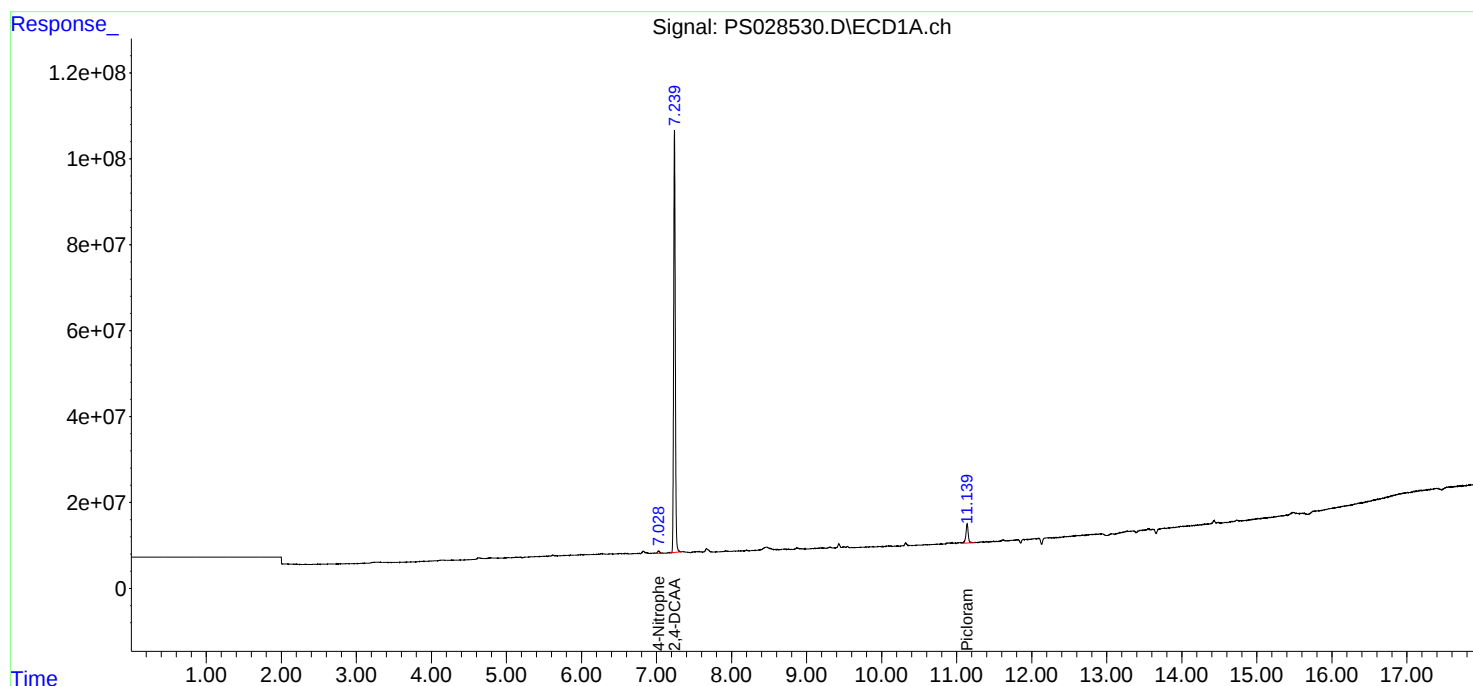


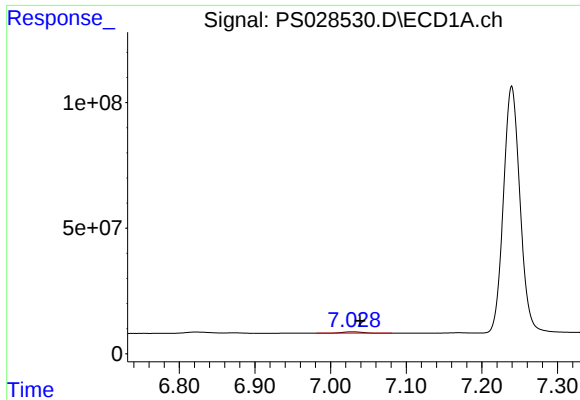

#3 4-Nitrophenol


R.T.: 7.029 min
Delta R.T.: -0.010 min
Response: 10322797
Conc: 6.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

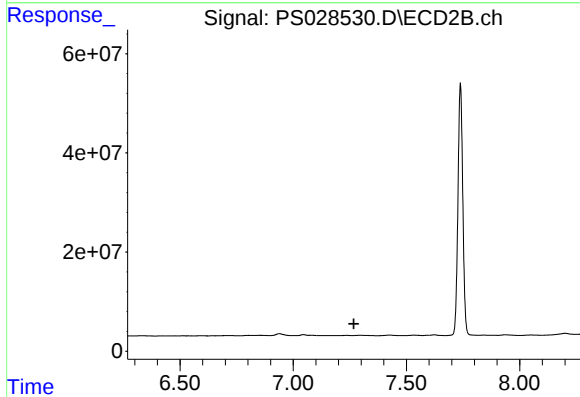


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.268 min
Response: 0
Conc: N.D.

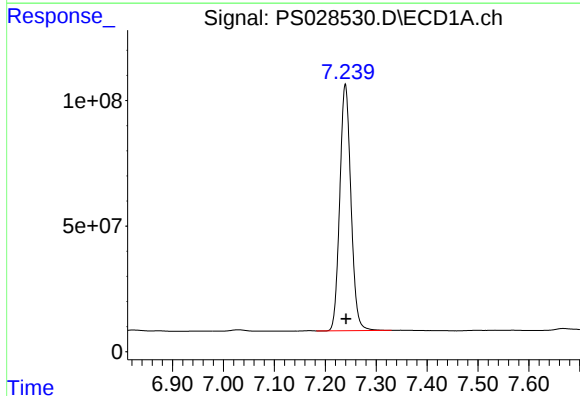


#4 2,4-DCAA

R.T.: 7.239 min
Delta R.T.: -0.001 min
Response: 1491471609
Conc: 583.54 ng/ml

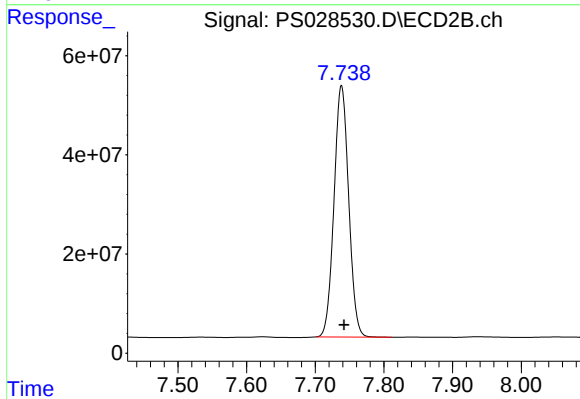

#4 2,4-DCAA


R.T.: 7.738 min
Delta R.T.: -0.004 min
Response: 752146136
Conc: 582.02 ng/ml

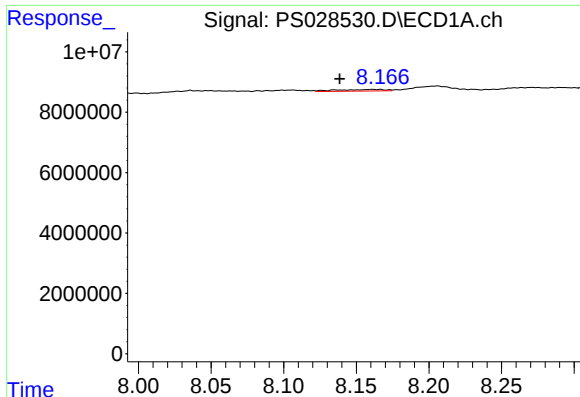

#8 DICHLORPROP


R.T.: 8.162 min
Delta R.T.: 0.024 min
Response: 1190542
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

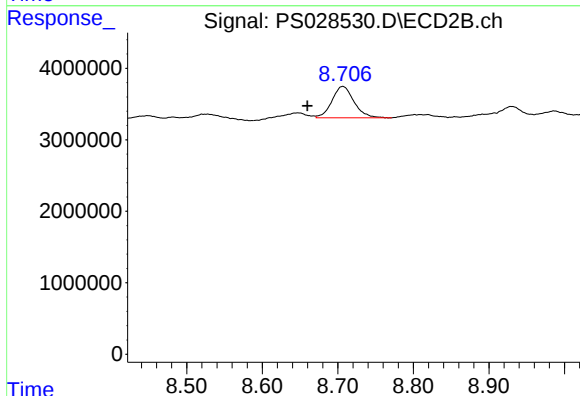


#8 DICHLORPROP

R.T.: 8.706 min
Delta R.T.: 0.047 min
Response: 8867135
Conc: 6.07 ng/ml

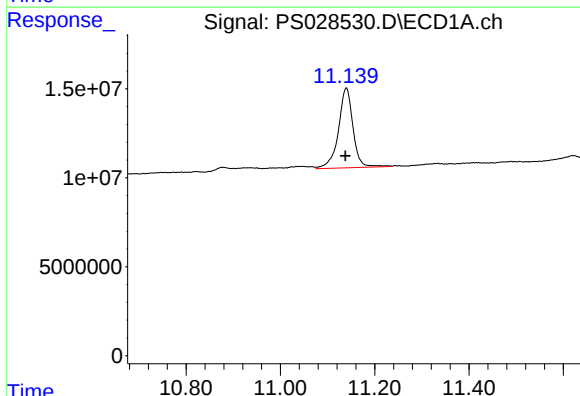


#15 Picloram

R.T.: 11.140 min
Delta R.T.: 0.002 min
Response: 96395755
Conc: 3.42 ng/ml

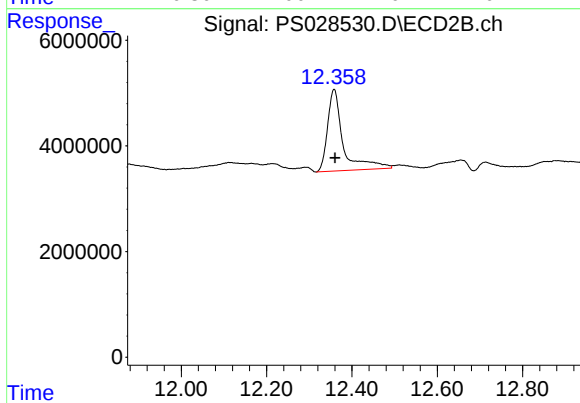

#15 Picloram


R.T.: 12.358 min
Delta R.T.: -0.002 min
Response: 39444347
Conc: 3.48 ng/ml

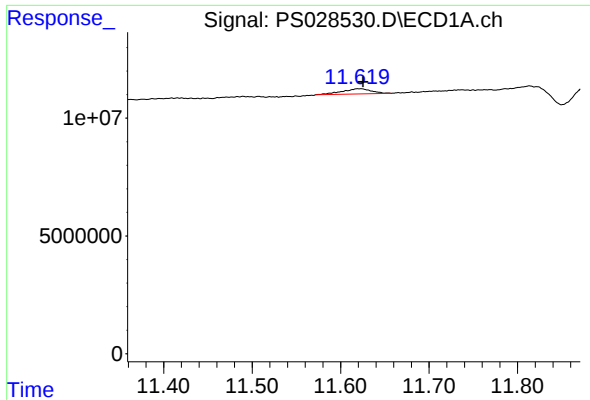

#16 DCPA

R.T.: 11.621 min
Delta R.T.: -0.004 min
Response: 5062732
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

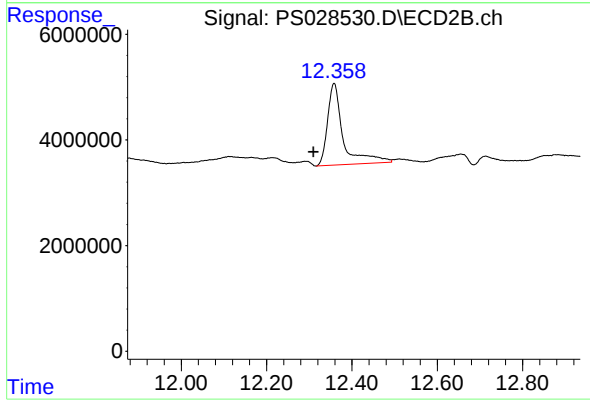

#16 DCPA

R.T.: 12.358 min
Delta R.T.: 0.049 min
Response: 39444347
Conc: 4.07 ng/ml