

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111424\
 Data File : PS028533.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2024 11:38
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 00:17:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	7.739	1502.5E6	754.4E6	587.866	583.768
Target Compounds							
1) T	Dalapon	2.643	0.000	915760	0	<MDL	N.D. #
3) T	4-Nitroph...	7.033	0.000	7845492	0	4.619	N.D. #
5) T	DICAMBA	0.000	7.932	0	3333758	N.D.	<MDL
8) T	DICHLORPROP	8.172f	8.706f	157715	6696049	<MDL	4.585 #
10) T	Pentachlo...	8.677	0.000	455281	0	<MDL	N.D. #
12) T	2,4,5-T	9.548	10.313	3317310	3756680	<MDL	<MDL #
14) T	DINOSEB	11.342	0.000	2384136	0	<MDL	N.D. #
15) T	Picloram	11.144	12.357	33625791	13736683	1.194	1.214
16) T	DCPA	11.616	12.357f	4876563	13736683	<MDL	1.416 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111424\
Data File : PS028533.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2024 11:38
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 00:17:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

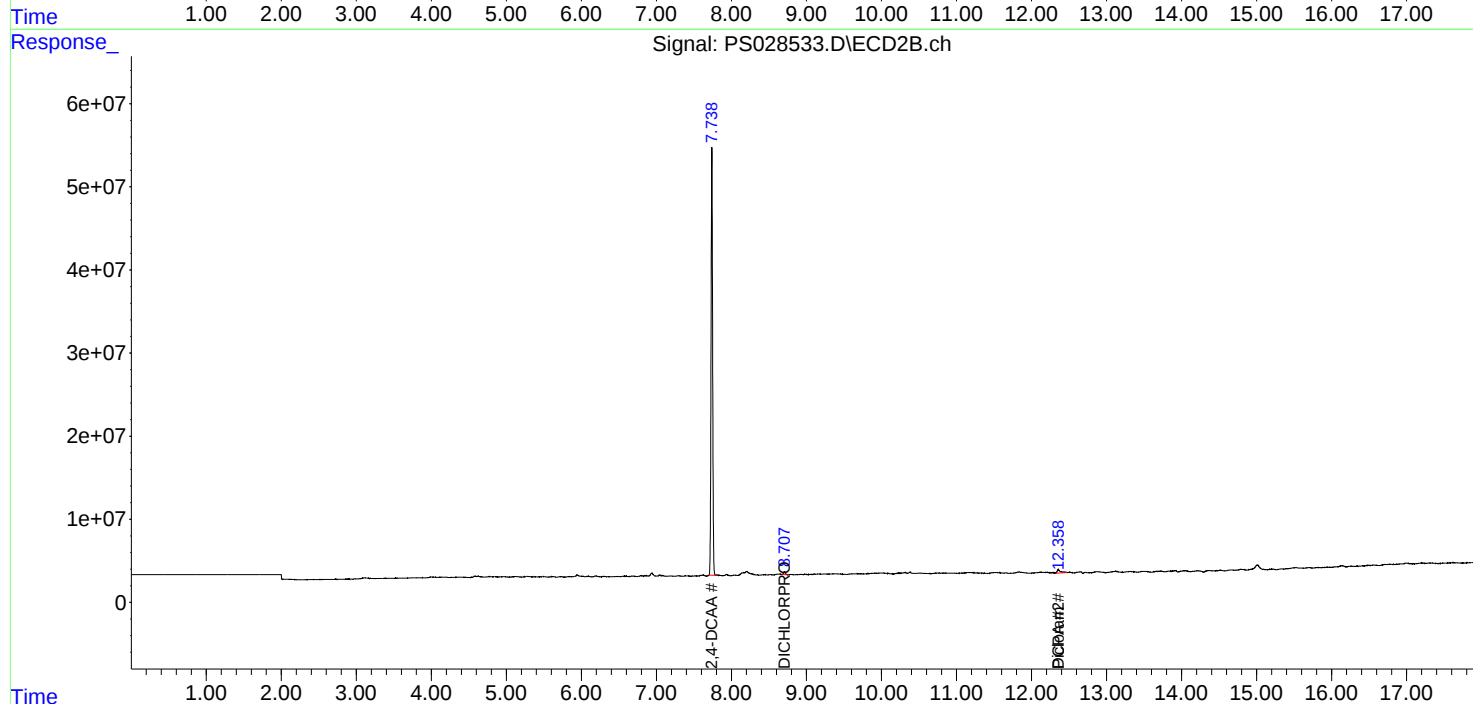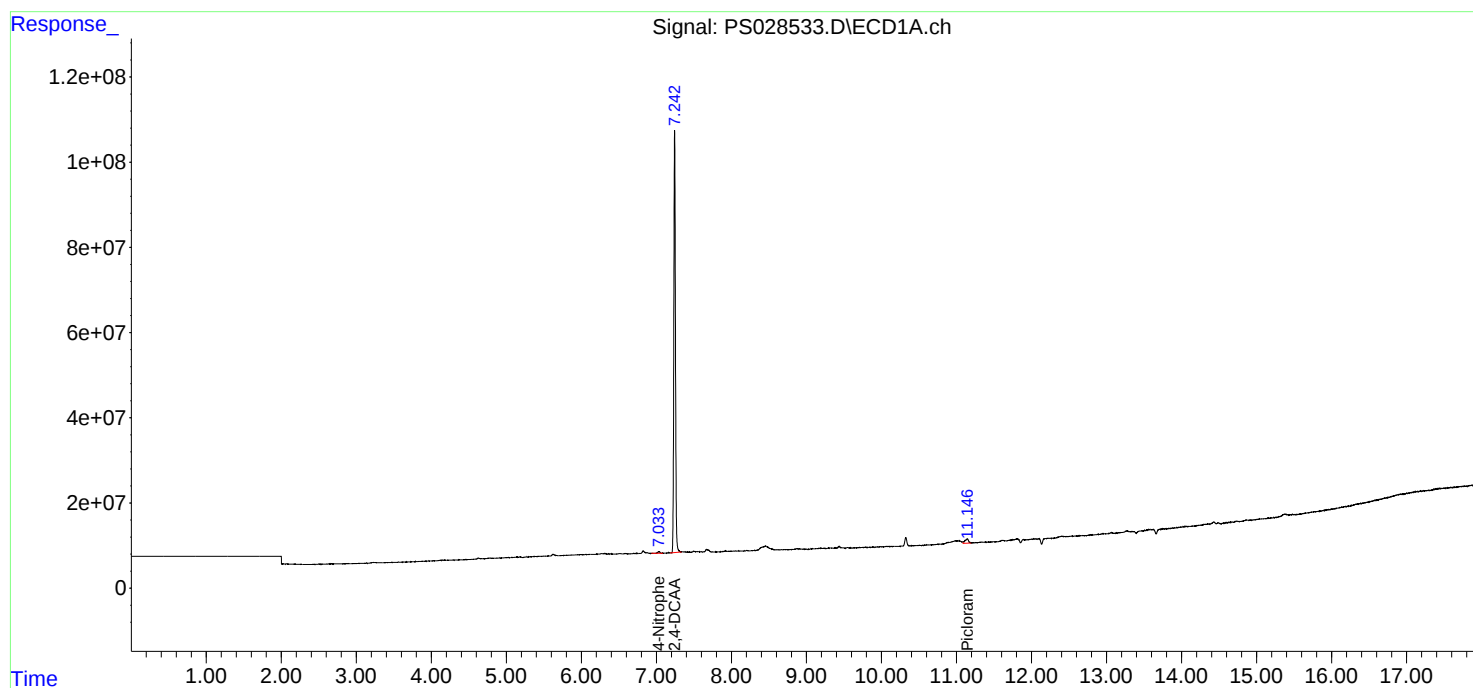


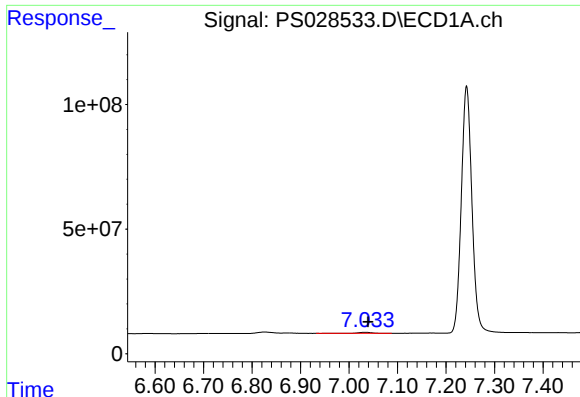

#3 4-Nitrophenol


R.T.: 7.033 min
Delta R.T.: -0.006 min
Response: 7845492
Conc: 4.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

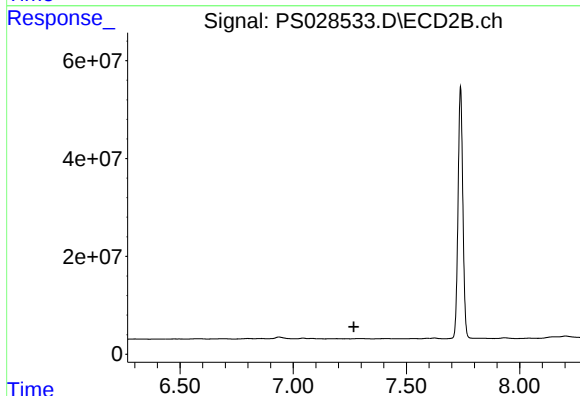


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.268 min
Response: 0
Conc: N.D.

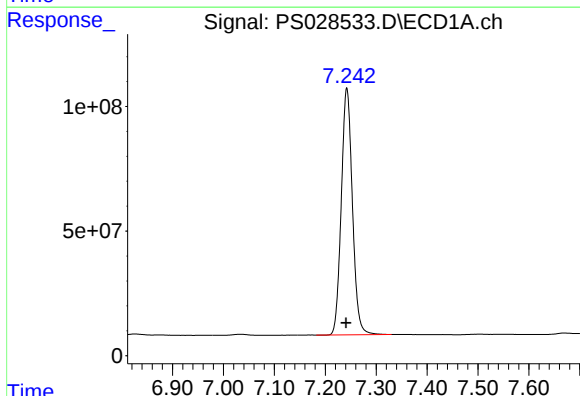


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.002 min
Response: 1502516485
Conc: 587.87 ng/ml

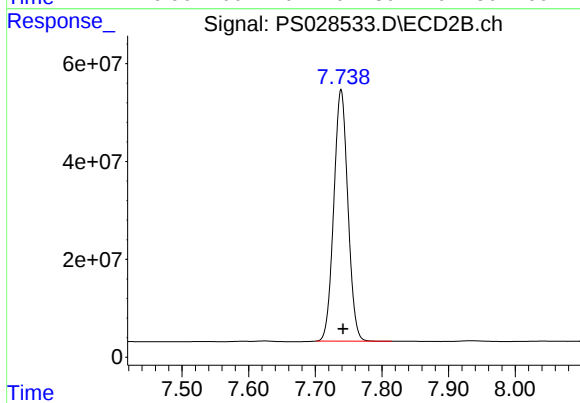

#4 2,4-DCAA


R.T.: 7.739 min
Delta R.T.: -0.003 min
Response: 754405643
Conc: 583.77 ng/ml

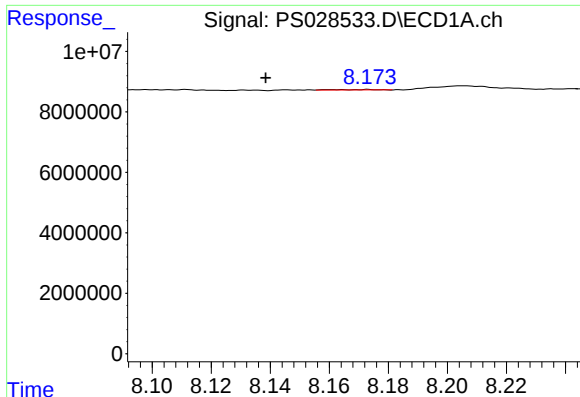

#8 DICHLORPROP


R.T.: 8.172 min
Delta R.T.: 0.034 min
Response: 157715
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

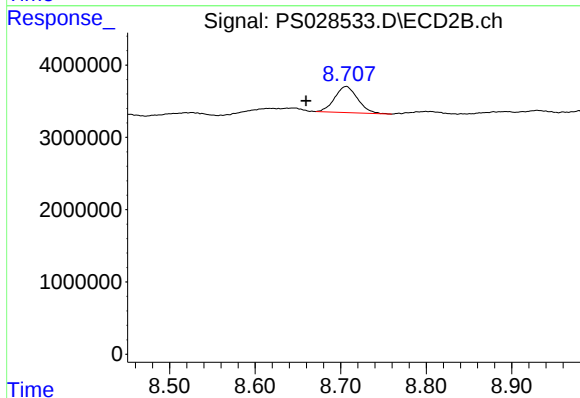


#8 DICHLORPROP

R.T.: 8.706 min
Delta R.T.: 0.047 min
Response: 6696049
Conc: 4.58 ng/ml

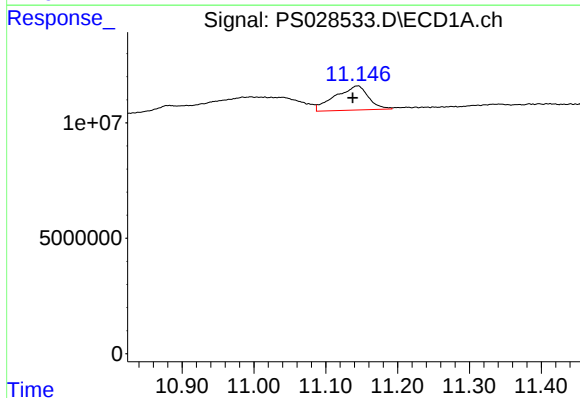


#15 Picloram

R.T.: 11.144 min
Delta R.T.: 0.006 min
Response: 33625791
Conc: 1.19 ng/ml

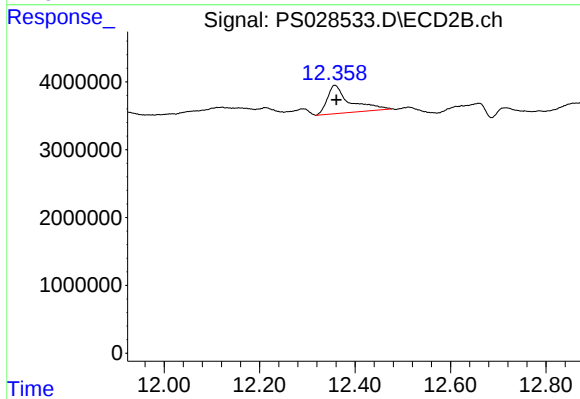

#15 Picloram


R.T.: 12.357 min
Delta R.T.: -0.004 min
Response: 13736683
Conc: 1.21 ng/ml

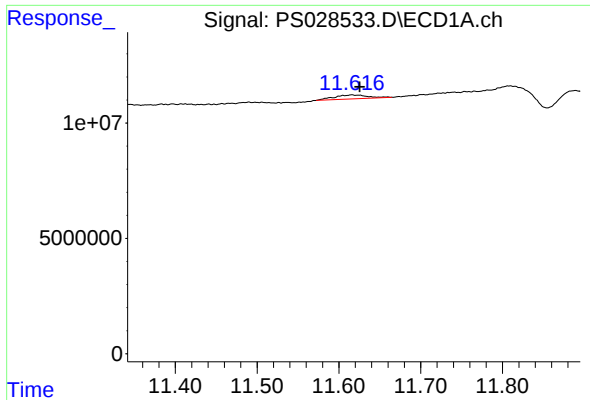

#16 DCPA

R.T.: 11.616 min
Delta R.T.: -0.009 min
Response: 4876563
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

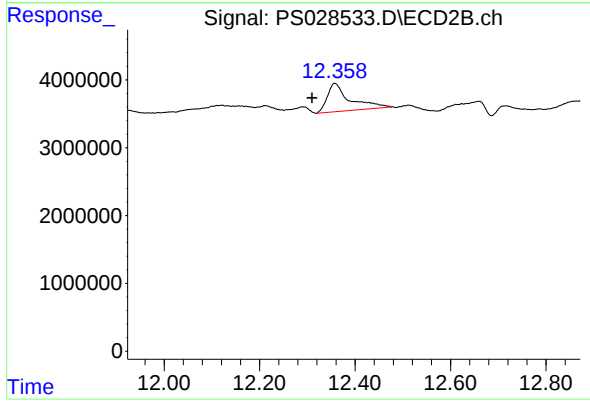

#16 DCPA

R.T.: 12.357 min
Delta R.T.: 0.048 min
Response: 13736683
Conc: 1.42 ng/ml