

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111424\
 Data File : PS028538.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2024 17:49
 Operator : AR\AJ
 Sample : P4821-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 BP-F-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 00:22:56 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.239	7.739	960.1E6	434.0E6	375.644	335.800
Target Compounds							
1) T	Dalapon	0.000	2.700	0	210.2E6	N.D.	86.848
2) T	3,5-DICHL...	6.398	6.700	2138633	3077289	<MDL	1.592 #
3) T	4-Nitroph...	7.005f	7.294f	22489892	5381219	13.241	6.233 #
5) T	DICAMBA	7.446	7.932	14811446	9188065	1.354	1.611
6) T	MCPD	7.662f	8.032	211.9E6	6409289	30.127	1.490 #
7) T	MCPA	7.804f	8.278	6672391	11171478	<MDL	1.804 #
8) T	DICHLORPROP	8.148	8.628f	6585853	11420214	2.231	7.819 #
9) T	2,4-D	8.319f	0.000	5958042	0	1.864	N.D. #
10) T	Pentachlo...	8.665	9.514	5090786	7884179	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	9.854f	0	49936205	N.D.	5.918
12) T	2,4,5-T	9.546	10.308	633524	64382092	<MDL	7.681 #
13) T	2,4-DB	10.101	0.000	19442292	0	7.133	N.D. #
14) T	DINOSEB	11.318	11.264	24946183	22037411	1.750	3.986 #
15) T	Picloram	11.139	12.357	72569028	10957737	2.577	<MDL #
16) T	DCPA	0.000	12.312	0	301709	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111424\
Data File : PS028538.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2024 17:49
Operator : AR\AJ
Sample : P4821-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
BP-F-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 00:22:56 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

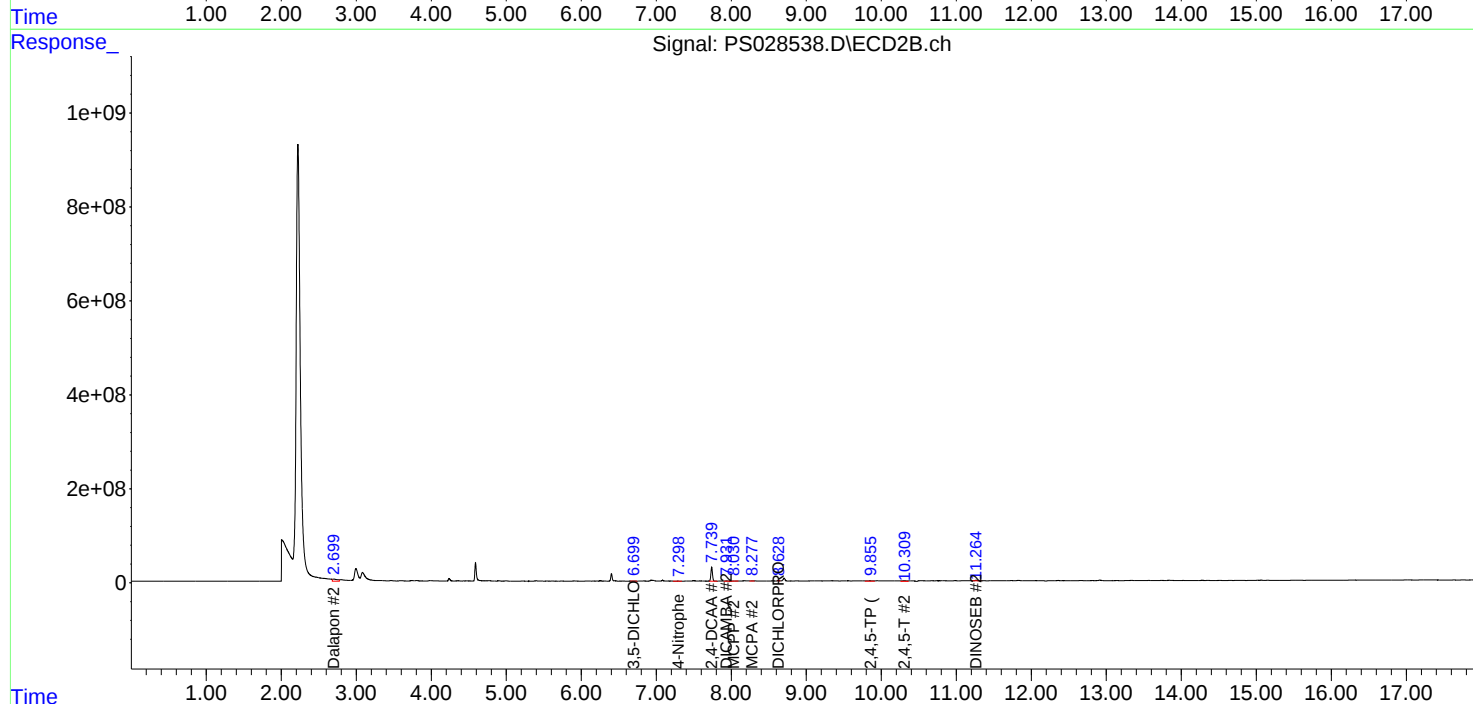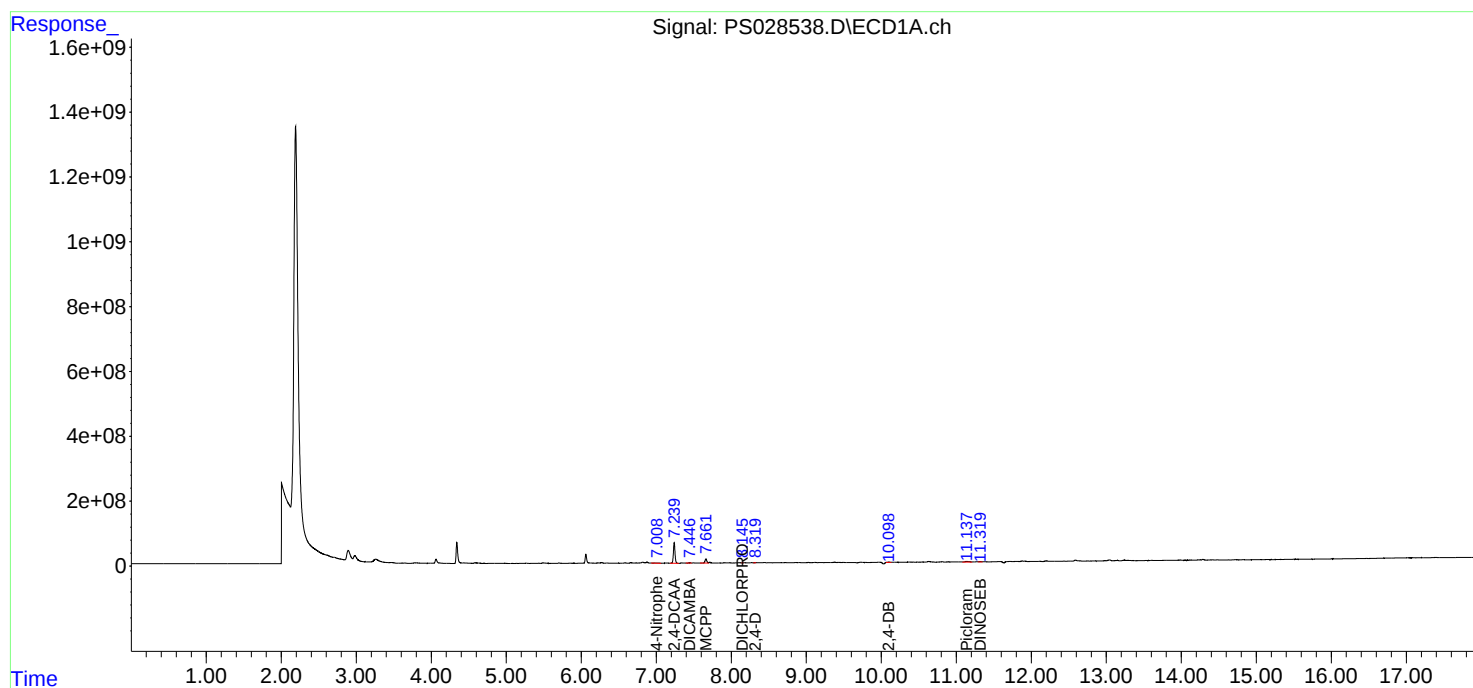


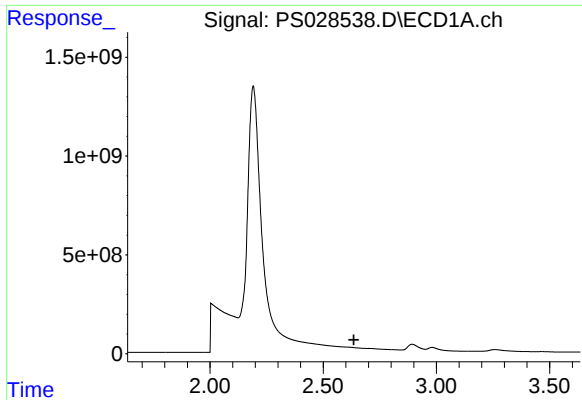

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.635 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BP-F-2

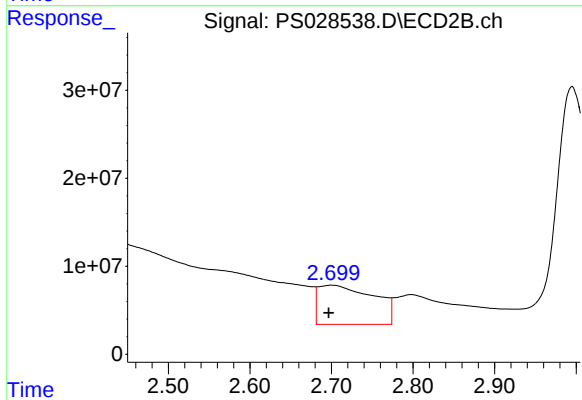


#1 Dalapon

R.T.: 2.700 min
Delta R.T.: 0.003 min
Response: 210165249
Conc: 86.85 ng/ml

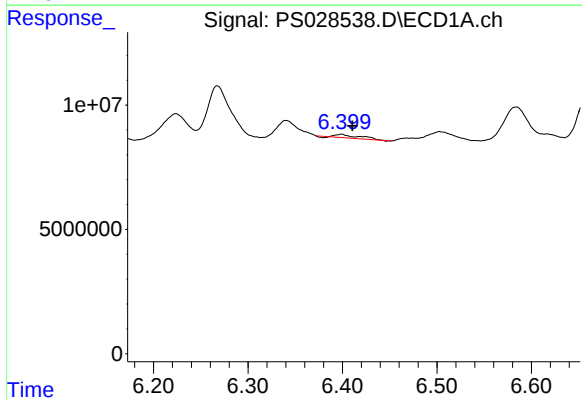


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.398 min
Delta R.T.: -0.012 min
Response: 2138633
Conc: N.D.

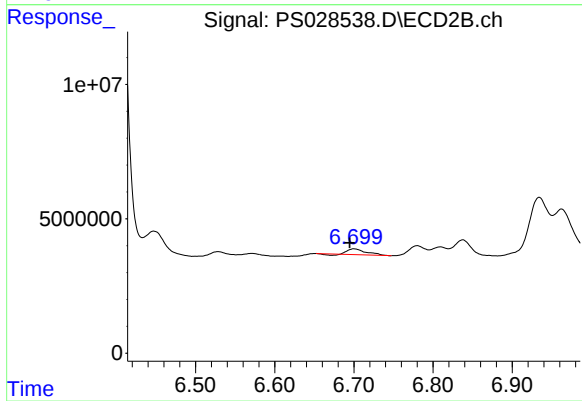

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.700 min
Delta R.T.: 0.005 min
Response: 3077289
Conc: 1.59 ng/ml

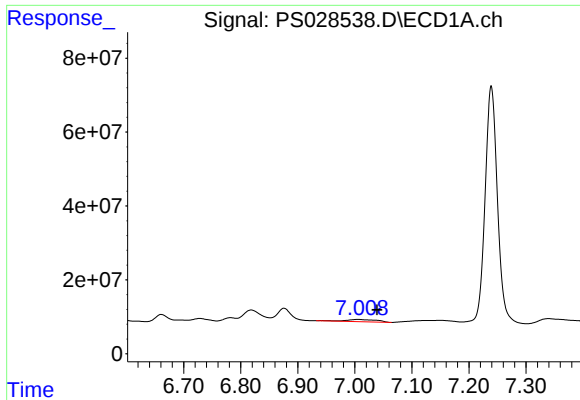

#3 4-Nitrophenol


R.T.: 7.005 min
Delta R.T.: -0.034 min
Response: 22489892
Conc: 13.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
BP-F-2

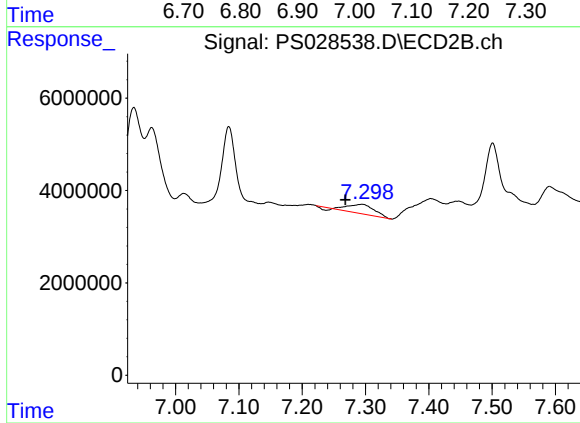


#3 4-Nitrophenol

R.T.: 7.294 min
Delta R.T.: 0.026 min
Response: 5381219
Conc: 6.23 ng/ml

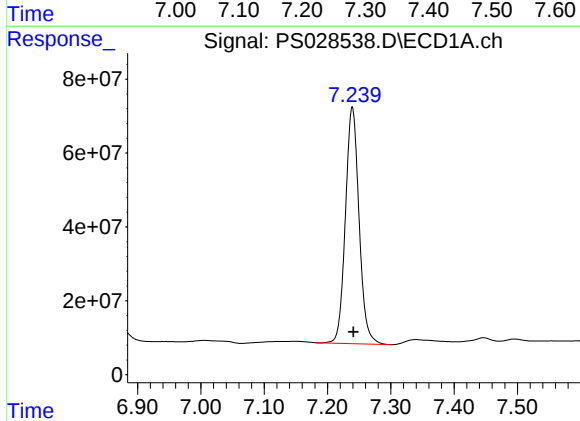


#4 2,4-DCAA

R.T.: 7.239 min
Delta R.T.: -0.002 min
Response: 960101170
Conc: 375.64 ng/ml

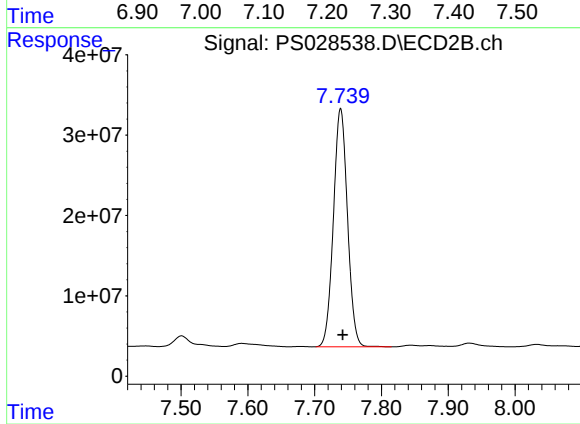

#4 2,4-DCAA


R.T.: 7.739 min
Delta R.T.: -0.003 min
Response: 433955490
Conc: 335.80 ng/ml

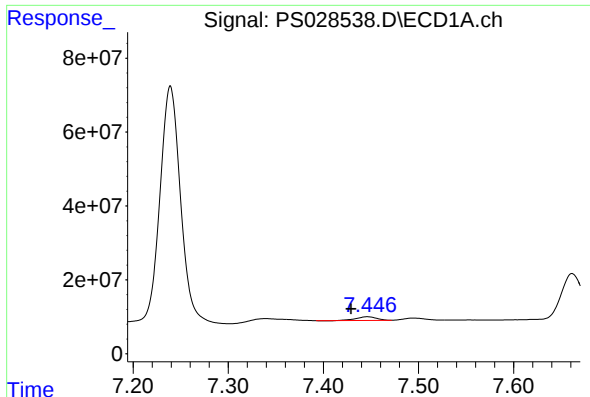

#5 DICAMBA


R.T.: 7.446 min
Delta R.T.: 0.017 min
Response: 14811446
Conc: 1.35 ng/ml

Instrument :
ECD_S
ClientSampleId :
BP-F-2

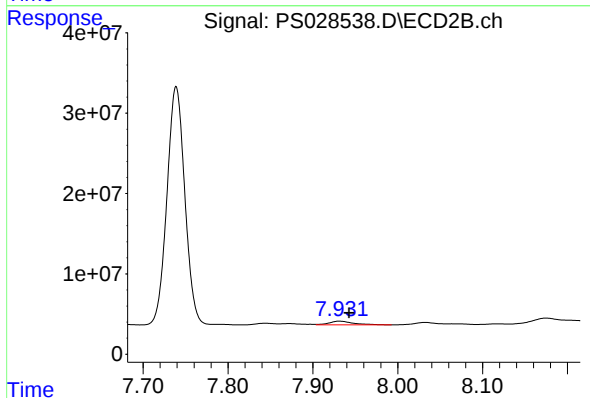


#5 DICAMBA

R.T.: 7.932 min
Delta R.T.: -0.011 min
Response: 9188065
Conc: 1.61 ng/ml

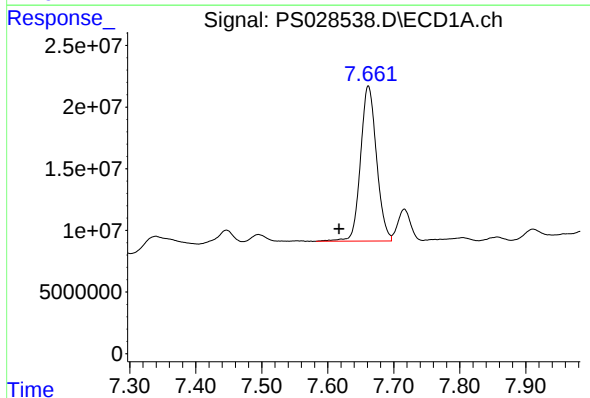


#6 MCP

R.T.: 7.662 min
Delta R.T.: 0.044 min
Response: 211930871
Conc: 30.13 ug/ml

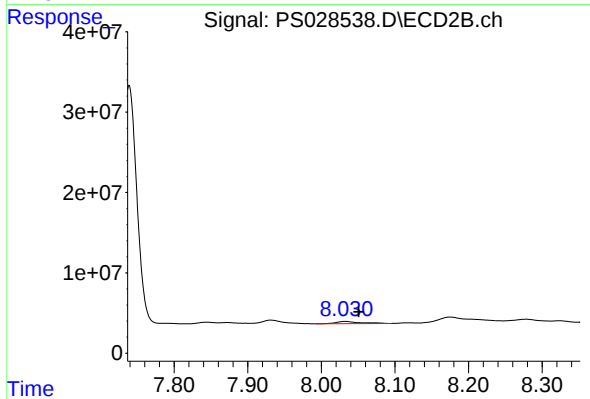

#6 MCP


R.T.: 8.032 min
Delta R.T.: -0.018 min
Response: 6409289
Conc: 1.49 ug/ml

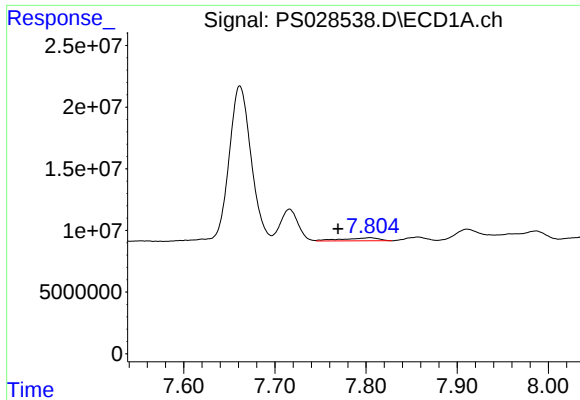

#7 MCPA


R.T.: 7.804 min
Delta R.T.: 0.035 min
Response: 6672391
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BP-F-2

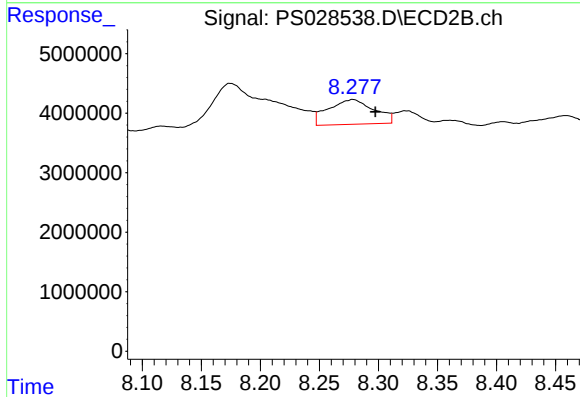


#7 MCPA

R.T.: 8.278 min
Delta R.T.: -0.019 min
Response: 11171478
Conc: 1.80 ug/ml

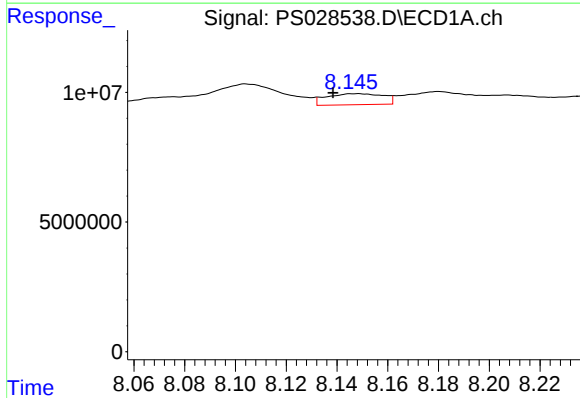


#8 DICHLORPROP

R.T.: 8.148 min
Delta R.T.: 0.010 min
Response: 6585853
Conc: 2.23 ng/ml

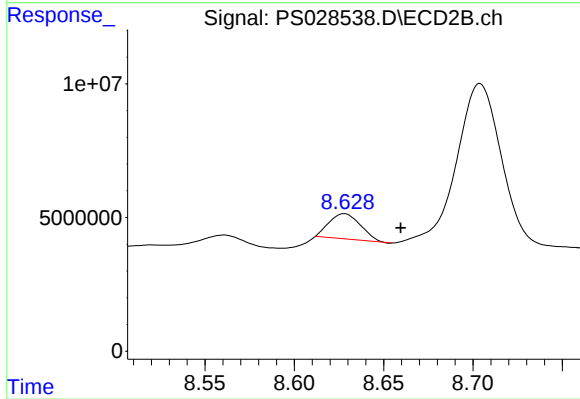

#8 DICHLORPROP


R.T.: 8.628 min
Delta R.T.: -0.032 min
Response: 11420214
Conc: 7.82 ng/ml

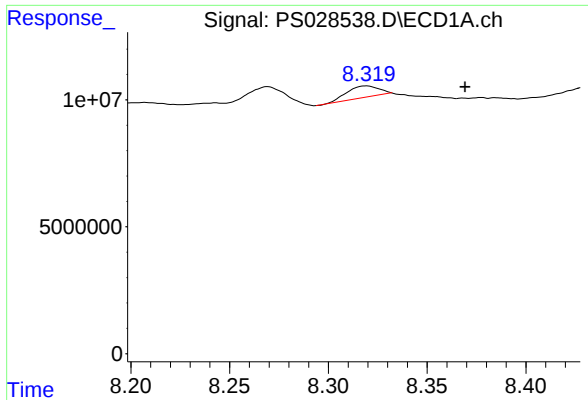

#9 2,4-D


R.T.: 8.319 min
Delta R.T.: -0.050 min
Response: 5958042
Conc: 1.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
BP-F-2

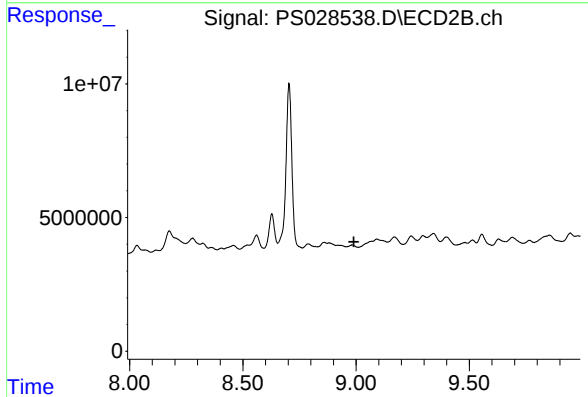


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.990 min
Response: 0
Conc: N.D.

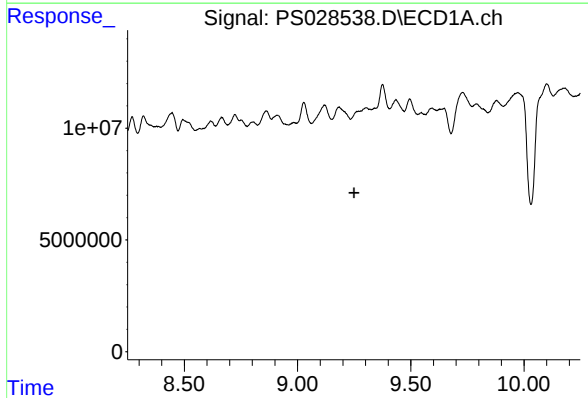


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.249 min
Response: 0
Conc: N.D.

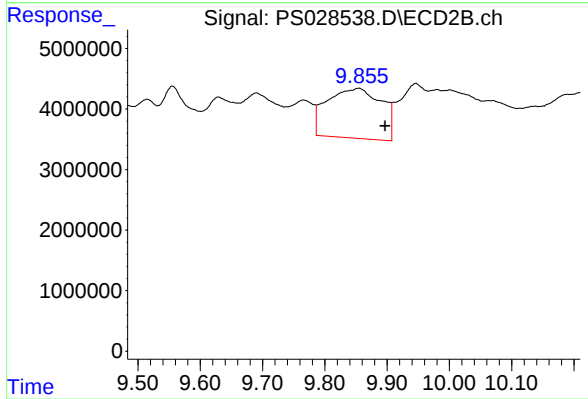

#11 2,4,5-TP (SILVEX)


R.T.: 9.854 min
Delta R.T.: -0.043 min
Response: 49936205
Conc: 5.92 ng/ml

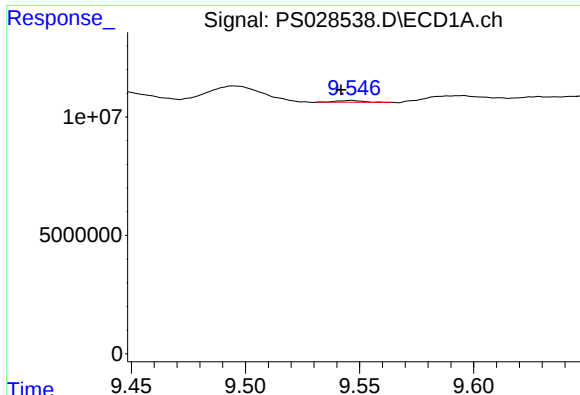

#12 2,4,5-T


R.T.: 9.546 min
Delta R.T.: 0.004 min
Response: 633524
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BP-F-2

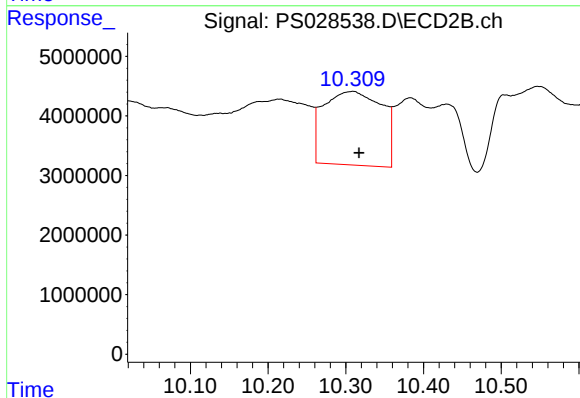


#12 2,4,5-T

R.T.: 10.308 min
Delta R.T.: -0.009 min
Response: 64382092
Conc: 7.68 ng/ml

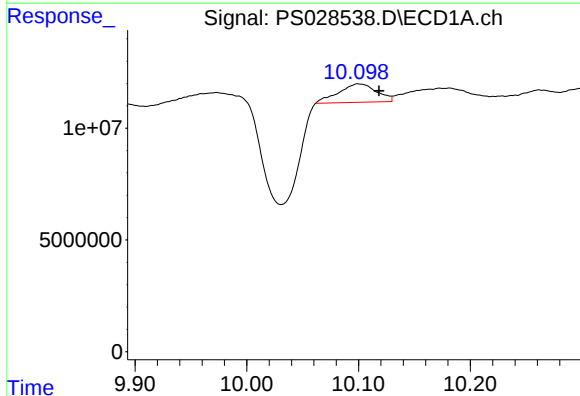


#13 2,4-DB

R.T.: 10.101 min
Delta R.T.: -0.018 min
Response: 19442292
Conc: 7.13 ng/ml

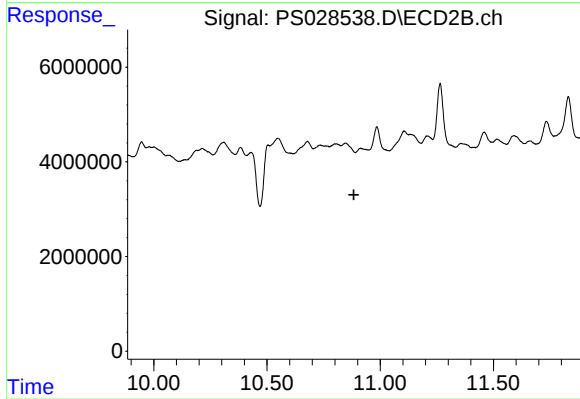

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.884 min
Response: 0
Conc: N.D.

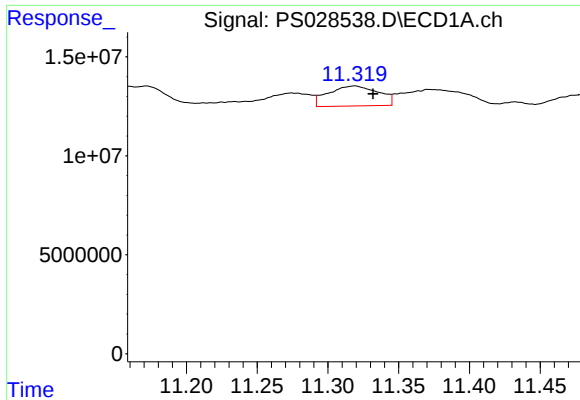

#14 DINOSEB


R.T.: 11.318 min
Delta R.T.: -0.014 min
Response: 24946183
Conc: 1.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
BP-F-2

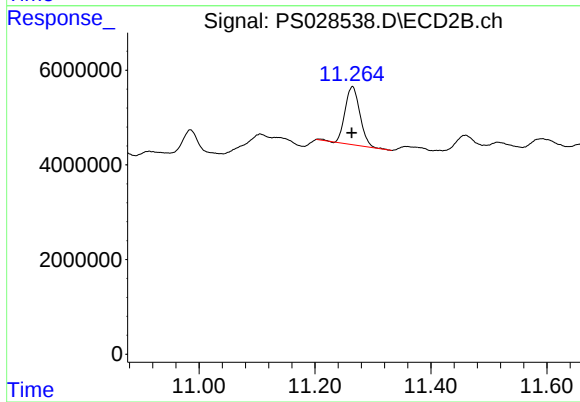


#14 DINOSEB

R.T.: 11.264 min
Delta R.T.: 0.001 min
Response: 22037411
Conc: 3.99 ng/ml

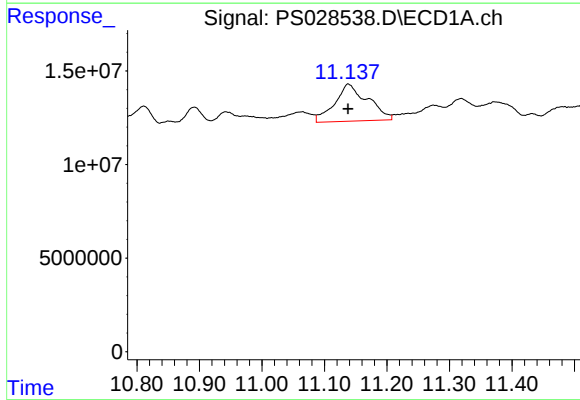

#15 Picloram

R.T.: 11.139 min
Delta R.T.: 0.000 min
Response: 72569028
Conc: 2.58 ng/ml

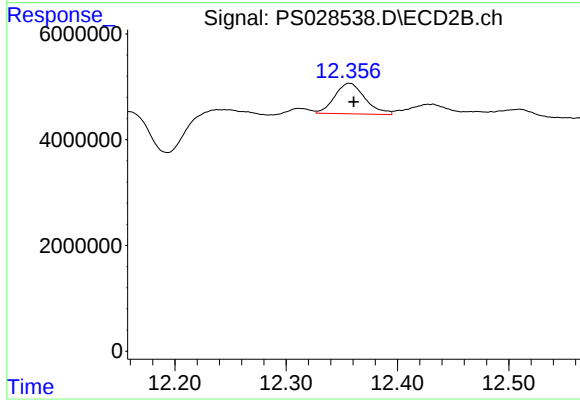

#15 Picloram

R.T.: 12.357 min
Delta R.T.: -0.004 min
Response: 10957737
Conc: N.D.