

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111424\
 Data File : PS028544.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Nov 2024 20:16
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 00:28:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.240	7.739	1551.5E6	775.9E6	607.024	600.428
Target Compounds							
2) T	3,5-DICHL...	6.393	0.000	323221	0	<MDL	N.D. #
3) T	4-Nitroph...	7.031	0.000	8632066	0	5.082	N.D. #
5) T	DICAMBA	0.000	7.934	0	3226974	N.D.	<MDL
6) T	MCP	7.667f	0.000	25996880	0	3.696	N.D. #
8) T	DICHLORPROP	8.141	8.707f	76816	12536713	<MDL	8.583 #
10) T	Pentachlo...	8.674	0.000	270542	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	9.895	0	1484819	N.D.	<MDL
12) T	2,4,5-T	9.542	10.312	1955410	6920096	<MDL	<MDL #
14) T	DINOSEB	11.344	0.000	1251808	0	<MDL	N.D. #
15) T	Picloram	11.139	12.359	19488564	19764936	<MDL	1.746 #
16) T	DCPA	11.620	12.359f	2154984	19764936	<MDL	2.038 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111424\
Data File : PS028544.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Nov 2024 20:16
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 00:28:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

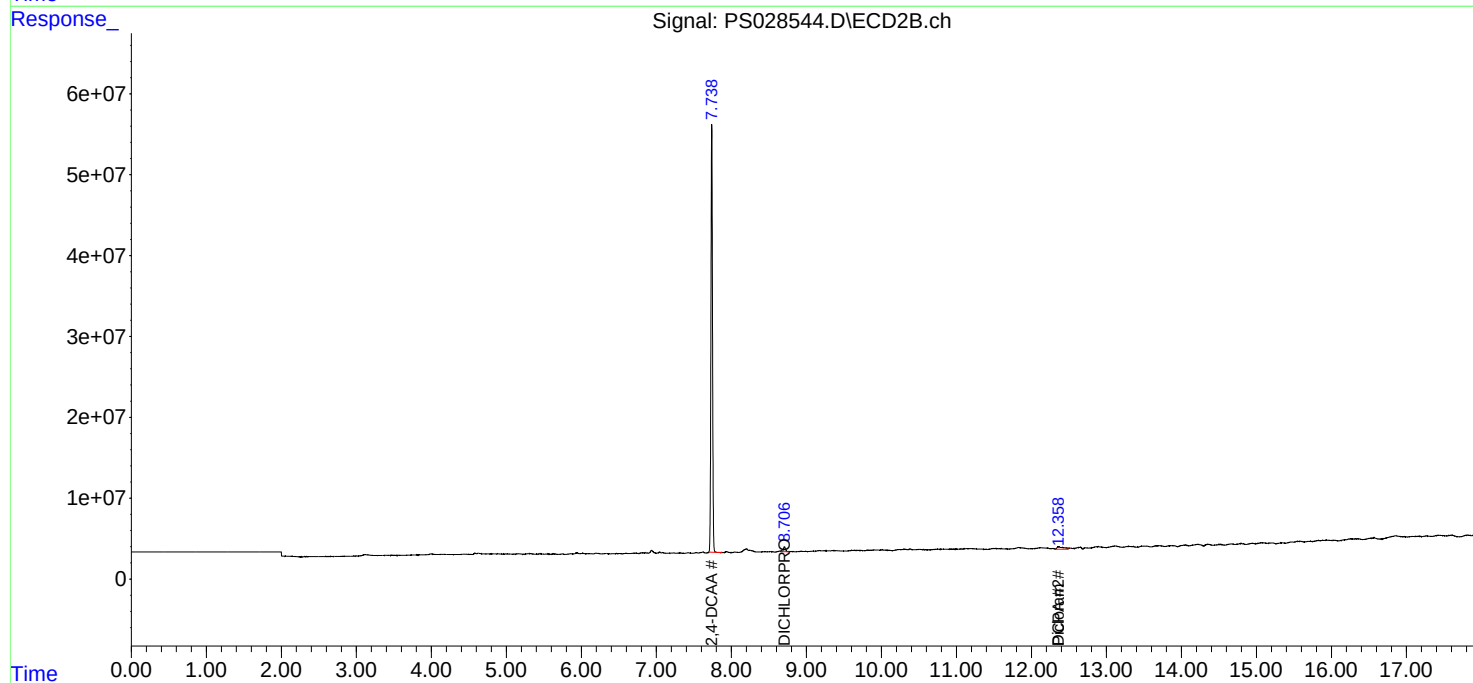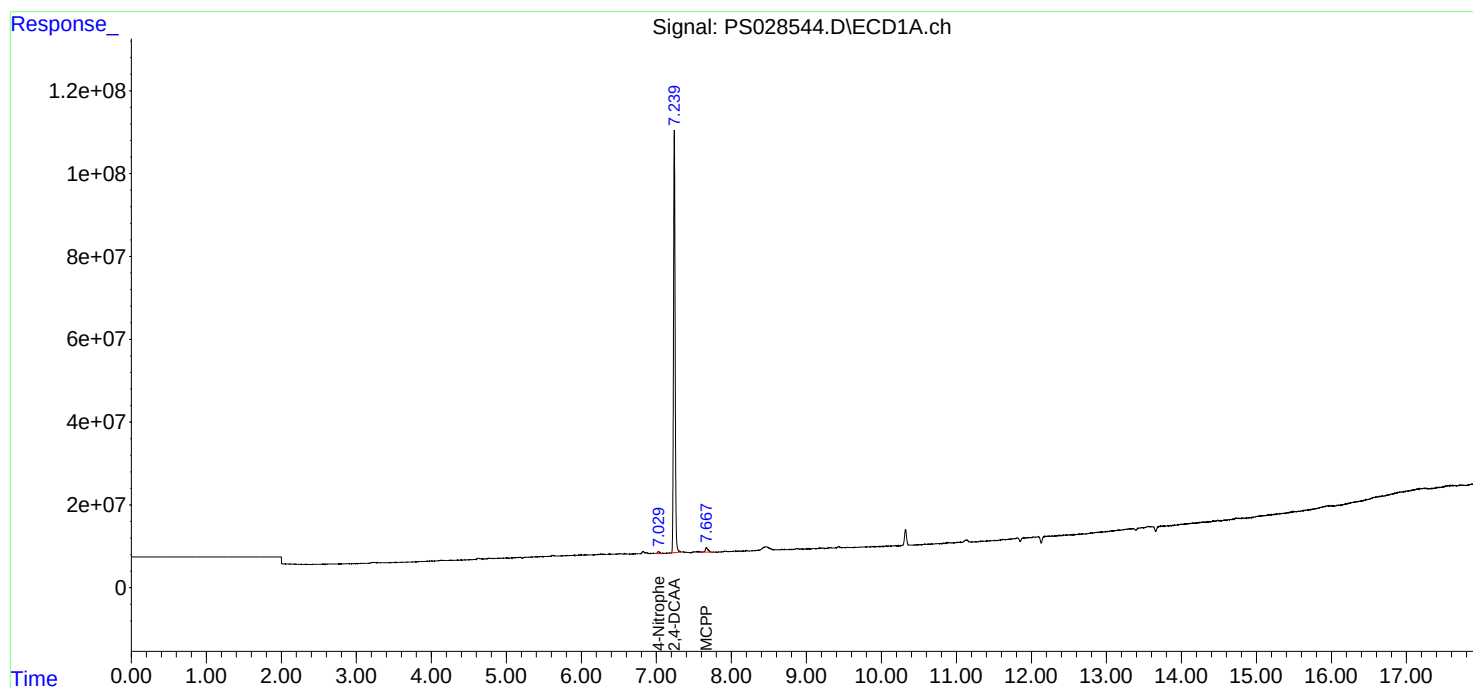


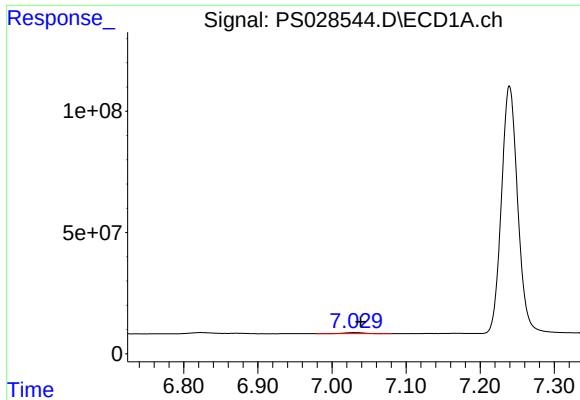

#3 4-Nitrophenol


R.T.: 7.031 min
Delta R.T.: -0.008 min
Response: 8632066
Conc: 5.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

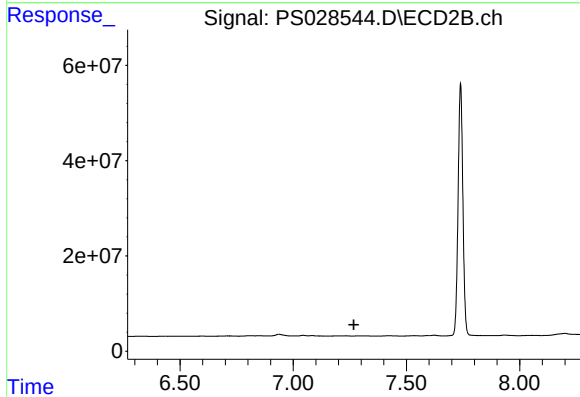


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.268 min
Response: 0
Conc: N.D.

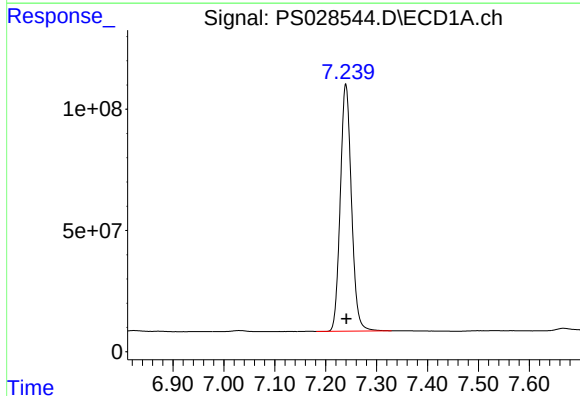


#4 2,4-DCAA

R.T.: 7.240 min
Delta R.T.: -0.001 min
Response: 1551480385
Conc: 607.02 ng/ml

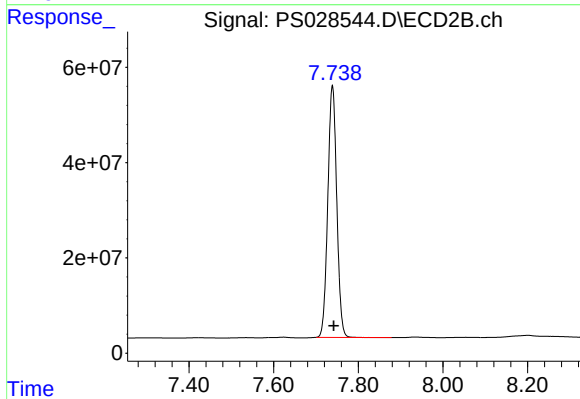

#4 2,4-DCAA


R.T.: 7.739 min
Delta R.T.: -0.003 min
Response: 775936630
Conc: 600.43 ng/ml

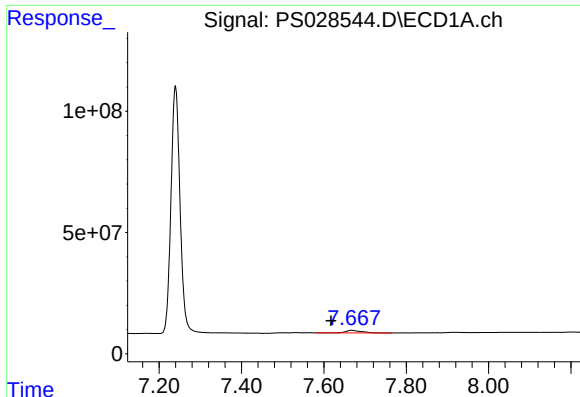

#6 MCP


R.T.: 7.667 min
Delta R.T.: 0.050 min
Response: 25996880
Conc: 3.70 ug/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

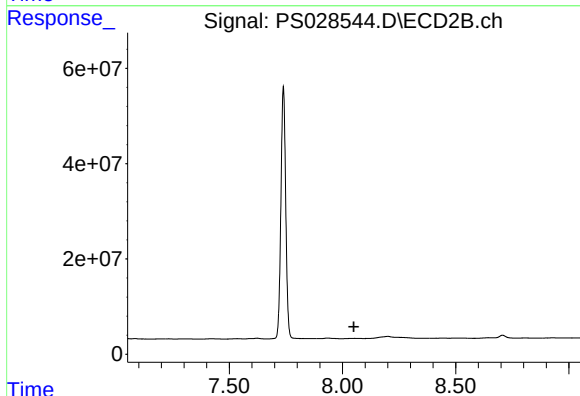


#6 MCP

R.T.: 0.000 min
Exp R.T. : 8.051 min
Response: 0
Conc: N.D.

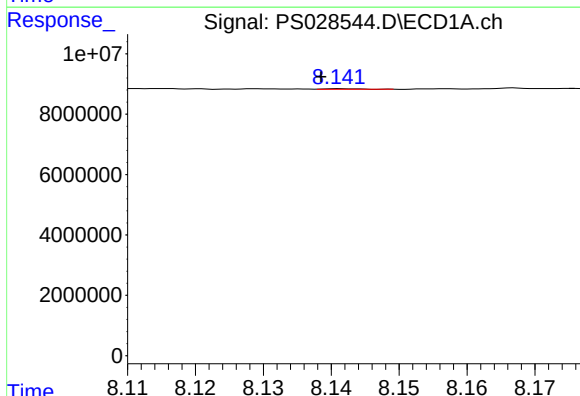


#8 DICHLORPROP

R.T.: 8.141 min
Delta R.T.: 0.003 min
Response: 76816
Conc: N.D.

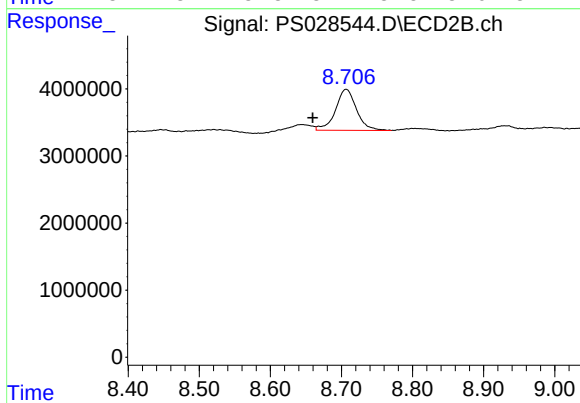

#8 DICHLORPROP


R.T.: 8.707 min
Delta R.T.: 0.047 min
Response: 12536713
Conc: 8.58 ng/ml

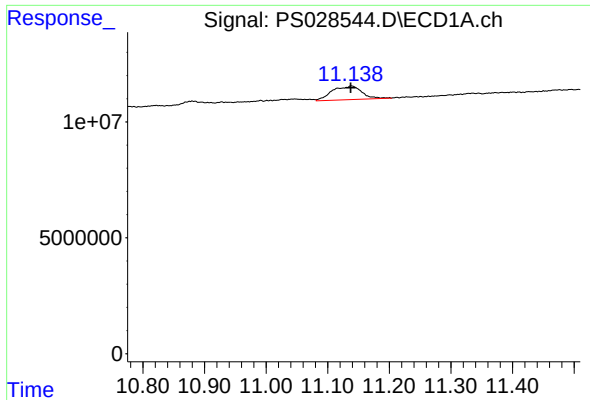

#15 Picloram


R.T.: 11.139 min
Delta R.T.: 0.001 min
Response: 19488564
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

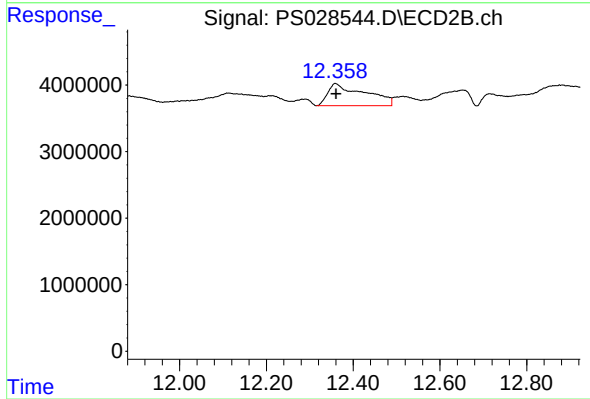


#15 Picloram

R.T.: 12.359 min
Delta R.T.: -0.002 min
Response: 19764936
Conc: 1.75 ng/ml

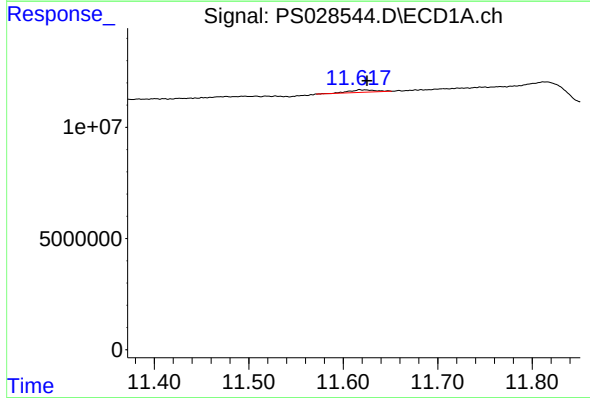

#16 DCPA

R.T.: 11.620 min
Delta R.T.: -0.006 min
Response: 2154984
Conc: N.D.

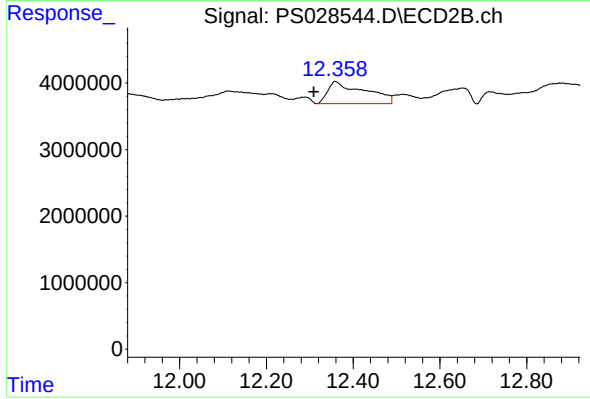

#16 DCPA

R.T.: 12.359 min
Delta R.T.: 0.049 min
Response: 19764936
Conc: 2.04 ng/ml