

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111521\
 Data File : PS017412.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2021 13:39
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 00:29:51 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
 Quant Title : 8080.M
 QLast Update : Tue Oct 19 01:21:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

5) T	DICAMBA	7.338	0.000	5688379	0	<MDL	N.D.	#
7) T	MCPA	7.668	0.000	1589014	0	<MDL	N.D.	#
9) T	2,4-D	8.268	0.000	36224985	0	20.452	N.D.	#
10) T	Pentachlo...	8.564	0.000	11079463	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	9.116	0.000	9660903	0	1.188	N.D.	#
12) T	2,4,5-T	9.408	9.021f	16041490	23087388	1.997	7.284	#
13) T	2,4-DB	9.963	0.000	5672480	0	3.771	N.D.	#
14) T	DINOSEB	11.100	0.000	12277288	0	2.167	N.D.	#
15) T	Picloram	10.938	10.781	135.1E6	44006130	12.645	11.491	
16) T	DCPA	11.367	10.722	16626102	6747837	1.633	1.581	



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111521\
Data File : PS017412.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2021 13:39
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 00:29:51 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS101821.M
Quant Title : 8080.M
QLast Update : Tue Oct 19 01:21:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

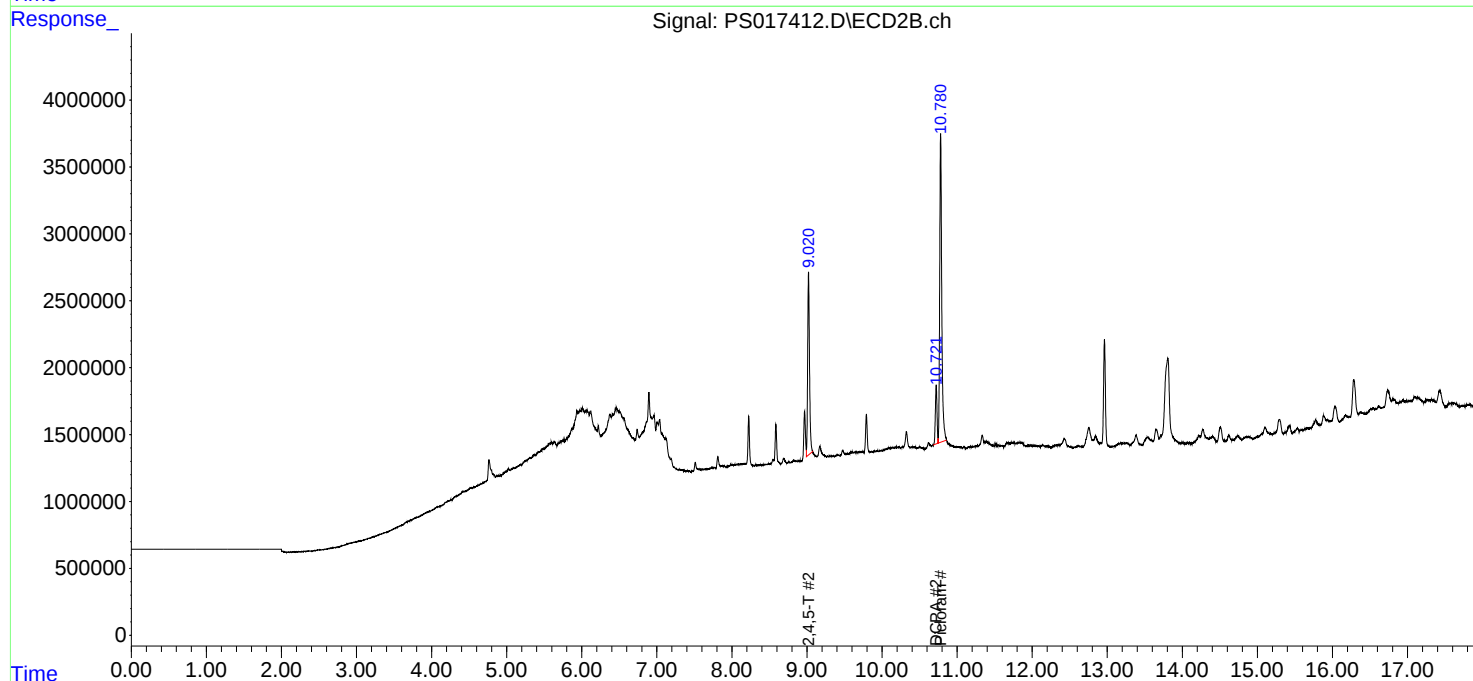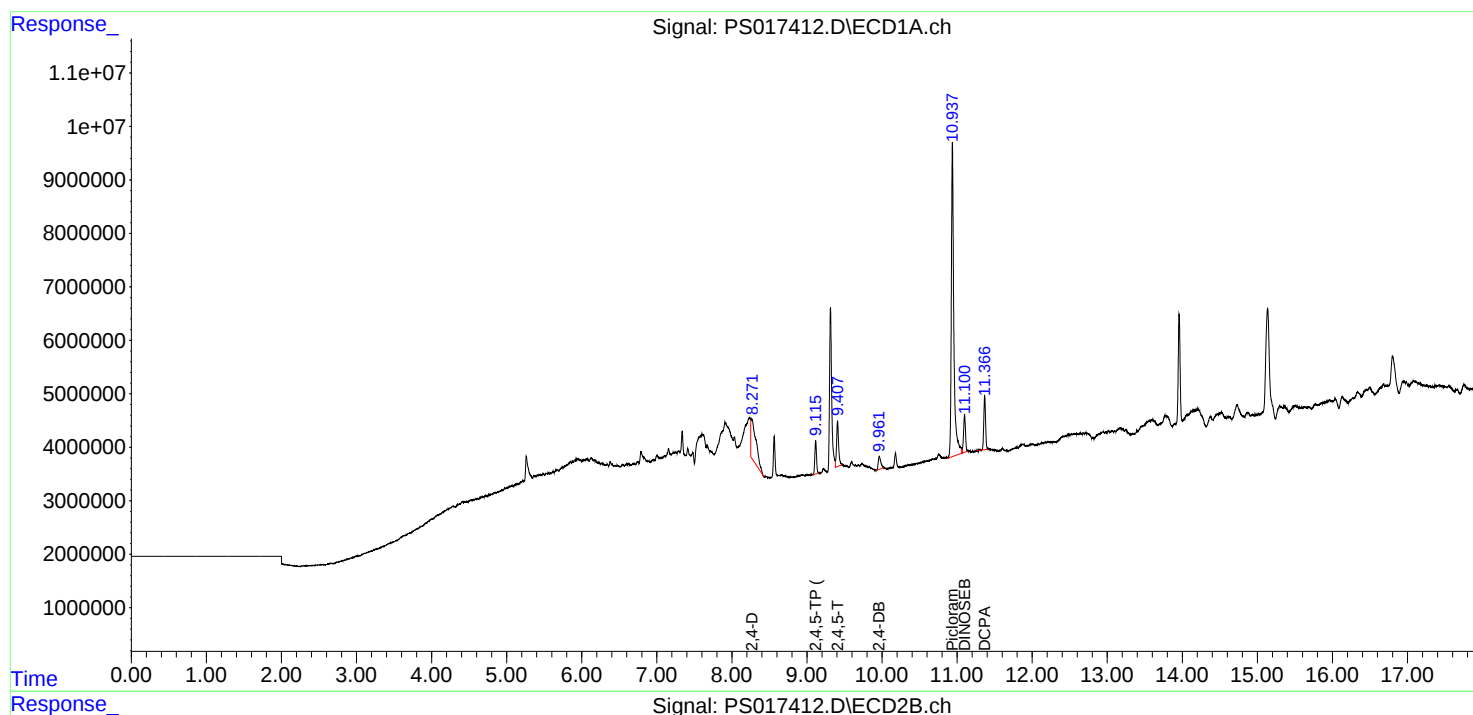


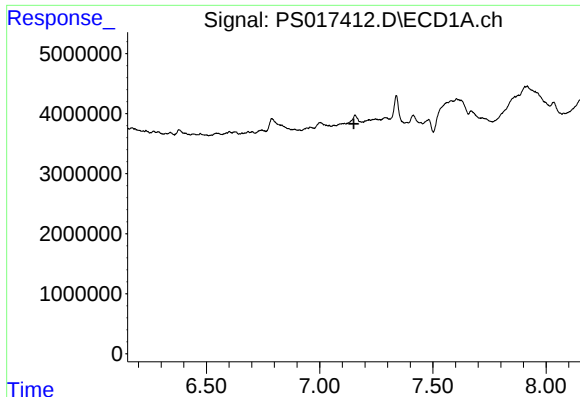

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.151 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

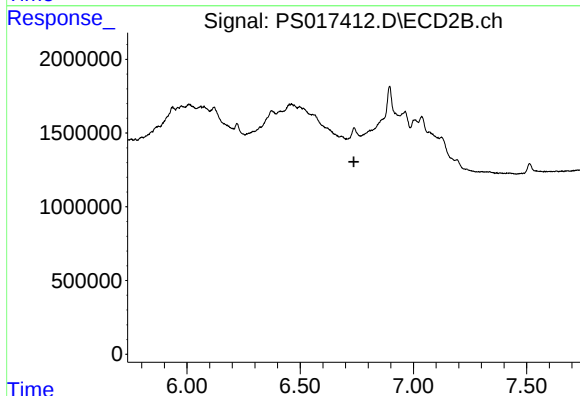


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.737 min
Response: 0
Conc: N.D.

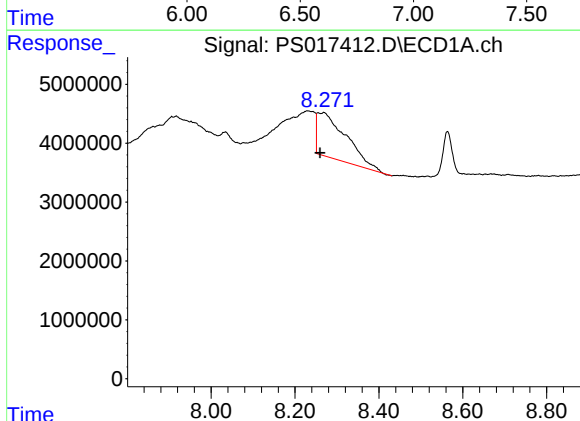


#9 2,4-D

R.T.: 8.268 min
Delta R.T.: 0.009 min
Response: 36224985
Conc: 20.45 ng/ml

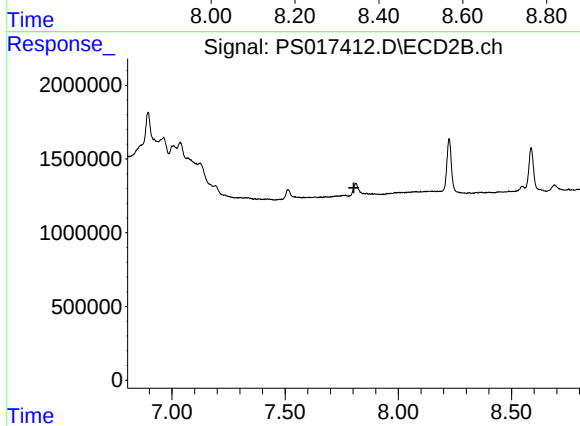

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.804 min
Response: 0
Conc: N.D.

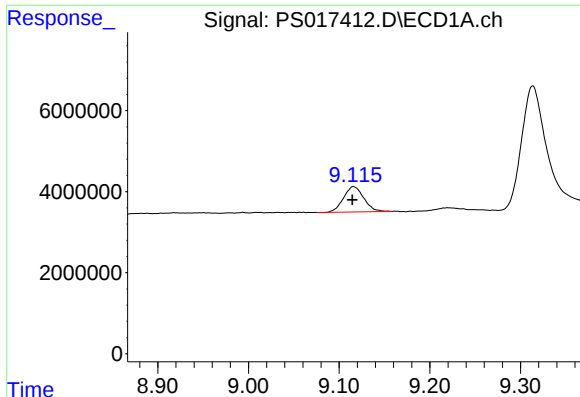

#11 2,4,5-TP (SILVEX)


R.T.: 9.116 min
Delta R.T.: 0.001 min
Response: 9660903
Conc: 1.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

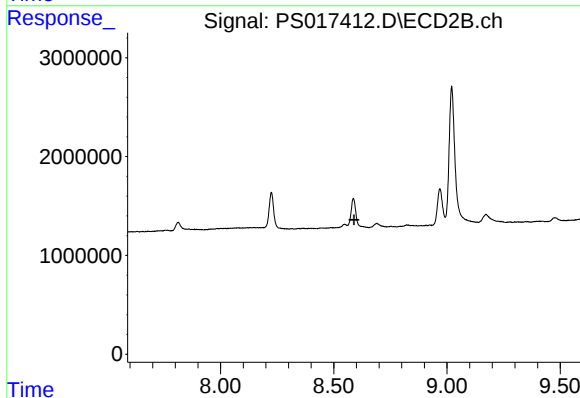


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 8.589 min
Response: 0
Conc: N.D.

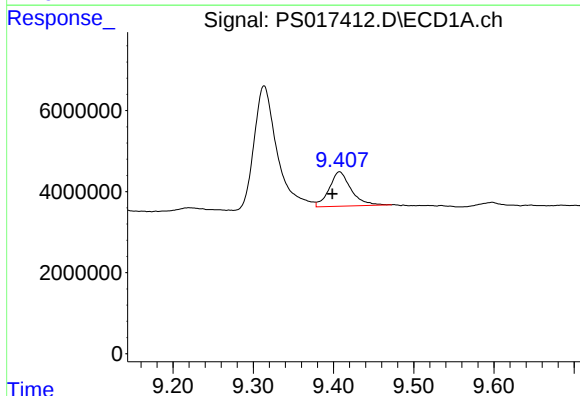


#12 2,4,5-T

R.T.: 9.408 min
Delta R.T.: 0.009 min
Response: 16041490
Conc: 2.00 ng/ml

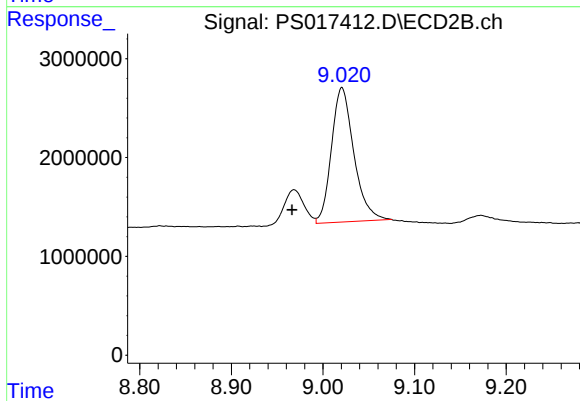

#12 2,4,5-T


R.T.: 9.021 min
Delta R.T.: 0.054 min
Response: 23087388
Conc: 7.28 ng/ml

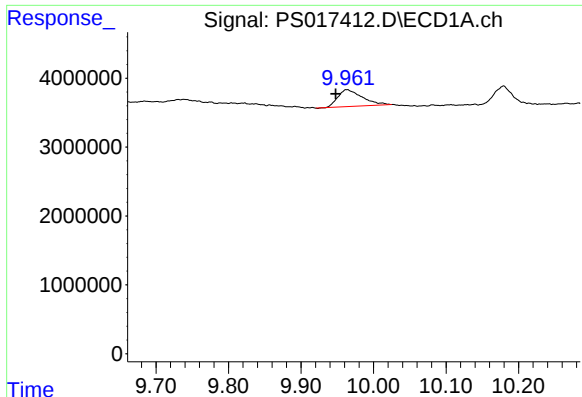

#13 2,4-DB


R.T.: 9.963 min
Delta R.T.: 0.015 min
Response: 5672480
Conc: 3.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

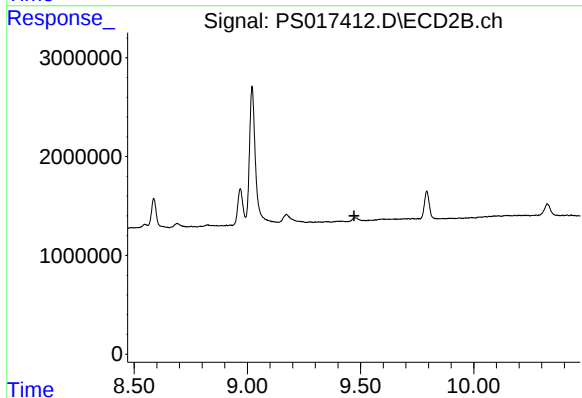


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.471 min
Response: 0
Conc: N.D.

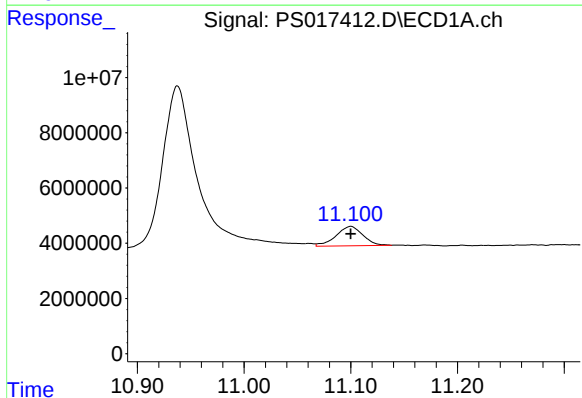


#14 DINOSEB

R.T.: 11.100 min
Delta R.T.: 0.000 min
Response: 12277288
Conc: 2.17 ng/ml

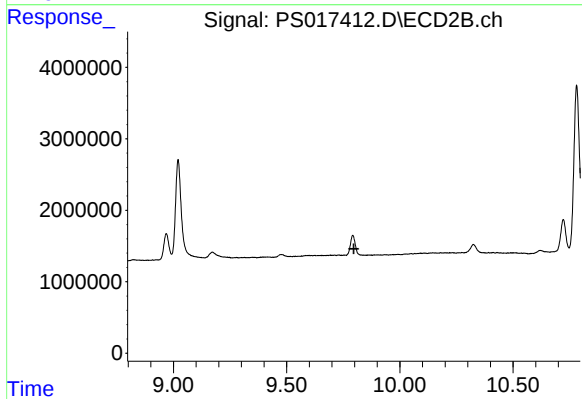

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.797 min
Response: 0
Conc: N.D.

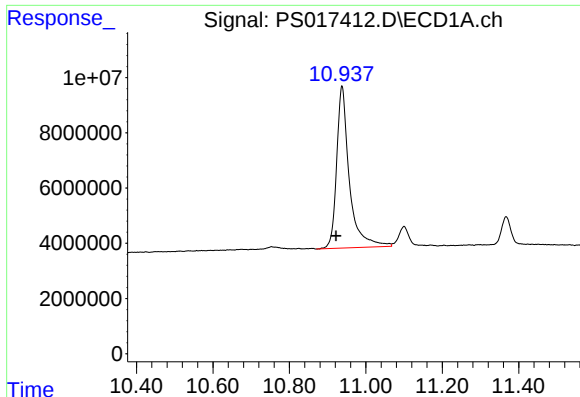

#15 Picloram


R.T.: 10.938 min
Delta R.T.: 0.016 min
Response: 135067699
Conc: 12.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

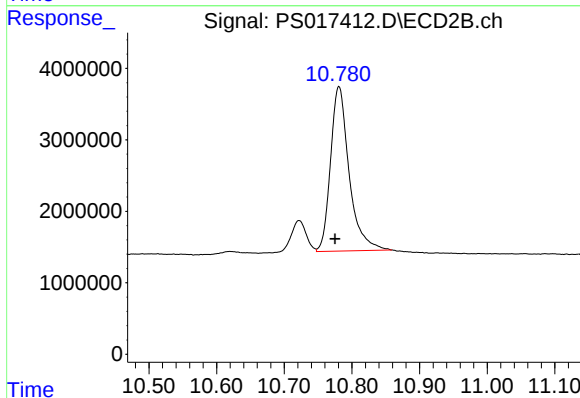


#15 Picloram

R.T.: 10.781 min
Delta R.T.: 0.006 min
Response: 44006130
Conc: 11.49 ng/ml

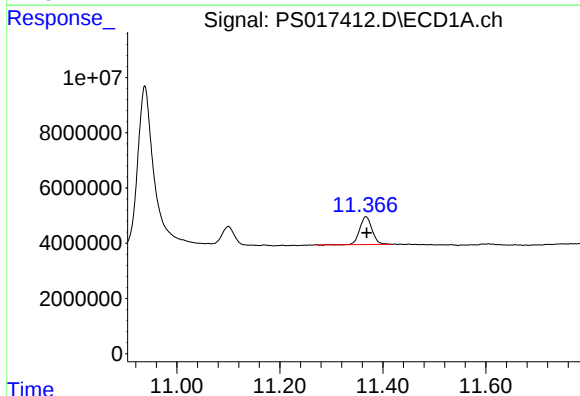

#16 DCPA

R.T.: 11.367 min
Delta R.T.: -0.002 min
Response: 16626102
Conc: 1.63 ng/ml

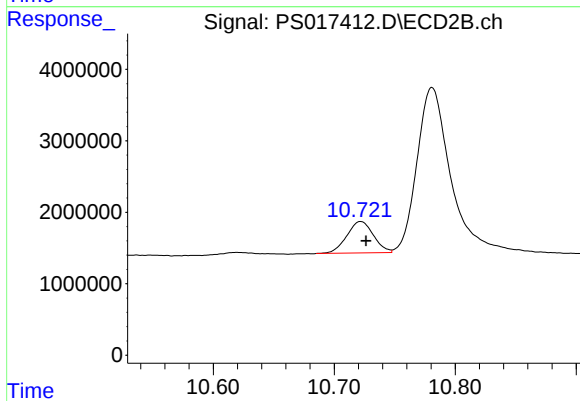

#16 DCPA

R.T.: 10.722 min
Delta R.T.: -0.005 min
Response: 6747837
Conc: 1.58 ng/ml