

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111523\
 Data File : PS024832.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2023 08:04
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 23:57:04 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 03 15:07:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	2.512	2.565	6618676	1710259	2.748	1.623 #
3) T	4-Nitroph...	0.000	6.374	0	1190603	N.D.	2.711
5) T	DICAMBA	0.000	6.933	0	526644	N.D.	<MDL
6) T	MCPP	6.684	6.976f	403862	2026452	<MDL	1.044 #
7) T	MCPA	0.000	7.186f	0	13321351	N.D.	4.321
8) T	DICHLORPROP	0.000	7.564	0	2342188	N.D.	3.206
9) T	2,4-D	0.000	7.778f	0	1234263	N.D.	1.379
11) T	2,4,5-TP ...	0.000	8.613	0	628758	N.D.	<MDL
12) T	2,4,5-T	0.000	8.986	0	547425	N.D.	<MDL
13) T	2,4-DB	0.000	9.481	0	707849	N.D.	1.452
15) T	Picloram	9.685	10.771	53065032	20845937	2.983	3.431
16) T	DCPA	0.000	10.771	0	20845937	N.D.	4.148



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111523\
Data File : PS024832.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2023 08:04
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 23:57:04 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
Quant Title : 8080.M
QLast Update : Fri Nov 03 15:07:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

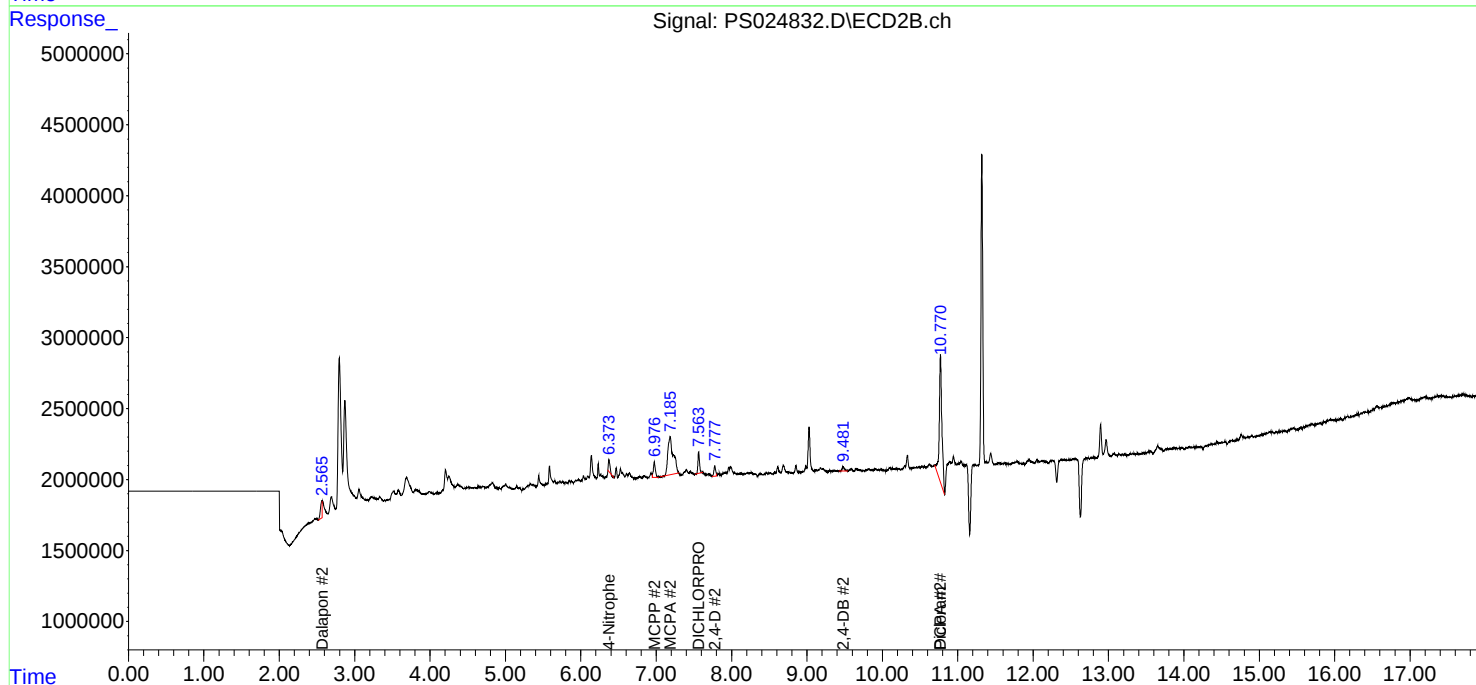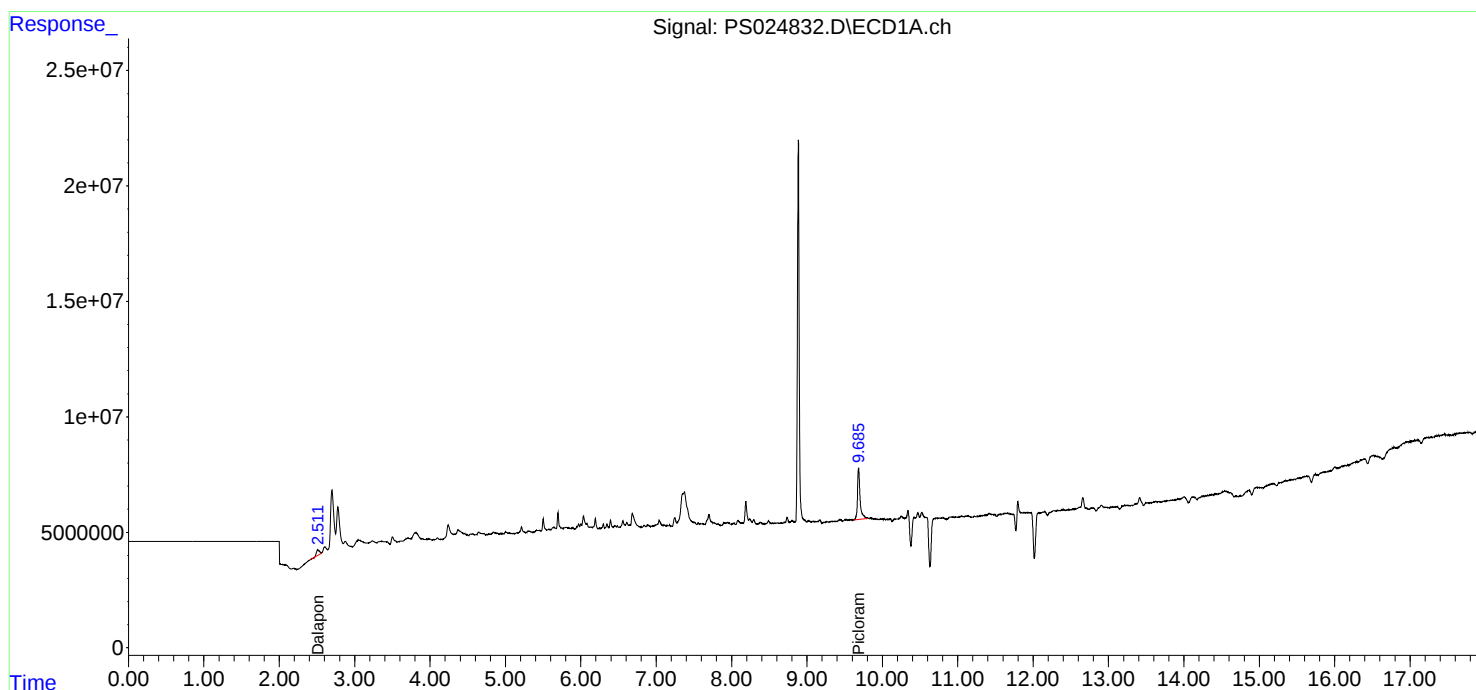


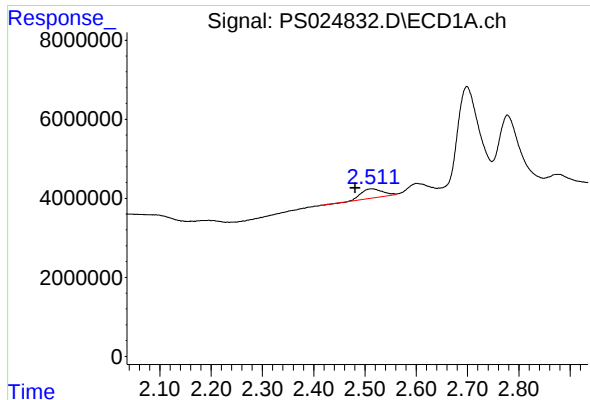

#1 Dalapon


R.T.: 2.512 min
Delta R.T.: 0.031 min
Response: 6618676
Conc: 2.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

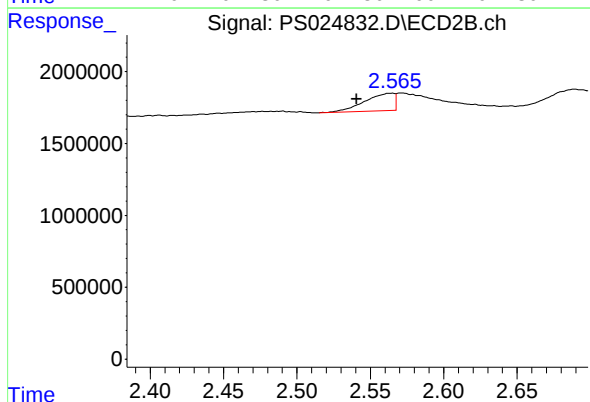


#1 Dalapon

R.T.: 2.565 min
Delta R.T.: 0.024 min
Response: 1710259
Conc: 1.62 ng/ml

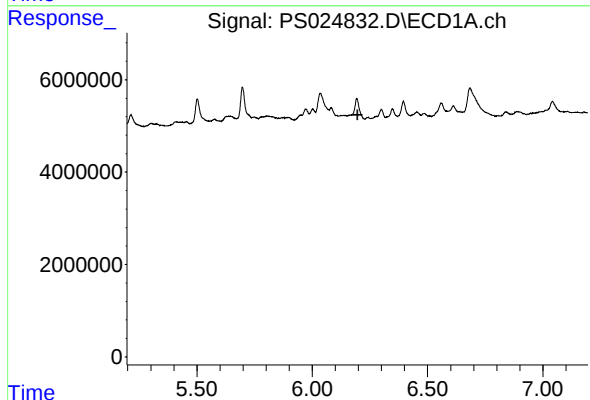


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.196 min
Response: 0
Conc: N.D.

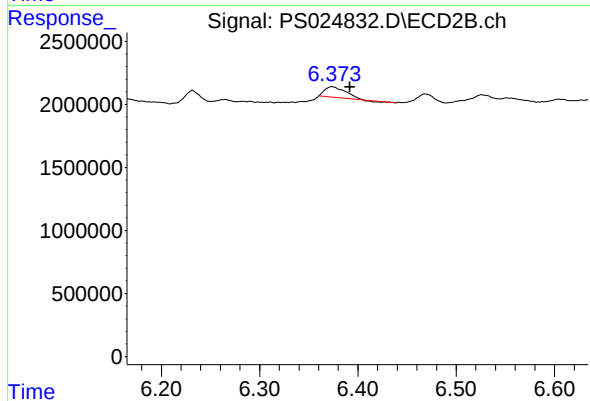

#3 4-Nitrophenol


R.T.: 6.374 min
Delta R.T.: -0.018 min
Response: 1190603
Conc: 2.71 ng/ml

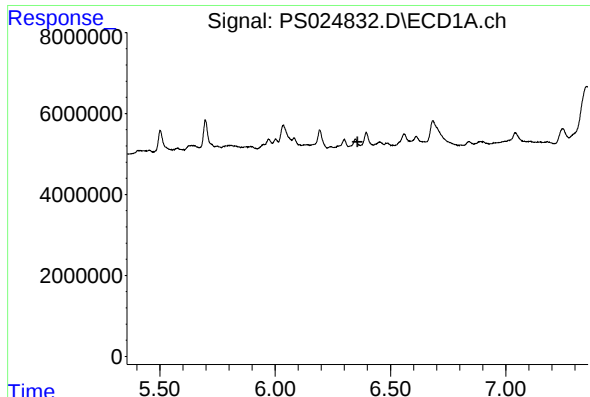

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 6.357 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

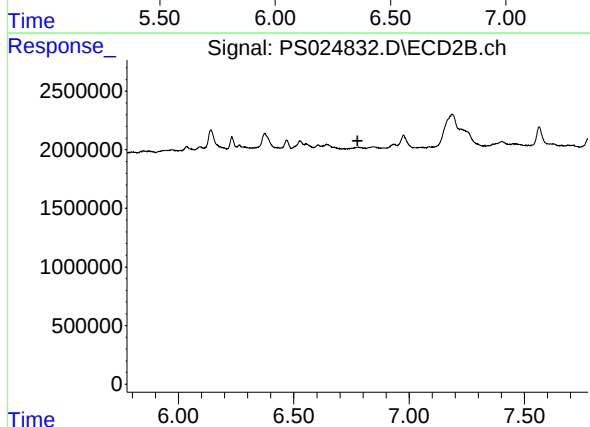


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.777 min
Response: 0
Conc: N.D.

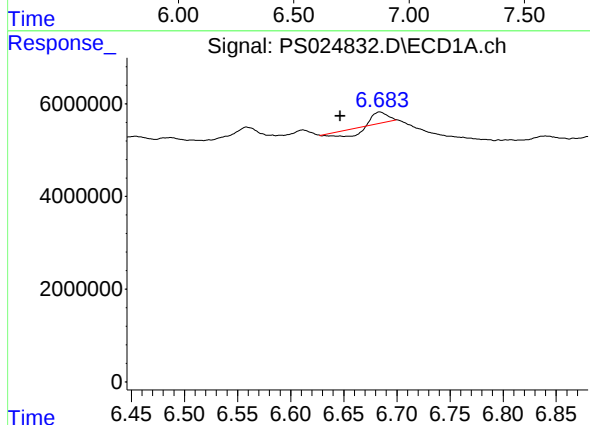


#6 MCPP

R.T.: 6.684 min
Delta R.T.: 0.038 min
Response: 403862
Conc: N.D.

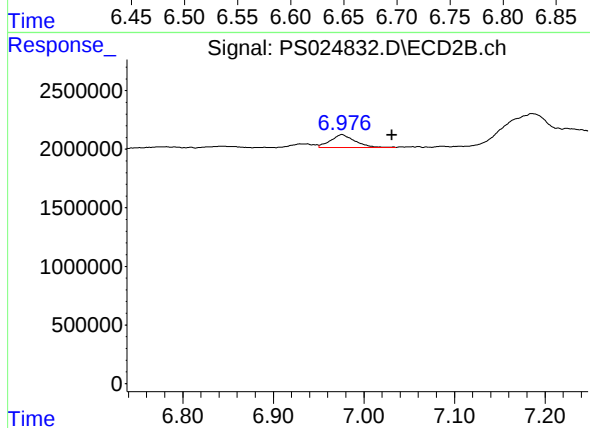

#6 MCPP


R.T.: 6.976 min
Delta R.T.: -0.055 min
Response: 2026452
Conc: 1.04 ug/ml

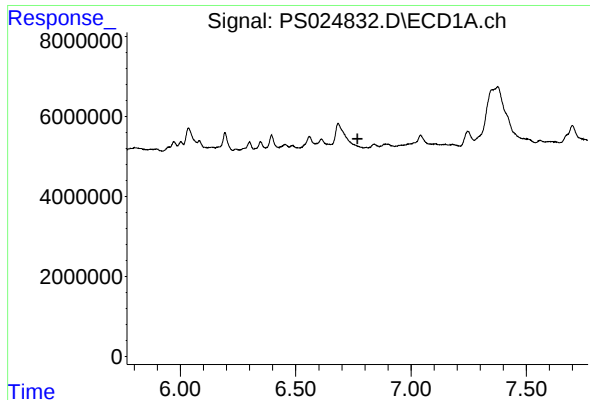

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.768 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

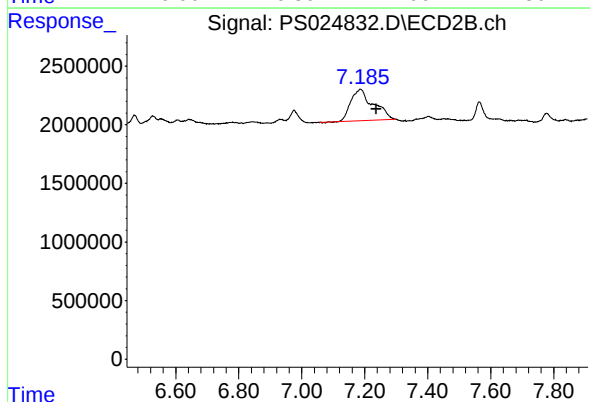


#7 MCPA

R.T.: 7.186 min
Delta R.T.: -0.050 min
Response: 13321351
Conc: 4.32 ug/ml

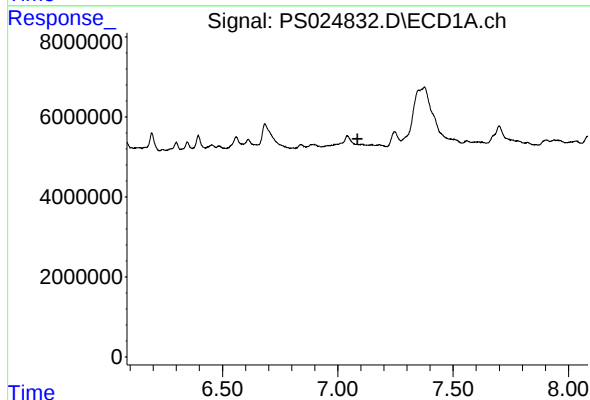


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.085 min
Response: 0
Conc: N.D.

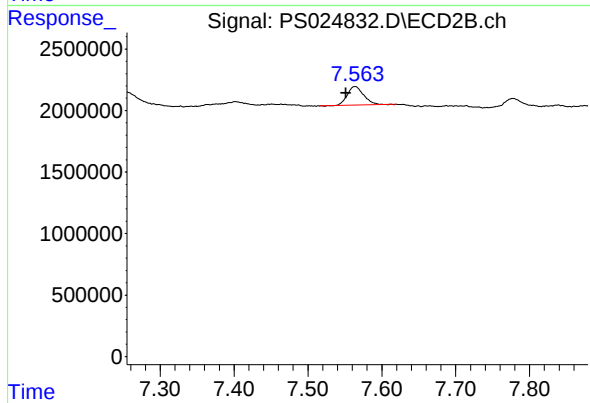

#8 DICHLORPROP


R.T.: 7.564 min
Delta R.T.: 0.013 min
Response: 2342188
Conc: 3.21 ng/ml

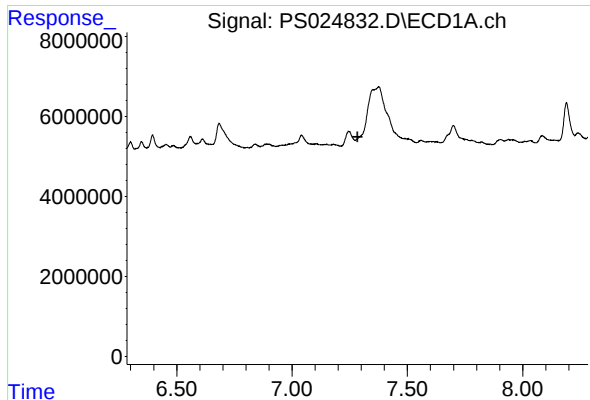

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.284 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

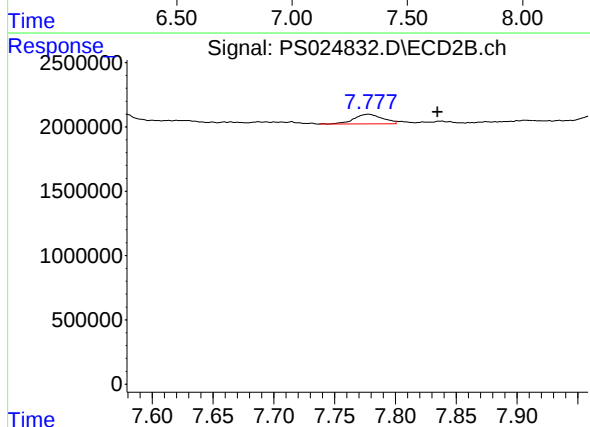


#9 2,4-D

R.T.: 7.778 min
Delta R.T.: -0.057 min
Response: 1234263
Conc: 1.38 ng/ml

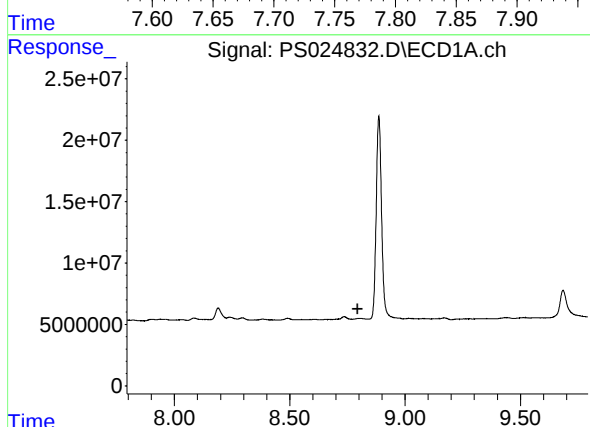


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.794 min
Response: 0
Conc: N.D.

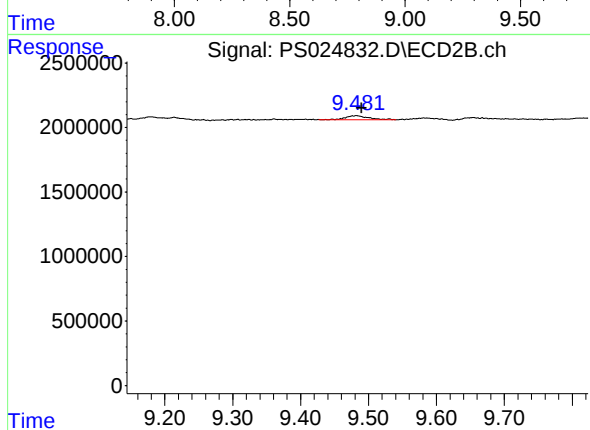

#13 2,4-DB


R.T.: 9.481 min
Delta R.T.: -0.009 min
Response: 707849
Conc: 1.45 ng/ml

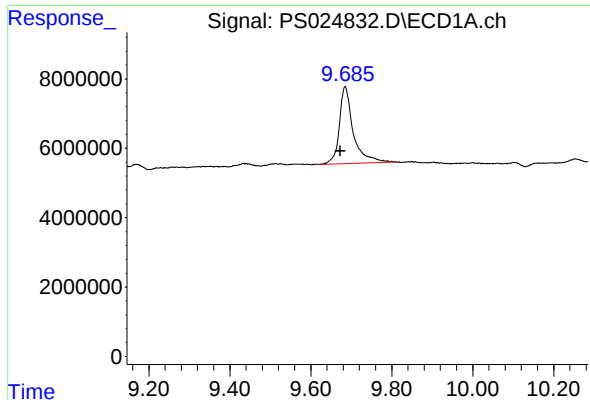

#15 Picloram


R.T.: 9.685 min
Delta R.T.: 0.013 min
Response: 53065032
Conc: 2.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

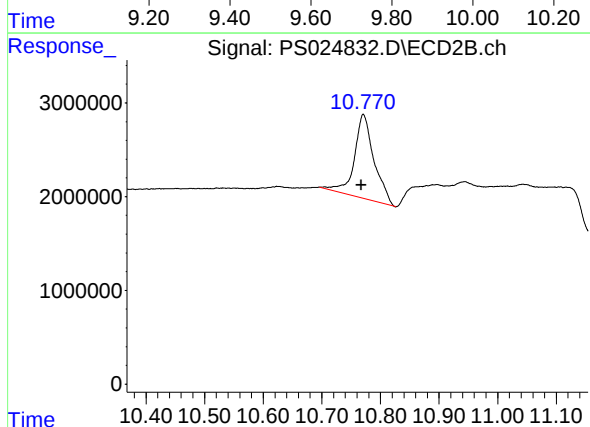


#15 Picloram

R.T.: 10.771 min
Delta R.T.: 0.003 min
Response: 20845937
Conc: 3.43 ng/ml

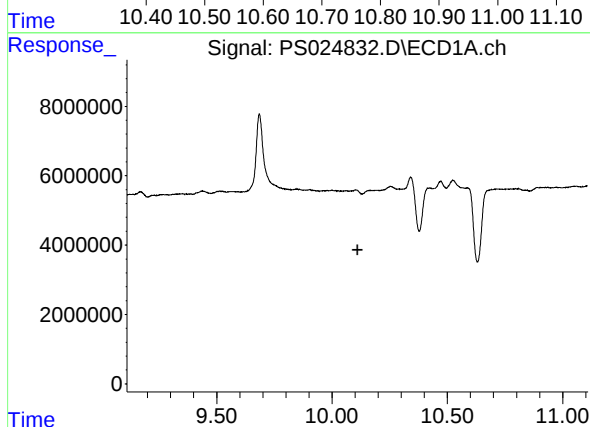

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.111 min
Response: 0
Conc: N.D.

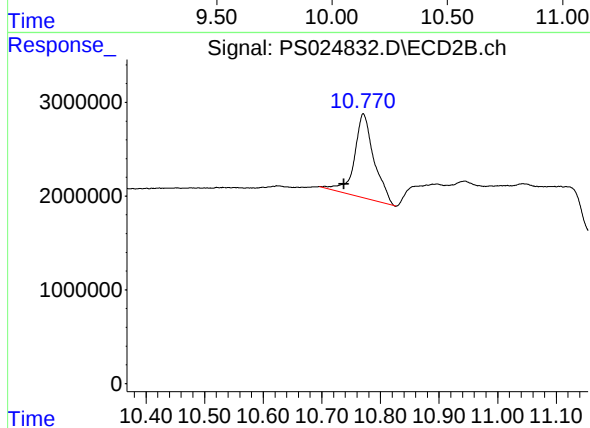

#16 DCPA

R.T.: 10.771 min
Delta R.T.: 0.033 min
Response: 20845937
Conc: 4.15 ng/ml