

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111523\
 Data File : PS024833.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2023 08:28
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 23:57:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 03 15:07:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.357	6.774	1027.7E6	338.7E6	503.391	502.019
Target Compounds						
1) T Dalapon	0.000	2.570	0	2701343	N.D.	2.564
7) T MCPA	0.000	7.240	0	5689948	N.D.	1.846
8) T DICHLORPROP	0.000	7.566	0	1390807	N.D.	1.904
9) T 2,4-D	0.000	7.781f	0	568374	N.D.	<MDL
12) T 2,4,5-T	0.000	8.987	0	421188	N.D.	<MDL
15) T Picloram	9.686	10.771	39654668	11516766	2.229	1.895
16) T DCPA	0.000	10.771	0	11516766	N.D.	2.292



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111523\
Data File : PS024833.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2023 08:28
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 23:57:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
Quant Title : 8080.M
QLast Update : Fri Nov 03 15:07:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

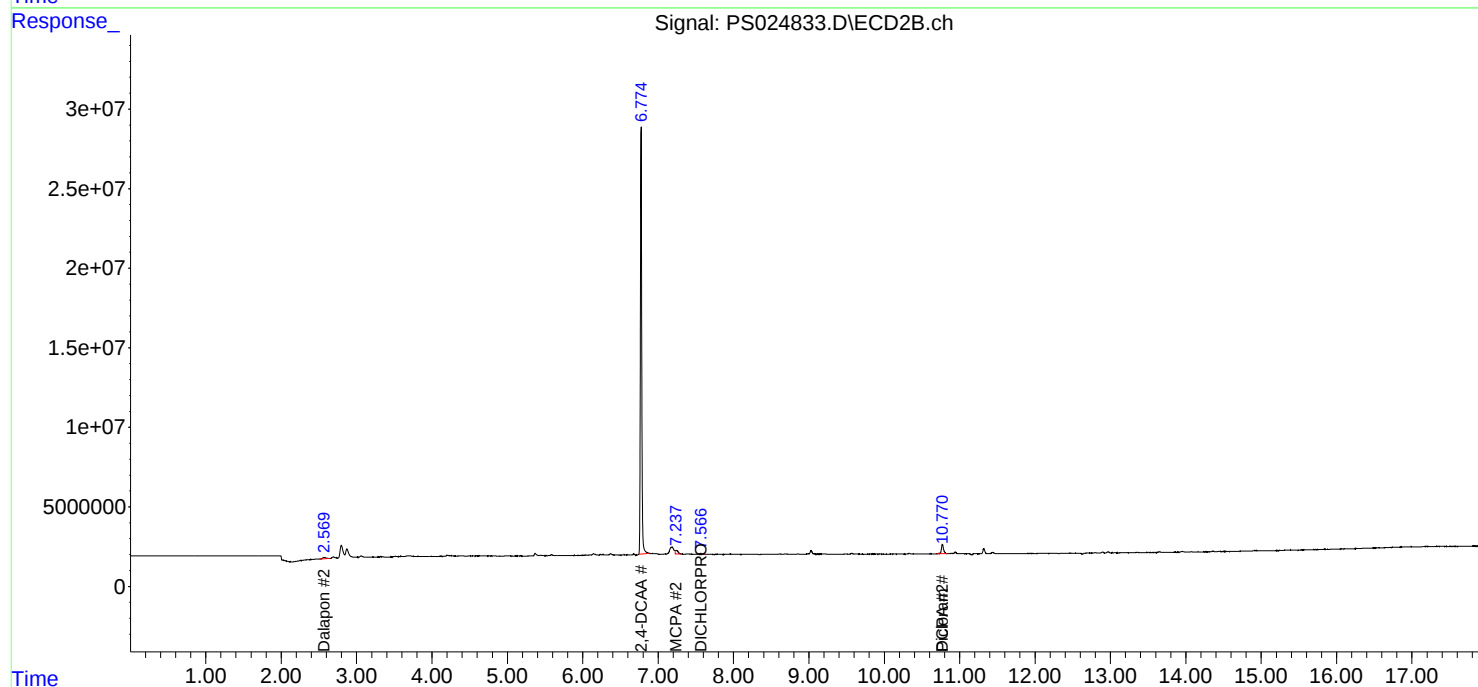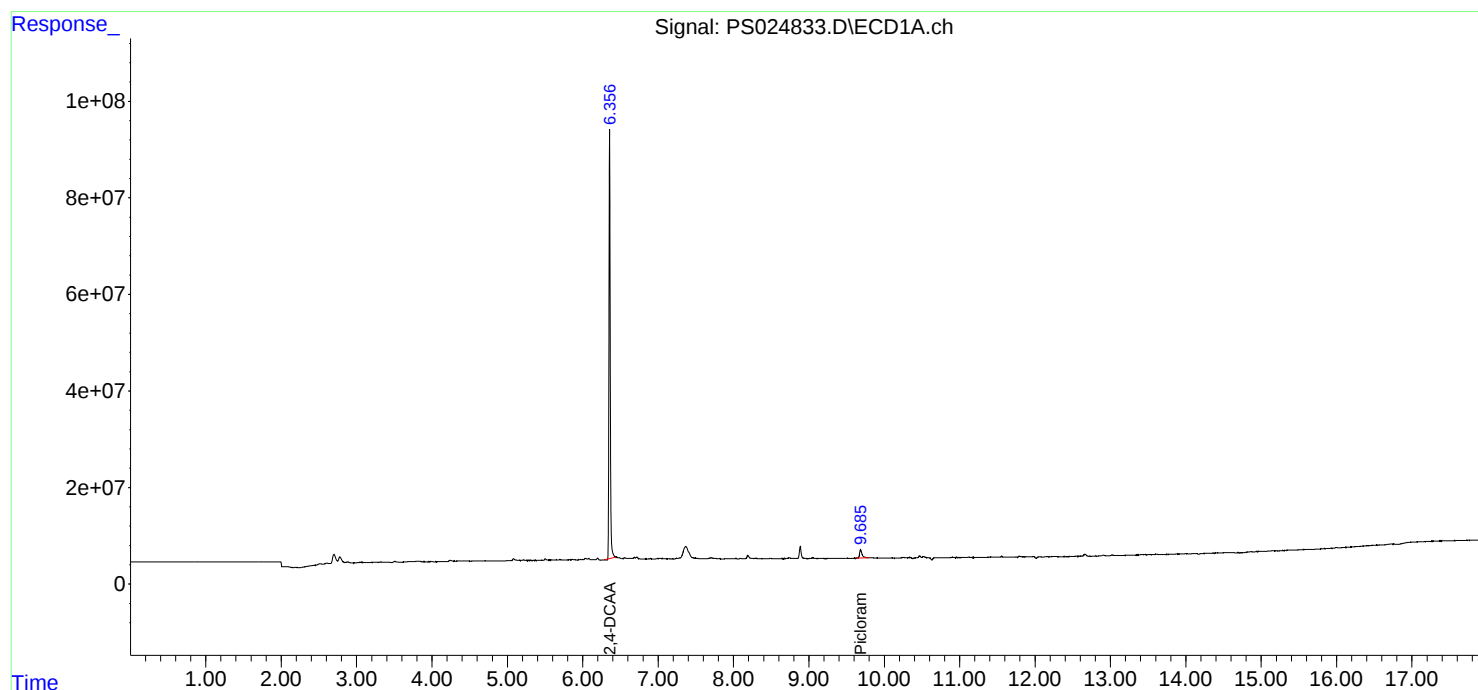


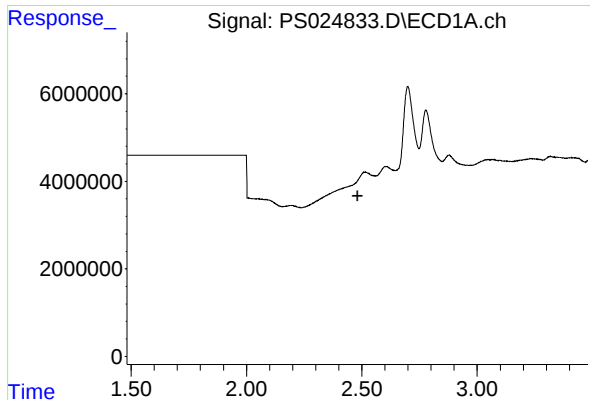

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.481 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

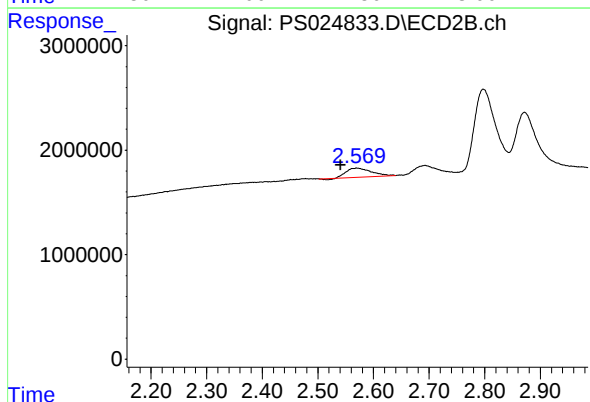


#1 Dalapon

R.T.: 2.570 min
Delta R.T.: 0.029 min
Response: 2701343
Conc: 2.56 ng/ml

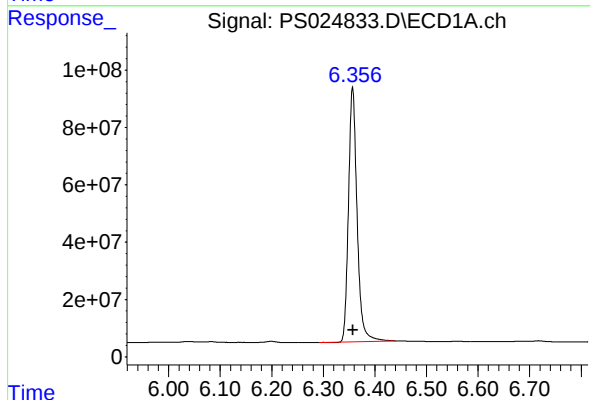


#4 2,4-DCAA

R.T.: 6.357 min
Delta R.T.: 0.000 min
Response: 1027673691
Conc: 503.39 ng/ml

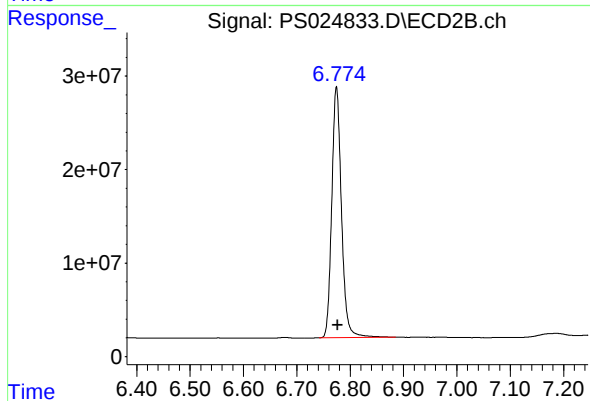

#4 2,4-DCAA


R.T.: 6.774 min
Delta R.T.: -0.002 min
Response: 338661184
Conc: 502.02 ng/ml

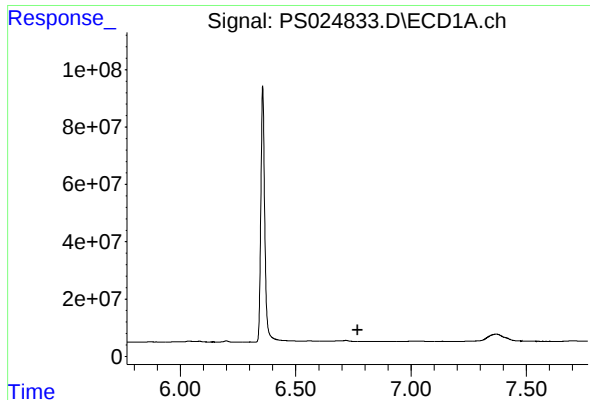

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.768 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

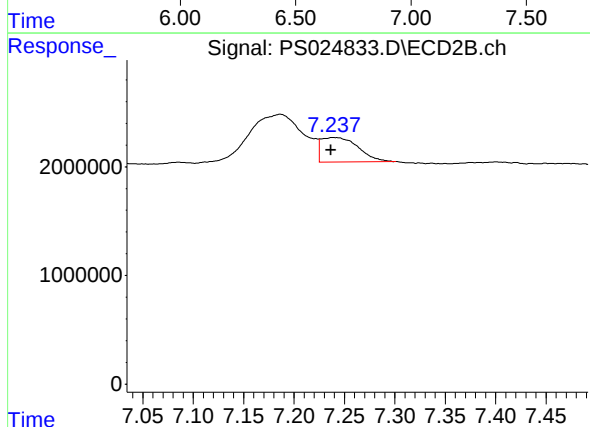


#7 MCPA

R.T.: 7.240 min
Delta R.T.: 0.004 min
Response: 5689948
Conc: 1.85 ug/ml

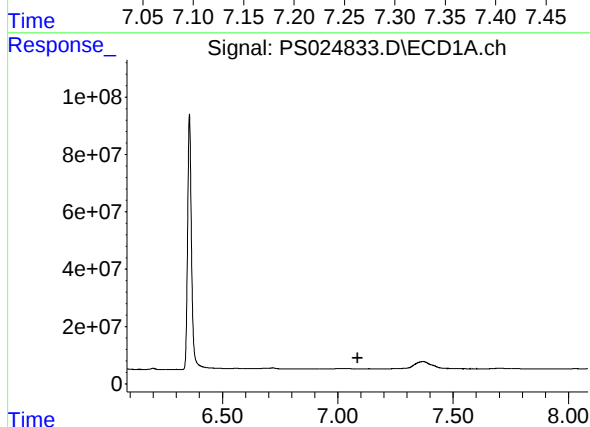


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.085 min
Response: 0
Conc: N.D.

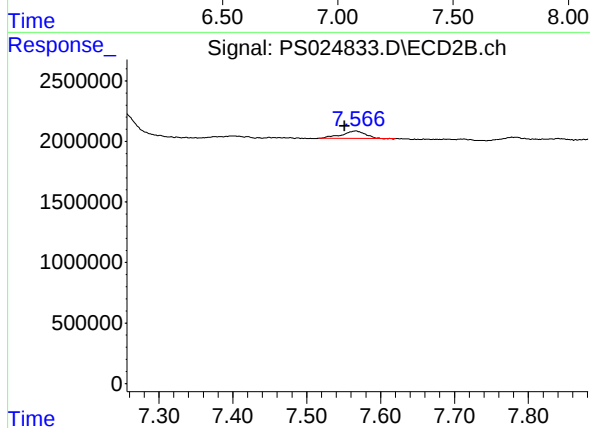

#8 DICHLORPROP


R.T.: 7.566 min
Delta R.T.: 0.015 min
Response: 1390807
Conc: 1.90 ng/ml

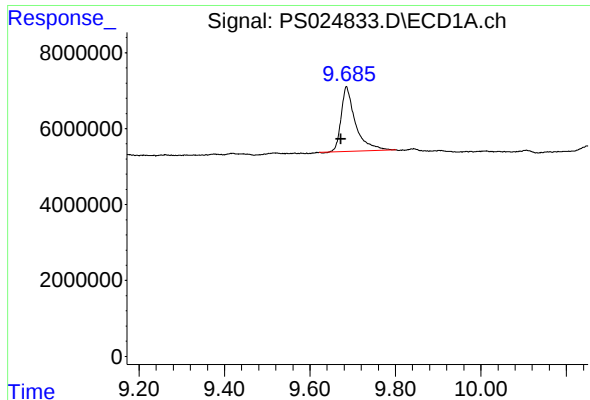

#15 Picloram


R.T.: 9.686 min
Delta R.T.: 0.013 min
Response: 39654668
Conc: 2.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

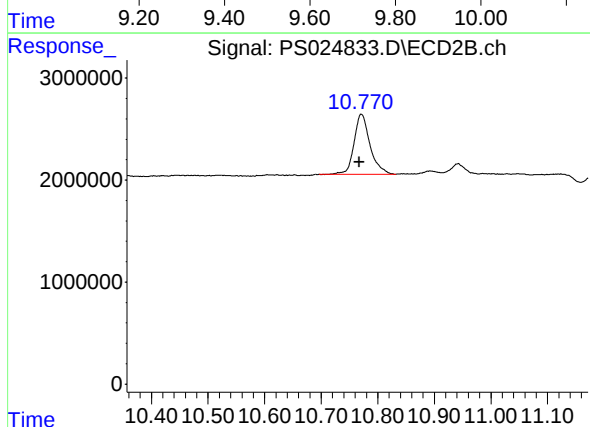


#15 Picloram

R.T.: 10.771 min
Delta R.T.: 0.004 min
Response: 11516766
Conc: 1.90 ng/ml

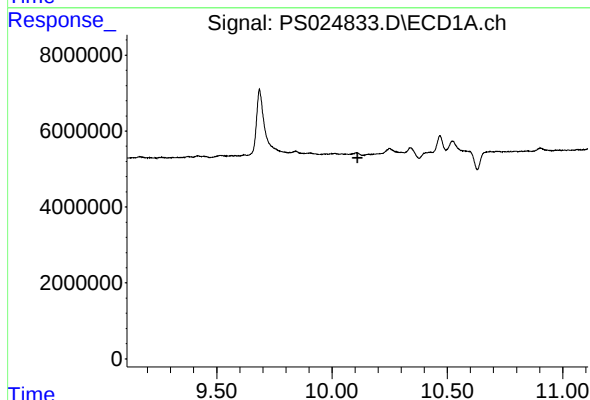

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.111 min
Response: 0
Conc: N.D.

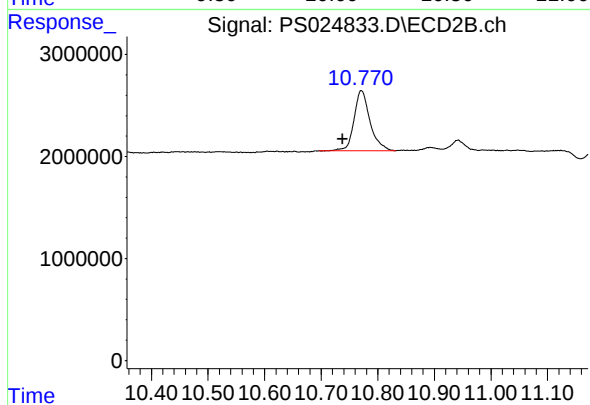

#16 DCPA

R.T.: 10.771 min
Delta R.T.: 0.033 min
Response: 11516766
Conc: 2.29 ng/ml