

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111523\
 Data File : PS024836.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2023 11:25
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 15 23:57:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 03 15:07:01 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.357	6.774	1022.8E6	337.9E6	501.015	500.904
Target Compounds						
1) T Dalapon	0.000	2.568	0	3128313	N.D.	2.969
3) T 4-Nitroph...	0.000	6.370	0	847311	N.D.	1.930
7) T MCPA	0.000	7.176f	0	26966407	N.D.	8.747
8) T DICHLORPROP	0.000	7.564	0	1619372	N.D.	2.217
9) T 2,4-D	0.000	7.782f	0	65209	N.D.	<MDL
11) T 2,4,5-TP ...	0.000	8.612	0	488497	N.D.	<MDL
12) T 2,4,5-T	0.000	8.992	0	515175	N.D.	<MDL
15) T Picloram	9.688	10.772	22735698	7650260	1.278	1.259
16) T DCPA	0.000	10.772	0	7650260	N.D.	1.522



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111523\
Data File : PS024836.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2023 11:25
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 15 23:57:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110323.M
Quant Title : 8080.M
QLast Update : Fri Nov 03 15:07:01 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

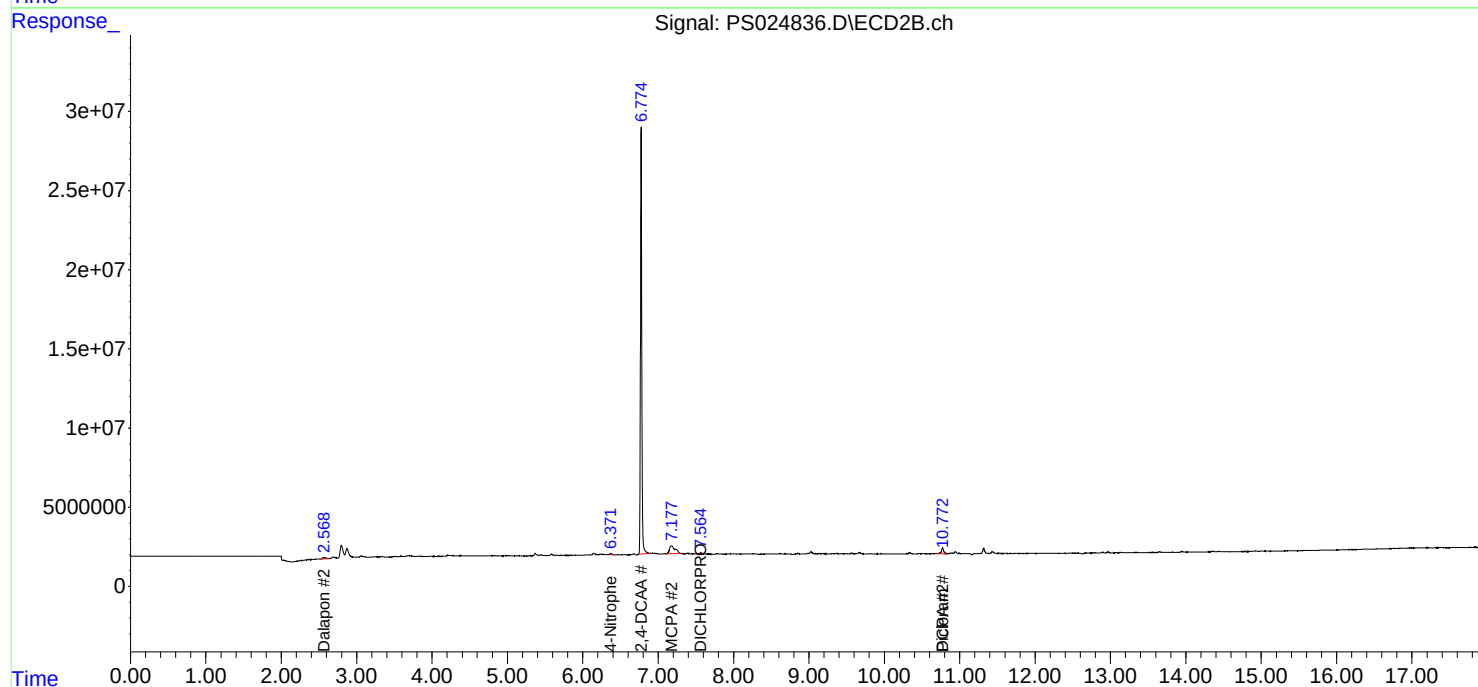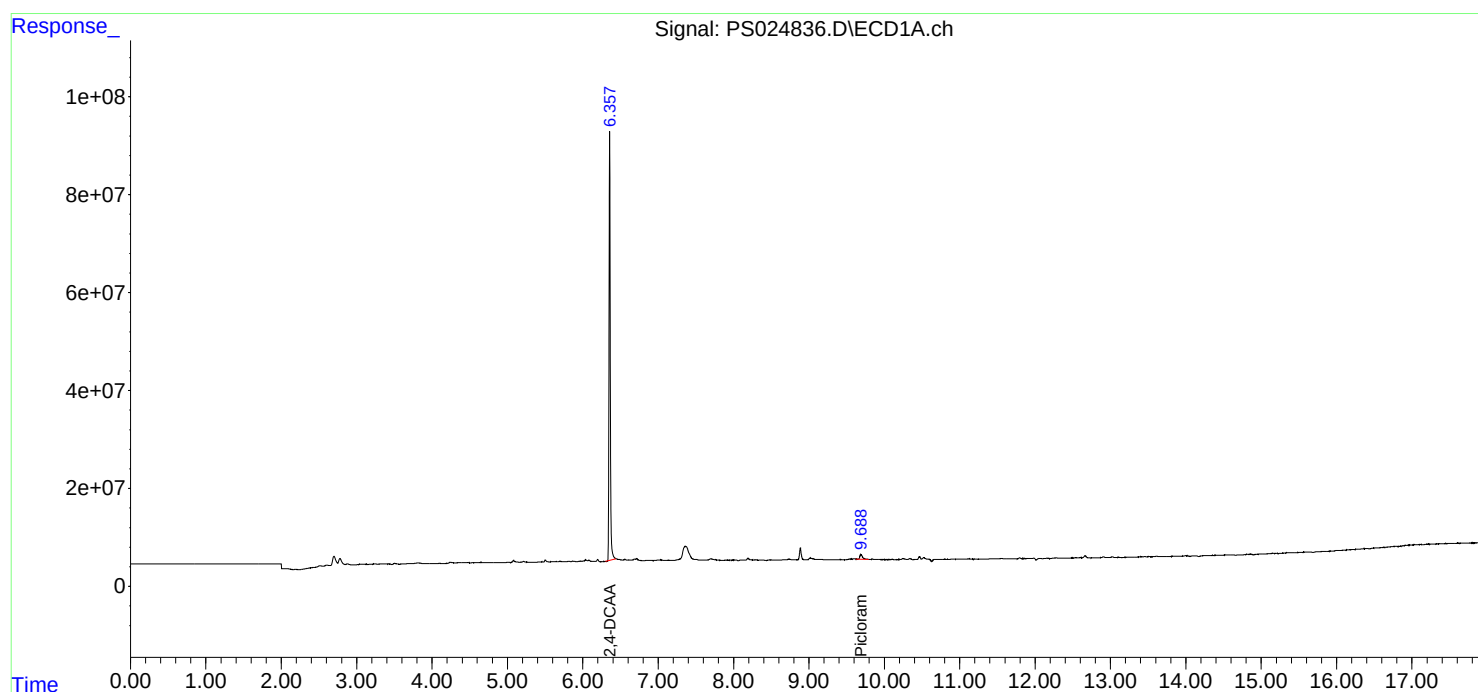


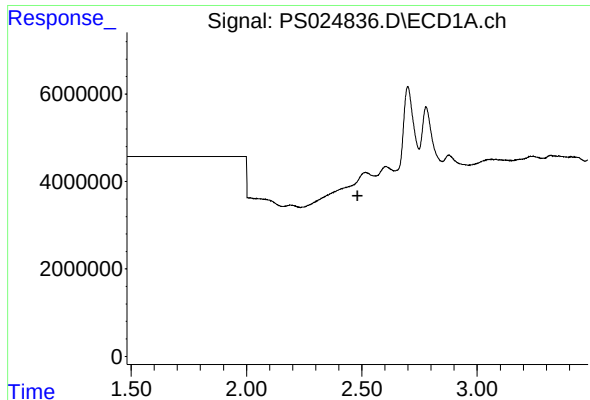

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.481 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

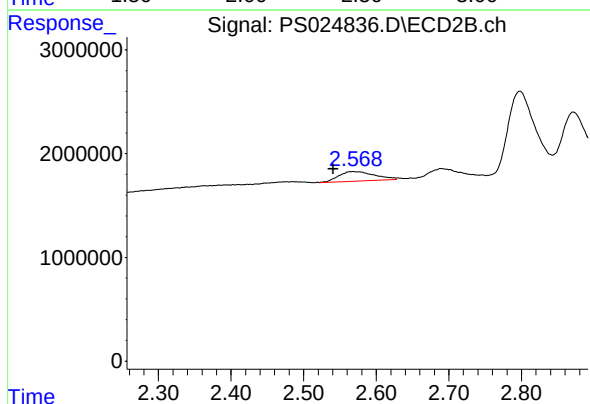


#1 Dalapon

R.T.: 2.568 min
Delta R.T.: 0.028 min
Response: 3128313
Conc: 2.97 ng/ml

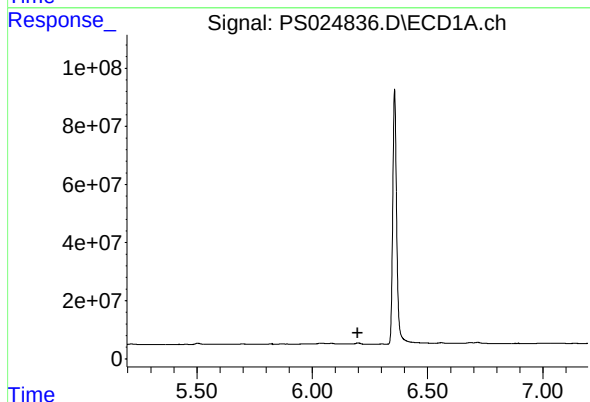


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.196 min
Response: 0
Conc: N.D.

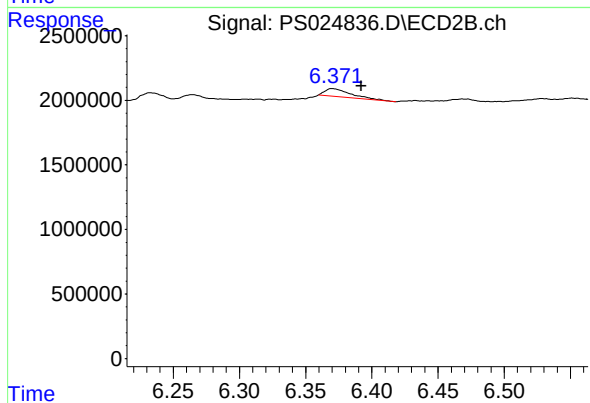

#3 4-Nitrophenol


R.T.: 6.370 min
Delta R.T.: -0.022 min
Response: 847311
Conc: 1.93 ng/ml

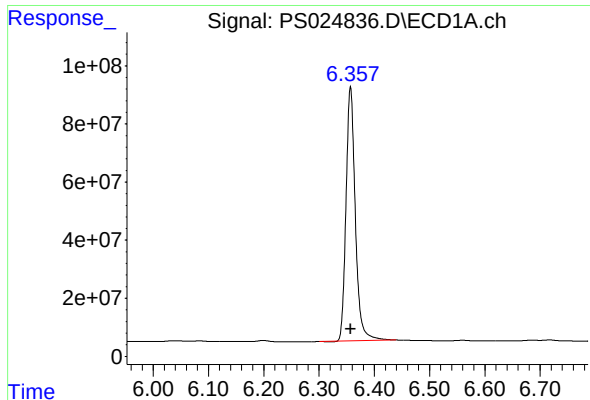

#4 2,4-DCAA


R.T.: 6.357 min
Delta R.T.: 0.000 min
Response: 1022822488
Conc: 501.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

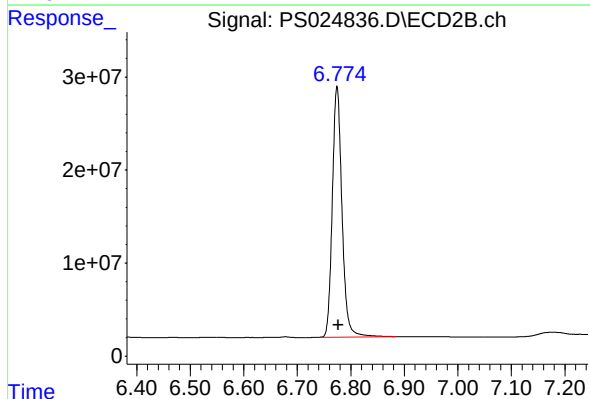


#4 2,4-DCAA

R.T.: 6.774 min
Delta R.T.: -0.002 min
Response: 337909551
Conc: 500.90 ng/ml

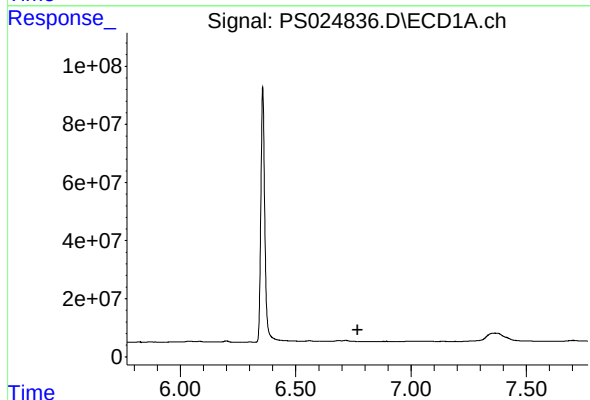


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.768 min
Response: 0
Conc: N.D.

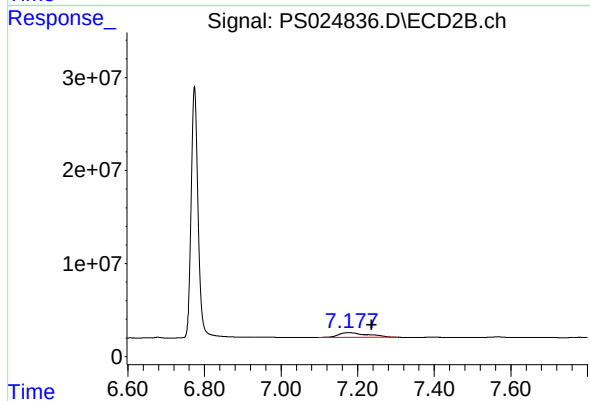

#7 MCPA


R.T.: 7.176 min
Delta R.T.: -0.061 min
Response: 26966407
Conc: 8.75 ug/ml

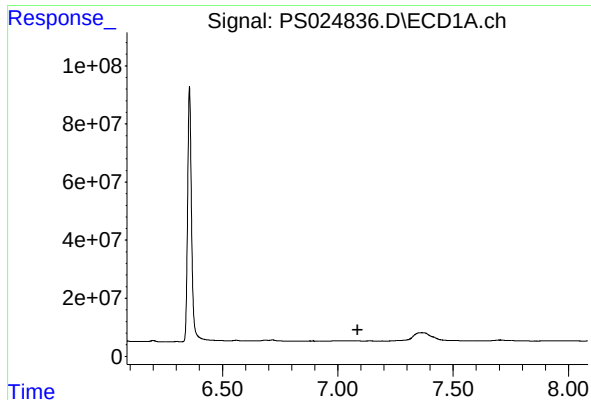

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.085 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

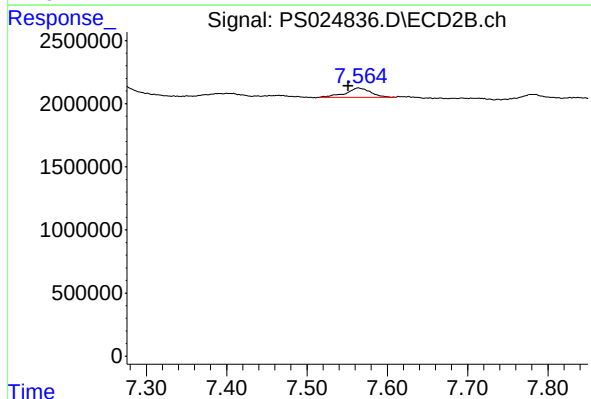


#8 DICHLORPROP

R.T.: 7.564 min
Delta R.T.: 0.013 min
Response: 1619372
Conc: 2.22 ng/ml

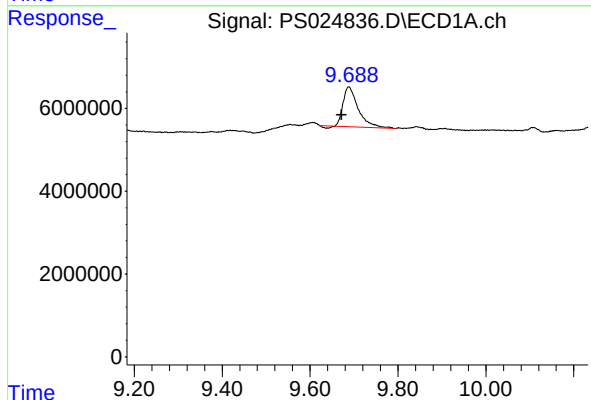


#15 Picloram

R.T.: 9.688 min
Delta R.T.: 0.016 min
Response: 22735698
Conc: 1.28 ng/ml

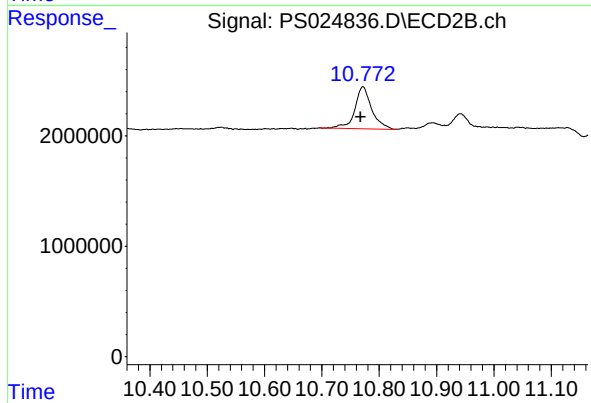

#15 Picloram


R.T.: 10.772 min
Delta R.T.: 0.004 min
Response: 7650260
Conc: 1.26 ng/ml

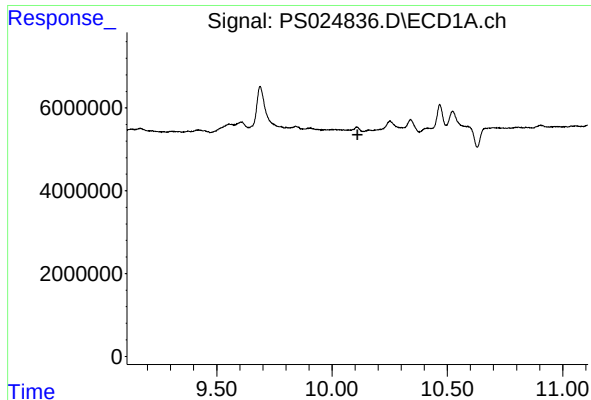

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.111 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

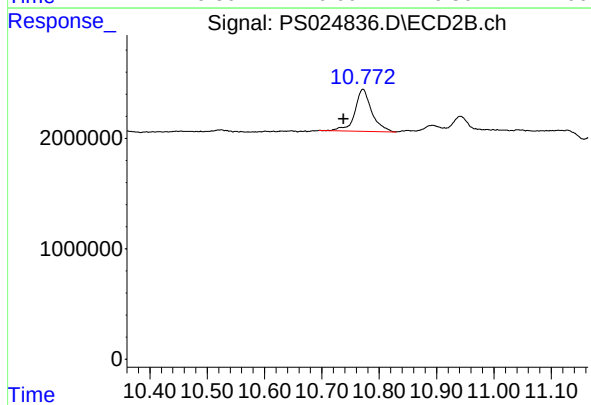

#16 DCPA

R.T.: 10.772 min
Delta R.T.: 0.034 min
Response: 7650260
Conc: 1.52 ng/ml