

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111622\
 Data File : PS021173.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Nov 2022 17:16
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 01:20:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
 Quant Title : 8080.M
 QLast Update : Thu Nov 17 00:46:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.409	6.844	1033.9E6	812.1E6	475.495	537.073
Target Compounds							
1) T	Dalapon	2.461	0.000	33865	0	<MDL	N.D. #
3) T	4-Nitroph...	6.251	0.000	6312160	0	4.672	N.D. #
6) T	MCP	0.000	7.158f	0	3628030	N.D.	<MDL
7) T	MCPA	6.789f	0.000	4536782	0	<MDL	N.D. #
8) T	DICHLORPROP	7.170	7.689f	272608	408734	<MDL	<MDL #
10) T	Pentachlo...	7.579	0.000	1383774	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.114	0.000	1325662	0	<MDL	N.D. #
12) T	2,4,5-T	8.335	0.000	10577399	0	<MDL	N.D. #
13) T	2,4-DB	8.859	9.544f	4772577	9381366	2.088	8.014 #
14) T	DINOSEB	9.876f	0.000	17980982	0	1.568	N.D. #
15) T	Picloram	9.767	0.000	336398	0	<MDL	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111622\
Data File : PS021173.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Nov 2022 17:16
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 01:20:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
Quant Title : 8080.M
QLast Update : Thu Nov 17 00:46:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

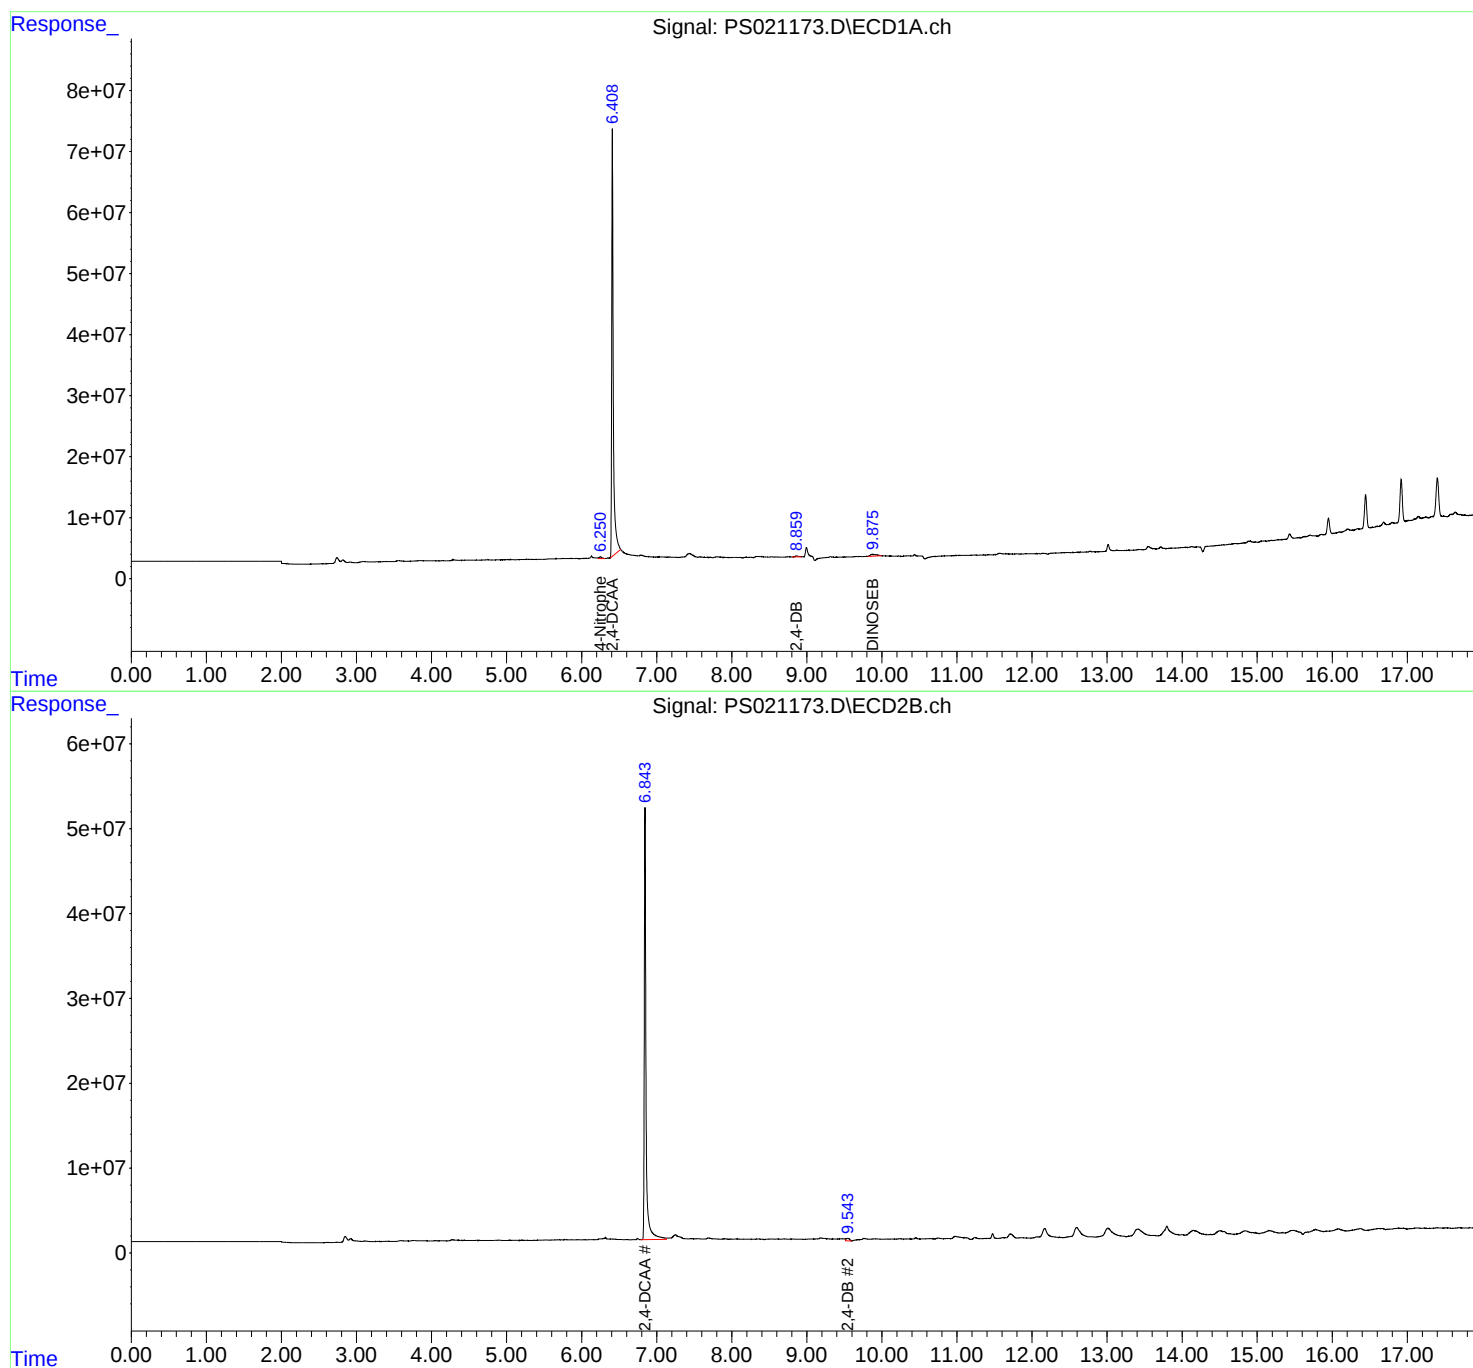


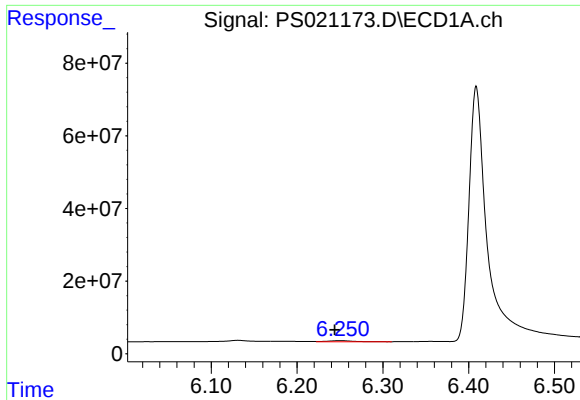

#3 4-Nitrophenol


R.T.: 6.251 min
Delta R.T.: 0.007 min
Response: 6312160
Conc: 4.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

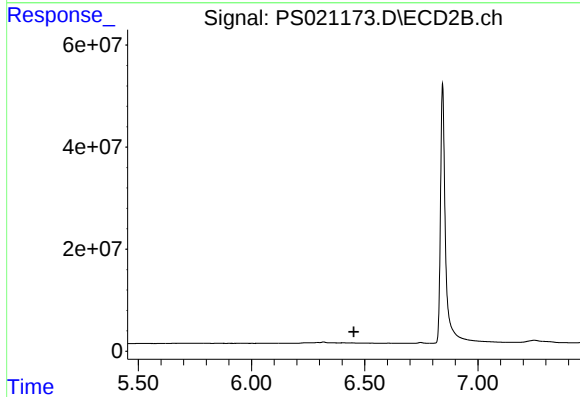


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.452 min
Response: 0
Conc: N.D.

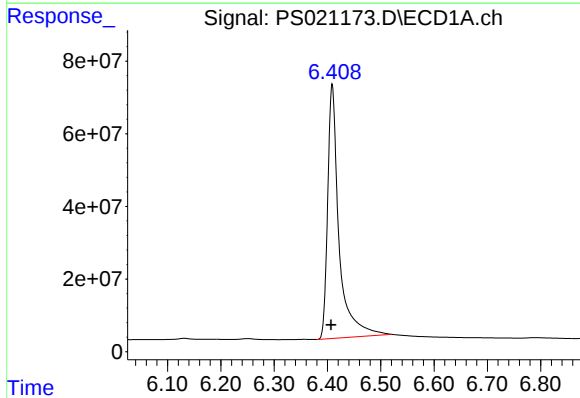


#4 2,4-DCAA

R.T.: 6.409 min
Delta R.T.: 0.002 min
Response: 1033866784
Conc: 475.50 ng/ml

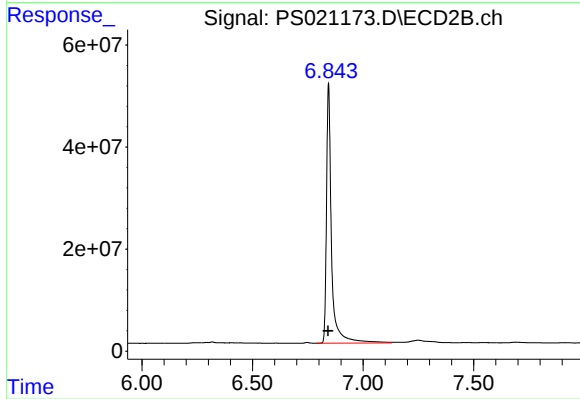

#4 2,4-DCAA


R.T.: 6.844 min
Delta R.T.: 0.002 min
Response: 812118011
Conc: 537.07 ng/ml

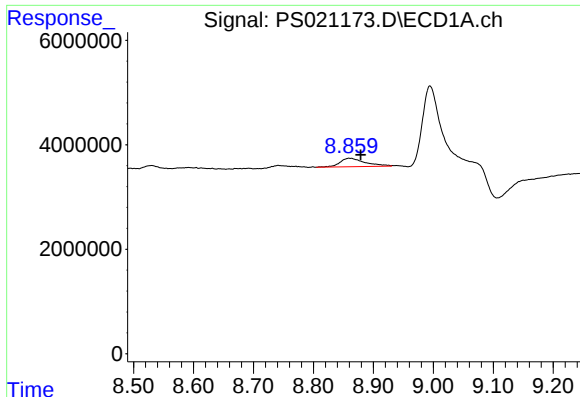

#13 2,4-DB


R.T.: 8.859 min
Delta R.T.: -0.019 min
Response: 4772577
Conc: 2.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

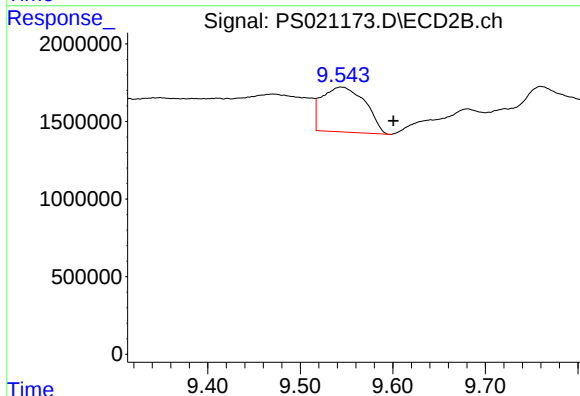


#13 2,4-DB

R.T.: 9.544 min
Delta R.T.: -0.057 min
Response: 9381366
Conc: 8.01 ng/ml

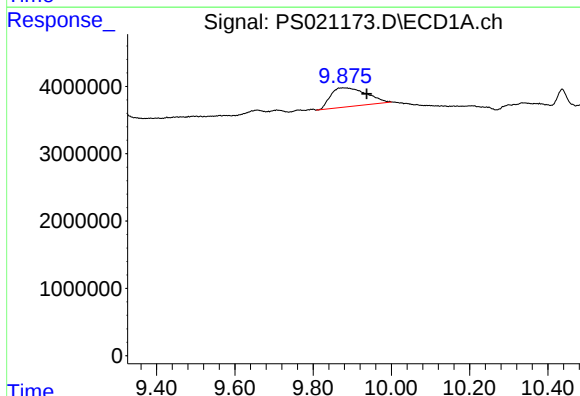

#14 DINOSEB

R.T.: 9.876 min
Delta R.T.: -0.061 min
Response: 17980982
Conc: 1.57 ng/ml

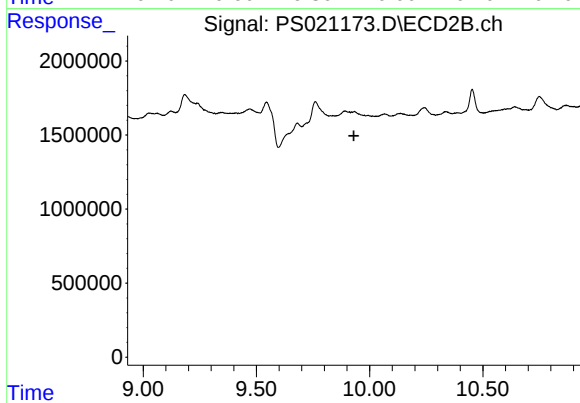

#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.930 min
Response: 0
Conc: N.D.