

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111819\
 Data File : PS007708.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2019 12:07
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 04:01:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
3) T	4-Nitroph...	0.000	4.881	0	55555095	N.D. 135.008
12) T	2,4,5-T	0.000	7.196	0	33085415	N.D. 8.959
15) T	Picloram	8.941	8.888	202.9E6	122.9E6	18.274 20.979
16) T	DCPA	0.000	8.888	0	122.9E6	N.D. 23.524



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111819\
Data File : PS007708.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2019 12:07
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 04:01:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

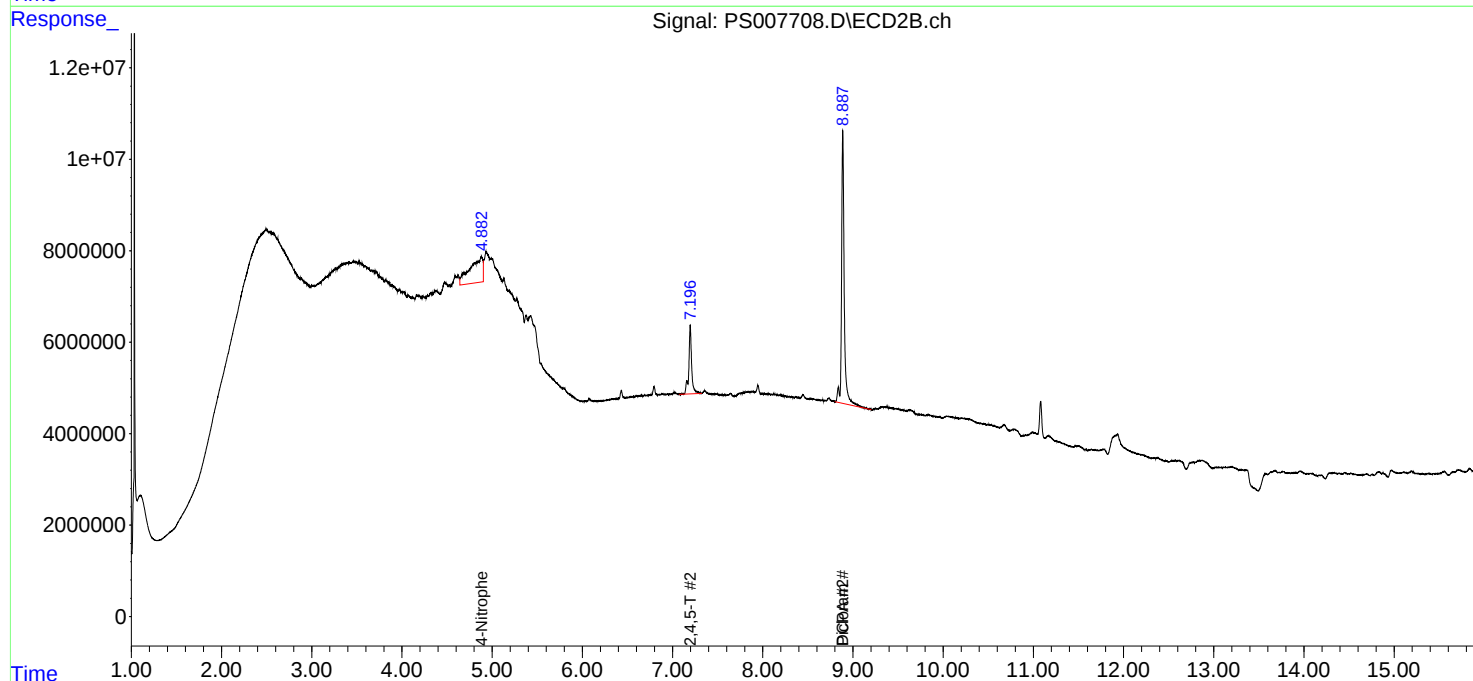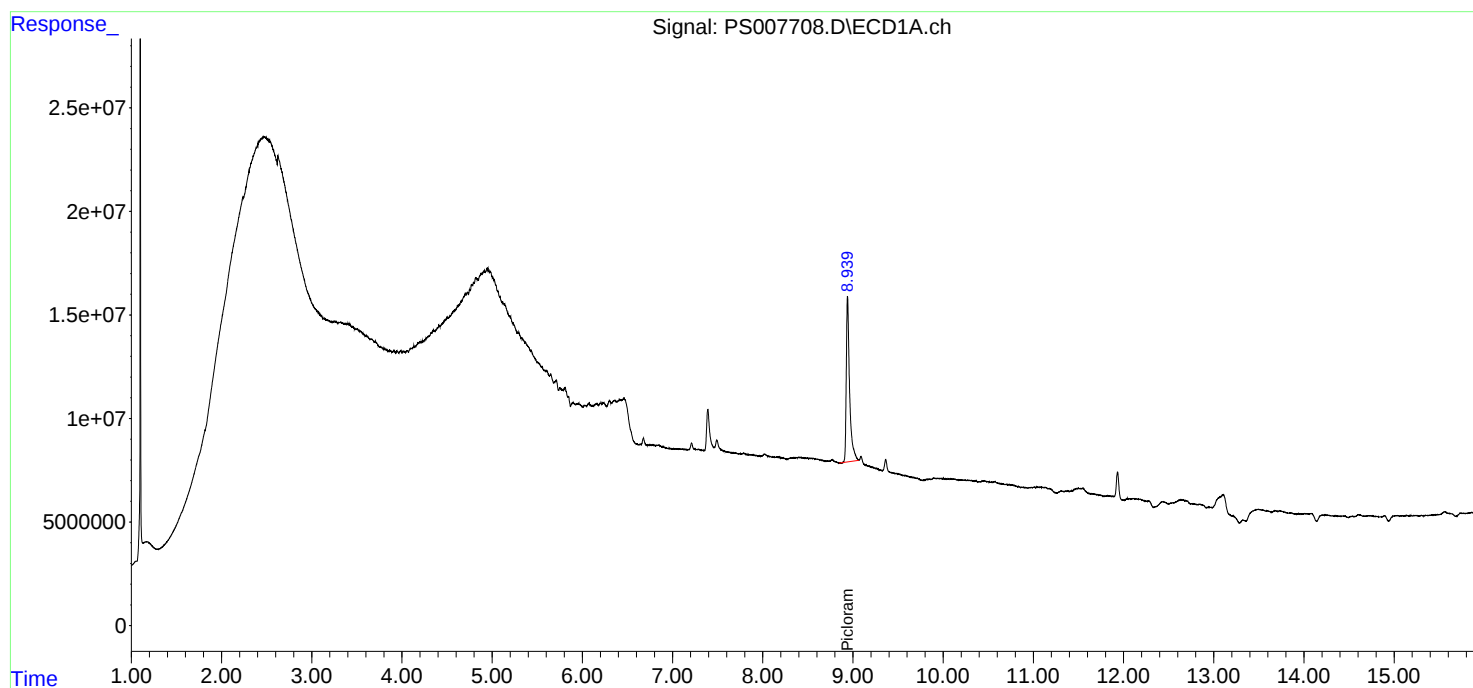


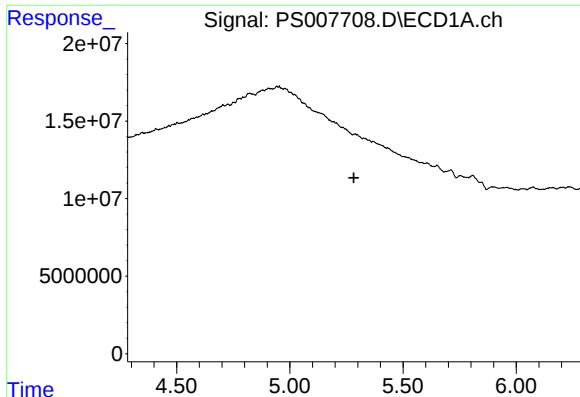

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

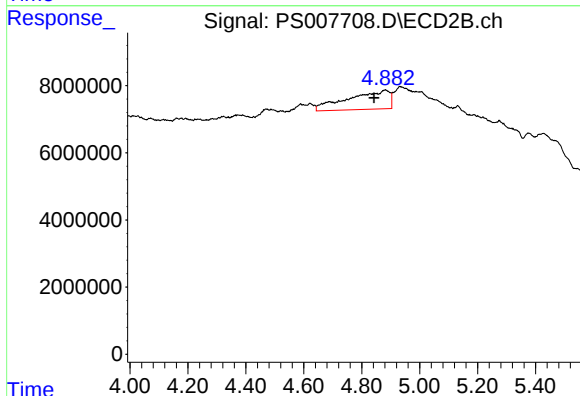


#3 4-Nitrophenol

R.T.: 4.881 min
Delta R.T.: 0.038 min
Response: 55555095
Conc: 135.01 ng/ml

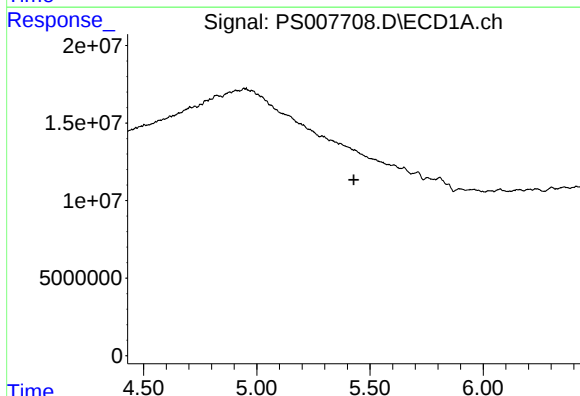


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 5.428 min
Response: 0
Conc: N.D.

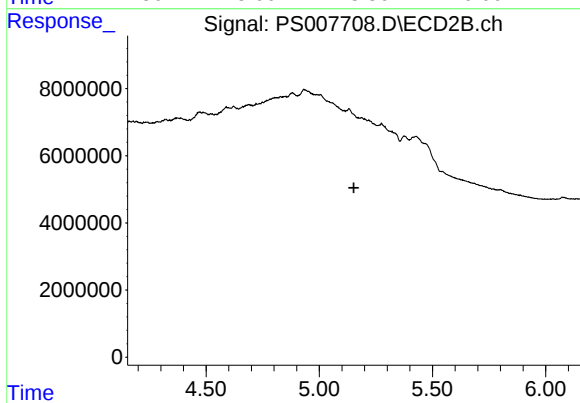

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 5.153 min
Response: 0
Conc: N.D.

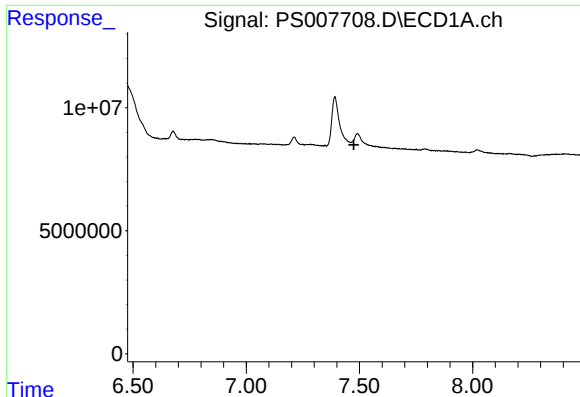

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.475 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

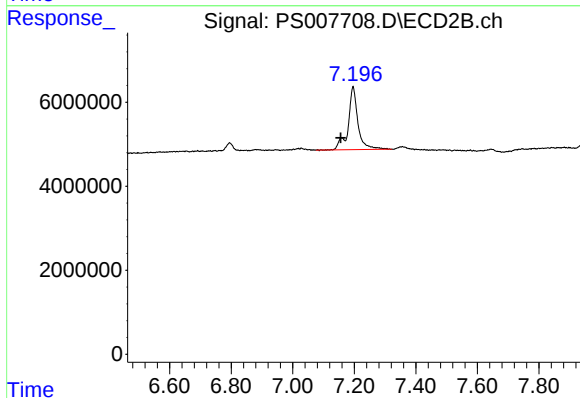


#12 2,4,5-T

R.T.: 7.196 min
Delta R.T.: 0.041 min
Response: 33085415
Conc: 8.96 ng/ml

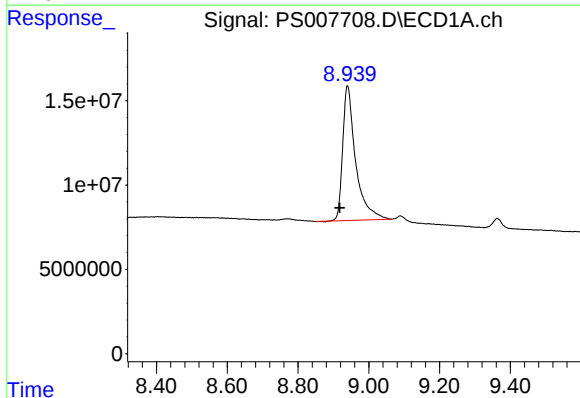


#15 Picloram

R.T.: 8.941 min
Delta R.T.: 0.023 min
Response: 202897369
Conc: 18.27 ng/ml

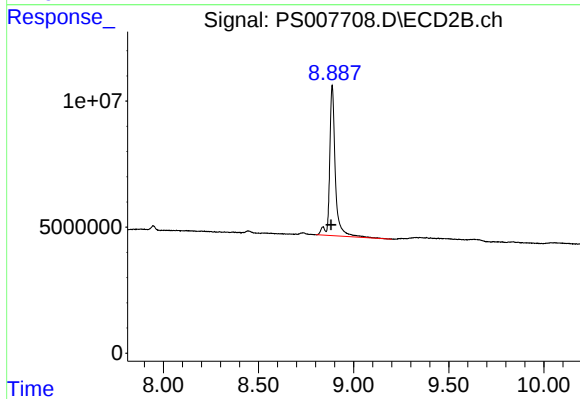

#15 Picloram


R.T.: 8.888 min
Delta R.T.: 0.006 min
Response: 122916595
Conc: 20.98 ng/ml

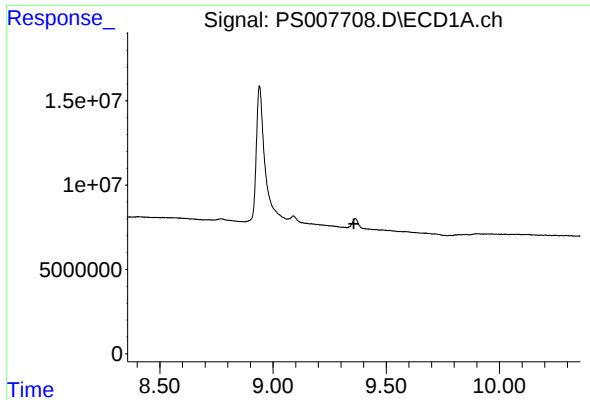

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.357 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

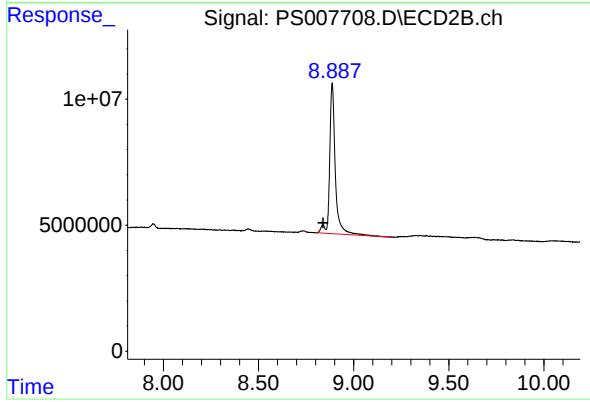

#16 DCPA

R.T.: 8.888 min
Delta R.T.: 0.048 min
Response: 122916595
Conc: 23.52 ng/ml