

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111819\
 Data File : PS007711.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2019 16:57
 Operator : SM\AJ
 Sample : PB124909BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB124909BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 04:02:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.431	5.154	589.0E6	315.4E6	427.687	448.868
Target Compounds							
1) T	Dalapon	1.991	1.698	77934846	198.4E6	43.077	167.051 #
2) T	3,5-DICHL...	0.000	4.489	0	37614288	N.D.	41.635
5) T	DICAMBA	5.521	0.000	44779292	0	8.802	N.D. #
7) T	MCPA	5.897	5.522	36769893	40734480	6.680	13.552 #
9) T	2,4-D	6.483	6.056	127.1E6	6293003	90.621	7.804 #
10) T	Pentachlo...	0.000	6.444	0	6898389	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.758	0	16625995	N.D.	4.246
15) T	Picloram	0.000	8.913	0	22264214	N.D.	3.800



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111819\
Data File : PS007711.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2019 16:57
Operator : SM\AJ
Sample : PB124909BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB124909BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 04:02:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

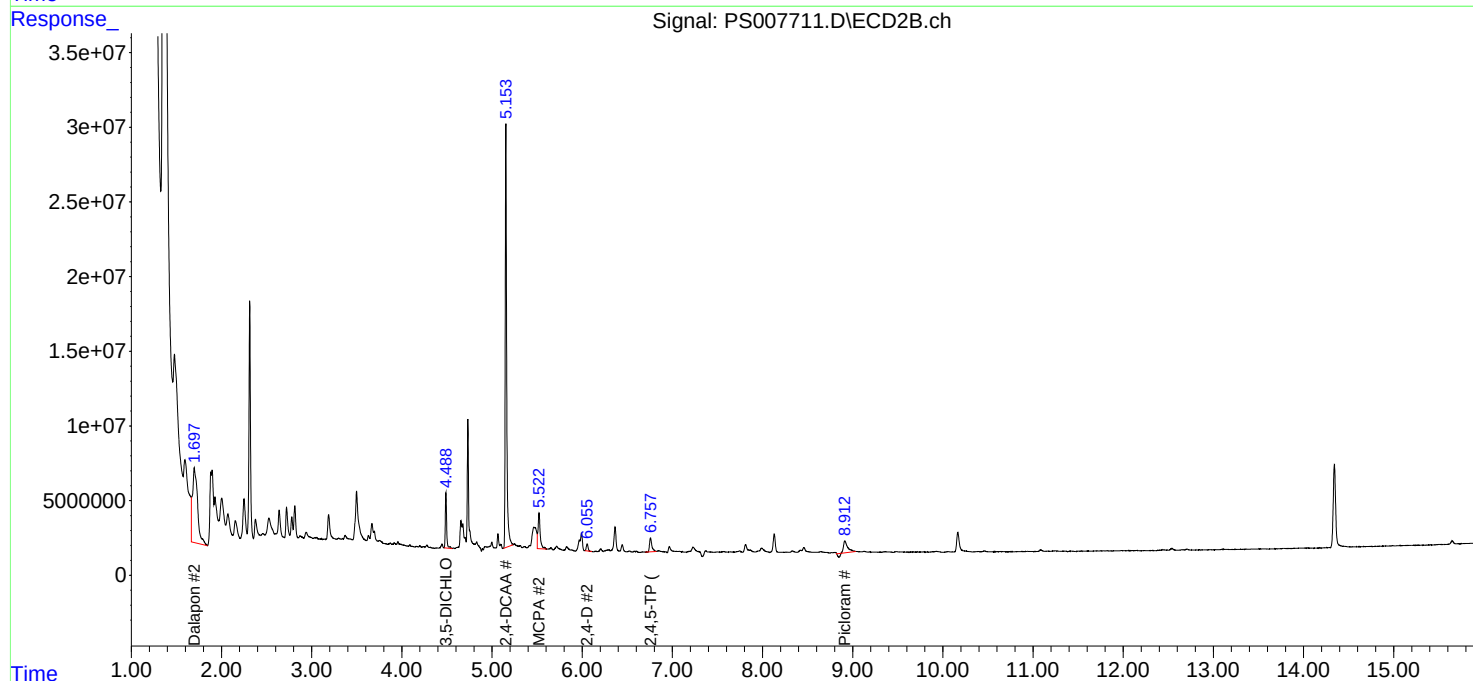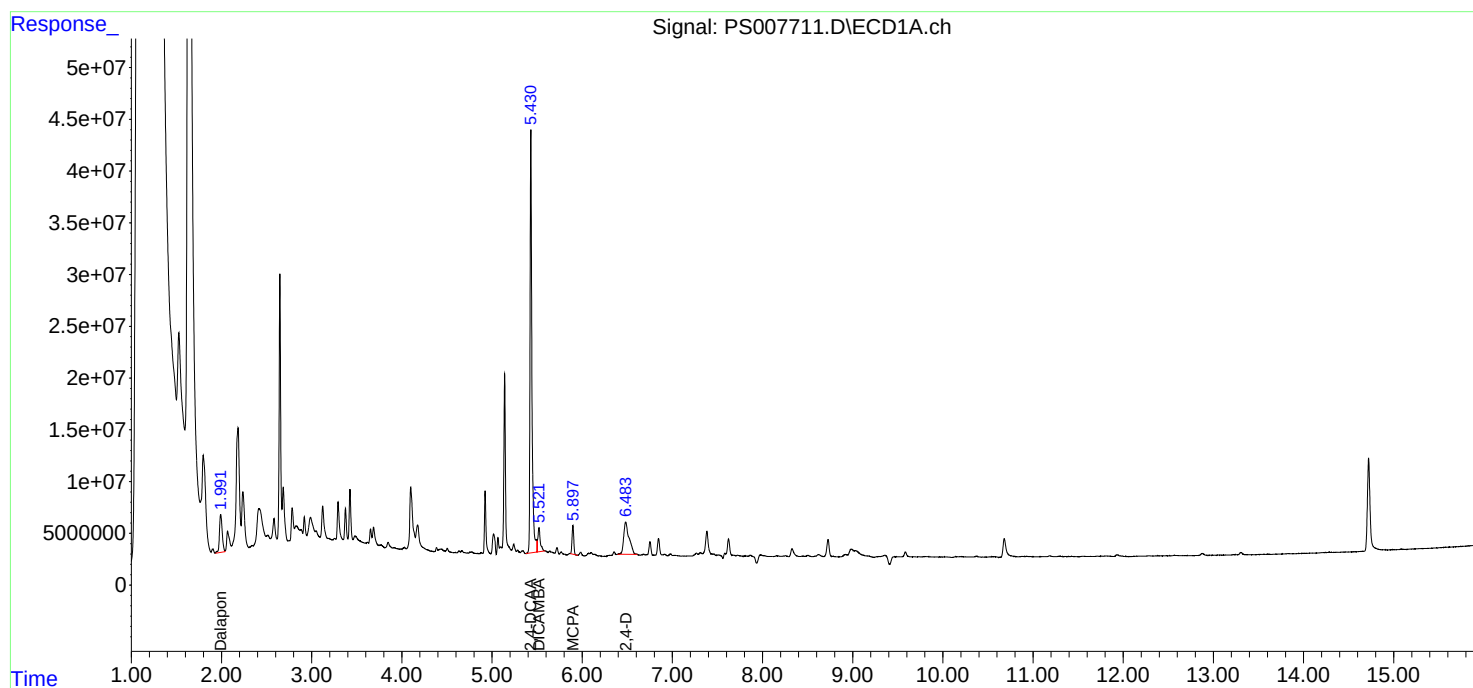


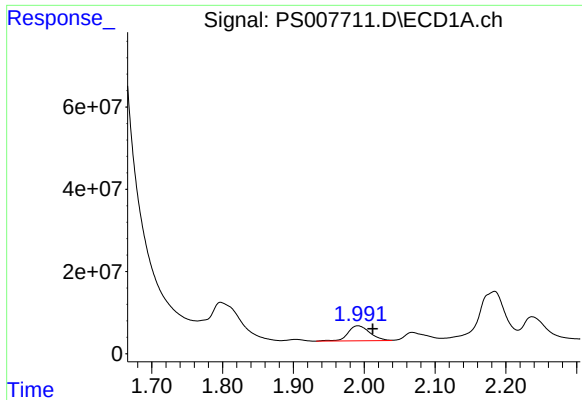

#1 Dalapon


R.T.: 1.991 min
Delta R.T.: -0.021 min
Response: 77934846
Conc: 43.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB124909BL

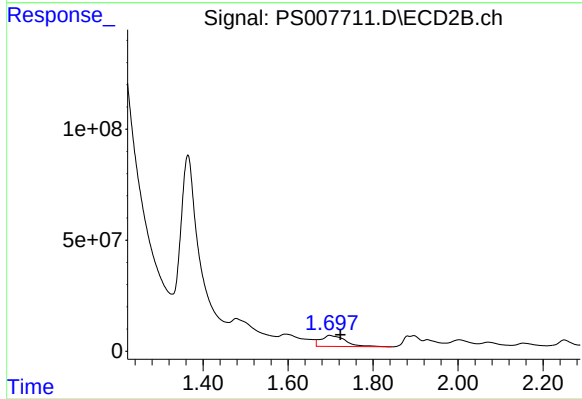


#1 Dalapon

R.T.: 1.698 min
Delta R.T.: -0.025 min
Response: 198357112
Conc: 167.05 ng/ml

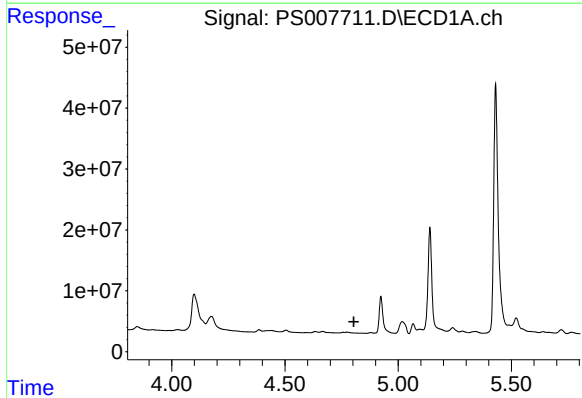


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

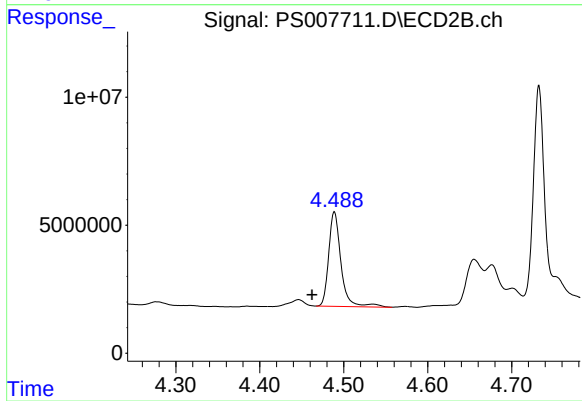

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.489 min
Delta R.T.: 0.027 min
Response: 37614288
Conc: 41.63 ng/ml

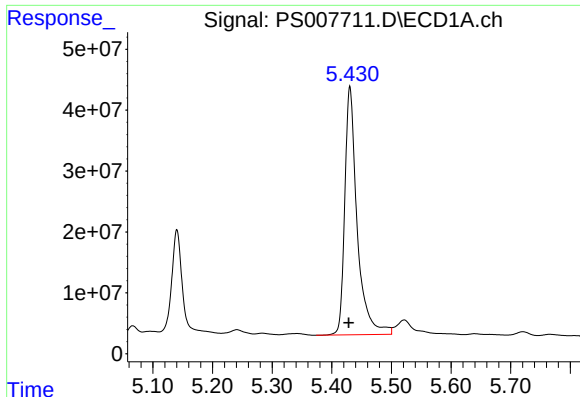

#4 2,4-DCAA


R.T.: 5.431 min
Delta R.T.: 0.002 min
Response: 589003887
Conc: 427.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB124909BL

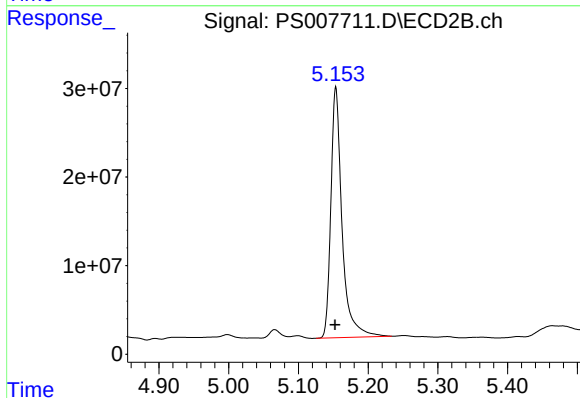


#4 2,4-DCAA

R.T.: 5.154 min
Delta R.T.: 0.001 min
Response: 315358428
Conc: 448.87 ng/ml

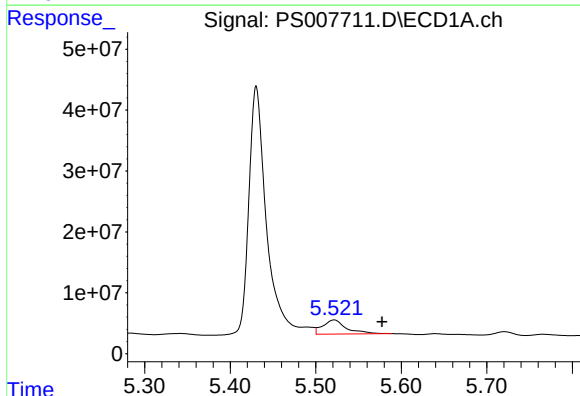


#5 DICAMBA

R.T.: 5.521 min
Delta R.T.: -0.056 min
Response: 44779292
Conc: 8.80 ng/ml

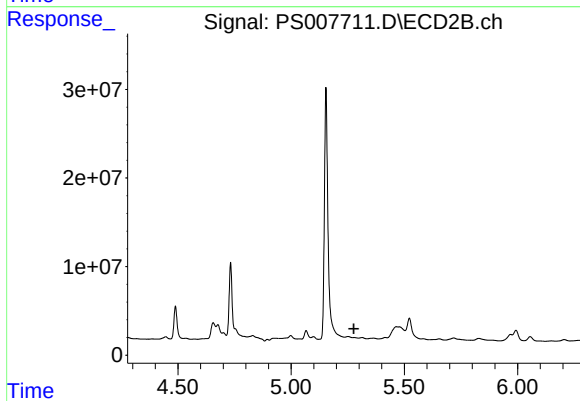

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.277 min
Response: 0
Conc: N.D.

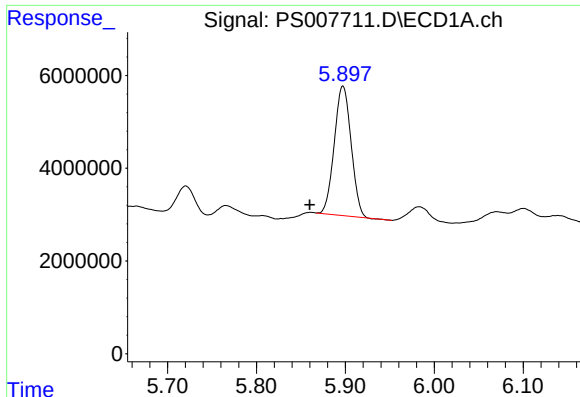

#7 MCPA


R.T.: 5.897 min
Delta R.T.: 0.037 min
Response: 36769893
Conc: 6.68 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB124909BL

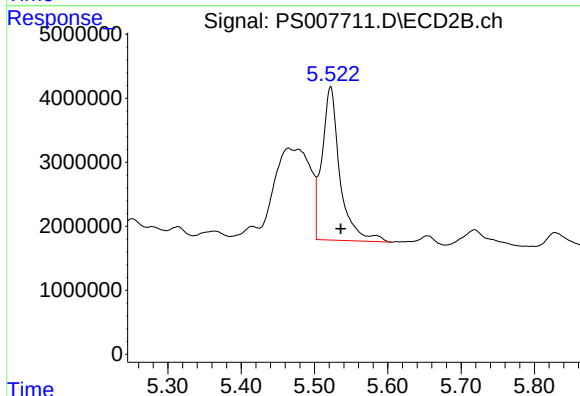


#7 MCPA

R.T.: 5.522 min
Delta R.T.: -0.014 min
Response: 40734480
Conc: 13.55 ug/ml

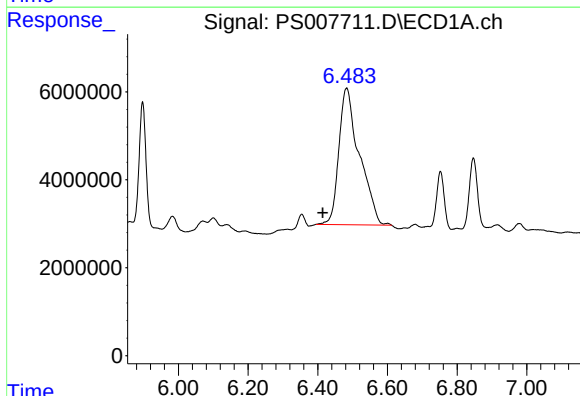


#9 2,4-D

R.T.: 6.483 min
Delta R.T.: 0.069 min
Response: 127099985
Conc: 90.62 ng/ml

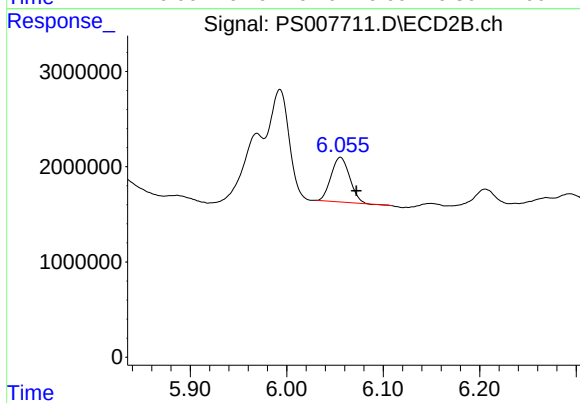

#9 2,4-D


R.T.: 6.056 min
Delta R.T.: -0.017 min
Response: 6293003
Conc: 7.80 ng/ml

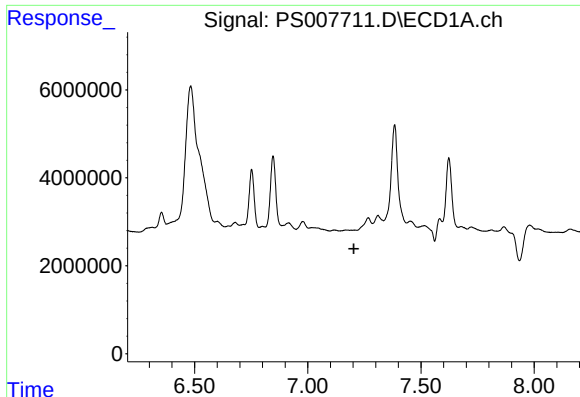

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB124909BL

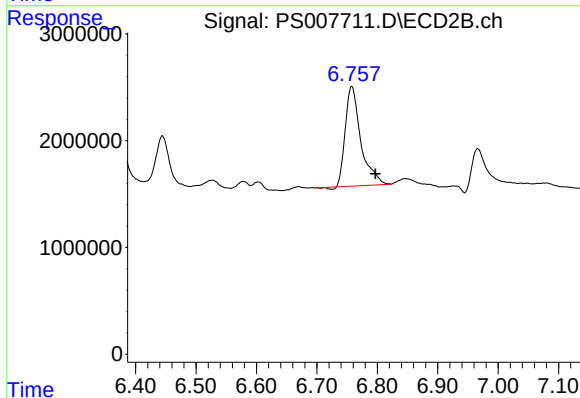


#11 2,4,5-TP (SILVEX)

R.T.: 6.758 min
Delta R.T.: -0.039 min
Response: 16625995
Conc: 4.25 ng/ml

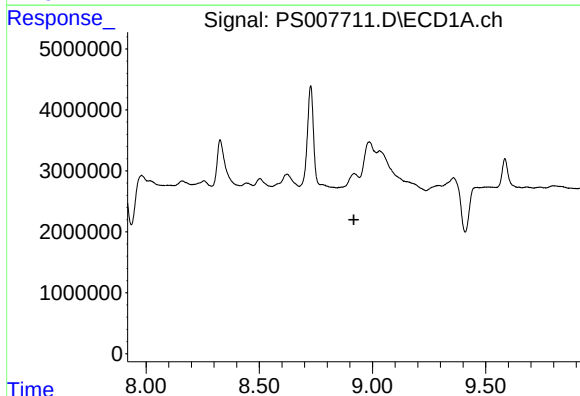

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.918 min
Response: 0
Conc: N.D.

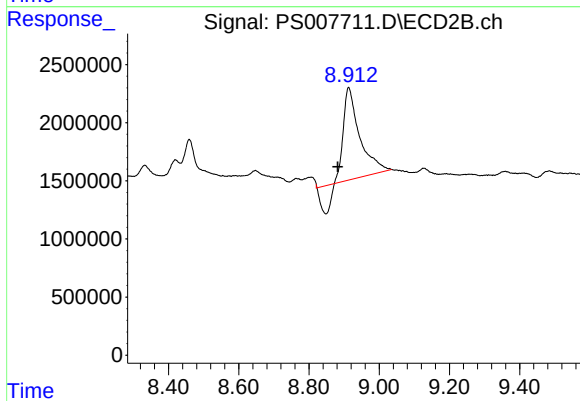

#15 Picloram

R.T.: 8.913 min
Delta R.T.: 0.031 min
Response: 22264214
Conc: 3.80 ng/ml