

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111819\
 Data File : PS007720.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2019 20:15
 Operator : SM\AJ
 Sample : K5782-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TP-2A-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 04:05:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.433	5.157	230.5E6	145.1E6	167.374	206.478
Target Compounds							
1) T	Dalapon	1.996	1.701	117.5E6	349.0E6	64.939	293.896 #
2) T	3,5-DICHL...	0.000	4.447	0	6171252	N.D.	6.831
3) T	4-Nitroph...	0.000	4.833	0	17352665	N.D.	42.170
7) T	MCPA	0.000	5.466	0	60173904	N.D.	20.020
9) T	2,4-D	6.483	6.057	113.9E6	6282664	81.176	7.791 #
10) T	Pentachlo...	0.000	6.366	0	16688149	N.D.	1.704
11) T	2,4,5-TP ...	0.000	6.756	0	17543296	N.D.	4.480



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111819\
Data File : PS007720.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2019 20:15
Operator : SM\AJ
Sample : K5782-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-2A-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 04:05:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

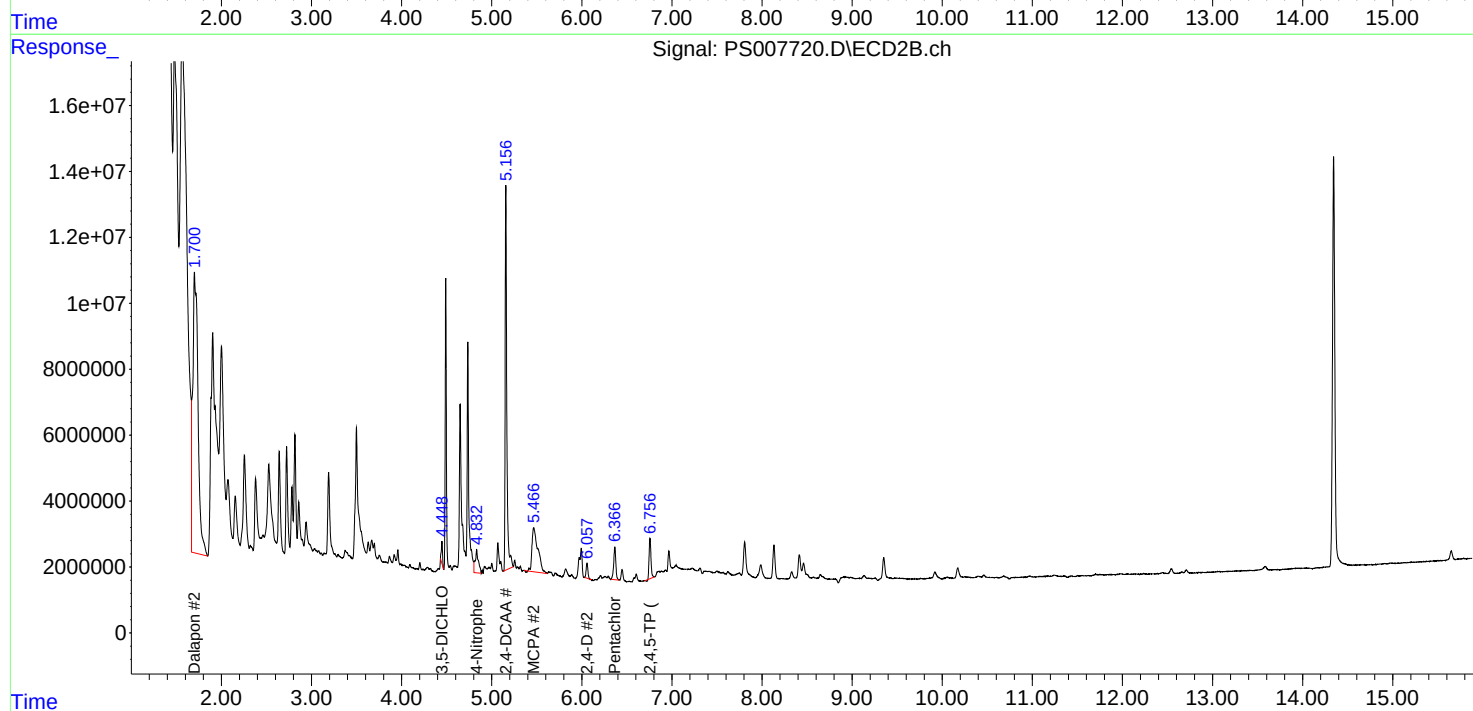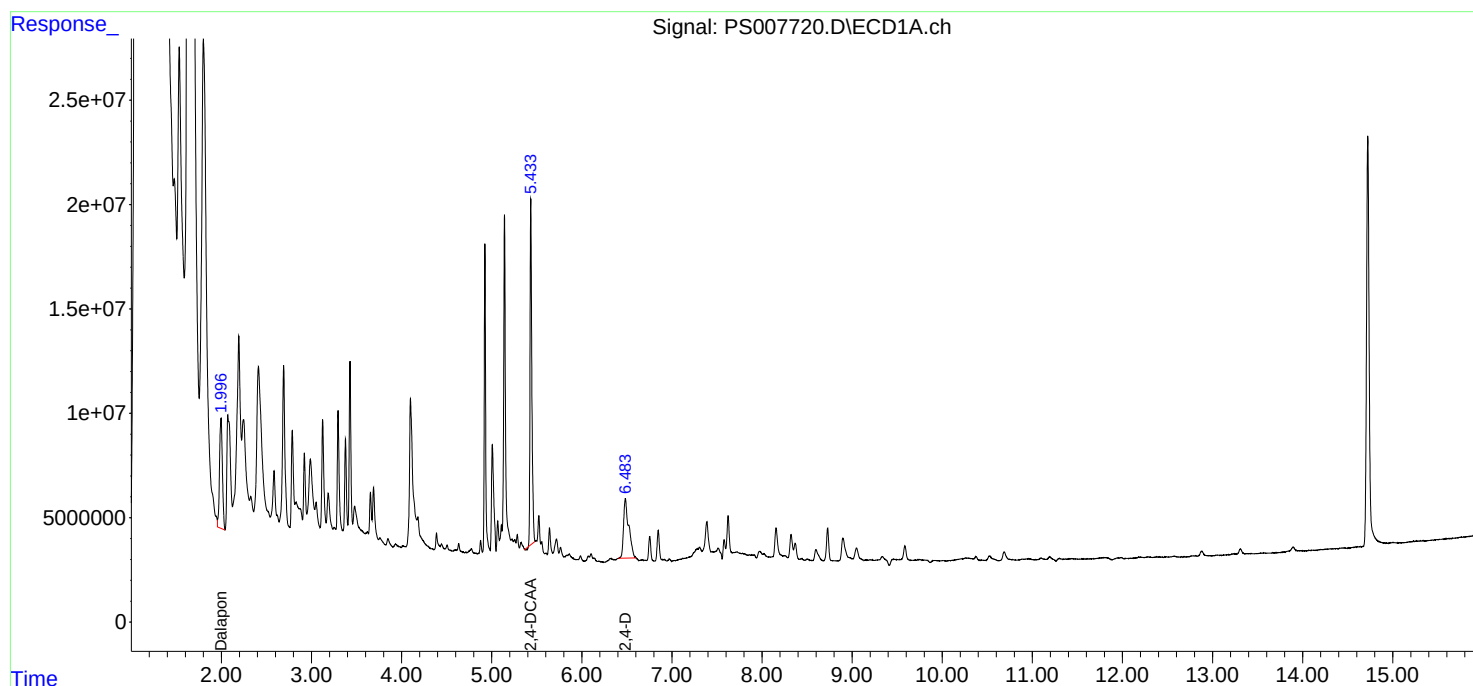


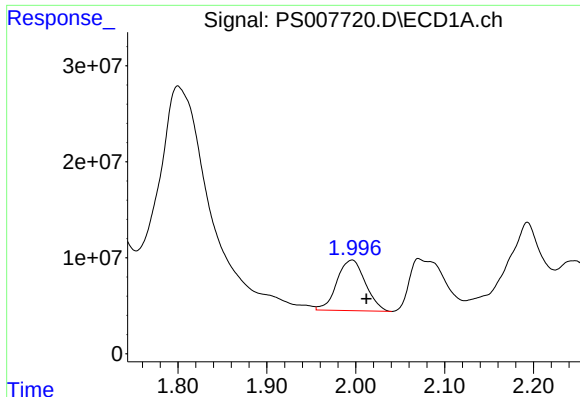

#1 Dalapon


R.T.: 1.996 min
Delta R.T.: -0.016 min
Response: 117486405
Conc: 64.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-2A-COMP

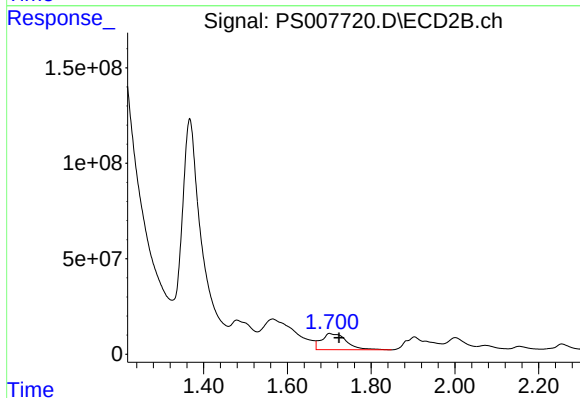


#1 Dalapon

R.T.: 1.701 min
Delta R.T.: -0.022 min
Response: 348972345
Conc: 293.90 ng/ml

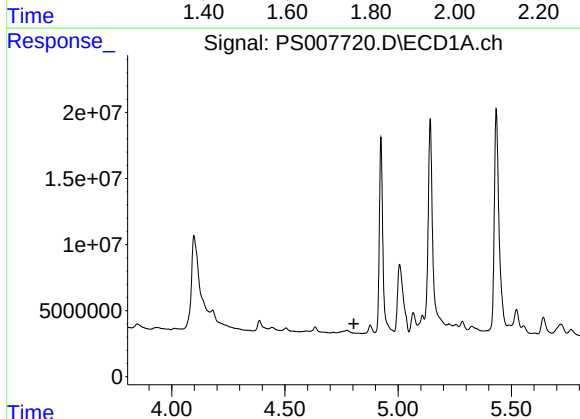


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

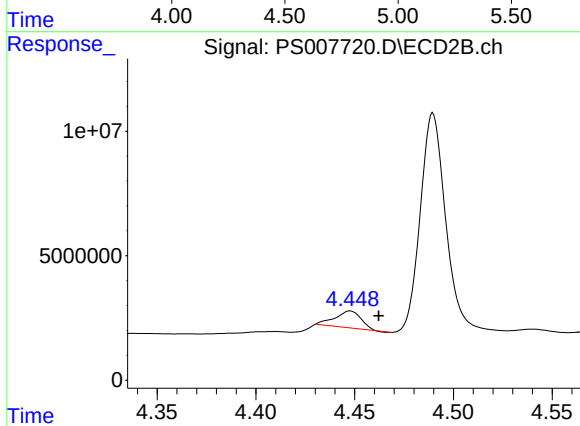

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.447 min
Delta R.T.: -0.015 min
Response: 6171252
Conc: 6.83 ng/ml

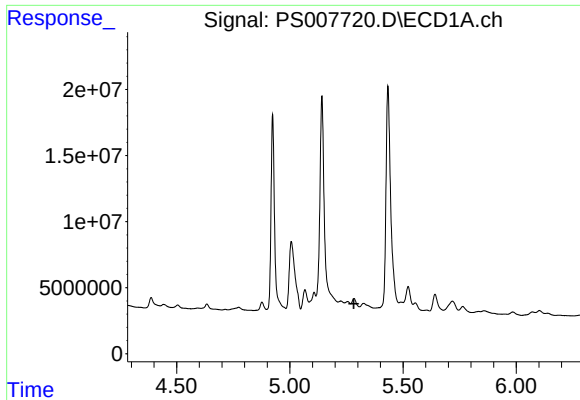

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-2A-COMP

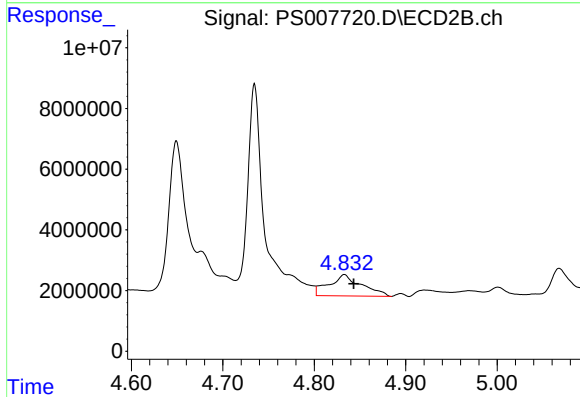


#3 4-Nitrophenol

R.T.: 4.833 min
Delta R.T.: -0.010 min
Response: 17352665
Conc: 42.17 ng/ml

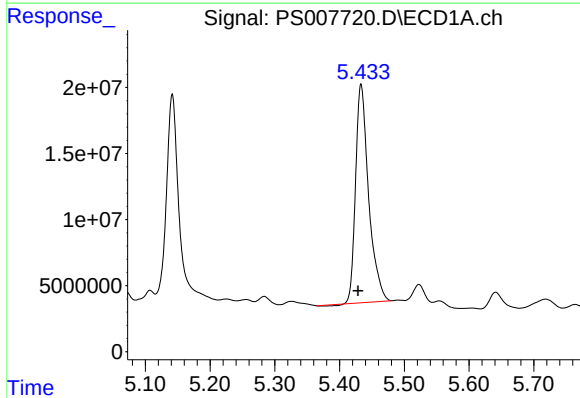


#4 2,4-DCAA

R.T.: 5.433 min
Delta R.T.: 0.005 min
Response: 230504637
Conc: 167.37 ng/ml

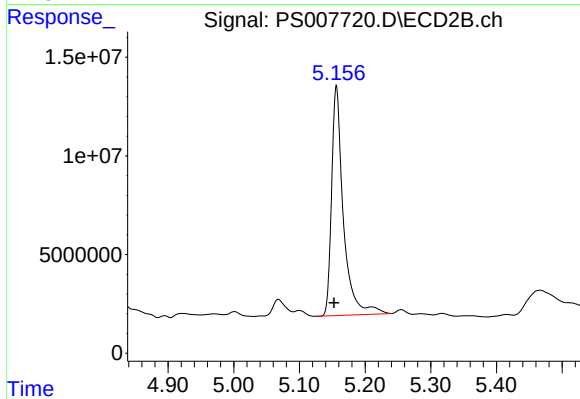

#4 2,4-DCAA


R.T.: 5.157 min
Delta R.T.: 0.004 min
Response: 145064291
Conc: 206.48 ng/ml

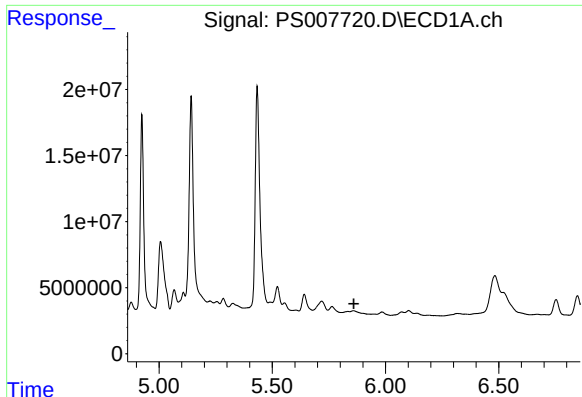

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.860 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-2A-COMP

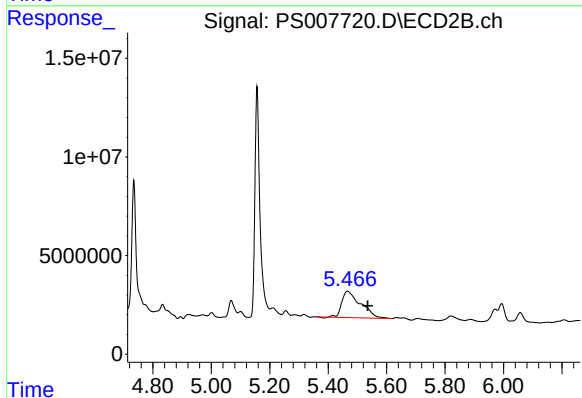


#7 MCPA

R.T.: 5.466 min
Delta R.T.: -0.070 min
Response: 60173904
Conc: 20.02 ug/ml

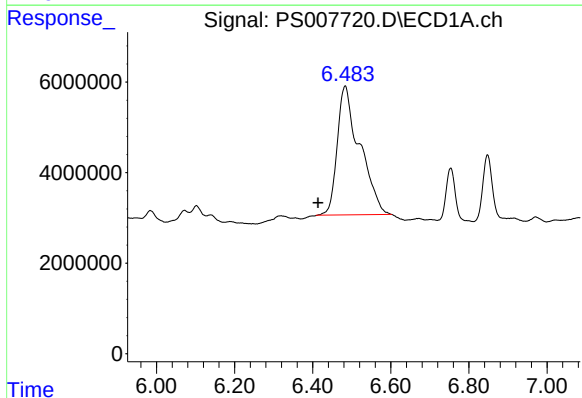


#9 2,4-D

R.T.: 6.483 min
Delta R.T.: 0.069 min
Response: 113852643
Conc: 81.18 ng/ml

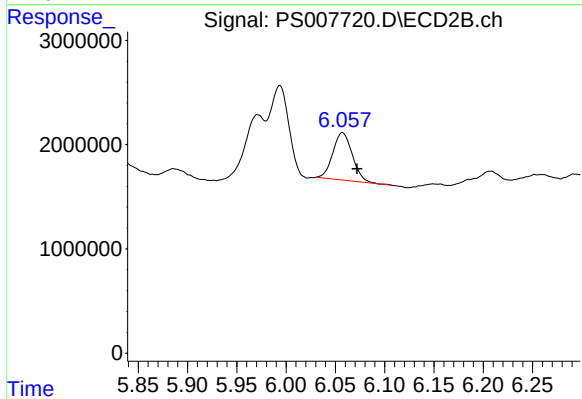

#9 2,4-D


R.T.: 6.057 min
Delta R.T.: -0.015 min
Response: 6282664
Conc: 7.79 ng/ml

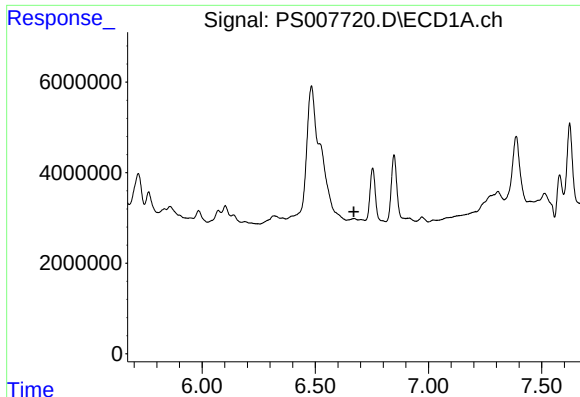

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TP-2A-COMP

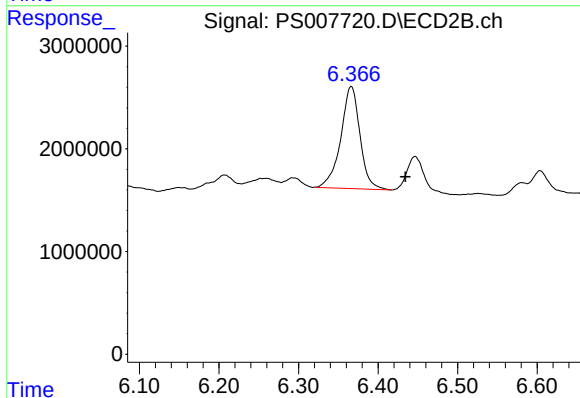


#10 Pentachlorophenol

R.T.: 6.366 min
Delta R.T.: -0.068 min
Response: 16688149
Conc: 1.70 ng/ml

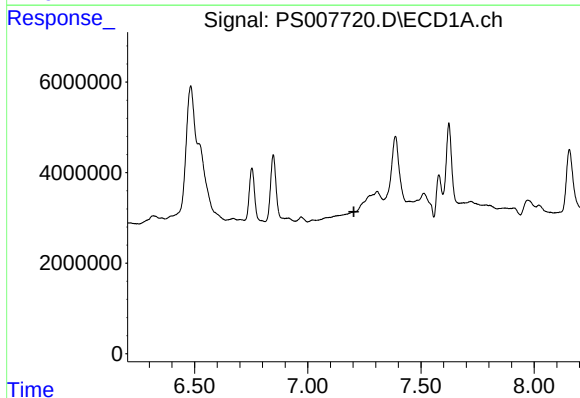

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

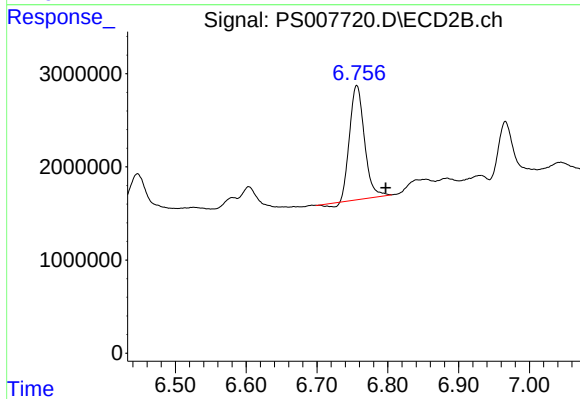

#11 2,4,5-TP (SILVEX)

R.T.: 6.756 min
Delta R.T.: -0.041 min
Response: 17543296
Conc: 4.48 ng/ml