

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111819\
 Data File : PS007723.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2019 21:21
 Operator : SM\AJ
 Sample : K5848-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 ESW

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 04:06:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.428	5.143	245.0E6	133.8E6	177.864	190.435
Target Compounds							
1) T	Dalapon	1.990	1.687	130.1E6	388.7E6	71.898	327.336 #
2) T	3,5-DICHL...	0.000	4.476	0	67570078	N.D.	74.793
3) T	4-Nitroph...	0.000	4.818	0	19494749	N.D.	47.375
9) T	2,4-D	6.477	0.000	120.2E6	0	85.701	N.D. #
11) T	2,4,5-TP ...	0.000	6.742	0	20508410	N.D.	5.237
15) T	Picloram	0.000	8.897	0	8655609	N.D.	1.477
16) T	DCPA	0.000	8.897	0	8655609	N.D.	1.656



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111819\
Data File : PS007723.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2019 21:21
Operator : SM\AJ
Sample : K5848-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
ESW

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 04:06:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

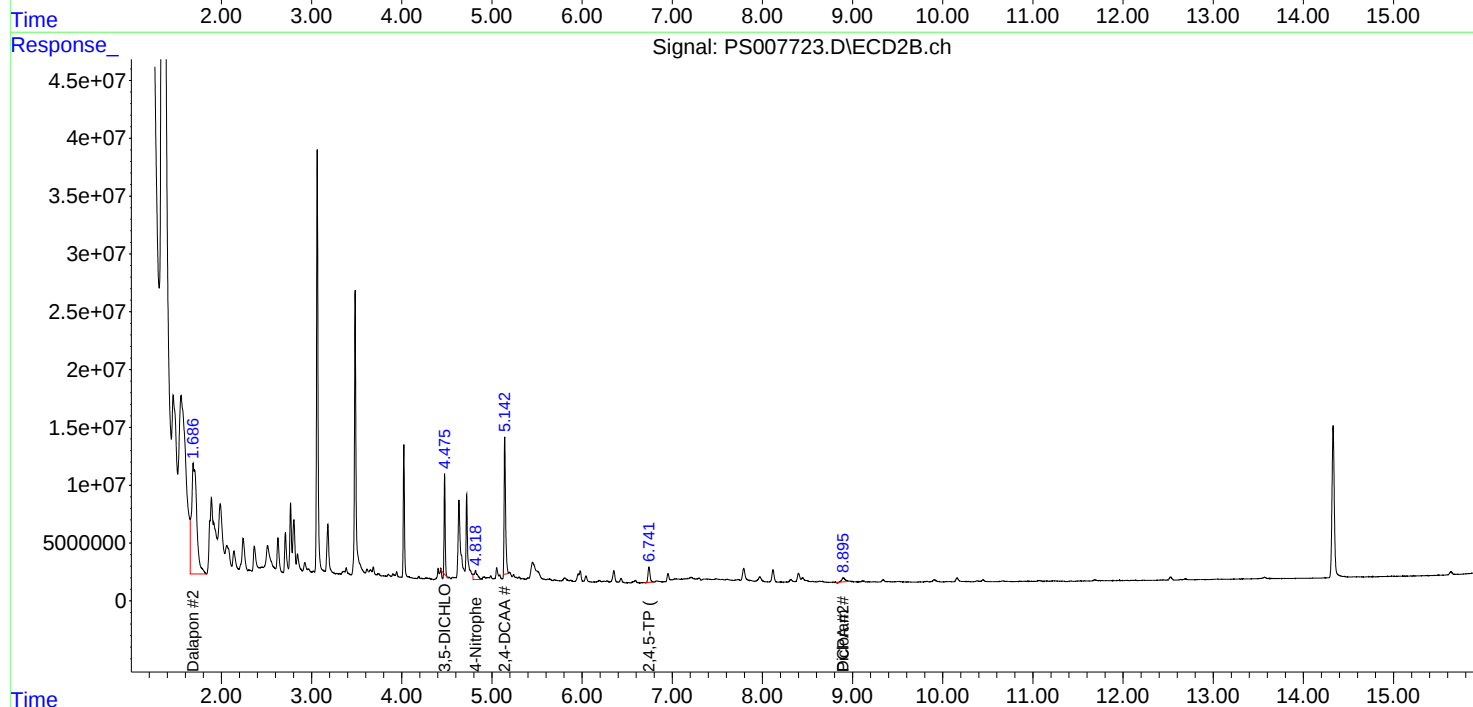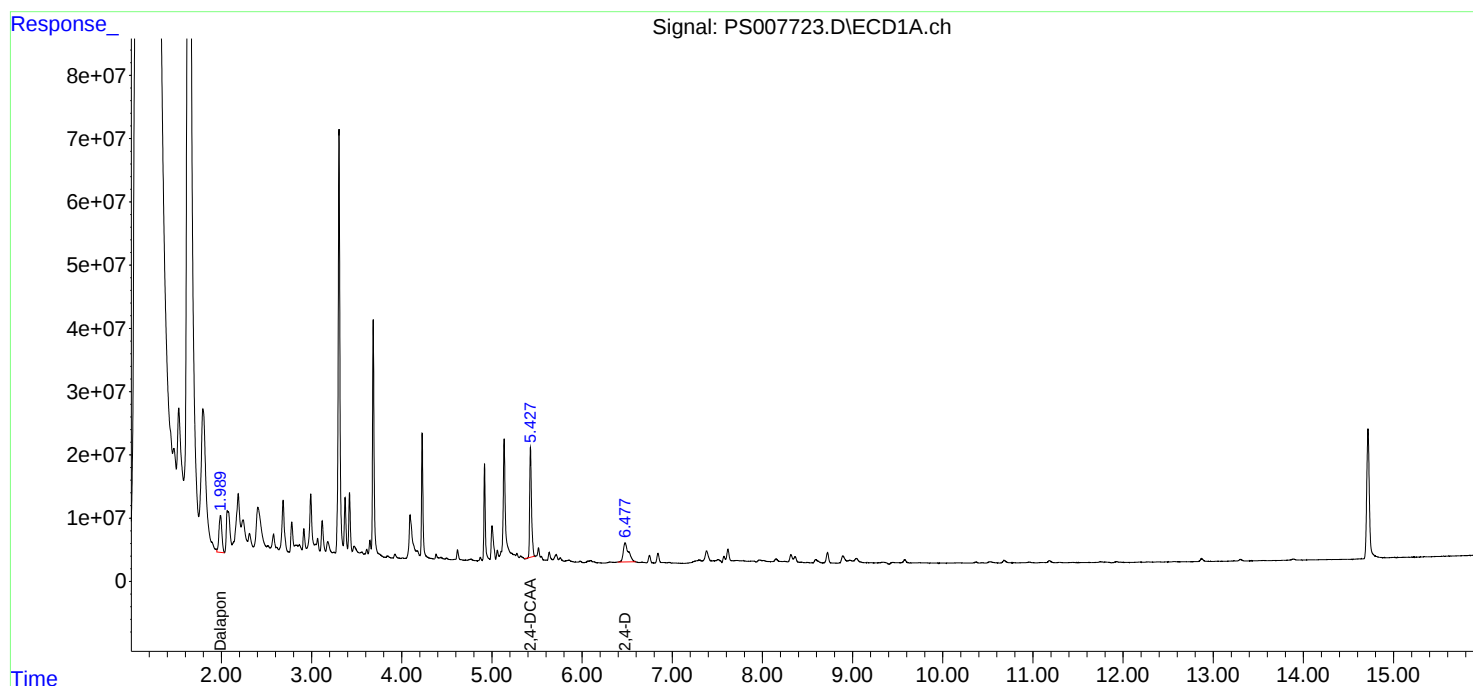


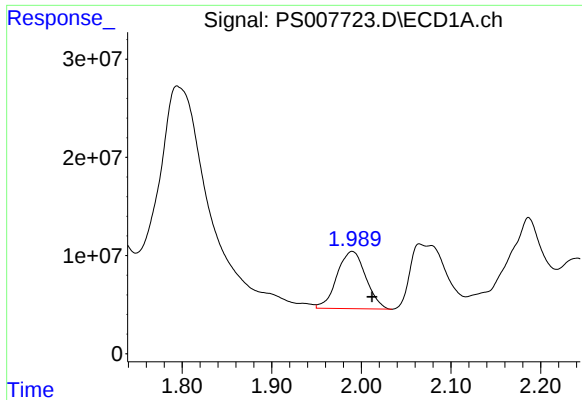

#1 Dalapon


R.T.: 1.990 min
Delta R.T.: -0.022 min
Response: 130077224
Conc: 71.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
ESW

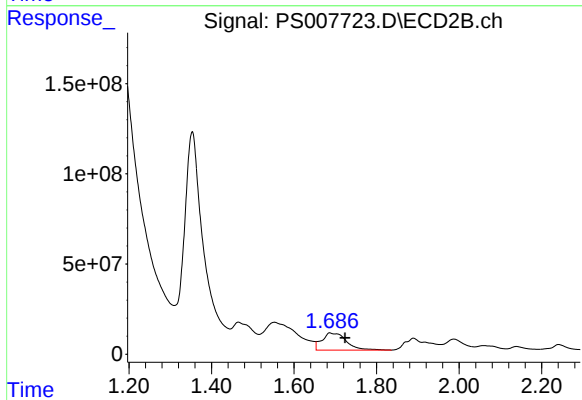


#1 Dalapon

R.T.: 1.687 min
Delta R.T.: -0.036 min
Response: 388679312
Conc: 327.34 ng/ml

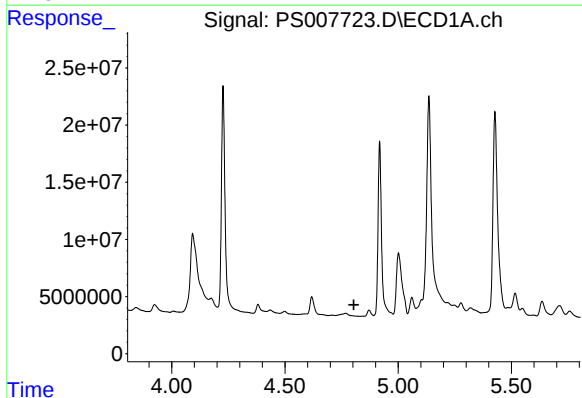


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

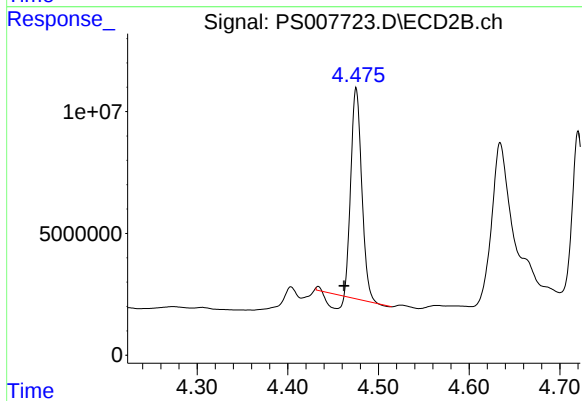

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.476 min
Delta R.T.: 0.013 min
Response: 67570078
Conc: 74.79 ng/ml

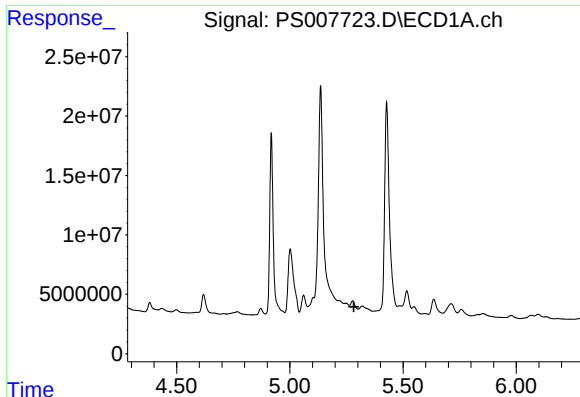

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
ESW

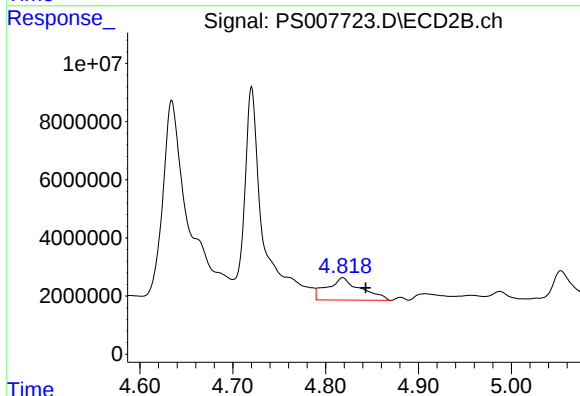


#3 4-Nitrophenol

R.T.: 4.818 min
Delta R.T.: -0.025 min
Response: 19494749
Conc: 47.38 ng/ml

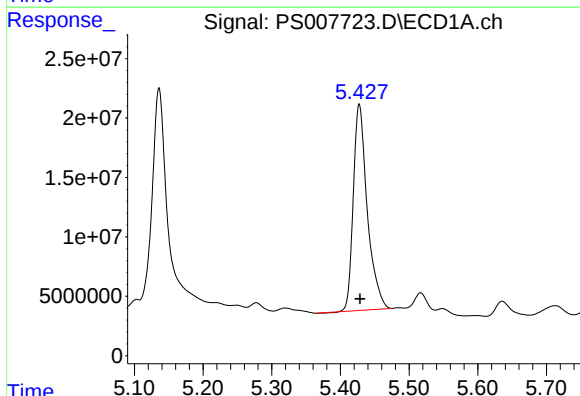


#4 2,4-DCAA

R.T.: 5.428 min
Delta R.T.: 0.000 min
Response: 244951654
Conc: 177.86 ng/ml

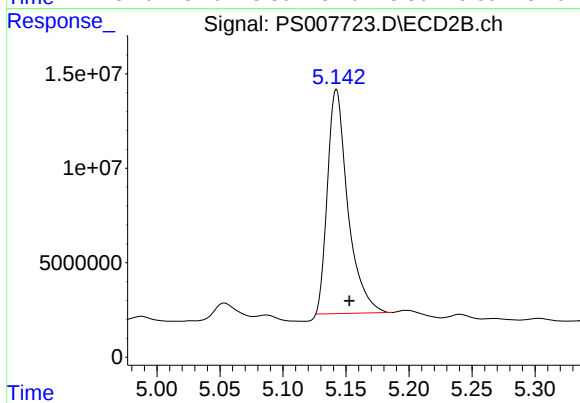

#4 2,4-DCAA


R.T.: 5.143 min
Delta R.T.: -0.010 min
Response: 133792542
Conc: 190.43 ng/ml

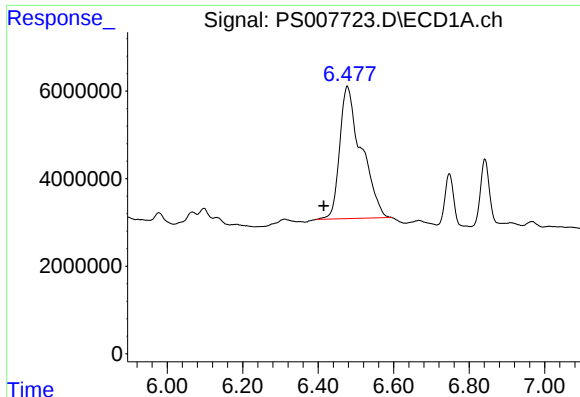

#9 2,4-D


R.T.: 6.477 min
Delta R.T.: 0.063 min
Response: 120199488
Conc: 85.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
ESW

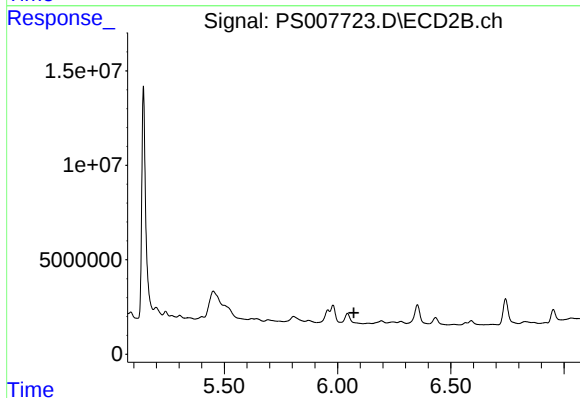


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

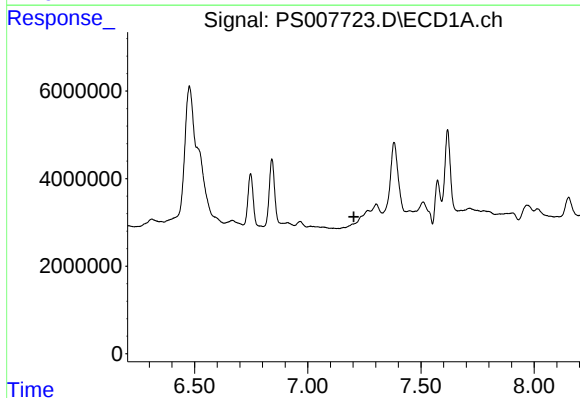


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.203 min
Response: 0
Conc: N.D.

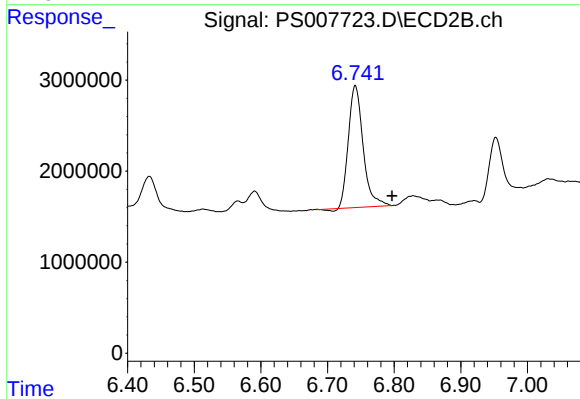

#11 2,4,5-TP (SILVEX)


R.T.: 6.742 min
Delta R.T.: -0.055 min
Response: 20508410
Conc: 5.24 ng/ml

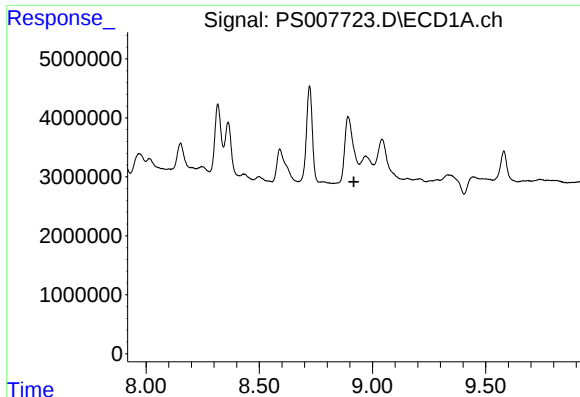

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 8.918 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
ESW

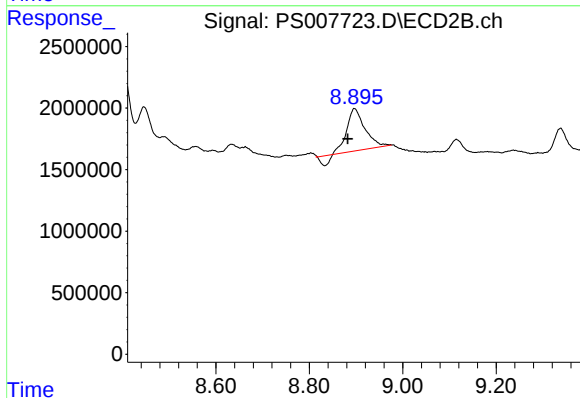


#15 Picloram

R.T.: 8.897 min
Delta R.T.: 0.015 min
Response: 8655609
Conc: 1.48 ng/ml

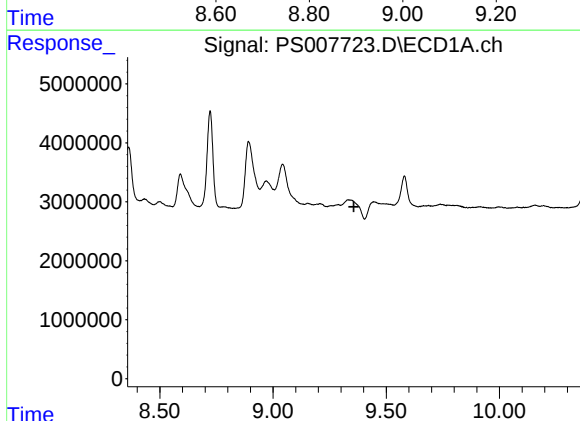

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.357 min
Response: 0
Conc: N.D.

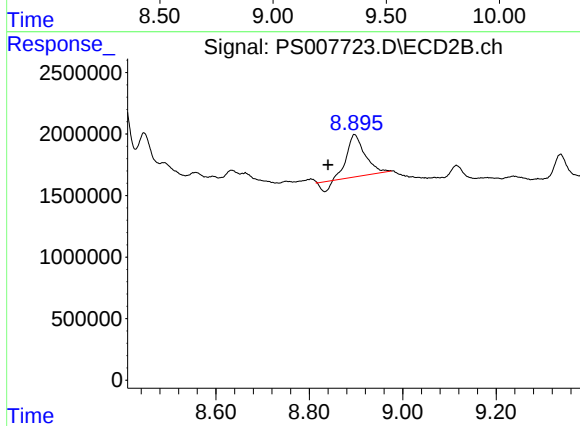

#16 DCPA

R.T.: 8.897 min
Delta R.T.: 0.057 min
Response: 8655609
Conc: 1.66 ng/ml