

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111819\
 Data File : PS007731.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2019 00:17
 Operator : SM\AJ
 Sample : K5840-09
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PHIPPS-BH-SE-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 04:08:44 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.446	5.171	149.5E6	26808761	108.585	38.158 #
Target Compounds							
1) T	Dalapon	2.005	1.677	209.4E6	2598.7E6	115.743	2188.573 #
2) T	3,5-DICHL...	0.000	4.505	0	21287181	N.D.	23.563
5) T	DICAMBA	5.541	0.000	124.9E6	0	24.552	N.D. #
7) T	MCPA	5.914	5.538	29100308	35691490	5.287	11.875 #
9) T	2,4-D	0.000	6.073	0	3873901	N.D.	4.804
10) T	Pentachlo...	0.000	6.381	0	40736713	N.D.	4.160
11) T	2,4,5-TP ...	0.000	6.770	0	20746368	N.D.	5.298
14) T	DINOSEB	0.000	7.918	0	28566276	N.D.	9.826
15) T	Picloram	0.000	8.945	0	34062714	N.D.	5.814
16) T	DCPA	9.390	8.797	62797715	74845514	6.403	14.324 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111819\
Data File : PS007731.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2019 00:17
Operator : SM\AJ
Sample : K5840-09
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PHIPPS-BH-SE-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 04:08:44 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

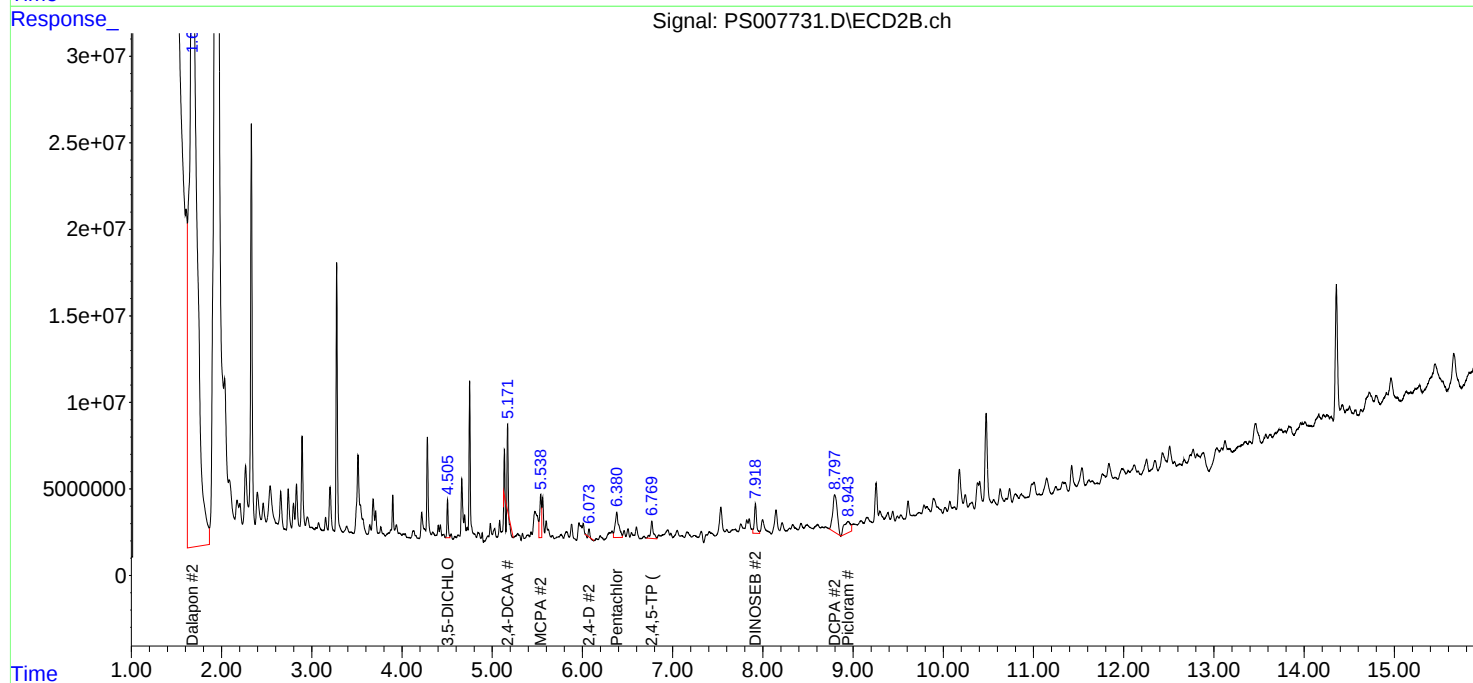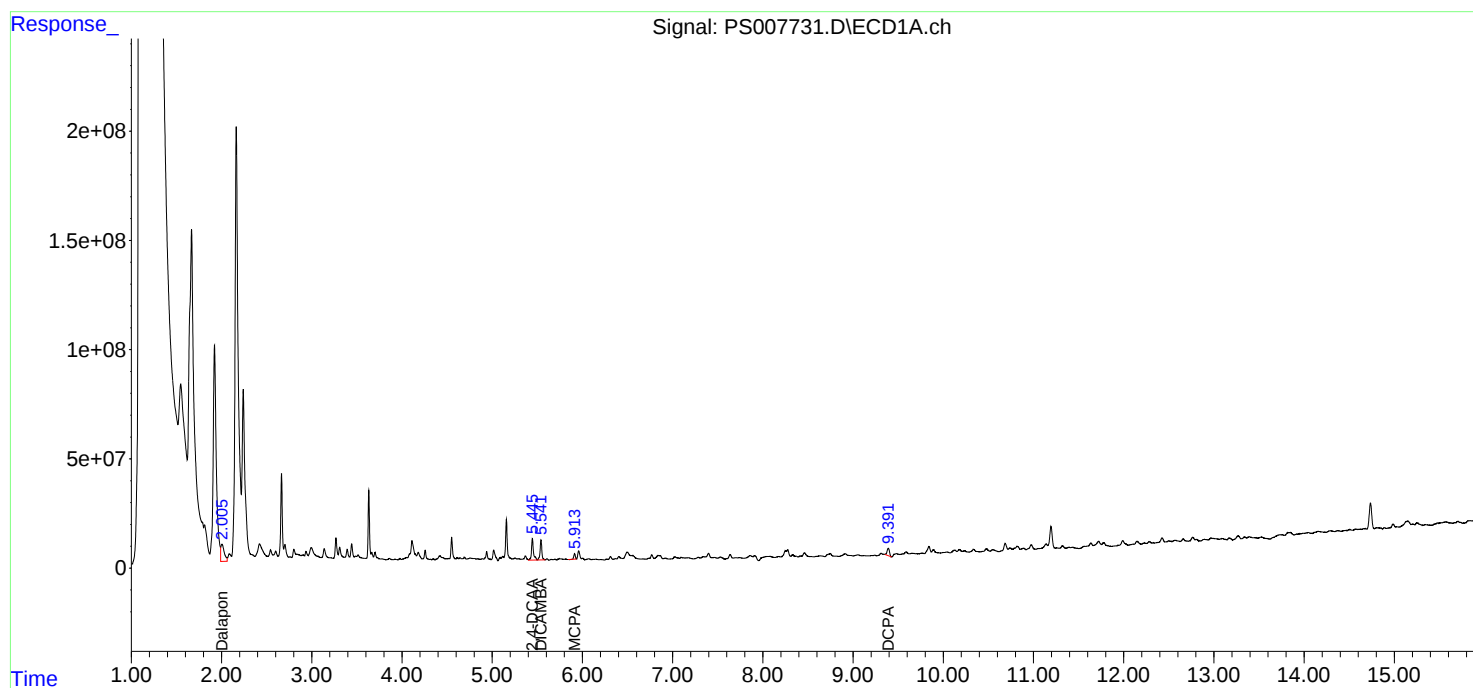


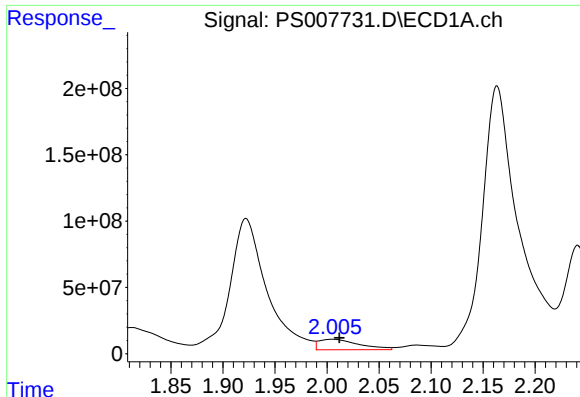

#1 Dalapon


R.T.: 2.005 min
Delta R.T.: -0.007 min
Response: 209399514
Conc: 115.74 ng/ml

Instrument :
ECD_S
ClientSampleId :
PHIPPS-BH-SE-01

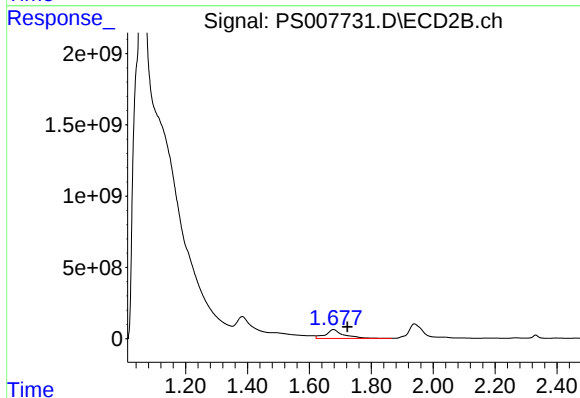


#1 Dalapon

R.T.: 1.677 min
Delta R.T.: -0.046 min
Response: 2598717591
Conc: 2188.57 ng/ml

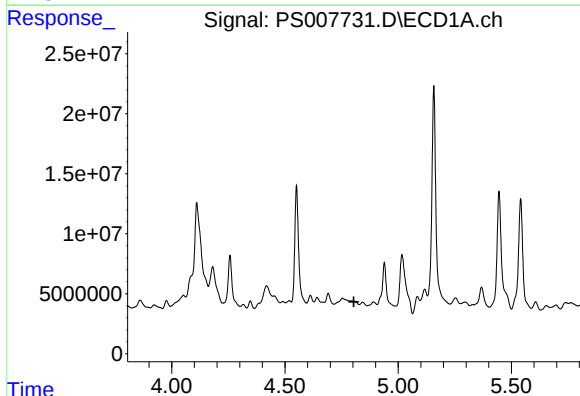


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

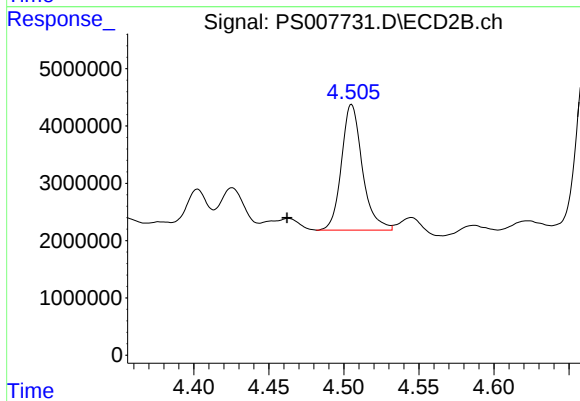

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.505 min
Delta R.T.: 0.043 min
Response: 21287181
Conc: 23.56 ng/ml

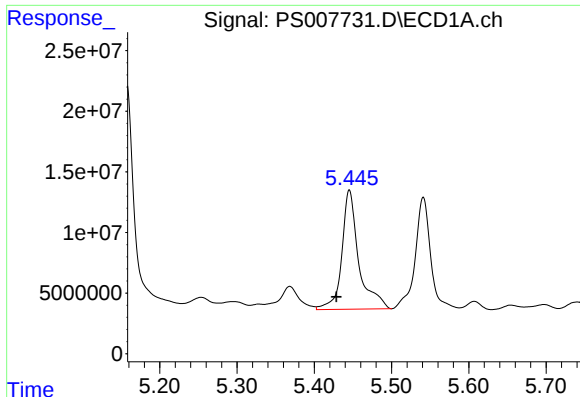

#4 2,4-DCAA


R.T.: 5.446 min
Delta R.T.: 0.017 min
Response: 149541602
Conc: 108.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
PHIPPS-BH-SE-01

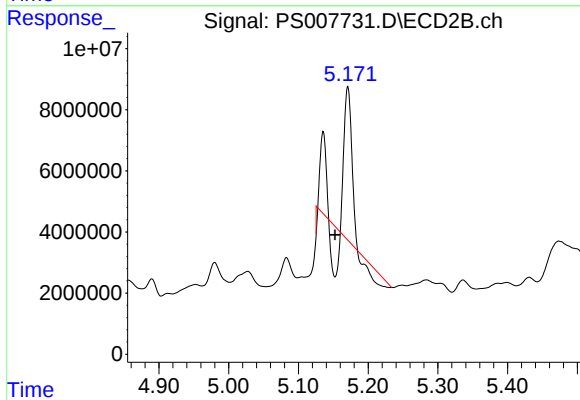


#4 2,4-DCAA

R.T.: 5.171 min
Delta R.T.: 0.018 min
Response: 26808761
Conc: 38.16 ng/ml

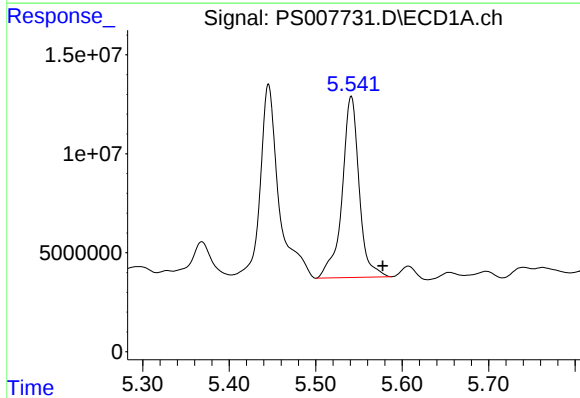


#5 DICAMBA

R.T.: 5.541 min
Delta R.T.: -0.036 min
Response: 124907037
Conc: 24.55 ng/ml

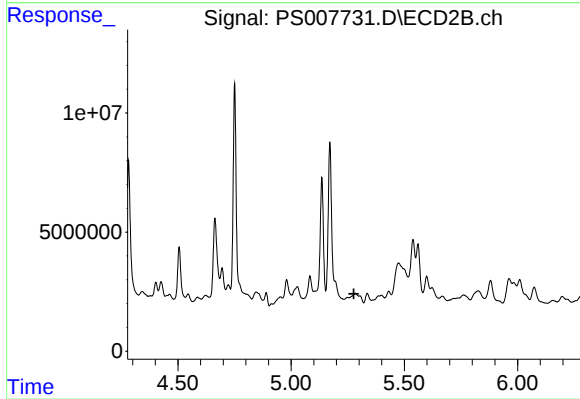

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.277 min
Response: 0
Conc: N.D.

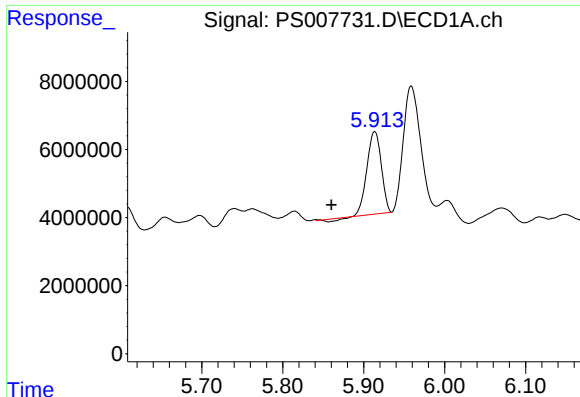

#7 MCPA


R.T.: 5.914 min
Delta R.T.: 0.054 min
Response: 29100308
Conc: 5.29 ug/ml

Instrument :
ECD_S
ClientSampleId :
PHIPPS-BH-SE-01

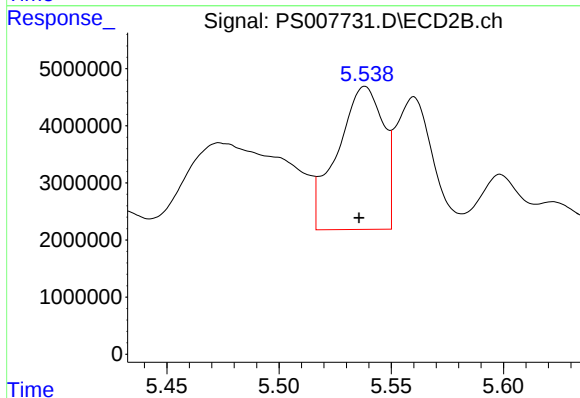


#7 MCPA

R.T.: 5.538 min
Delta R.T.: 0.003 min
Response: 35691490
Conc: 11.87 ug/ml

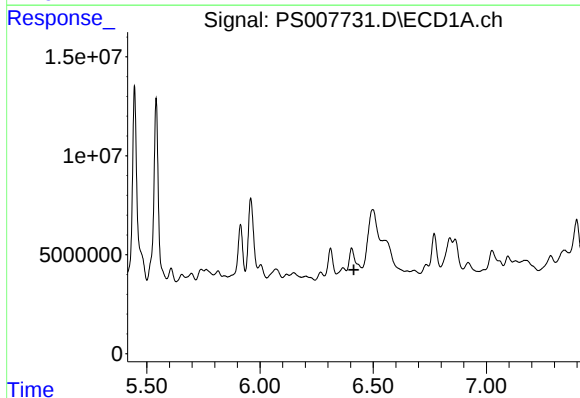


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.414 min
Response: 0
Conc: N.D.

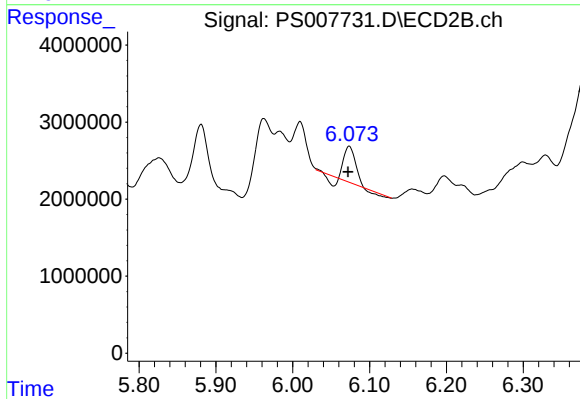

#9 2,4-D


R.T.: 6.073 min
Delta R.T.: 0.001 min
Response: 3873901
Conc: 4.80 ng/ml

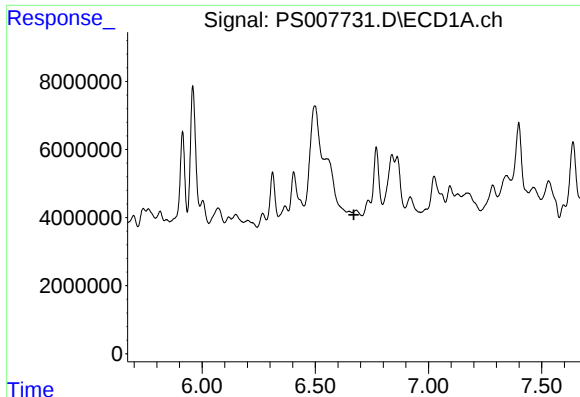

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PHIPPS-BH-SE-01

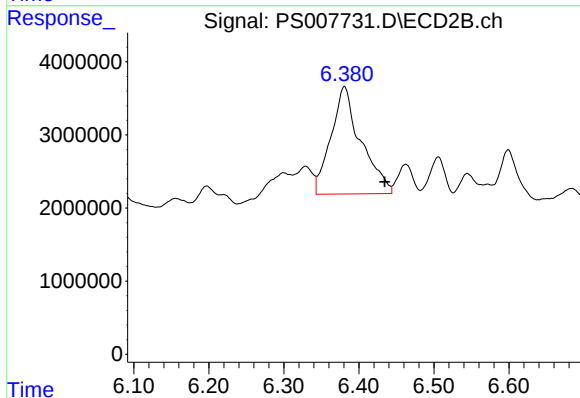


#10 Pentachlorophenol

R.T.: 6.381 min
Delta R.T.: -0.054 min
Response: 40736713
Conc: 4.16 ng/ml

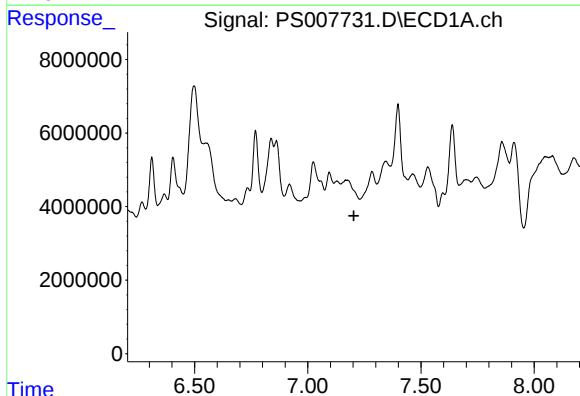


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

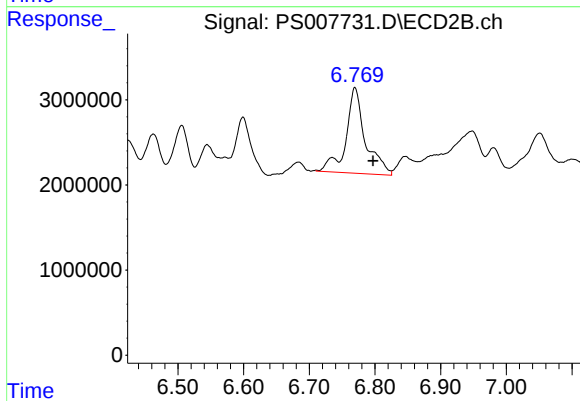

#11 2,4,5-TP (SILVEX)


R.T.: 6.770 min
Delta R.T.: -0.027 min
Response: 20746368
Conc: 5.30 ng/ml

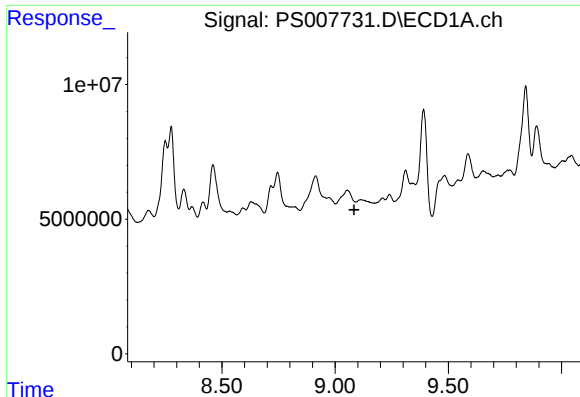

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PHIPPS-BH-SE-01

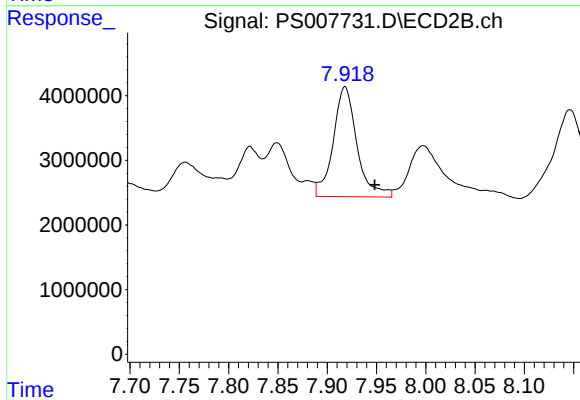


#14 DINOSEB

R.T.: 7.918 min
Delta R.T.: -0.030 min
Response: 28566276
Conc: 9.83 ng/ml

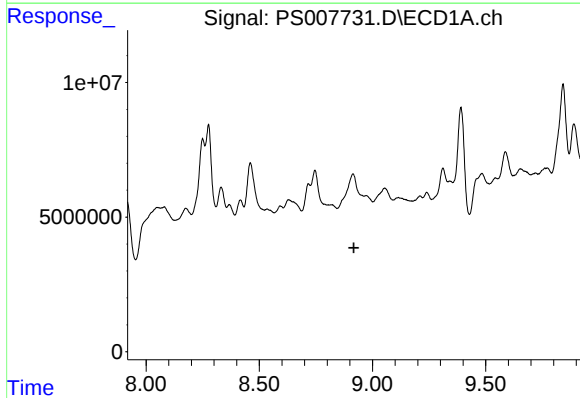


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.918 min
Response: 0
Conc: N.D.

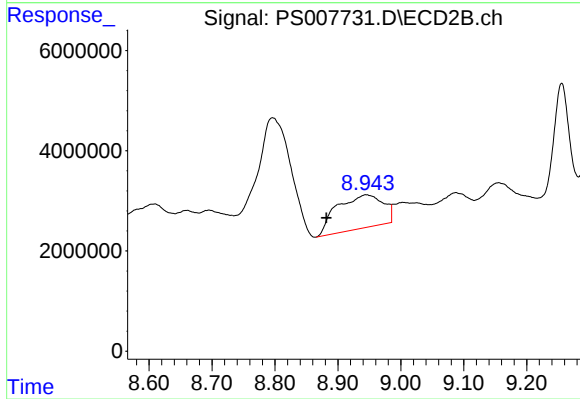

#15 Picloram


R.T.: 8.945 min
Delta R.T.: 0.063 min
Response: 34062714
Conc: 5.81 ng/ml

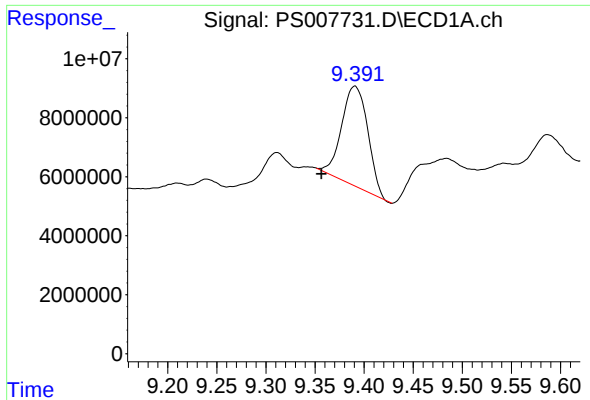

#16 DCPA

R.T.: 9.390 min
Delta R.T.: 0.034 min
Response: 62797715
Conc: 6.40 ng/ml

Instrument :
ECD_S
ClientSampleId :
PHIPPS-BH-SE-01

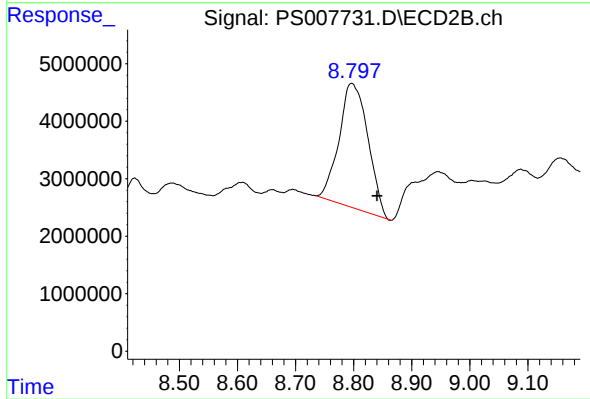

#16 DCPA

R.T.: 8.797 min
Delta R.T.: -0.044 min
Response: 74845514
Conc: 14.32 ng/ml