

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111821\
 Data File : PS017453.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2021 19:44
 Operator : AJ\MA
 Sample : HSTDICC1500
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC1500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 04:28:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 19 04:25:46 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.149	6.739	2349.9E6	921.1E6	1471.273	1495.486
Target Compounds							
1) T	Dalapon	2.986	2.492	3275.2E6	971.5E6	1356.790	1360.308
2) T	3,5-DICHL...	6.373	5.936	2987.8E6	1261.4E6	1354.225	1369.768
3) T	4-Nitroph...	6.977	6.363	1216.7E6	456.3E6	1378.035	1345.851
5) T	DICAMBA	7.339	6.900	8398.5E6	3596.1E6	1361.680	1359.503
6) T	MCPD	7.515	7.004	706.7E6	314.9E6	142.704	141.964
7) T	MCPA	7.665	7.217	950.3E6	427.0E6	139.102	138.493
8) T	DICHLORPROP	8.030	7.517	2136.5E6	953.8E6	1377.891	1401.429
9) T	2,4-D	8.258	7.807	2577.7E6	1133.5E6	1372.828	1397.890
10) T	Pentachlo...	8.564	8.232	26764.1E6	10463.9E6	1315.669	1302.826
11) T	2,4,5-TP ...	9.113	8.592	11305.7E6	4878.8E6	1362.290	1364.988
12) T	2,4,5-T	9.397	8.969	11553.5E6	4653.7E6	1363.711	1372.646
13) T	2,4-DB	9.945	9.474	2586.0E6	643.3E6	1430.877	1433.989
14) T	DINOSEB	11.099	9.800	8440.9E6	3336.7E6	1357.383	1375.355
15) T	Picloram	10.920	10.778	17432.5E6	6298.3E6	1386.131	1384.969
16) T	DCPA	11.367	10.730	14309.5E6	5986.2E6	1363.351	1365.794



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111821\
Data File : PS017453.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2021 19:44
Operator : AJ\MA
Sample : HSTDICC1500
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 04:28:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
Quant Title : 8080.M
QLast Update : Fri Nov 19 04:25:46 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

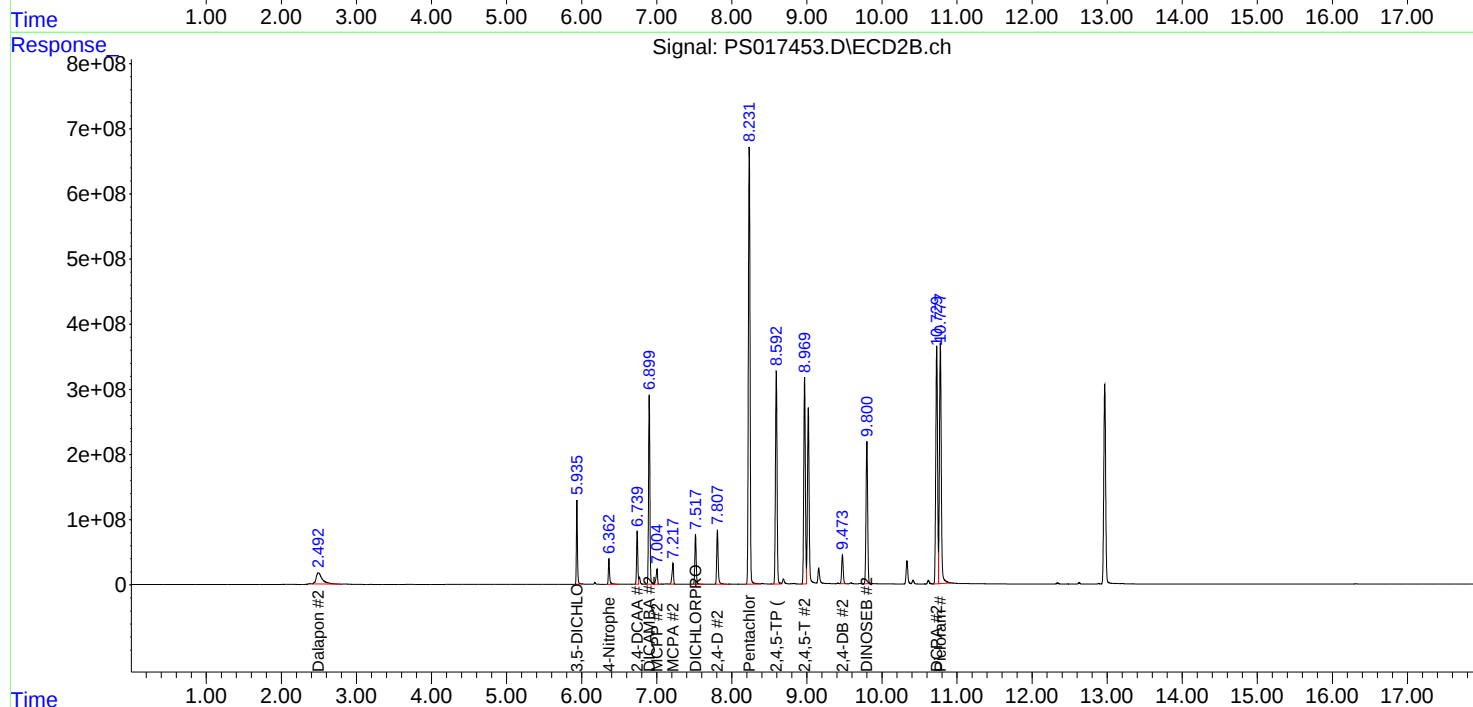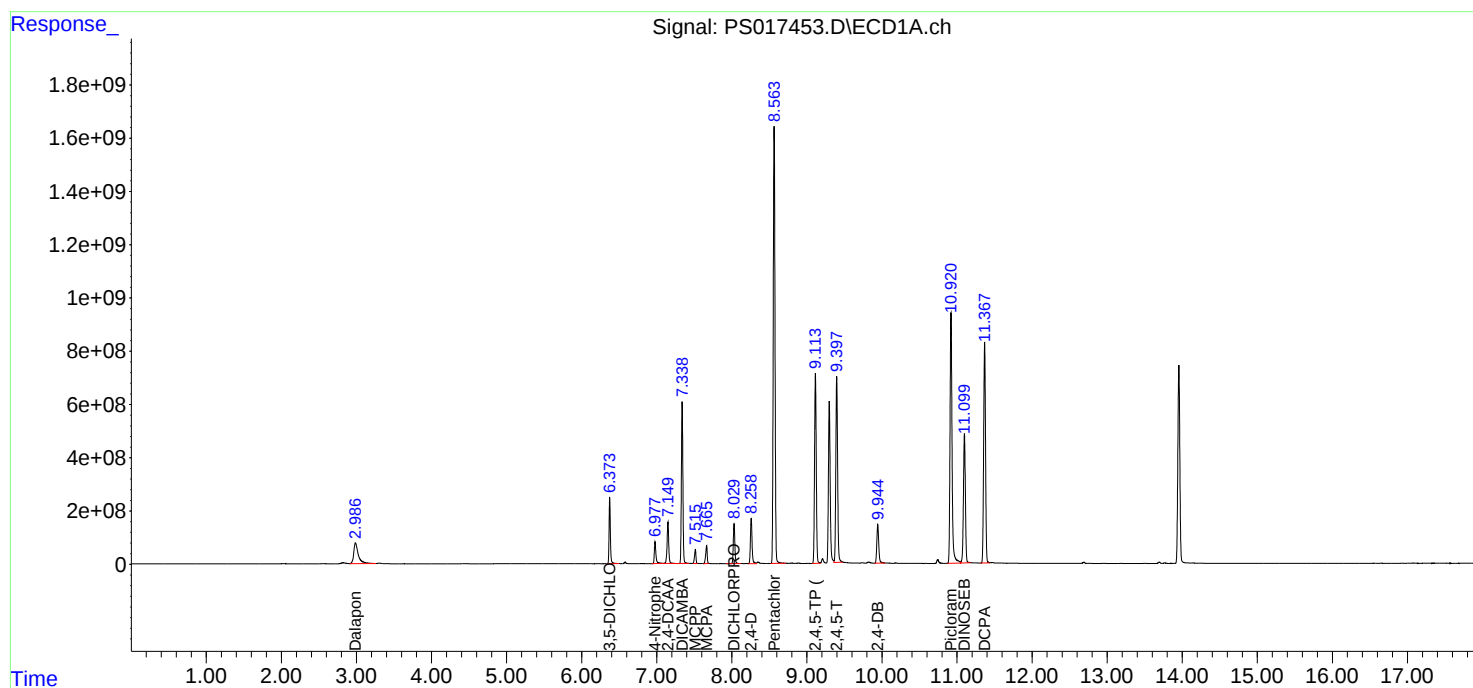


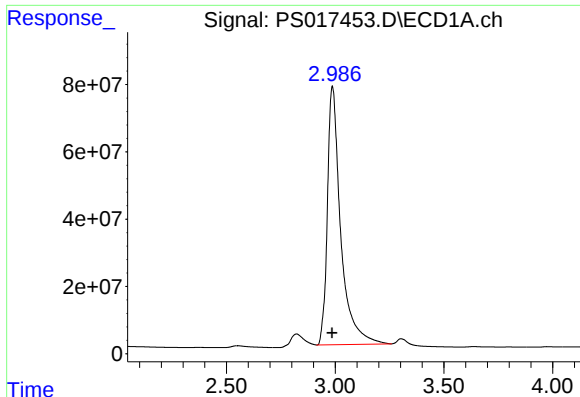

#1 Dalapon


R.T.: 2.986 min
Delta R.T.: 0.000 min
Response: 3275160298
Conc: 1356.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

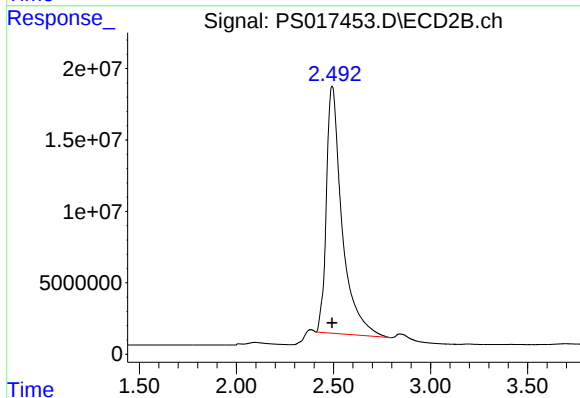


#1 Dalapon

R.T.: 2.492 min
Delta R.T.: 0.000 min
Response: 971503779
Conc: 1360.31 ng/ml

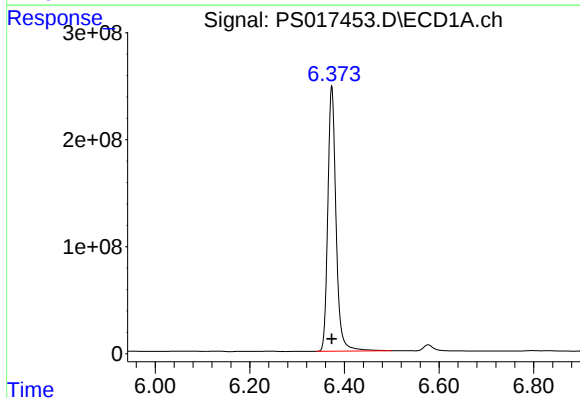


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.373 min
Delta R.T.: 0.000 min
Response: 2987801967
Conc: 1354.22 ng/ml

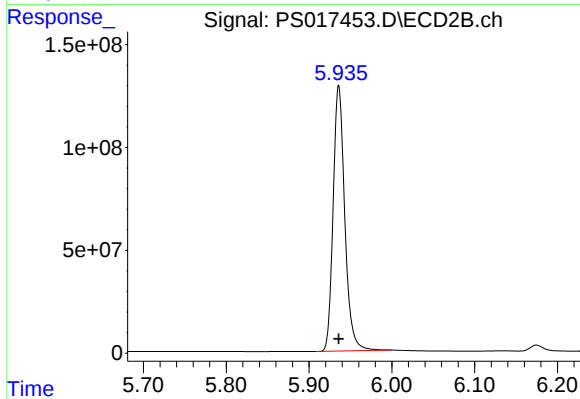

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.936 min
Delta R.T.: 0.000 min
Response: 1261372430
Conc: 1369.77 ng/ml

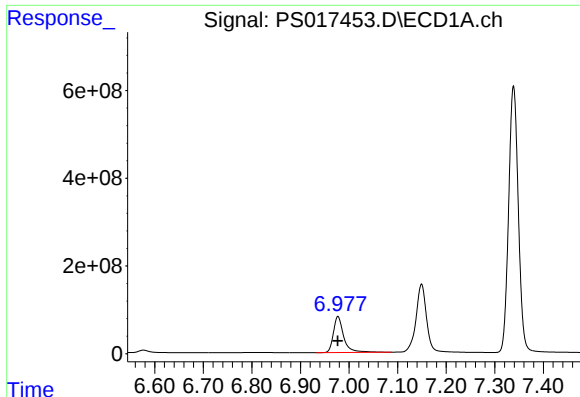

#3 4-Nitrophenol


R.T.: 6.977 min
Delta R.T.: 0.000 min
Response: 1216736638
Conc: 1378.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

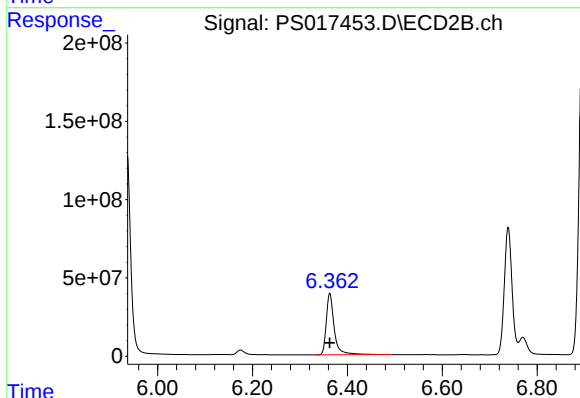


#3 4-Nitrophenol

R.T.: 6.363 min
Delta R.T.: 0.000 min
Response: 456297866
Conc: 1345.85 ng/ml

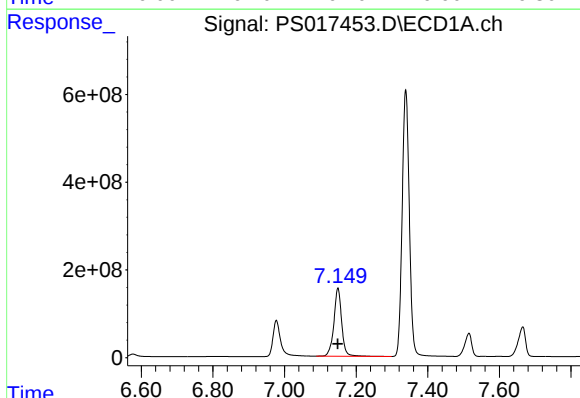


#4 2,4-DCAA

R.T.: 7.149 min
Delta R.T.: 0.000 min
Response: 2349859583
Conc: 1471.27 ng/ml

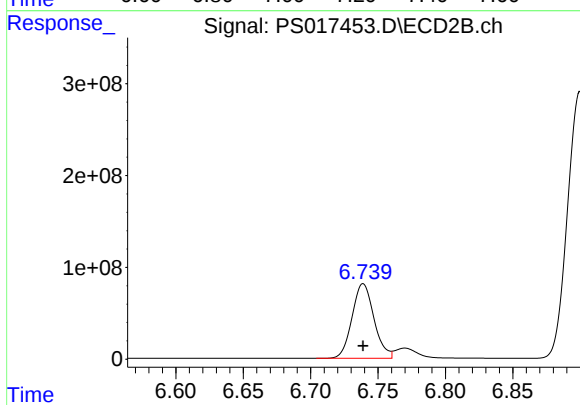

#4 2,4-DCAA


R.T.: 6.739 min
Delta R.T.: 0.000 min
Response: 921125058
Conc: 1495.49 ng/ml

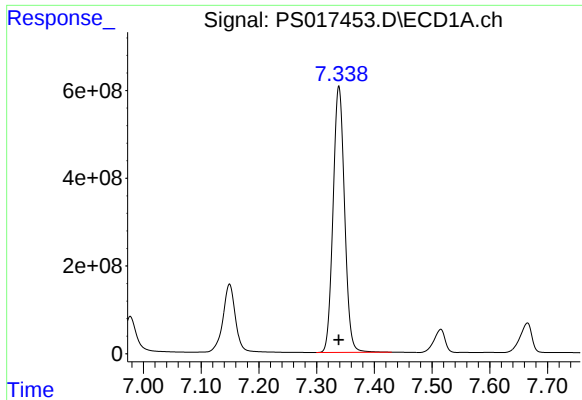

#5 DICAMBA


R.T.: 7.339 min
Delta R.T.: 0.000 min
Response: 8398503537
Conc: 1361.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

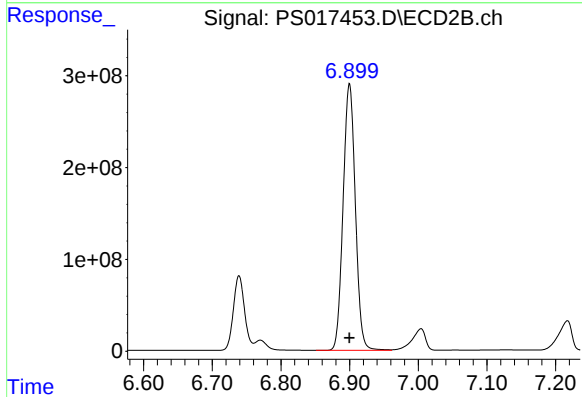


#5 DICAMBA

R.T.: 6.900 min
Delta R.T.: 0.000 min
Response: 3596084699
Conc: 1359.50 ng/ml

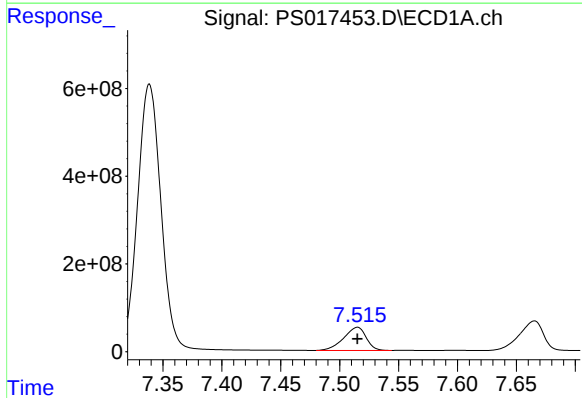


#6 MCP

R.T.: 7.515 min
Delta R.T.: 0.000 min
Response: 706680930
Conc: 142.70 ug/ml

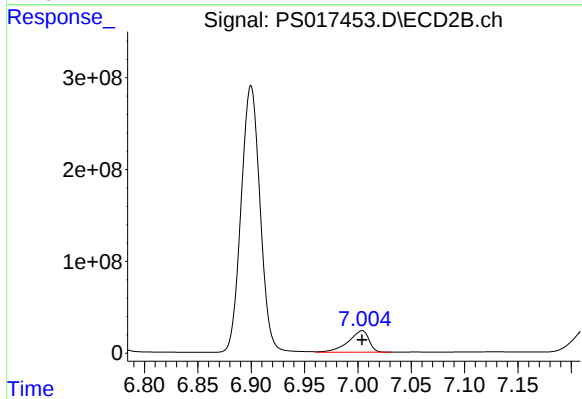

#6 MCP


R.T.: 7.004 min
Delta R.T.: 0.000 min
Response: 314905751
Conc: 141.96 ug/ml

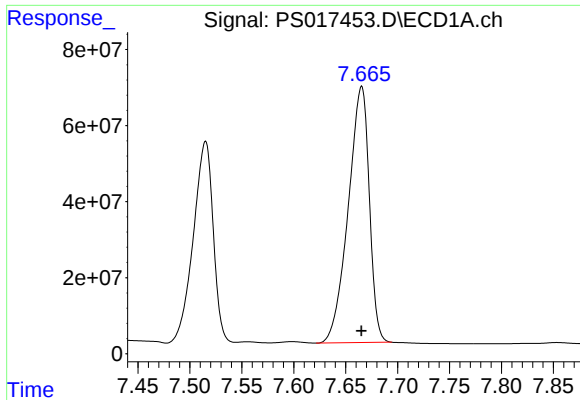

#7 MCPA


R.T.: 7.665 min
Delta R.T.: 0.000 min
Response: 950279936
Conc: 139.10 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

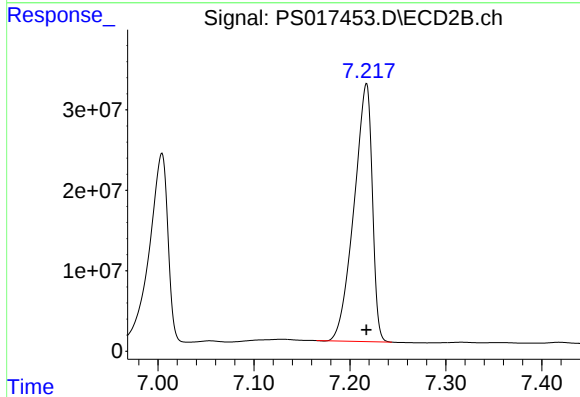


#7 MCPA

R.T.: 7.217 min
Delta R.T.: 0.000 min
Response: 426988648
Conc: 138.49 ug/ml

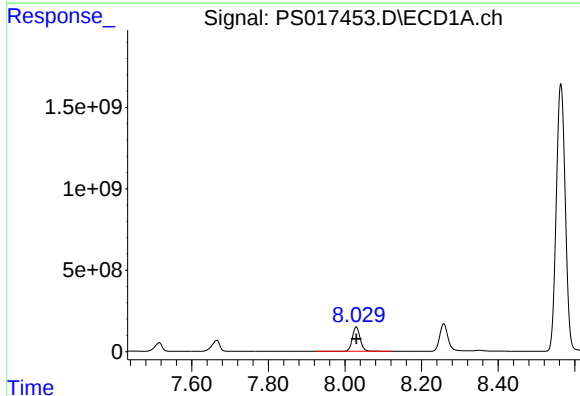


#8 DICHLORPROP

R.T.: 8.030 min
Delta R.T.: 0.000 min
Response: 2136533235
Conc: 1377.89 ng/ml

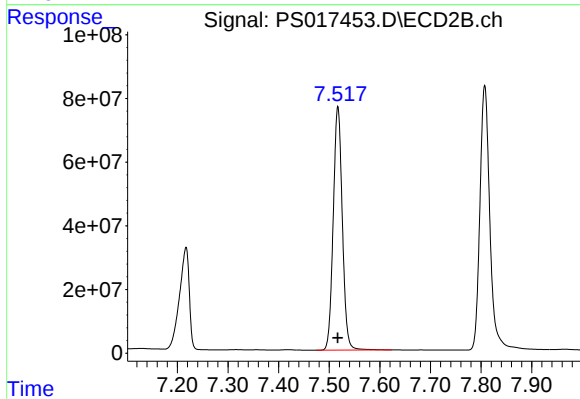

#8 DICHLORPROP


R.T.: 7.517 min
Delta R.T.: 0.000 min
Response: 953814884
Conc: 1401.43 ng/ml

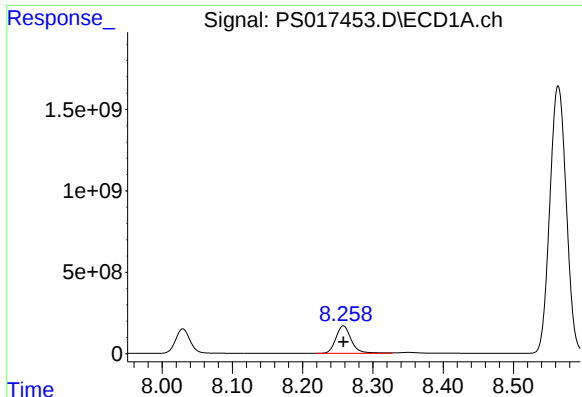

#9 2,4-D


R.T.: 8.258 min
Delta R.T.: 0.000 min
Response: 2577693617
Conc: 1372.83 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

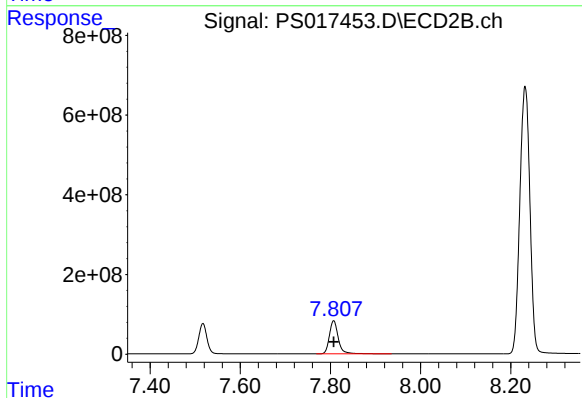


#9 2,4-D

R.T.: 7.807 min
Delta R.T.: 0.000 min
Response: 1133501805
Conc: 1397.89 ng/ml

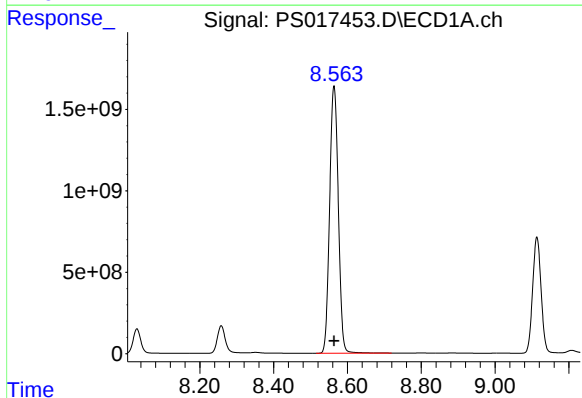


#10 Pentachlorophenol

R.T.: 8.564 min
Delta R.T.: 0.000 min
Response: 26764142980
Conc: 1315.67 ng/ml

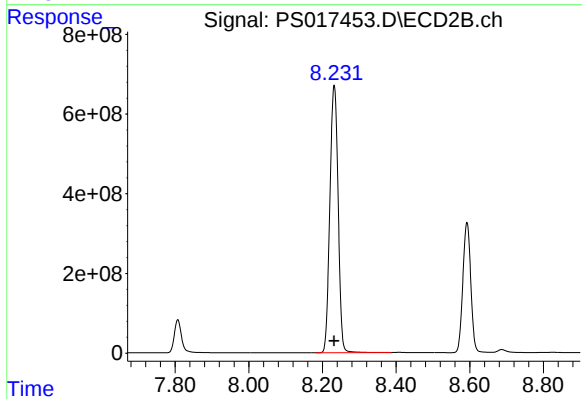

#10 Pentachlorophenol


R.T.: 8.232 min
Delta R.T.: 0.000 min
Response: 10463888155
Conc: 1302.83 ng/ml

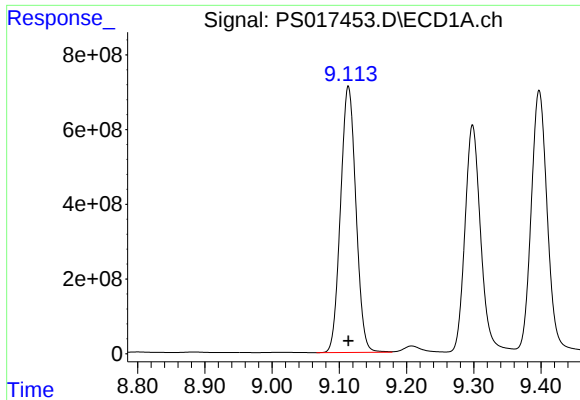

#11 2,4,5-TP (SILVEX)


R.T.: 9.113 min
Delta R.T.: 0.000 min
Response: 11305691309
Conc: 1362.29 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

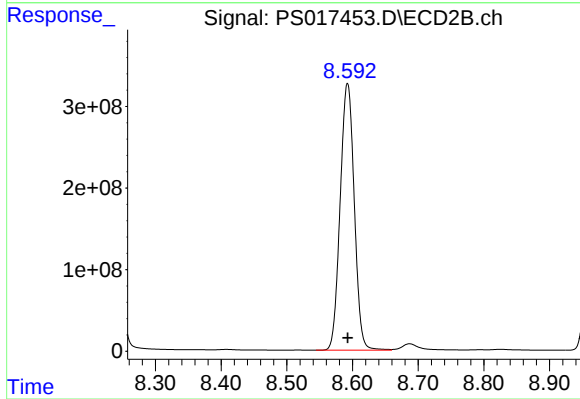


#11 2,4,5-TP (SILVEX)

R.T.: 8.592 min
Delta R.T.: 0.000 min
Response: 4878786650
Conc: 1364.99 ng/ml

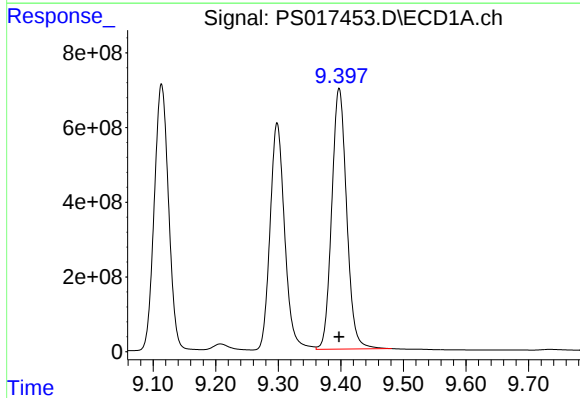


#12 2,4,5-T

R.T.: 9.397 min
Delta R.T.: 0.000 min
Response: 11553473500
Conc: 1363.71 ng/ml

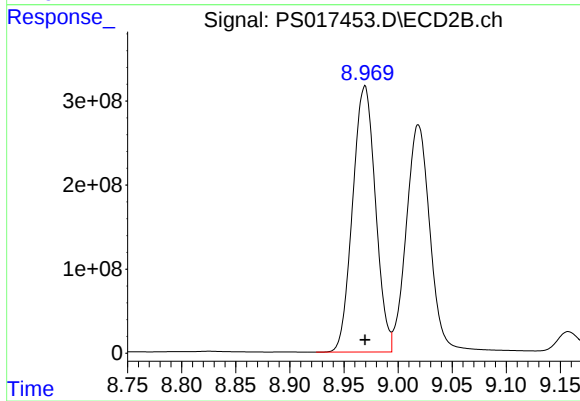

#12 2,4,5-T


R.T.: 8.969 min
Delta R.T.: 0.000 min
Response: 4653729440
Conc: 1372.65 ng/ml

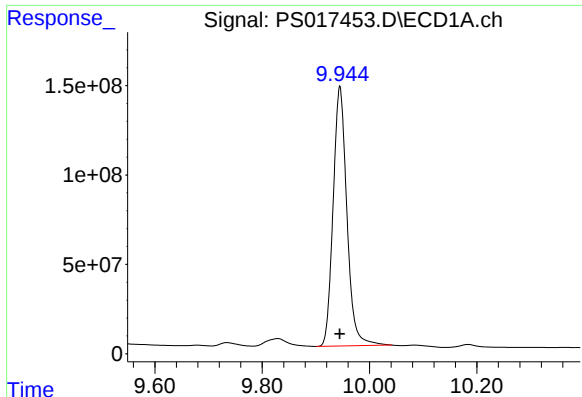

#13 2,4-DB


R.T.: 9.945 min
Delta R.T.: 0.000 min
Response: 2585958886
Conc: 1430.88 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

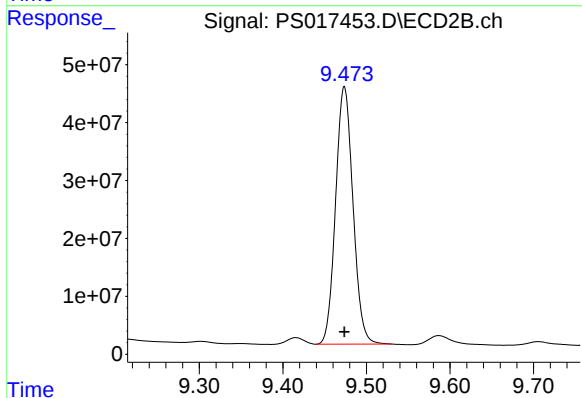


#13 2,4-DB

R.T.: 9.474 min
Delta R.T.: 0.000 min
Response: 643261959
Conc: 1433.99 ng/ml

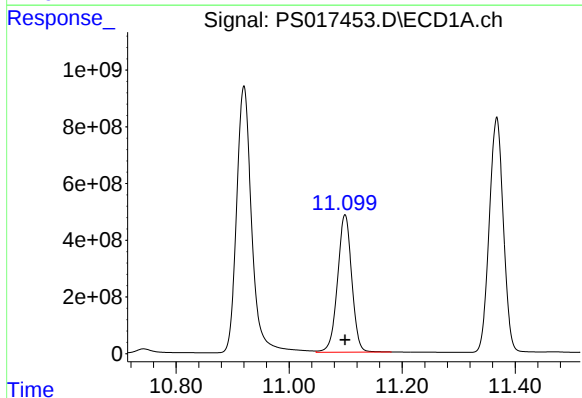


#14 DINOSEB

R.T.: 11.099 min
Delta R.T.: 0.000 min
Response: 8440858357
Conc: 1357.38 ng/ml

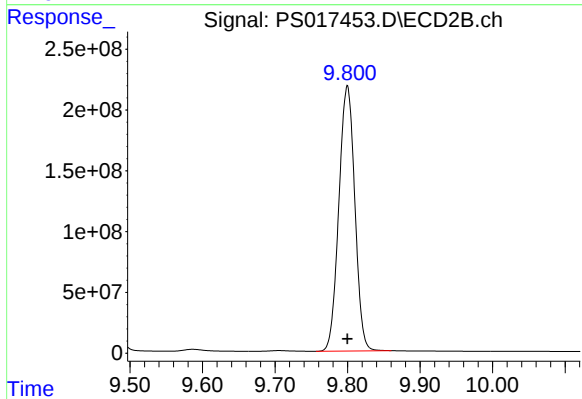

#14 DINOSEB


R.T.: 9.800 min
Delta R.T.: 0.000 min
Response: 3336672480
Conc: 1375.36 ng/ml

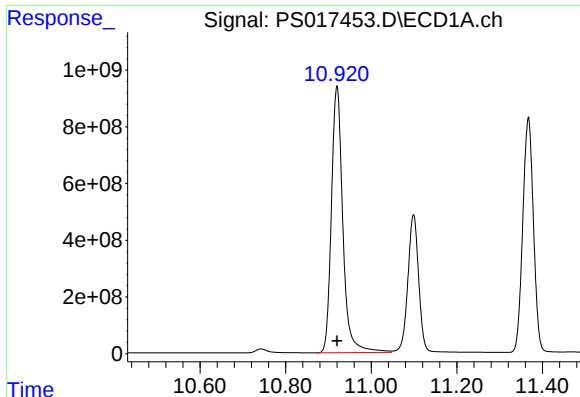

#15 Picloram


R.T.: 10.920 min
Delta R.T.: 0.000 min
Response: 1743246044
Conc: 1386.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC1500

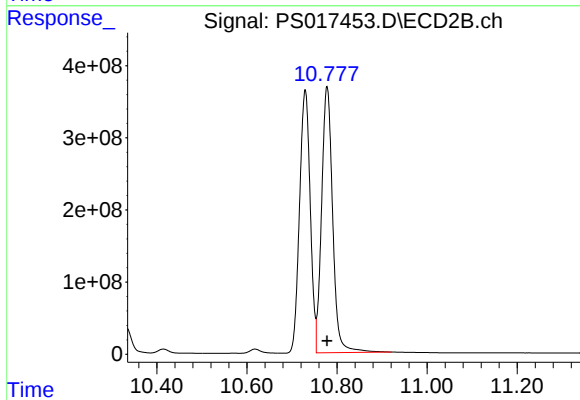


#15 Picloram

R.T.: 10.778 min
Delta R.T.: 0.000 min
Response: 6298349266
Conc: 1384.97 ng/ml

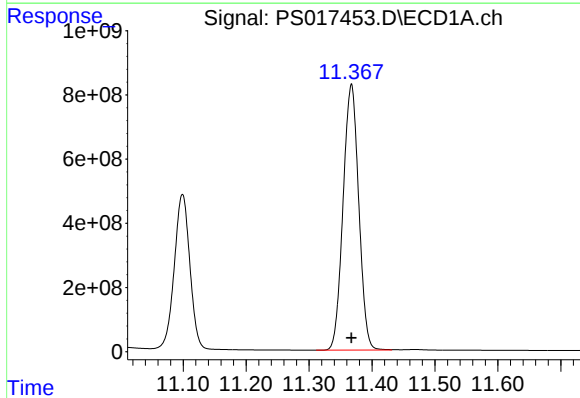

#16 DCPA

R.T.: 11.367 min
Delta R.T.: 0.000 min
Response: 14309539826
Conc: 1363.35 ng/ml

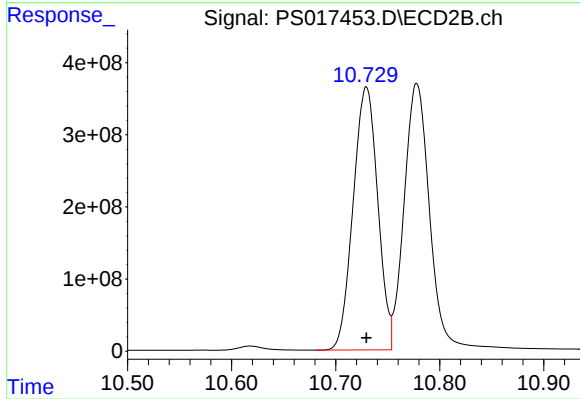

#16 DCPA

R.T.: 10.730 min
Delta R.T.: 0.000 min
Response: 5986158618
Conc: 1365.79 ng/ml