

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111822\
 Data File : PS021193.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2022 10:31
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 00:28:17 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
 Quant Title : 8080.M
 QLast Update : Thu Nov 17 00:46:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.409	6.843	987.8E6	757.0E6	454.304	500.619
Target Compounds							
1) T	Dalapon	2.490	0.000	125072	0	<MDL	N.D. #
3) T	4-Nitroph...	6.249	0.000	5145394	0	3.809	N.D. #
5) T	DICAMBA	0.000	7.065f	0	12326259	N.D.	1.791
6) T	MCP	6.785f	7.156f	921607	2573539	<MDL	<MDL #
7) T	MCPA	6.785f	0.000	921607	0	<MDL	N.D. #
9) T	2,4-D	7.335	0.000	4628007	0	1.631	N.D. #
10) T	Pentachlo...	7.578	0.000	1347174	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.120	0.000	3618894	0	<MDL	N.D. #
12) T	2,4,5-T	8.357	0.000	3033172	0	<MDL	N.D. #
13) T	2,4-DB	8.868	0.000	976037	0	<MDL	N.D. #
15) T	Picloram	9.764	10.858f	17104227	21361660	<MDL	1.655 #
16) T	DCPA	10.246f	10.858	803836	21361660	<MDL	1.784 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111822\
Data File : PS021193.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2022 10:31
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 00:28:17 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
Quant Title : 8080.M
QLast Update : Thu Nov 17 00:46:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

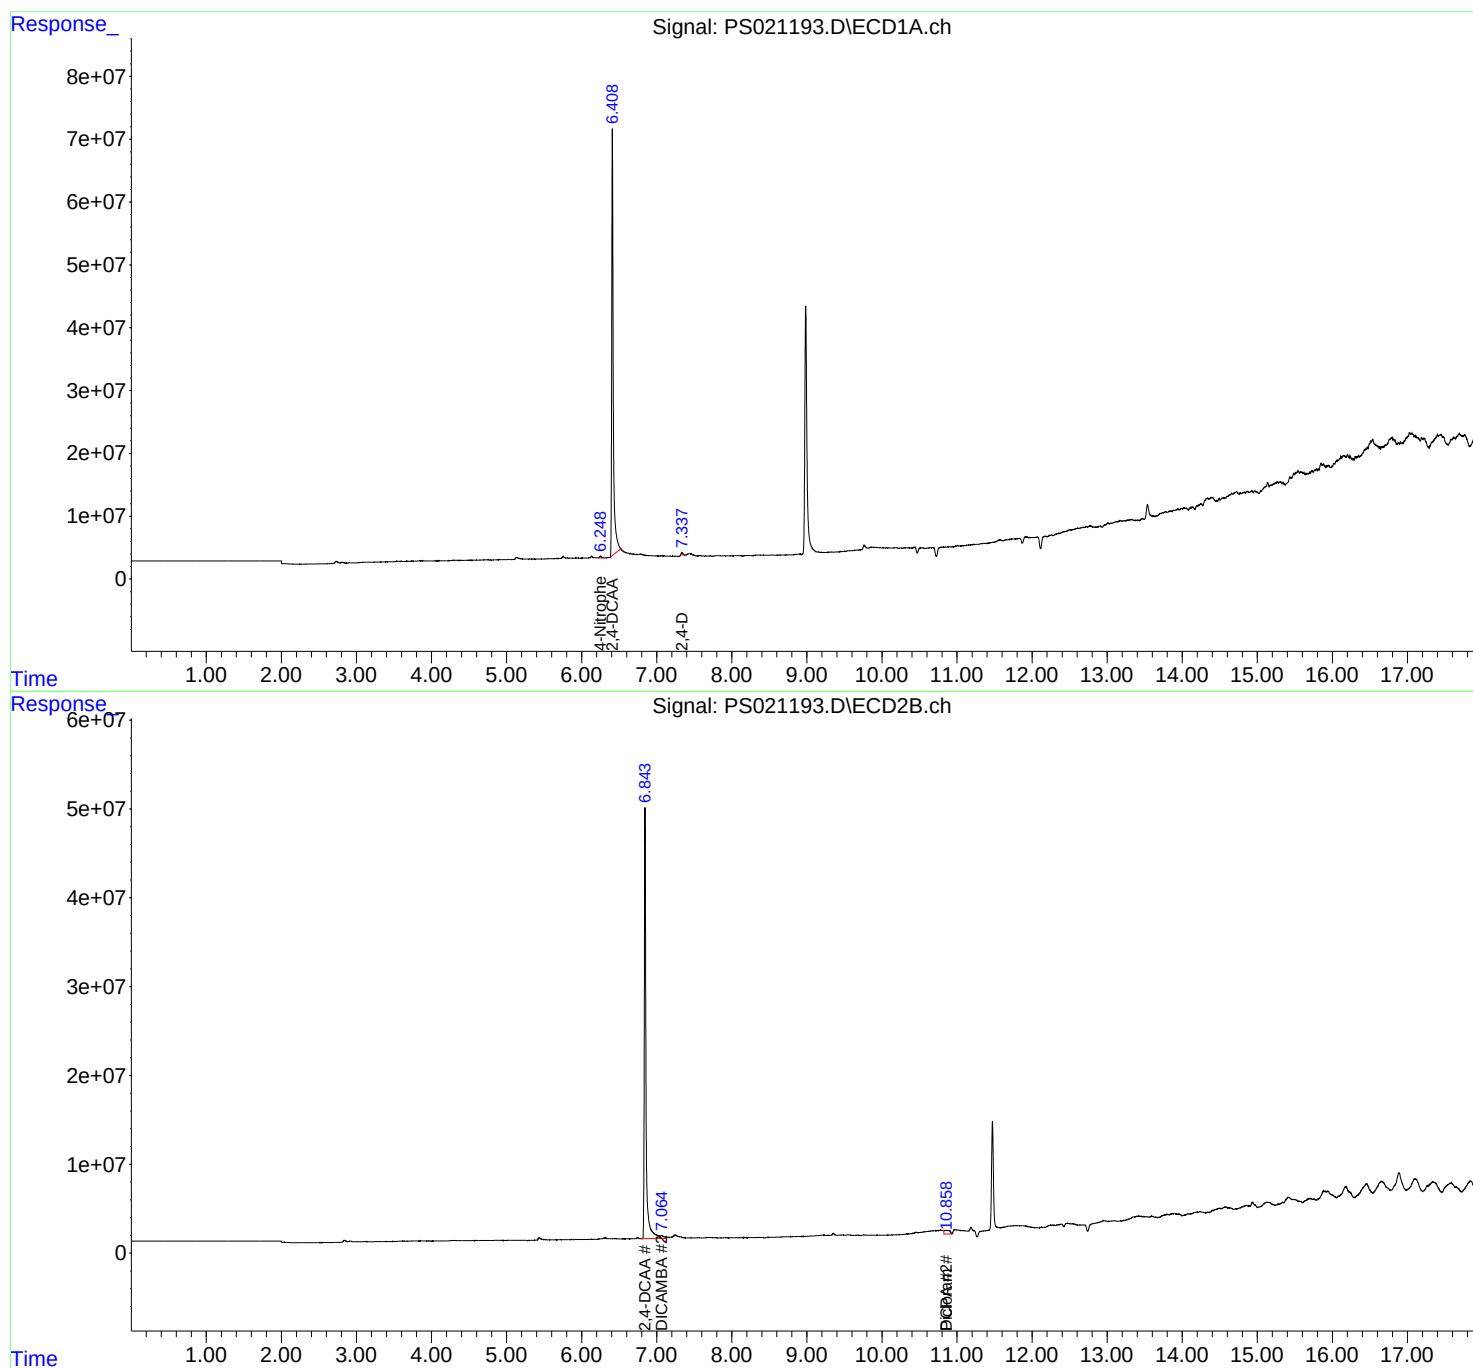


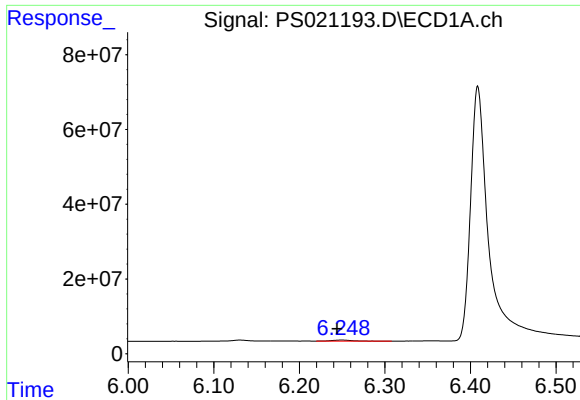

#3 4-Nitrophenol


R.T.: 6.249 min
Delta R.T.: 0.005 min
Response: 5145394
Conc: 3.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

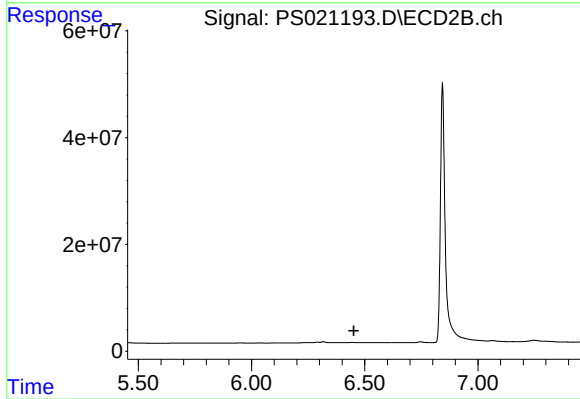


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.452 min
Response: 0
Conc: N.D.

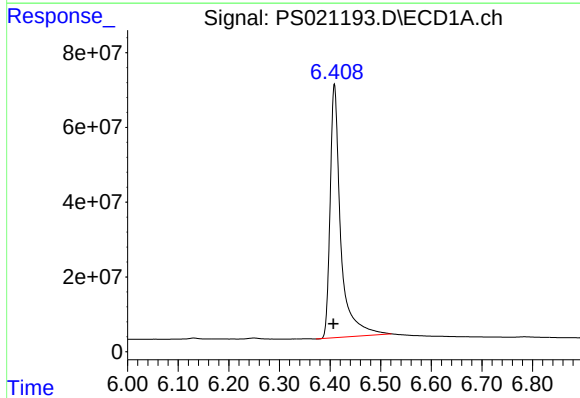


#4 2,4-DCAA

R.T.: 6.409 min
Delta R.T.: 0.002 min
Response: 987790432
Conc: 454.30 ng/ml

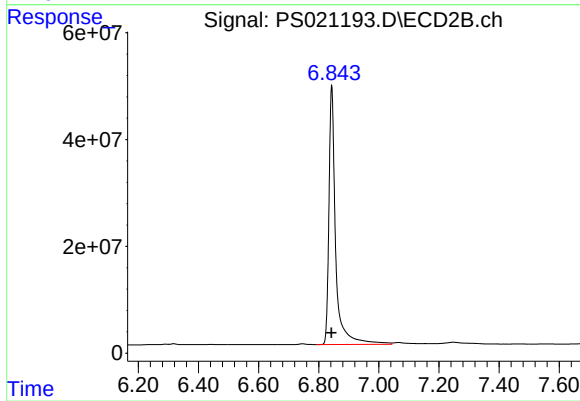

#4 2,4-DCAA


R.T.: 6.843 min
Delta R.T.: 0.001 min
Response: 756995226
Conc: 500.62 ng/ml

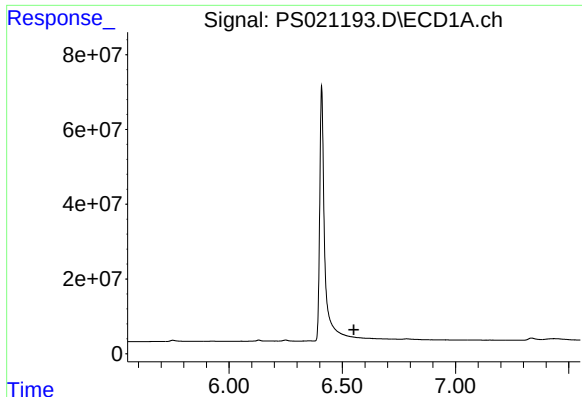

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.551 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

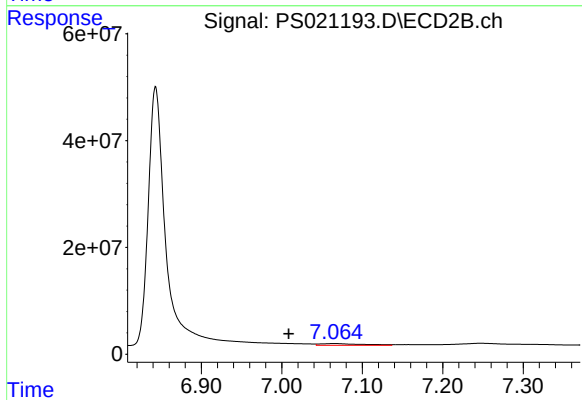


#5 DICAMBA

R.T.: 7.065 min
Delta R.T.: 0.057 min
Response: 12326259
Conc: 1.79 ng/ml

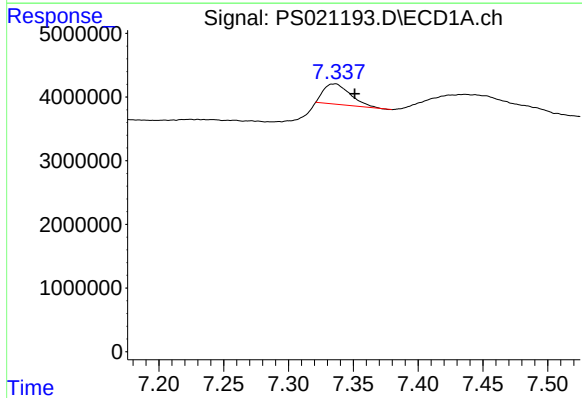


#9 2,4-D

R.T.: 7.335 min
Delta R.T.: -0.016 min
Response: 4628007
Conc: 1.63 ng/ml

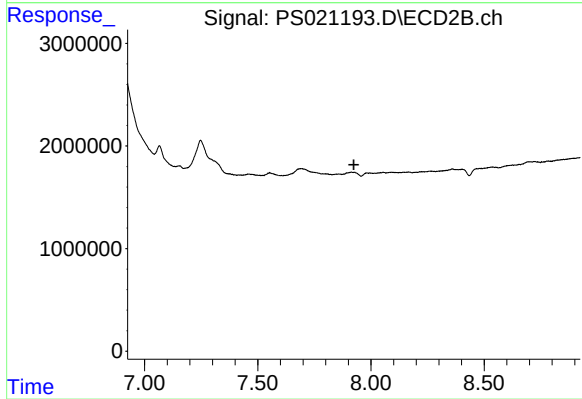

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.925 min
Response: 0
Conc: N.D.

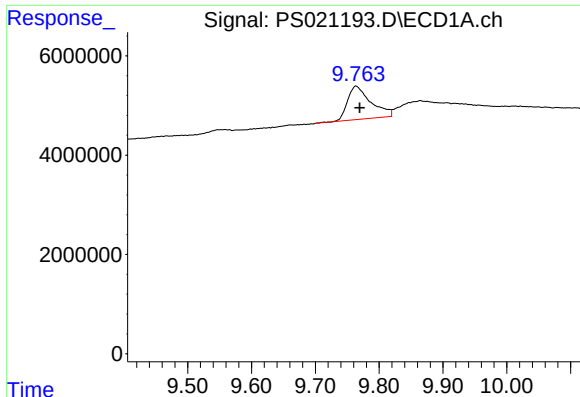

#15 Picloram


R.T.: 9.764 min
Delta R.T.: -0.005 min
Response: 17104227
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

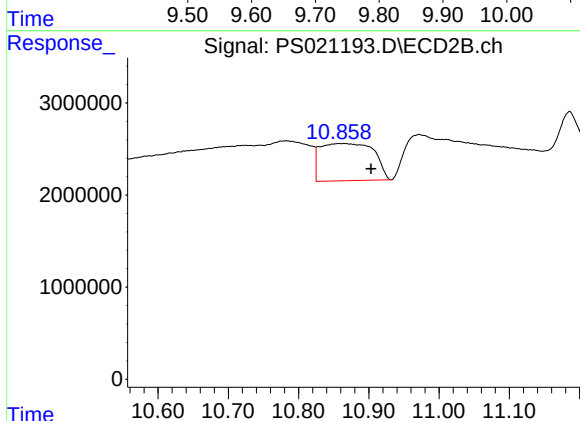


#15 Picloram

R.T.: 10.858 min
Delta R.T.: -0.046 min
Response: 21361660
Conc: 1.65 ng/ml

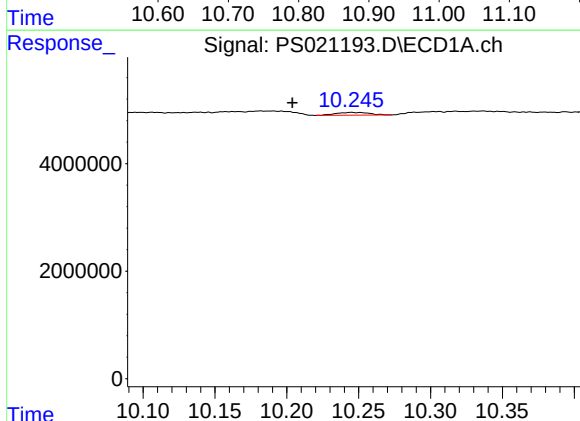

#16 DCPA

R.T.: 10.246 min
Delta R.T.: 0.042 min
Response: 803836
Conc: N.D.

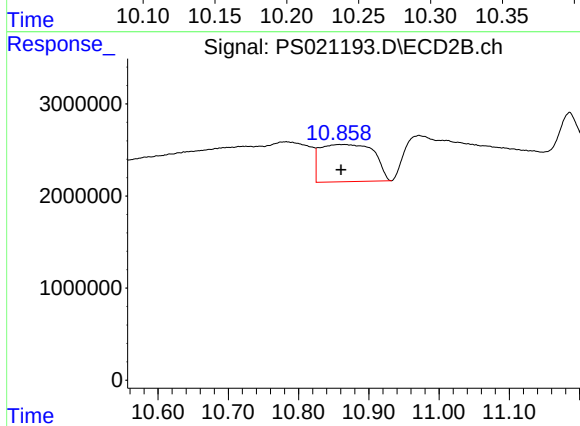

#16 DCPA

R.T.: 10.858 min
Delta R.T.: -0.003 min
Response: 21361660
Conc: 1.78 ng/ml