

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111822\
 Data File : PS021206.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2022 17:33
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 00:37:33 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
 Quant Title : 8080.M
 QLast Update : Thu Nov 17 00:46:07 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.409	6.844	1019.2E6	774.9E6	468.759	512.443
Target Compounds							
1) T	Dalapon	2.488	0.000	146375	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.707f	0.000	166085	0	<MDL	N.D. #
3) T	4-Nitroph...	6.248	0.000	6242414	0	4.621	N.D. #
5) T	DICAMBA	0.000	7.005	0	7698884	N.D.	1.119
6) T	MCPD	6.723	7.065f	-1029959	6456580	N.D.	1.238
7) T	MCPA	6.785f	0.000	6639581	0	<MDL	N.D. #
8) T	DICHLORPROP	7.166	7.682f	649269	3743158	<MDL	2.192 #
9) T	2,4-D	7.337	0.000	6071486	0	2.140	N.D. #
10) T	Pentachlo...	7.587	8.357	3117031	3984983	<MDL	<MDL #
11) T	2,4,5-TP ...	8.124	8.726	3857325	8573340	<MDL	<MDL #
12) T	2,4,5-T	8.341	9.127	21126588	4088574	1.501	<MDL #
13) T	2,4-DB	8.873	9.547f	1188536	2036545	<MDL	1.740 #
14) T	DINOSEB	0.000	9.934	0	1745934	N.D.	<MDL
15) T	Picloram	9.765	10.862f	19047523	13115499	<MDL	1.016 #
16) T	DCPA	10.204	10.862	2704435	13115499	<MDL	1.095 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111822\
Data File : PS021206.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2022 17:33
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 00:37:33 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111622.M
Quant Title : 8080.M
QLast Update : Thu Nov 17 00:46:07 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

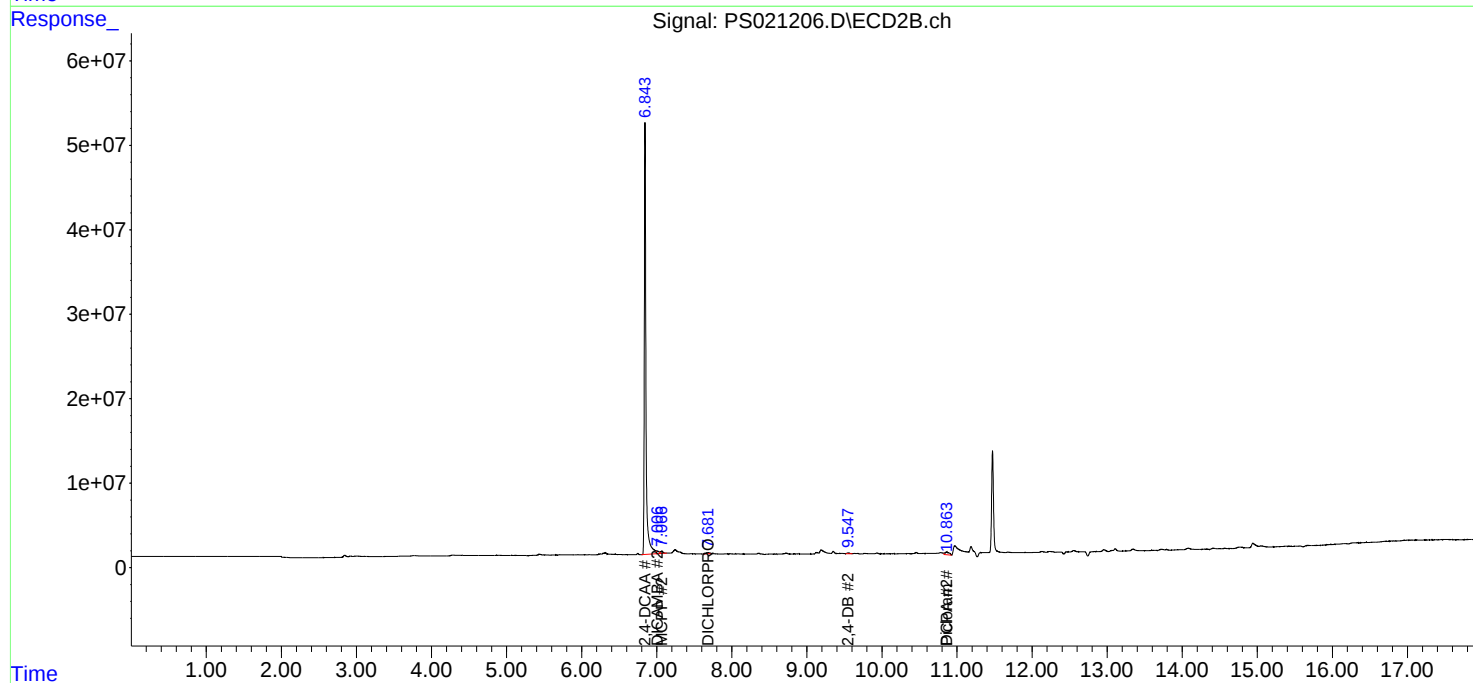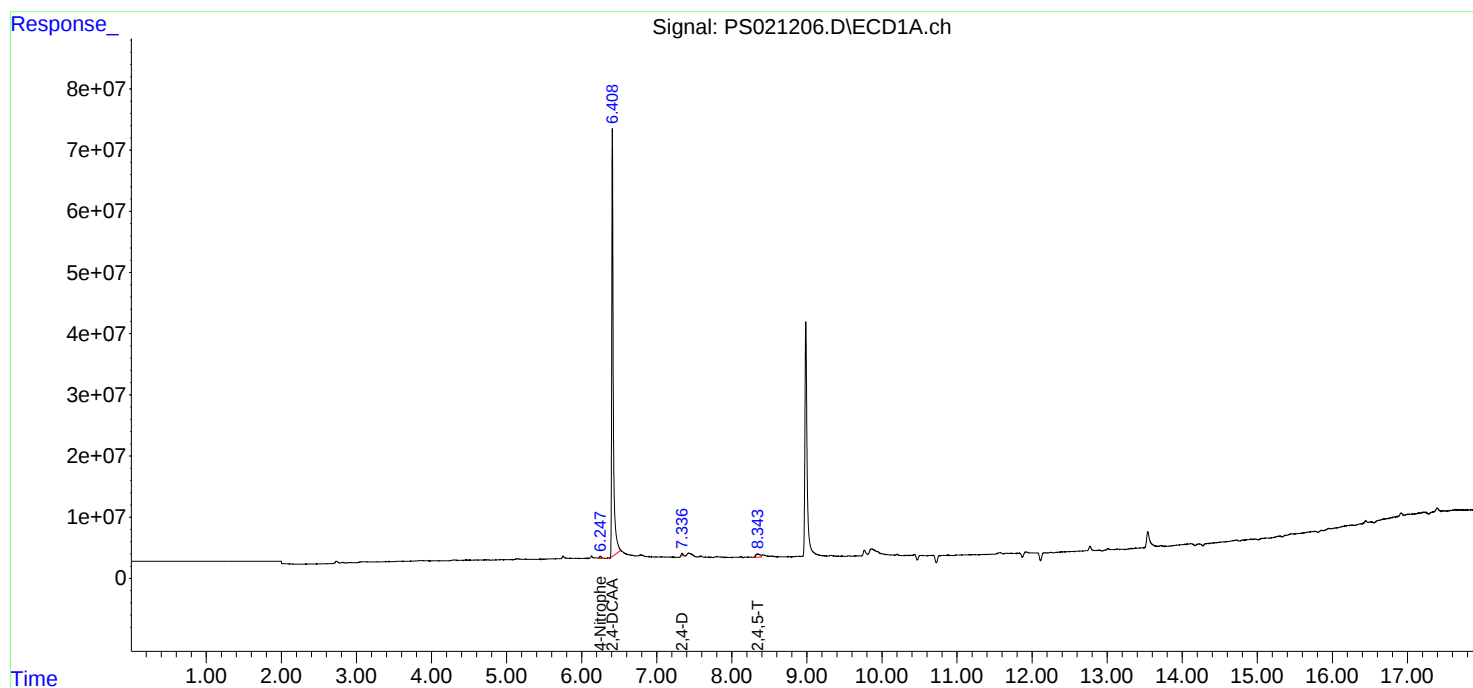


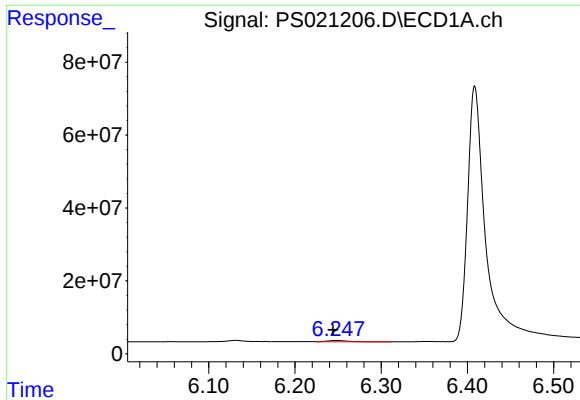

#3 4-Nitrophenol


R.T.: 6.248 min
Delta R.T.: 0.004 min
Response: 6242414
Conc: 4.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

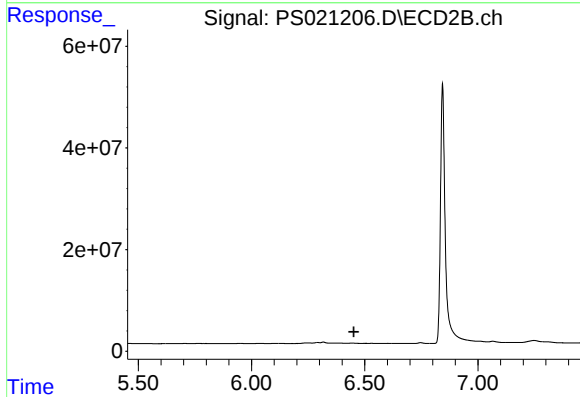


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.452 min
Response: 0
Conc: N.D.

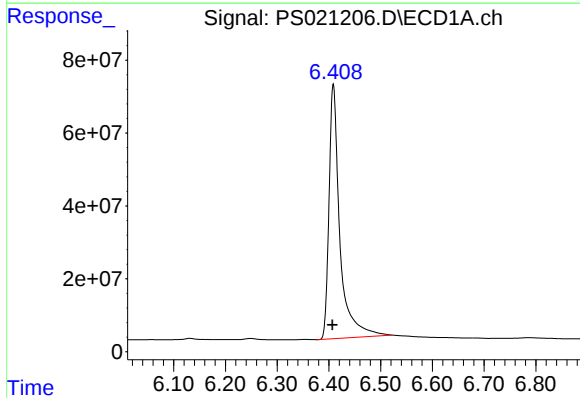


#4 2,4-DCAA

R.T.: 6.409 min
Delta R.T.: 0.002 min
Response: 1019220661
Conc: 468.76 ng/ml

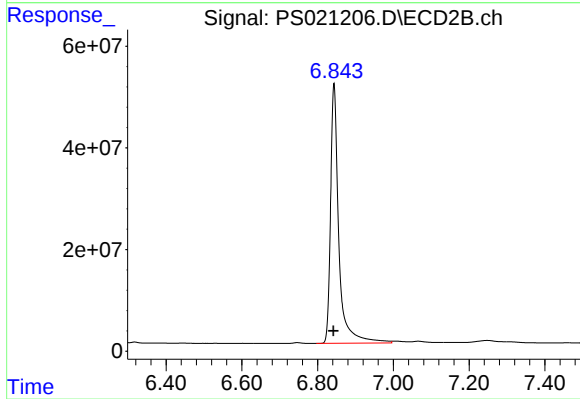

#4 2,4-DCAA


R.T.: 6.844 min
Delta R.T.: 0.002 min
Response: 774874721
Conc: 512.44 ng/ml

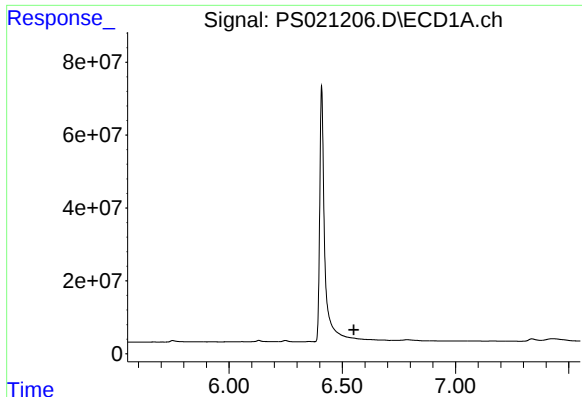

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.551 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

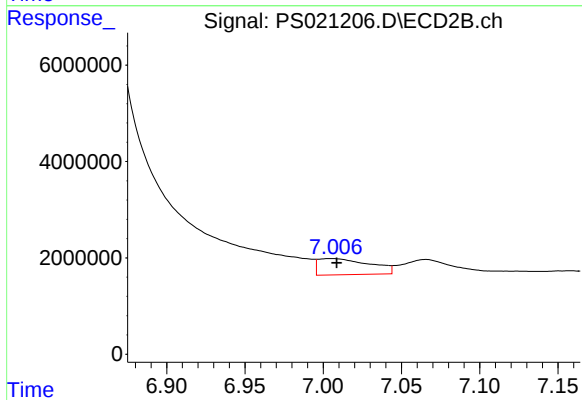


#5 DICAMBA

R.T.: 7.005 min
Delta R.T.: -0.003 min
Response: 7698884
Conc: 1.12 ng/ml

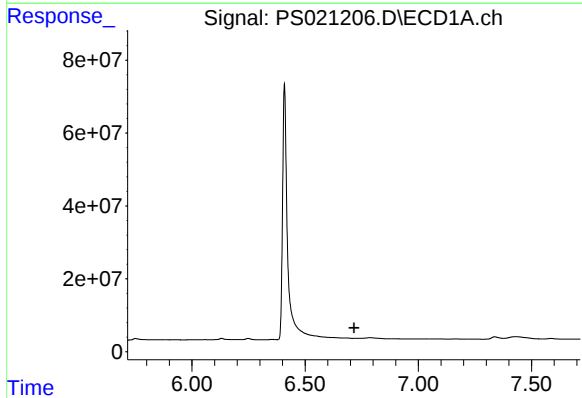


#6 MCP

R.T.: 6.723 min
Delta R.T.: 0.008 min
Response: -1029959
Conc: N.D.

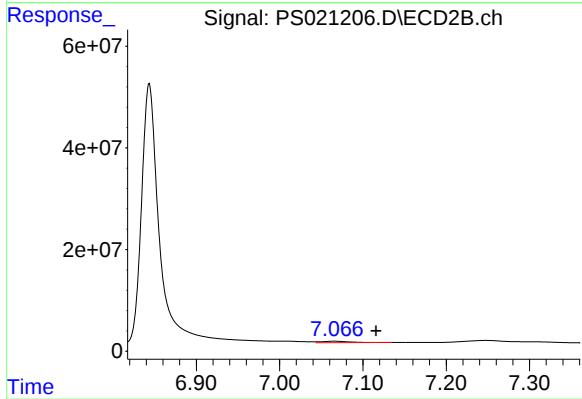

#6 MCP


R.T.: 7.065 min
Delta R.T.: -0.050 min
Response: 6456580
Conc: 1.24 ug/ml

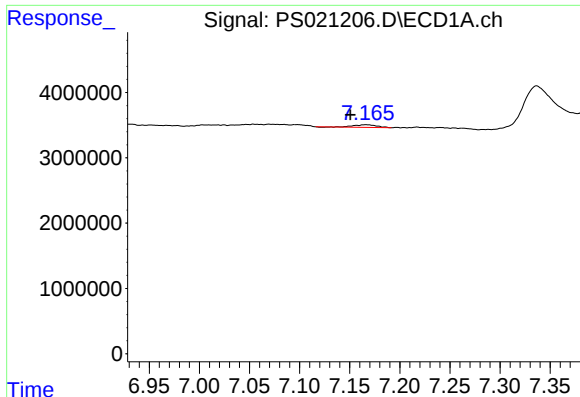

#8 DICHLORPROP


R.T.: 7.166 min
Delta R.T.: 0.015 min
Response: 649269
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

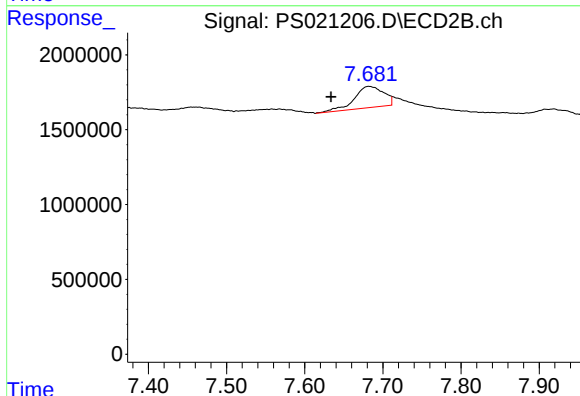


#8 DICHLORPROP

R.T.: 7.682 min
Delta R.T.: 0.049 min
Response: 3743158
Conc: 2.19 ng/ml

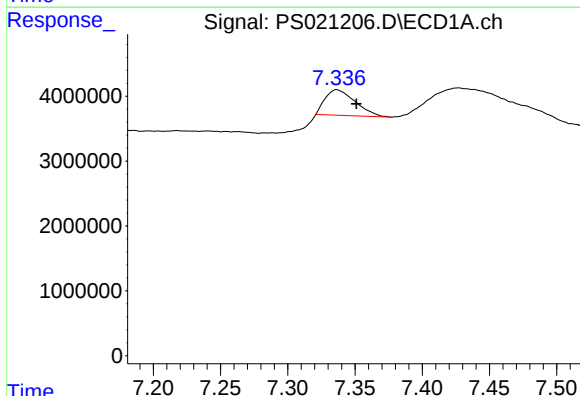


#9 2,4-D

R.T.: 7.337 min
Delta R.T.: -0.014 min
Response: 6071486
Conc: 2.14 ng/ml

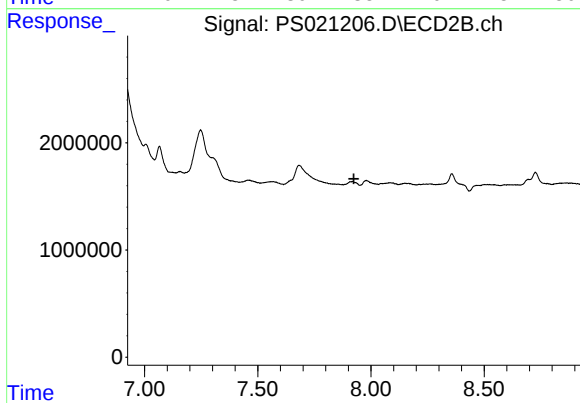

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.925 min
Response: 0
Conc: N.D.

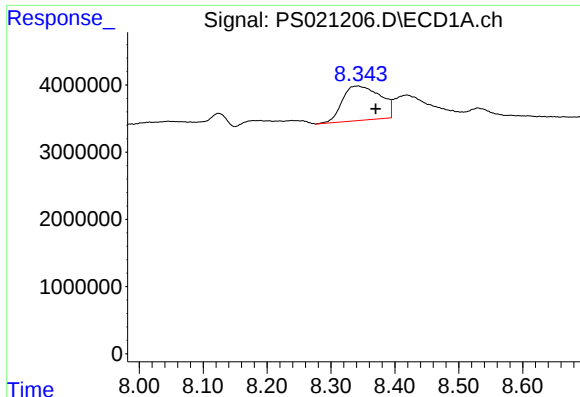

#12 2,4,5-T


R.T.: 8.341 min
Delta R.T.: -0.029 min
Response: 21126588
Conc: 1.50 ng/ml

Instrument :
ECD_S
ClientSampleId :

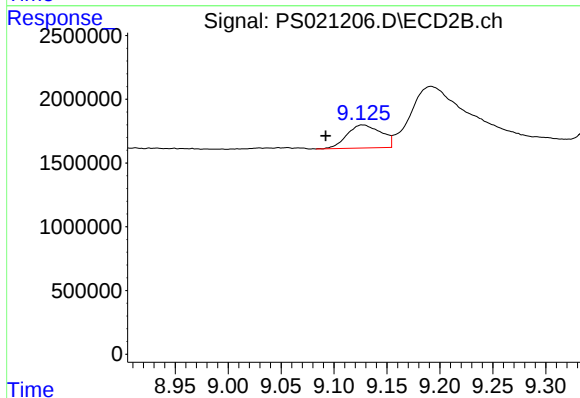


#12 2,4,5-T

R.T.: 9.127 min
Delta R.T.: 0.035 min
Response: 4088574
Conc: N.D.

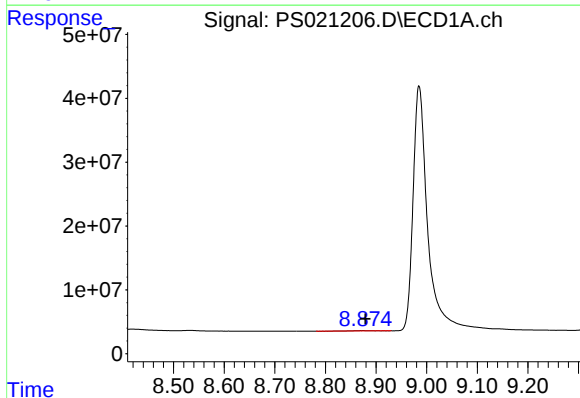


#13 2,4-DB

R.T.: 8.873 min
Delta R.T.: -0.006 min
Response: 1188536
Conc: N.D.

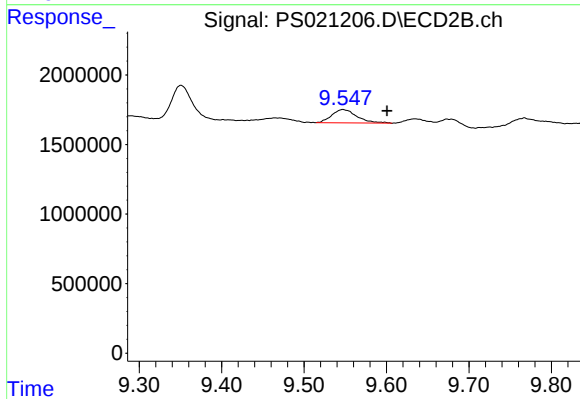

#13 2,4-DB


R.T.: 9.547 min
Delta R.T.: -0.053 min
Response: 2036545
Conc: 1.74 ng/ml

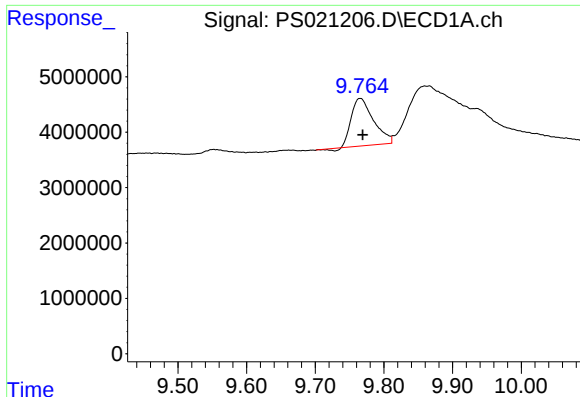

#15 Picloram


R.T.: 9.765 min
Delta R.T.: -0.004 min
Response: 19047523
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

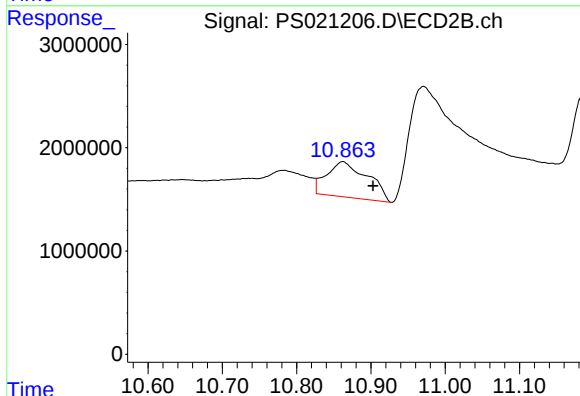


#15 Picloram

R.T.: 10.862 min
Delta R.T.: -0.041 min
Response: 13115499
Conc: 1.02 ng/ml

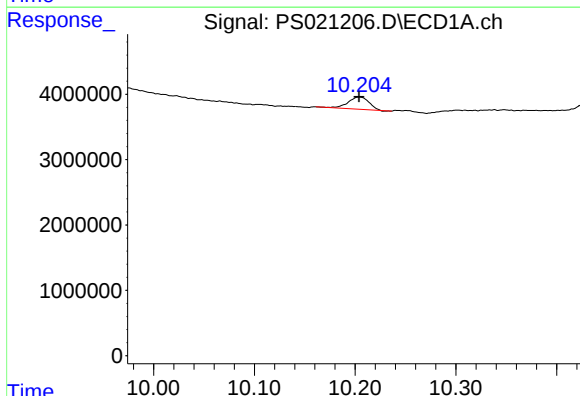

#16 DCPA

R.T.: 10.204 min
Delta R.T.: 0.000 min
Response: 2704435
Conc: N.D.

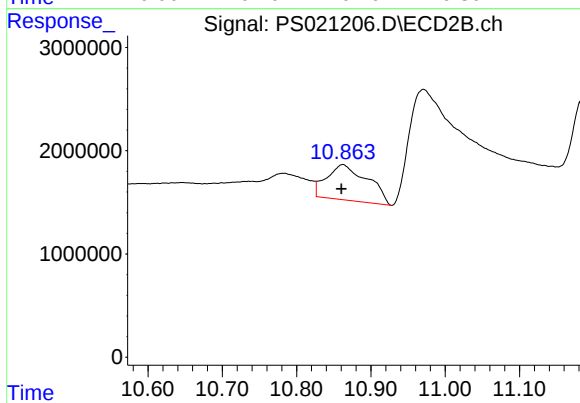

#16 DCPA

R.T.: 10.862 min
Delta R.T.: 0.002 min
Response: 13115499
Conc: 1.10 ng/ml