

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111824\
 Data File : PS028547.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 14:18
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 02:40:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 13 13:41:03 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.236	7.736	1434.0E6	649.0E6	561.075	502.199
Target Compounds							
1) T	Dalapon	2.665f	0.000	3337488	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.425	0.000	292933	0	<MDL	N.D. #
3) T	4-Nitroph...	7.032	0.000	5243358	0	3.087	N.D. #
7) T	MCPA	7.764	8.268f	134883	16602970	<MDL	2.681 #
8) T	DICHLORPROP	0.000	8.704f	0	2359561	N.D.	1.616
12) T	2,4,5-T	9.545	0.000	279192	0	<MDL	N.D. #
14) T	DINOSEB	11.326	0.000	919597	0	<MDL	N.D. #
15) T	Picloram	11.135	12.352	33487250	16842495	1.189	1.488 #
16) T	DCPA	11.611	12.352f	2028335	16842495	<MDL	1.737 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111824\
Data File : PS028547.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 14:18
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:40:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111324.M
Quant Title : 8080.M
QLast Update : Wed Nov 13 13:41:03 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

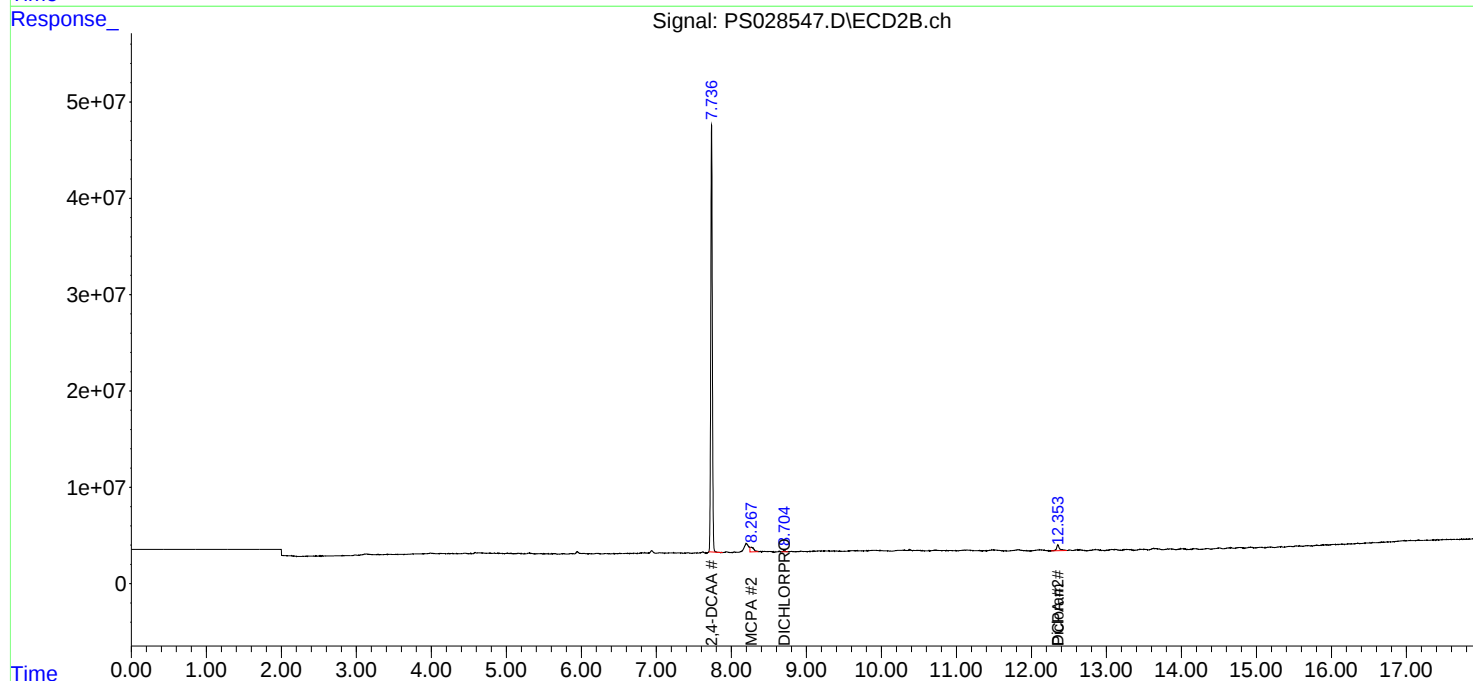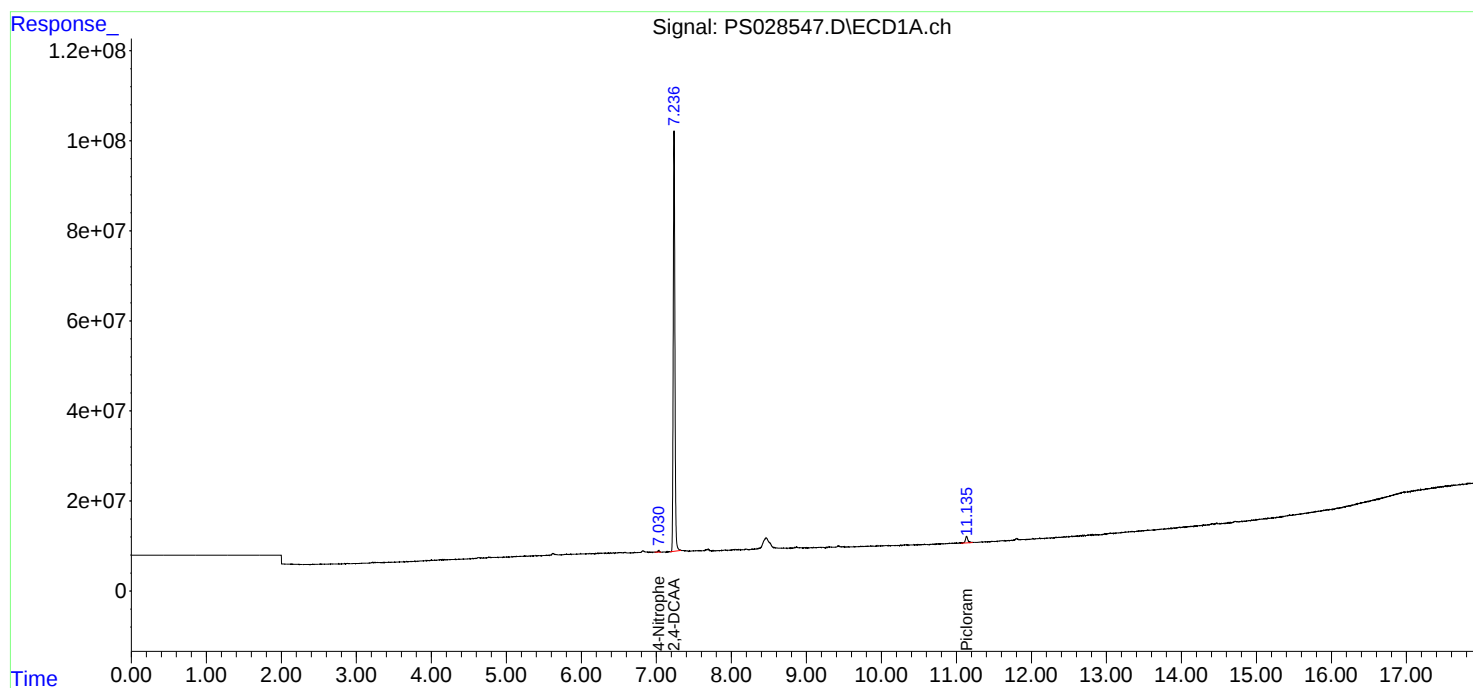


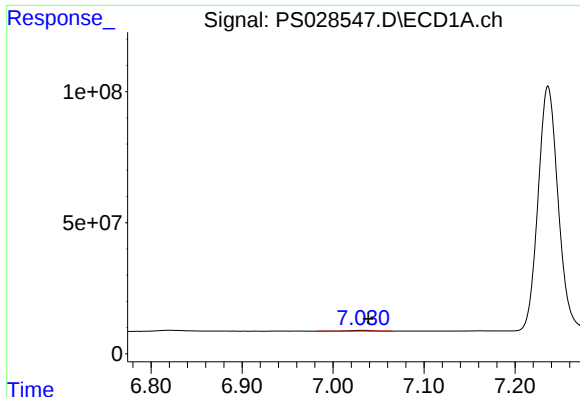

#3 4-Nitrophenol


R.T.: 7.032 min
Delta R.T.: -0.007 min
Response: 5243358
Conc: 3.09 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

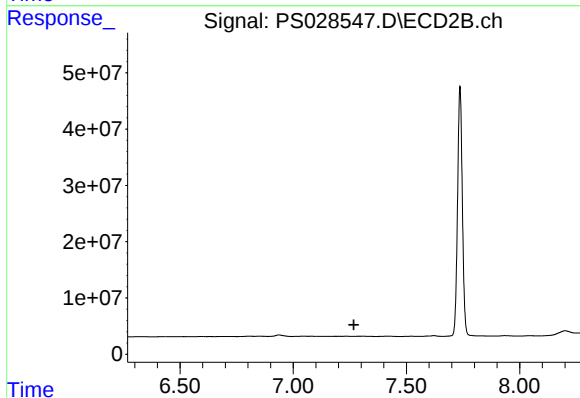


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.268 min
Response: 0
Conc: N.D.

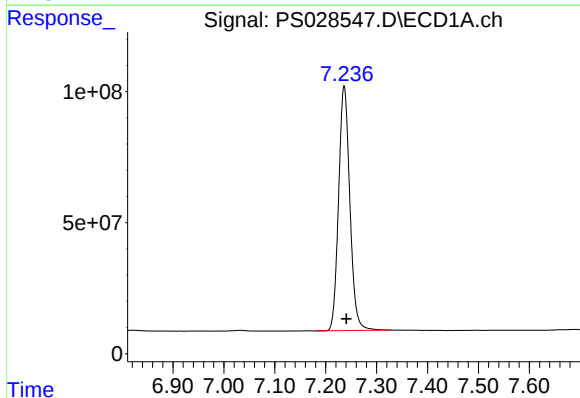


#4 2,4-DCAA

R.T.: 7.236 min
Delta R.T.: -0.005 min
Response: 1434041212
Conc: 561.07 ng/ml

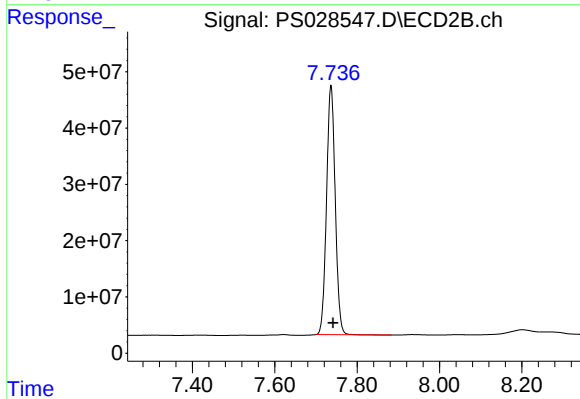

#4 2,4-DCAA


R.T.: 7.736 min
Delta R.T.: -0.005 min
Response: 648994709
Conc: 502.20 ng/ml

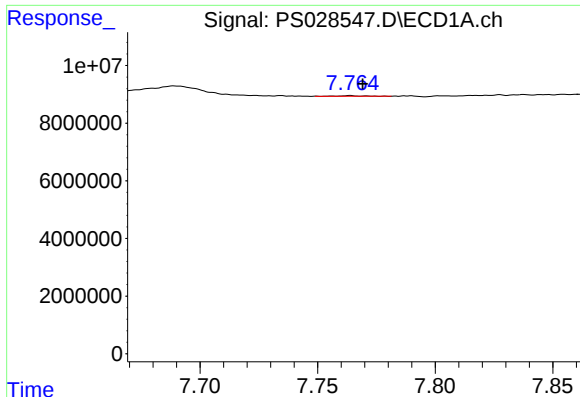

#7 MCPA


R.T.: 7.764 min
Delta R.T.: -0.005 min
Response: 134883
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

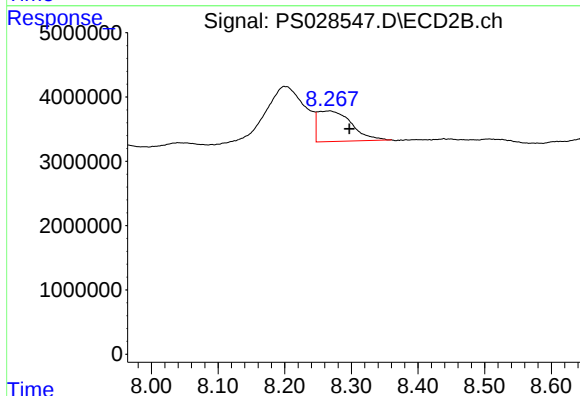


#7 MCPA

R.T.: 8.268 min
Delta R.T.: -0.030 min
Response: 16602970
Conc: 2.68 ug/ml

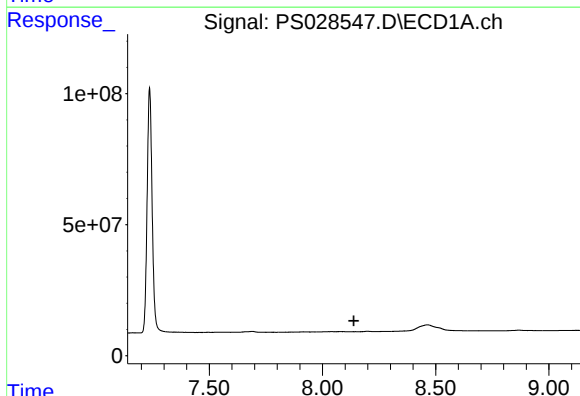


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.139 min
Response: 0
Conc: N.D.

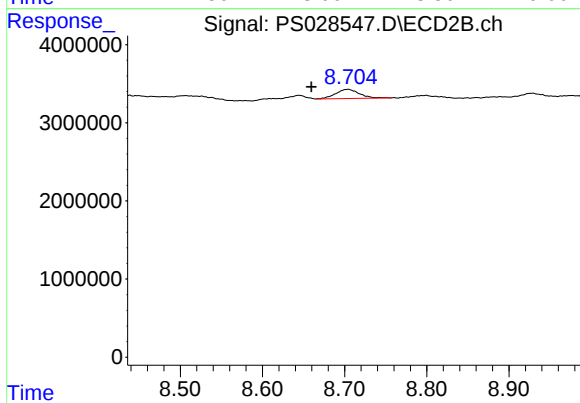

#8 DICHLORPROP


R.T.: 8.704 min
Delta R.T.: 0.045 min
Response: 2359561
Conc: 1.62 ng/ml

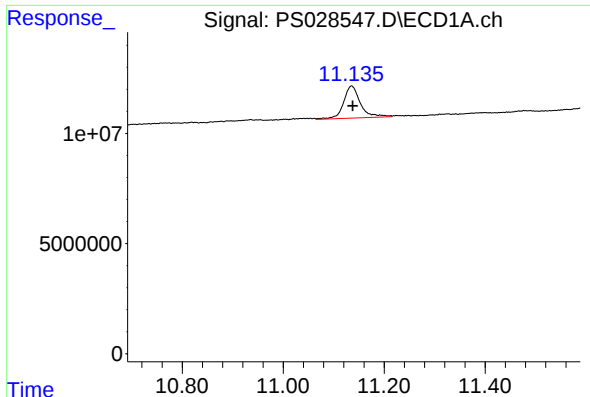

#15 Picloram


R.T.: 11.135 min
Delta R.T.: -0.002 min
Response: 33487250
Conc: 1.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

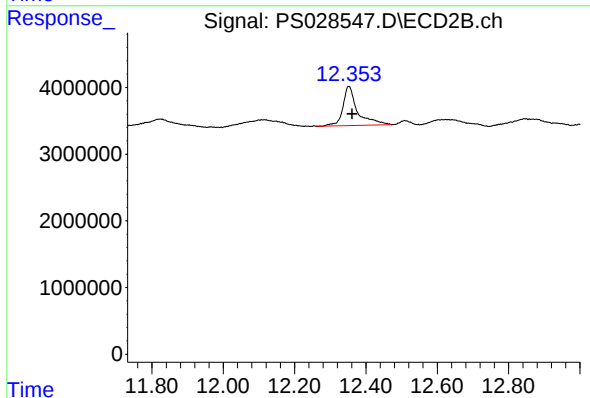


#15 Picloram

R.T.: 12.352 min
Delta R.T.: -0.009 min
Response: 16842495
Conc: 1.49 ng/ml

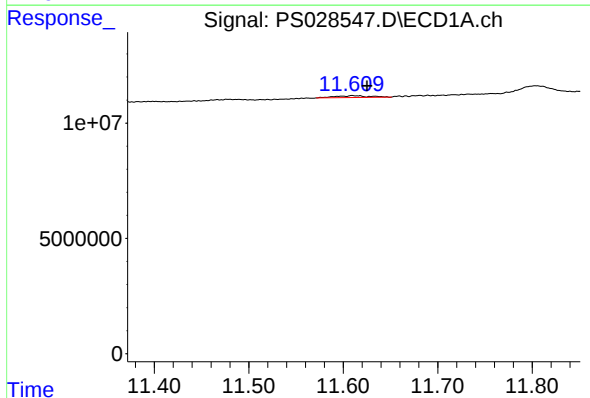

#16 DCPA

R.T.: 11.611 min
Delta R.T.: -0.014 min
Response: 2028335
Conc: N.D.

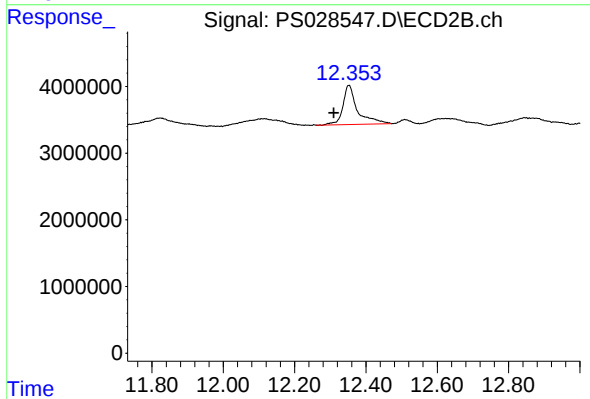

#16 DCPA

R.T.: 12.352 min
Delta R.T.: 0.043 min
Response: 16842495
Conc: 1.74 ng/ml