

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111825\
 Data File : PS032455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2025 09:17
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 13:38:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.280	0.000	772873	0	<MDL	N.D. #
Target Compounds							
2) T	3,5-DICHL...	6.446	0.000	7880718	0	1.219	N.D. #
3) T	4-Nitroph...	7.129f	0.000	325835	0	<MDL	N.D. #
5) T	DICAMBA	7.446	7.840f	1088912	5433107	<MDL	<MDL #
6) T	MCP	7.641	7.904	390702	11783612	<MDL	<MDL #
7) T	MCPA	7.792	0.000	1668622	0	<MDL	N.D. #
8) T	DICHLORPROP	8.167	0.000	286615	0	<MDL	N.D. #
9) T	2,4-D	8.412	0.000	1748238	0	<MDL	N.D. #
10) T	Pentachlo...	8.710	0.000	1971331	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.271	9.780f	567141	1817594	<MDL	<MDL #
12) T	2,4,5-T	9.580	0.000	2837444	0	<MDL	N.D. #
13) T	2,4-DB	10.150	0.000	416846	0	<MDL	N.D. #
14) T	DINOSEB	11.358	11.112	3310258	372362	<MDL	<MDL #
15) T	Picloram	11.202	12.195f	5439553	2266800	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111825\
Data File : PS032455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2025 09:17
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 13:38:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

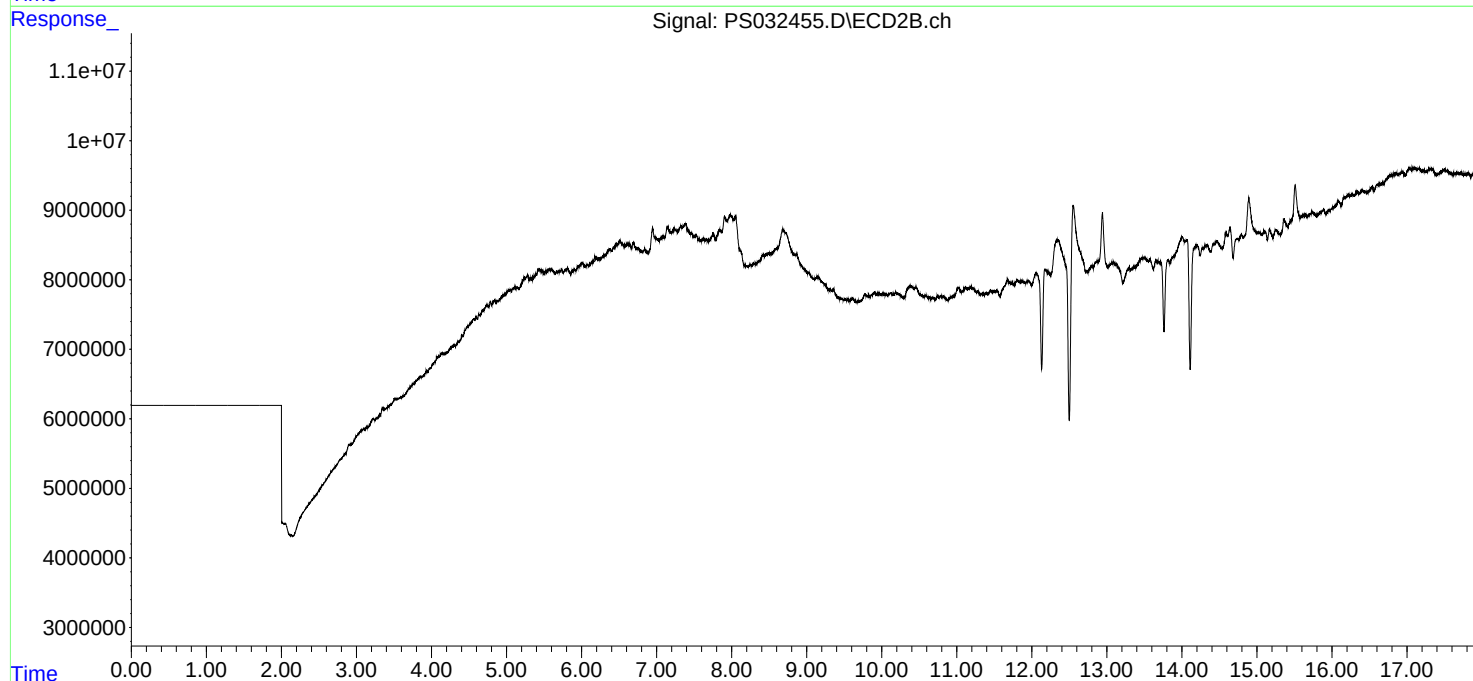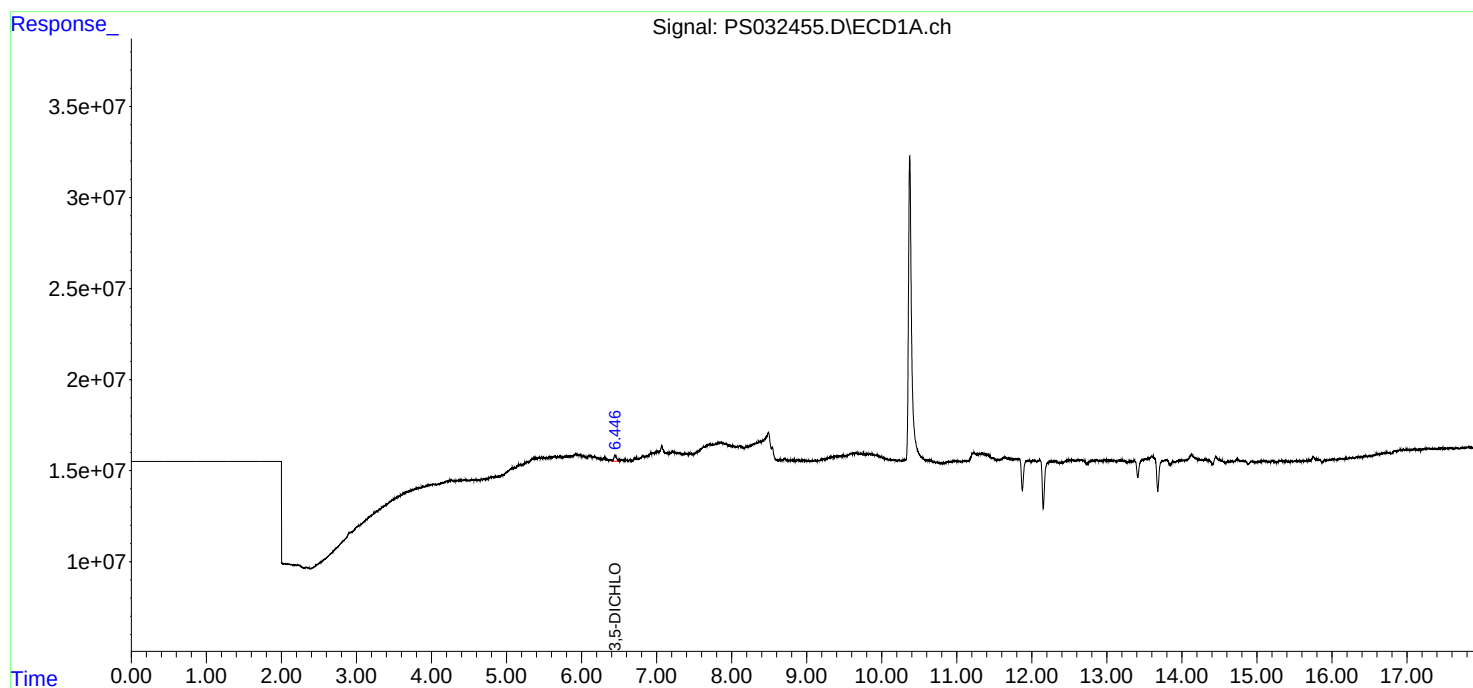

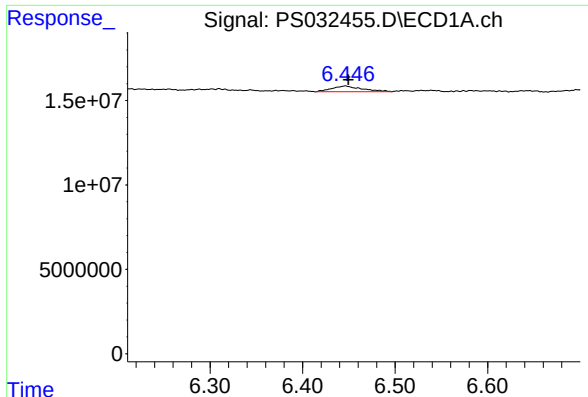


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.446 min
Delta R.T.: -0.003 min
Response: 7880718
Conc: 1.22 ng/ml

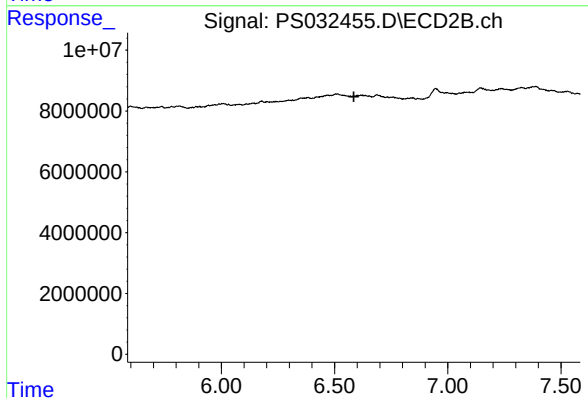


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.585 min
Response: 0
Conc: N.D.

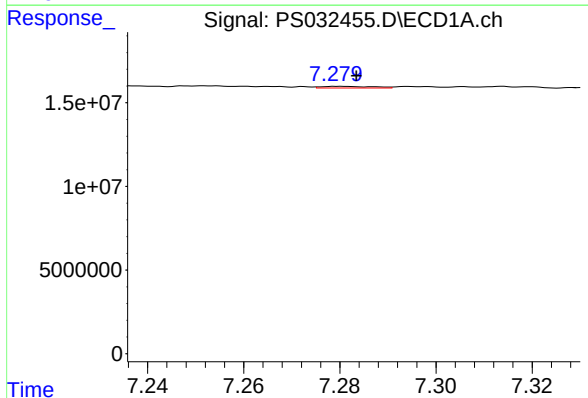

#4 2,4-DCAA

R.T.: 7.280 min
Delta R.T.: -0.003 min
Response: 772873
Conc: N.D.

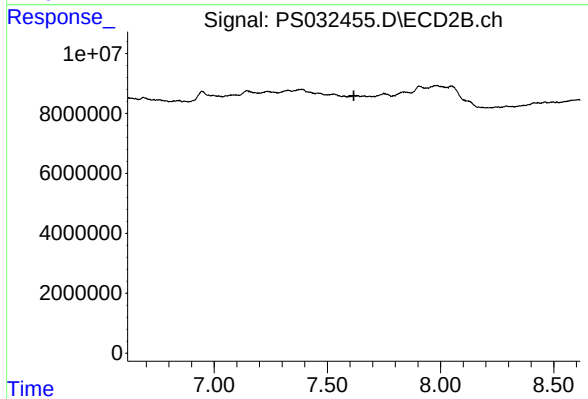

#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 7.617 min
Response: 0
Conc: N.D.