

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111825\
 Data File : PS032460.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2025 12:38
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 13:41:05 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	



System Monitoring Compounds								
4) S	2,4-DCAA	7.287	7.622	1684.9E6	1987.2E6	371.847	545.107	#
Target Compounds								
2) T	3,5-DICHL...	6.448	6.631f	9050084	4435668	1.400	<MDL	#
3) T	4-Nitroph...	7.129f	0.000	251485	0	<MDL	N.D.	#
6) T	MCP	7.627	7.911	-3635	226.1E6	N.D.	16.996	
7) T	MCPA	7.792	0.000	191839	0	<MDL	N.D.	#
8) T	DICHLORPROP	8.169	0.000	312917	0	<MDL	N.D.	#
9) T	2,4-D	8.419	0.000	2466970	0	<MDL	N.D.	#
10) T	Pentachlo...	8.715	0.000	6145993	0	<MDL	N.D.	#
11) T	2,4,5-TP ...	9.274	0.000	2887026	0	<MDL	N.D.	#
12) T	2,4,5-T	9.601	10.190	7965064	3866935	<MDL	<MDL	#
13) T	2,4-DB	10.185f	10.750	284392	3564902	<MDL	<MDL	#
14) T	DINOSEB	11.354	11.121	11517688	1673110	<MDL	<MDL	#
15) T	Picloram	0.000	12.204	0	65526539	N.D.	1.762	
16) T	DCPA	11.644	0.000	5119520	0	<MDL	N.D.	#


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111825\
Data File : PS032460.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2025 12:38
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 13:41:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

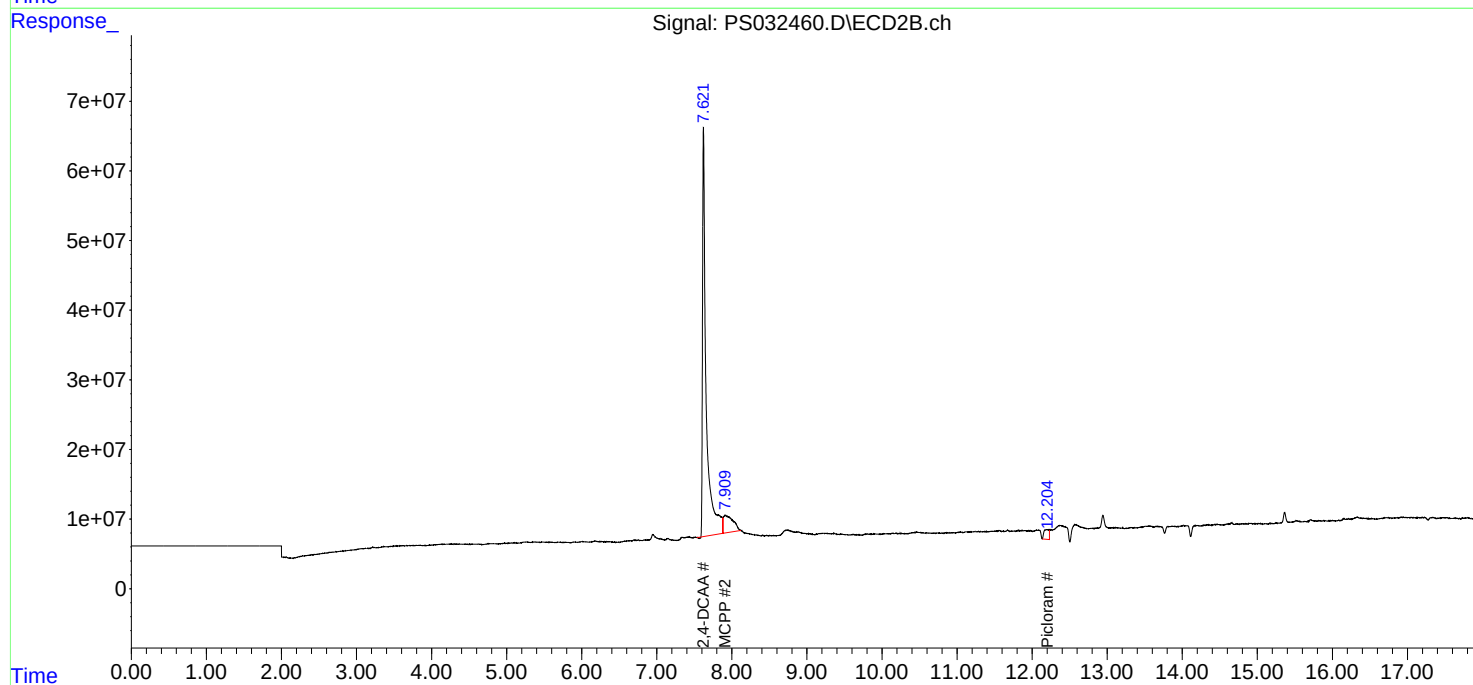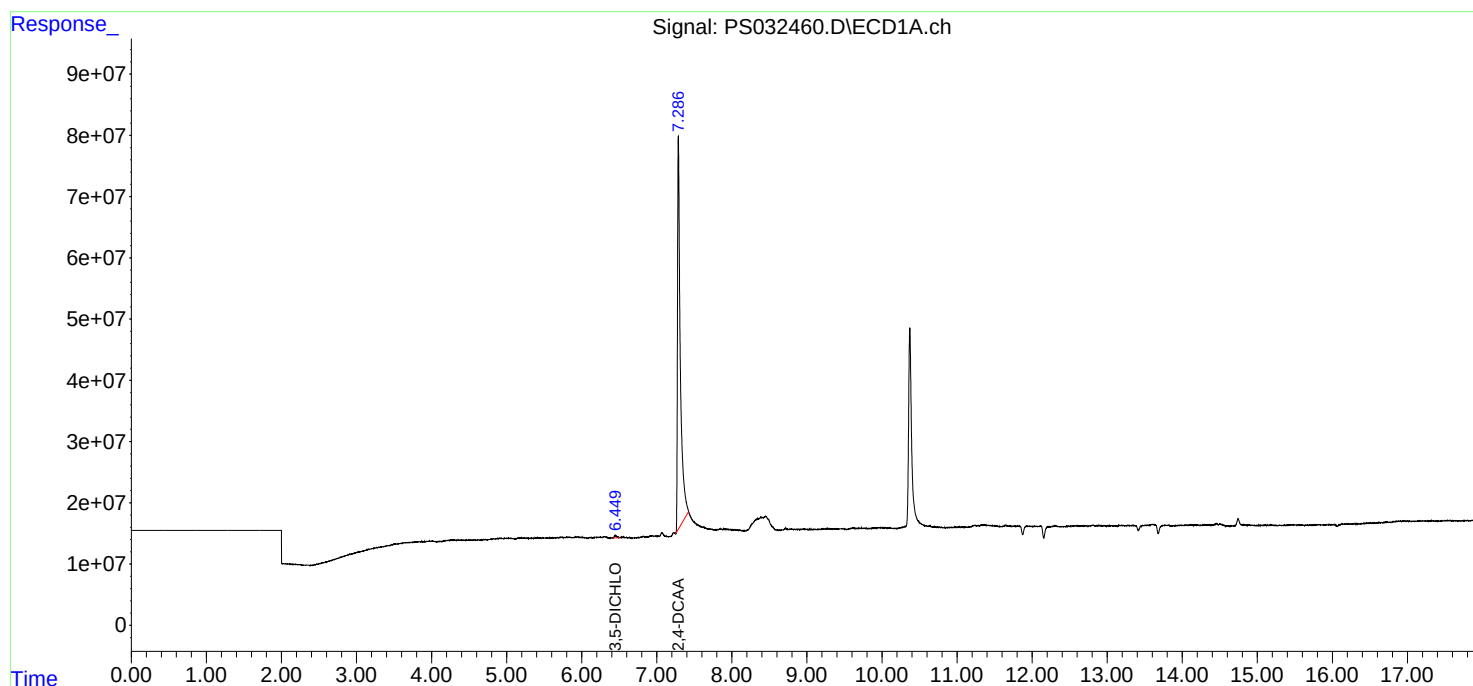

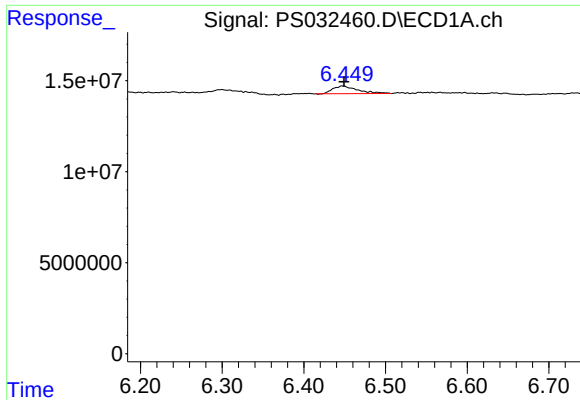


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.448 min
Delta R.T.: -0.001 min
Response: 9050084
Conc: 1.40 ng/ml

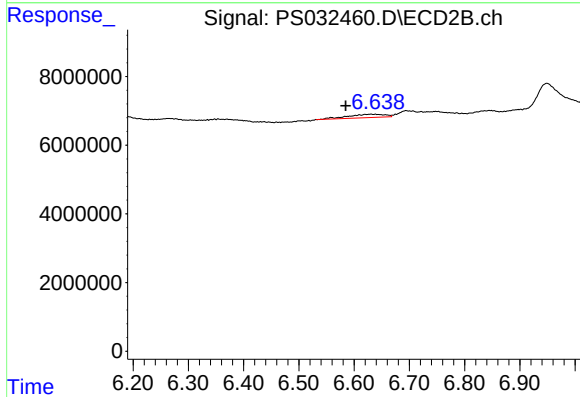


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.631 min
Delta R.T.: 0.045 min
Response: 4435668
Conc: N.D.

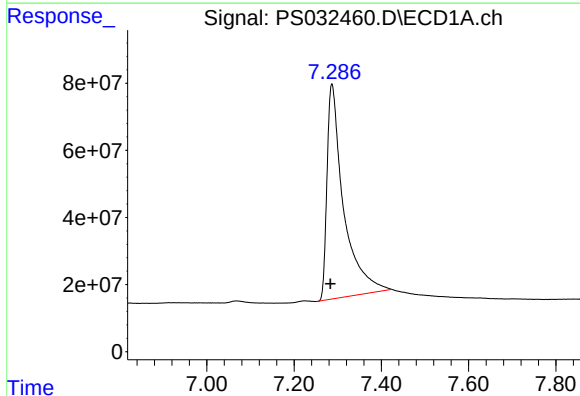


#4 2,4-DCAA

R.T.: 7.287 min
Delta R.T.: 0.003 min
Response: 1684941090
Conc: 371.85 ng/ml

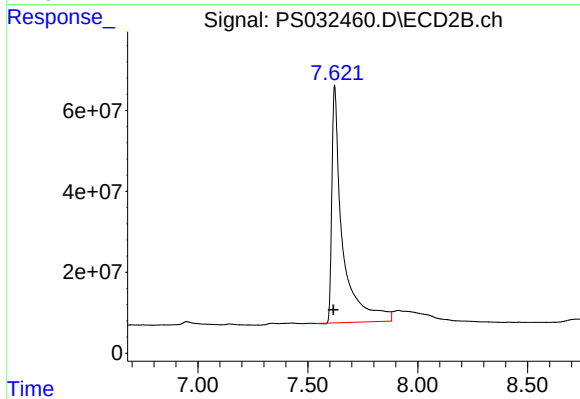


#4 2,4-DCAA

R.T.: 7.622 min
Delta R.T.: 0.005 min
Response: 1987184969
Conc: 545.11 ng/ml

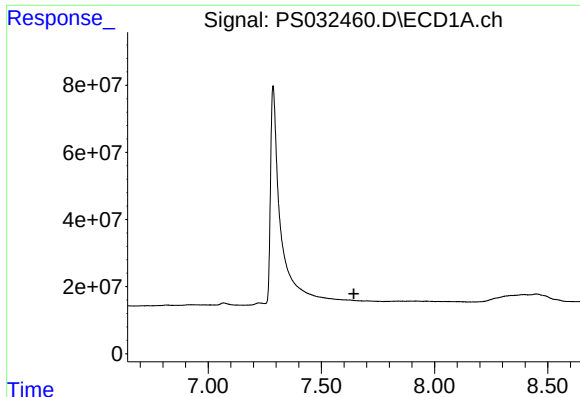


#6 MCP

R.T.: 7.627 min
Delta R.T.: -0.017 min
Response: -3635
Conc: N.D.

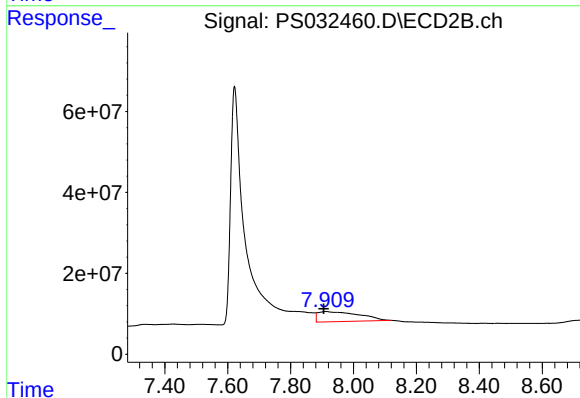


#6 MCP

R.T.: 7.911 min
Delta R.T.: 0.005 min
Response: 226065488
Conc: 17.00 ug/ml

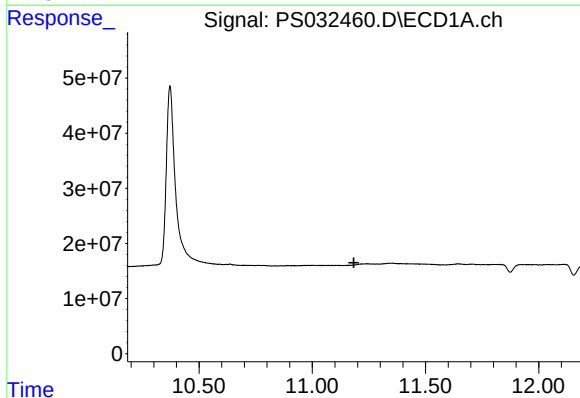

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.184 min
Response: 0
Conc: N.D.

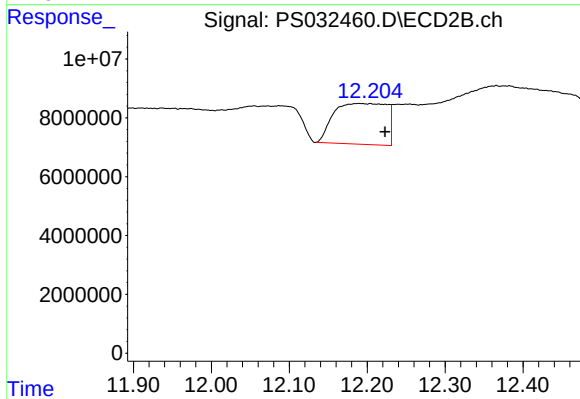

#15 Picloram

R.T.: 12.204 min
Delta R.T.: -0.019 min
Response: 65526539
Conc: 1.76 ng/ml