

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111825\
 Data File : PS032462.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2025 15:39
 Operator : AR\AJ
 Sample : PB170606BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 00:50:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
4) S	2,4-DCAA	7.284	7.616	1818.6E6	1997.1E6	401.335	547.834 #
Target Compounds							
1) T	Dalapon	2.620f	2.564f	669.5E6	2977.1E6	93.263	428.118 #
2) T	3,5-DICHL...	6.444	0.000	8775415	0	1.357	N.D. #
6) T	MCP	7.637	7.952f	2386510	28862919	<MDL	2.170 #
7) T	MCPA	7.775	0.000	81785367	0	6.092	N.D. #
8) T	DICHLORPROP	0.000	8.511	0	1478786	N.D.	<MDL
9) T	2,4-D	8.410	0.000	4977279	0	1.103	N.D. #
10) T	Pentachlo...	8.706	9.359	5910084	18067102	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	9.747	0	114.6E6	N.D.	4.266
12) T	2,4,5-T	9.581	0.000	105.2E6	0	4.415	N.D. #
13) T	2,4-DB	10.155	10.759	386.0E6	64081288	146.487	16.992 #
14) T	DINOSEB	0.000	11.106	0	10408244	N.D.	<MDL
15) T	Picloram	11.172	0.000	9737454	0	<MDL	N.D. #
16) T	DCPA	11.623	12.152	63625920	48677006	1.896	1.528


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111825\
Data File : PS032462.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2025 15:39
Operator : AR\AJ
Sample : PB170606BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 00:50:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

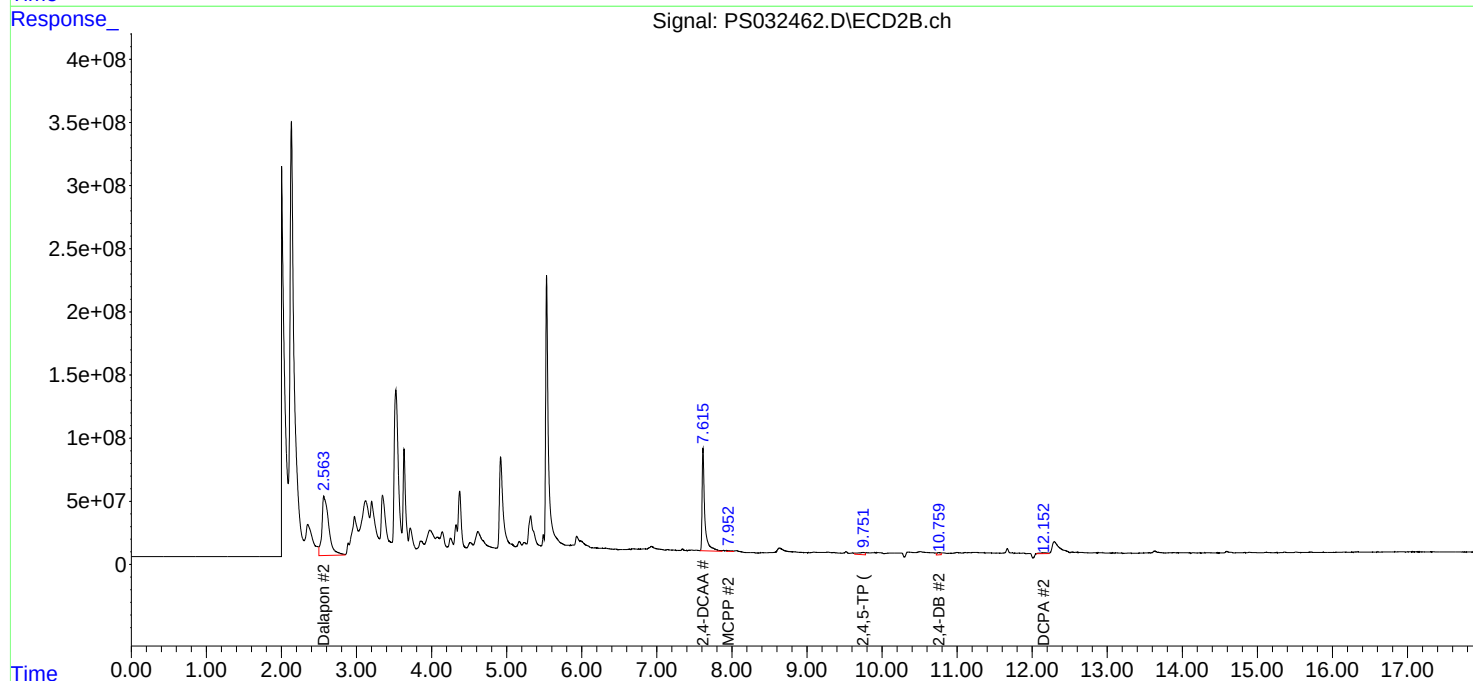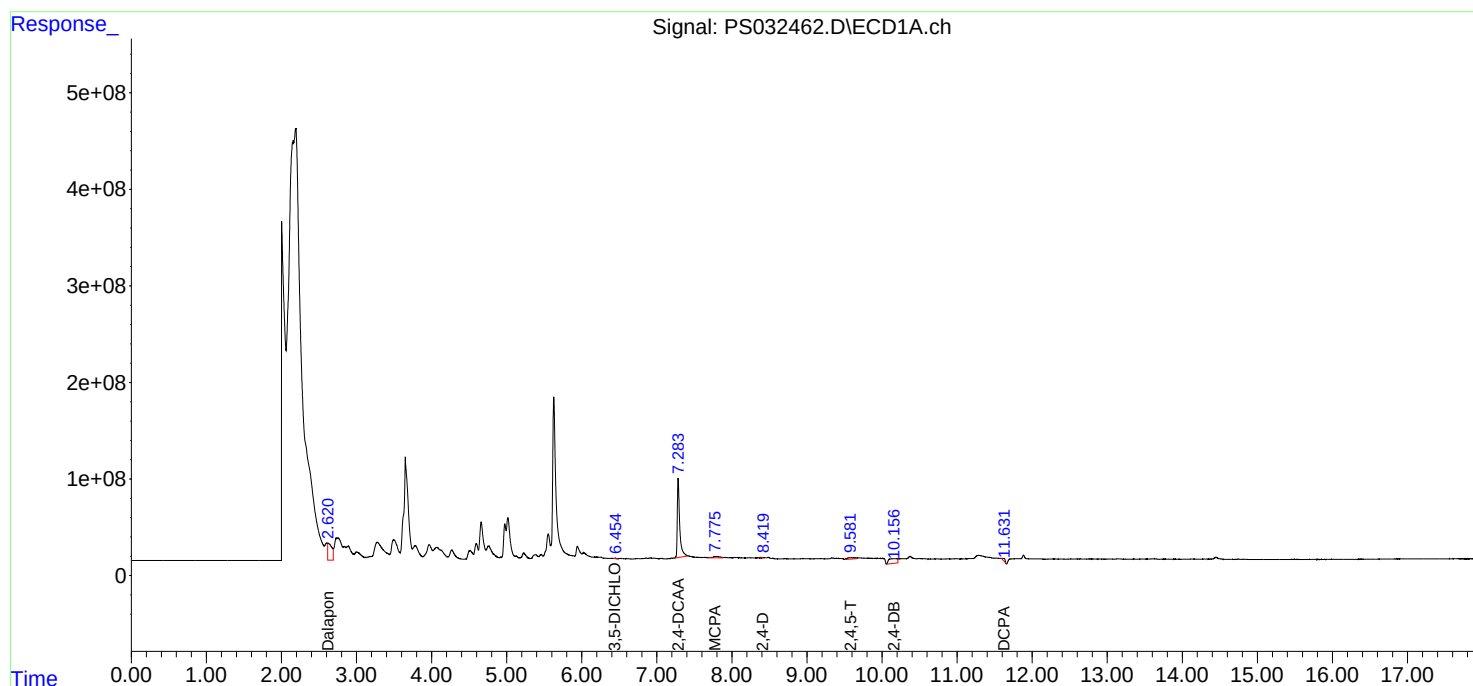

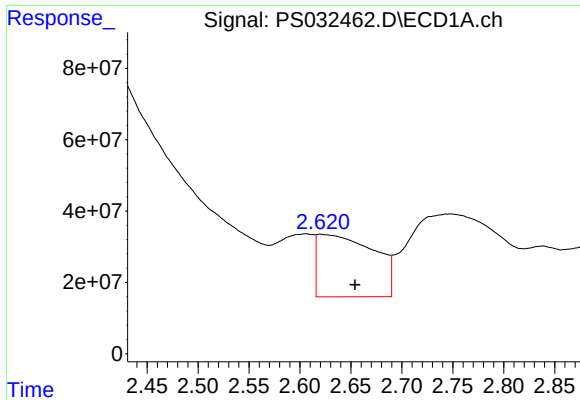


#1 Dalapon

R.T.: 2.620 min
Delta R.T.: -0.034 min
Response: 669516621
Conc: 93.26 ng/ml

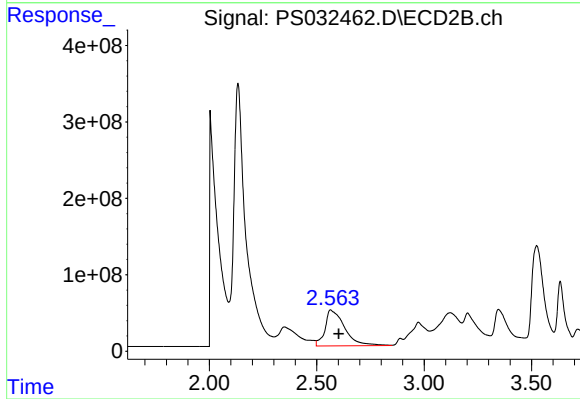


#1 Dalapon

R.T.: 2.564 min
Delta R.T.: -0.039 min
Response: 2977127961
Conc: 428.12 ng/ml

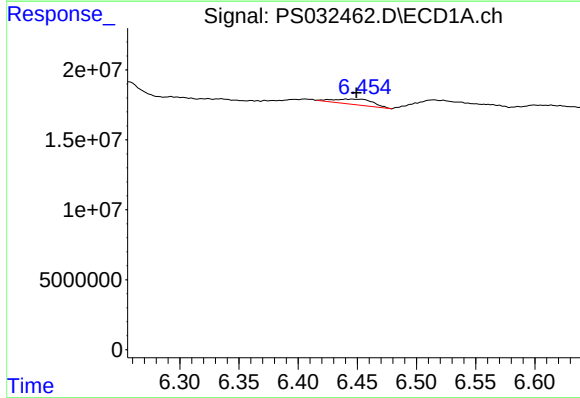


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.444 min
Delta R.T.: -0.005 min
Response: 8775415
Conc: 1.36 ng/ml

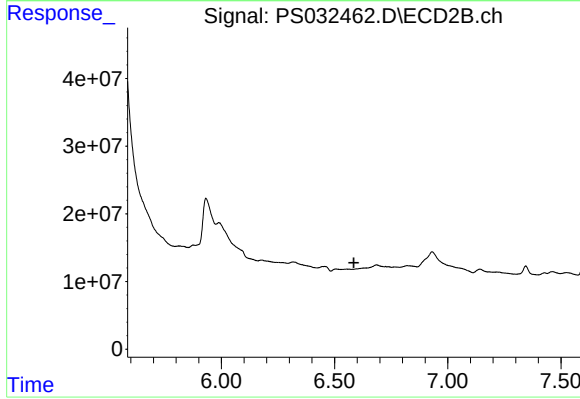


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.585 min
Response: 0
Conc: N.D.

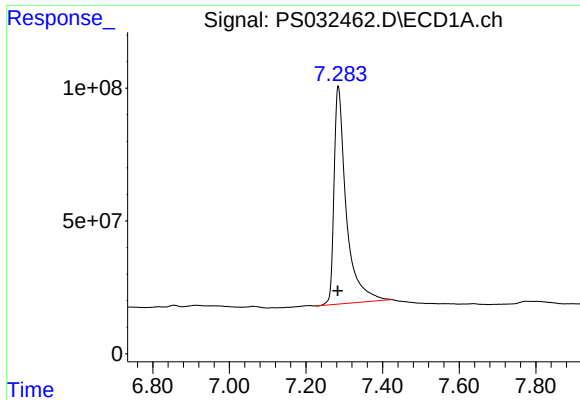


#4 2,4-DCAA

R.T.: 7.284 min
Delta R.T.: 0.000 min
Response: 1818560020
Conc: 401.34 ng/ml

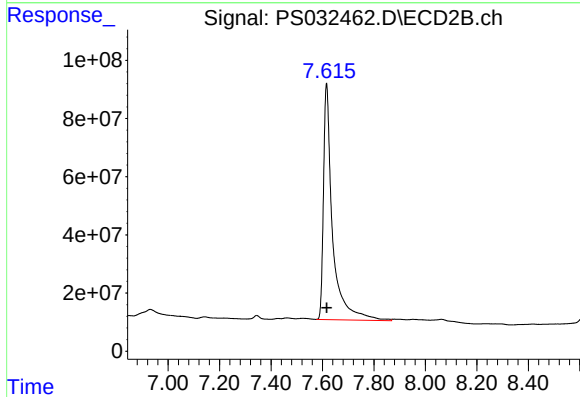


#4 2,4-DCAA

R.T.: 7.616 min
Delta R.T.: -0.001 min
Response: 1997127874
Conc: 547.83 ng/ml

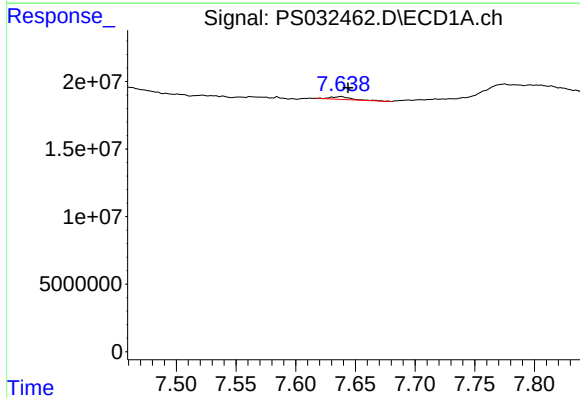


#6 MCPP

R.T.: 7.637 min
Delta R.T.: -0.007 min
Response: 2386510
Conc: N.D.

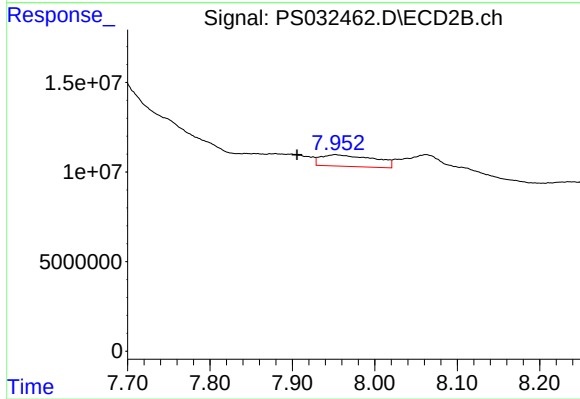


#6 MCPP

R.T.: 7.952 min
Delta R.T.: 0.047 min
Response: 28862919
Conc: 2.17 ug/ml

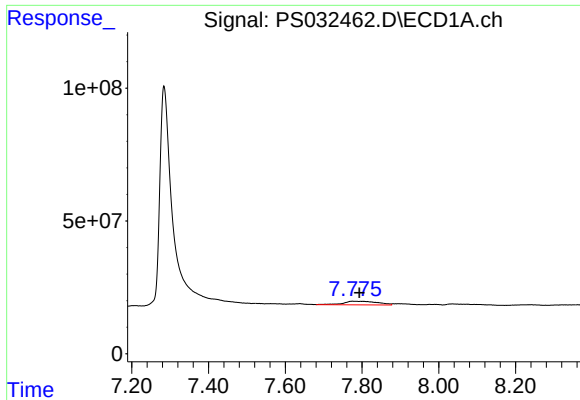


#7 MCPA

R.T.: 7.775 min
Delta R.T.: -0.018 min
Response: 81785367
Conc: 6.09 ug/ml

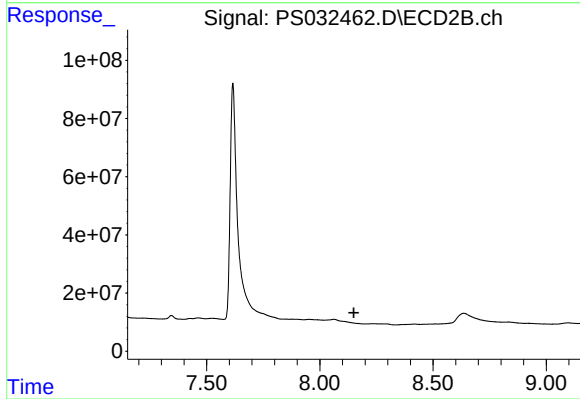


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 8.151 min
Response: 0
Conc: N.D.

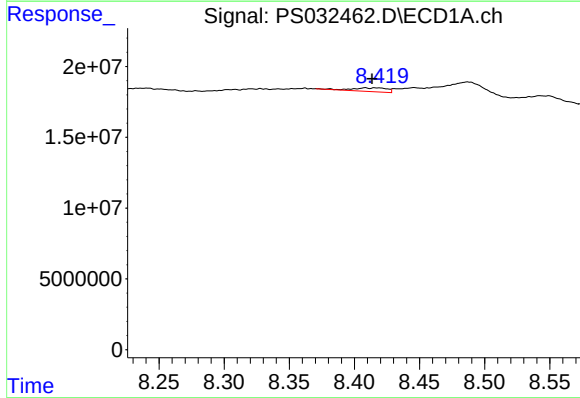


#9 2,4-D

R.T.: 8.410 min
Delta R.T.: -0.004 min
Response: 4977279
Conc: 1.10 ng/ml

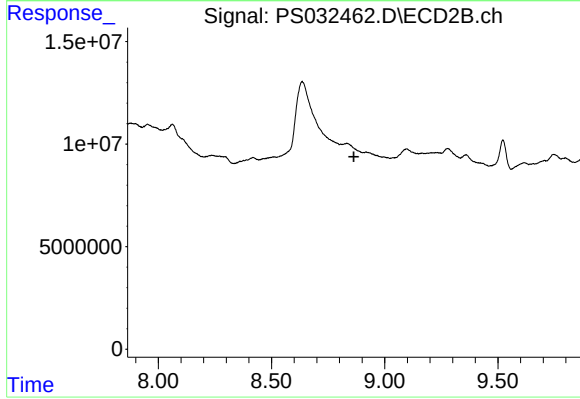


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.864 min
Response: 0
Conc: N.D.

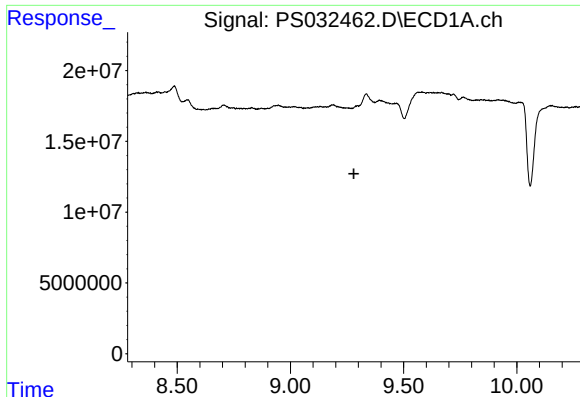


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.280 min
Response: 0
Conc: N.D.

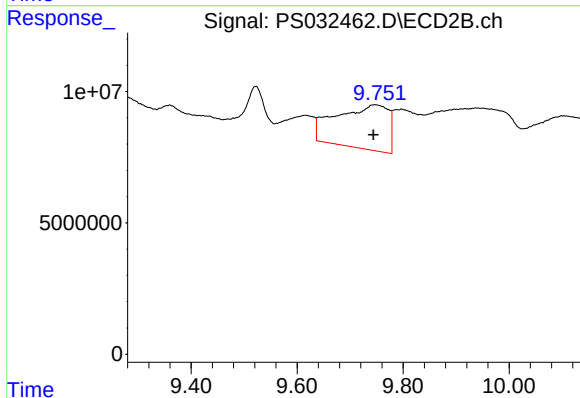


#11 2,4,5-TP (SILVEX)

R.T.: 9.747 min
Delta R.T.: 0.003 min
Response: 114565744
Conc: 4.27 ng/ml

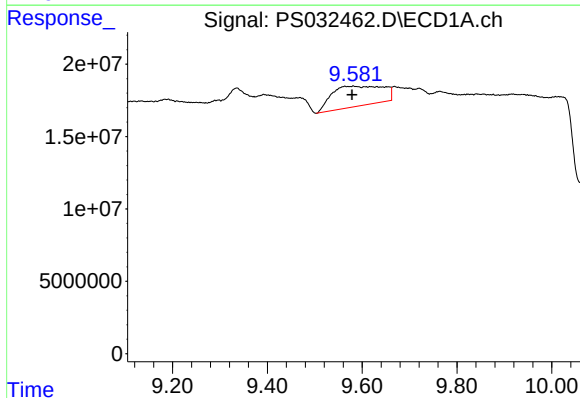


#12 2,4,5-T

R.T.: 9.581 min
Delta R.T.: 0.003 min
Response: 105234525
Conc: 4.41 ng/ml

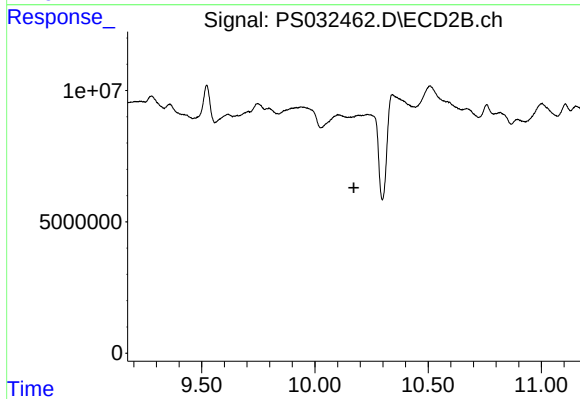


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 10.172 min
Response: 0
Conc: N.D.

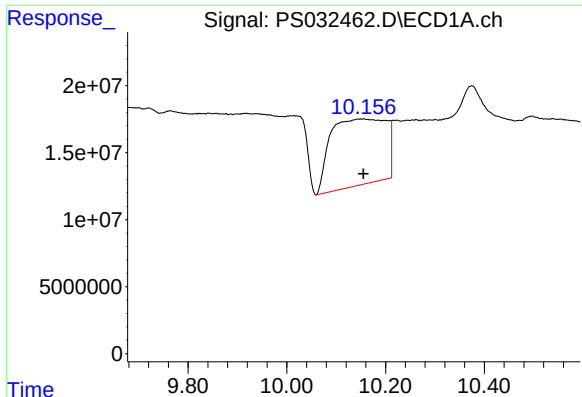


#13 2,4-DB

R.T.: 10.155 min
Delta R.T.: 0.000 min
Response: 386009085
Conc: 146.49 ng/ml

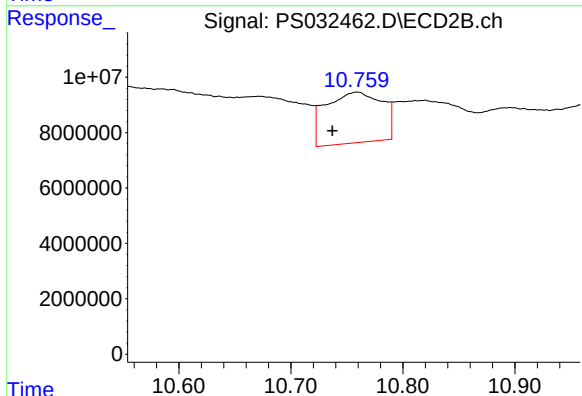


#13 2,4-DB

R.T.: 10.759 min
Delta R.T.: 0.022 min
Response: 64081288
Conc: 16.99 ng/ml

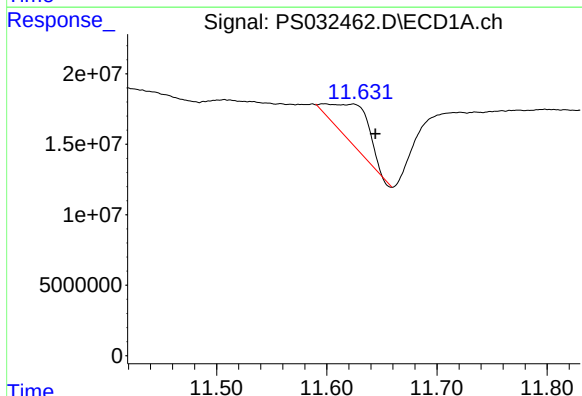

#16 DCPA

R.T.: 11.623 min
Delta R.T.: -0.021 min
Response: 63625920
Conc: 1.90 ng/ml

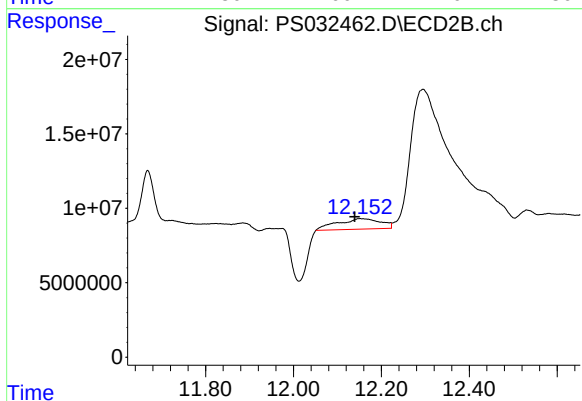

#16 DCPA

R.T.: 12.152 min
Delta R.T.: 0.012 min
Response: 48677006
Conc: 1.53 ng/ml