

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111825\
 Data File : PS032466.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2025 17:15
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 01:57:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
4) S	2,4-DCAA	7.286	7.628	1654.6E6	1942.0E6	365.146	532.724 #
Target Compounds							
2) T	3,5-DICHL...	6.445	0.000	35013519	0	5.415	N.D. #
6) T	MCP	0.000	7.914	0	58550617	N.D.	4.402
8) T	DICHLORPROP	8.165	0.000	944622	0	<MDL	N.D. #
9) T	2,4-D	8.457f	0.000	120.0E6	0	26.600	N.D. #
10) T	Pentachlo...	8.711	9.374	5072530	2760858	<MDL	<MDL #
11) T	2,4,5-TP ...	9.280	0.000	5028524	0	<MDL	N.D. #
12) T	2,4,5-T	0.000	10.149	0	5094307	N.D.	<MDL
13) T	2,4-DB	10.187f	0.000	205380	0	<MDL	N.D. #
14) T	DINOSEB	11.352	11.118	11072483	6679985	<MDL	<MDL #
15) T	Picloram	11.233f	12.197f	20542011	153.2E6	<MDL	4.121 #
16) T	DCPA	11.643	0.000	7478714	0	<MDL	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111825\
Data File : PS032466.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2025 17:15
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:57:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

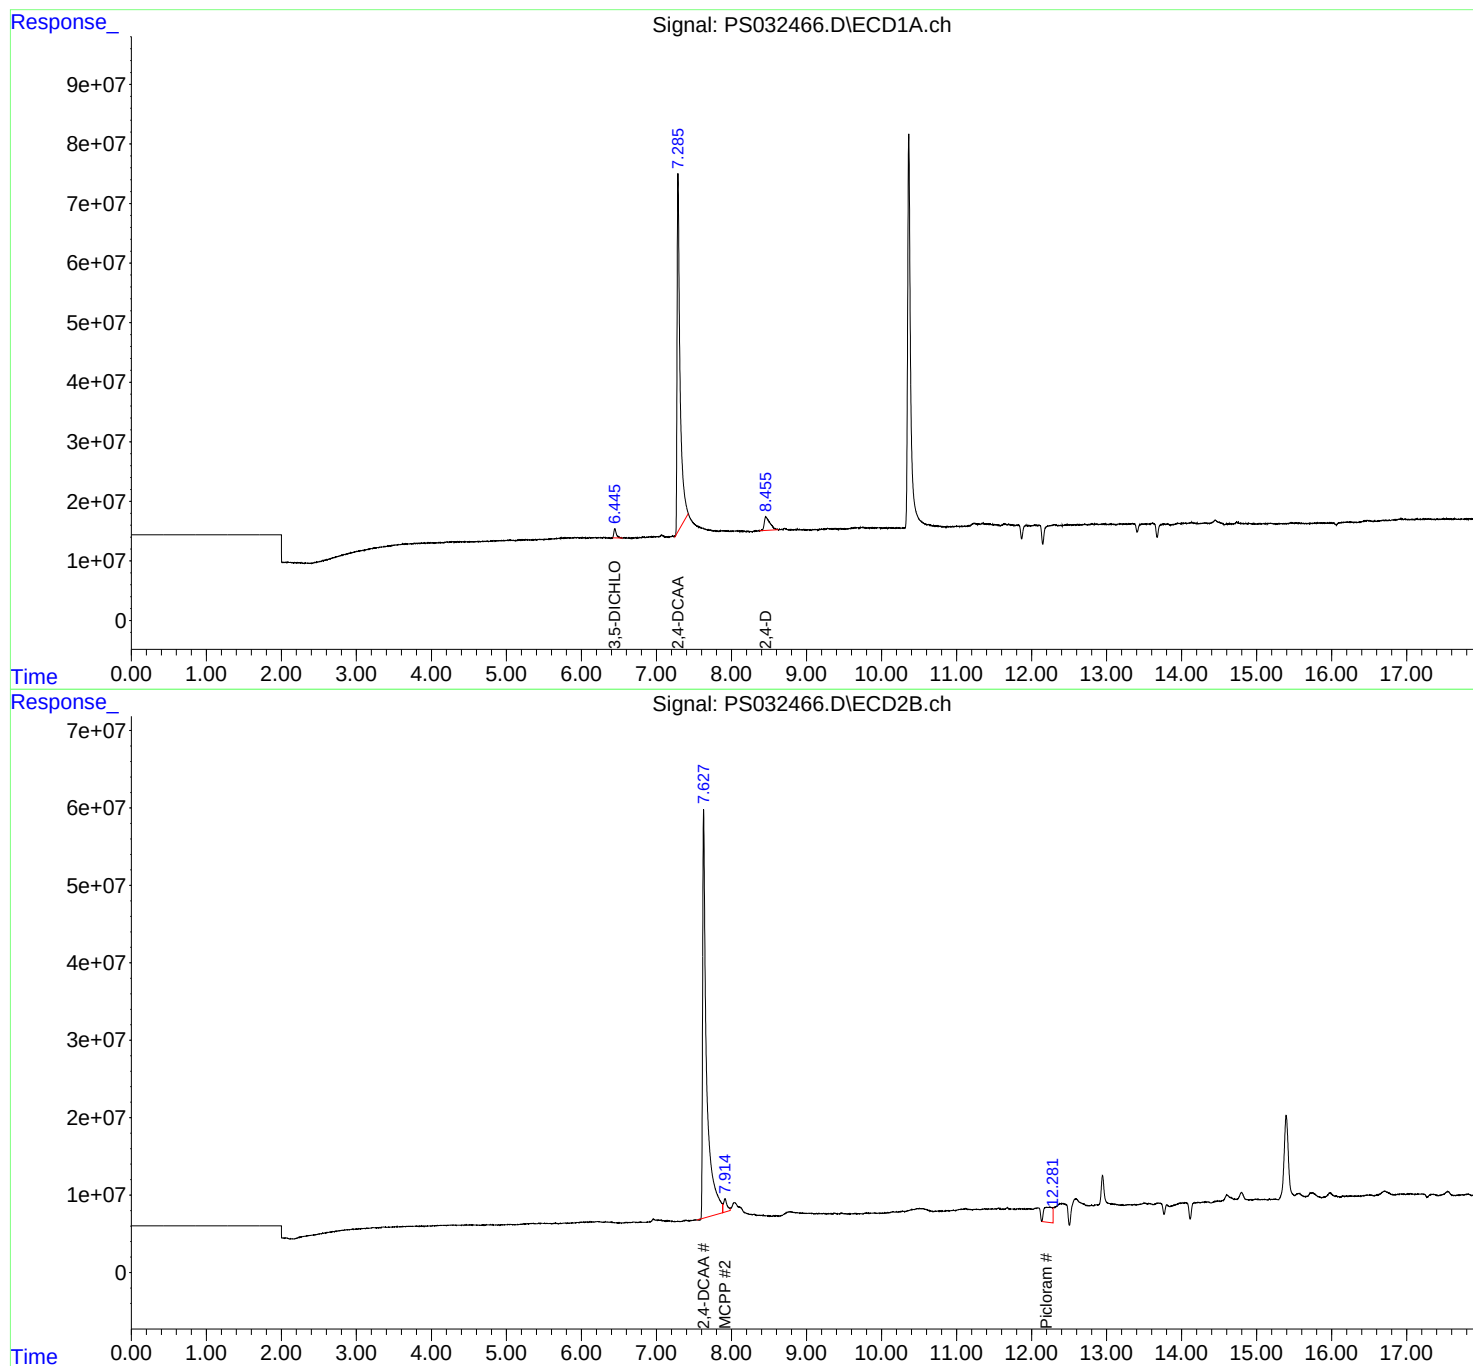

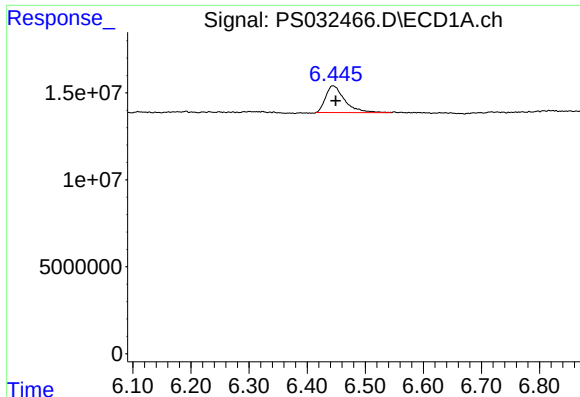


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.445 min
Delta R.T.: -0.005 min
Response: 35013519
Conc: 5.41 ng/ml

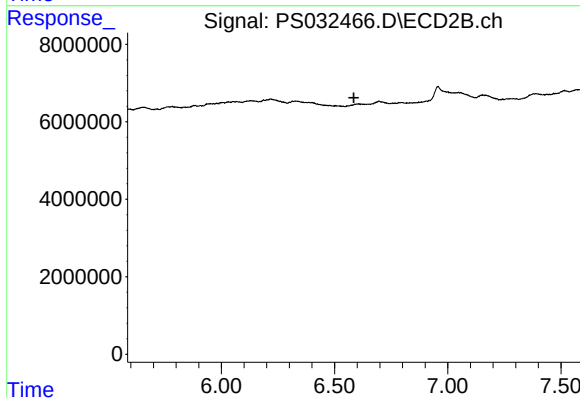


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 6.585 min
Response: 0
Conc: N.D.

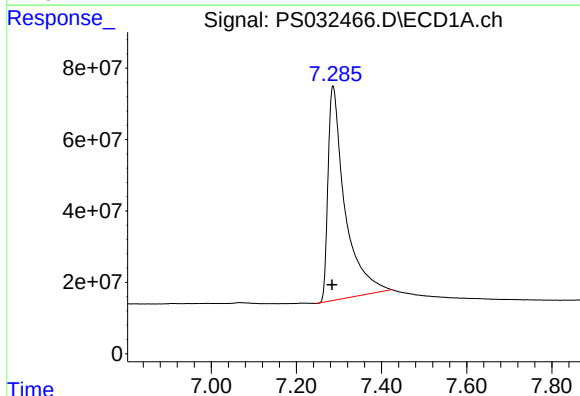


#4 2,4-DCAA

R.T.: 7.286 min
Delta R.T.: 0.003 min
Response: 1654574474
Conc: 365.15 ng/ml

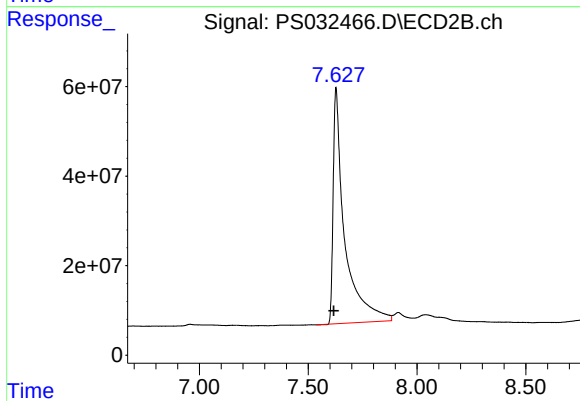


#4 2,4-DCAA

R.T.: 7.628 min
Delta R.T.: 0.011 min
Response: 1942044926
Conc: 532.72 ng/ml

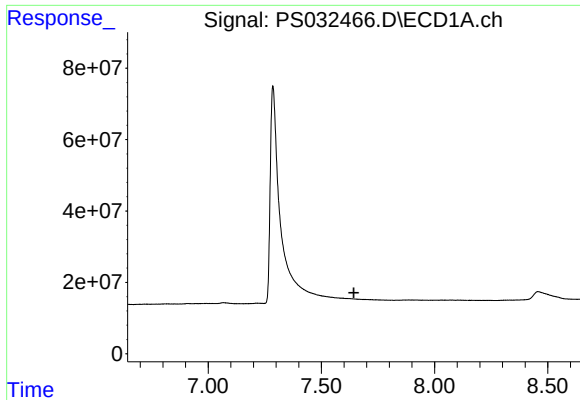


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.644 min
Response: 0
Conc: N.D.

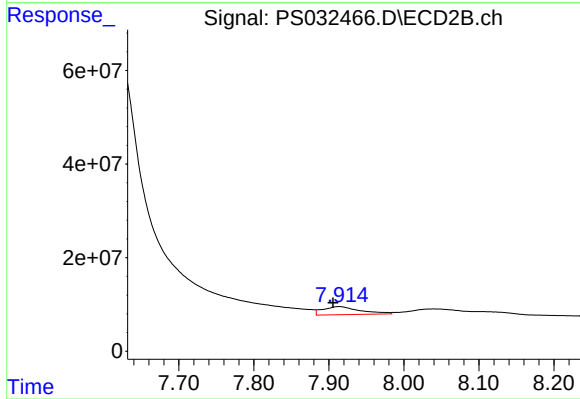


#6 MCP

R.T.: 7.914 min
Delta R.T.: 0.008 min
Response: 58550617
Conc: 4.40 ug/ml

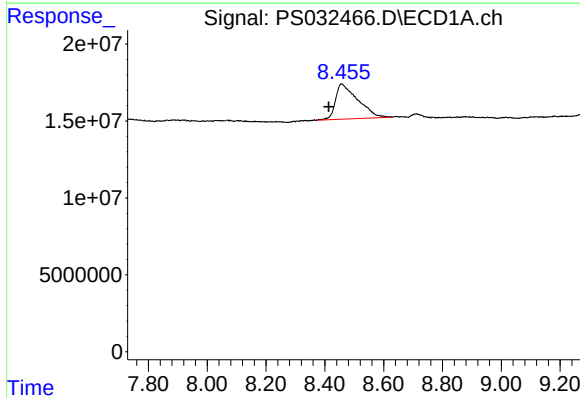


#9 2,4-D

R.T.: 8.457 min
Delta R.T.: 0.043 min
Response: 120013412
Conc: 26.60 ng/ml

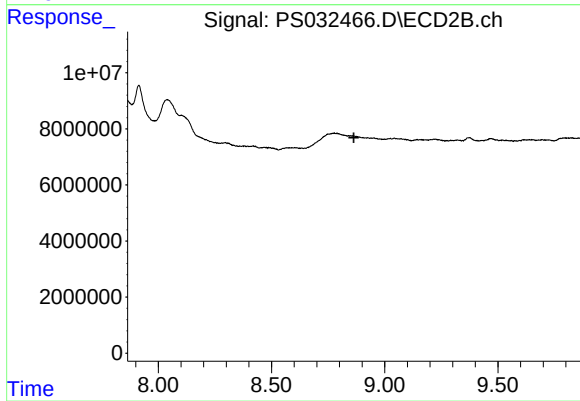


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.864 min
Response: 0
Conc: N.D.

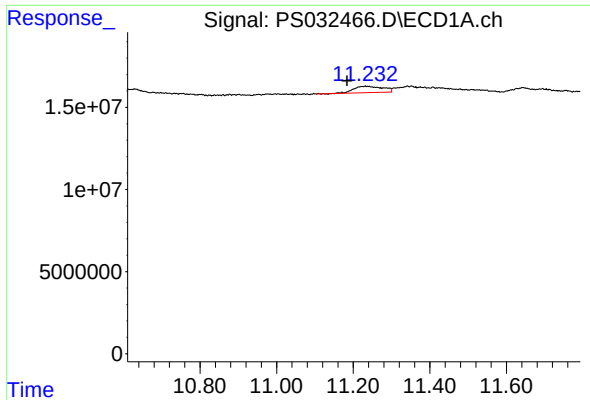

#15 Picloram

R.T.: 11.233 min
Delta R.T.: 0.049 min
Response: 20542011
Conc: N.D.

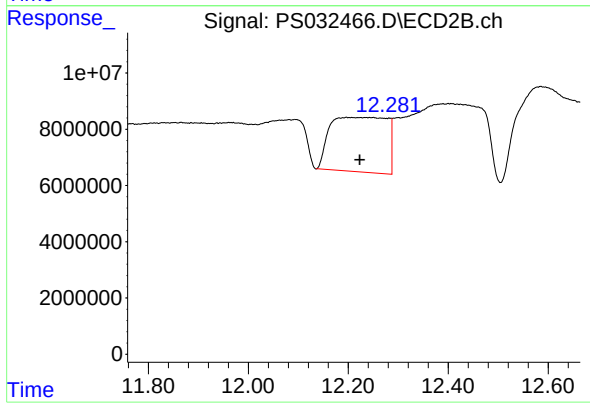

#15 Picloram

R.T.: 12.197 min
Delta R.T.: -0.026 min
Response: 153229326
Conc: 4.12 ng/ml