

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111918\
 Data File : PS002439.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2018 09:45
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 02:31:26 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.933	0	177212	N.D.	0.484 #
Target Compounds							
2) T	3,5-DICHL...	0.000	9.092	0	60005	N.D.	0.132 #
3) T	4-Nitroph...	0.000	10.093	0	46027	N.D.	0.263 #
5) T	DICAMBA	0.000	11.220	0	184399	N.D.	0.136 #
6) T	MCP	0.000	11.440	0	603370	N.D.	0.665 #
7) T	MCPA	0.000	11.793	0	110711	N.D.	0.079 #
8) T	DICHLORPROP	0.000	12.339	0	78244	N.D.	0.236 #
9) T	2,4-D	0.000	12.849	0	181708	N.D.	0.455 #
10) T	Pentachlo...	0.000	13.374	0	69377	N.D.	0.014 #
11) T	2,4,5-TP ...	0.000	13.996	0	100555	N.D.	0.050 #
12) T	2,4,5-T	0.000	14.562	0	244106	N.D.	0.156 #
13) T	2,4-DB	0.000	15.209	0	81227	N.D.	0.358 #
15) T	Picloram	0.000	16.802	0	604429	N.D.	0.227 #
16) T	DCPA	0.000	16.814	0	647082	N.D.	0.270 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
Data File : PS002439.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2018 09:45
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 02:31:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

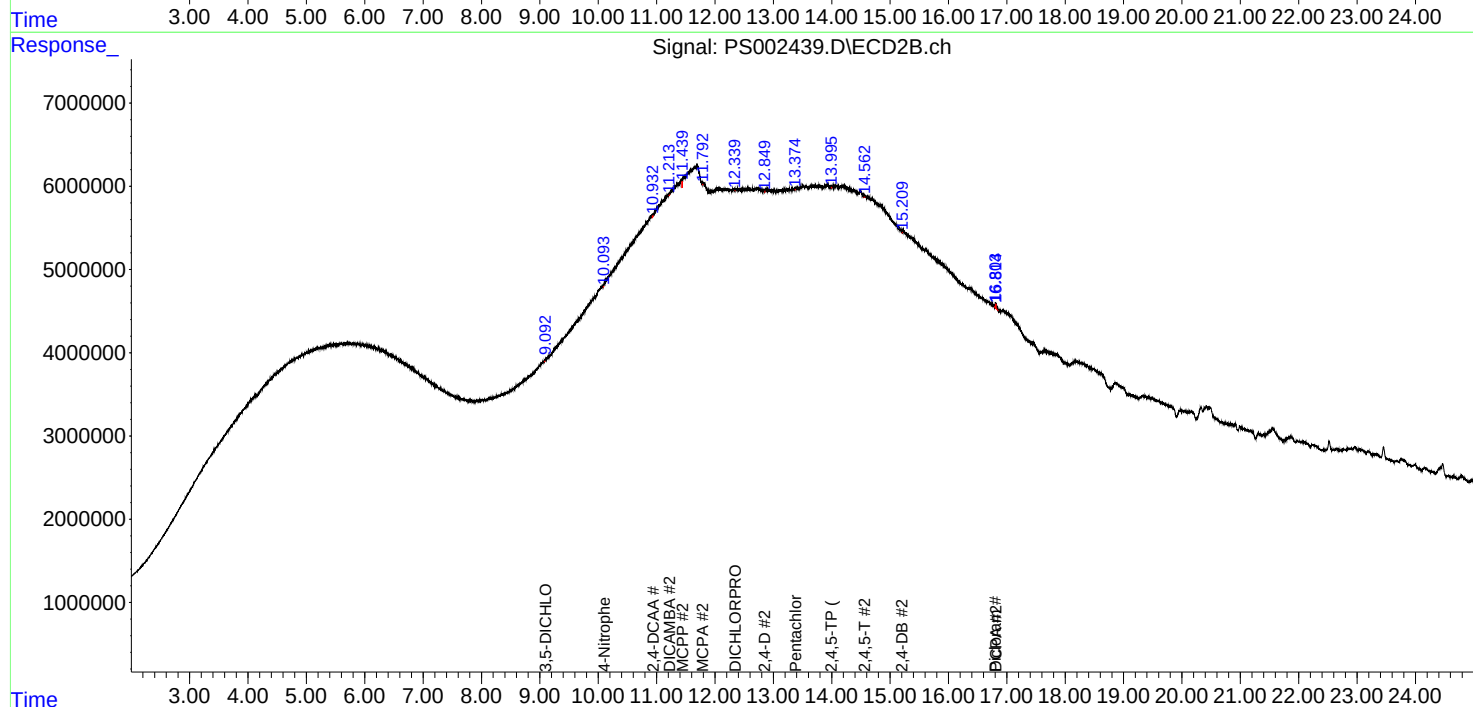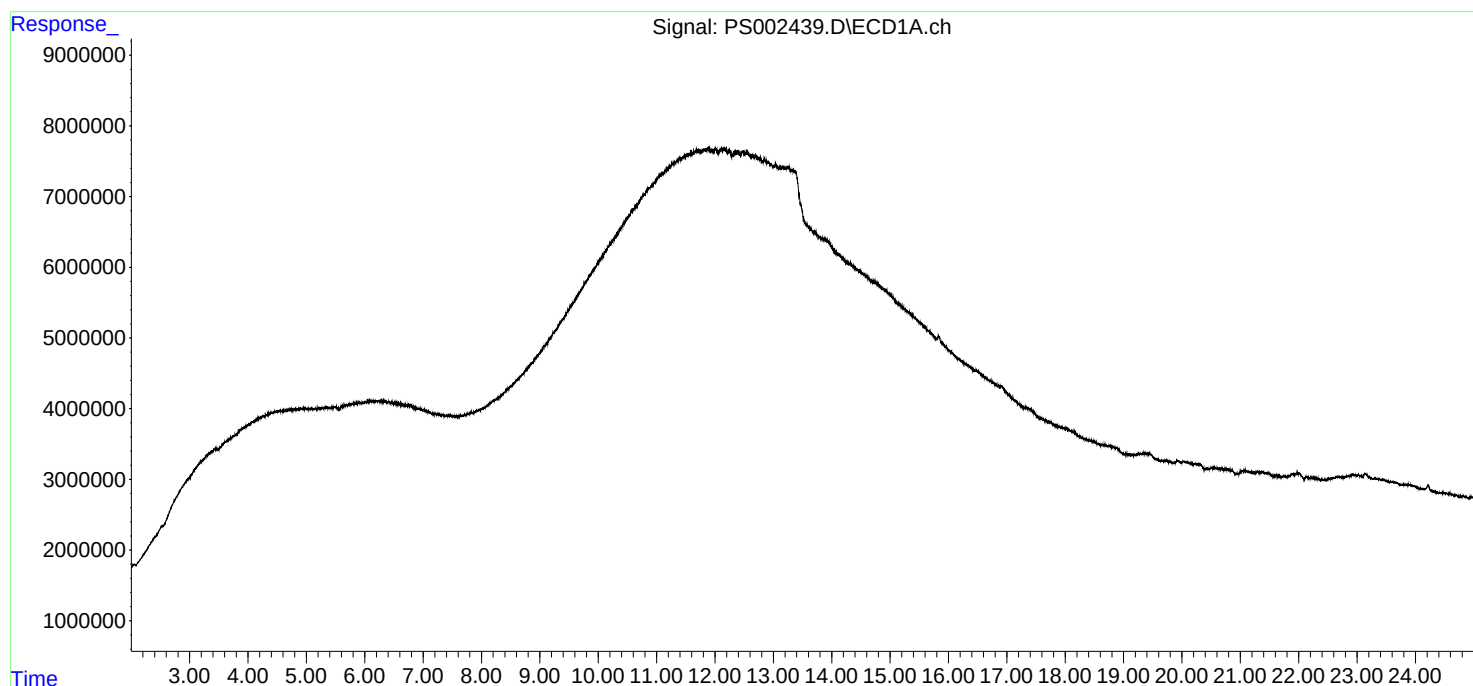


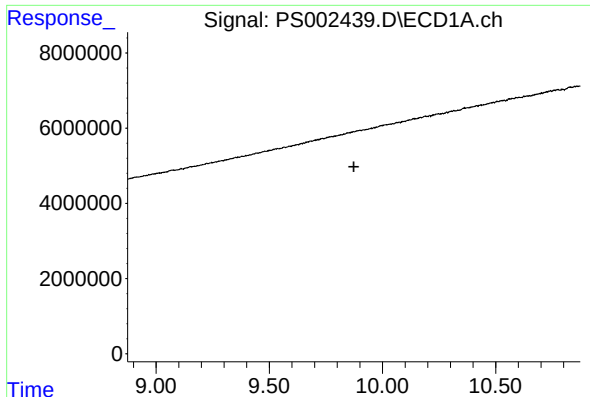

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.874 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

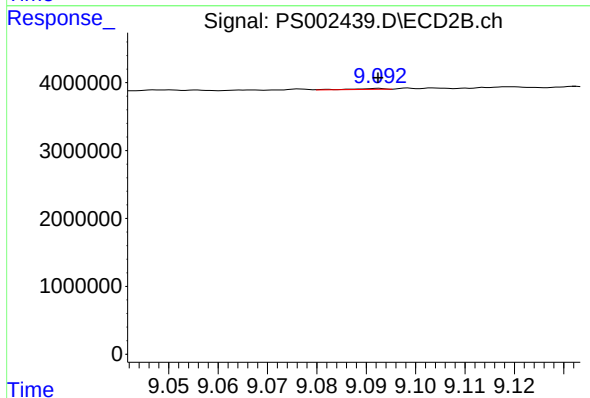


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.092 min
Delta R.T.: 0.000 min
Response: 60005
Conc: 0.13 ng/ml

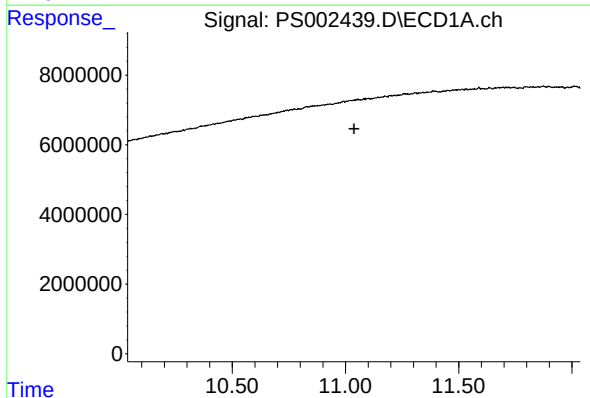


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 11.037 min
Response: 0
Conc: N.D.

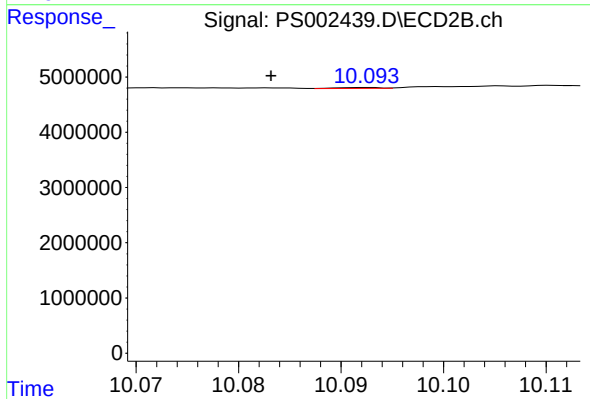

#3 4-Nitrophenol


R.T.: 10.093 min
Delta R.T.: 0.009 min
Response: 46027
Conc: 0.26 ng/ml

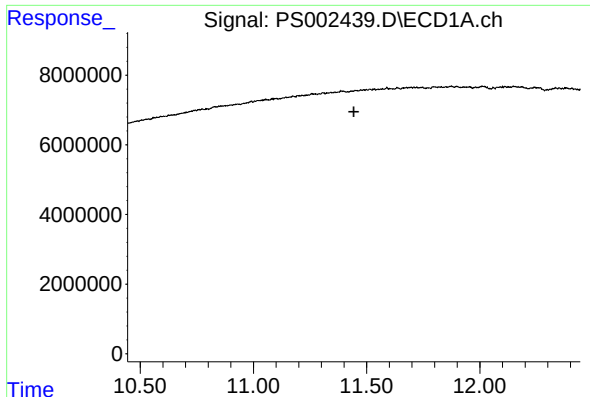

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 11.444 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

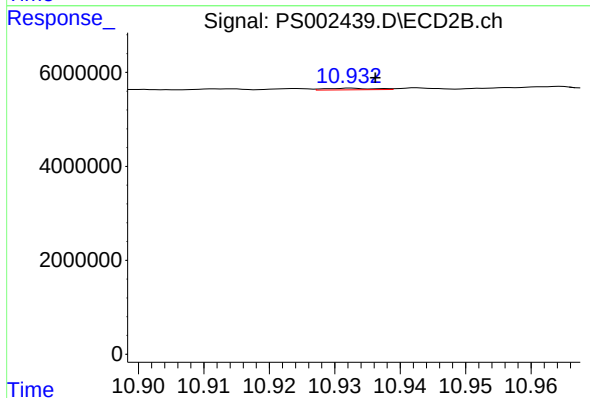


#4 2,4-DCAA

R.T.: 10.933 min
Delta R.T.: -0.004 min
Response: 177212
Conc: 0.48 ng/ml

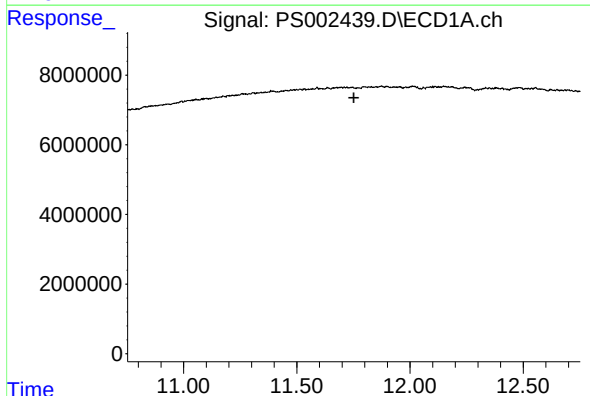


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.752 min
Response: 0
Conc: N.D.

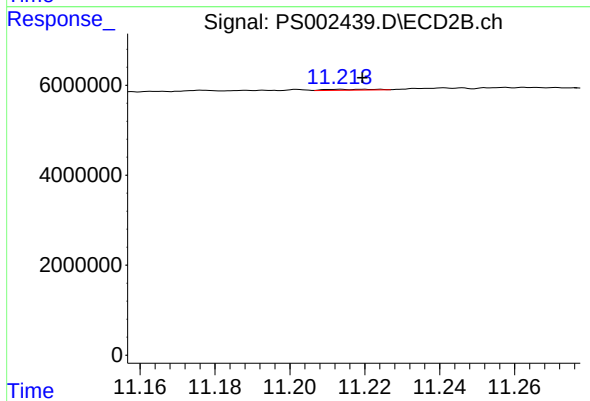

#5 DICAMBA


R.T.: 11.220 min
Delta R.T.: 0.000 min
Response: 184399
Conc: 0.14 ng/ml

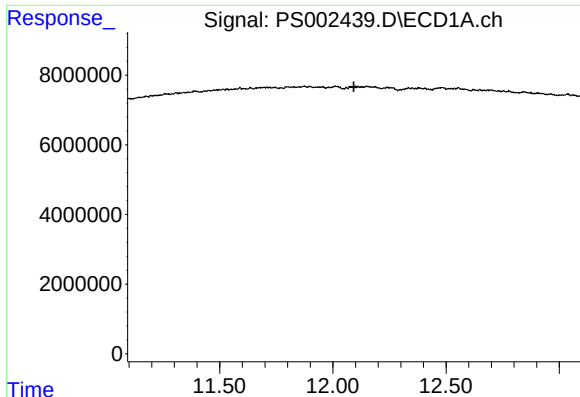

#6 MCPP


R.T.: 0.000 min
Exp R.T. : 12.093 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

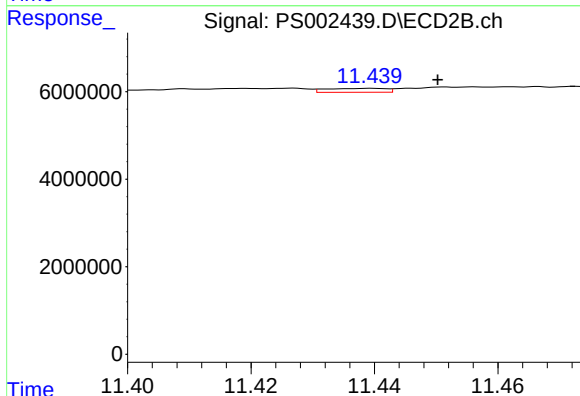


#6 MCPP

R.T.: 11.440 min
Delta R.T.: -0.011 min
Response: 603370
Conc: 0.67 ug/ml

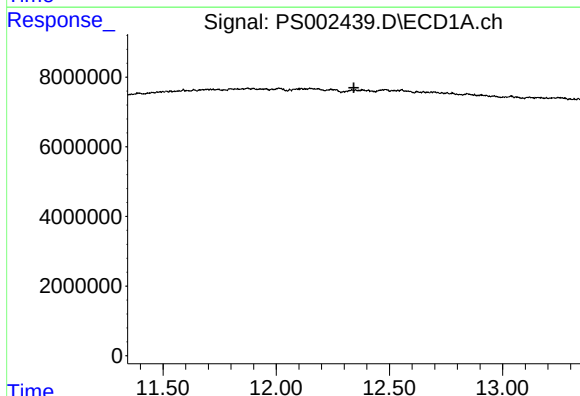


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.343 min
Response: 0
Conc: N.D.

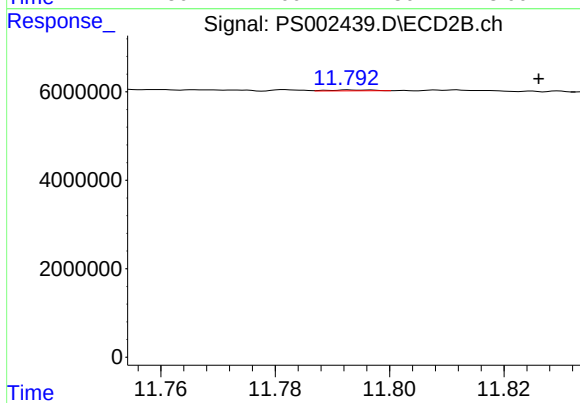

#7 MCPA


R.T.: 11.793 min
Delta R.T.: -0.033 min
Response: 110711
Conc: 0.08 ug/ml

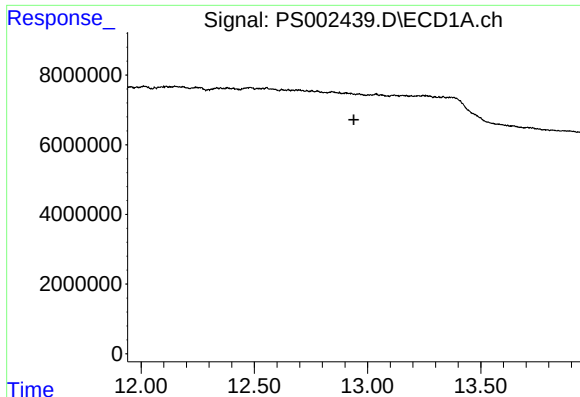

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.939 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

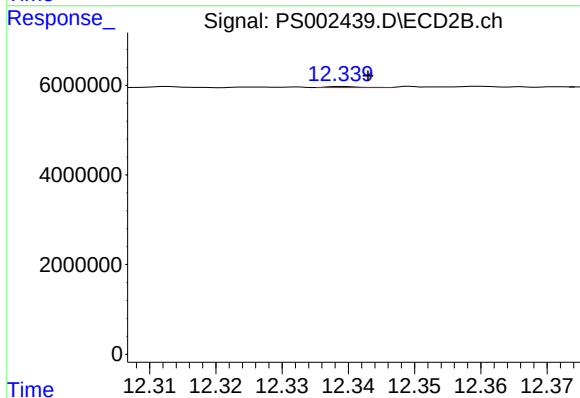


#8 DICHLORPROP

R.T.: 12.339 min
Delta R.T.: -0.004 min
Response: 78244
Conc: 0.24 ng/ml

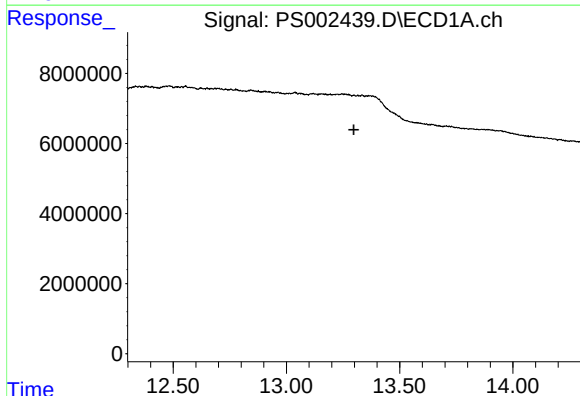


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.298 min
Response: 0
Conc: N.D.

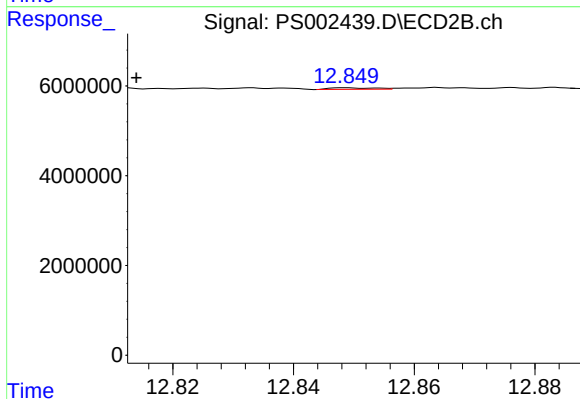

#9 2,4-D


R.T.: 12.849 min
Delta R.T.: 0.035 min
Response: 181708
Conc: 0.45 ng/ml

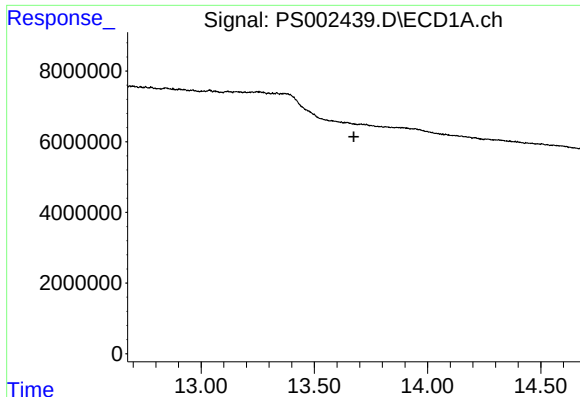

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.675 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

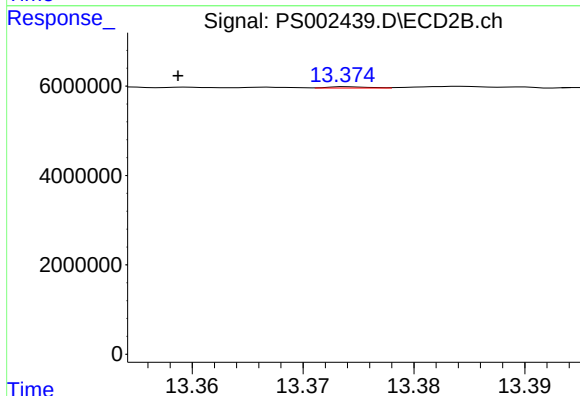


#10 Pentachlorophenol

R.T.: 13.374 min
Delta R.T.: 0.015 min
Response: 69377
Conc: 0.01 ng/ml

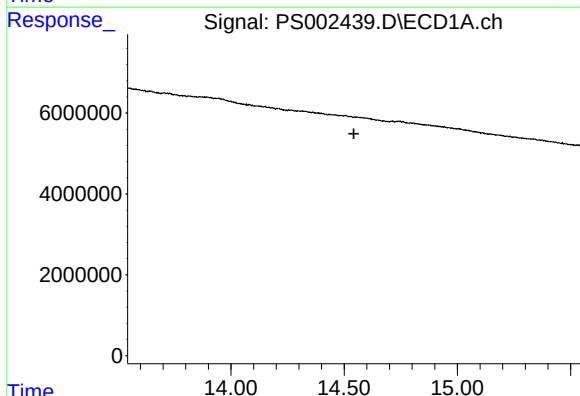


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.543 min
Response: 0
Conc: N.D.

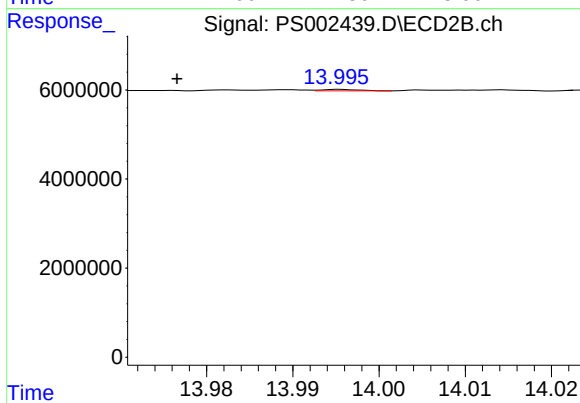

#11 2,4,5-TP (SILVEX)


R.T.: 13.996 min
Delta R.T.: 0.019 min
Response: 100555
Conc: 0.05 ng/ml

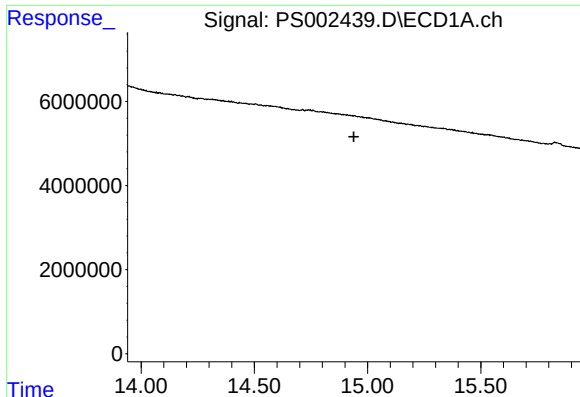

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.940 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

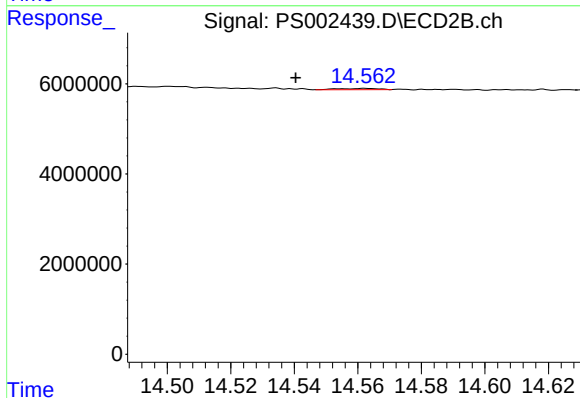


#12 2,4,5-T

R.T.: 14.562 min
Delta R.T.: 0.022 min
Response: 244106
Conc: 0.16 ng/ml

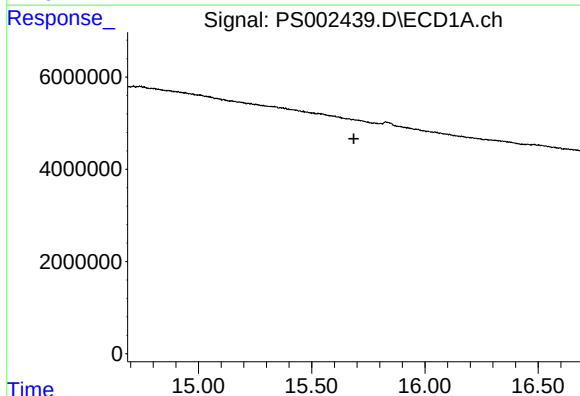


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.686 min
Response: 0
Conc: N.D.

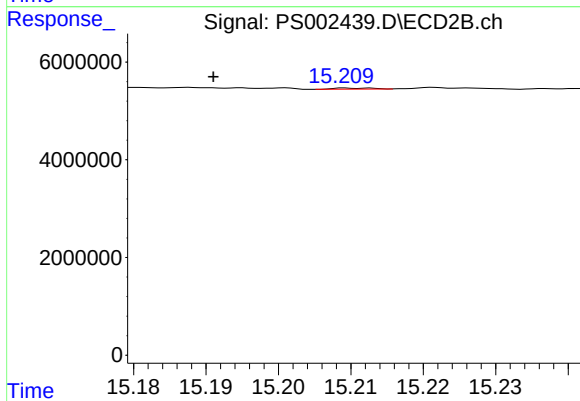

#13 2,4-DB


R.T.: 15.209 min
Delta R.T.: 0.018 min
Response: 81227
Conc: 0.36 ng/ml

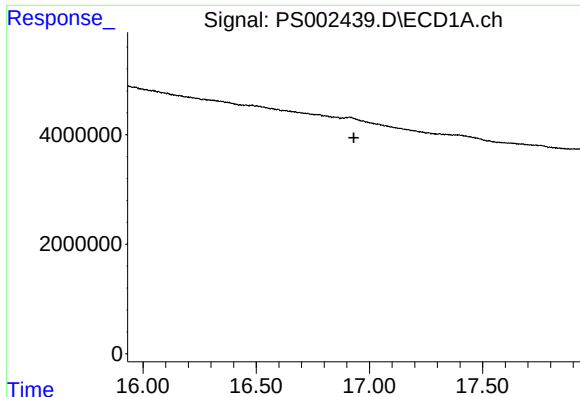

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 16.931 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

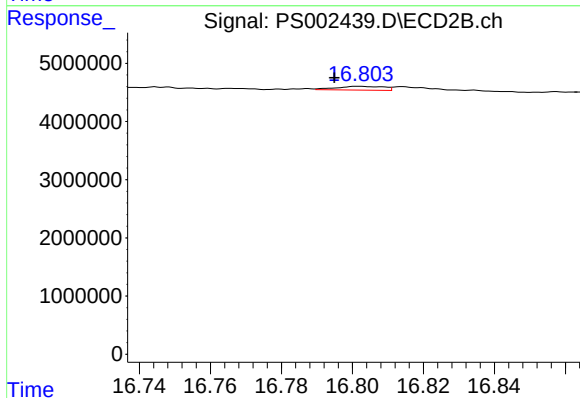


#15 Picloram

R.T.: 16.802 min
Delta R.T.: 0.007 min
Response: 604429
Conc: 0.23 ng/ml

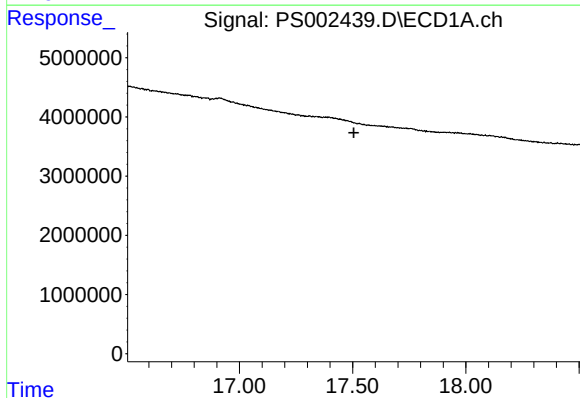

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.506 min
Response: 0
Conc: N.D.

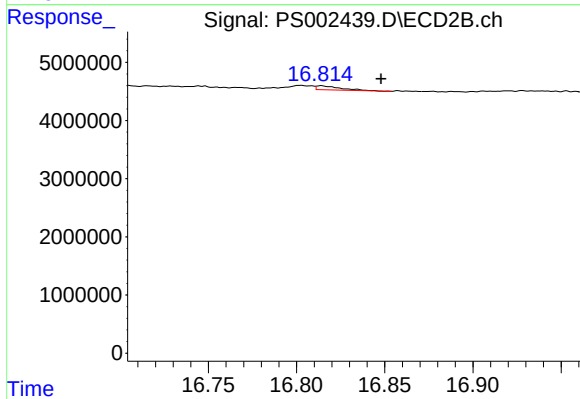

#16 DCPA

R.T.: 16.814 min
Delta R.T.: -0.034 min
Response: 647082
Conc: 0.27 ng/ml