

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111918\
 Data File : PS002449.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2018 20:32
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 02:35:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.422	10.917	156.4E6	153.7E6	513.328	420.072
Target Compounds							
7) T	MCPA	0.000	11.816	0	4017778	N.D.	2.855 #
10) T	Pentachlo...	0.000	13.340	0	593246	N.D.	0.117 #
15) T	Picloram	0.000	16.773	0	365428	N.D.	0.137 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
Data File : PS002449.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2018 20:32
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 02:35:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

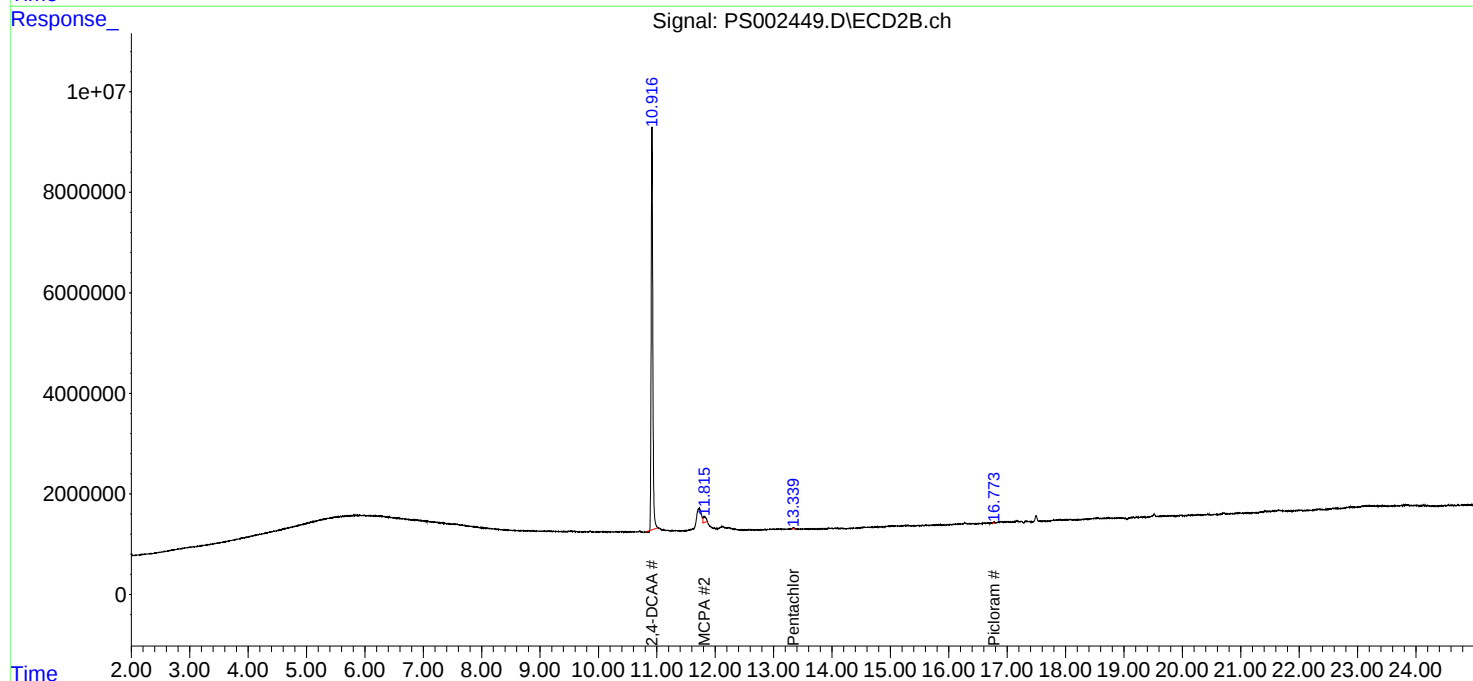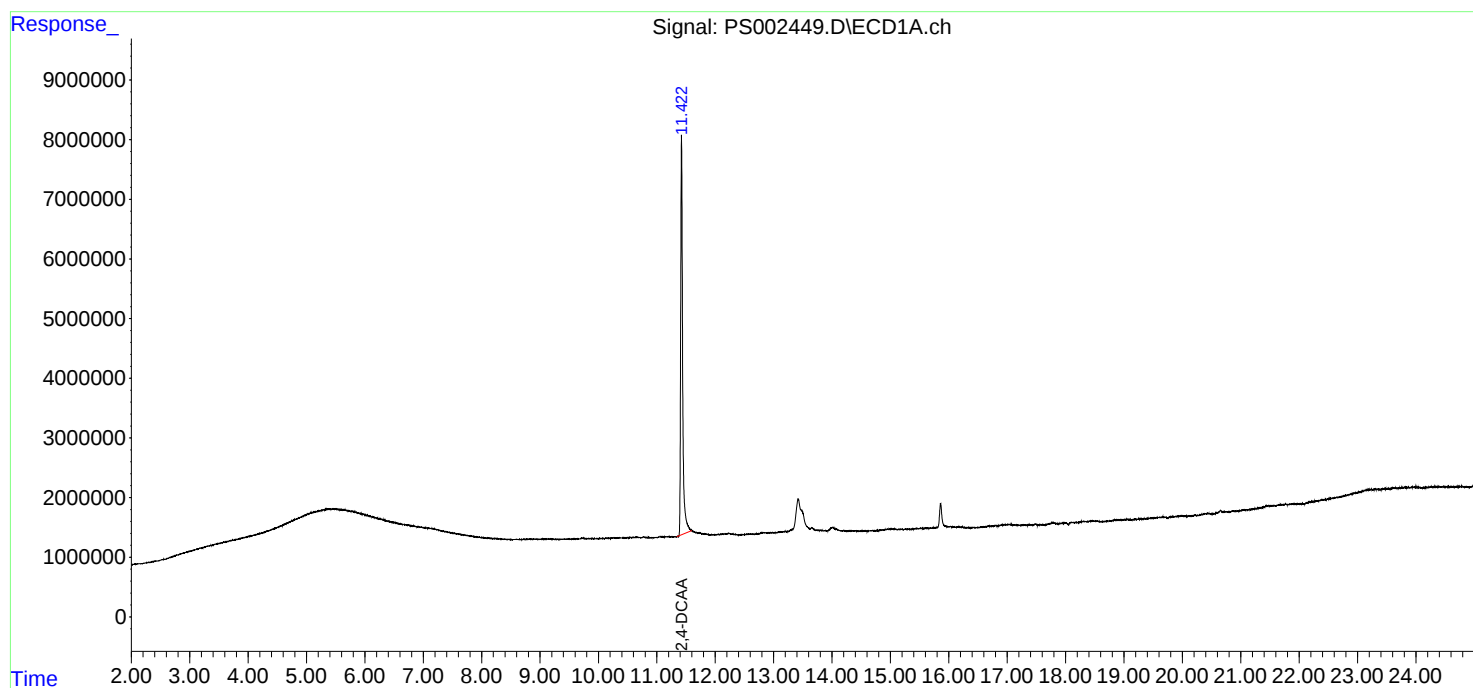


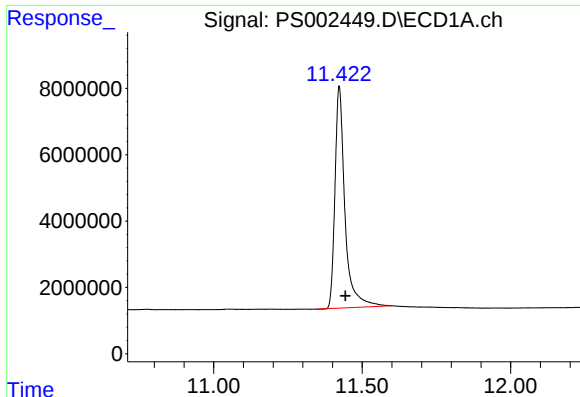

#4 2,4-DCAA


R.T.: 11.422 min
Delta R.T.: -0.021 min
Response: 156359573
Conc: 513.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

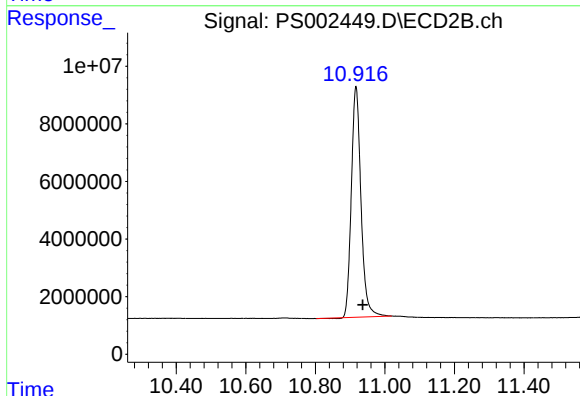


#4 2,4-DCAA

R.T.: 10.917 min
Delta R.T.: -0.019 min
Response: 153709444
Conc: 420.07 ng/ml

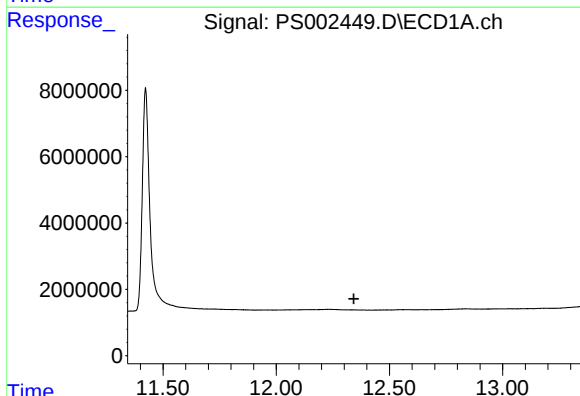


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.343 min
Response: 0
Conc: N.D.

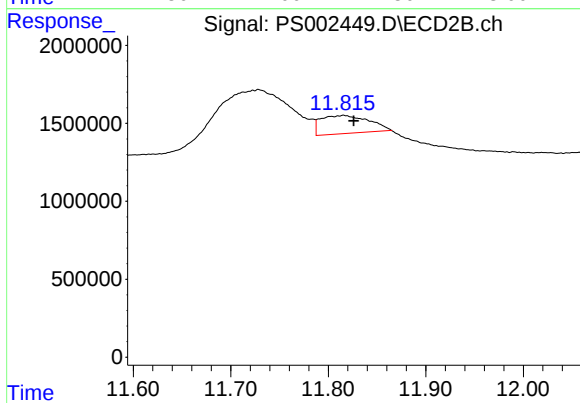

#7 MCPA


R.T.: 11.816 min
Delta R.T.: -0.010 min
Response: 4017778
Conc: 2.86 ug/ml

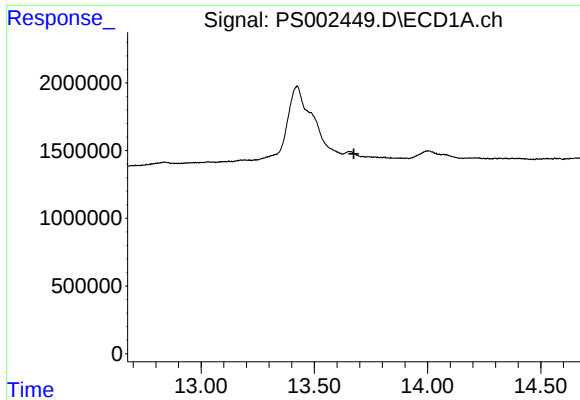

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.675 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

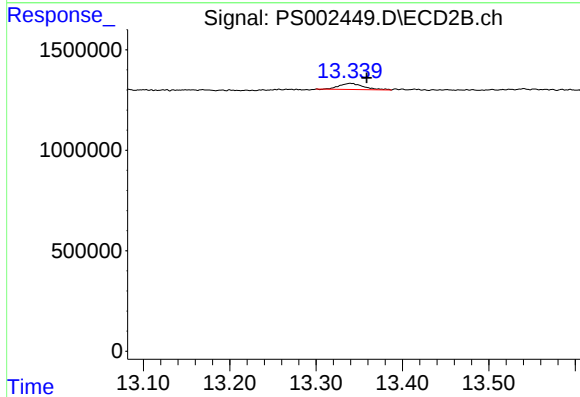


#10 Pentachlorophenol

R.T.: 13.340 min
Delta R.T.: -0.019 min
Response: 593246
Conc: 0.12 ng/ml

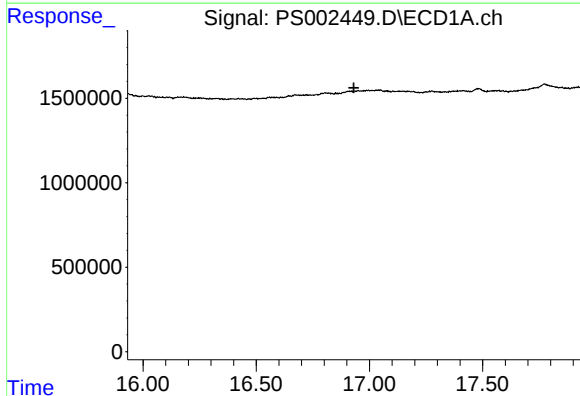

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.931 min
Response: 0
Conc: N.D.

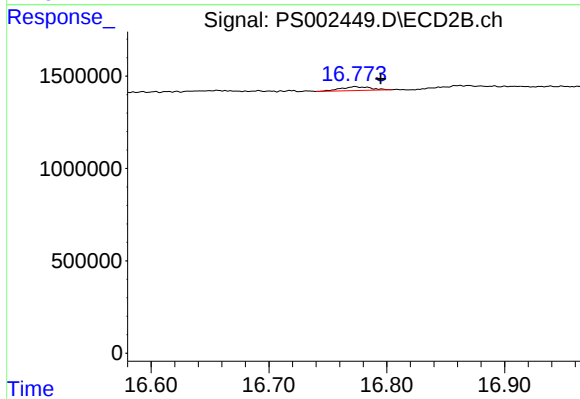

#15 Picloram

R.T.: 16.773 min
Delta R.T.: -0.022 min
Response: 365428
Conc: 0.14 ng/ml