

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111918\
 Data File : PS002455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2018 23:39
 Operator : EI\SJ
 Sample : J5774-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 02:38:01 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.401	10.896	141.2E6	145.0E6	463.674	396.392
Target Compounds							
2) T	3,5-DICHL...	0.000	9.057	0	2516655	N.D.	5.551 #
3) T	4-Nitroph...	11.049	10.113	2683261	4287274	16.537	24.469 #
6) T	MCP	12.082	11.394	12219430	615964	13.020	0.679 #
7) T	MCPA	0.000	11.800	0	5602573	N.D.	3.981 #
9) T	2,4-D	0.000	12.878	0	272535	N.D.	0.682 #
10) T	Pentachlo...	13.635	13.394	5271965	802605	1.090	0.158 #
12) T	2,4,5-T	0.000	14.553	0	634751	N.D.	0.406 #
14) T	DINOSEB	0.000	15.642	0	2271143	N.D.	1.517 #
15) T	Picloram	0.000	16.821	0	796575	N.D.	0.299 #
16) T	DCPA	0.000	16.840	0	396813	N.D.	0.165 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS110918\
Data File : PS002455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2018 23:39
Operator : EI\SJ
Sample : J5774-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 02:38:01 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

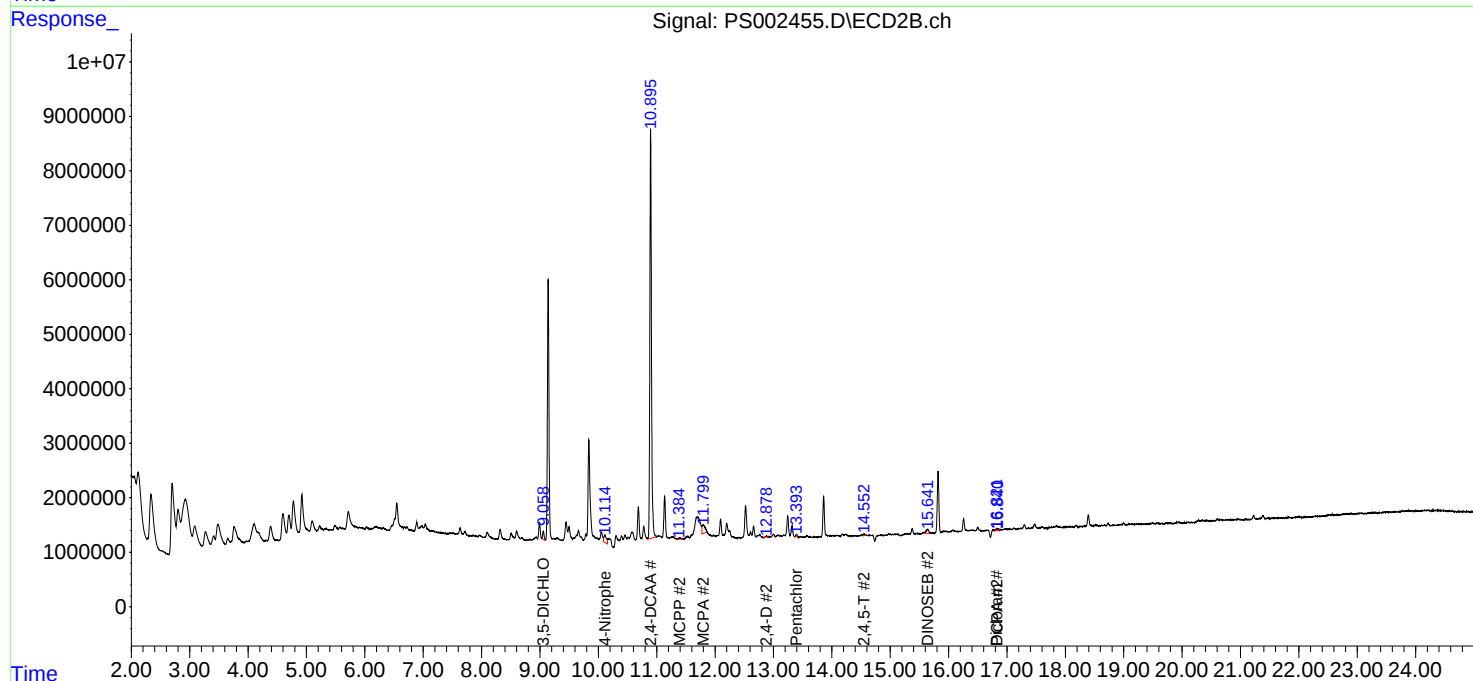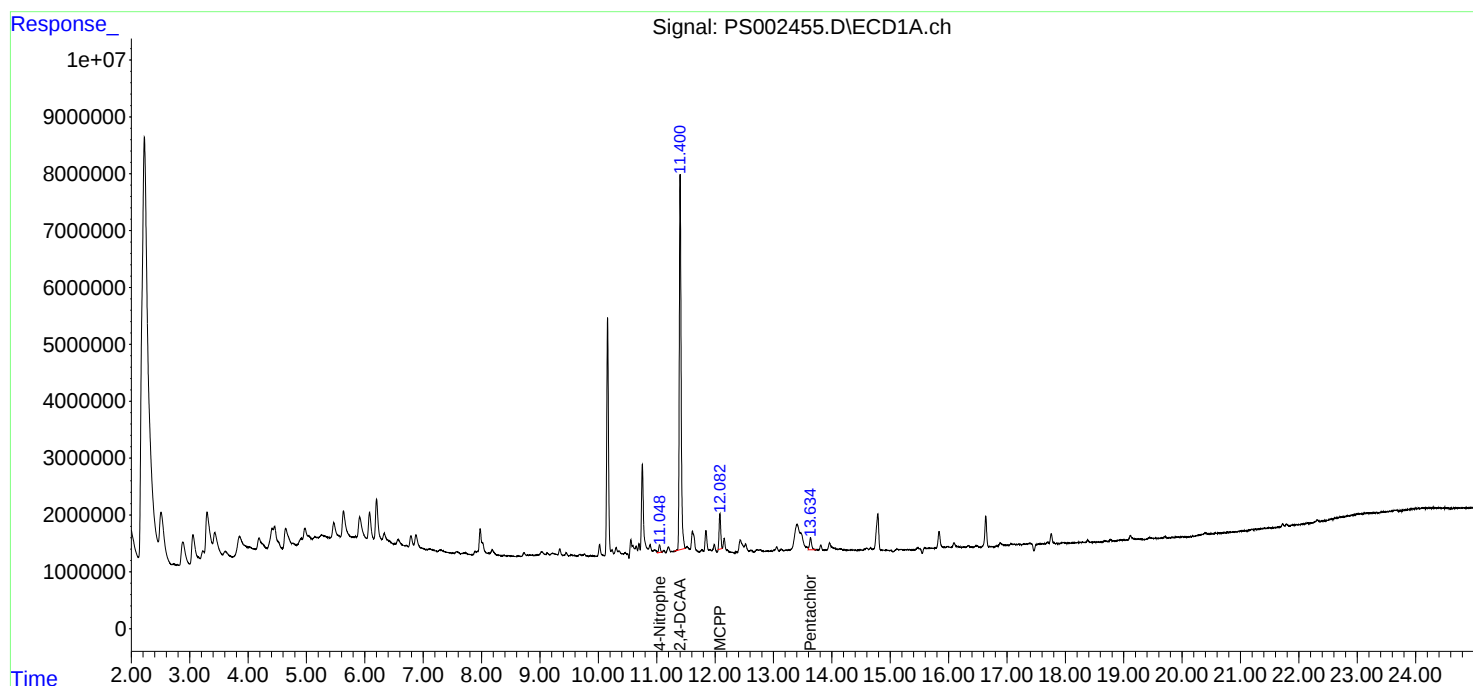


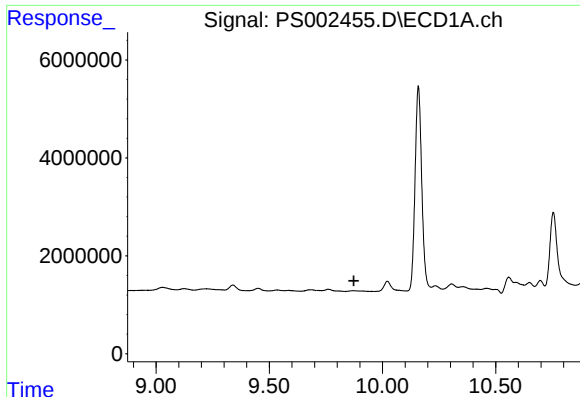

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.874 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

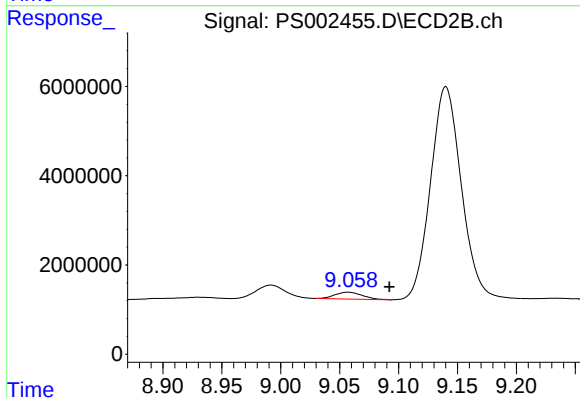


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.057 min
Delta R.T.: -0.035 min
Response: 2516655
Conc: 5.55 ng/ml

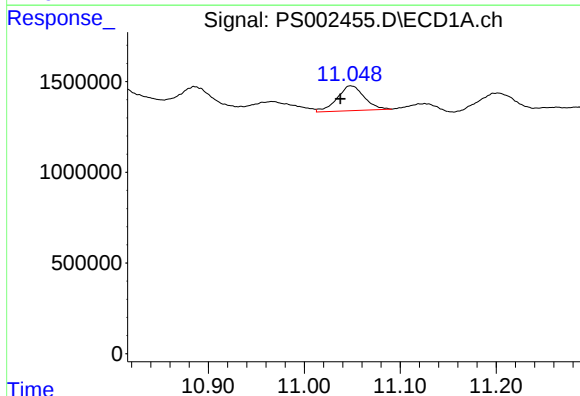


#3 4-Nitrophenol

R.T.: 11.049 min
Delta R.T.: 0.011 min
Response: 2683261
Conc: 16.54 ng/ml

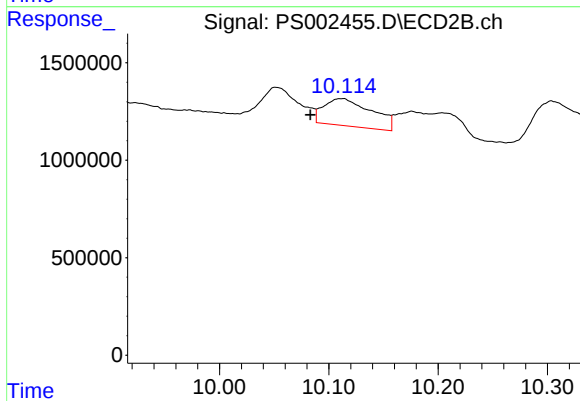

#3 4-Nitrophenol


R.T.: 10.113 min
Delta R.T.: 0.030 min
Response: 4287274
Conc: 24.47 ng/ml

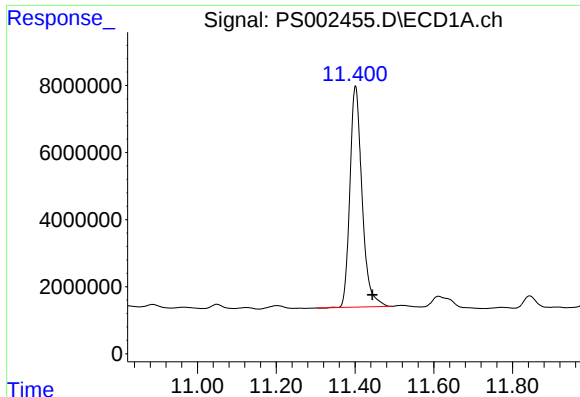

#4 2,4-DCAA


R.T.: 11.401 min
Delta R.T.: -0.042 min
Response: 141234781
Conc: 463.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

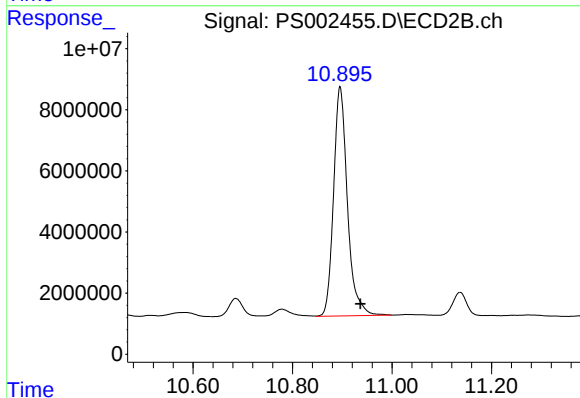


#4 2,4-DCAA

R.T.: 10.896 min
Delta R.T.: -0.041 min
Response: 145044804
Conc: 396.39 ng/ml

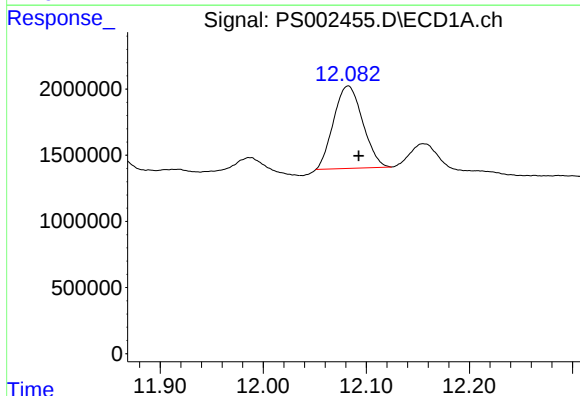


#6 MCP

R.T.: 12.082 min
Delta R.T.: -0.011 min
Response: 12219430
Conc: 13.02 ug/ml

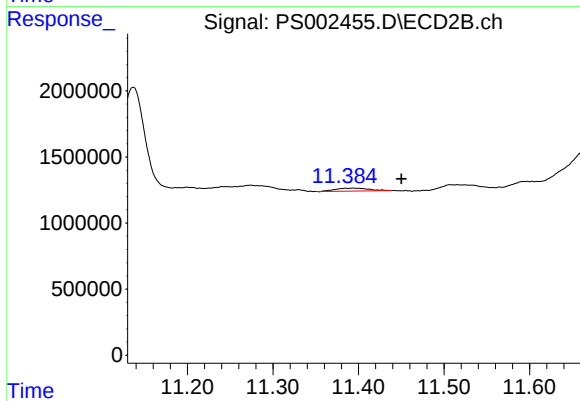

#6 MCP


R.T.: 11.394 min
Delta R.T.: -0.056 min
Response: 615964
Conc: 0.68 ug/ml

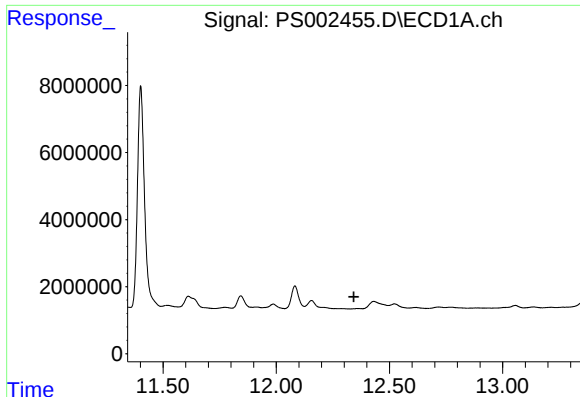

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

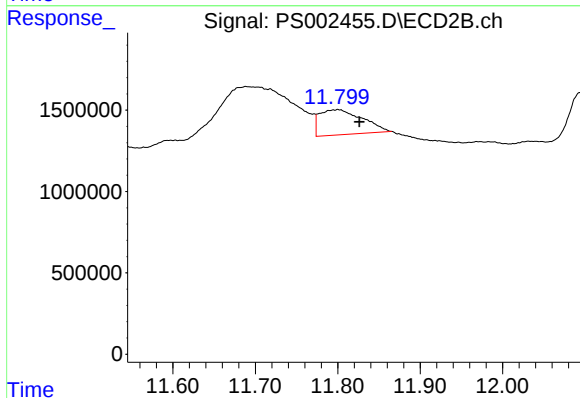


#7 MCPA

R.T.: 11.800 min
Delta R.T.: -0.026 min
Response: 5602573
Conc: 3.98 ug/ml

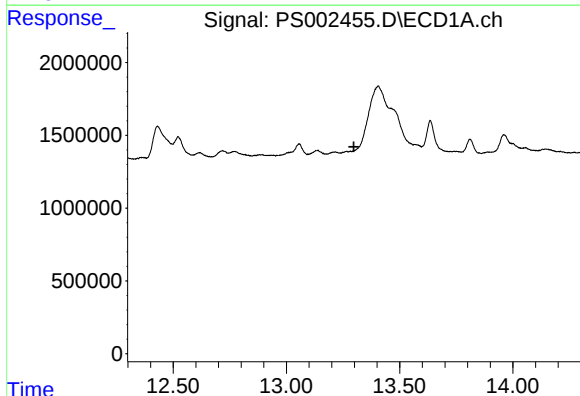


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.298 min
Response: 0
Conc: N.D.

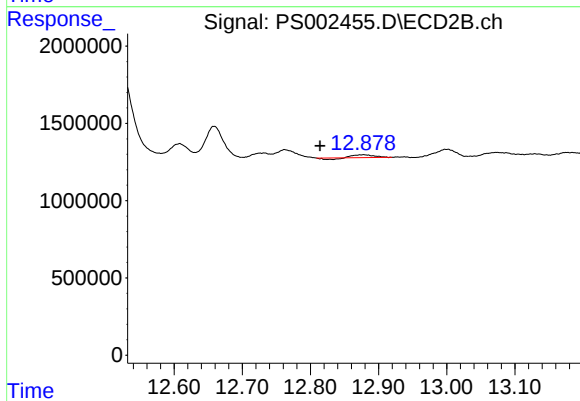

#9 2,4-D


R.T.: 12.878 min
Delta R.T.: 0.064 min
Response: 272535
Conc: 0.68 ng/ml

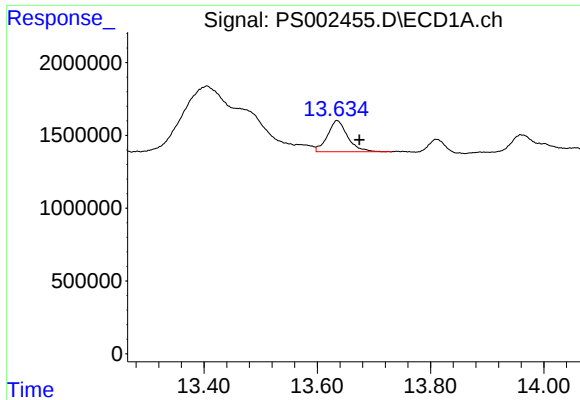

#10 Pentachlorophenol


R.T.: 13.635 min
Delta R.T.: -0.039 min
Response: 5271965
Conc: 1.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

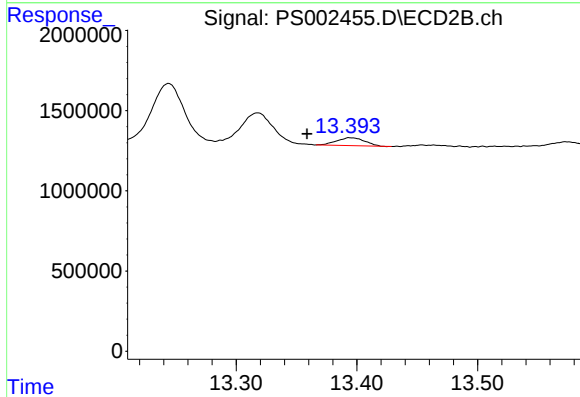


#10 Pentachlorophenol

R.T.: 13.394 min
Delta R.T.: 0.036 min
Response: 802605
Conc: 0.16 ng/ml

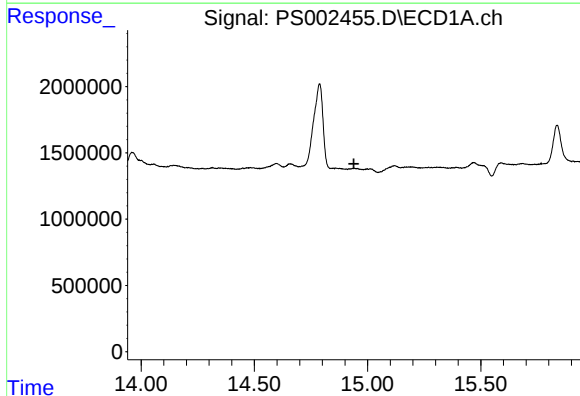


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 14.940 min
Response: 0
Conc: N.D.

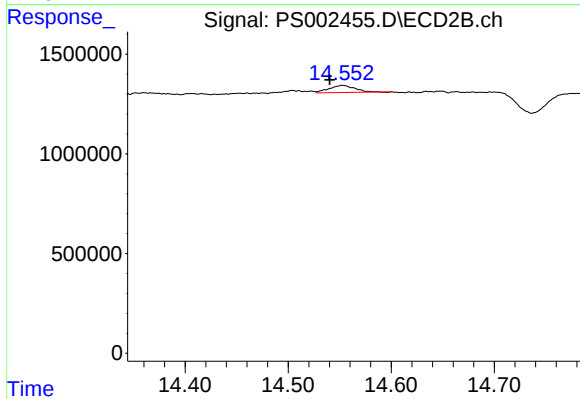

#12 2,4,5-T


R.T.: 14.553 min
Delta R.T.: 0.012 min
Response: 634751
Conc: 0.41 ng/ml

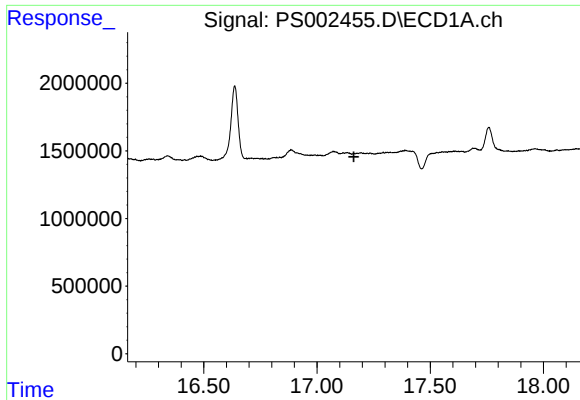

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.163 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

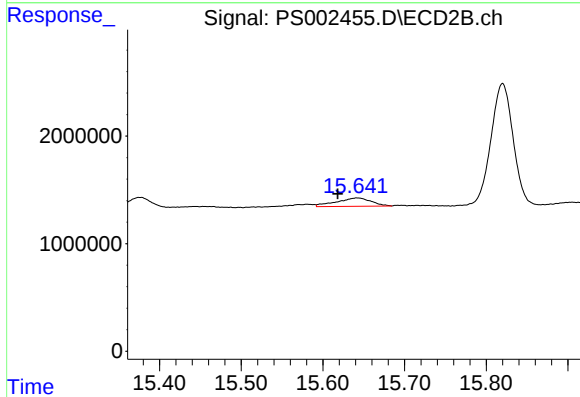


#14 DINOSEB

R.T.: 15.642 min
Delta R.T.: 0.024 min
Response: 2271143
Conc: 1.52 ng/ml

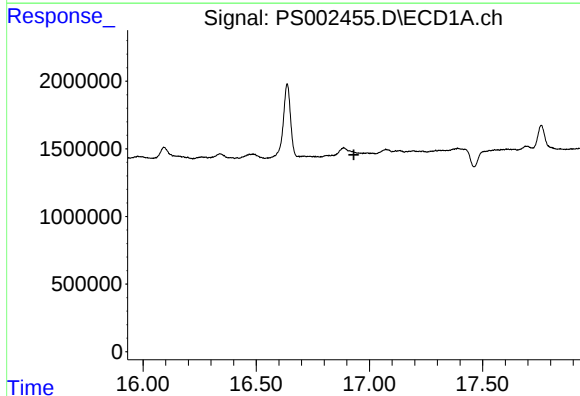


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.931 min
Response: 0
Conc: N.D.

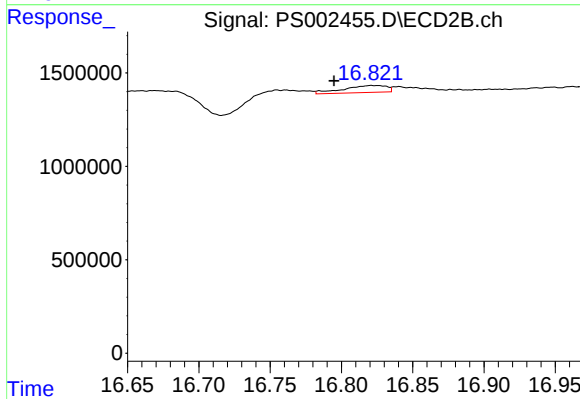

#15 Picloram


R.T.: 16.821 min
Delta R.T.: 0.026 min
Response: 796575
Conc: 0.30 ng/ml

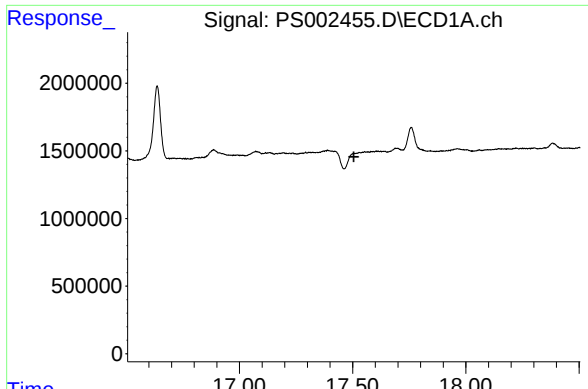

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.506 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

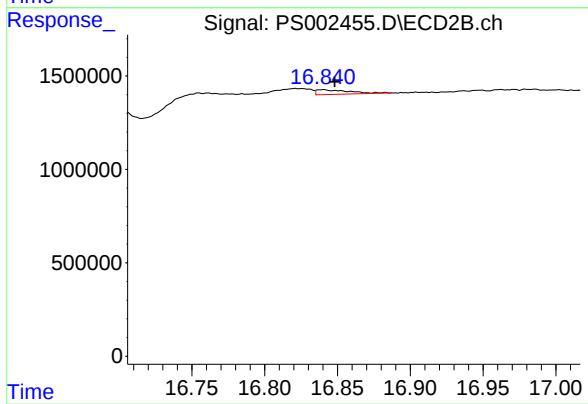

#16 DCPA

R.T.: 16.840 min
Delta R.T.: -0.008 min
Response: 396813
Conc: 0.17 ng/ml