

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111918\
 Data File : PS002441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2018 10:47 am
 Operator : EI\SJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDCCC750

Manual Integrations
 APPROVED

Sohil
 11/20/2018 2:41:28 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 02:32:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 09 15:54:35 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
4) S	2,4-DCAA	11.405	10.897	221.3E6	277.4E6	726.482m	758.195
Target Compounds							
1) T	Dalapon	2.931	2.373	307.5E6	308.5E6	697.457	716.704
2) T	3,5-DICHL...	9.834	9.053	316.7E6	314.8E6	683.579m	694.460m
3) T	4-Nitroph...	11.001	10.046	111.4E6	119.2E6	686.711	680.065
5) T	DICAMBA	11.713	11.179	990.6E6	983.2E6	714.951	726.817m
6) T	MCPD	12.052	11.410	71268696	66237391	75.936m	73.019m
7) T	MCPA	12.302	11.786	101.2E6	107.6E6	70.047m	76.490
8) T	DICHLORPROP	12.900	12.304	247.1E6	243.2E6	713.709	733.704m
9) T	2,4-D	13.260	12.775	211.6E6	271.7E6	658.250m	680.347m
10) T	Pentachlo...	13.635	13.319	3488.1E6	3694.5E6	721.103	725.973m
11) T	2,4,5-TP ...	14.504	13.938	1350.1E6	1462.1E6	718.444	724.794
12) T	2,4,5-T	14.902	14.501	1145.8E6	1094.9E6	679.771m	700.391
13) T	2,4-DB	15.648	15.152	127.6E6	147.1E6	658.486m	649.047m
14) T	DINOSEB	17.123	15.579	1003.0E6	1065.6E6	702.301	711.946
15) T	Picloram	16.894	16.755	1333.5E6	1946.0E6	627.903	731.478m
16) T	DCPA	17.467	16.809	1652.8E6	1580.0E6	713.443m	658.798m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111918\
Data File : PS002441.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2018 10:47 am
Operator : EI\SJ
Sample : HSTDCCT750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 02:32:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110918.M
Quant Title : 8080.M
QLast Update : Fri Nov 09 15:54:35 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

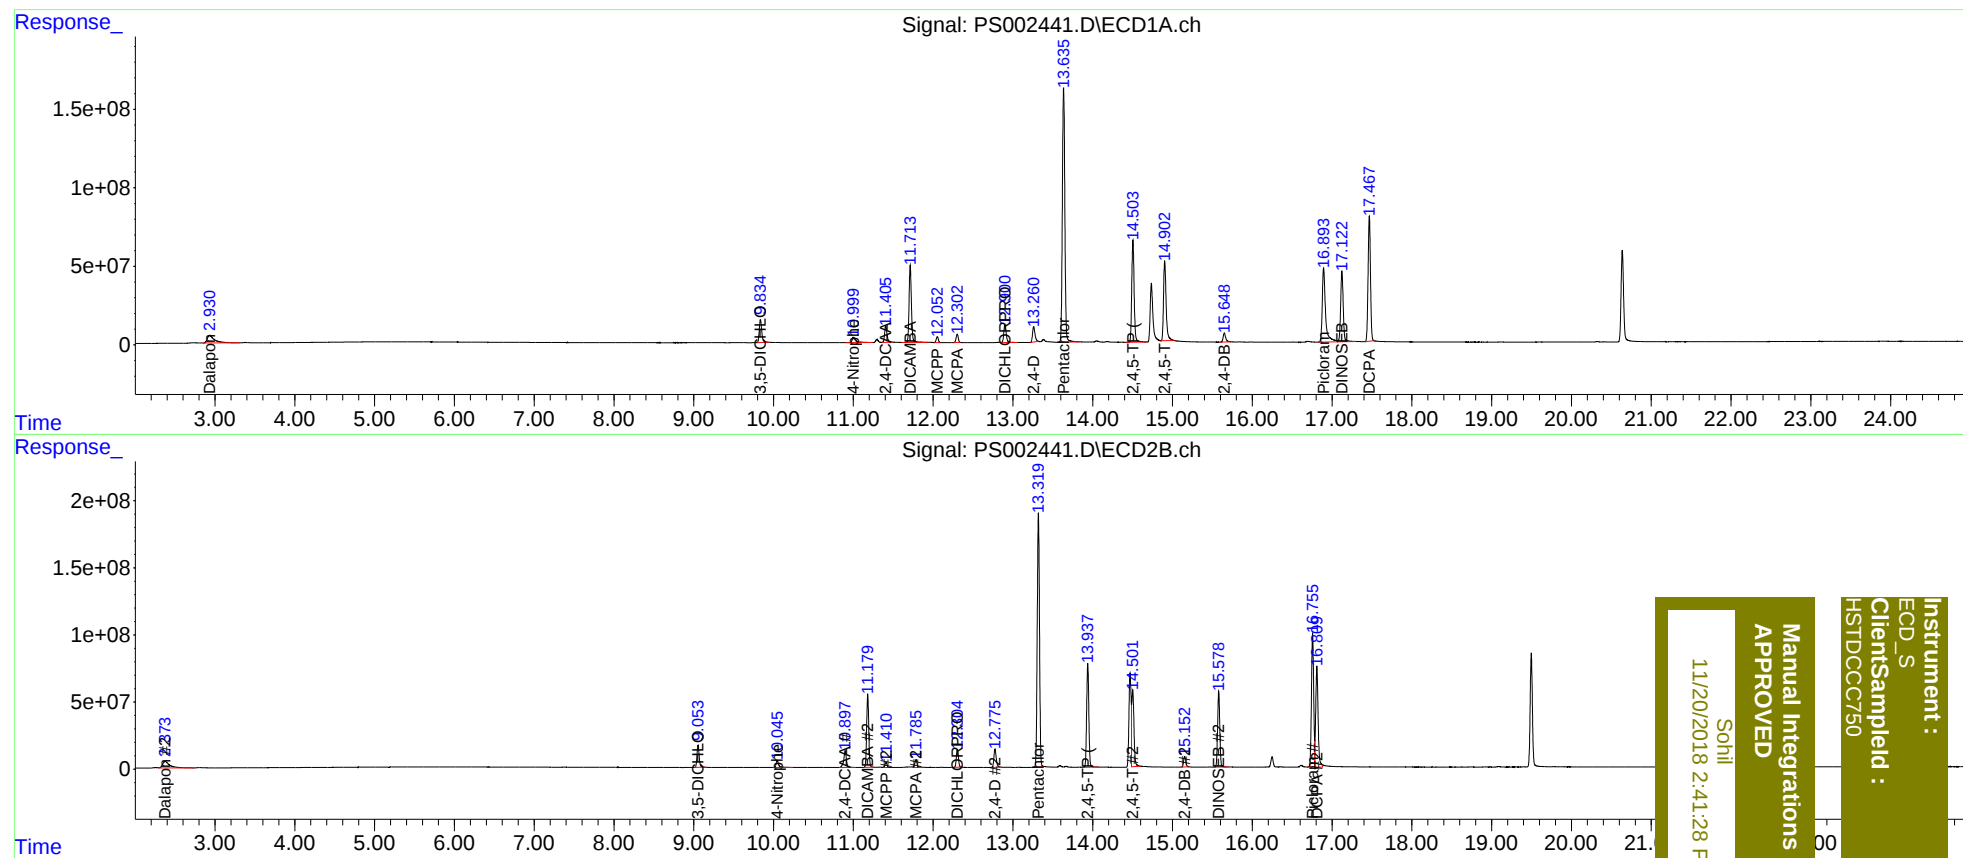

11/20/2018 2:41:28 PM

Manual Integrations
APPROVED

Sohil

Instrument :
ECD_S
Client Sampled :
HSTDCCT750