

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111919\
 Data File : PS007745.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2019 10:36
 Operator : SM\AJ
 Sample : K5863-07RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 10:52:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.436	5.160	292.8E6	145.2E6	212.628	206.736
Target Compounds							
1) T	Dalapon	2.000	1.705	125.4E6	412.7E6	69.333	347.568 #
2) T	3,5-DICHL...	0.000	4.452	0	8687220	N.D.	9.616
3) T	4-Nitroph...	0.000	4.837	0	18666545	N.D.	45.363
7) T	MCPA	0.000	5.476	0	53806849	N.D.	17.902
8) T	DICHLORPROP	0.000	5.821	0	7482163	N.D.	11.409
10) T	Pentachlo...	0.000	6.370	0	17852022	N.D.	1.823
11) T	2,4,5-TP ...	0.000	6.760	0	19011155	N.D.	4.855



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111919\
Data File : PS007745.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2019 10:36
Operator : SM\AJ
Sample : K5863-07RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 10:52:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

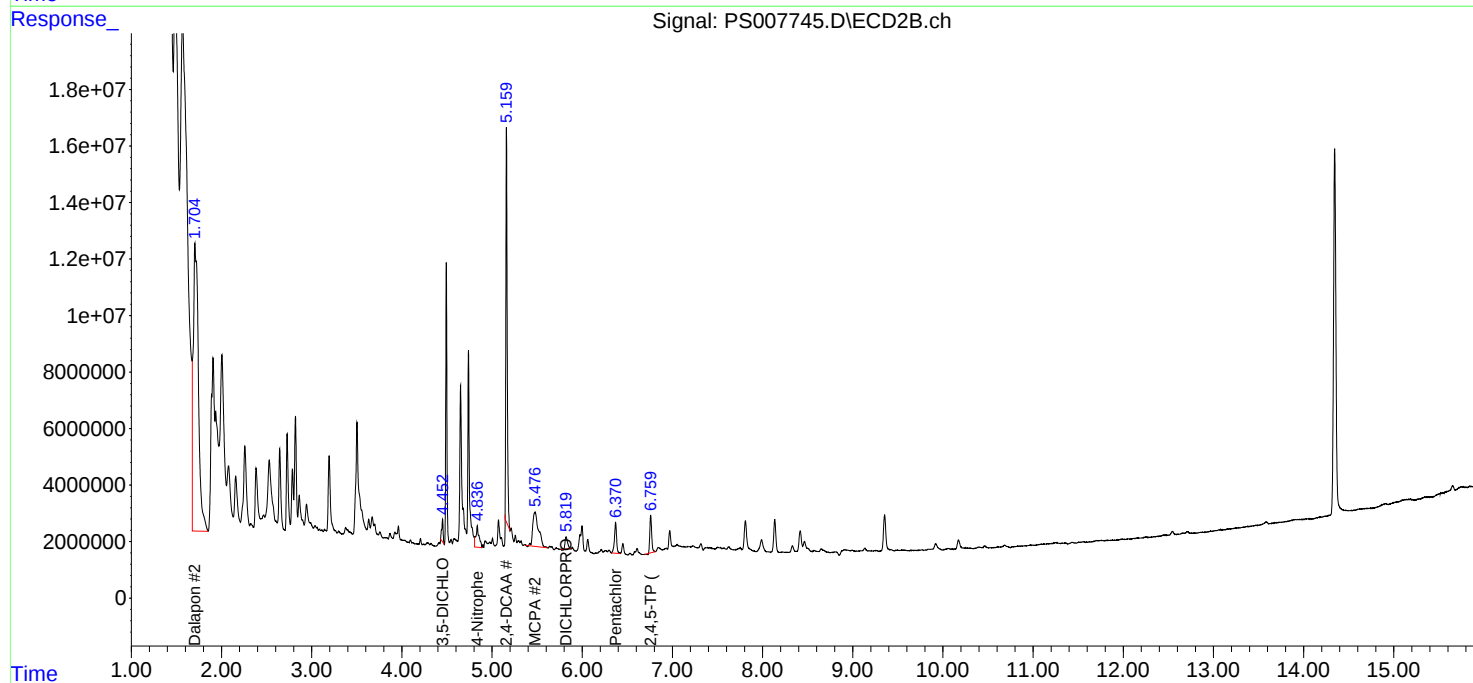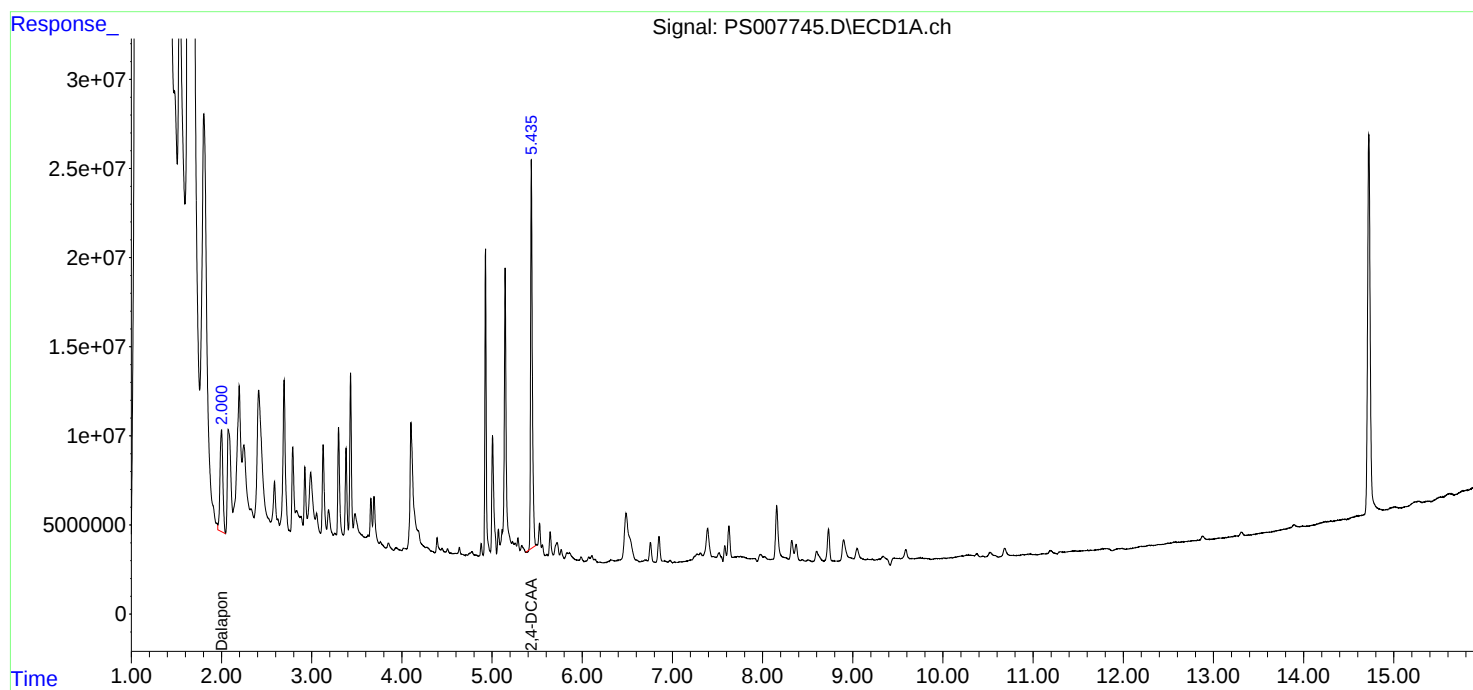


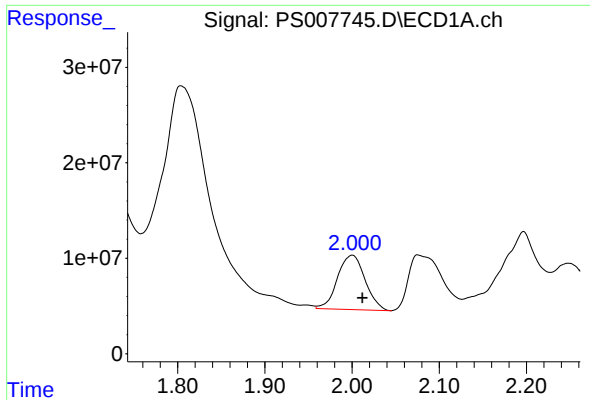

#1 Dalapon


R.T.: 2.000 min
Delta R.T.: -0.012 min
Response: 125435248
Conc: 69.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

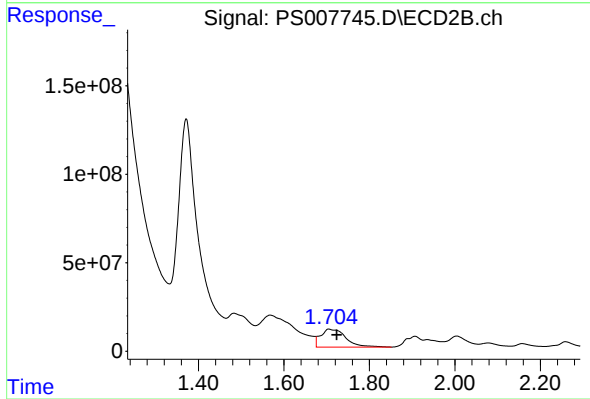


#1 Dalapon

R.T.: 1.705 min
Delta R.T.: -0.018 min
Response: 412703631
Conc: 347.57 ng/ml

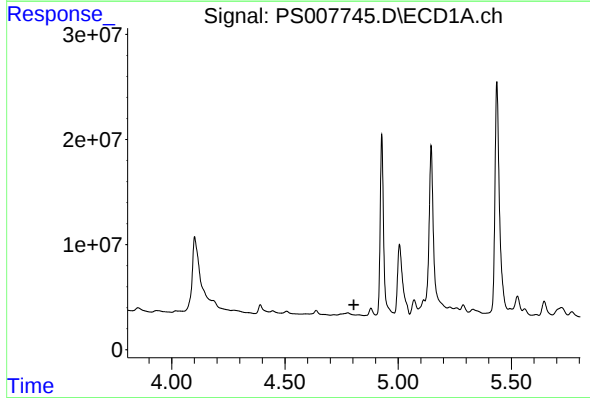


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

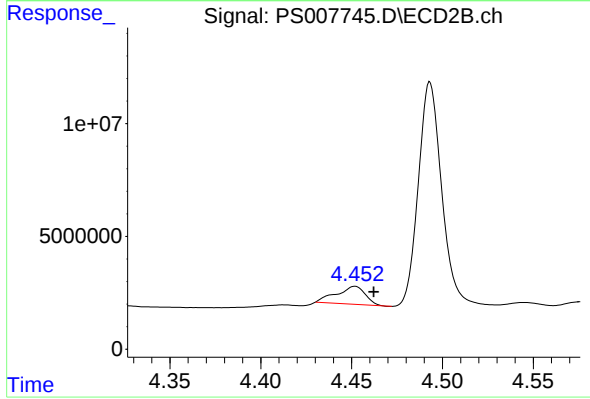

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.452 min
Delta R.T.: -0.011 min
Response: 8687220
Conc: 9.62 ng/ml

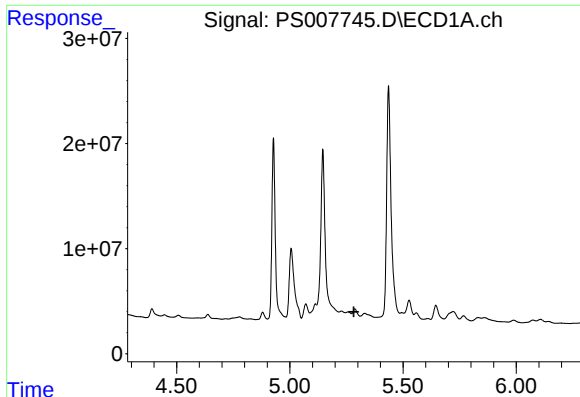

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

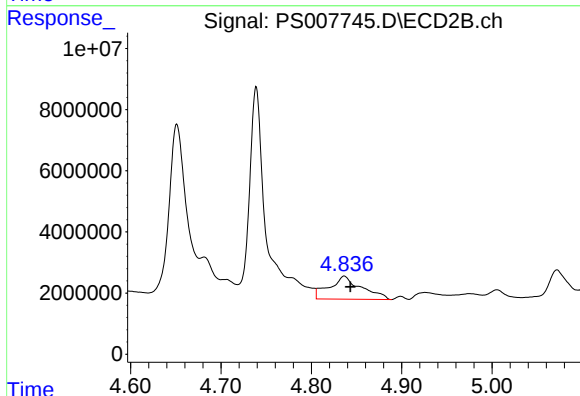


#3 4-Nitrophenol

R.T.: 4.837 min
Delta R.T.: -0.007 min
Response: 18666545
Conc: 45.36 ng/ml

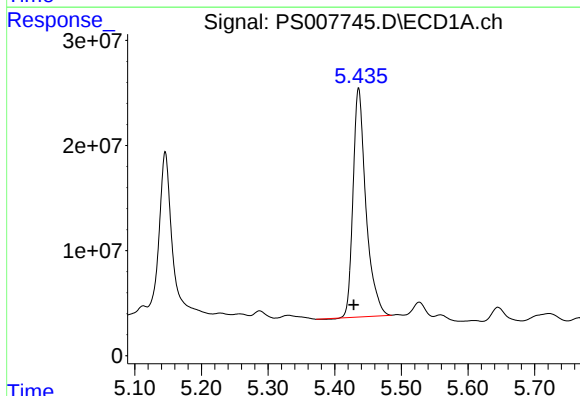


#4 2,4-DCAA

R.T.: 5.436 min
Delta R.T.: 0.008 min
Response: 292827747
Conc: 212.63 ng/ml

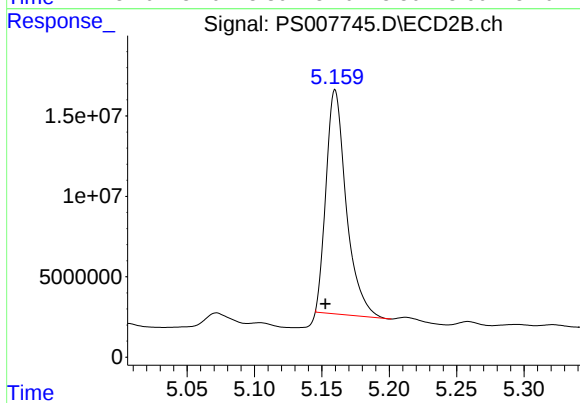

#4 2,4-DCAA


R.T.: 5.160 min
Delta R.T.: 0.007 min
Response: 145245251
Conc: 206.74 ng/ml

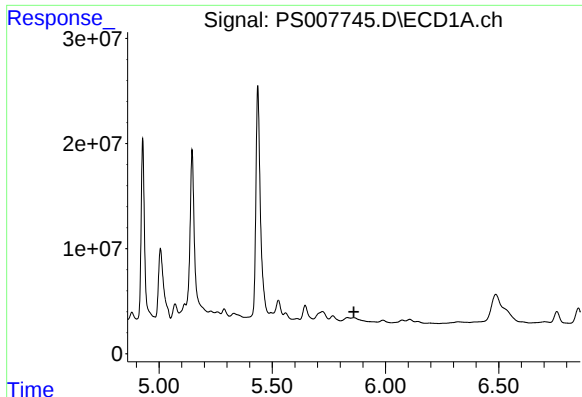

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.860 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

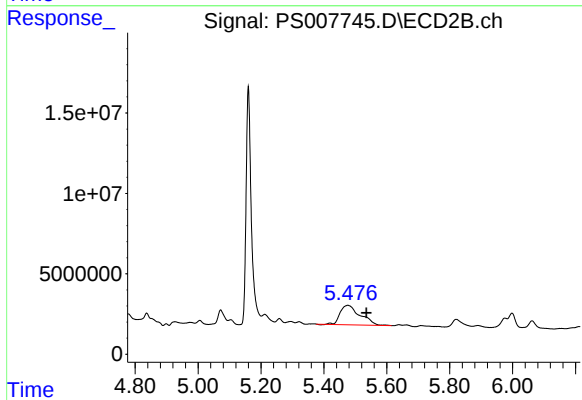


#7 MCPA

R.T.: 5.476 min
Delta R.T.: -0.060 min
Response: 53806849
Conc: 17.90 ug/ml

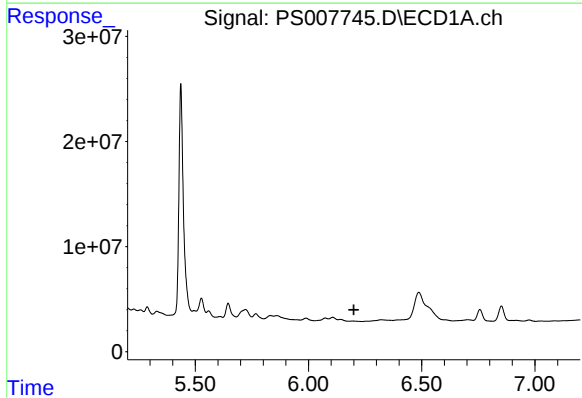


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 6.200 min
Response: 0
Conc: N.D.

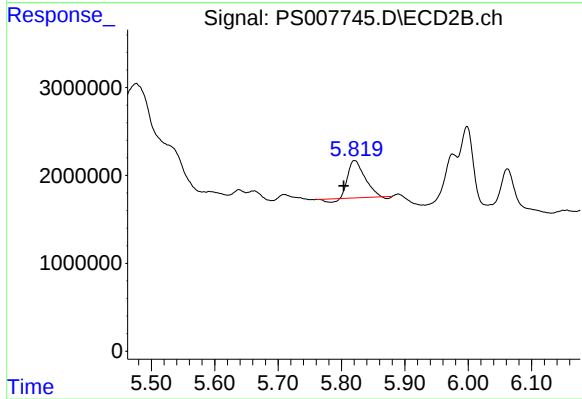

#8 DICHLORPROP


R.T.: 5.821 min
Delta R.T.: 0.017 min
Response: 7482163
Conc: 11.41 ng/ml

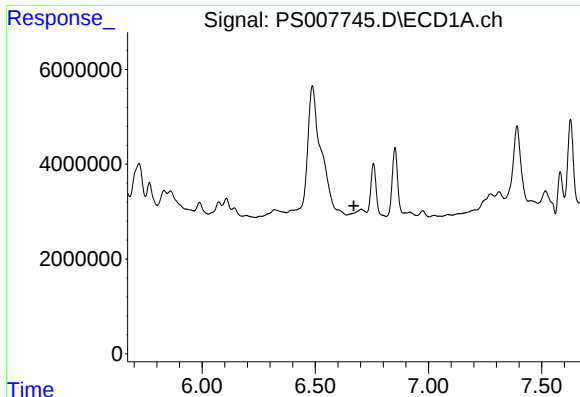

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.671 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

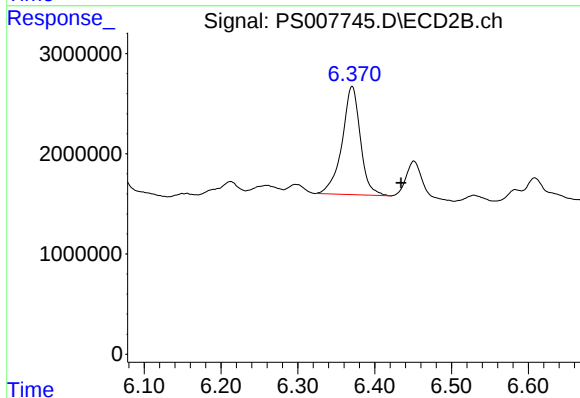


#10 Pentachlorophenol

R.T.: 6.370 min
Delta R.T.: -0.064 min
Response: 17852022
Conc: 1.82 ng/ml

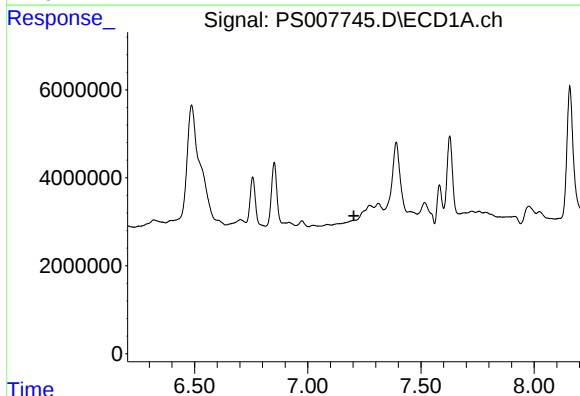

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.203 min
Response: 0
Conc: N.D.

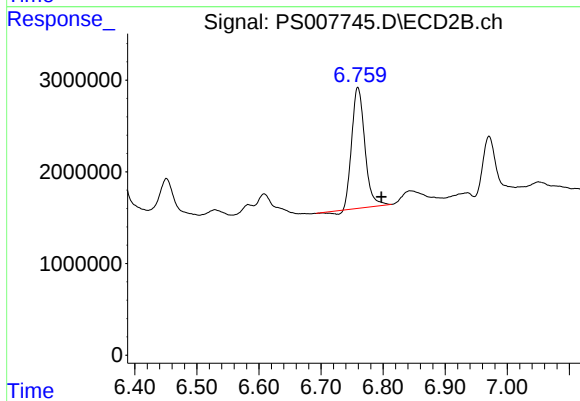

#11 2,4,5-TP (SILVEX)

R.T.: 6.760 min
Delta R.T.: -0.037 min
Response: 19011155
Conc: 4.85 ng/ml