

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111919\
 Data File : PS007746.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2019 10:58
 Operator : SM\AJ
 Sample : K5782-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 11:21:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.427	0.000	514.2E6	0	373.371	N.D. #
Target Compounds							
1) T	Dalapon	1.991	1.698	114.9E6	337.0E6	63.534	283.850 #
2) T	3,5-DICHL...	0.000	4.444	0	4831793	N.D.	5.348
3) T	4-Nitroph...	0.000	4.829	0	17295883	N.D.	42.032
7) T	MCPA	0.000	5.509	0	14757036	N.D.	4.910
8) T	DICHLORPROP	0.000	5.813	0	10873828	N.D.	16.581
9) T	2,4-D	6.477	0.000	103.0E6	0	73.432	N.D. #
11) T	2,4,5-TP ...	0.000	6.752	0	18214965	N.D.	4.652



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111919\
Data File : PS007746.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2019 10:58
Operator : SM\AJ
Sample : K5782-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 11:21:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

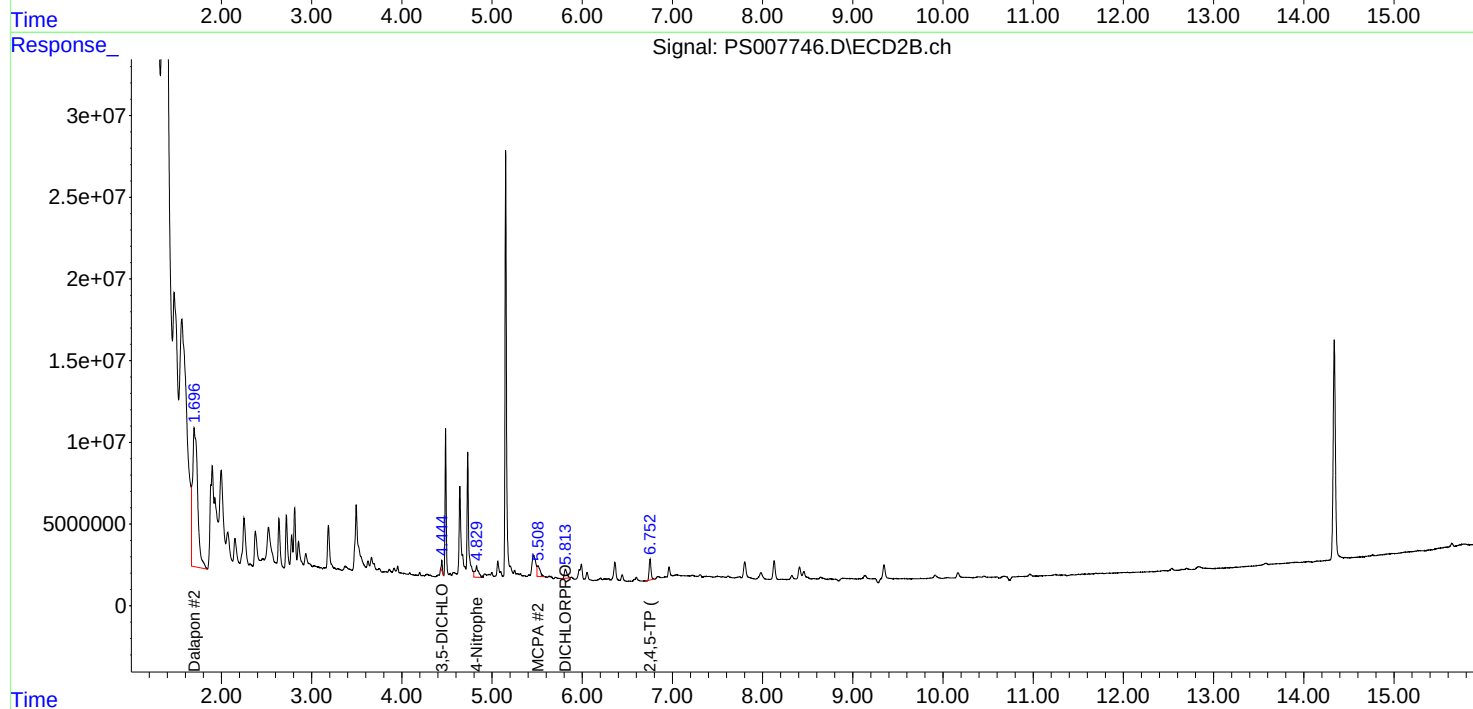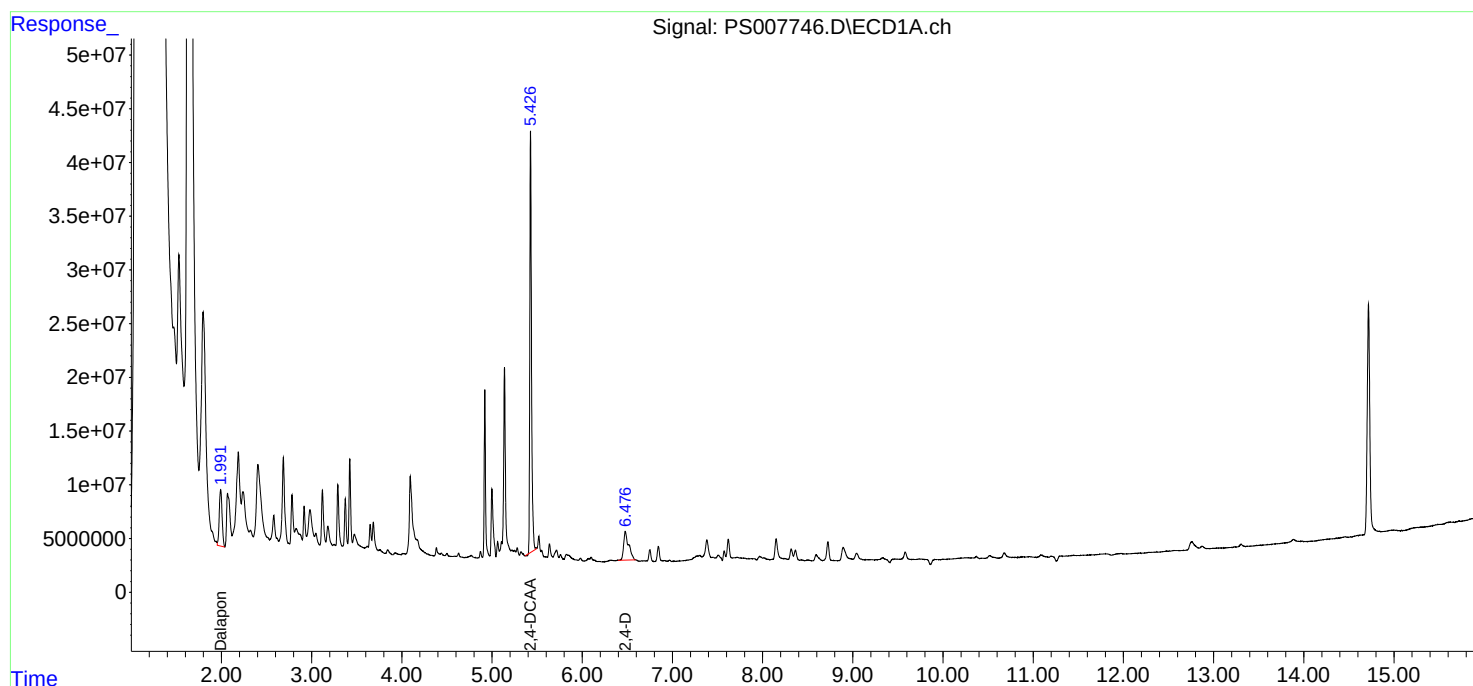


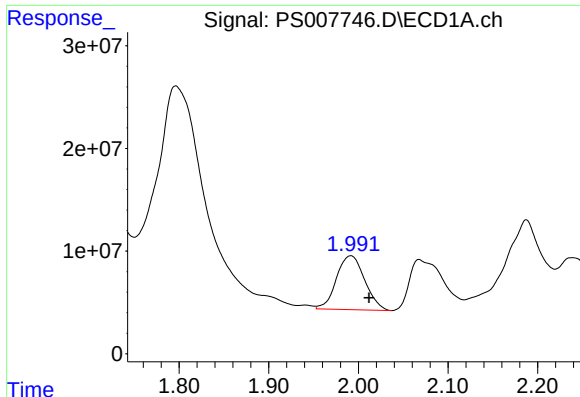

#1 Dalapon


R.T.: 1.991 min
Delta R.T.: -0.021 min
Response: 114944000
Conc: 63.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

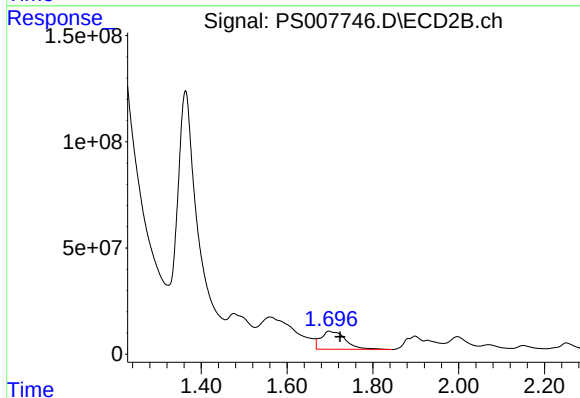


#1 Dalapon

R.T.: 1.698 min
Delta R.T.: -0.026 min
Response: 337043789
Conc: 283.85 ng/ml

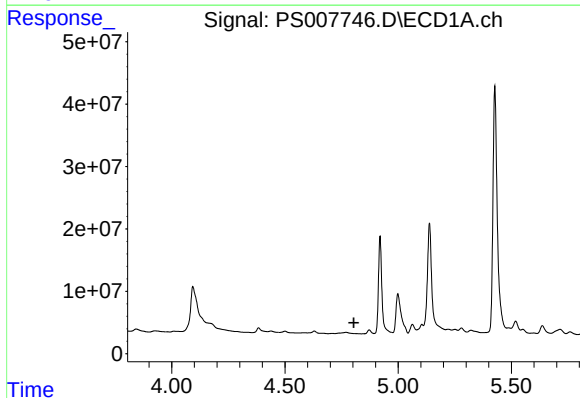


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.804 min
Response: 0
Conc: N.D.

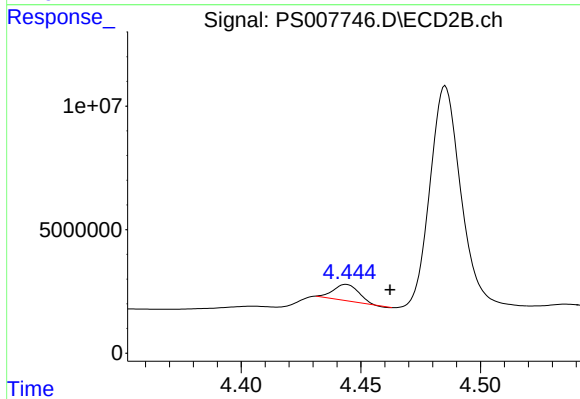

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.444 min
Delta R.T.: -0.018 min
Response: 4831793
Conc: 5.35 ng/ml

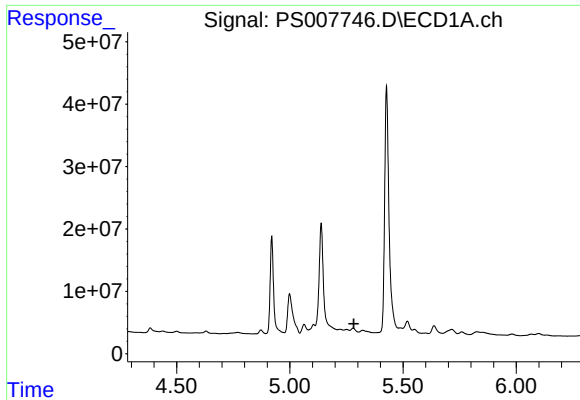

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

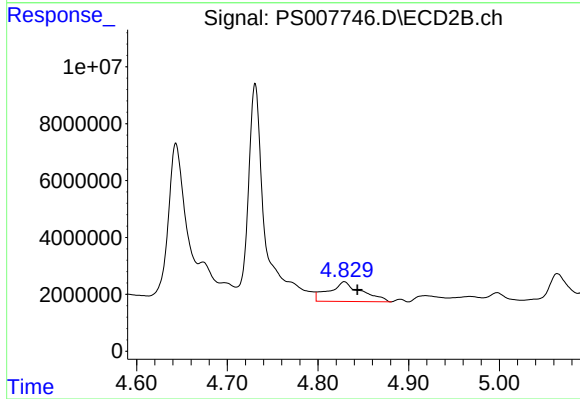


#3 4-Nitrophenol

R.T.: 4.829 min
Delta R.T.: -0.014 min
Response: 17295883
Conc: 42.03 ng/ml

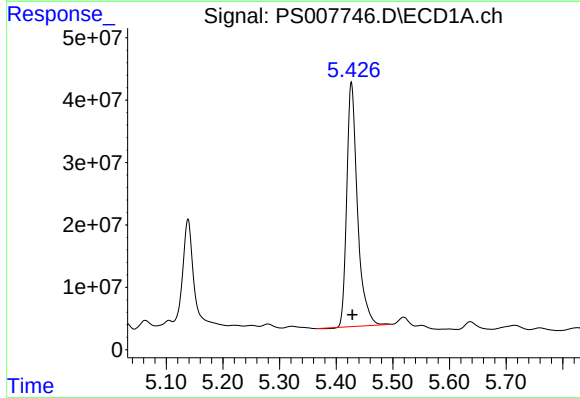


#4 2,4-DCAA

R.T.: 5.427 min
Delta R.T.: -0.001 min
Response: 514200170
Conc: 373.37 ng/ml

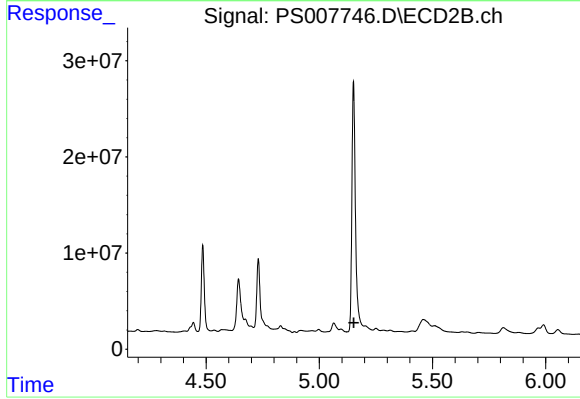

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 5.153 min
Response: 0
Conc: N.D.

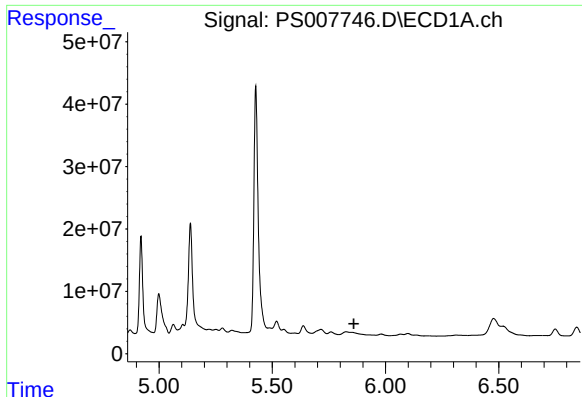

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 5.860 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

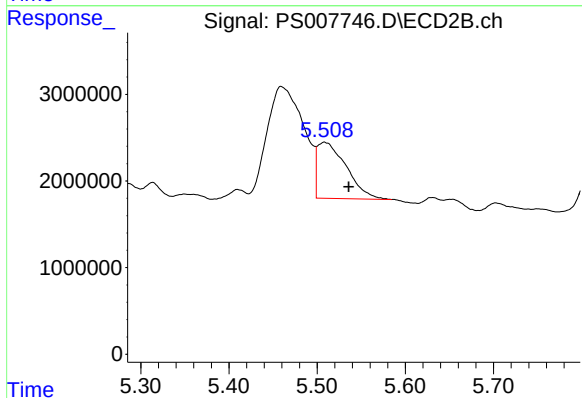


#7 MCPA

R.T.: 5.509 min
Delta R.T.: -0.027 min
Response: 14757036
Conc: 4.91 ug/ml

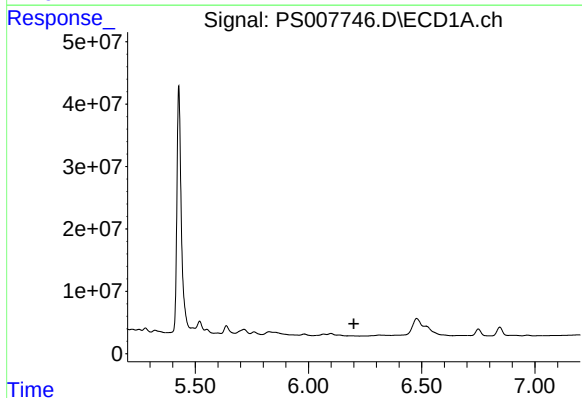


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.200 min
Response: 0
Conc: N.D.

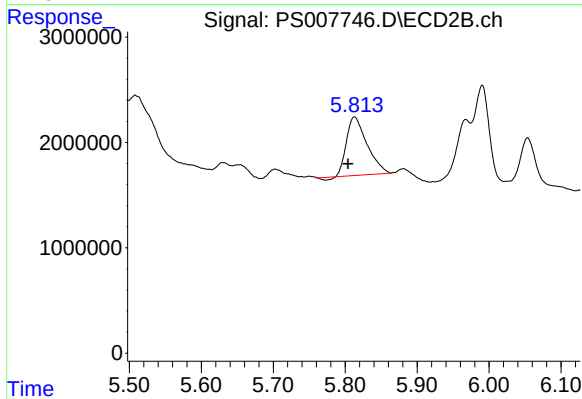

#8 DICHLORPROP


R.T.: 5.813 min
Delta R.T.: 0.009 min
Response: 10873828
Conc: 16.58 ng/ml

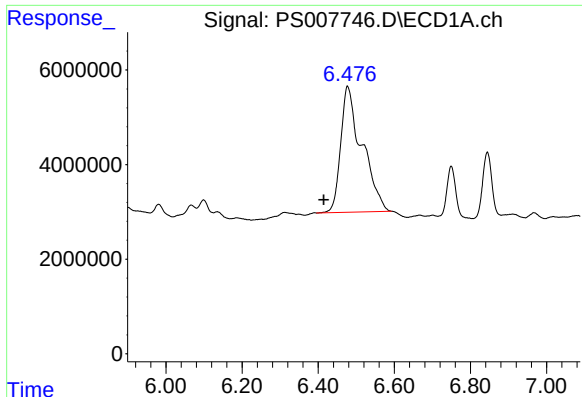

#9 2,4-D


R.T.: 6.477 min
Delta R.T.: 0.063 min
Response: 102991575
Conc: 73.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

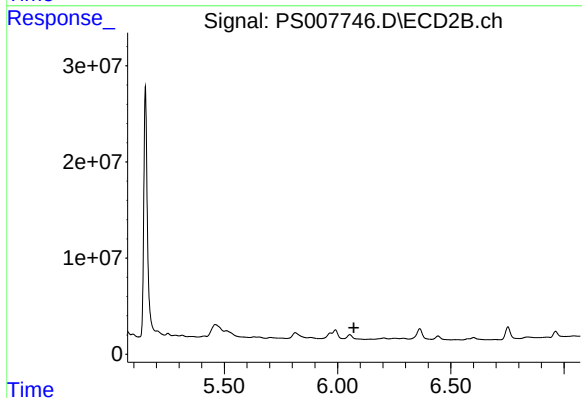


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

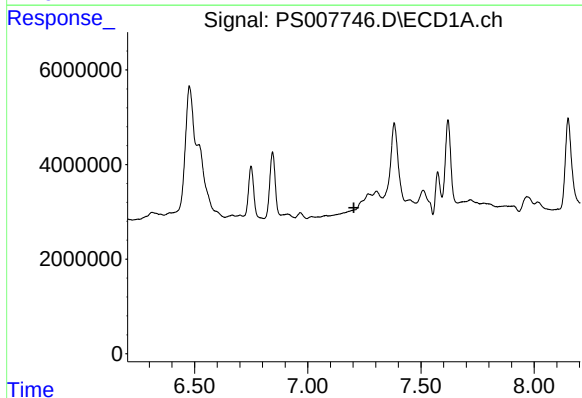

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.203 min
Response: 0
Conc: N.D.

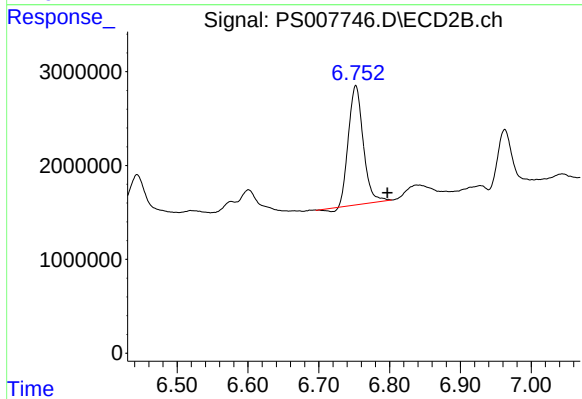

#11 2,4,5-TP (SILVEX)

R.T.: 6.752 min
Delta R.T.: -0.045 min
Response: 18214965
Conc: 4.65 ng/ml