

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111919\
 Data File : PS007748.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2019 12:23
 Operator : SM\AJ
 Sample : PB124879BS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 13:55:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
 Quant Title : 8080.M
 QLast Update : Wed Nov 06 02:45:11 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.424	0.000	566.0E6	0	410.974	N.D. #
Target Compounds							
1) T	Dalapon	2.005	1.718	753.1E6	511.8E6	416.249	431.065
2) T	3,5-DICHL...	4.798	4.458	788.3E6	408.7E6	441.868	452.339
3) T	4-Nitroph...	5.282	4.841	227.7E6	116.0E6	357.358	281.916
5) T	DICAMBA	5.572	5.272	2247.0E6	1117.0E6	441.671	422.084
6) T	MCPD	5.722	5.354	167.0E6	84042801	43.829	43.261
7) T	MCPA	5.852	5.527	240.0E6	147.3E6	43.596	48.998
8) T	DICHLORPROP	6.195	5.799	567.9E6	305.5E6	449.309	465.788
9) T	2,4-D	6.410	6.068	729.0E6	414.4E6	519.761	513.882
10) T	Pentachlo...	6.665	6.429	9362.7E6	4725.4E6	494.046	482.556
11) T	2,4,5-TP ...	7.198	6.791	3683.6E6	1882.0E6	490.170	480.616
12) T	2,4,5-T	7.469	7.151	3666.6E6	1671.0E6	447.911	452.478
13) T	2,4-DB	7.998	7.636	410.7E6	230.9E6	384.065	472.404
14) T	DINOSEB	9.077	7.943	2640.1E6	1221.4E6	439.615	420.154
15) T	Picloram	8.916	8.879	4568.1E6	2394.2E6	411.423	408.646
16) T	DCPA	9.351	8.834	3224.6E6	1465.2E6	328.770	280.398



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111919\
Data File : PS007748.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2019 12:23
Operator : SM\AJ
Sample : PB124879BS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 13:55:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110619.M
Quant Title : 8080.M
QLast Update : Wed Nov 06 02:45:11 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

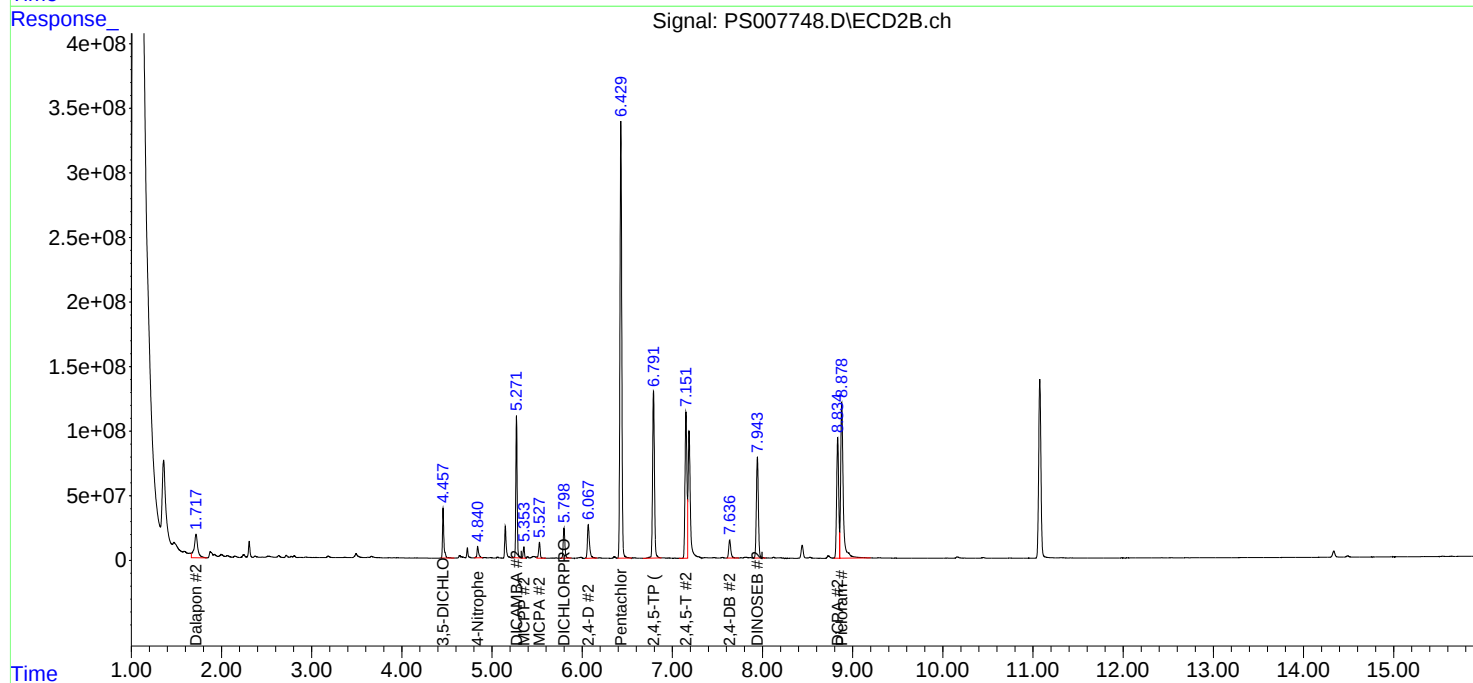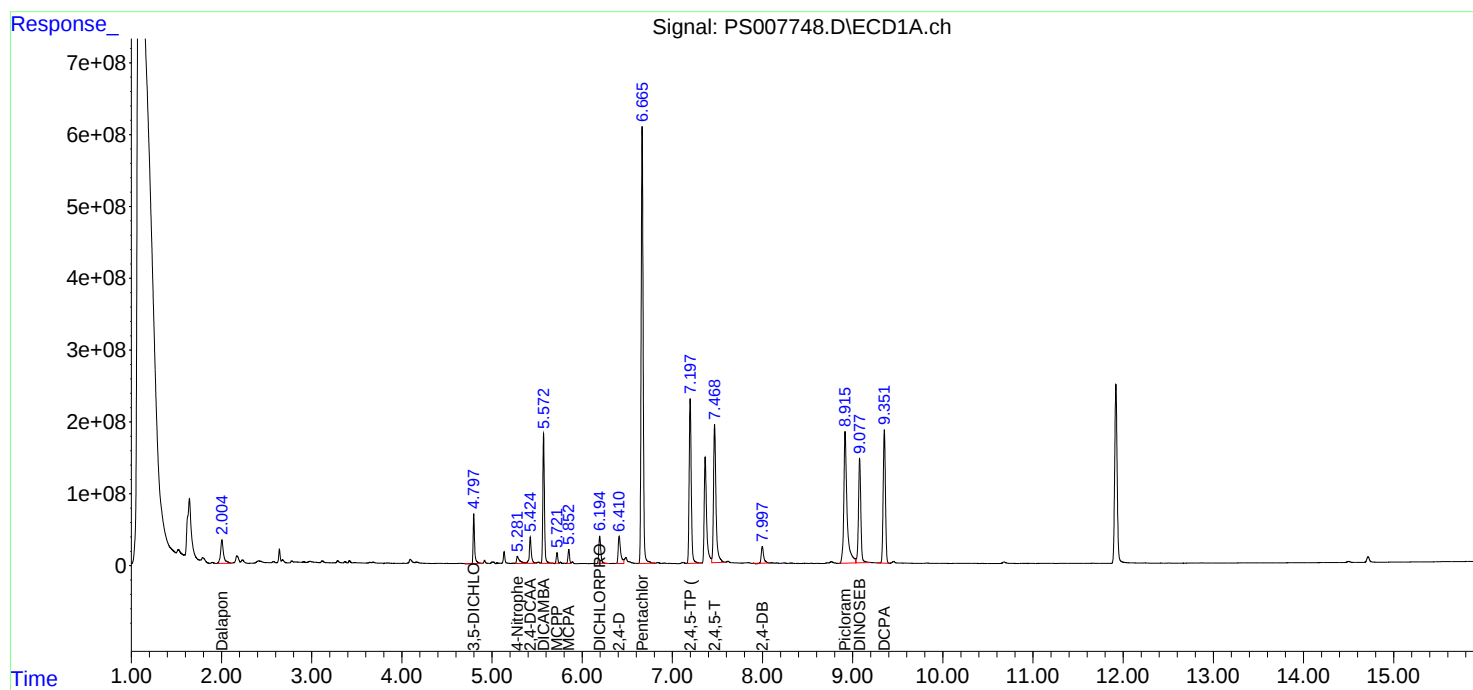


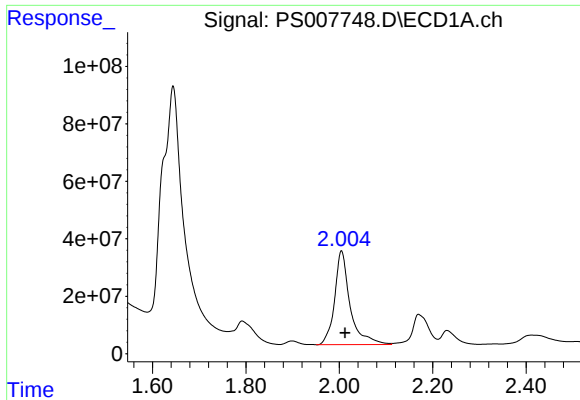

#1 Dalapon


R.T.: 2.005 min
Delta R.T.: -0.007 min
Response: 753069583
Conc: 416.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

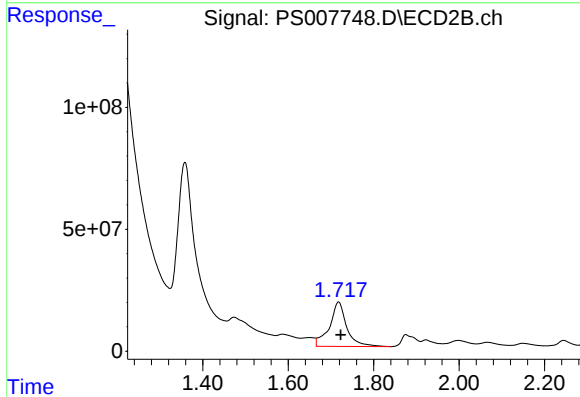


#1 Dalapon

R.T.: 1.718 min
Delta R.T.: -0.005 min
Response: 511847726
Conc: 431.07 ng/ml

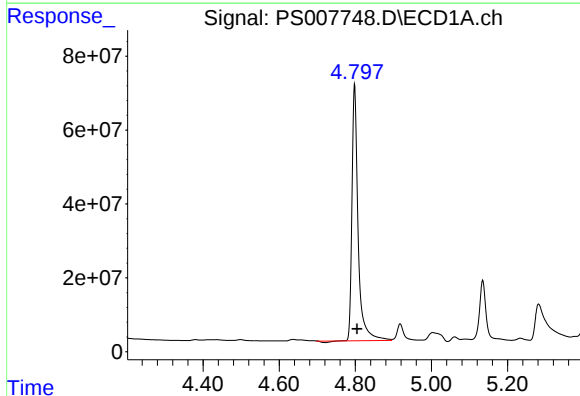


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.798 min
Delta R.T.: -0.006 min
Response: 788336397
Conc: 441.87 ng/ml

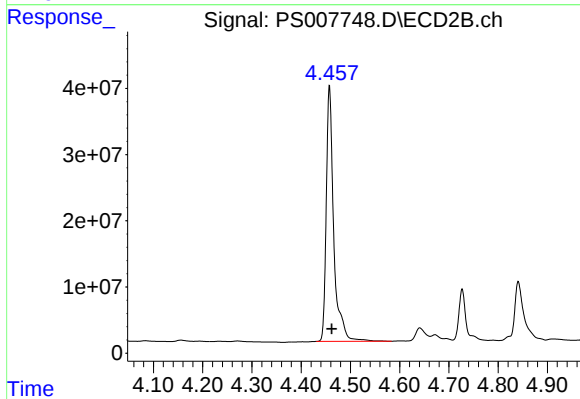

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.458 min
Delta R.T.: -0.005 min
Response: 408656948
Conc: 452.34 ng/ml

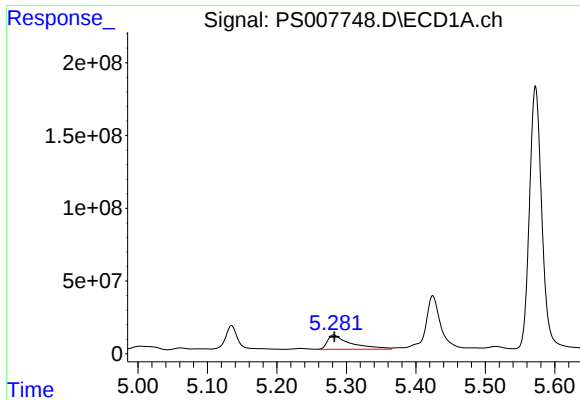

#3 4-Nitrophenol


R.T.: 5.282 min
Delta R.T.: 0.000 min
Response: 227741858
Conc: 357.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

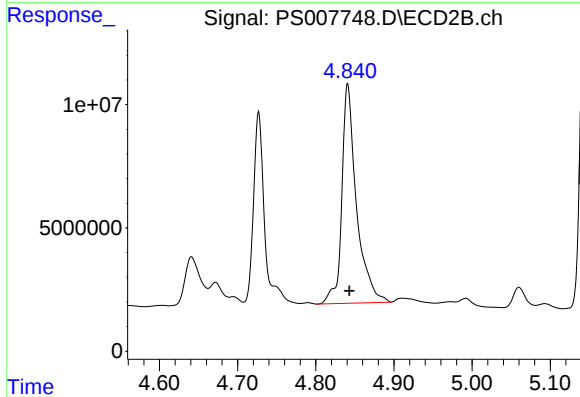


#3 4-Nitrophenol

R.T.: 4.841 min
Delta R.T.: -0.002 min
Response: 116007048
Conc: 281.92 ng/ml

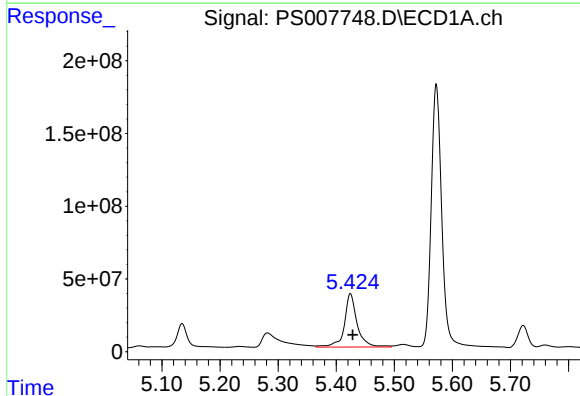


#4 2,4-DCAA

R.T.: 5.424 min
Delta R.T.: -0.004 min
Response: 565987219
Conc: 410.97 ng/ml

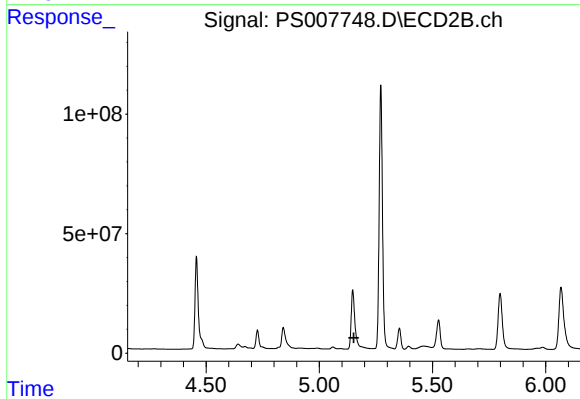

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 5.153 min
Response: 0
Conc: N.D.

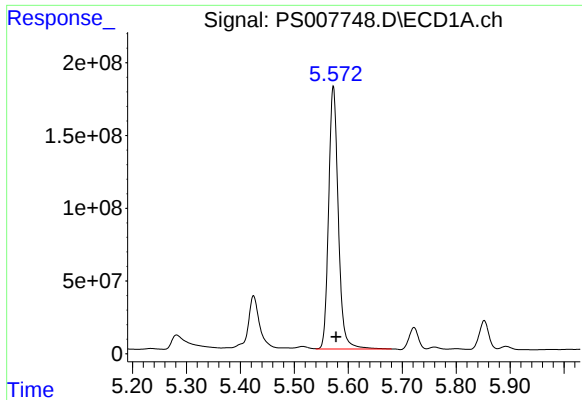

#5 DICAMBA


R.T.: 5.572 min
Delta R.T.: -0.005 min
Response: 2246954035
Conc: 441.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

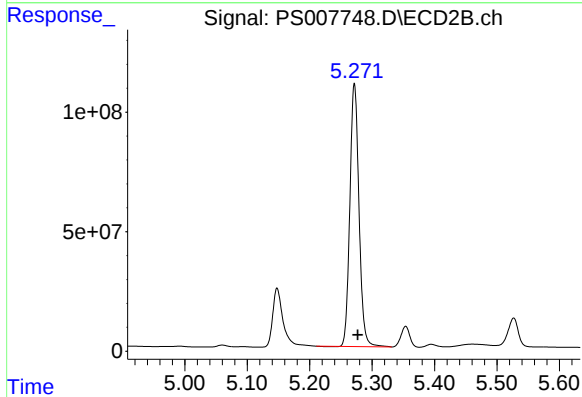


#5 DICAMBA

R.T.: 5.272 min
Delta R.T.: -0.005 min
Response: 1116977322
Conc: 422.08 ng/ml

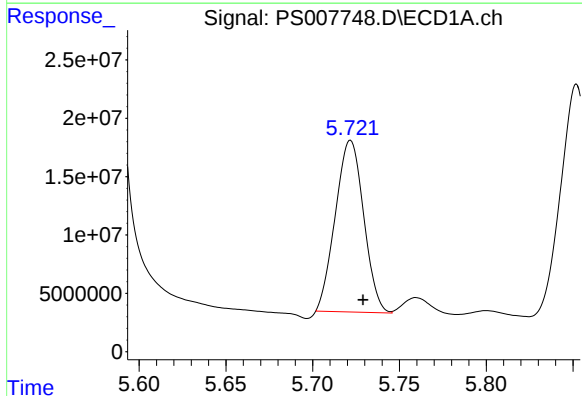


#6 MCP

R.T.: 5.722 min
Delta R.T.: -0.007 min
Response: 167033208
Conc: 43.83 ug/ml

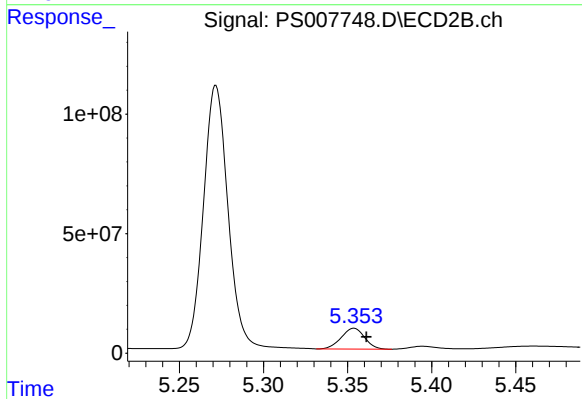

#6 MCP


R.T.: 5.354 min
Delta R.T.: -0.007 min
Response: 84042801
Conc: 43.26 ug/ml

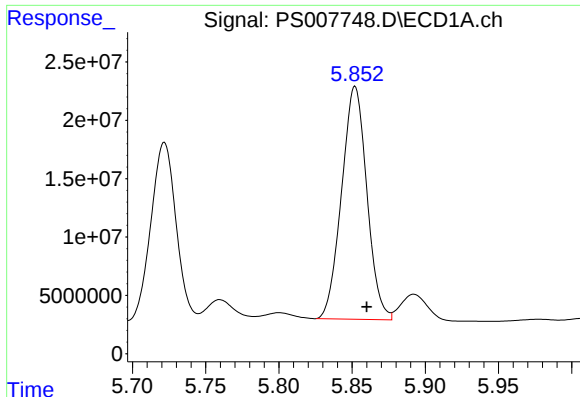

#7 MCPA


R.T.: 5.852 min
Delta R.T.: -0.008 min
Response: 239965938
Conc: 43.60 ug/ml

Instrument :
ECD_S
ClientSampleId :

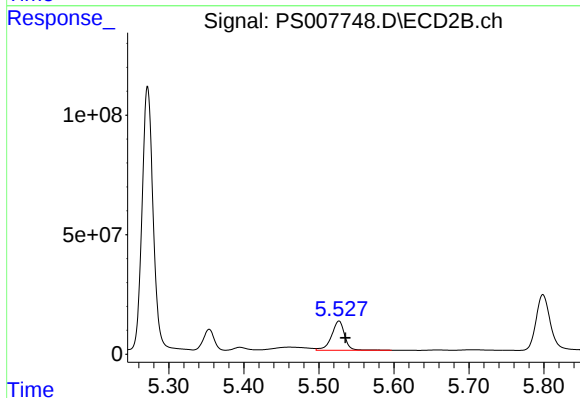


#7 MCPA

R.T.: 5.527 min
Delta R.T.: -0.009 min
Response: 147274033
Conc: 49.00 ug/ml

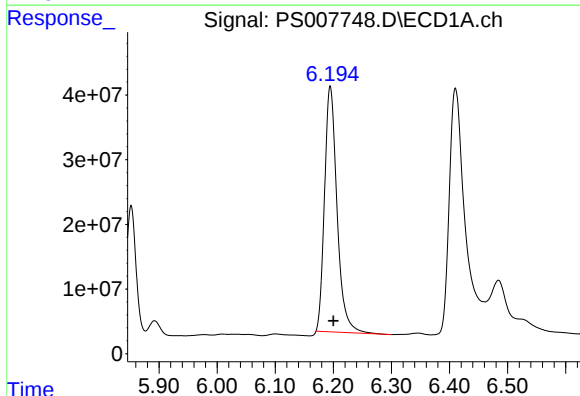


#8 DICHLORPROP

R.T.: 6.195 min
Delta R.T.: -0.005 min
Response: 567898703
Conc: 449.31 ng/ml

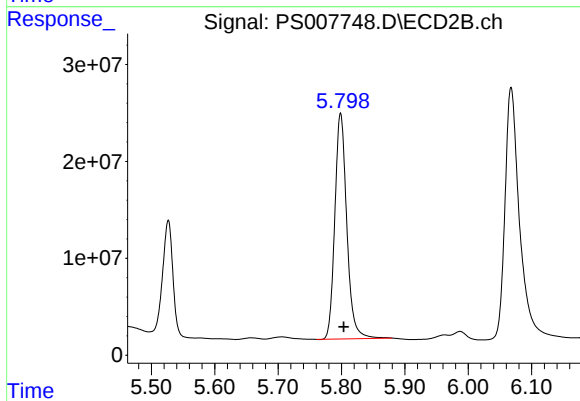

#8 DICHLORPROP


R.T.: 5.799 min
Delta R.T.: -0.005 min
Response: 305463249
Conc: 465.79 ng/ml

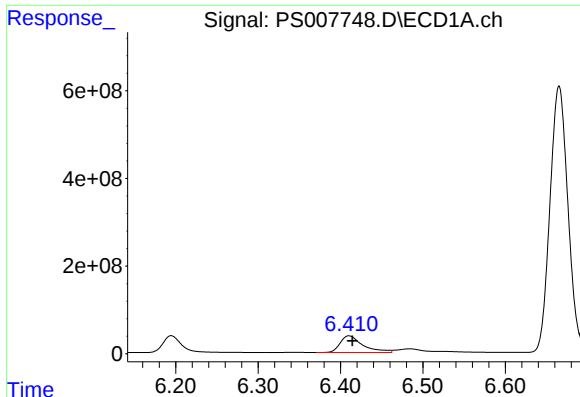

#9 2,4-D


R.T.: 6.410 min
Delta R.T.: -0.004 min
Response: 728990008
Conc: 519.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

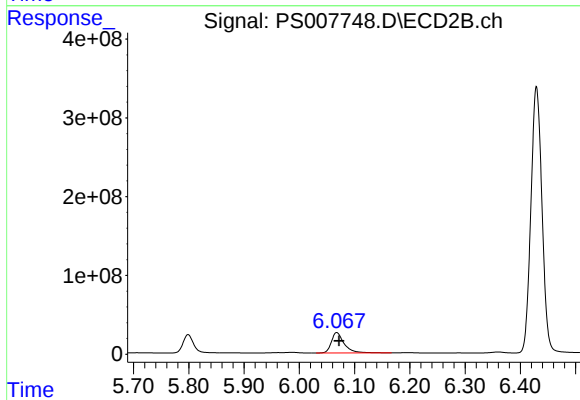


#9 2,4-D

R.T.: 6.068 min
Delta R.T.: -0.004 min
Response: 414393944
Conc: 513.88 ng/ml

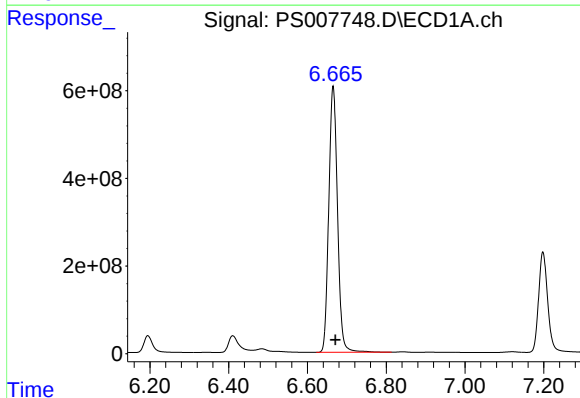


#10 Pentachlorophenol

R.T.: 6.665 min
Delta R.T.: -0.005 min
Response: 9362703046
Conc: 494.05 ng/ml

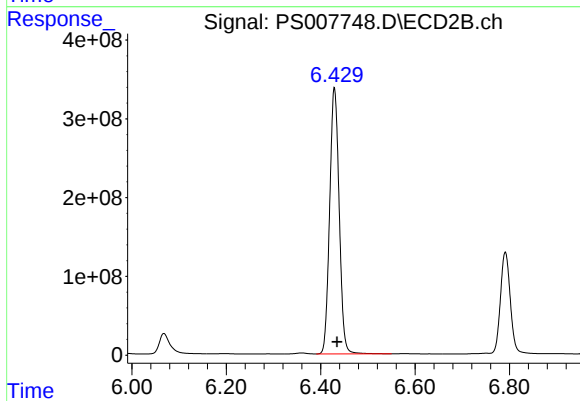

#10 Pentachlorophenol


R.T.: 6.429 min
Delta R.T.: -0.005 min
Response: 4725405255
Conc: 482.56 ng/ml

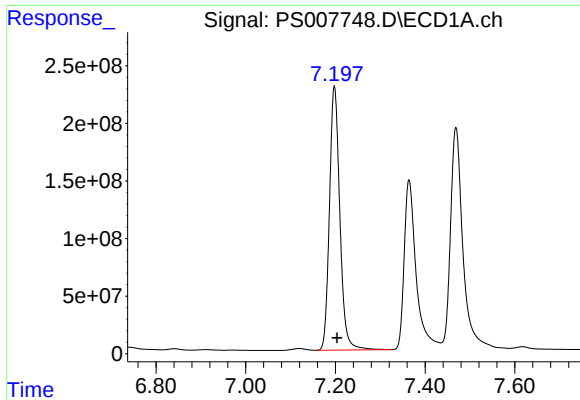

#11 2,4,5-TP (SILVEX)


R.T.: 7.198 min
Delta R.T.: -0.006 min
Response: 3683616216
Conc: 490.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

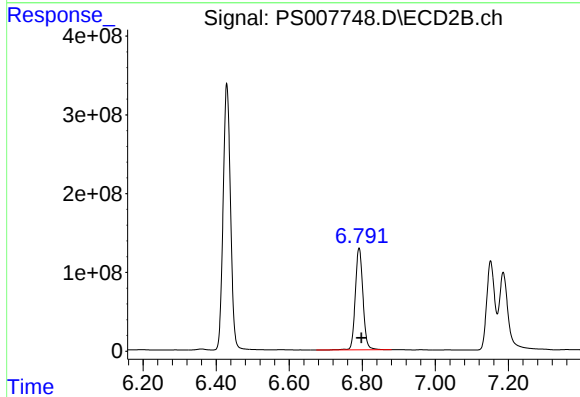


#11 2,4,5-TP (SILVEX)

R.T.: 6.791 min
Delta R.T.: -0.006 min
Response: 1882027056
Conc: 480.62 ng/ml

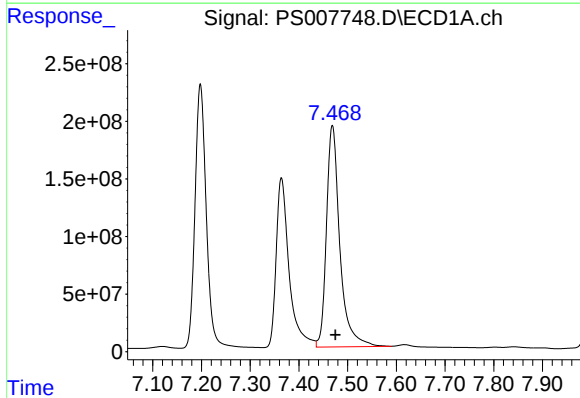


#12 2,4,5-T

R.T.: 7.469 min
Delta R.T.: -0.006 min
Response: 3666621270
Conc: 447.91 ng/ml

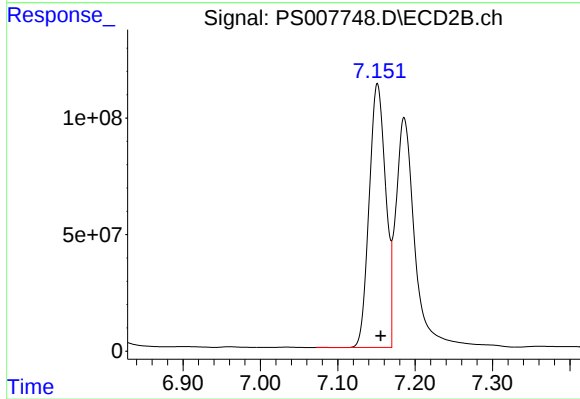

#12 2,4,5-T


R.T.: 7.151 min
Delta R.T.: -0.004 min
Response: 1670959470
Conc: 452.48 ng/ml

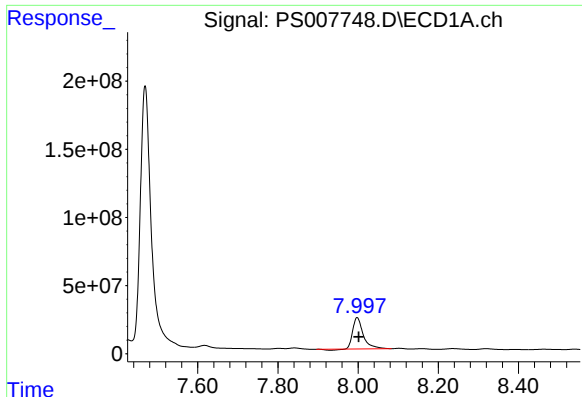

#13 2,4-DB


R.T.: 7.998 min
Delta R.T.: -0.004 min
Response: 410724861
Conc: 384.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

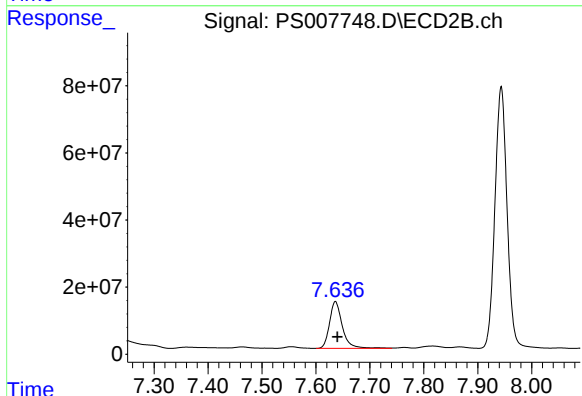


#13 2,4-DB

R.T.: 7.636 min
Delta R.T.: -0.004 min
Response: 230939537
Conc: 472.40 ng/ml

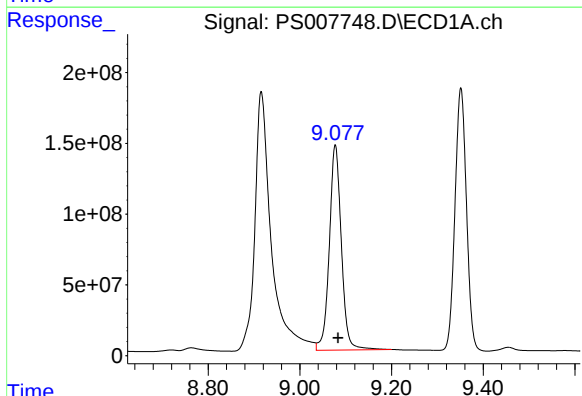


#14 DINOSEB

R.T.: 9.077 min
Delta R.T.: -0.006 min
Response: 2640090146
Conc: 439.61 ng/ml

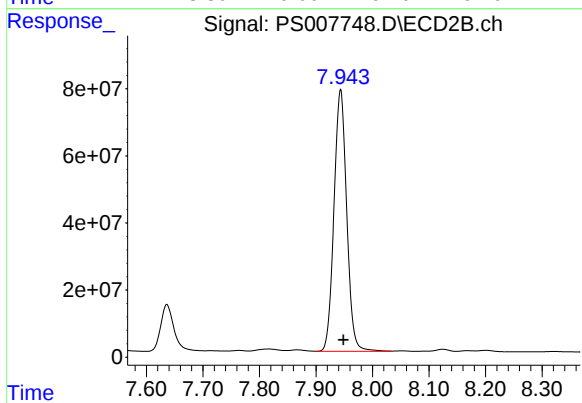

#14 DINOSEB


R.T.: 7.943 min
Delta R.T.: -0.005 min
Response: 1221447923
Conc: 420.15 ng/ml

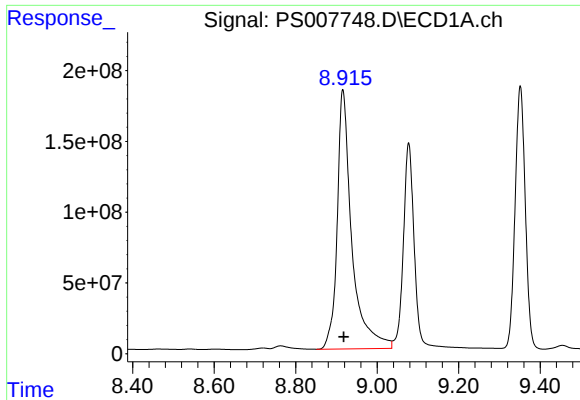

#15 Picloram


R.T.: 8.916 min
Delta R.T.: -0.002 min
Response: 4568092062
Conc: 411.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

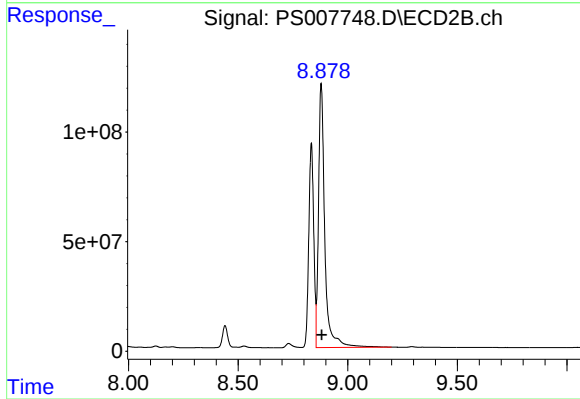


#15 Picloram

R.T.: 8.879 min
Delta R.T.: -0.003 min
Response: 2394232474
Conc: 408.65 ng/ml

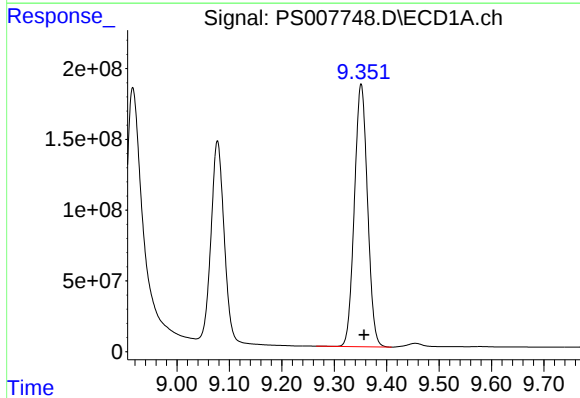

#16 DCPA

R.T.: 9.351 min
Delta R.T.: -0.005 min
Response: 3224620232
Conc: 328.77 ng/ml

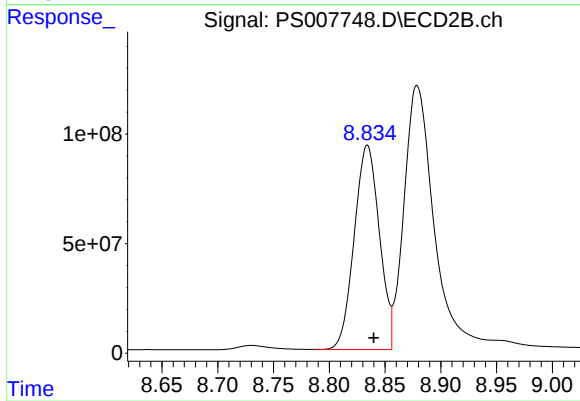

#16 DCPA

R.T.: 8.834 min
Delta R.T.: -0.006 min
Response: 1465151302
Conc: 280.40 ng/ml