

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111921\
 Data File : PS017455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2021 13:16
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 22:49:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 19 21:46:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
13) T	2,4-DB	9.945	0.000	4567948	0	2.685 N.D. #
15) T	Picloram	10.931	10.779	26661528	8691857	2.187 1.992
16) T	DCPA	0.000	10.779f	0	8691857	N.D. 1.973



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111921\
Data File : PS017455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2021 13:16
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 22:49:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
Quant Title : 8080.M
QLast Update : Fri Nov 19 21:46:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

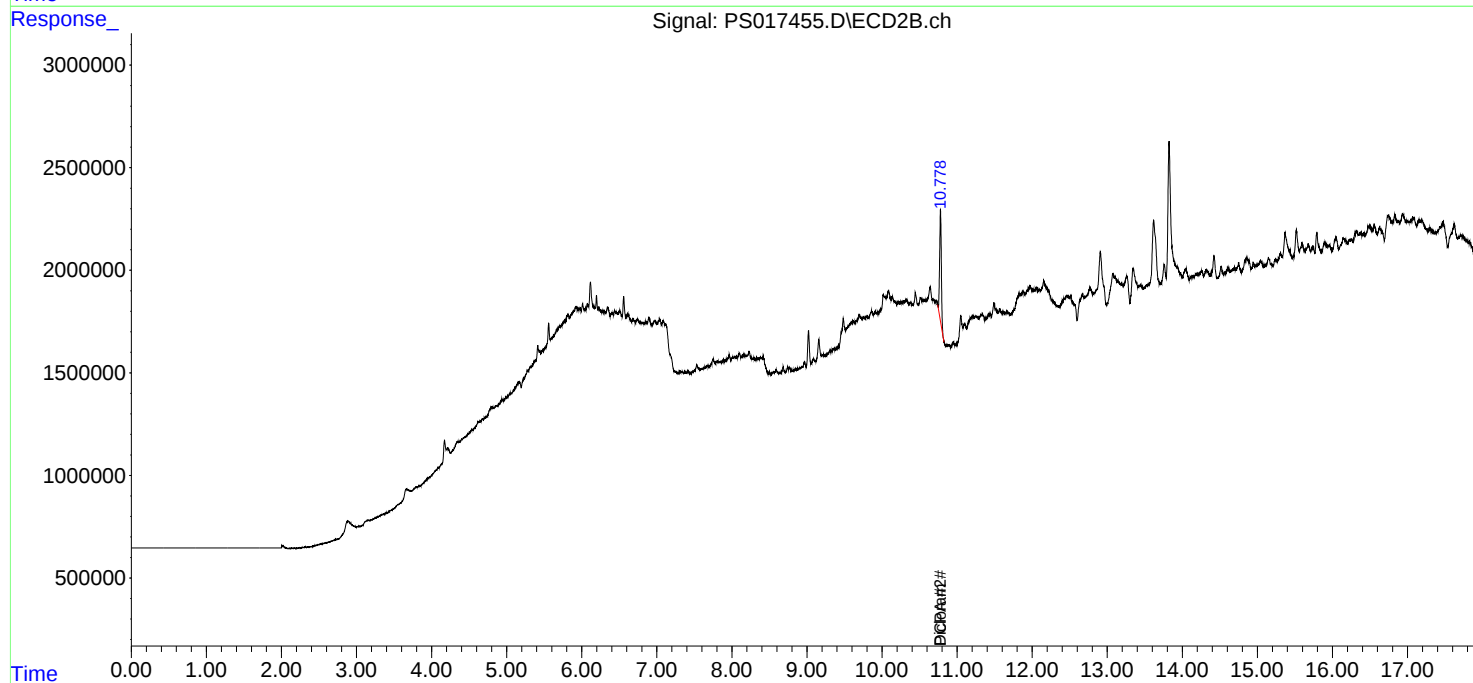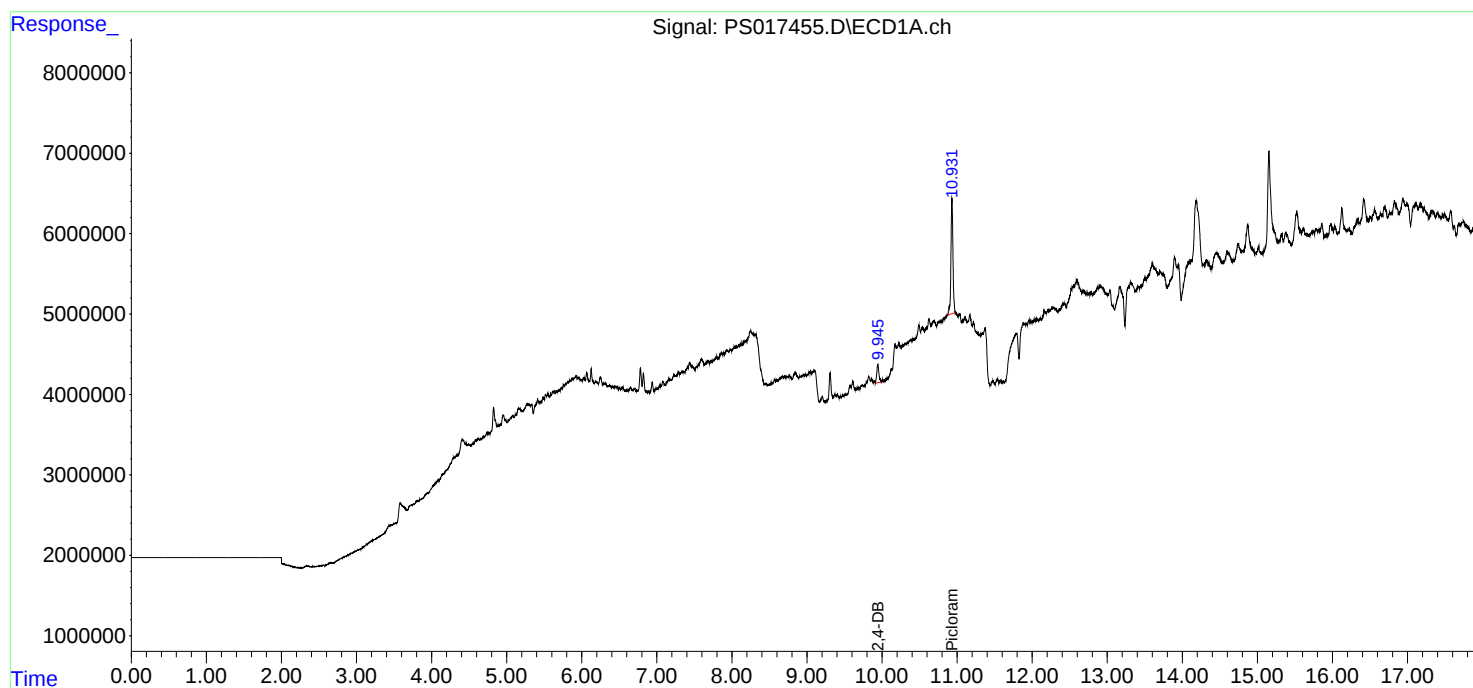


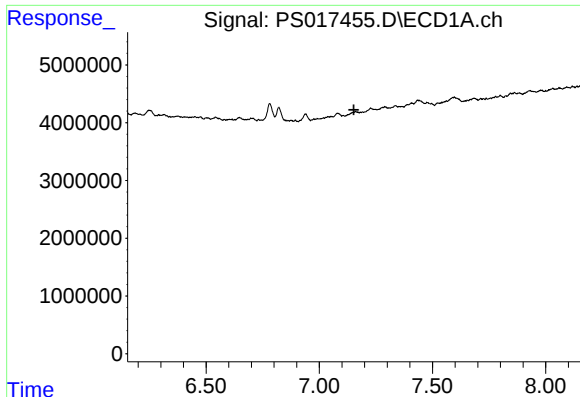

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.153 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

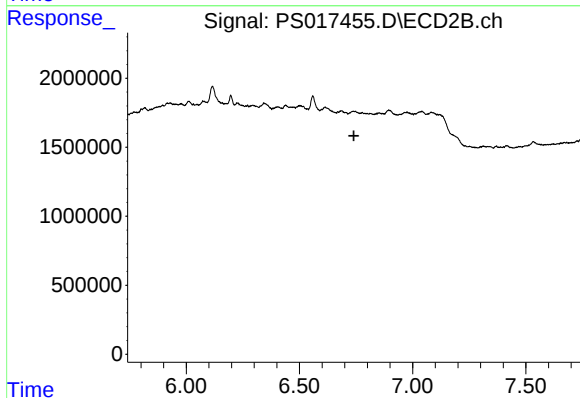


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.740 min
Response: 0
Conc: N.D.

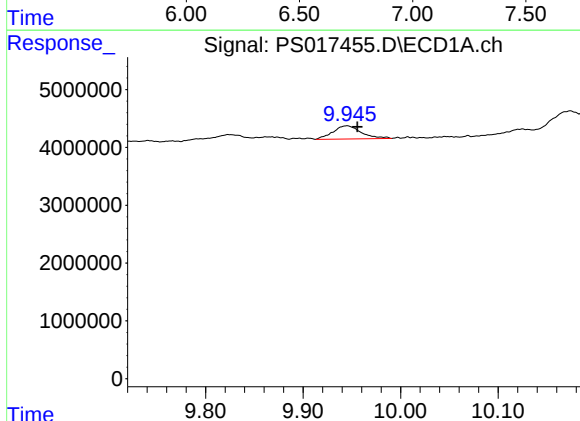


#13 2,4-DB

R.T.: 9.945 min
Delta R.T.: -0.010 min
Response: 4567948
Conc: 2.68 ng/ml

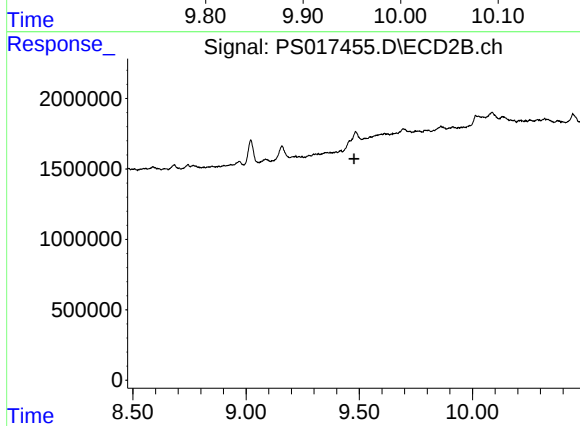

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 9.477 min
Response: 0
Conc: N.D.

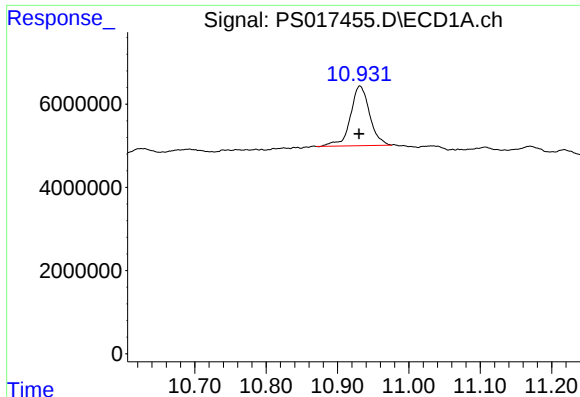

#15 Picloram


R.T.: 10.931 min
Delta R.T.: 0.000 min
Response: 26661528
Conc: 2.19 ng/ml

Instrument :
ECD_S
ClientSampleId :

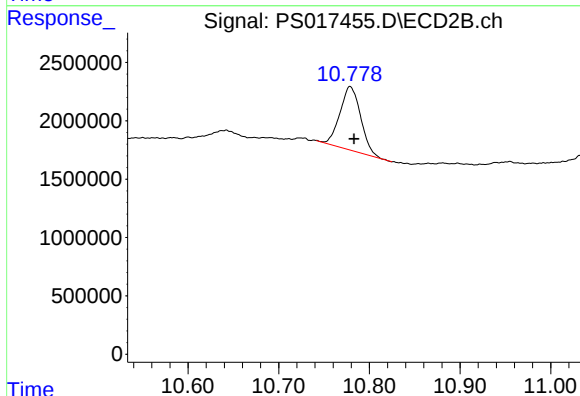


#15 Picloram

R.T.: 10.779 min
Delta R.T.: -0.004 min
Response: 8691857
Conc: 1.99 ng/ml

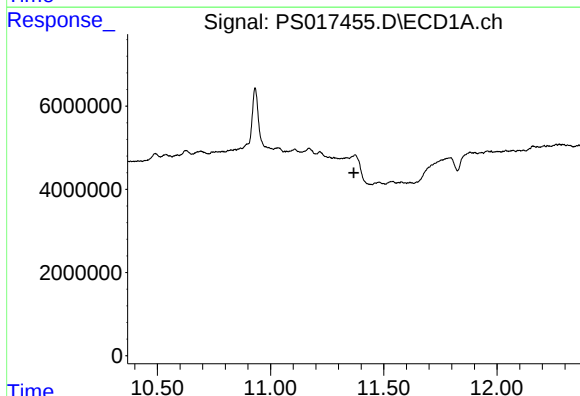

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.368 min
Response: 0
Conc: N.D.

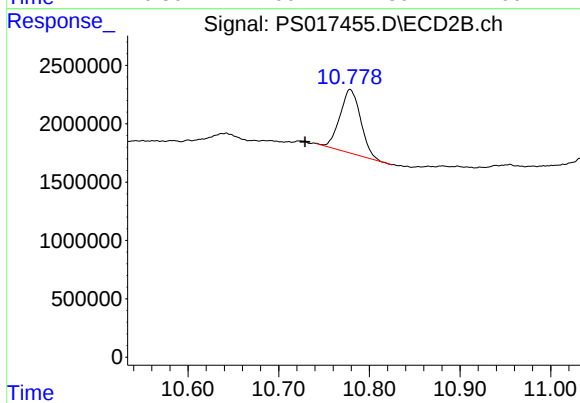

#16 DCPA

R.T.: 10.779 min
Delta R.T.: 0.049 min
Response: 8691857
Conc: 1.97 ng/ml