

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111921\
 Data File : PS017476.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2021 23:17
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 00:13:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 19 21:46:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.151	6.739	685.4E6	281.7E6	435.955	475.423
Target Compounds							
3) T	4-Nitroph...	6.943f	0.000	4228658	0	5.056	N.D. #
7) T	MCPA	7.622	0.000	8497941	0	1.296	N.D. #
9) T	2,4-D	8.330f	0.000	42013836	0	22.484	N.D. #
15) T	Picloram	10.898	0.000	17400093	0	1.427	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111921\
Data File : PS017476.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2021 23:17
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 00:13:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
Quant Title : 8080.M
QLast Update : Fri Nov 19 21:46:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

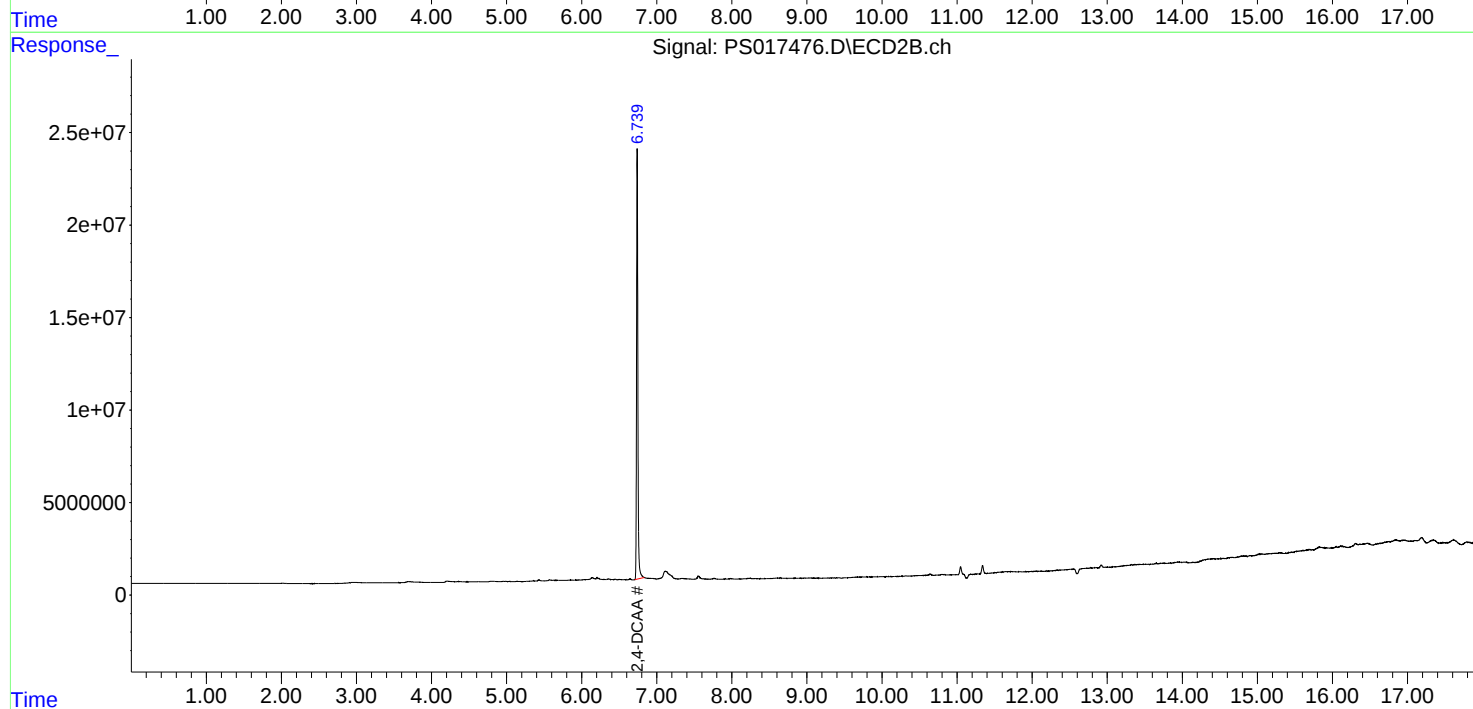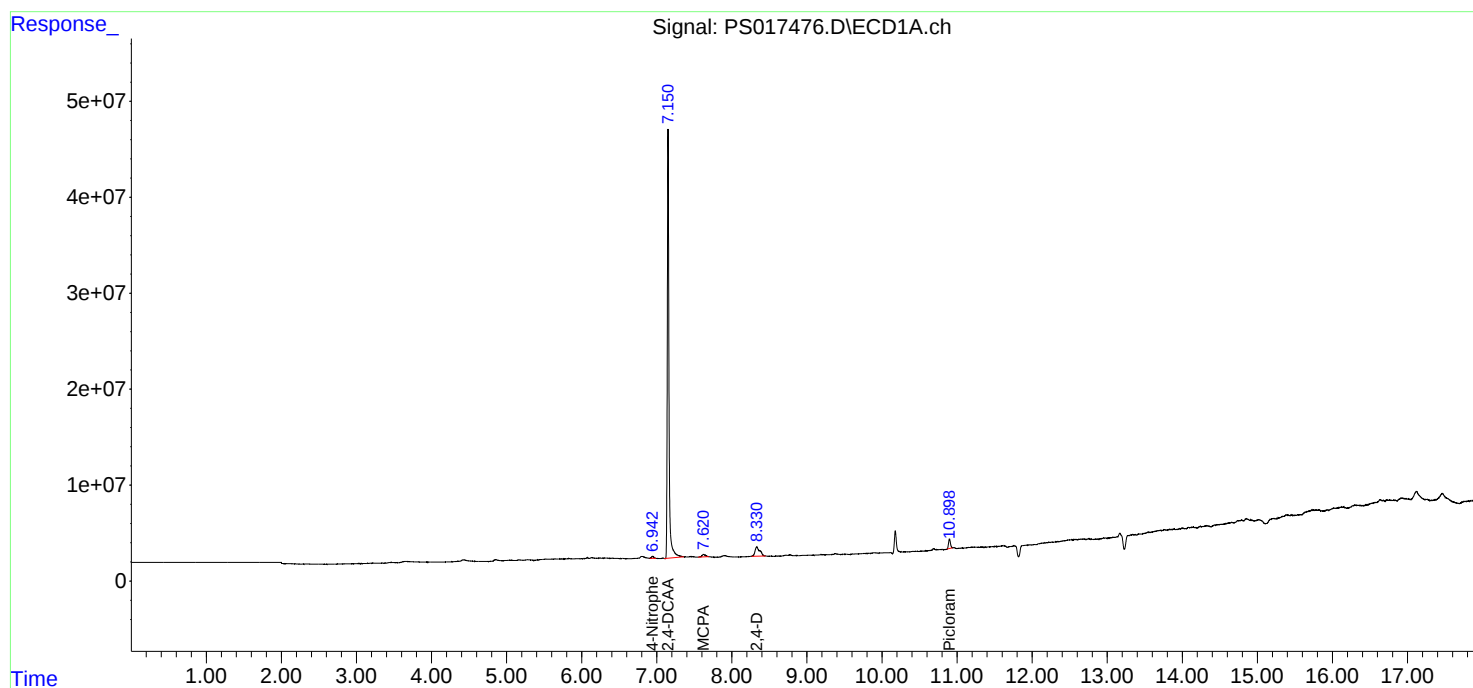


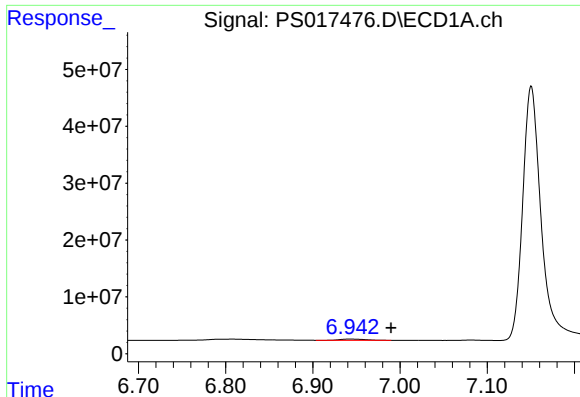

#3 4-Nitrophenol


R.T.: 6.943 min
Delta R.T.: -0.047 min
Response: 4228658
Conc: 5.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

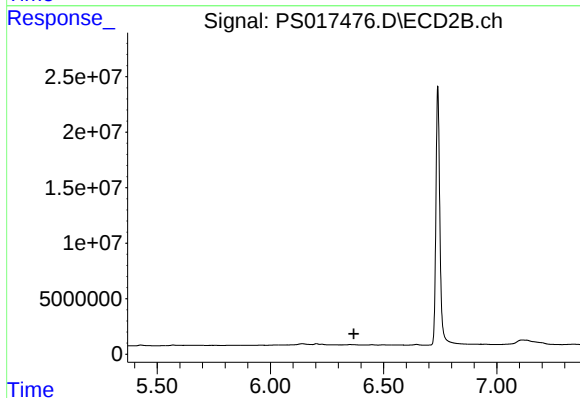


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.369 min
Response: 0
Conc: N.D.

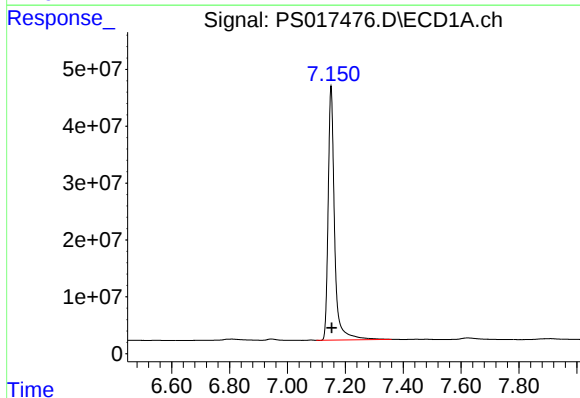


#4 2,4-DCAA

R.T.: 7.151 min
Delta R.T.: -0.002 min
Response: 685406320
Conc: 435.96 ng/ml

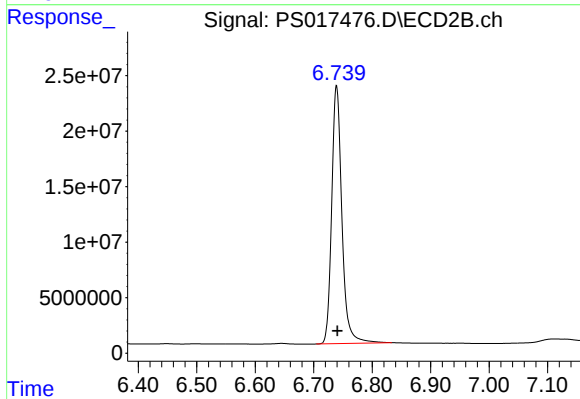

#4 2,4-DCAA


R.T.: 6.739 min
Delta R.T.: -0.001 min
Response: 281725415
Conc: 475.42 ng/ml

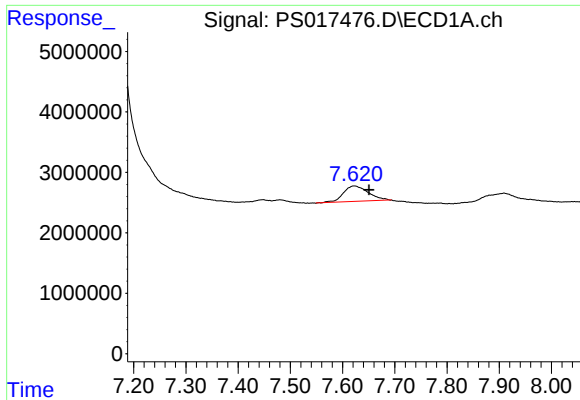

#7 MCPA


R.T.: 7.622 min
Delta R.T.: -0.029 min
Response: 8497941
Conc: 1.30 ug/ml

Instrument :
ECD_S
ClientSampleId :

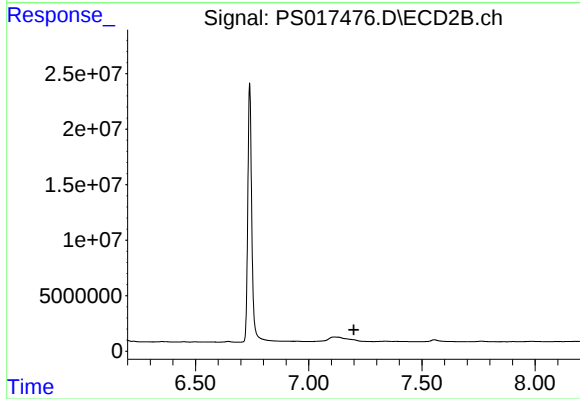


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.200 min
Response: 0
Conc: N.D.

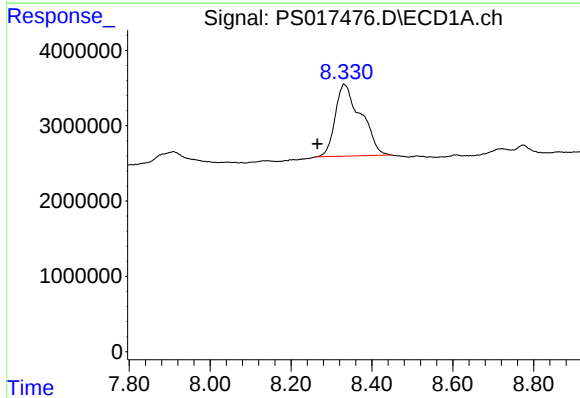


#9 2,4-D

R.T.: 8.330 min
Delta R.T.: 0.065 min
Response: 42013836
Conc: 22.48 ng/ml

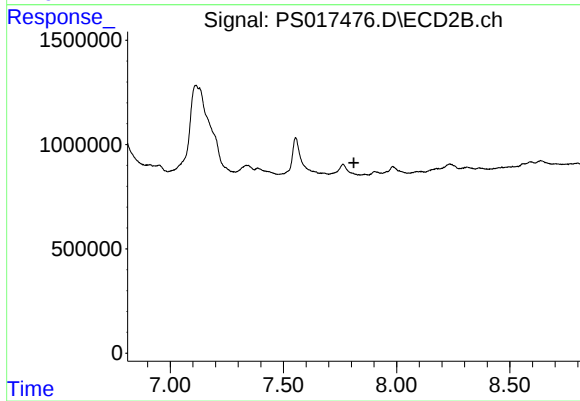

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.811 min
Response: 0
Conc: N.D.

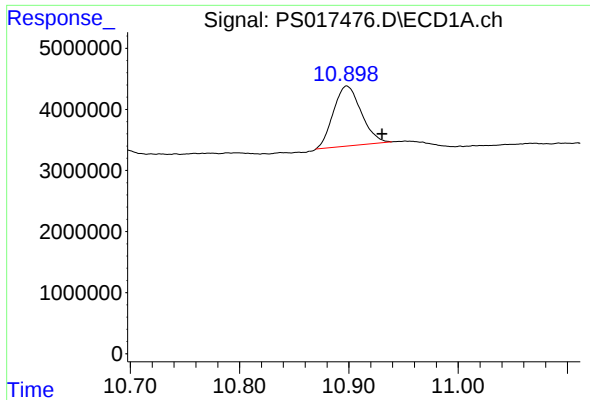

#15 Picloram

R.T.: 10.898 min
Delta R.T.: -0.032 min
Response: 17400093
Conc: 1.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

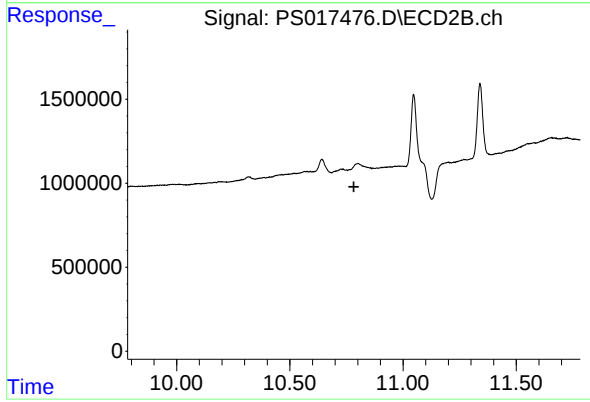

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.783 min
Response: 0
Conc: N.D.