

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111925\
 Data File : PS032486.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2025 15:57
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 03:35:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
4) S	2,4-DCAA	7.281	7.619	1820.1E6	1911.3E6	401.678	524.284	#
Target Compounds								
2) T	3,5-DICHL...	6.441	0.000	34982883	0	5.410	N.D.	#
3) T	4-Nitroph...	7.138f	0.000	58329	0	<MDL	N.D.	#
6) T	MCP	7.660	7.911	49509	21555545	<MDL	1.621	#
7) T	MCPA	7.796	0.000	7798855	0	<MDL	N.D.	#
8) T	DICHLORPROP	8.165	0.000	247600	0	<MDL	N.D.	#
9) T	2,4-D	8.444f	8.845	202.4E6	19485870	44.862	3.715	#
10) T	Pentachlo...	8.709	9.359	2677049	16505927	<MDL	<MDL	#
11) T	2,4,5-TP ...	9.281	0.000	4514475	0	<MDL	N.D.	#
12) T	2,4,5-T	9.586	0.000	1658288	0	<MDL	N.D.	#
13) T	2,4-DB	10.151	0.000	1237341	0	<MDL	N.D.	#
14) T	DINOSEB	11.328	0.000	6422665	0	<MDL	N.D.	#
15) T	Picloram	11.171	12.202	44145042	148.7E6	2.080	4.000	#
16) T	DCPA	11.637	12.097f	9157045	37587920	<MDL	1.180	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111925\
Data File : PS032486.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2025 15:57
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 03:35:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

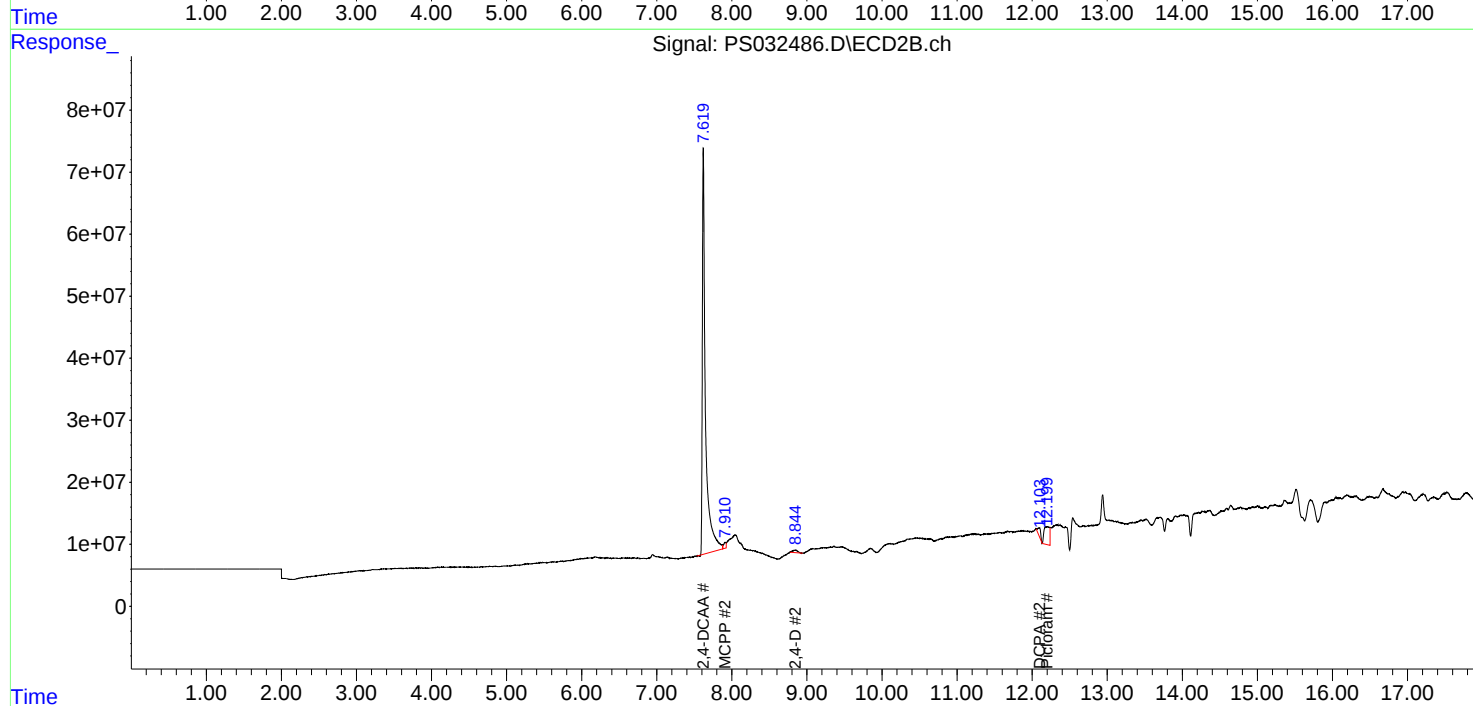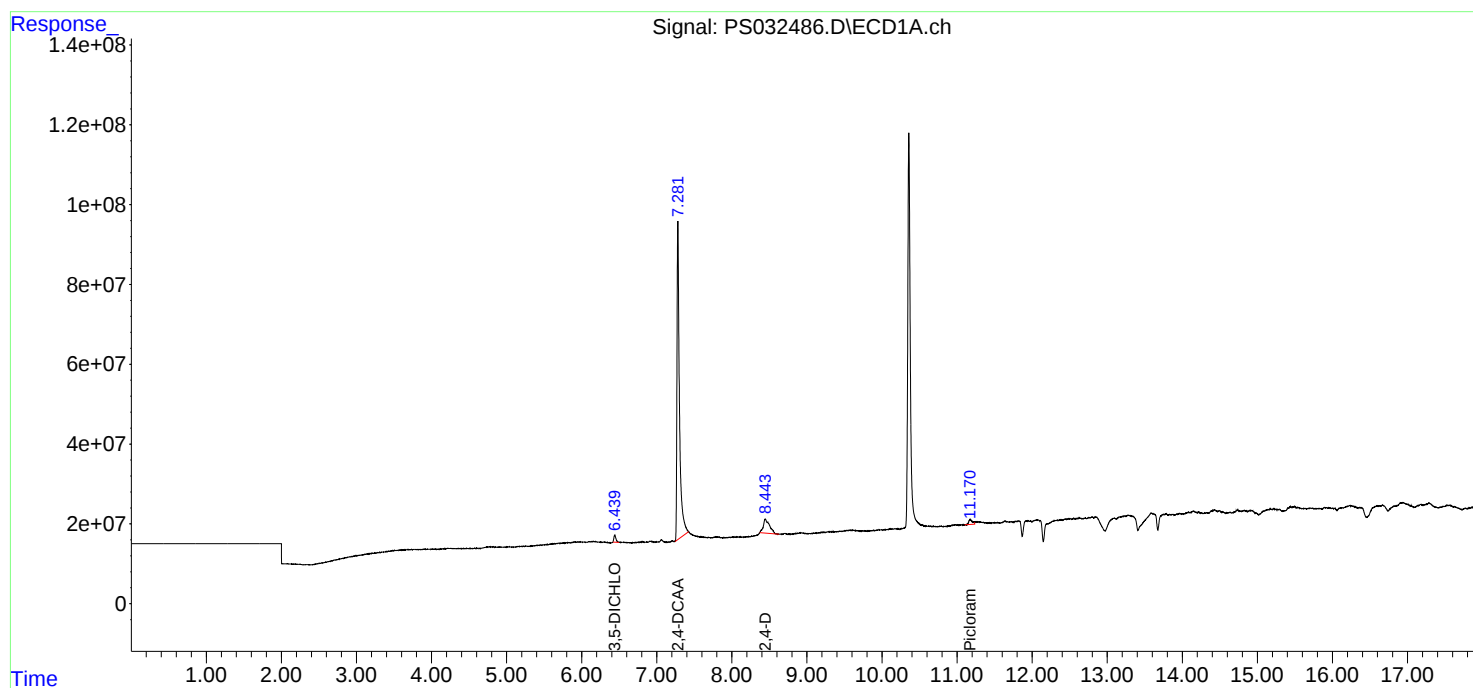


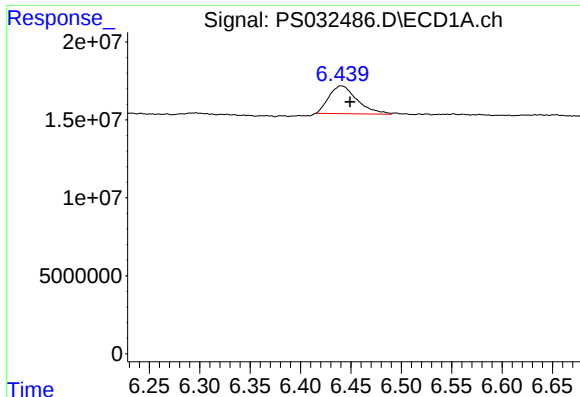

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.441 min
Delta R.T.: -0.009 min
Response: 34982883
Conc: 5.41 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

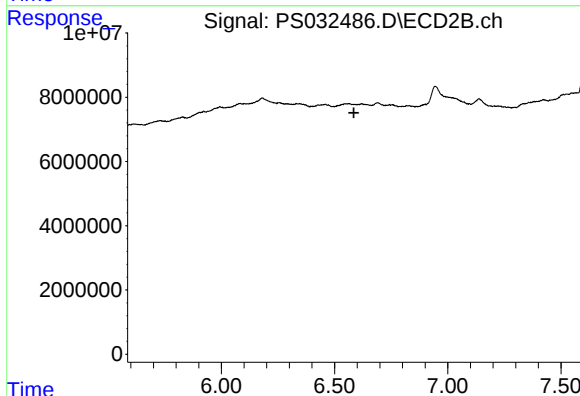


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.585 min
Response: 0
Conc: N.D.

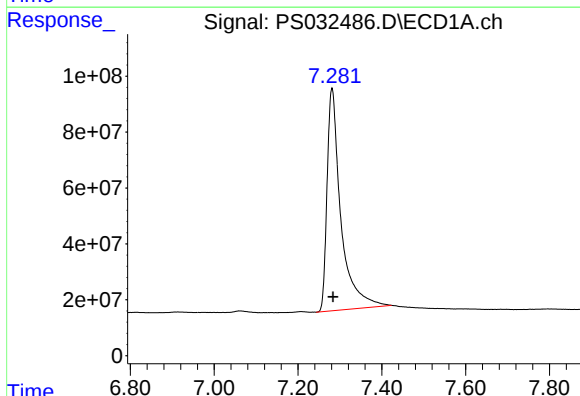


#4 2,4-DCAA

R.T.: 7.281 min
Delta R.T.: -0.002 min
Response: 1820111598
Conc: 401.68 ng/ml

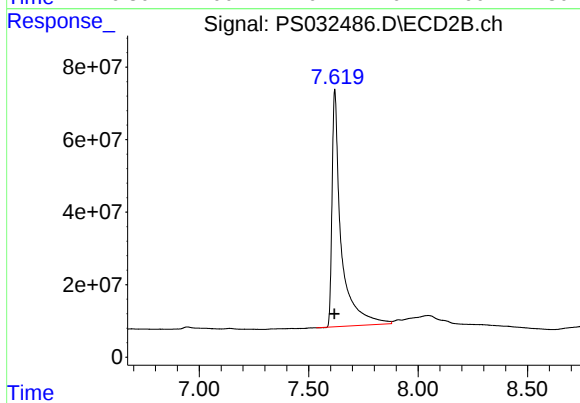

#4 2,4-DCAA


R.T.: 7.619 min
Delta R.T.: 0.002 min
Response: 1911274961
Conc: 524.28 ng/ml

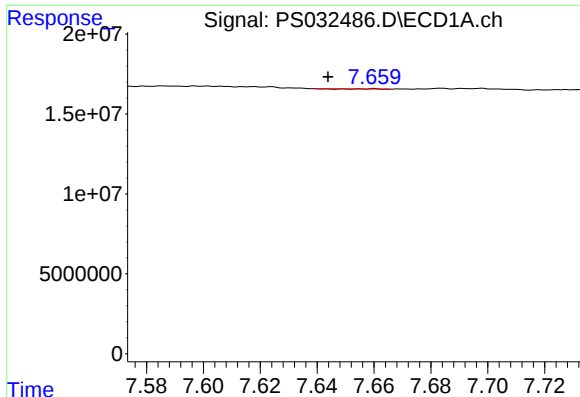

#6 MCPP


R.T.: 7.660 min
Delta R.T.: 0.016 min
Response: 49509
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

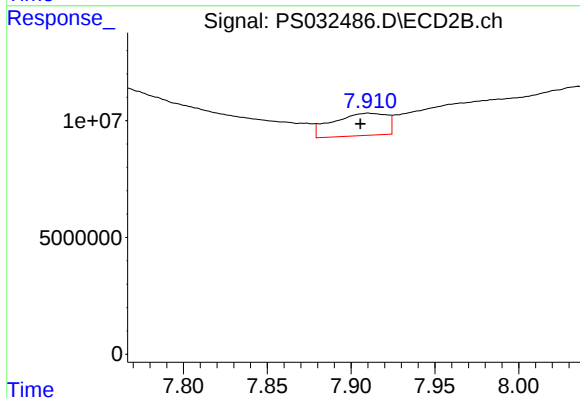


#6 MCPP

R.T.: 7.911 min
Delta R.T.: 0.005 min
Response: 2155545
Conc: 1.62 ug/ml

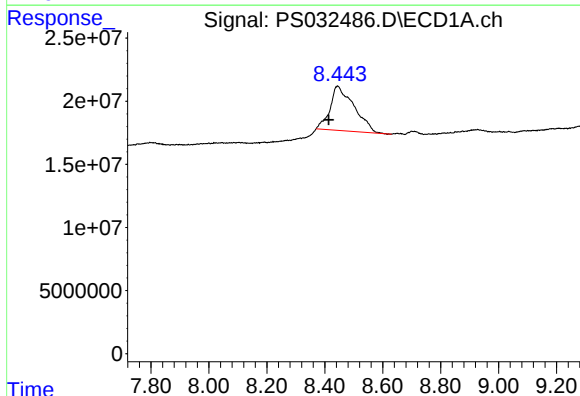


#9 2,4-D

R.T.: 8.444 min
Delta R.T.: 0.030 min
Response: 202409877
Conc: 44.86 ng/ml

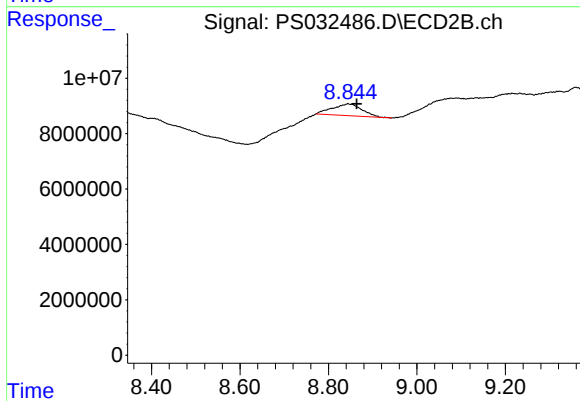

#9 2,4-D


R.T.: 8.845 min
Delta R.T.: -0.019 min
Response: 19485870
Conc: 3.71 ng/ml

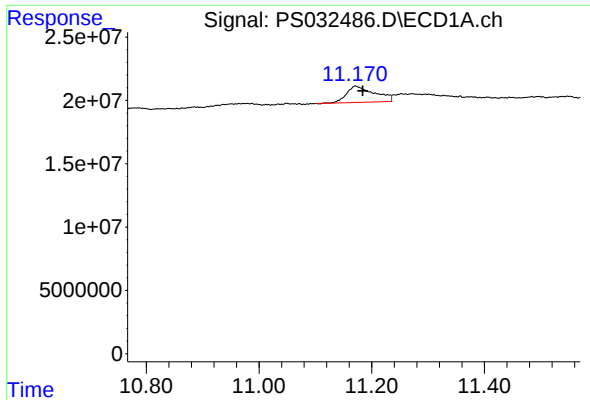

#15 Picloram


R.T.: 11.171 min
Delta R.T.: -0.013 min
Response: 44145042
Conc: 2.08 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

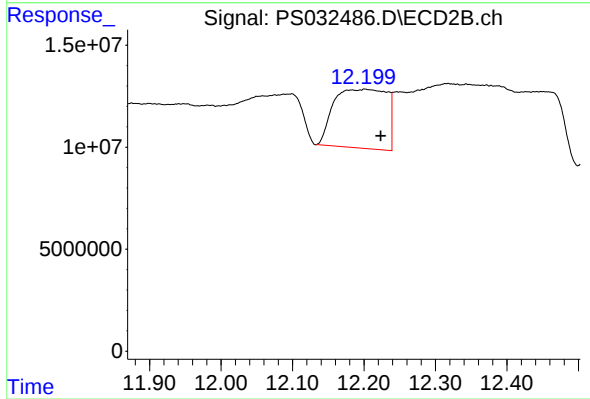


#15 Picloram

R.T.: 12.202 min
Delta R.T.: -0.021 min
Response: 148730418
Conc: 4.00 ng/ml

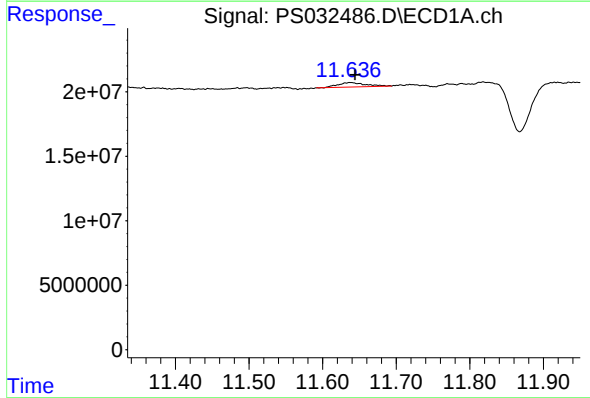

#16 DCPA

R.T.: 11.637 min
Delta R.T.: -0.007 min
Response: 9157045
Conc: N.D.

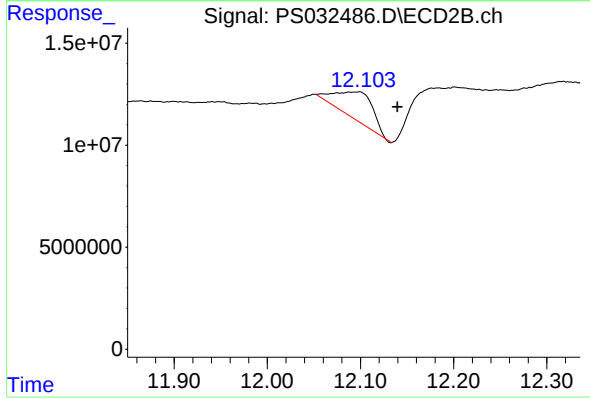

#16 DCPA

R.T.: 12.097 min
Delta R.T.: -0.043 min
Response: 37587920
Conc: 1.18 ng/ml