

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111925\
 Data File : PS032496.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2025 20:08
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 20 03:36:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 04 04:59:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.278	7.621	1802.8E6	1936.8E6	397.852	531.277 #
Target Compounds							
1) T	Dalapon	2.658	0.000	5708060	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.437	0.000	38513078	0	5.956	N.D. #
3) T	4-Nitroph...	7.122	0.000	42444	0	<MDL	N.D. #
6) T	MCP	7.661	7.909	624713	35408154	<MDL	2.662 #
7) T	MCPA	7.806	8.109f	2385612	2388919	<MDL	<MDL #
8) T	DICHLORPROP	8.174	0.000	631110	0	<MDL	N.D. #
9) T	2,4-D	8.441f	0.000	142.6E6	0	31.614	N.D. #
10) T	Pentachlo...	8.704	9.363	5527093	3386841	<MDL	<MDL #
11) T	2,4,5-TP ...	9.295	0.000	380981	0	<MDL	N.D. #
12) T	2,4,5-T	9.575	10.137f	1582168	3733342	<MDL	<MDL #
13) T	2,4-DB	10.154	0.000	763459	0	<MDL	N.D. #
14) T	DINOSEB	11.331	0.000	5248279	0	<MDL	N.D. #
15) T	Picloram	11.170	12.228	39566798	142.4E6	1.864	3.831 #
16) T	DCPA	11.636	0.000	4645440	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS111925\
Data File : PS032496.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2025 20:08
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 20 03:36:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS110325.M
Quant Title : 8080.M
QLast Update : Tue Nov 04 04:59:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

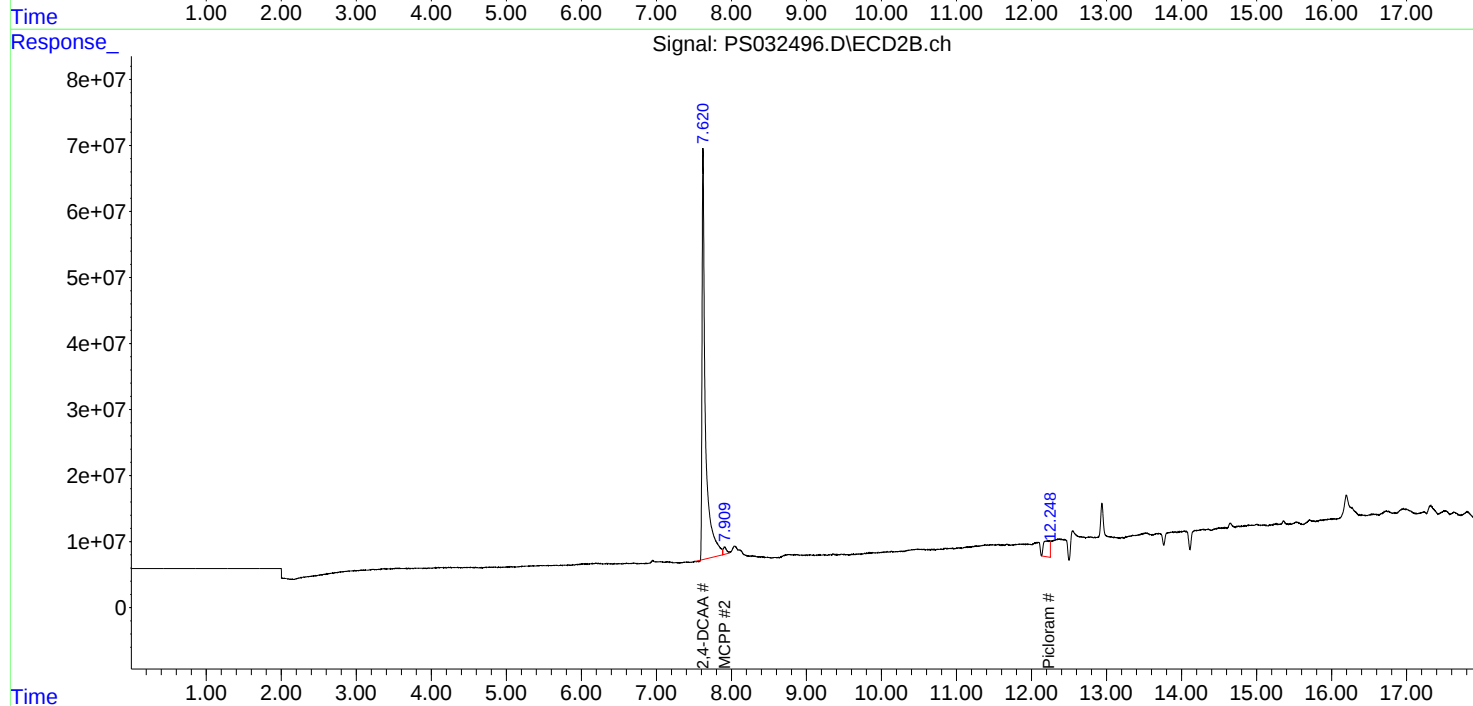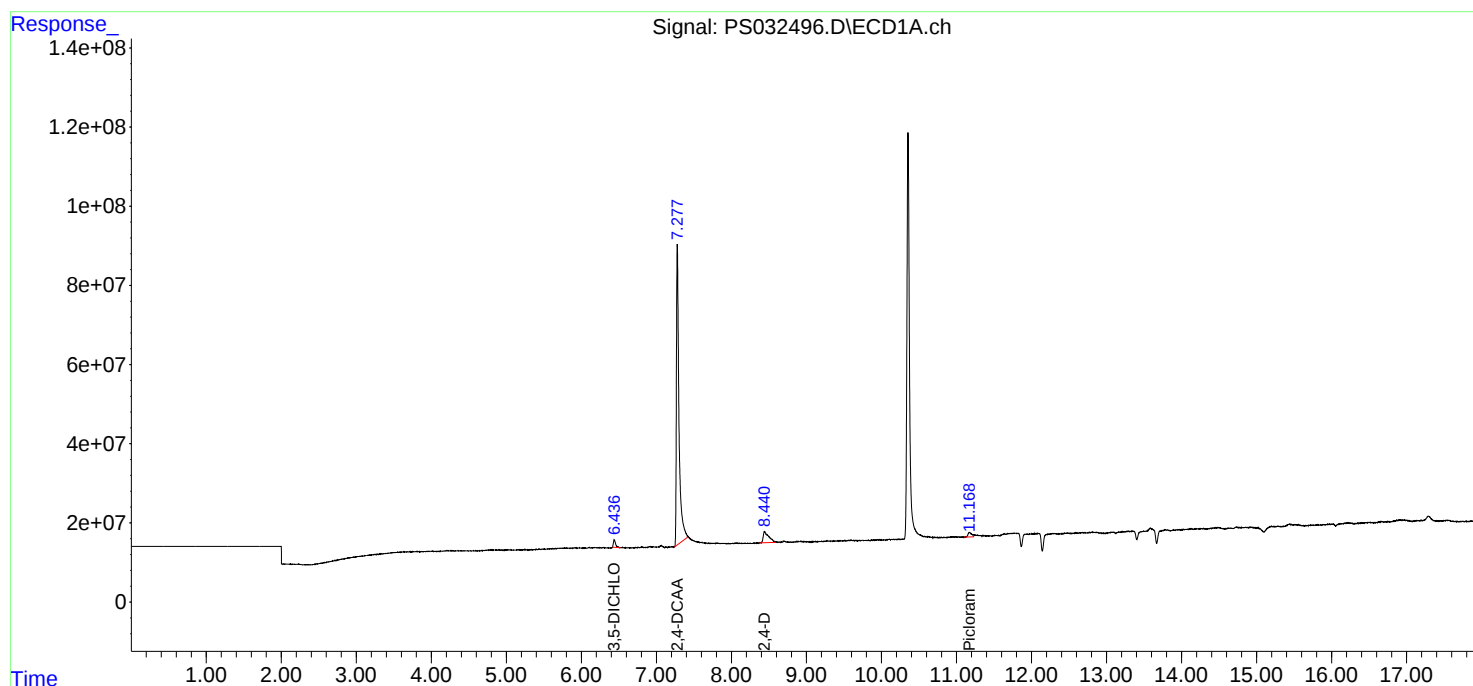


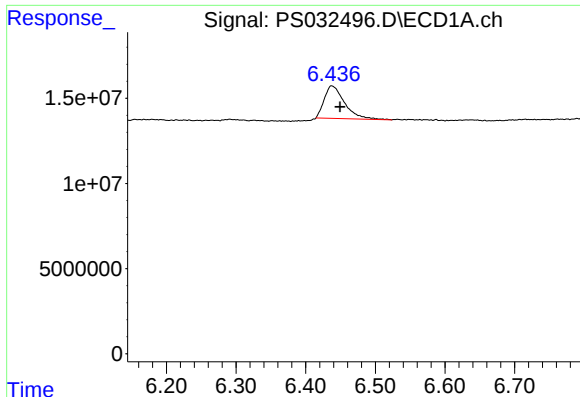

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.437 min
Delta R.T.: -0.012 min
Response: 38513078
Conc: 5.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

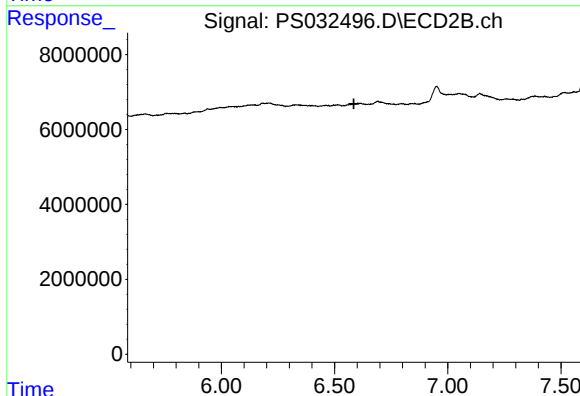


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.585 min
Response: 0
Conc: N.D.

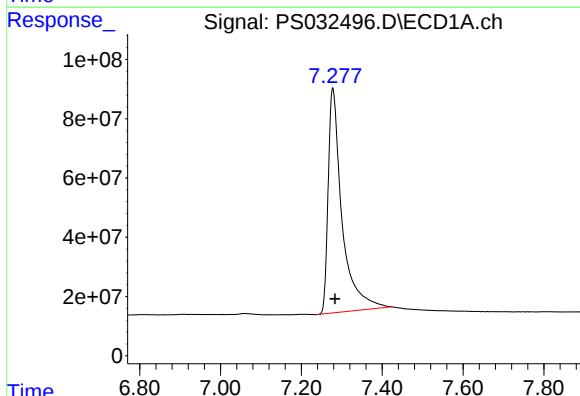


#4 2,4-DCAA

R.T.: 7.278 min
Delta R.T.: -0.006 min
Response: 1802776457
Conc: 397.85 ng/ml

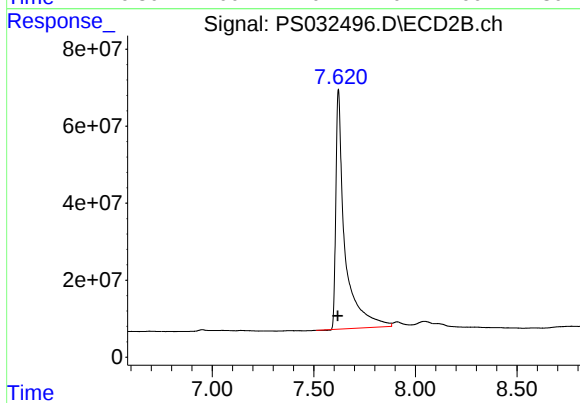

#4 2,4-DCAA


R.T.: 7.621 min
Delta R.T.: 0.004 min
Response: 1936769868
Conc: 531.28 ng/ml

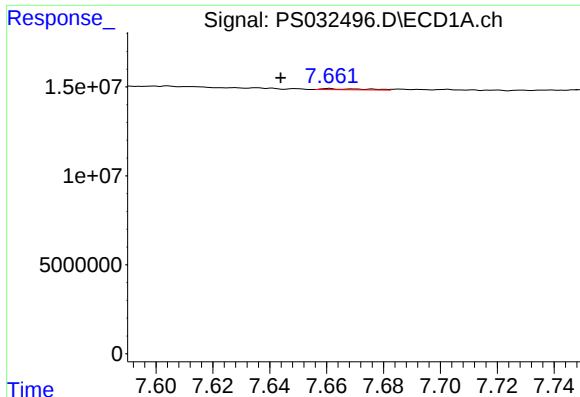

#6 MCPP


R.T.: 7.661 min
Delta R.T.: 0.017 min
Response: 624713
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

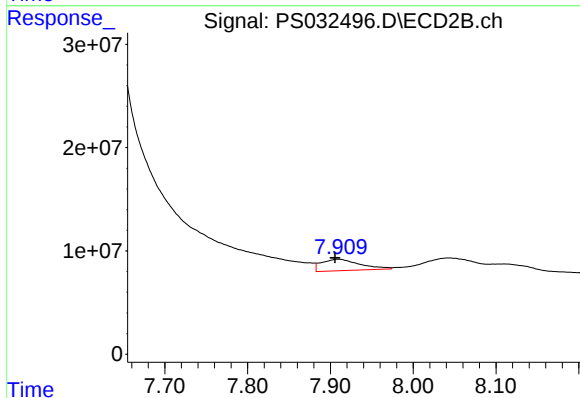


#6 MCPP

R.T.: 7.909 min
Delta R.T.: 0.004 min
Response: 35408154
Conc: 2.66 ug/ml

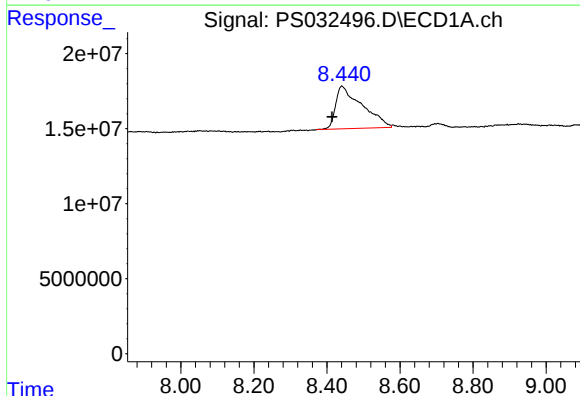


#9 2,4-D

R.T.: 8.441 min
Delta R.T.: 0.027 min
Response: 142638055
Conc: 31.61 ng/ml

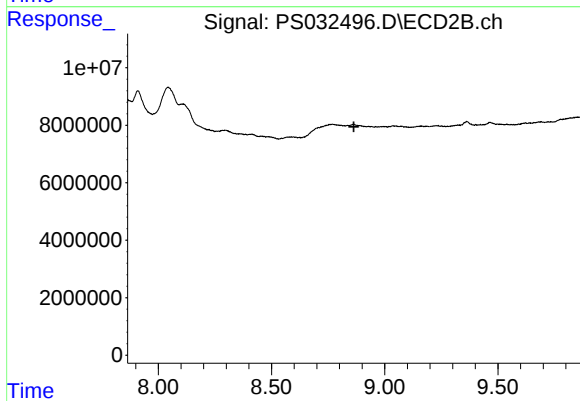

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.864 min
Response: 0
Conc: N.D.

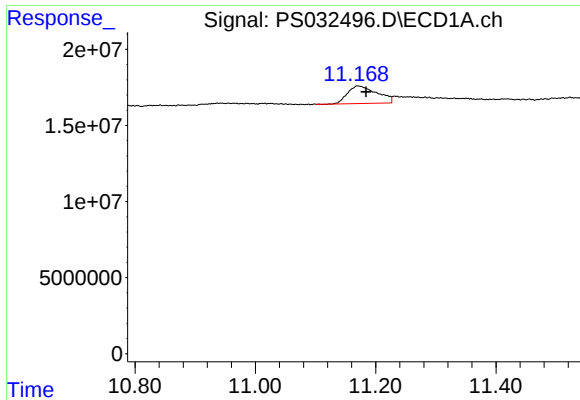

#15 Picloram

R.T.: 11.170 min
Delta R.T.: -0.014 min
Response: 39566798
Conc: 1.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

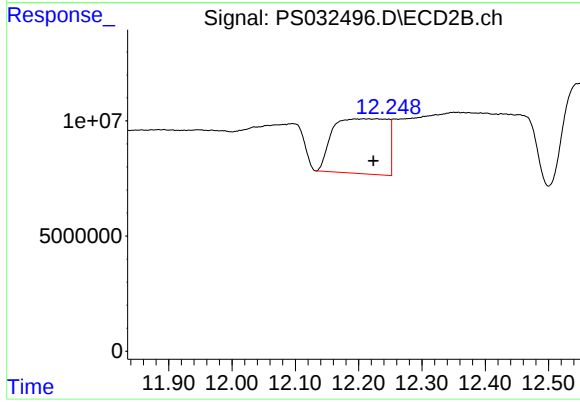

#15 Picloram

R.T.: 12.228 min
Delta R.T.: 0.005 min
Response: 142442520
Conc: 3.83 ng/ml